


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN122221\
Data File : VN070283.D
Acq On : 22 Dec 2021 9:47
Operator : JC/MD
Sample : BFB
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N120221W.M
Title : SW846 8260
Last Update : Fri Dec 03 08:46:47 2021

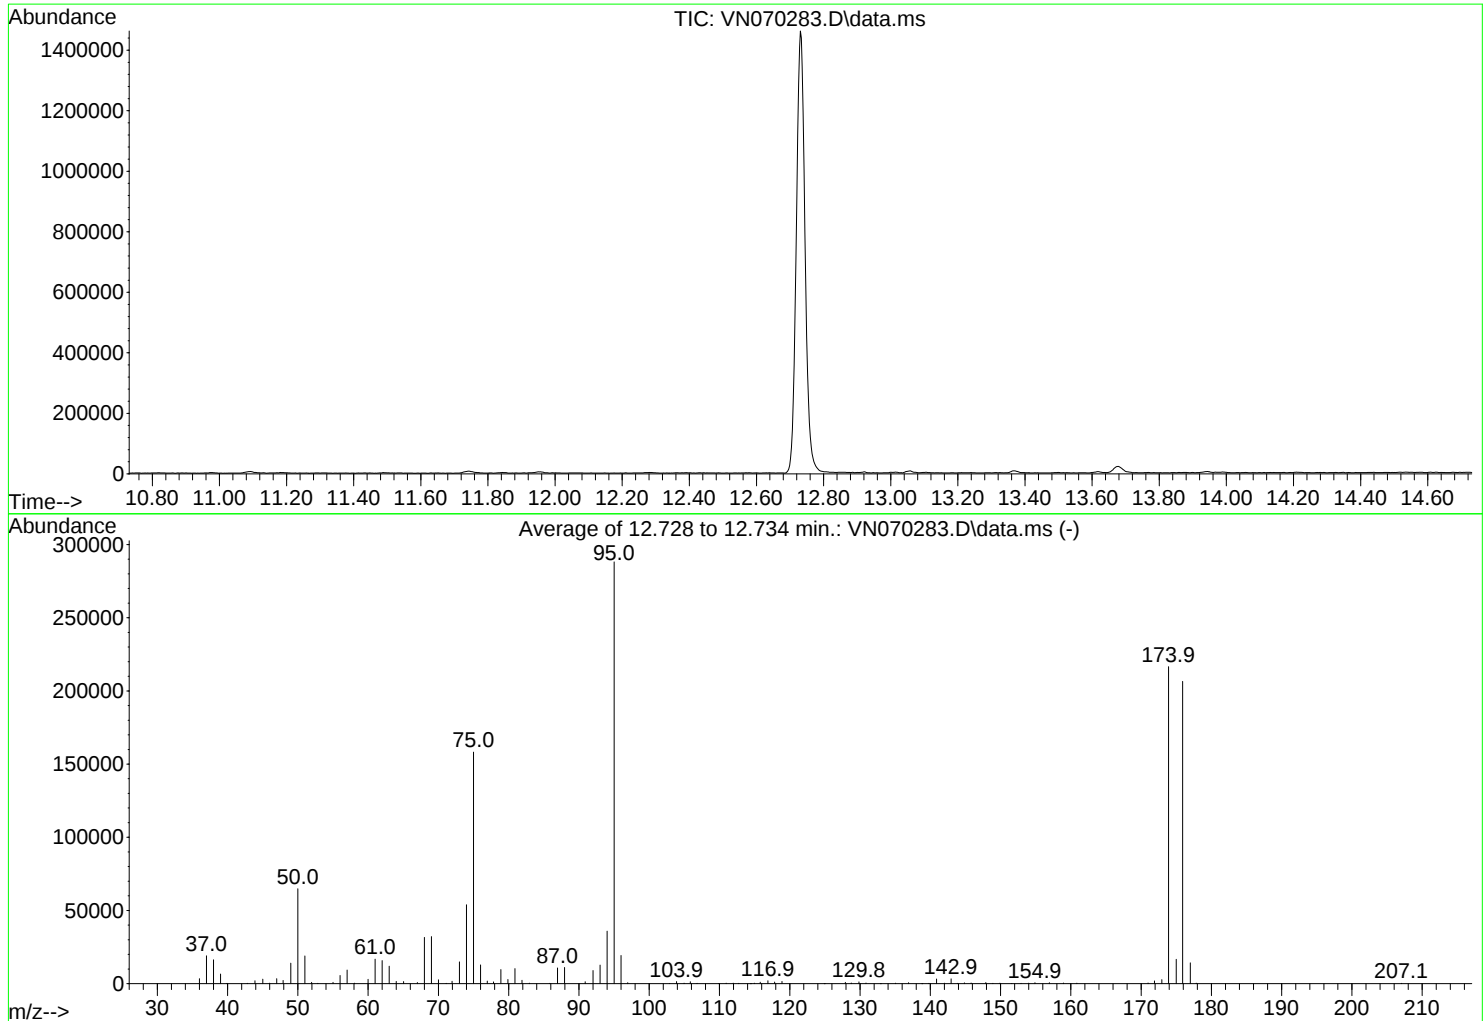

AutoFind: Scans 4004, 4005, 4006; Background Corrected with Scan 3986

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	22.5	64808	PASS
75	95	30	60	54.9	158165	PASS
95	95	100	100	100.0	288213	PASS
96	95	5	9	6.7	19293	PASS
173	174	0.00	2	1.3	2792	PASS
174	95	50	100	75.1	216555	PASS
175	174	5	9	7.7	16594	PASS
176	174	95	101	95.4	206507	PASS
177	176	5	9	6.9	14226	PASS