

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN122222\
Data File : VN075946.D
Acq On : 22 Dec 2022 15:39
Operator : JC\MD
Sample : N6168-06 50X
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
AUD-1691

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N121422W.M

Title : SW846 8260

Signal : TIC: VN075946.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.830	125	132	139	rVB5	9382	25190	1.66%	0.313%
2	3.806	291	298	307	rBV2	16347	45630	3.00%	0.568%
3	4.301	371	382	393	rBV	24566	73196	4.82%	0.911%
4	8.177	1031	1041	1045	rBV	217280	523819	34.50%	6.516%
5	8.230	1045	1050	1062	rVB	408557	927514	61.08%	11.538%
6	8.583	1097	1110	1125	rBV	213168	487961	32.13%	6.070%
7	9.106	1190	1199	1216	rBV	571410	1143242	75.29%	14.221%
8	10.571	1440	1448	1458	rBV	847169	1518474	100.00%	18.889%
9	11.871	1661	1669	1681	rVB	724047	1285911	84.68%	15.996%
10	12.853	1828	1836	1844	rBV	560441	921440	60.68%	11.462%
11	13.794	1988	1996	2008	rBV	639430	1086557	71.56%	13.516%




Sum of corrected areas: 8038934

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN122222\
Data File : VN075946.D
Acq On : 22 Dec 2022 15:39
Operator : JC\MD
Sample : N6168-06 50X
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
AUD-1691

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N121422W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

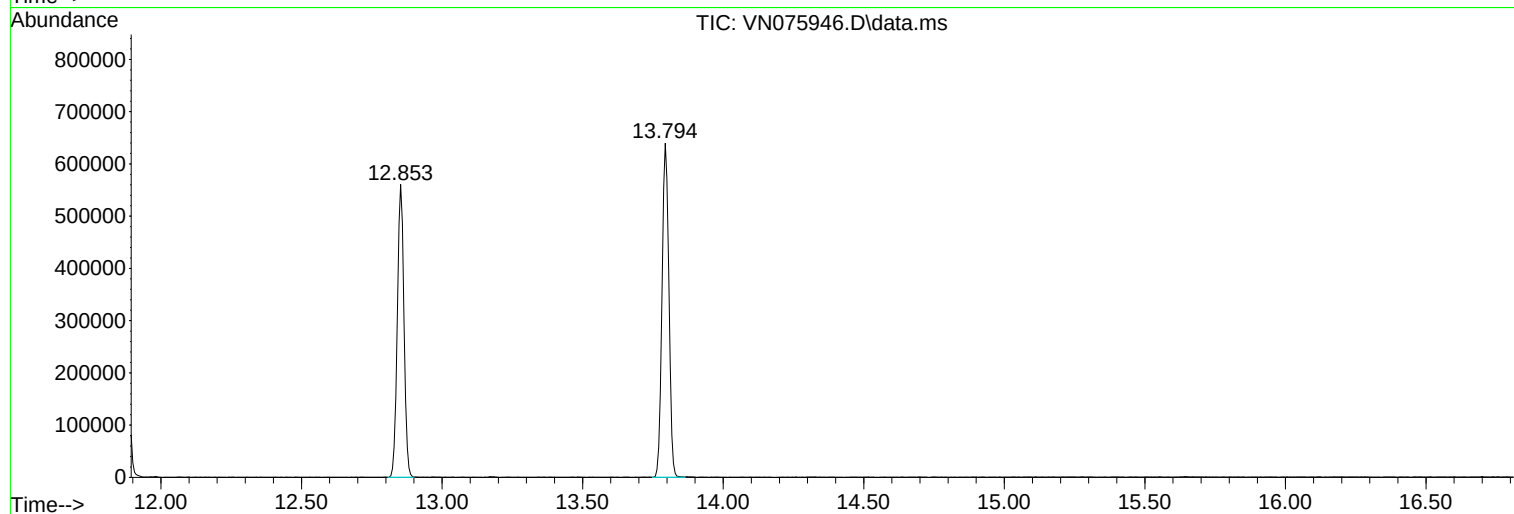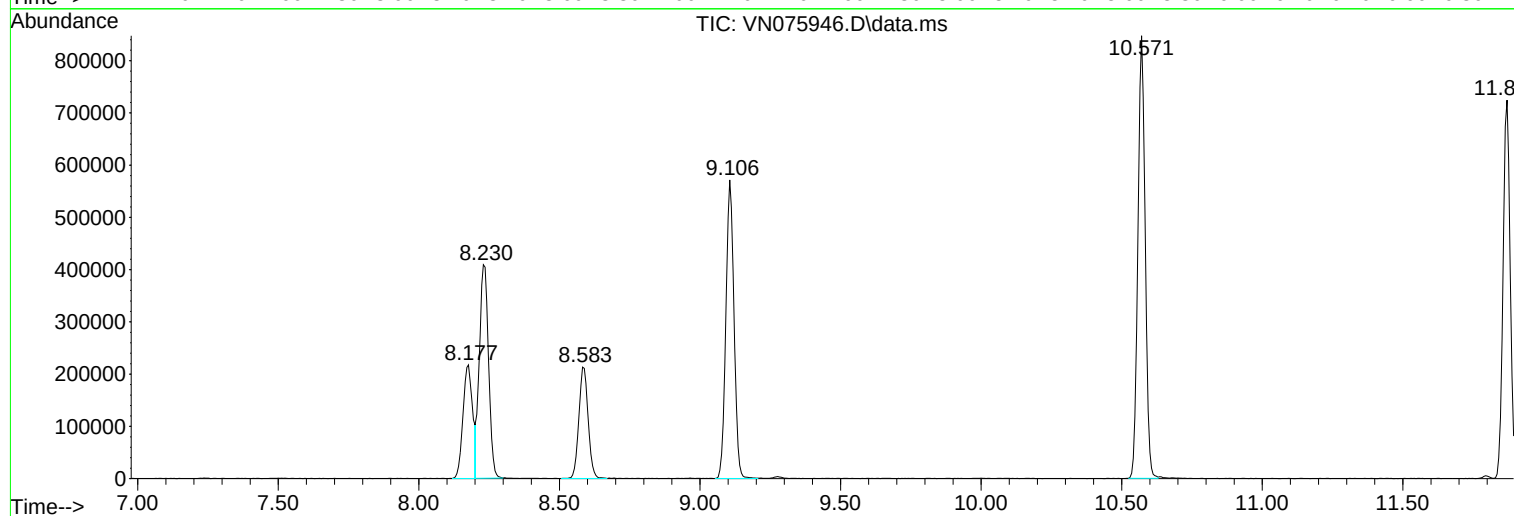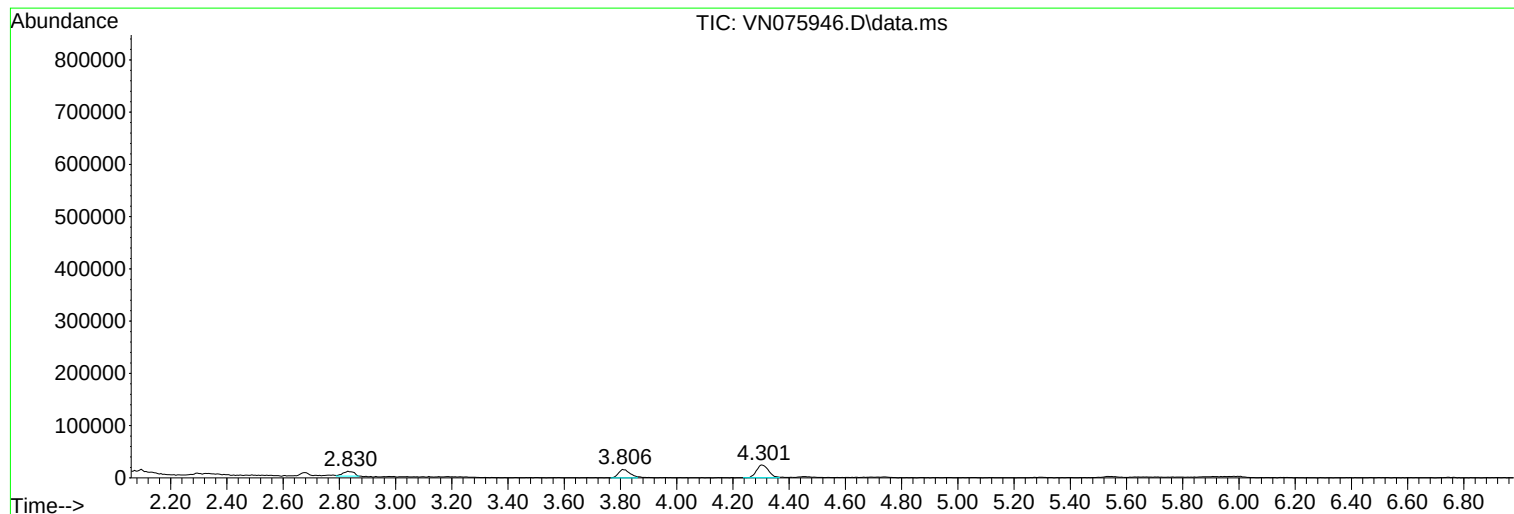

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN122222\
Data File : VN075946.D
Acq On : 22 Dec 2022 15:39
Operator : JC\MD
Sample : N6168-06 50X
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
AUD-1691

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N121422W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN122222\
Data File : VN075946.D
Acq On : 22 Dec 2022 15:39
Operator : JC\MD
Sample : N6168-06 50X
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
AUD-1691

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N121422W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc