
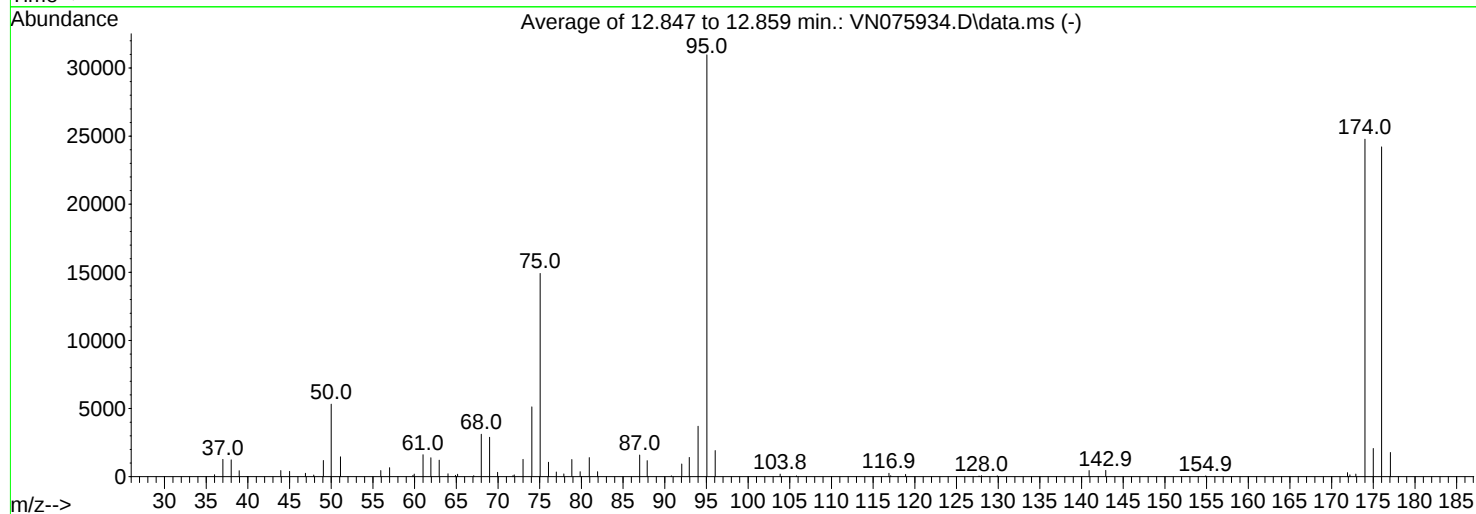


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN122222\
 Data File : VN075934.D
 Acq On : 22 Dec 2022 10:07
 Operator : JC\MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N121422W.M
 Title : SW846 8260
 Last Update : Wed Dec 14 13:03:41 2022

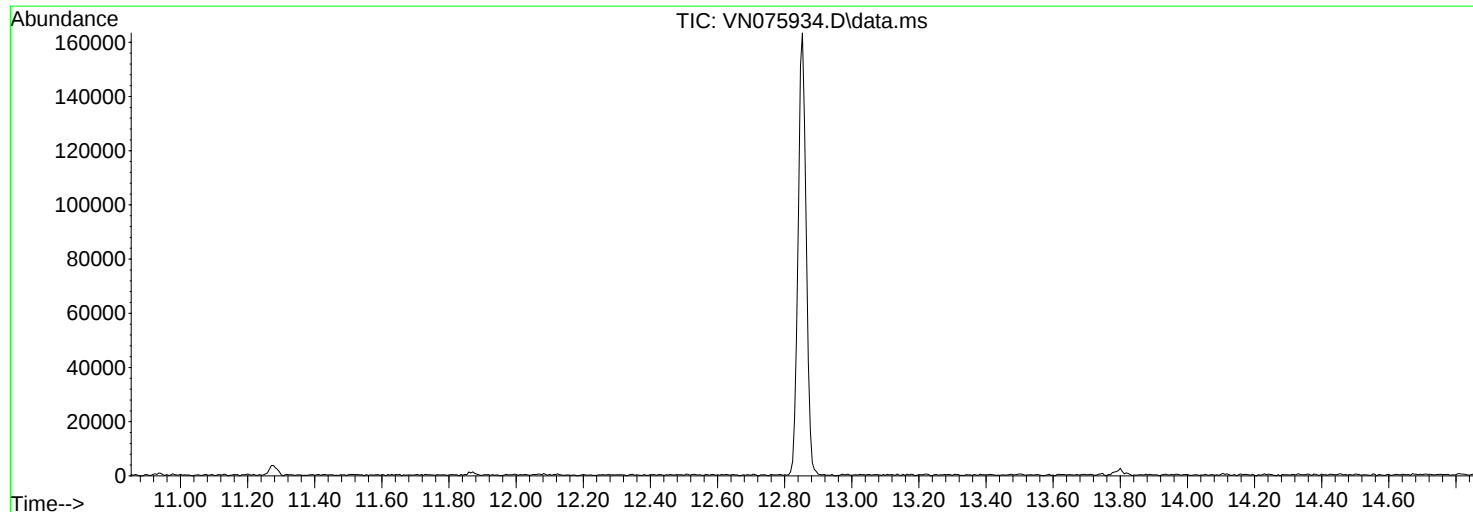

AutoFind: Scans 1835, 1836, 1837; Background Corrected with Scan 1826

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.2	5327	PASS
75	95	30	60	48.2	14924	PASS
95	95	100	100	100.0	30968	PASS
96	95	5	9	6.2	1914	PASS
173	174	0.00	2	0.8	194	PASS
174	95	50	100	80.0	24771	PASS
175	174	5	9	8.4	2073	PASS
176	174	95	101	97.7	24208	PASS
177	176	5	9	7.3	1779	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.00	139	51.10	1456	67.10	65	77.90	201
37.00	1268	55.95	447	68.00	3118	78.85	125
38.00	1238	57.00	662	69.00	2888	79.85	36
38.95	440	59.80	95	69.95	313	80.95	140
39.90	0	59.95	183	71.80	67	81.95	359
43.95	451	61.00	1610	71.95	133	87.00	1589
45.00	391	61.95	1381	73.00	1274	87.90	1170
46.90	247	62.95	1209	74.05	5125	90.80	63
47.90	123	64.00	206	75.05	14924	92.05	923
49.05	1188	64.90	89	76.05	1063	92.95	1406
50.00	5327	65.15	173	77.00	342	94.00	3704

Average of 12.847 to 12.859 min.: VN075934.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
95.05	30968	142.90	454				
96.05	1914	154.90	59				
103.85	187	171.90	289				
105.80	58	172.20	130				
116.90	244	172.90	194				
117.10	65	174.00	24771				
118.90	163	175.00	2073				
127.70	53	176.00	24208				
128.00	69	177.05	1779				
129.90	55						
140.90	447						

Instrument :

MSVOA_N

ClientSampleId :

BFB