
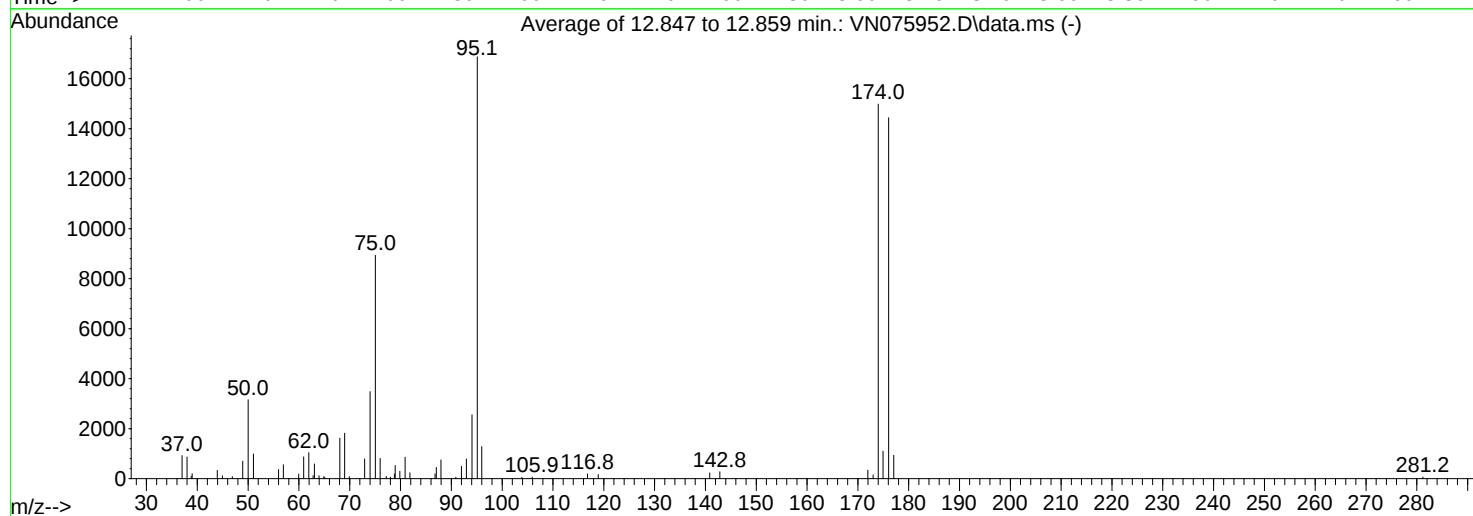


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN122322\
Data File : VN075952.D
Acq On : 23 Dec 2022 08:45
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N121422W.M
Title : SW846 8260
Last Update : Wed Dec 14 13:03:41 2022

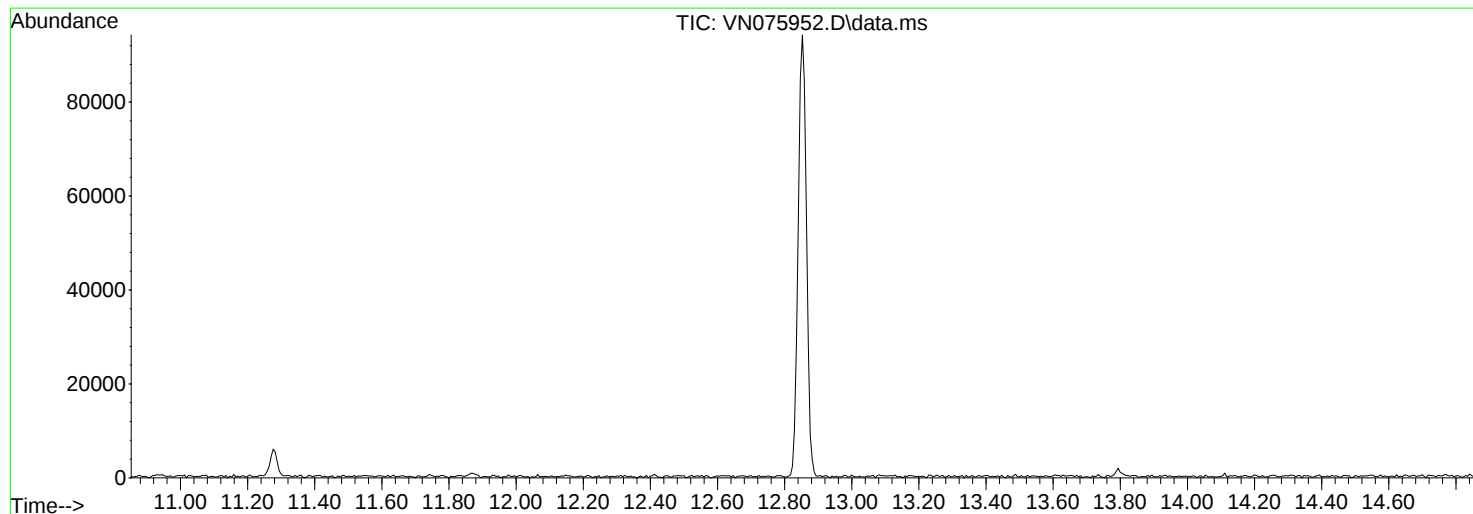

AutoFind: Scans 1835, 1836, 1837; Background Corrected with Scan 1827

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.7	3158	PASS
75	95	30	60	53.0	8938	PASS
95	95	100	100	100.0	16872	PASS
96	95	5	9	7.6	1280	PASS
173	174	0.00	2	1.0	145	PASS
174	95	50	100	88.8	14986	PASS
175	174	5	9	7.3	1100	PASS
176	174	95	101	96.4	14440	PASS
177	176	5	9	6.5	932	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
37.00	922	56.95	557	69.90	84	81.85	23
38.00	863	59.95	188	72.95	787	86.80	19
38.80	99	60.95	871	74.00	3481	87.05	44
39.00	201	61.95	1038	75.05	8938	87.95	74
43.95	331	62.80	121	76.00	807	90.90	56
44.95	114	63.05	586	77.20	90	92.00	494
46.90	82	63.95	113	78.00	58	92.95	786
48.95	700	64.90	84	78.80	183	94.05	2553
50.00	3158	65.10	51	78.95	523	95.10	16872
51.05	984	68.05	1621	79.85	293	96.00	1280
56.00	365	69.00	1820	80.90	855	103.90	54

Average of 12.847 to 12.859 min.: VN075952.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
105.90	65	281.20	62				
116.80	190						
118.90	169						
140.85	232						
142.85	278						
171.95	341						
173.00	145						
174.00	14986						
174.95	1100						
176.05	14440						
177.05	932						

Instrument :

MSVOA_N

ClientSampleId :

BFB