
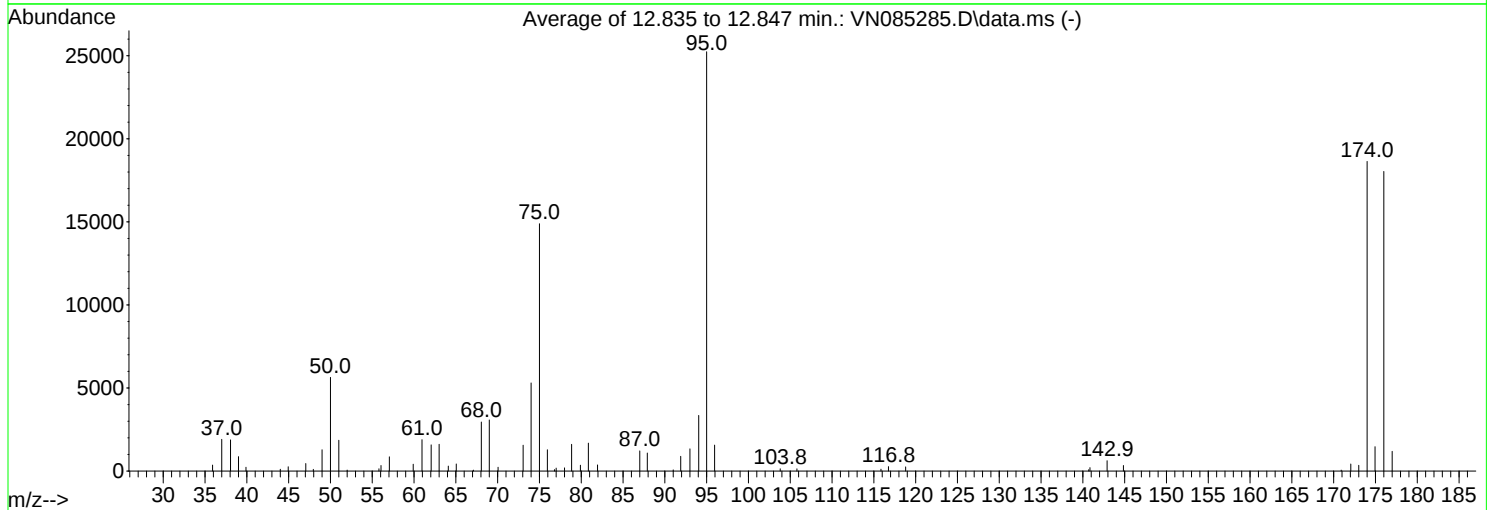


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN122324\
Data File : VN085285.D
Acq On : 23 Dec 2024 10:14
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N121824W.M
Title : SW846 8260
Last Update : Thu Dec 19 06:31:00 2024

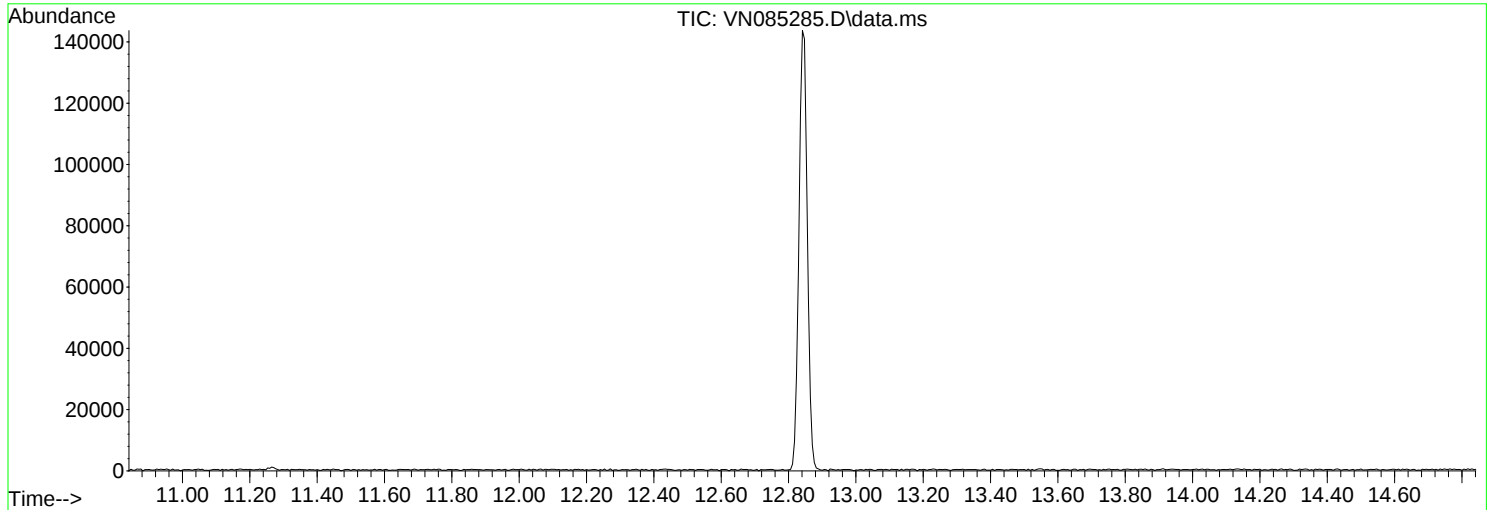

AutoFind: Scans 1850, 1851, 1852; Background Corrected with Scan 1843

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.3	5640	PASS
75	95	30	60	59.0	14888	PASS
95	95	100	100	100.0	25240	PASS
96	95	5	9	6.2	1562	PASS
173	174	0.00	2	1.9	348	PASS
174	95	50	100	73.8	18638	PASS
175	174	5	9	7.9	1468	PASS
176	174	95	101	96.8	18033	PASS
177	176	5	9	6.6	1188	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.90	362	51.00	1855	67.10	57	78.85	1609
37.00	1910	52.00	62	68.05	2954	79.90	354
38.05	1877	55.80	140	69.00	3077	80.85	1685
39.00	870	56.05	335	70.05	231	81.95	371
39.90	232	57.05	858	73.05	1557	87.00	1213
44.00	110	59.90	412	74.00	5305	87.90	1086
44.95	261	60.95	1889	75.00	14888	91.00	71
47.05	455	62.05	1578	75.95	1282	91.90	887
47.95	103	63.00	1611	76.80	86	93.00	1337
49.00	1283	64.10	300	77.00	178	94.05	3350
50.00	5640	65.05	428	78.00	193	95.00	25240

Average of 12.835 to 12.847 min.: VN085285.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
95.95	1562	172.05	426				
103.80	140	173.00	348				
105.80	135	174.00	18638				
115.85	117	174.95	1468				
116.75	268	176.00	18033				
118.80	251	177.00	1188				
140.70	83						
140.85	207						
142.90	623						
144.85	336						
170.90	58						

Instrument :

MSVOA_N

ClientSampleId :

BFB