
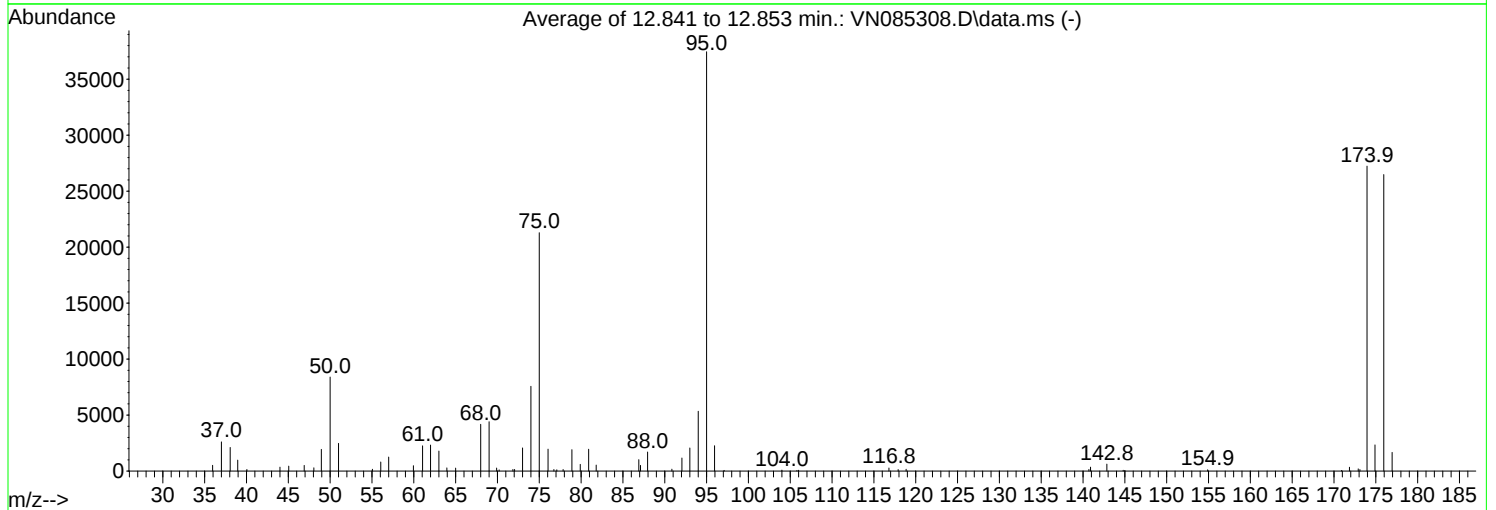


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN122624\
Data File : VN085308.D
Acq On : 26 Dec 2024 08:41
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N121824W.M
Title : SW846 8260
Last Update : Thu Dec 19 06:31:00 2024

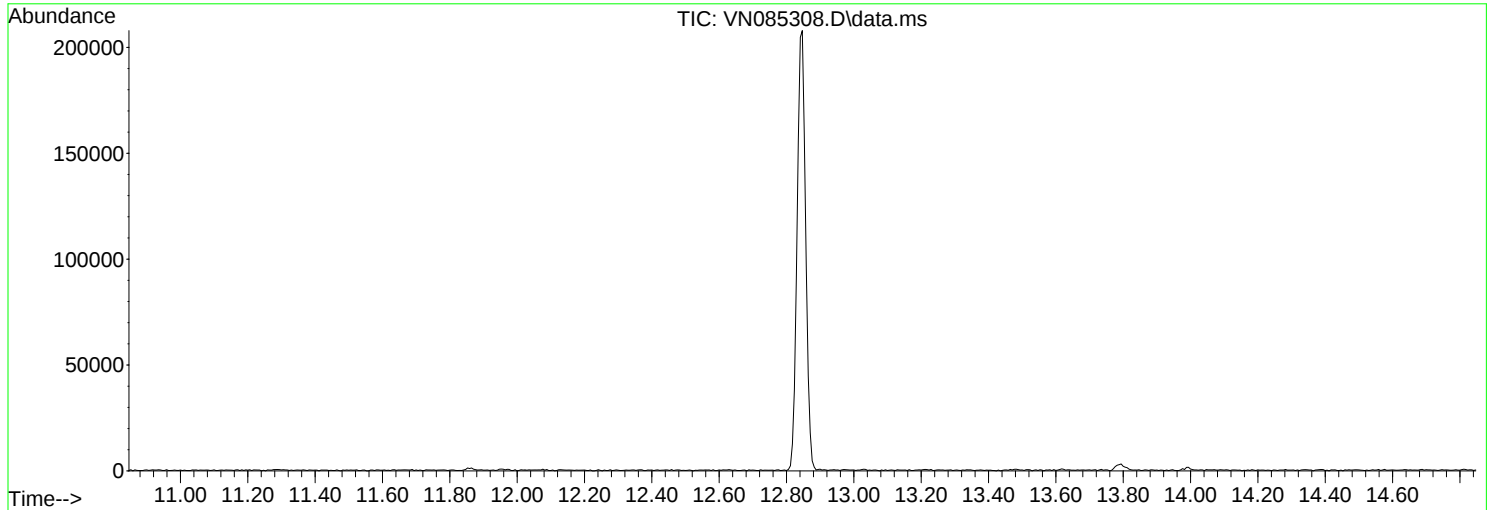

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1842

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.4	8398	PASS
75	95	30	60	56.8	21291	PASS
95	95	100	100	100.0	37453	PASS
96	95	5	9	6.0	2262	PASS
173	174	0.00	2	0.7	197	PASS
174	95	50	100	72.7	27237	PASS
175	174	5	9	8.6	2338	PASS
176	174	95	101	97.2	26483	PASS
177	176	5	9	6.3	1666	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.95	516	51.00	2472	69.00	4408	77.85	142
37.00	2608	55.05	165	69.90	272	78.90	1913
38.05	2111	56.05	810	70.20	106	79.90	600
38.95	978	57.00	1250	71.85	144	80.90	1953
40.05	149	59.95	482	72.05	147	81.80	535
44.00	351	61.05	2257	73.00	2068	86.90	1021
45.05	443	62.00	2324	74.00	7571	87.10	509
46.90	504	63.00	1789	75.00	21291	87.95	1700
48.05	292	63.95	284	76.05	1960	90.85	170
48.95	1939	65.00	266	76.75	140	92.05	1168
50.00	8398	68.00	4176	77.10	117	93.00	2063

Average of 12.841 to 12.853 min.: VN085308.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
94.00	5342	140.90	352	175.95	26483		
95.00	37453	142.85	623	176.95	1666		
95.95	2262	144.80	73				
97.10	60	145.00	58				
104.00	86	154.90	119				
105.80	57	170.90	51				
106.00	74	171.85	345				
116.80	274	172.90	197				
117.90	136	173.10	137				
118.85	162	173.95	27237				
140.70	151	174.90	2338				

Instrument :

MSVOA_N

ClientSampleId :

BFB