

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN122722\
 Data File : VN075981.D
 Acq On : 27 Dec 2022 12:23
 Operator : JC\MD
 Sample : N6206-01 10X
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 MW-1

Quant Time: Dec 28 04:44:16 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N121422W.M
 Quant Title : SW846 8260
 QLast Update : Wed Dec 14 13:03:41 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.230	168	324345	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.106	114	502760	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.870	117	441102	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.794	152	204367	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.588	65	163853	46.436	ug/l	0.00
Spiked Amount 50.000	Range 74 - 125		Recovery =	92.880%		
35) Dibromofluoromethane	8.177	113	150811	48.437	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery =	96.880%		
50) Toluene-d8	10.571	98	573383	49.255	ug/l	0.00
Spiked Amount 50.000	Range 86 - 113		Recovery =	98.520%		
62) 4-Bromofluorobenzene	12.853	95	190206	49.332	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery =	98.660%		
Target Compounds						Qvalue
11) Tert butyl alcohol	5.506	59	872	1.746	ug/l #	72
16) Acetone	4.459	43	1155	0.950	ug/l #	39
18) Methyl Acetate	5.053	43	747	0.208	ug/l #	74
20) Methylene Chloride	5.283	84	892	Below Cal	#	85
31) Cyclohexane	8.230	56	8476	1.677	ug/l #	10
36) 1,1-Dichloropropene	8.230	75	23075	5.579	ug/l #	48
37) Ethyl Acetate	7.512	43	691	0.208	ug/l #	65
38) Carbon Tetrachloride	8.230	117	32116	6.938	ug/l #	18
39) Methylcyclohexane	9.600	83	6225	1.248	ug/l #	89
40) Benzene	8.612	78	3297	0.258	ug/l #	82
48) Methyl methacrylate	9.600	41	2618	1.061	ug/l #	61
51) 4-Methyl-2-Pentanone	10.453	43	942	0.284	ug/l #	32
55) 1,1,2-Trichloroethane	11.012	97	1014	0.311	ug/l #	16
59) 2-Hexanone	11.200	43	1698	0.703	ug/l	88
67) Ethyl Benzene	11.965	91	17527	1.147	ug/l	95
68) m/p-Xylenes	12.070	106	2012	0.333	ug/l	96
69) o-Xylene	12.400	106	1206	0.202	ug/l	89
73) Isopropylbenzene	12.700	105	25603	1.734	ug/l	97
76) 1,2,3-Trichloropropane	12.853	75	96959	23.536	ug/l #	1
78) n-propylbenzene	13.041	91	52657	3.233	ug/l	99
79) 2-Chlorotoluene	13.217	91	2087	0.205	ug/l	96
81) trans-1,4-Dichloro-2-b...	12.853	75	96959	84.719	ug/l #	12
82) 4-Chlorotoluene	13.217	91	2087	0.205	ug/l	96
84) 1,2,4-Trimethylbenzene	13.482	105	4328	0.353	ug/l	87
85) sec-Butylbenzene	13.617	105	18484	1.229	ug/l	87
86) p-Isopropyltoluene	13.729	119	5507	0.440	ug/l	93
87) 1,3-Dichlorobenzene	13.735	146	2199	0.319	ug/l	91
88) 1,4-Dichlorobenzene	13.735	146	2199	0.312	ug/l	89
89) n-Butylbenzene	14.059	91	15515	1.530	ug/l #	79
90) Hexachloroethane	14.335	117	7823	3.494	ug/l #	11
91) 1,2-Dichlorobenzene	14.106	146	2265	0.333	ug/l	94
92) 1,2-Dibromo-3-Chloropr...	14.735	75	165	0.204	ug/l #	12
93) 1,2,4-Trichlorobenzene	15.388	180	3307	0.982	ug/l #	90
95) Naphthalene	15.647	128	94984	10.346	ug/l	99
96) 1,2,3-Trichlorobenzene	15.841	180	3424	1.088	ug/l #	85

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN122722\
Data File : VN075981.D
Acq On : 27 Dec 2022 12:23
Operator : JC\MD
Sample : N6206-01 10X
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
MW-1

Quant Time: Dec 28 04:44:16 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N121422W.M
Quant Title : SW846 8260
QLast Update : Wed Dec 14 13:03:41 2022
Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
----------	------	------	----------	------	-------	----------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN122722\
Data File : VN075981.D
Acq On : 27 Dec 2022 12:23
Operator : JC\MD
Sample : N6206-01 10X
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
MW-1

Quant Time: Dec 28 04:44:16 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N121422W.M
Quant Title : SW846 8260
QLast Update : Wed Dec 14 13:03:41 2022
Response via : Initial Calibration




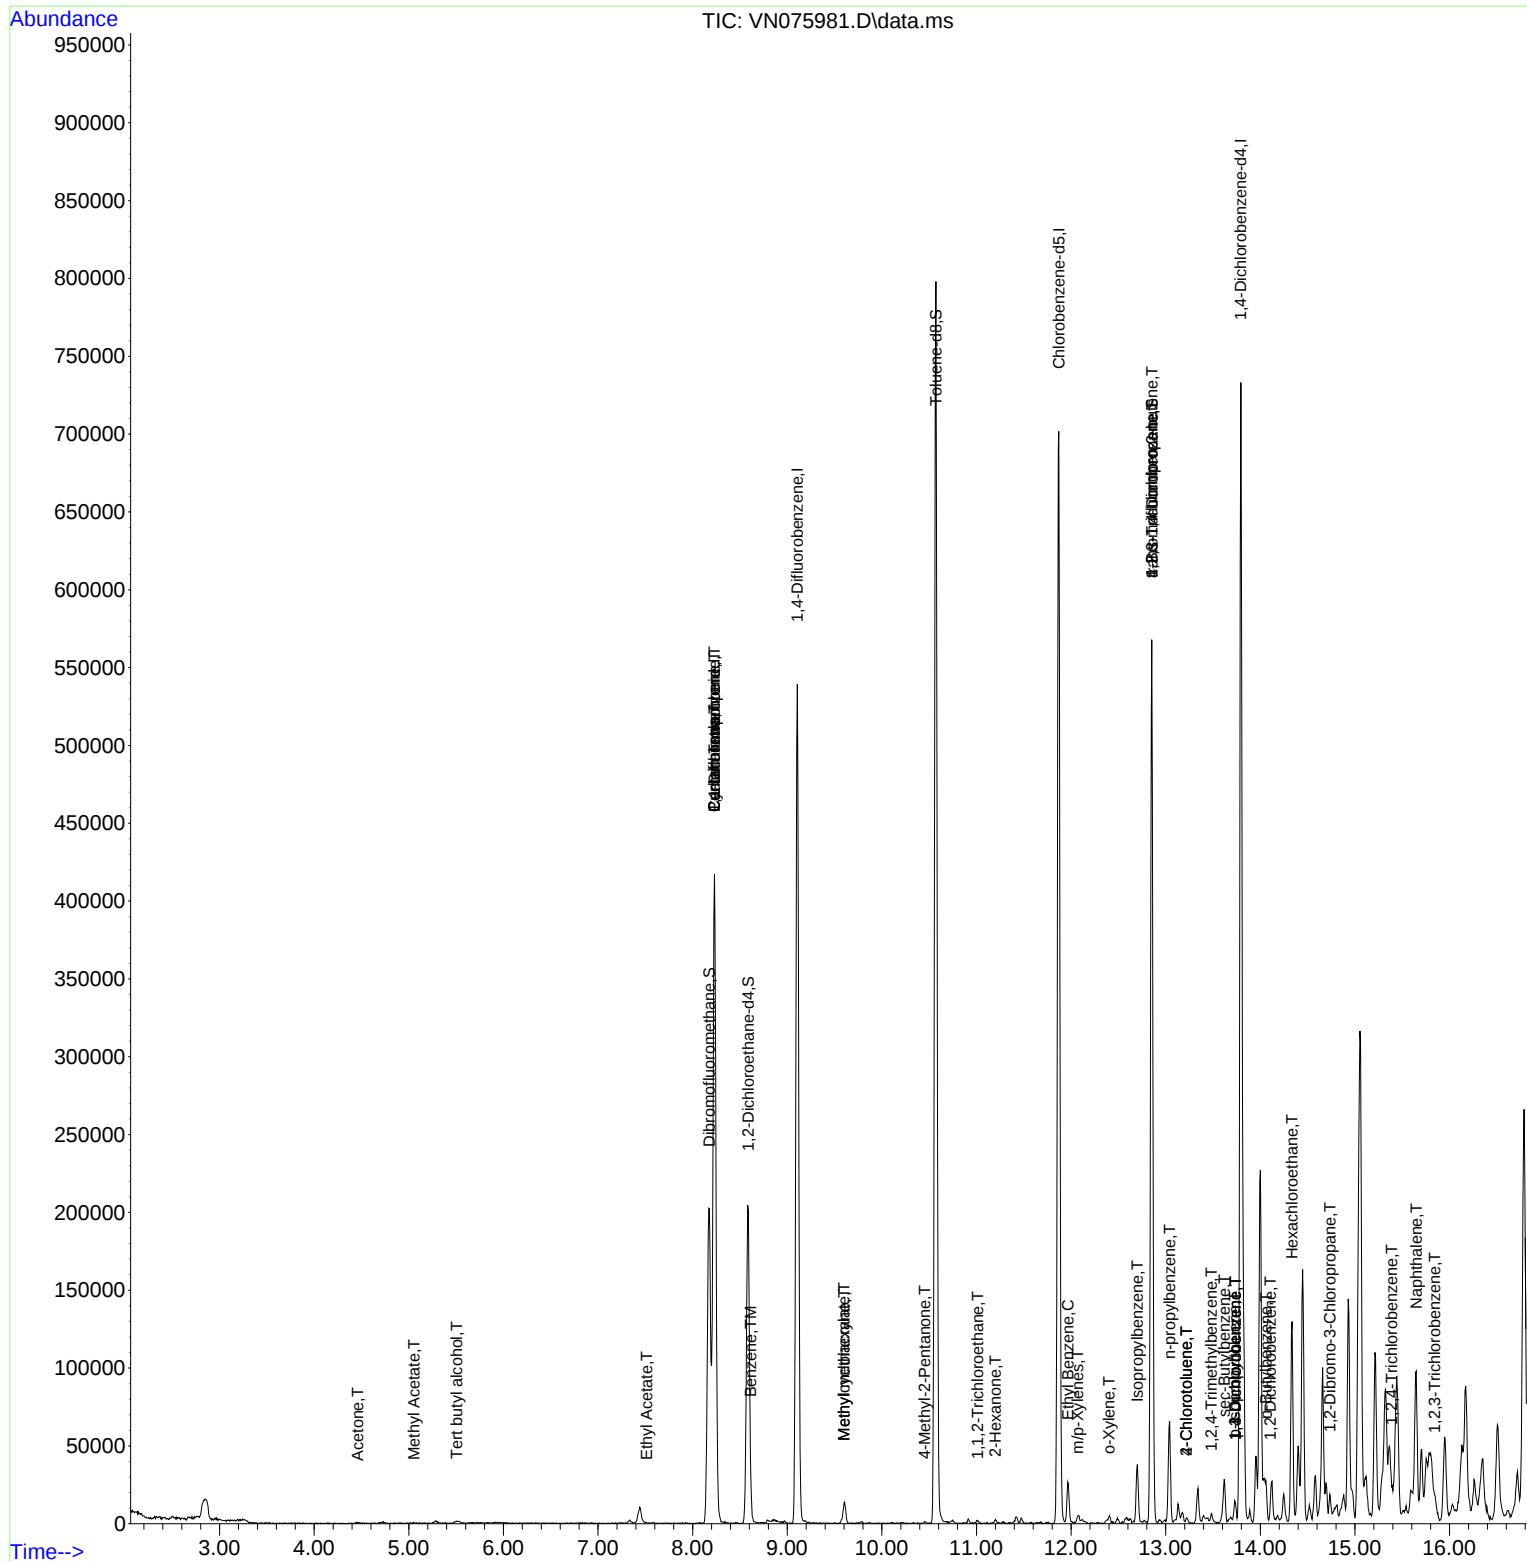




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.230 min Scan# 10
Delta R.T. -0.000 min
Lab File: VN075981.D
Acq: 27 Dec 2022 12:23




Instrument :
MSVOA_N
ClientSampleId :
MW-1


Tgt Ion:168 Resp: 324345
Ion Ratio Lower Upper
168 100
99 55.1 44.2 66.4

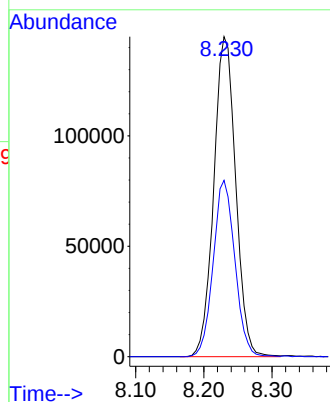

#11
Tert butyl alcohol
Concen: 1.746 ug/l
RT: 5.506 min Scan# 587
Delta R.T. -0.029 min
Lab File: VN075981.D
Acq: 27 Dec 2022 12:23

Tgt Ion: 59 Resp: 872
Ion Ratio Lower Upper
59 100
57 0.0 8.2 12.4#


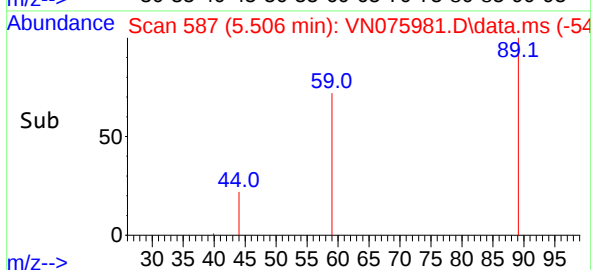






#16
Acetone
Concen: 0.950 ug/l
RT: 4.459 min Scan# 406
Delta R.T. 0.018 min
Lab File: VN075981.D
Acq: 27 Dec 2022 12:23




Instrument :
MSVOA_N
ClientSampleId :
MW-1


Tgt Ion: 43 Resp: 1155
Ion Ratio Lower Upper
43 100
58 0.0 28.6 43.0#

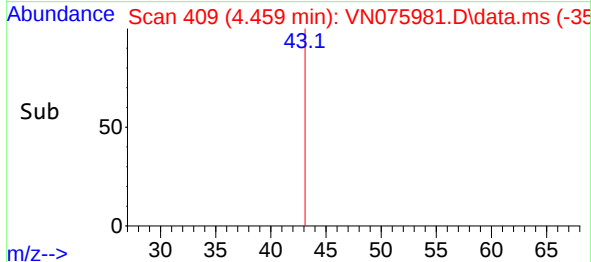

#18
Methyl Acetate
Concen: 0.208 ug/l
RT: 5.053 min Scan# 510
Delta R.T. 0.018 min
Lab File: VN075981.D
Acq: 27 Dec 2022 12:23

Tgt Ion: 43 Resp: 747
Ion Ratio Lower Upper
43 100
74 15.7 23.6 35.4#

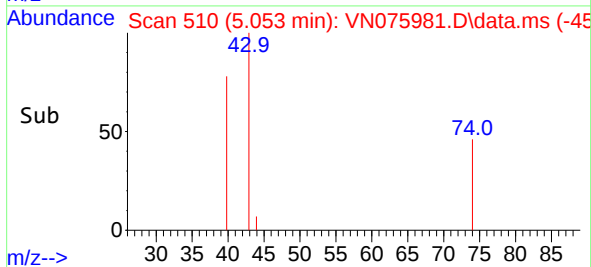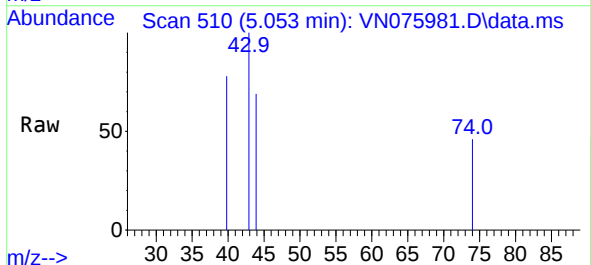







#20
Methylene Chloride
Concen: Below Cal
RT: 5.283 min Scan# 54
Delta R.T. -0.006 min
Lab File: VN075981.D
Acq: 27 Dec 2022 12:23

Instrument :
MSVOA_N
ClientSampleId :
MW-1

Tgt Ion: 84 Resp: 892




Ion	Ratio	Lower	Upper
84	100		
49	80.9	81.8	122.6#
51	32.1	26.7	40.1
86	55.7	51.5	77.3




#31
Cyclohexane
Concen: 1.677 ug/l
RT: 8.230 min Scan# 1050
Delta R.T. -0.035 min
Lab File: VN075981.D
Acq: 27 Dec 2022 12:23

Tgt Ion: 56 Resp: 8476

Ion	Ratio	Lower	Upper
56	100		
69	153.0	24.7	37.1#
84	141.2	76.5	114.7#

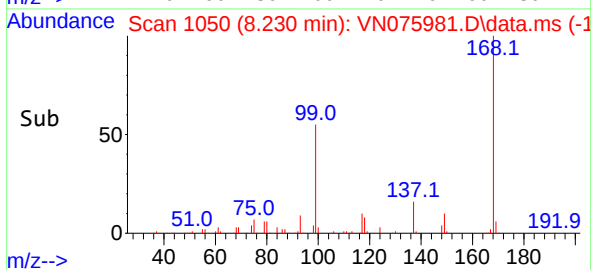

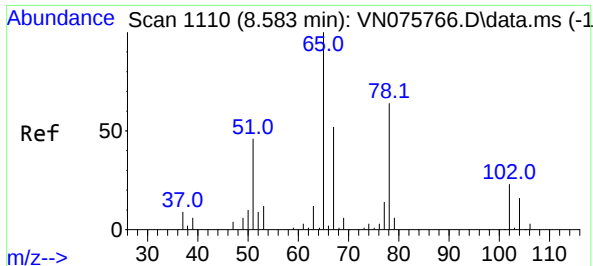

#33

1,2-Dichloroethane-d4

Concen: 46.436 ug/l

RT: 8.588 min Scan# 1110

Delta R.T. 0.006 min

Lab File: VN075981.D

Acq: 27 Dec 2022 12:23

Instrument :

MSVOA_N

ClientSampleId :





MW-1

Tgt Ion: 65 Resp: 163853

Ion Ratio Lower Upper

65 100

67 52.5 0.0 103.4

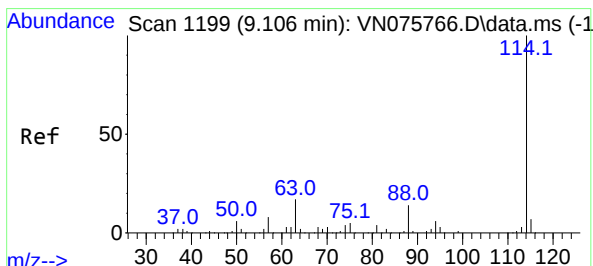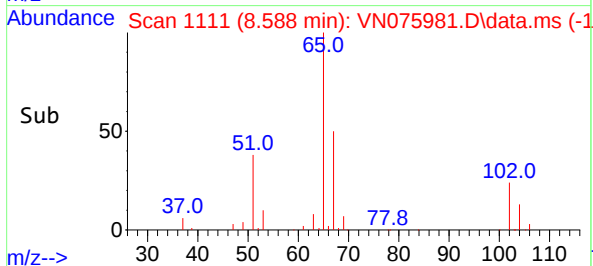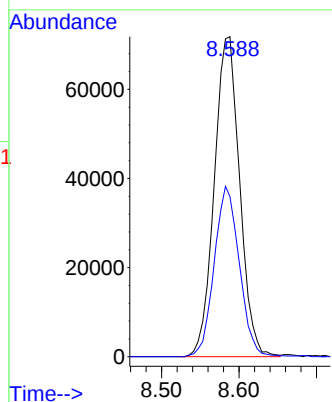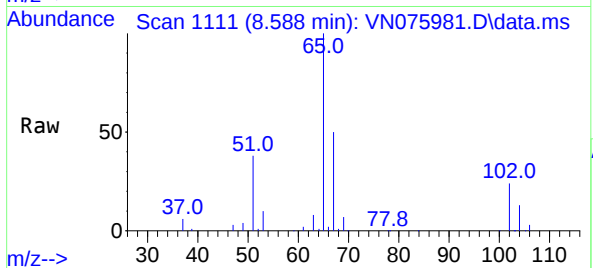

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 9.106 min Scan# 1199

Delta R.T. -0.000 min

Lab File: VN075981.D

Acq: 27 Dec 2022 12:23




Tgt Ion: 114 Resp: 502760


Ion Ratio Lower Upper

114 100

63 17.6 0.0 34.4

88 14.8 0.0 28.8


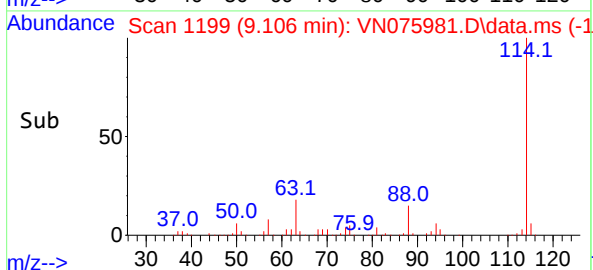

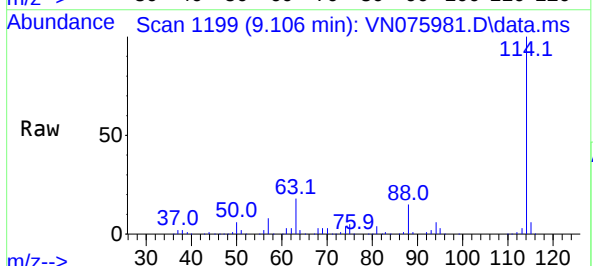


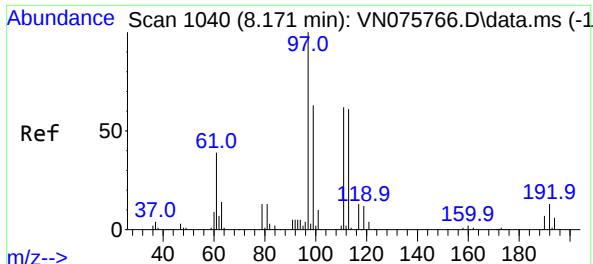

#35
Dibromofluoromethane
Concen: 48.437 ug/l
RT: 8.177 min Scan# 1040
Delta R.T. 0.006 min
Lab File: VN075981.D
Acq: 27 Dec 2022 12:23




Instrument :
MSVOA_N
ClientSampleId :
MW-1


Tgt Ion:113 Resp: 150811
Ion Ratio Lower Upper
113 100
111 101.7 83.4 125.2
192 19.6 16.1 24.1

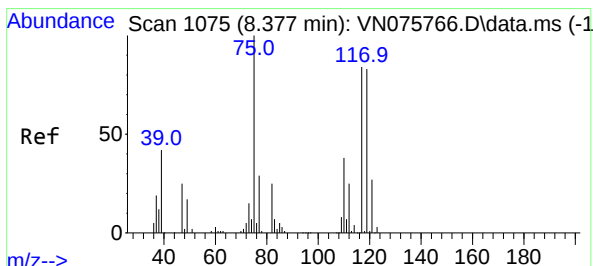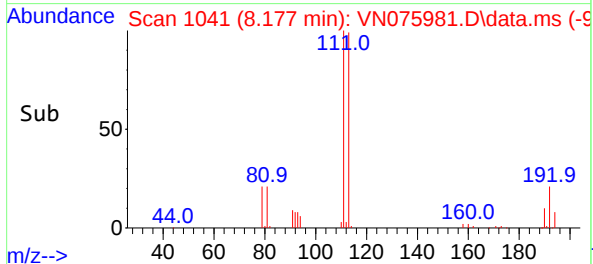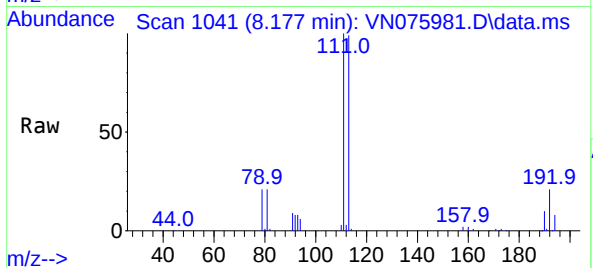

#36
1,1-Dichloropropene
Concen: 5.579 ug/l
RT: 8.230 min Scan# 1050
Delta R.T. -0.147 min
Lab File: VN075981.D
Acq: 27 Dec 2022 12:23

Tgt Ion: 75 Resp: 23075
Ion Ratio Lower Upper
75 100
110 8.0 18.8 56.4#
77 0.0 24.1 36.1#


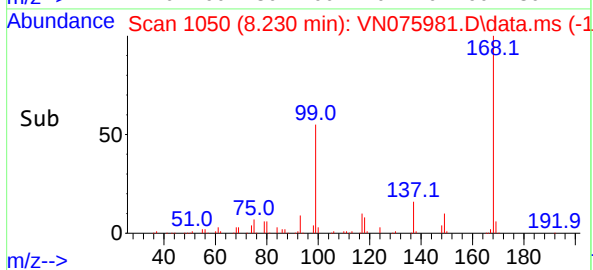

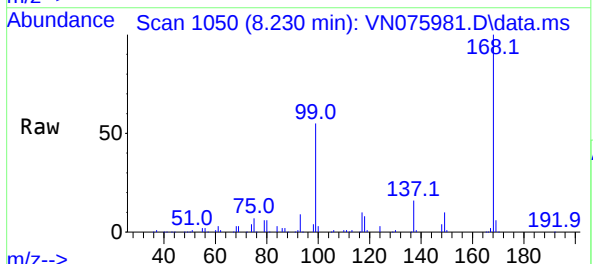




#37
Ethyl Acetate
Concen: 0.208 ug/l
RT: 7.512 min Scan# 91
Delta R.T. -0.053 min
Lab File: VN075981.D
Acq: 27 Dec 2022 12:23




Instrument :
MSVOA_N
ClientSampleId :
MW-1


Tgt Ion: 43 Resp: 691
Ion Ratio Lower Upper
43 100
61 0.0 13.0 19.4#
70 0.0 9.4 14.0#



#38
Carbon Tetrachloride
Concen: 6.938 ug/l
RT: 8.230 min Scan# 1050
Delta R.T. -0.135 min
Lab File: VN075981.D
Acq: 27 Dec 2022 12:23

Tgt Ion: 117 Resp: 32116
Ion Ratio Lower Upper
117 100
119 7.2 76.1 114.1#
121 0.0 24.5 36.7#

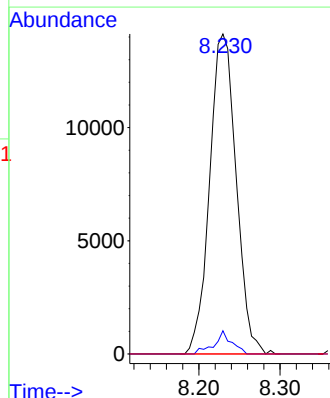

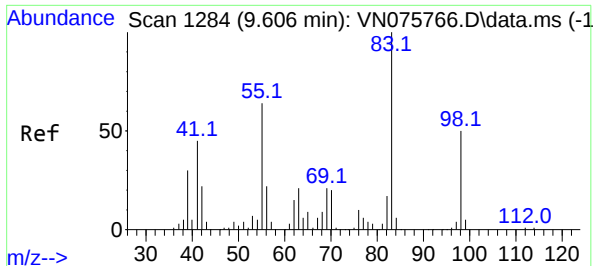

#39

Methylcyclohexane

Concen: 1.248 ug/l

RT: 9.600 min Scan# 11

Delta R.T. -0.006 min

Lab File: VN075981.D

Acq: 27 Dec 2022 12:23

Instrument :

MSVOA_N

ClientSampleId :

MW-1





Tgt Ion: 83 Resp: 6225

Ion Ratio Lower Upper

83 100

55 50.7 51.4 77.0#

98 48.0 39.8 59.8

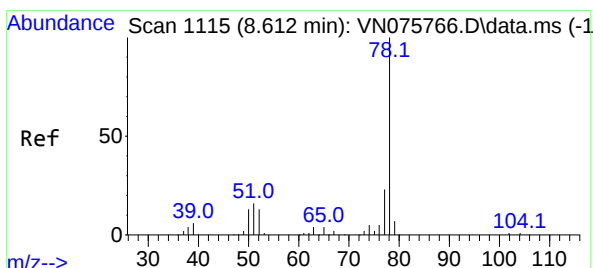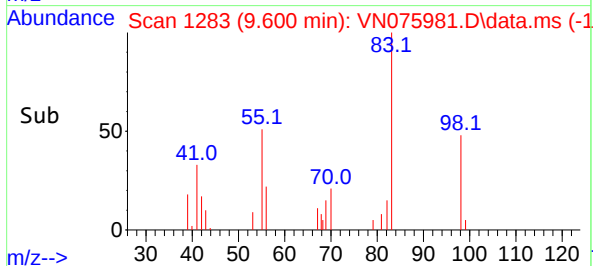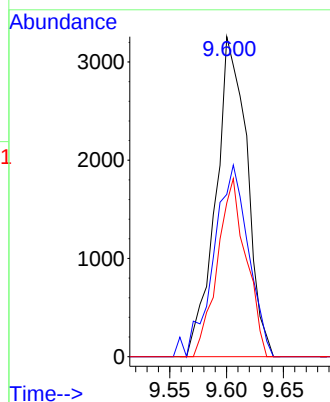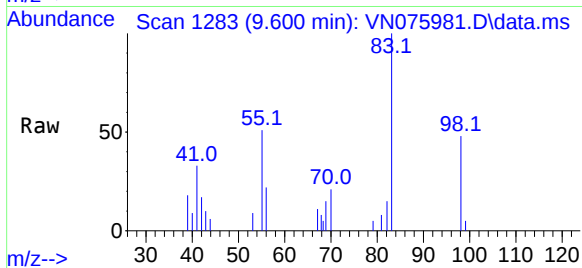

#40

Benzene

Concen: 0.258 ug/l

RT: 8.612 min Scan# 1115

Delta R.T. -0.000 min

Lab File: VN075981.D




Acq: 27 Dec 2022 12:23


Tgt Ion: 78 Resp: 3297

Ion Ratio Lower Upper

78 100

77 14.4 18.5 27.7#

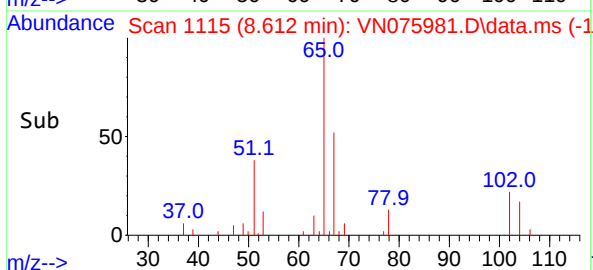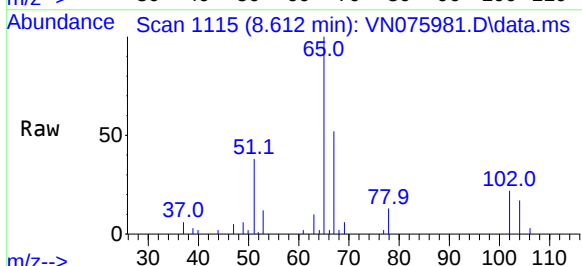

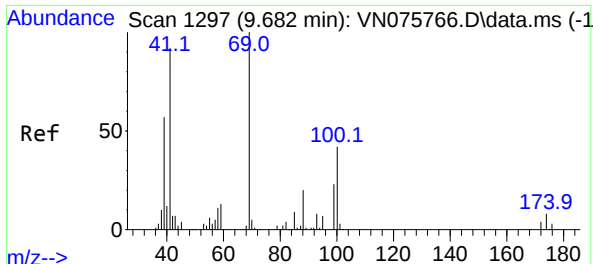

#48

Methyl methacrylate

Concen: 1.061 ug/l

RT: 9.600 min Scan# 11

Delta R.T. -0.082 min

Lab File: VN075981.D

Acq: 27 Dec 2022 12:23

Instrument :

MSVOA_N

ClientSampleId :

MW-1





Tgt Ion: 41 Resp: 2618

Ion Ratio Lower Upper

41 100

69 40.5 81.9 122.9#

39 62.3 51.6 77.4

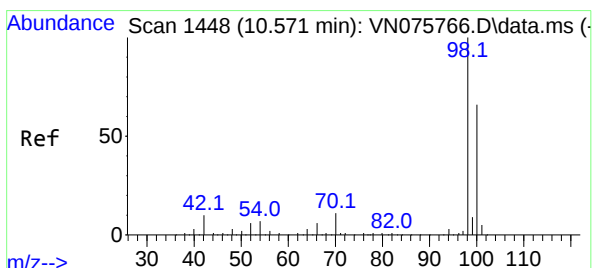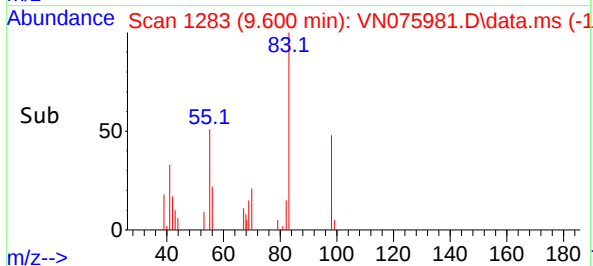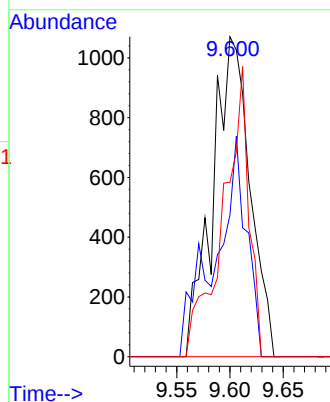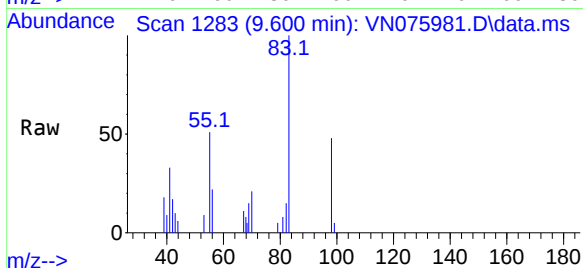

#50

Toluene-d8

Concen: 49.255 ug/l

RT: 10.571 min Scan# 1448

Delta R.T. -0.000 min

Lab File: VN075981.D




Acq: 27 Dec 2022 12:23


Tgt Ion: 98 Resp: 573383

Ion Ratio Lower Upper

98 100

100 65.6 52.1 78.1


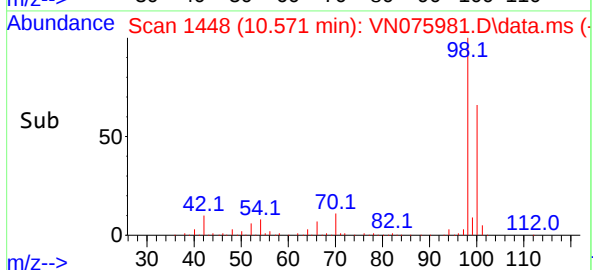

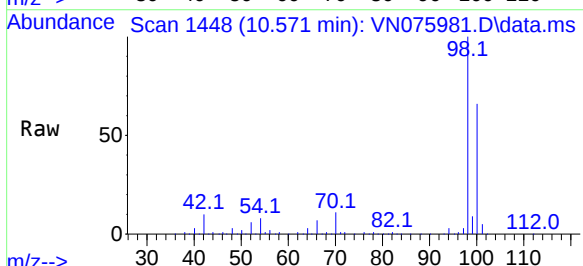




#51
4-Methyl-2-Pentanone
Concen: 0.284 ug/l
RT: 10.453 min Scan# 1428
Delta R.T. 0.006 min
Lab File: VN075981.D
Acq: 27 Dec 2022 12:23




Instrument :
MSVOA_N
ClientSampleId :
MW-1


Tgt Ion: 43 Resp: 942
Ion Ratio Lower Upper
43 100
58 0.0 35.5 53.3#

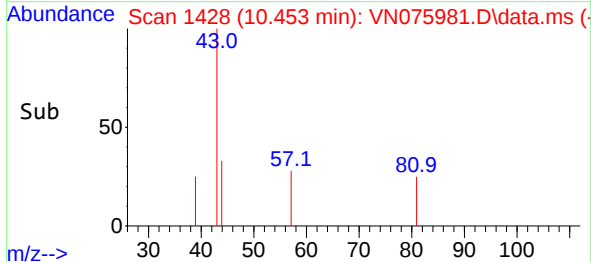

#55
1,1,2-Trichloroethane
Concen: 0.311 ug/l
RT: 11.012 min Scan# 1523
Delta R.T. -0.006 min
Lab File: VN075981.D
Acq: 27 Dec 2022 12:23

Tgt Ion: 97 Resp: 1014
Ion Ratio Lower Upper
97 100
83 0.0 65.0 97.4#
85 0.0 43.0 64.6#
99 0.0 50.2 75.2#


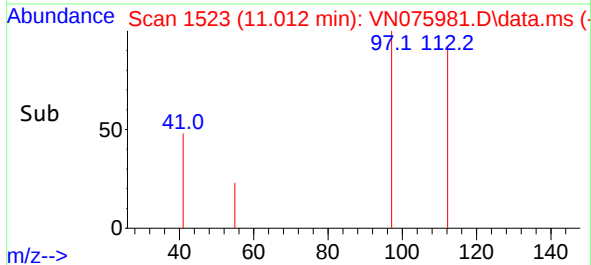

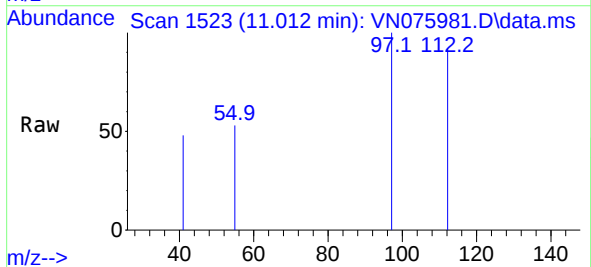




#59
2-Hexanone
Concen: 0.703 ug/l
RT: 11.200 min Scan# 11
Delta R.T. -0.000 min
Lab File: VN075981.D
Acq: 27 Dec 2022 12:23




Instrument :
MSVOA_N
ClientSampleId :
MW-1


Tgt Ion: 43 Resp: 1698
Ion Ratio Lower Upper
43 100
58 51.8 30.6 92.0



#62
4-Bromofluorobenzene
Concen: 49.332 ug/l
RT: 12.853 min Scan# 1836
Delta R.T. -0.000 min
Lab File: VN075981.D
Acq: 27 Dec 2022 12:23

Tgt Ion: 95 Resp: 190206
Ion Ratio Lower Upper
95 100
174 86.8 0.0 171.6
176 84.5 0.0 169.2



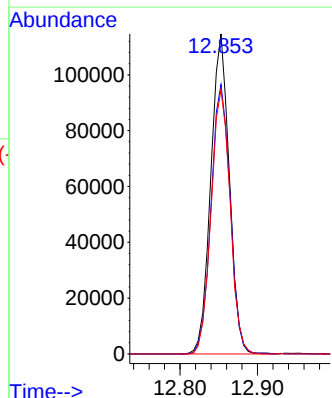





#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.870 min Scan# 117
Delta R.T. 0.006 min
Lab File: VN075981.D
Acq: 27 Dec 2022 12:23




Instrument :
MSVOA_N
ClientSampleId :
MW-1


Tgt Ion:117 Resp: 441102
Ion Ratio Lower Upper
117 100
82 50.4 41.3 61.9
119 31.5 24.6 37.0

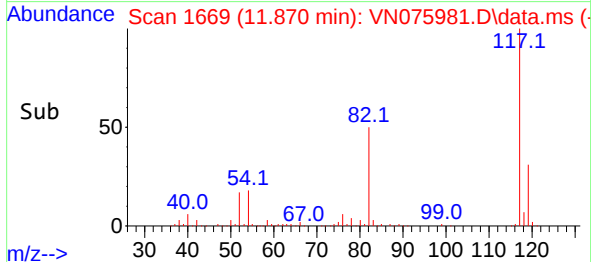

#67
Ethyl Benzene
Concen: 1.147 ug/l
RT: 11.965 min Scan# 1685
Delta R.T. -0.000 min
Lab File: VN075981.D
Acq: 27 Dec 2022 12:23

Tgt Ion: 91 Resp: 17527
Ion Ratio Lower Upper
91 100
106 29.4 25.7 38.5


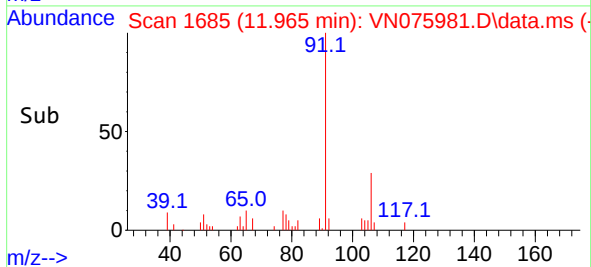

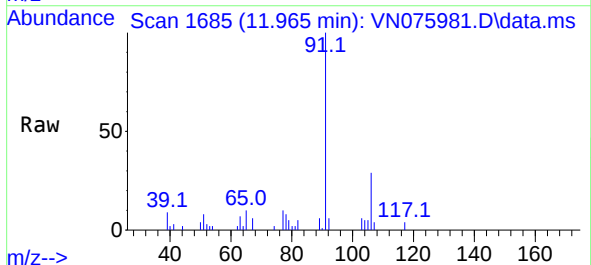




#68
m/p-Xylenes
Concen: 0.333 ug/l
RT: 12.070 min Scan# 11
Delta R.T. -0.006 min
Lab File: VN075981.D
Acq: 27 Dec 2022 12:23




Instrument :
MSVOA_N
ClientSampleId :
MW-1


Tgt Ion:106 Resp: 2012
Ion Ratio Lower Upper
106 100
91 201.7 156.6 235.0

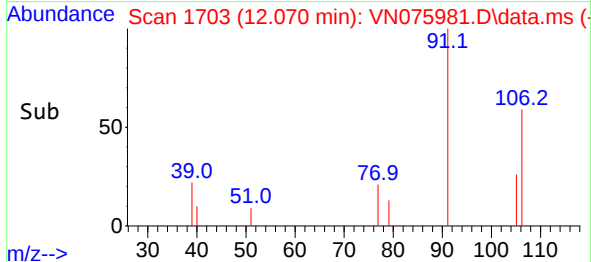

#69
o-Xylene
Concen: 0.202 ug/l
RT: 12.400 min Scan# 1759
Delta R.T. -0.000 min
Lab File: VN075981.D
Acq: 27 Dec 2022 12:23

Tgt Ion:106 Resp: 1206
Ion Ratio Lower Upper
106 100
91 190.0 103.8 311.6


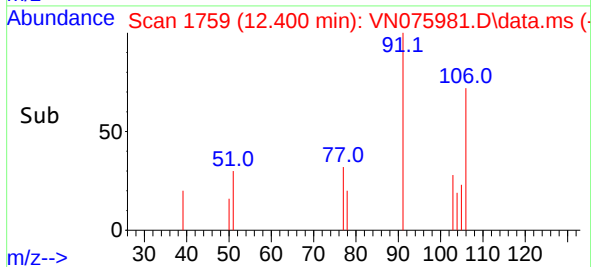

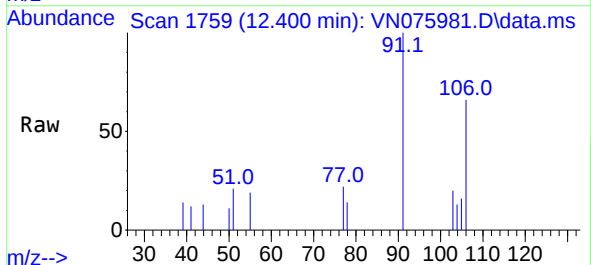




#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.794 min Scan# 1996
Delta R.T. -0.000 min
Lab File: VN075981.D
Acq: 27 Dec 2022 12:23




Instrument :
MSVOA_N
ClientSampleId :
MW-1


Tgt Ion:152 Resp: 204367
Ion Ratio Lower Upper
152 100
115 59.1 29.1 87.4
150 157.8 0.0 347.0

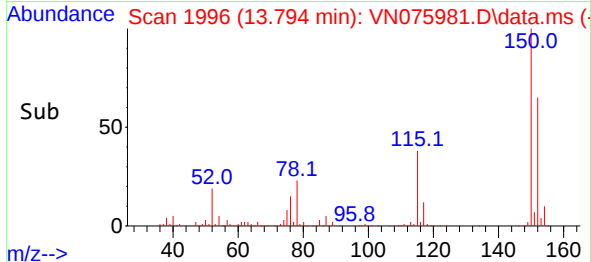

#73
Isopropylbenzene
Concen: 1.734 ug/l
RT: 12.700 min Scan# 1810
Delta R.T. -0.000 min
Lab File: VN075981.D
Acq: 27 Dec 2022 12:23

Tgt Ion:105 Resp: 25603
Ion Ratio Lower Upper
105 100
120 28.4 13.4 40.2



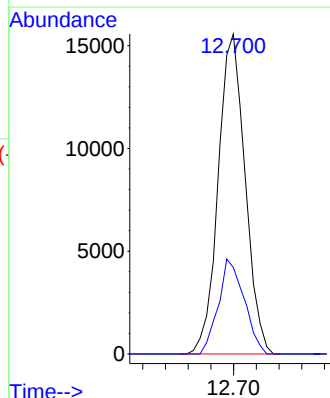





#76
1,2,3-Trichloropropane
Concen: 23.536 ug/l
RT: 12.853 min Scan# 1836
Delta R.T. -0.141 min
Lab File: VN075981.D
Acq: 27 Dec 2022 12:23




Instrument :
MSVOA_N
ClientSampleId :
MW-1


Tgt Ion: 75 Resp: 96959
Ion Ratio Lower Upper
75 100
77 1.1 82.6 247.8#



#78
n-propylbenzene
Concen: 3.233 ug/l
RT: 13.041 min Scan# 1868
Delta R.T. -0.000 min
Lab File: VN075981.D
Acq: 27 Dec 2022 12:23

Tgt Ion: 91 Resp: 52657
Ion Ratio Lower Upper
91 100
120 23.5 12.0 36.1

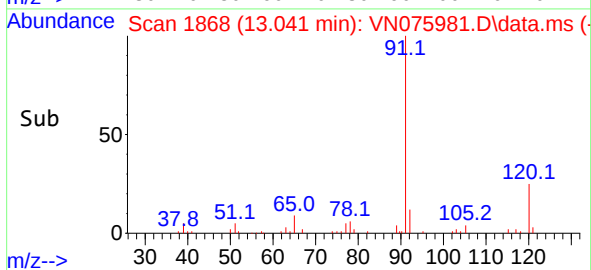



#79

2-Chlorotoluene

Concen: 0.205 ug/l

RT: 13.217 min Scan# 1898

Delta R.T. 0.088 min

Lab File: VN075981.D

Acq: 27 Dec 2022 12:23

Instrument :

MSVOA_N

ClientSampleId :





MW-1

Tgt Ion: 91 Resp: 2087

Ion Ratio Lower Upper

91 100

126 32.6 17.5 52.5

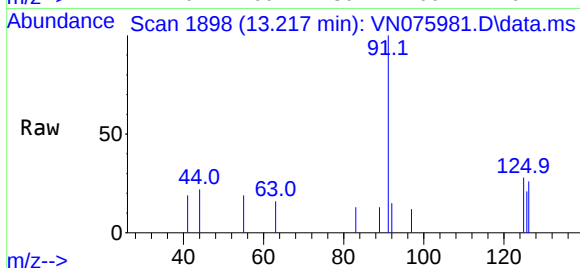

#81

trans-1,4-Dichloro-2-butene

Concen: 84.719 ug/l

RT: 12.853 min Scan# 1836

Delta R.T. 0.112 min

Lab File: VN075981.D

Acq: 27 Dec 2022 12:23




Tgt Ion: 75 Resp: 96959


Ion Ratio Lower Upper

75 100

53 0.0 73.8 110.6#

89 0.0 39.5 59.3#


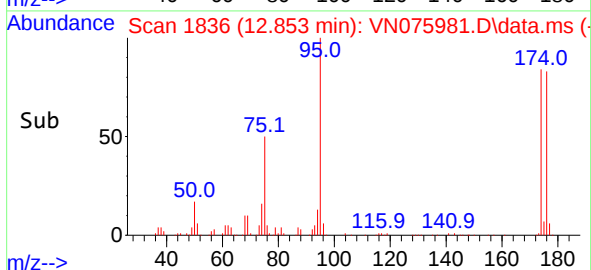
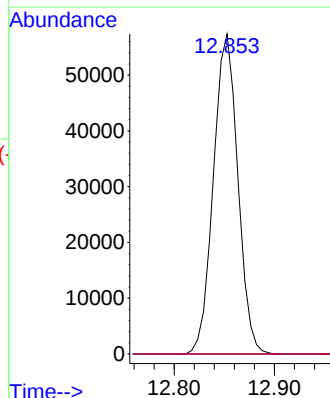
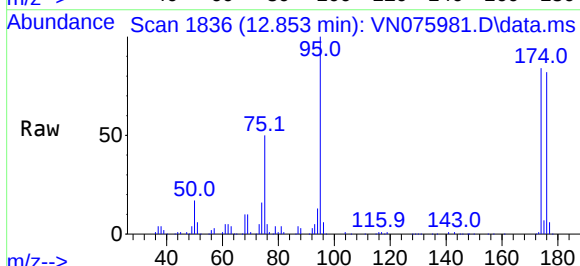




#82
4-Chlorotoluene
Concen: 0.205 ug/l
RT: 13.217 min Scan# 1883
Delta R.T. 0.088 min
Lab File: VN075981.D
Acq: 27 Dec 2022 12:23




Instrument :
MSVOA_N
ClientSampleId :
MW-1


Tgt Ion: 91 Resp: 2087
Ion Ratio Lower Upper
91 100
126 32.6 17.5 52.5

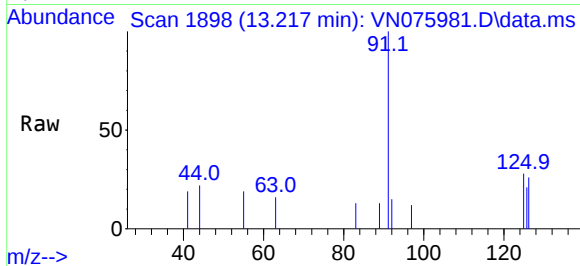

#84
1,2,4-Trimethylbenzene
Concen: 0.353 ug/l
RT: 13.482 min Scan# 1943
Delta R.T. -0.000 min
Lab File: VN075981.D
Acq: 27 Dec 2022 12:23

Tgt Ion: 105 Resp: 4328
Ion Ratio Lower Upper
105 100
120 38.2 23.3 69.8


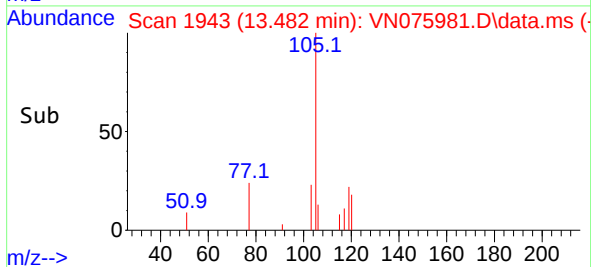

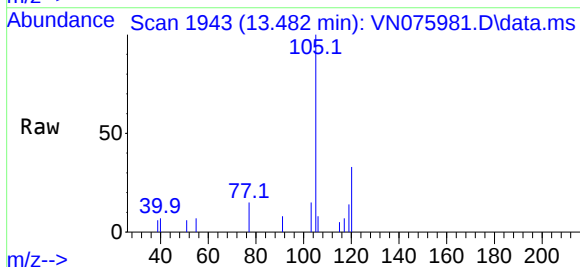




#85
 sec-Butylbenzene
 Concen: 1.229 ug/l
 RT: 13.617 min Scan# 1966
 Delta R.T. -0.000 min
 Lab File: VN075981.D
 Acq: 27 Dec 2022 12:23




Instrument :
 MSVOA_N
 ClientSampleId :
 MW-1


Tgt Ion:105 Resp: 18484
 Ion Ratio Lower Upper
 105 100
 134 26.3 10.1 30.1

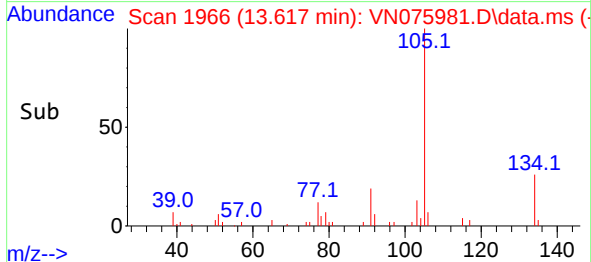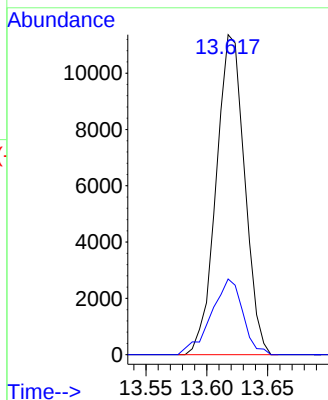

#86
 p-Isopropyltoluene
 Concen: 0.440 ug/l
 RT: 13.729 min Scan# 1985
 Delta R.T. -0.000 min
 Lab File: VN075981.D
 Acq: 27 Dec 2022 12:23

Tgt Ion:119 Resp: 5507
 Ion Ratio Lower Upper
 119 100
 134 30.3 13.0 39.0
 91 24.7 11.2 33.6


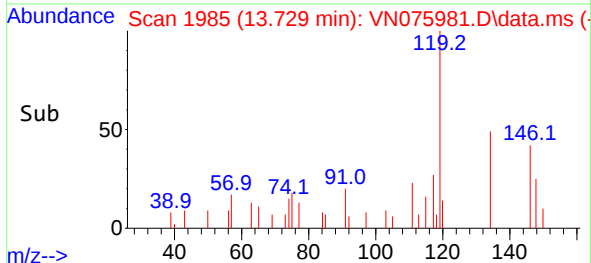
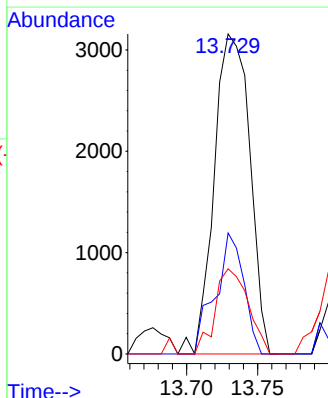
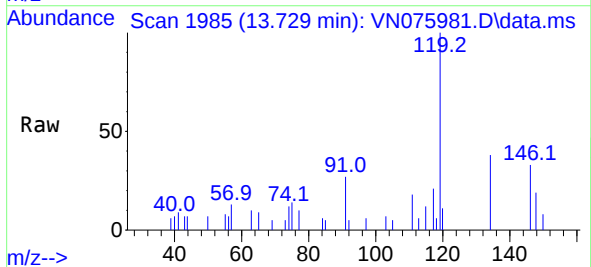




#87
1,3-Dichlorobenzene
Concen: 0.319 ug/l
RT: 13.735 min Scan# 1986
Delta R.T. -0.000 min
Lab File: VN075981.D
Acq: 27 Dec 2022 12:23




Instrument :
MSVOA_N
ClientSampleId :
MW-1


Tgt Ion:146 Resp: 2199
Ion Ratio Lower Upper
146 100
111 48.1 19.7 59.0
148 58.7 31.4 94.2

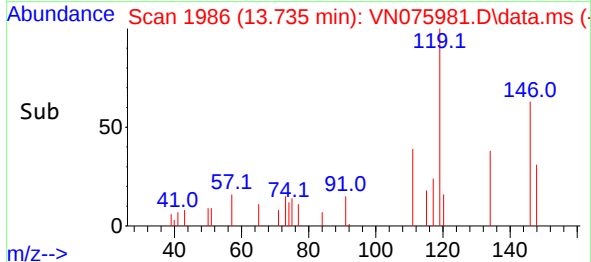

#88
1,4-Dichlorobenzene
Concen: 0.312 ug/l
RT: 13.735 min Scan# 1986
Delta R.T. -0.077 min
Lab File: VN075981.D
Acq: 27 Dec 2022 12:23

Tgt Ion:146 Resp: 2199
Ion Ratio Lower Upper
146 100
111 48.1 19.1 57.1
148 58.7 32.0 96.2


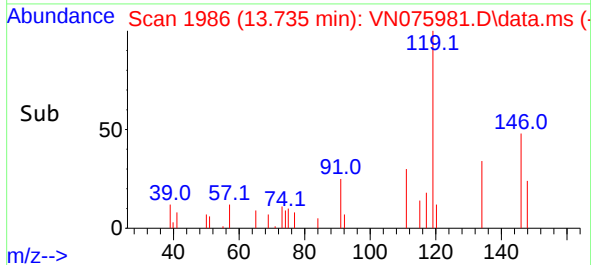

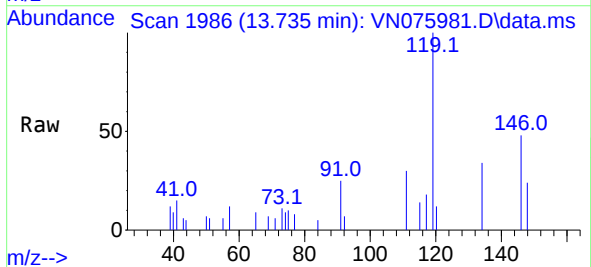




#89
n-Butylbenzene
Concen: 1.530 ug/l
RT: 14.059 min Scan# 2041
Delta R.T. -0.000 min
Lab File: VN075981.D
Acq: 27 Dec 2022 12:23




Instrument :
MSVOA_N
ClientSampleId :
MW-1


Tgt Ion: 91 Resp: 15515
Ion Ratio Lower Upper
91 100
92 47.3 26.4 79.2
134 50.8 13.4 40.2#

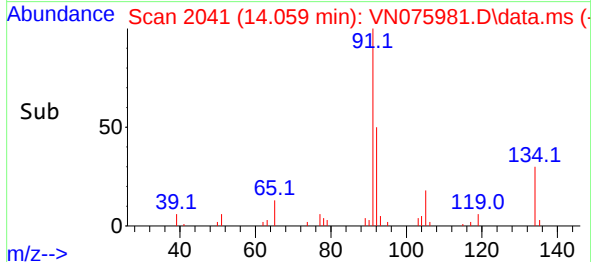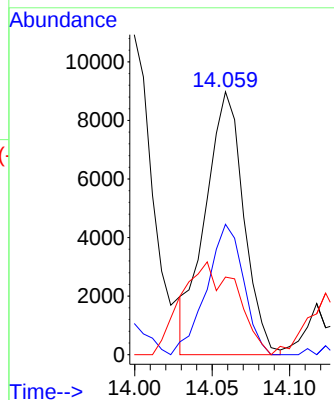

#90
Hexachloroethane
Concen: 3.494 ug/l
RT: 14.335 min Scan# 2088
Delta R.T. -0.000 min
Lab File: VN075981.D
Acq: 27 Dec 2022 12:23

Tgt Ion: 117 Resp: 7823
Ion Ratio Lower Upper
117 100
201 0.0 38.0 114.1#

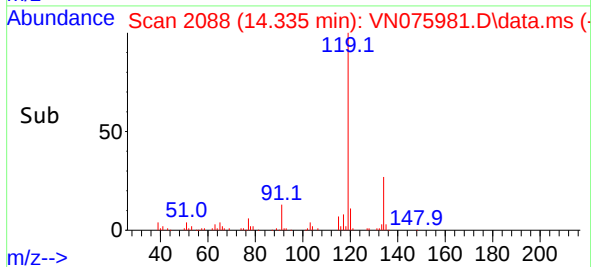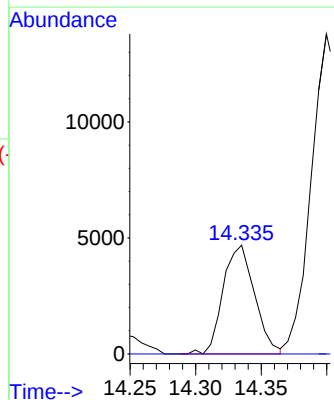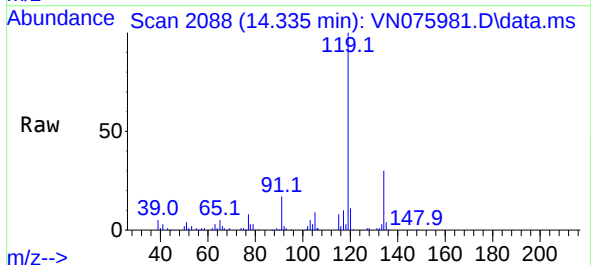







#91
1,2-Dichlorobenzene
Concen: 0.333 ug/l
RT: 14.106 min Scan# 2049
Delta R.T. -0.000 min
Lab File: VN075981.D
Acq: 27 Dec 2022 12:23

Instrument :
MSVOA_N
ClientSampleId :
MW-1

Tgt Ion:146 Resp: 2265




Ion	Ratio	Lower	Upper
146	100		
111	37.8	20.3	61.0
148	57.9	31.7	95.1




#92
1,2-Dibromo-3-Chloropropane
Concen: 0.204 ug/l
RT: 14.735 min Scan# 2156
Delta R.T. 0.012 min
Lab File: VN075981.D
Acq: 27 Dec 2022 12:23

Tgt Ion: 75 Resp: 165

Ion	Ratio	Lower	Upper
75	100		
155	40.6	49.3	147.8#
157	0.0	63.7	191.3#



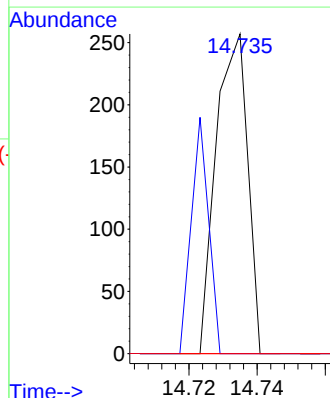





#93
1,2,4-Trichlorobenzene
Concen: 0.982 ug/l
RT: 15.388 min Scan# 21
Delta R.T. -0.006 min
Lab File: VN075981.D
Acq: 27 Dec 2022 12:23




Instrument :
MSVOA_N
ClientSampleId :
MW-1


Tgt Ion:180 Resp: 3307
Ion Ratio Lower Upper
180 100
182 95.4 47.5 142.5
145 52.7 15.3 45.8#

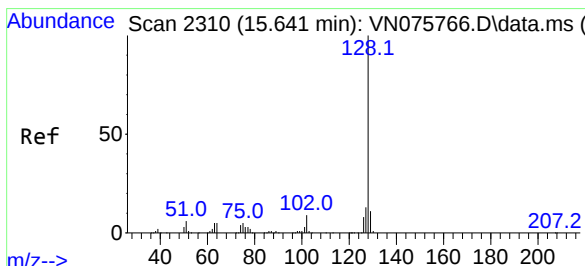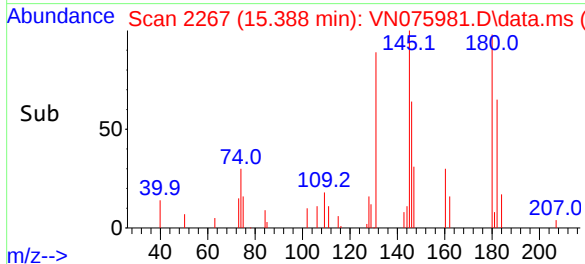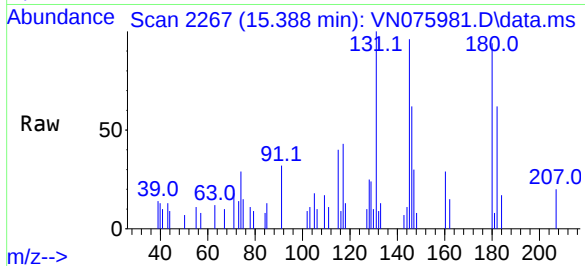

#95
Naphthalene
Concen: 10.346 ug/l
RT: 15.647 min Scan# 2311
Delta R.T. 0.006 min
Lab File: VN075981.D
Acq: 27 Dec 2022 12:23

Tgt Ion:128 Resp: 94984
Ion Ratio Lower Upper
128 100
127 13.4 10.4 15.6
129 10.3 8.7 13.1

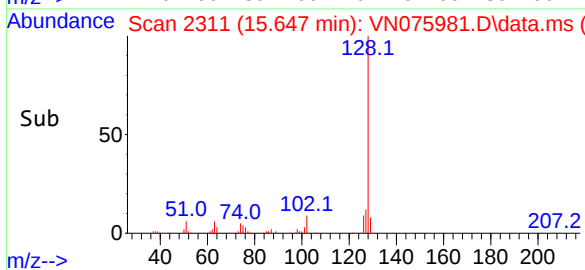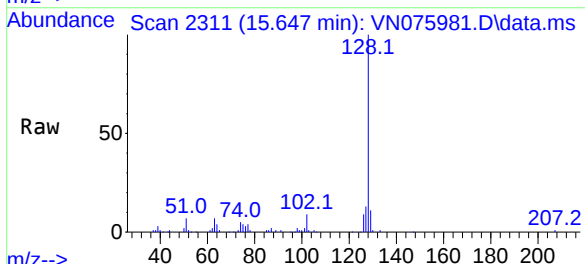



#96
 1,2,3-Trichlorobenzene
 Concen: 1.088 ug/l
 RT: 15.841 min Scan# 21
 Delta R.T. -0.000 min
 Lab File: VN075981.D
 Acq: 27 Dec 2022 12:23

Instrument :
 MSVOA_N
 ClientSampleId :
 MW-1

Tgt Ion:180 Resp: 3424
 Ion Ratio Lower Upper
 180 100
 182 94.2 47.0 141.0
 145 0.0 16.0 47.9#

