
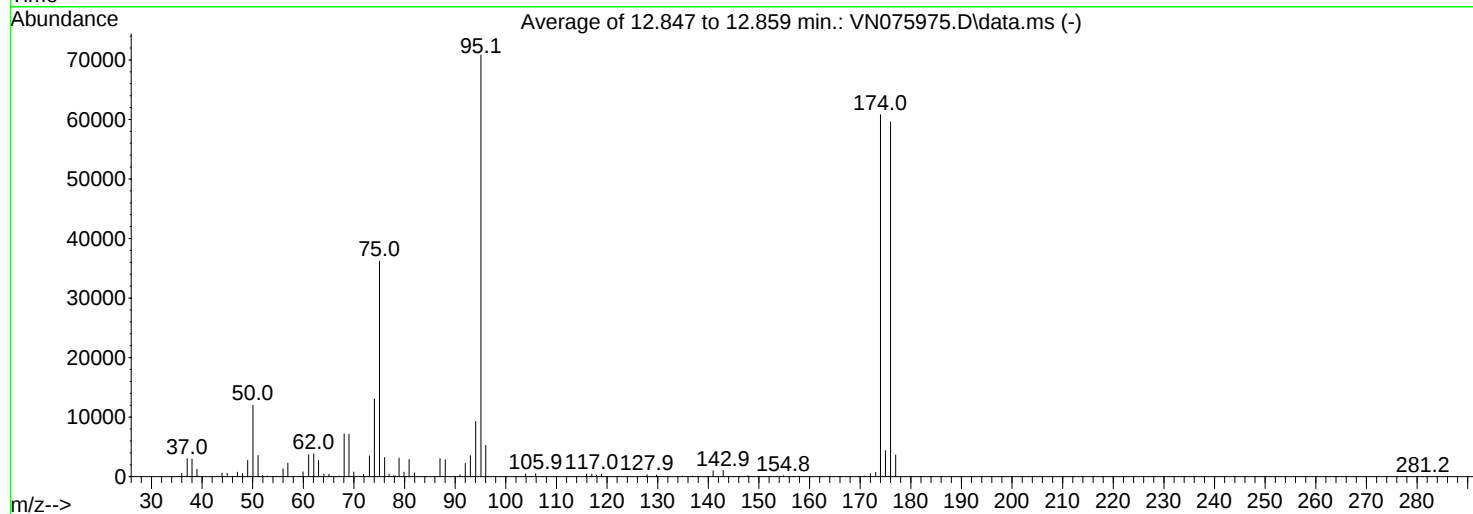


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN122722\
Data File : VN075975.D
Acq On : 27 Dec 2022 08:39
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N121422W.M
Title : SW846 8260
Last Update : Wed Dec 14 13:03:41 2022

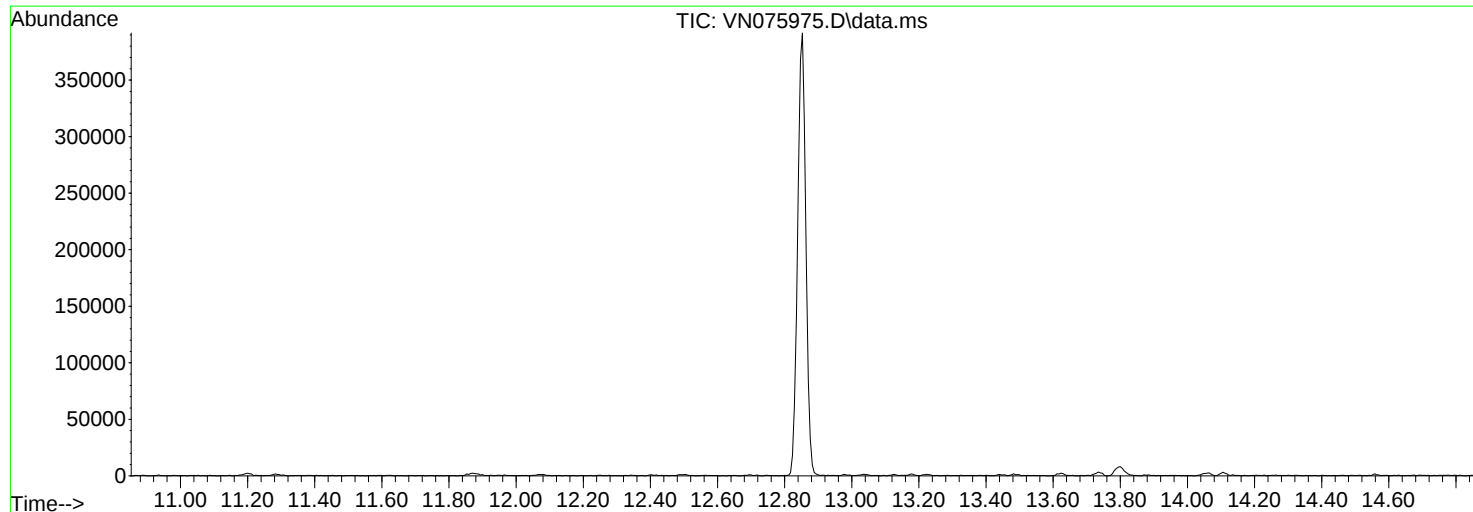

AutoFind: Scans 1835, 1836, 1837; Background Corrected with Scan 1827

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.9	11979	PASS
75	95	30	60	51.1	36181	PASS
95	95	100	100	100.0	70853	PASS
96	95	5	9	7.5	5281	PASS
173	174	0.00	2	1.2	724	PASS
174	95	50	100	85.8	60811	PASS
175	174	5	9	7.2	4375	PASS
176	174	95	101	98.0	59576	PASS
177	176	5	9	6.1	3627	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.00	564	51.05	3585	65.05	392	77.85	173
37.05	3034	51.95	194	67.10	106	78.15	14
38.00	2958	52.90	110	68.05	7173	78.90	313
39.00	1237	54.80	77	69.00	7135	79.90	74
40.00	9	56.00	1318	69.95	780	80.90	2902
43.95	622	56.95	2268	71.90	369	81.95	653
44.95	567	59.95	803	73.05	3488	87.00	3039
47.00	758	61.05	3673	74.05	13036	88.05	2827
47.95	505	62.05	3859	75.05	36181	90.95	339
49.00	2716	63.00	2731	76.05	3208	92.00	2231
50.05	11979	64.05	419	76.95	406	93.00	3515

Average of 12.847 to 12.859 min.: VN075975.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
94.05	9280	127.90	328	154.85	154		
95.10	70853	129.80	276	156.80	55		
96.05	5281	134.85	118	170.80	106		
103.90	429	136.90	109	172.00	483		
104.80	64	140.95	1001	173.05	724		
105.90	476	141.80	58	174.00	60811		
115.95	431	142.95	1038	175.00	4375		
116.70	81	144.80	53	176.00	59576		
117.00	458	146.00	57	177.00	3627		
117.90	278	147.85	155	281.20	51		
118.90	442	148.10	63				

Instrument :

MSVOA_N

ClientSampleId :

BFB