
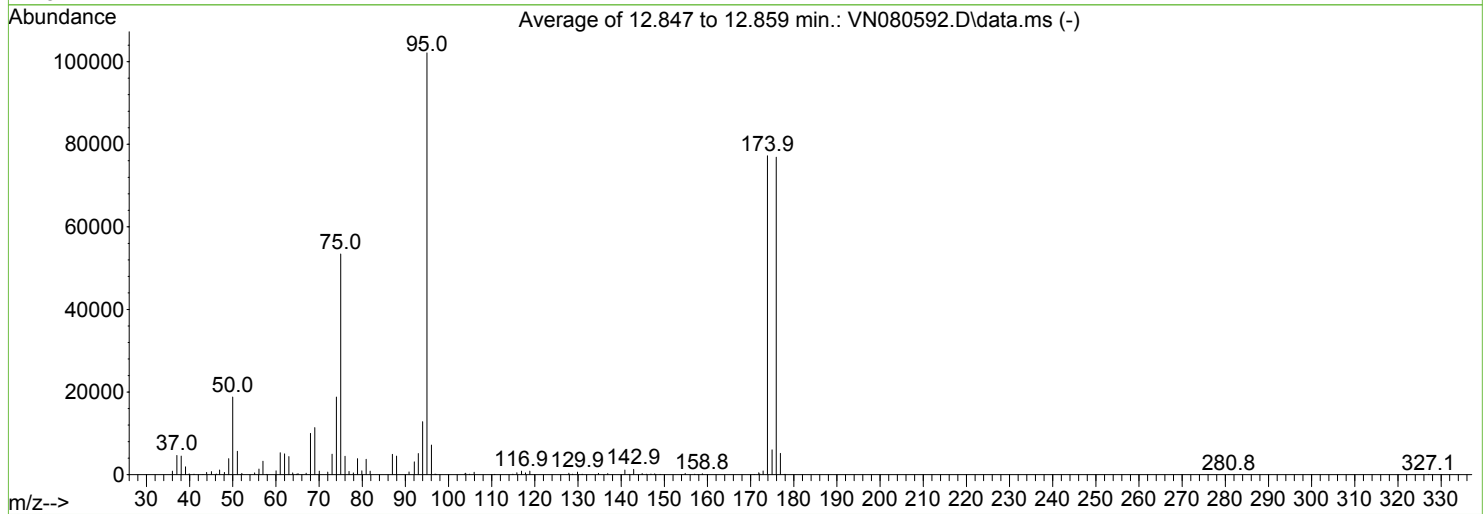


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN122723\
Data File : VN080592.D
Acq On : 27 Dec 2023 09:51
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N122723W.M
Title : SW846 8260
Last Update : Thu Dec 28 03:07:01 2023

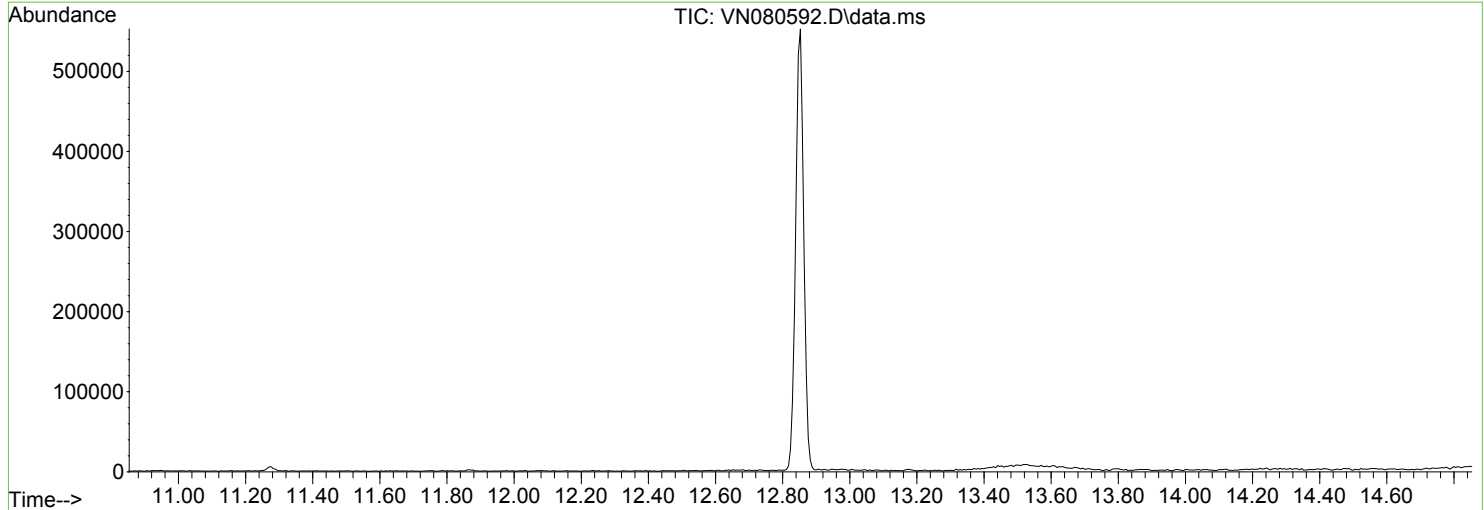

AutoFind: Scans 1852, 1853, 1854; Background Corrected with Scan 1843

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.4	18806	PASS
75	95	30	60	52.3	53421	PASS
95	95	100	100	100.0	102131	PASS
96	95	5	9	7.0	7164	PASS
173	174	0.00	2	1.1	886	PASS
174	95	50	100	75.6	77224	PASS
175	174	5	9	7.8	6001	PASS
176	174	95	101	99.5	76853	PASS
177	176	5	9	6.7	5166	PASS

Average of 12.847 to 12.859 min.: VN080592.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.00	875	48.05	540	61.00	5318	73.00	496
37.05	4652	49.05	3862	62.00	5048	74.00	1879
38.05	4479	50.00	18806	63.00	4381	75.00	5342
39.05	1885	51.05	5674	63.90	417	76.00	446
39.90	178	51.90	57	64.80	135	76.95	779
41.00	128	52.10	316	65.10	274	77.95	442
43.10	56	55.05	418	67.00	352	78.90	3873
43.95	553	56.05	1362	68.00	10005	79.90	951
45.05	741	57.00	3242	69.00	11389	80.90	3714
46.15	170	57.90	81	70.05	867	81.85	852
46.95	1128	60.05	914	72.00	626	87.00	4927

Average of 12.847 to 12.859 min.: VN080592.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
87.95	4481	104.85	126	130.95	136	149.00	62
90.85	671	105.95	576	134.75	317	154.85	331
92.05	3098	110.70	64	136.90	277	157.05	137
93.00	5106	114.90	100	140.85	1120	157.80	53
94.00	12820	115.85	475	141.90	80	158.80	222
95.00	102131	116.90	840	142.90	1295	170.80	59
96.05	7164	117.85	409	144.85	268	171.90	456
96.90	166	118.85	839	145.85	111	172.10	182
97.10	74	127.90	337	146.90	157	172.90	886
103.80	204	128.75	137	147.75	214	173.90	77224
103.95	361	129.90	637	148.00	95	174.95	6001

Average of 12.847 to 12.859 min.: VN080592.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
175.95	76853						
176.90	5166						
177.80	61						
178.00	96						
280.80	52						
327.10	76						

Instrument :

MSVOA_N

ClientSampleId :

BFB