
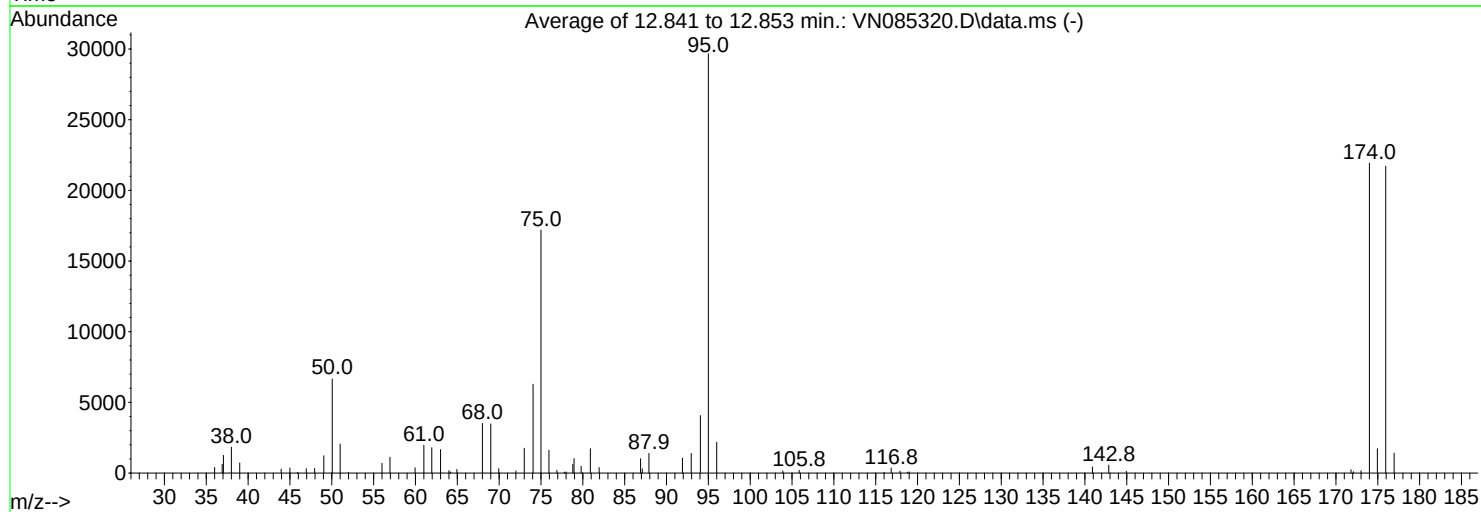


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN122724\
Data File : VN085320.D
Acq On : 27 Dec 2024 09:52
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N122724W.M
Title : SW846 8260
Last Update : Sat Dec 28 01:36:16 2024

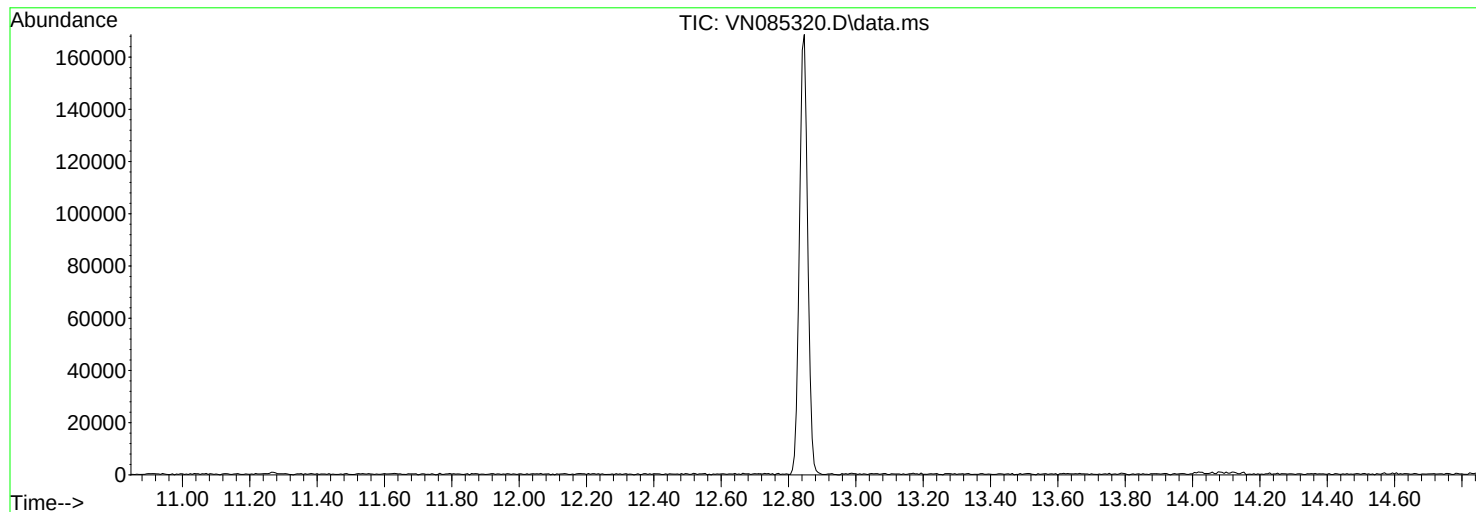

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1843

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.4	6656	PASS
75	95	30	60	58.0	17193	PASS
95	95	100	100	100.0	29667	PASS
96	95	5	9	7.3	2180	PASS
173	174	0.00	2	0.8	173	PASS
174	95	50	100	73.9	21933	PASS
175	174	5	9	7.9	1730	PASS
176	174	95	101	99.0	21707	PASS
177	176	5	9	6.5	1416	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.00	395	50.05	6656	64.95	258	78.00	82
36.90	615	51.00	2063	68.00	3516	78.80	618
37.05	1253	52.00	51	69.00	3482	78.95	1025
38.00	1836	56.00	691	69.95	311	79.80	481
39.00	716	56.95	1115	72.00	154	80.90	1729
43.95	280	59.95	376	73.00	1757	81.95	392
45.00	363	61.00	1966	74.05	6288	86.90	1016
45.90	51	61.95	1793	75.00	17193	87.10	304
46.95	311	63.00	1658	75.95	1618	87.90	1397
47.95	322	64.00	180	76.90	201	91.90	1064
49.05	1223	64.20	74	77.80	65	92.95	1389

Average of 12.841 to 12.853 min.: VN085320.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
94.05	4066	142.85	563				
95.00	29667	144.95	133				
96.00	2180	171.80	240				
103.90	155	172.10	100				
105.85	202	173.00	173				
116.00	57	174.00	21933				
116.85	353	174.95	1730				
117.90	143	175.95	21707				
118.80	68	176.95	1416				
119.00	86						
140.90	427						

Instrument :

MSVOA_N

ClientSampleId :

BFB