

Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN122818\
 Data File : VN053217.D
 Acq On : 28 Dec 2018 11:13
 Operator : MD\SY
 Sample : VN1228WBL01
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 8 Sample Multiplier: 28

Instrument :
 MSVOA_N
 ClientSampleId :
 VN1228WBL01

Quant Time: Dec 28 11:57:24 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA N\METHODS\624N122818W.M
 Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
 QLast Update : Fri Dec 28 10:33:50 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Bromochloromethane	7.20	128	175017	30.00	ug/l	0.00
28) 1,4-Difluorobenzene	8.59	114	1025168	30.00	ug/l	0.00
57) Chlorobenzene-d5	11.41	117	833993	30.00	ug/l	0.00

System Monitoring Compounds

27) 1,2-Dichloroethane-d4	8.03	65	335382	30.17	ug/l	0.00
Spiked Amount	30.000	Range	50 - 169	Recovery	=	100.57%
60) 4-Bromofluorobenzene	12.40	95	337084	26.41	ug/l	0.00
Spiked Amount	30.000	Range	56 - 143	Recovery	=	88.03%
63) Toluene-d8	10.09	98	1170143	31.14	ug/l	0.00
Spiked Amount	30.000	Range	66 - 137	Recovery	=	103.80%


Target Compounds	Ovalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA N\DATA\VN122818\
Data File : VN053217.D
Acq On : 28 Dec 2018 11:13
Operator : MD\SY
Sample : VN1228WBL01
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 8 Sample Multiplier: 28

Instrument :
MSVOA_N
ClientSampleId :
VN1228WBL01

Quant Time: Dec 28 11:57:24 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA N\METHODS\624N122818W.M
Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
QLast Update : Fri Dec 28 10:33:50 2018
Response via : Initial Calibration

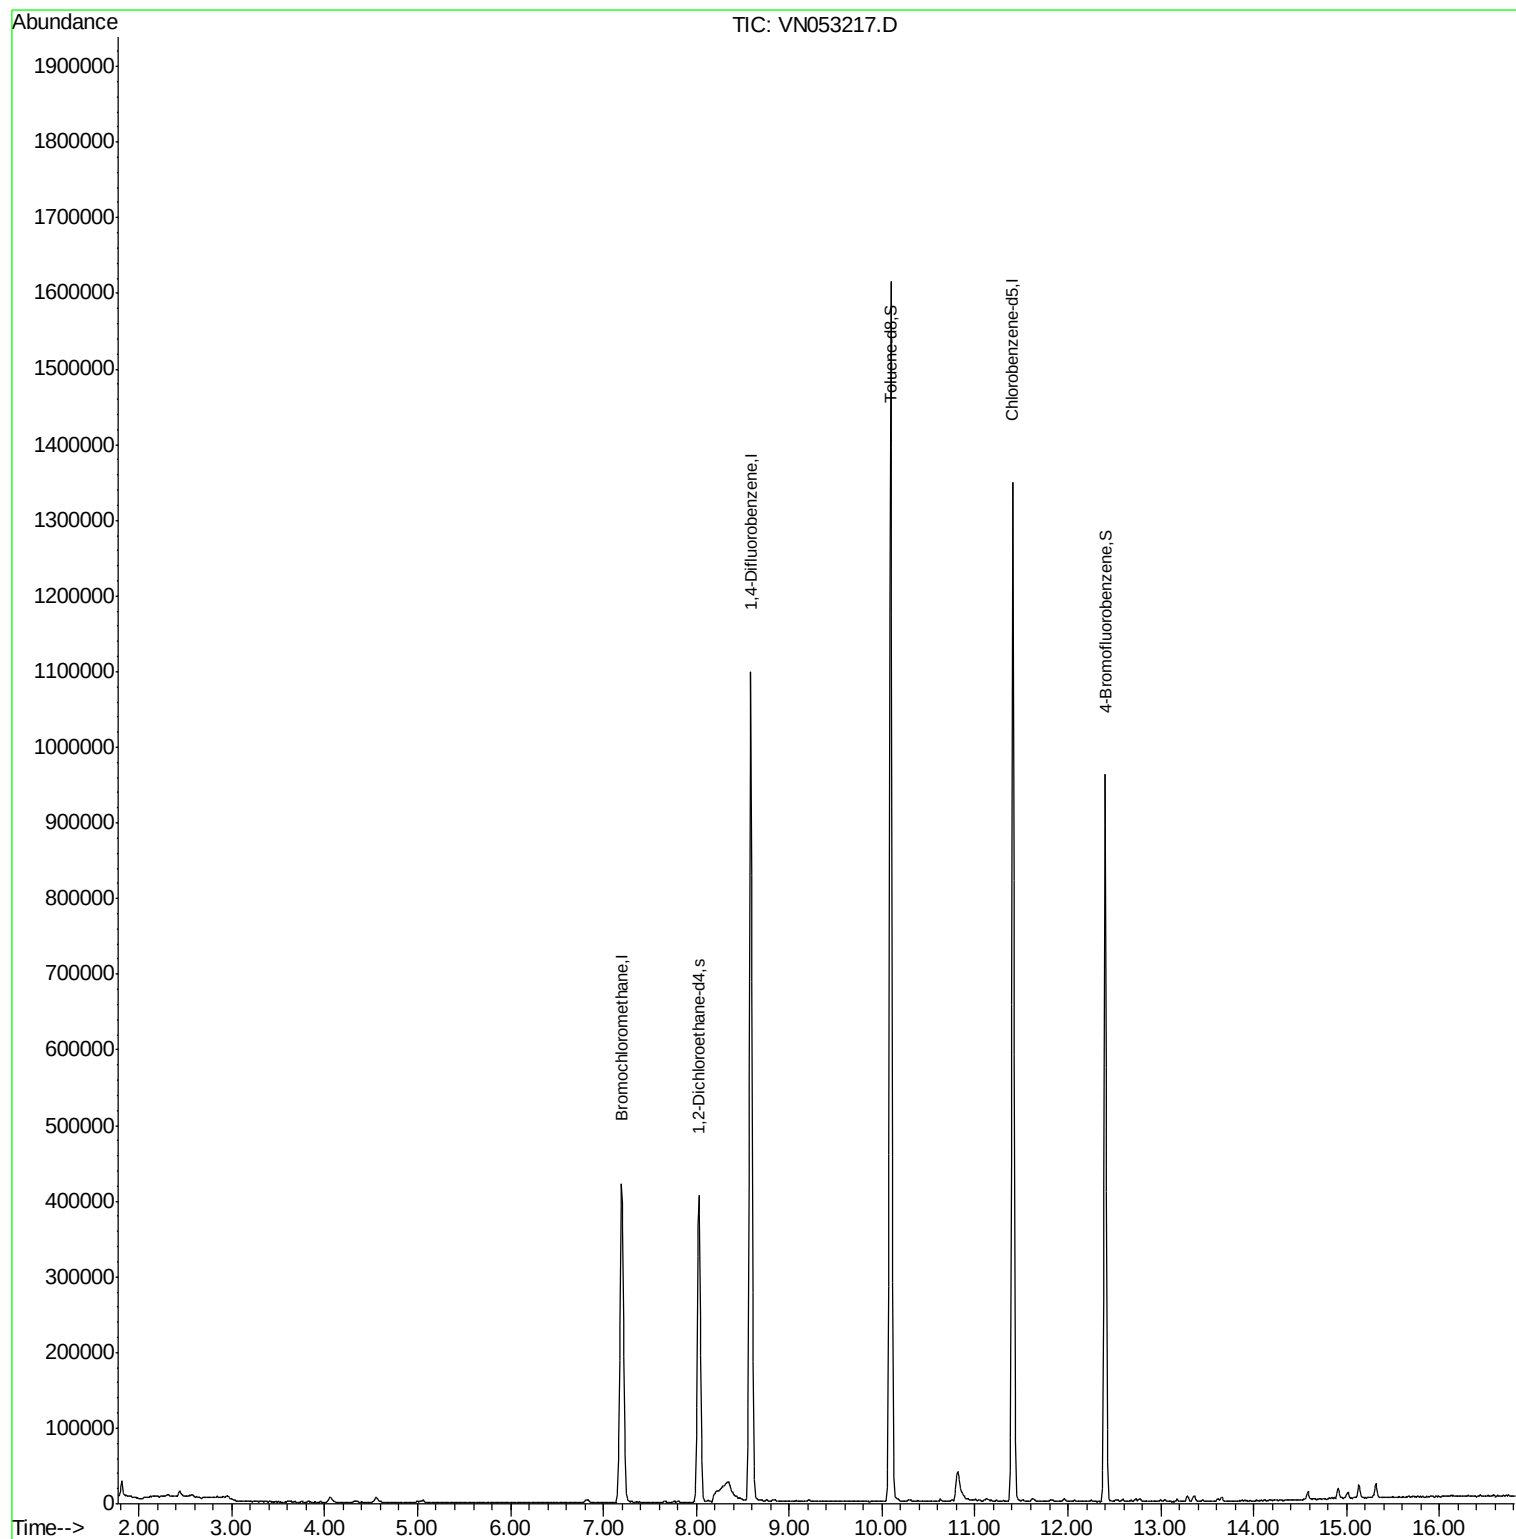


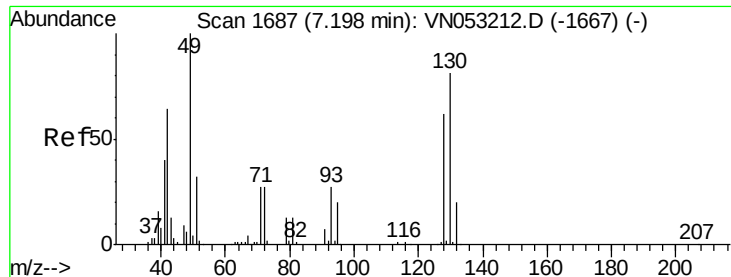




#1
 Bromochloromethane
 Concen: 30.000 ug/l
 RT: 7.20 min Scan# 1687
 Delta R.T. 0.00 min
 Lab File: VN053217.D
 Acq: 28 Dec 2018 11:13

Instrument :
 MSVOA_N
 ClientSampled :
 VN1228WBL01

Tot Ion:128 Resp: 175017
 Ion Ratio Lower Upper
 128 100
 49 155.9 0.0 431.8
 130 129.1 0.0 317.0

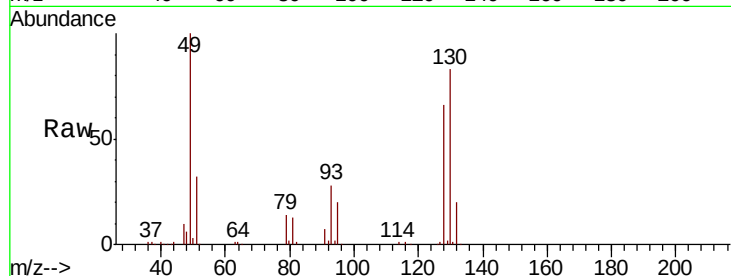


Abundance Ion 128.00 (127.70 to 128.70): V
 Ion 49.00 (48.70 to 49.70): VN
 Ion 130.00 (129.70 to 130.70): V

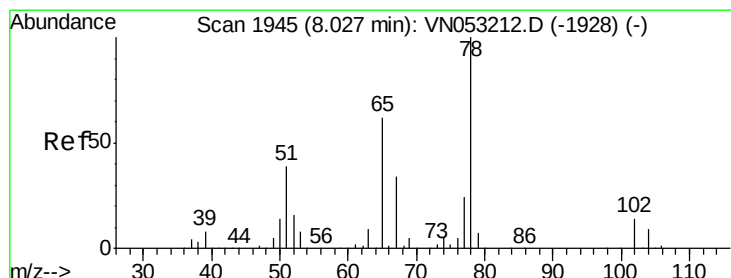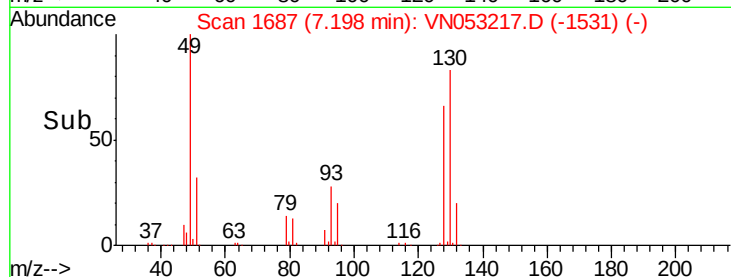
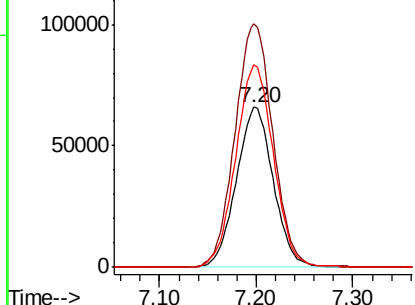



#27
 1,2-Dichloroethane-d4
 Concen: Below ug/l
 RT: 8.03 min Scan# 1945
 Delta R.T. 0.00 min
 Lab File: VN053217.D
 Acq: 28 Dec 2018 11:13

Tgt Ion: 65 Resp: 335382
 Ion Ratio Lower Upper
 65 100
 67 55.3 44.6 66.8

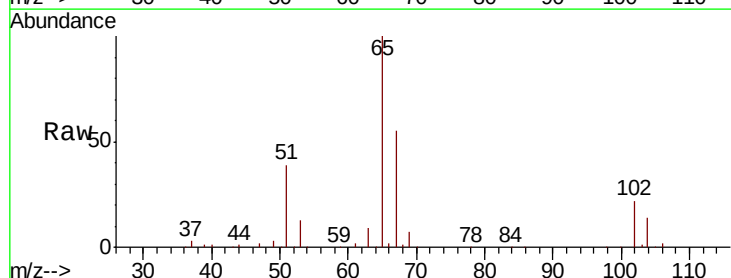

Abundance Ion 65.00 (64.70 to 65.70): VN
 Ion 67.00 (66.70 to 67.70): VN



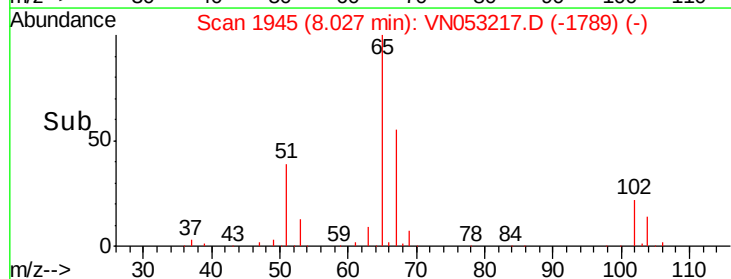
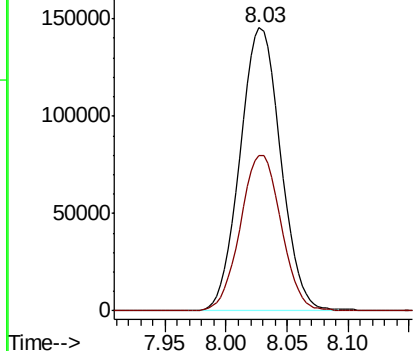


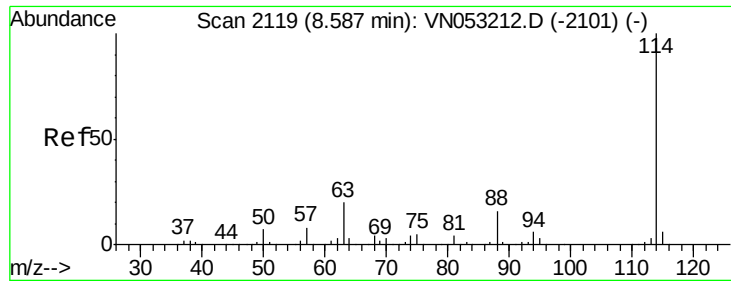

#28
 1,4-Difluorobenzene
 Concen: 30.000 ug/l
 RT: 8.59 min Scan# 2119
 Delta R.T. 0.00 min
 Lab File: VN053217.D
 Acq: 28 Dec 2018 11:13




Instrument :
 MSVOA_N
 ClientSampleId :
 VN1228WBL01


Tot Ion:114 Resp: 1025168
 Ion Ratio Lower Upper
 114 100
 63 19.5 16.9 25.3
 88 15.4 12.8 19.2

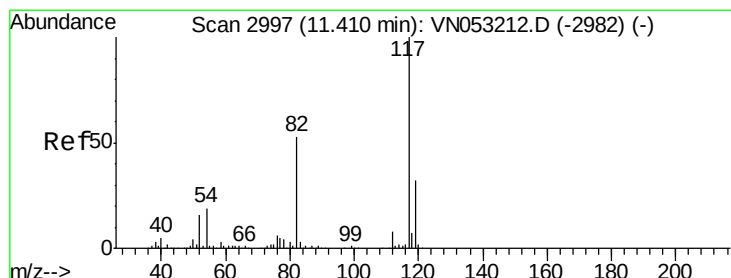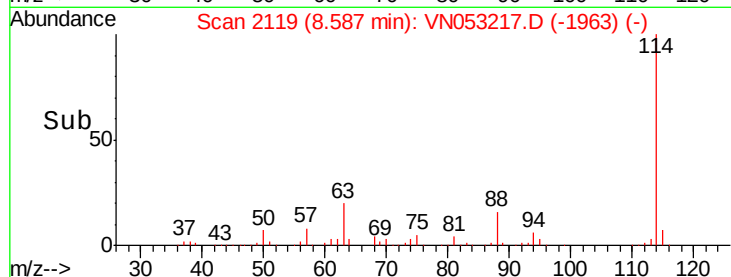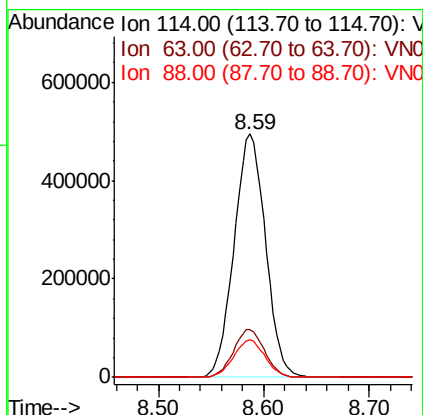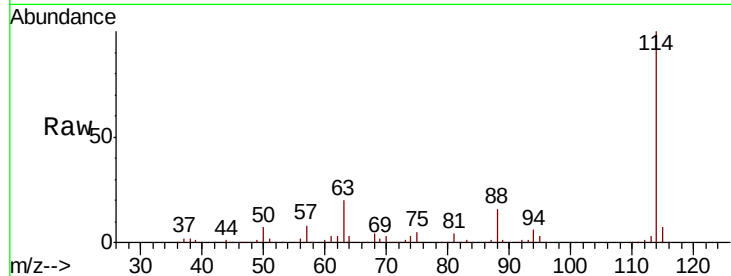

#57
 Chlorobenzene-d5
 Concen: 30.000 ug/l
 RT: 11.41 min Scan# 2996
 Delta R.T. -0.00 min
 Lab File: VN053217.D
 Acq: 28 Dec 2018 11:13

Tgt Ion:117 Resp: 833993
 Ion Ratio Lower Upper
 117 100
 82 53.1 44.2 66.2
 119 32.1 25.4 38.2

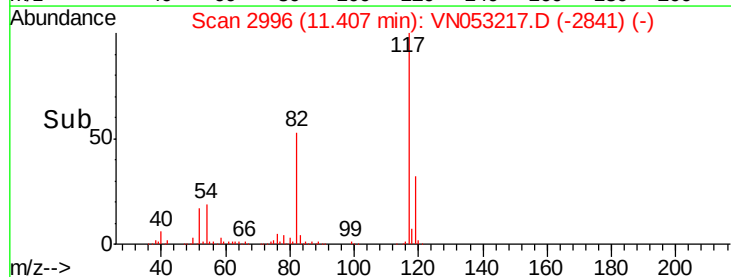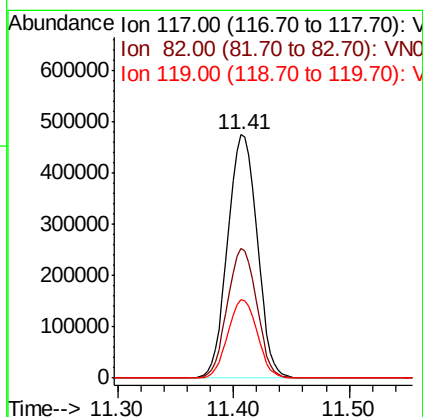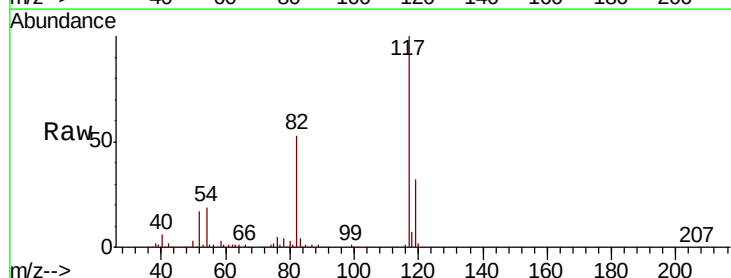

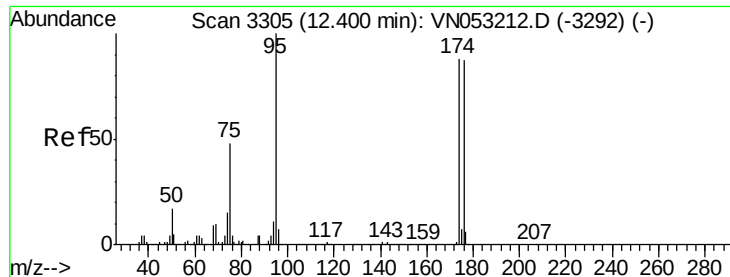

#60

4-Bromofluorobenzene

Concen: N.D. ug/l

RT: 12.40 min Scan# 3305

Delta R.T. 0.00 min

Lab File: VN053217.D

Acq: 28 Dec 2018 11:13

Instrument :

MSVOA_N

ClientSampled :

VN1228WBL01


Tot Ion: 95 Resp: 337084

Ion Ratio Lower Upper

95 100

174 89.6 67.9 101.9




176 87.0 66.4 99.6

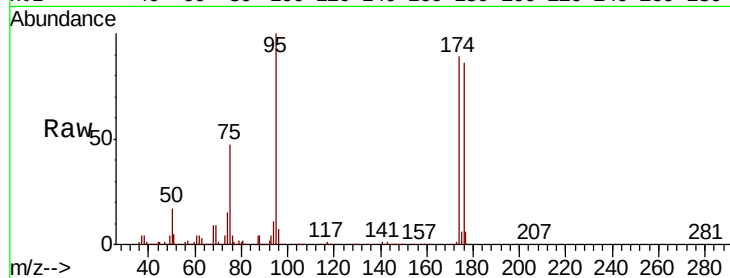

Abundance Ion 95.00 (94.70 to 95.70): VN053217.D (-3292) (-)

Ion 174.00 (173.70 to 174.70): VN053217.D (-3292) (-)

Ion 176.00 (175.70 to 176.70): VN053217.D (-3292) (-)

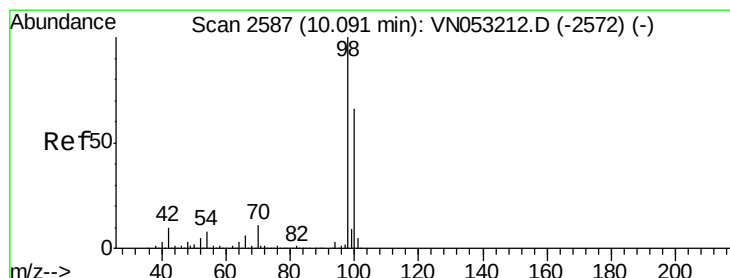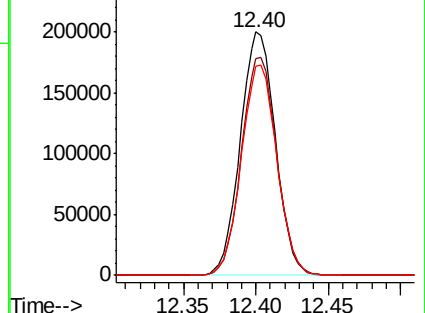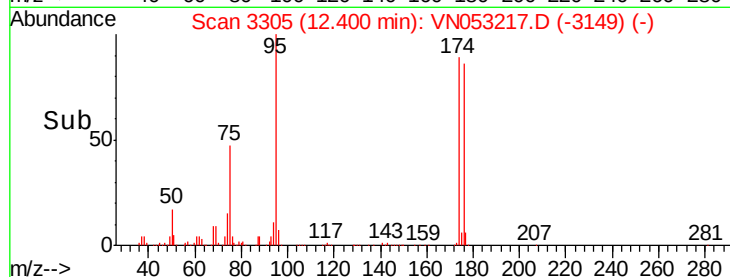

#63

Toluene-d8

Concen: Below ug/l

RT: 10.09 min Scan# 2587

Delta R.T. 0.00 min

Lab File: VN053217.D


Acq: 28 Dec 2018 11:13

Tgt Ion: 98 Resp: 1170143

Ion Ratio Lower Upper

98 100

100 64.7 51.1 76.7

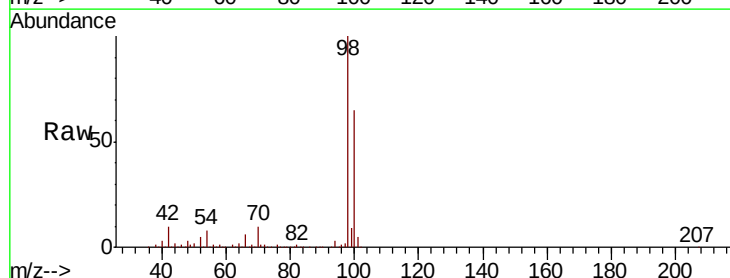

Abundance Ion 98.00 (97.70 to 98.70): VN053217.D (-2572) (-)

Ion 100.00 (99.70 to 100.70): VN053217.D (-2572) (-)

