

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN122820\
 Data File : VN065292.D
 Acq On : 28 Dec 2020 17:45
 Operator : JC/MD
 Sample : L4991-13
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 COMP-2

Quant Time: Dec 29 02:24:01 2020
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N122220W.M
 Quant Title : SW846 8260
 QLast Update : Tue Dec 22 15:42:18 2020
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	7.627	168	243634	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.550	114	403678	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.380	117	432535	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.318	152	201208	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	7.991	65	140008	50.90	ug/l	0.00
Spiked Amount 50.000	Range 61 - 141		Recovery = 101.80%			
35) Dibromofluoromethane	7.550	113	123866	50.86	ug/l	0.00
Spiked Amount 50.000	Range 69 - 133		Recovery = 101.72%			
50) Toluene-d8	10.058	98	507581	55.61	ug/l	0.00
Spiked Amount 50.000	Range 65 - 126		Recovery = 111.22%			
62) 4-Bromofluorobenzene	12.376	95	206091	56.37	ug/l	0.00
Spiked Amount 50.000	Range 58 - 135		Recovery = 112.74%			
Target Compounds						Qvalue
11) Tert butyl alcohol	4.772	59	61609	136.90	ug/l	98
13) Acrolein	3.583	56	976	5.59	ug/l	87
16) Acetone	3.785	43	226276	193.62	ug/l	96
18) Methyl Acetate	4.293	43	16702	6.76	ug/l	100
20) Methylene Chloride	4.509	84	4037	1.50	ug/l	95
22) Diisopropyl ether	6.016	45	2326	0.30	ug/l #	1
25) 2-Butanone	6.801	43	77154	49.97	ug/l	98
29) Tetrahydrofuran	7.180	42	1092	1.09	ug/l #	32
31) Cyclohexane	7.624	56	4233	1.04	ug/l #	5
36) 1,1-Dichloropropene	7.624	75	15597	4.25	ug/l #	49
37) Ethyl Acetate	6.801	43	77154	21.21	ug/l #	66
38) Carbon Tetrachloride	7.627	117	21000	5.45	ug/l #	16
40) Benzene	8.004	78	145263	13.30	ug/l	97
41) Methacrylonitrile	7.180	41	3830	2.02	ug/l #	28
43) Isopropyl Acetate	8.254	43	4395	0.70	ug/l #	59
48) Methyl methacrylate	9.135	41	22508	7.39	ug/l #	39
49) 1,4-Dioxane	9.171	88	5759	116.74	ug/l #	26
51) 4-Methyl-2-Pentanone	9.955	43	734741	208.41	ug/l	98
52) Toluene	10.126	92	55576	8.08	ug/l	98
59) 2-Hexanone	10.727	43	2929	1.13	ug/l	91
67) Ethyl Benzene	11.486	91	7399	0.47	ug/l	97
68) m/p-Xylenes	11.589	106	5943	0.99	ug/l	99
69) o-Xylene	11.923	106	3788	0.65	ug/l	100
70) Styrene	11.939	104	11246	1.16	ug/l	98
71) Bromoform	12.376	173	1207	0.41	ug/l #	1
74) N-amyl acetate	12.003	43	105125	17.23	ug/l #	43
76) 1,2,3-Trichloropropane	12.376	75	101170	24.65	ug/l #	100
81) trans-1,4-Dichloro-2-b...	12.376	75	101170	62.15	ug/l #	15
85) sec-Butylbenzene	13.039	105	36887	2.50	ug/l #	56
95) Naphthalene	15.097	128	31707	6.21	ug/l	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN122820\
Data File : VN065292.D
Acq On : 28 Dec 2020 17:45
Operator : JC/MD
Sample : L4991-13
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
COMP-2

Quant Time: Dec 29 02:24:01 2020
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N122220W.M
Quant Title : SW846 8260
QLast Update : Tue Dec 22 15:42:18 2020
Response via : Initial Calibration




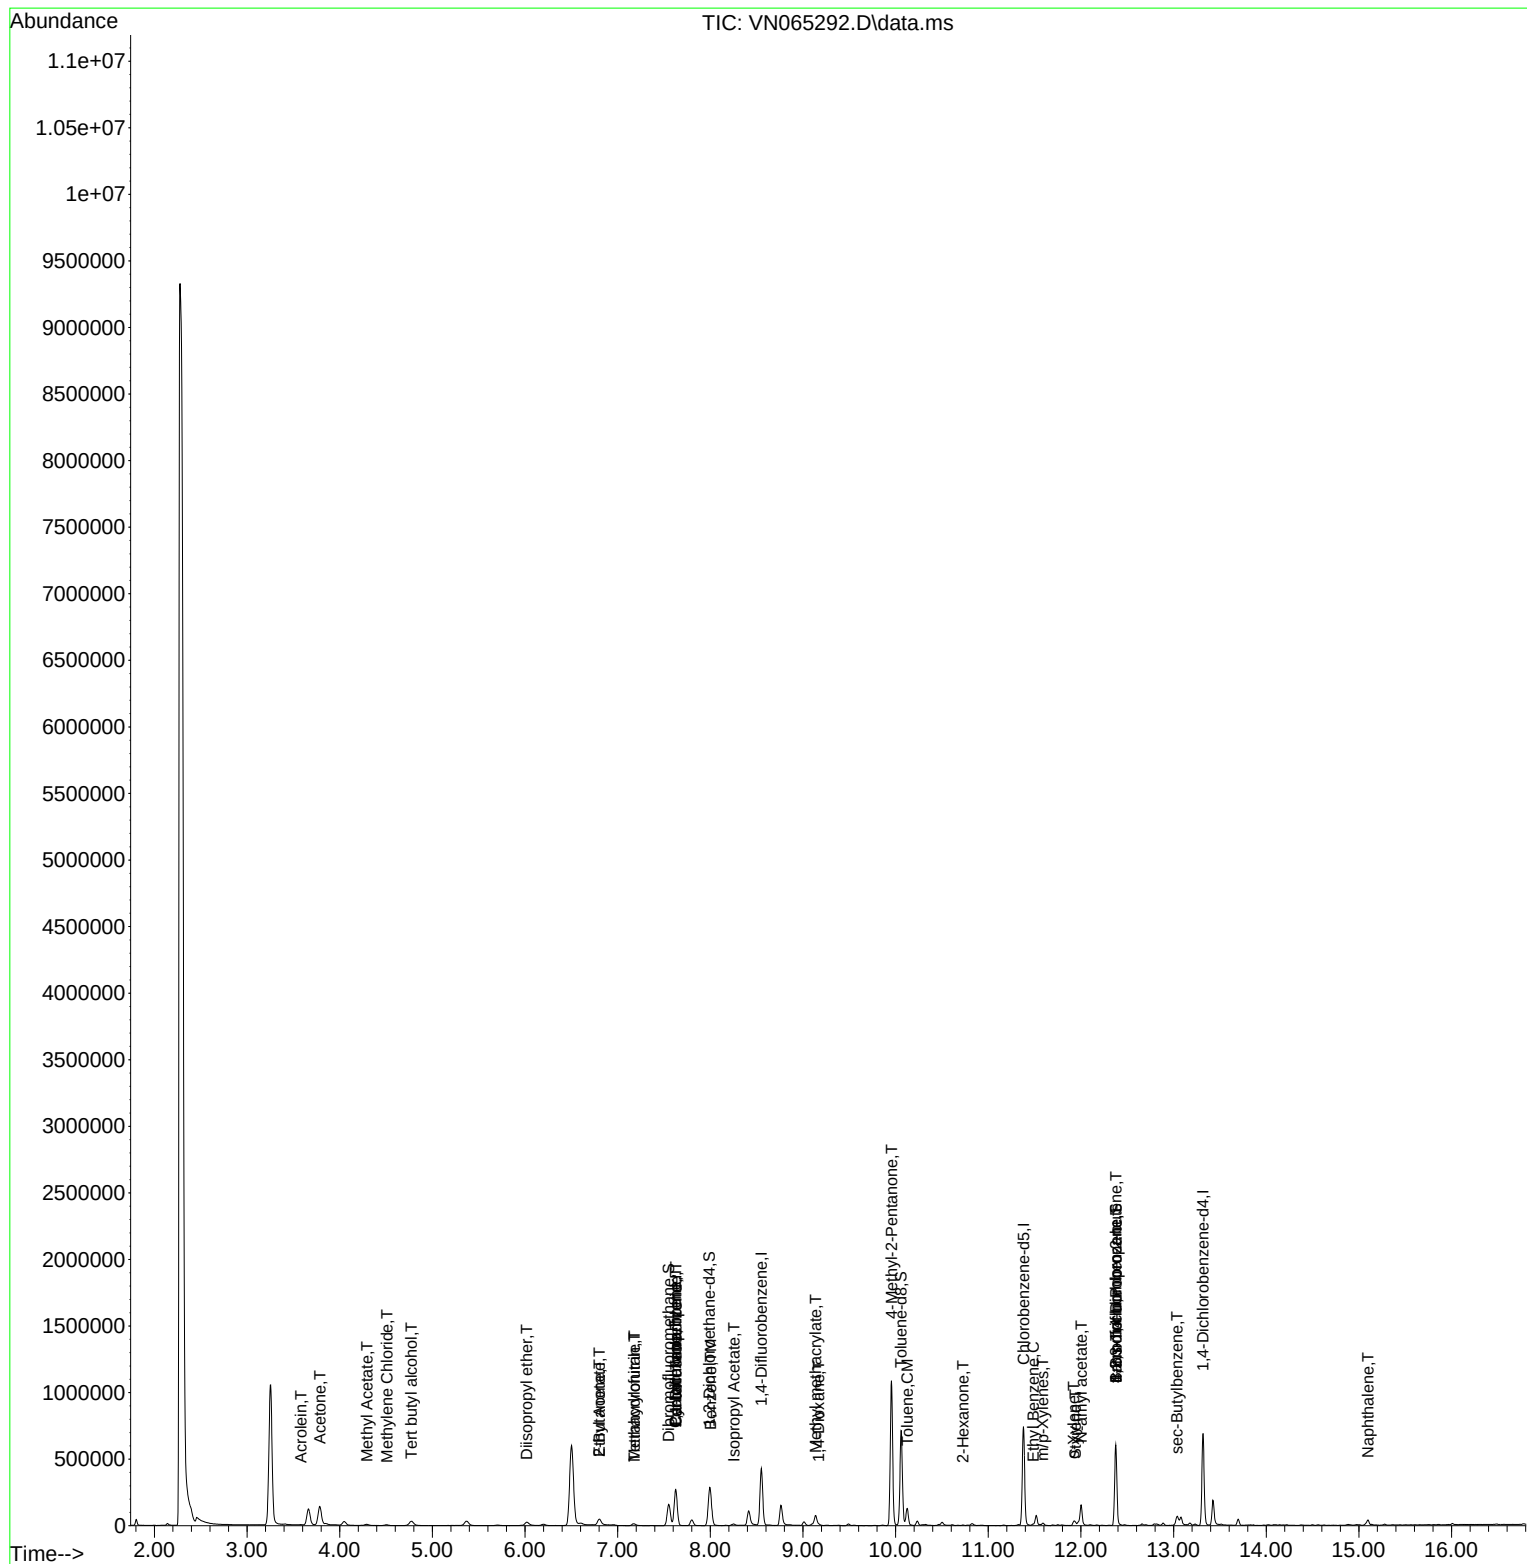


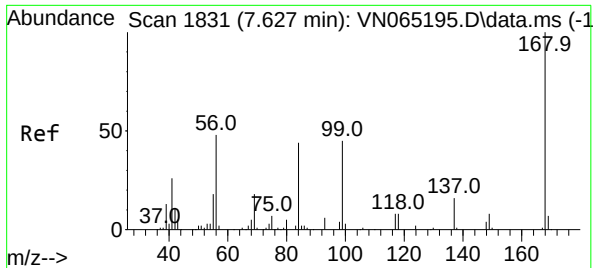

#1
Pentafluorobenzene
Concen: 50.00 ug/l
RT: 7.627 min Scan# 1831
Delta R.T. 0.000 min
Lab File: VN065292.D
Acq: 28 Dec 2020 17:45




Instrument :
MSVOA_N
ClientSampleId :
COMP-2


Tgt Ion:168 Resp: 243634
Ion Ratio Lower Upper
168 100
99 49.6 43.0 64.4

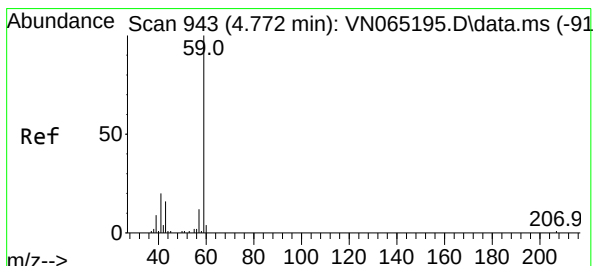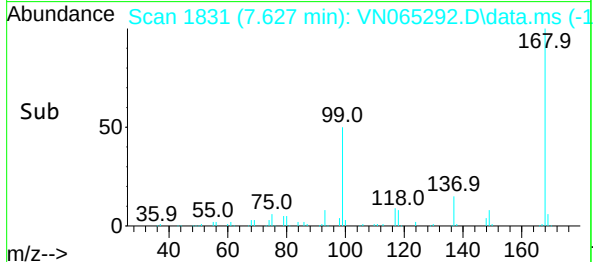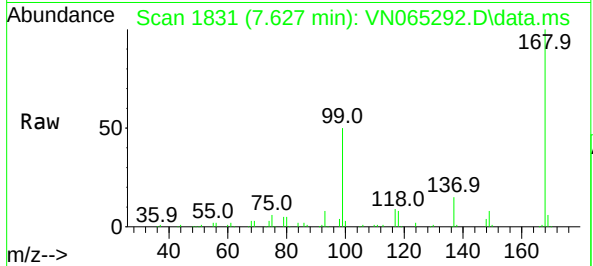

#11
Tert butyl alcohol
Concen: 136.90 ug/l
RT: 4.772 min Scan# 943
Delta R.T. 0.000 min
Lab File: VN065292.D
Acq: 28 Dec 2020 17:45

Tgt Ion: 59 Resp: 61609
Ion Ratio Lower Upper
59 100
57 10.5 7.9 11.9


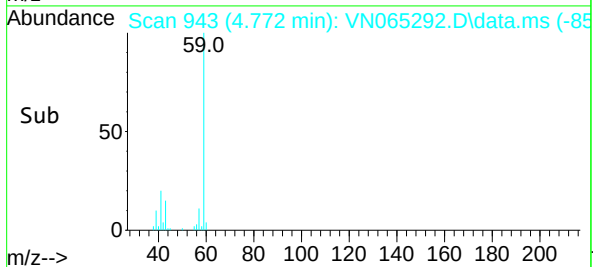

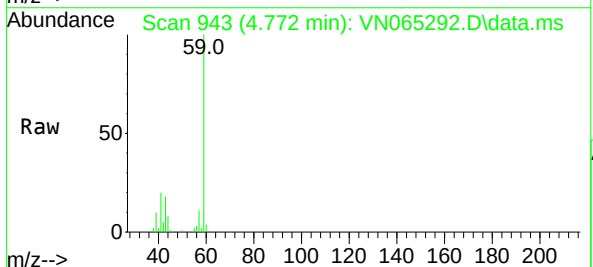




#13
Acrolein
Concen: 5.59 ug/l
RT: 3.583 min Scan# 573
Delta R.T. 0.010 min
Lab File: VN065292.D
Acq: 28 Dec 2020 17:45




Instrument :
MSVOA_N
ClientSampled :
COMP-2


Tgt Ion: 56 Resp: 976
Ion Ratio Lower Upper
56 100
55 59.9 56.5 84.7

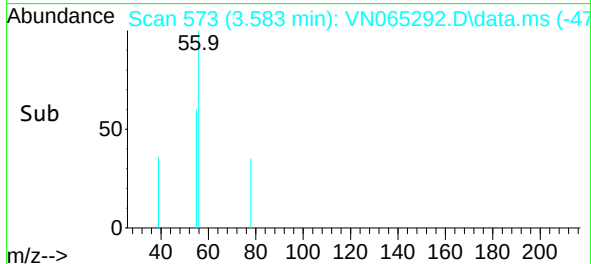

#16
Acetone
Concen: 193.62 ug/l
RT: 3.785 min Scan# 636
Delta R.T. 0.000 min
Lab File: VN065292.D
Acq: 28 Dec 2020 17:45


Tgt Ion: 43 Resp: 226276
Ion Ratio Lower Upper
43 100
58 34.6 25.7 38.5

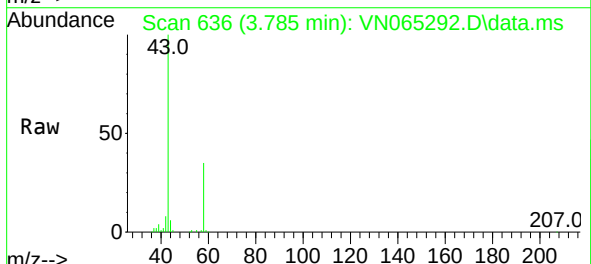






#18
Methyl Acetate
Concen: 6.76 ug/l
RT: 4.293 min Scan# 794
Delta R.T. 0.006 min
Lab File: VN065292.D
Acq: 28 Dec 2020 17:45

Instrument :
MSVOA_N
ClientSampled :
COMP-2







Tgt Ion: 43 Resp: 16702
Ion Ratio Lower Upper
43 100
74 25.2 20.2 30.2

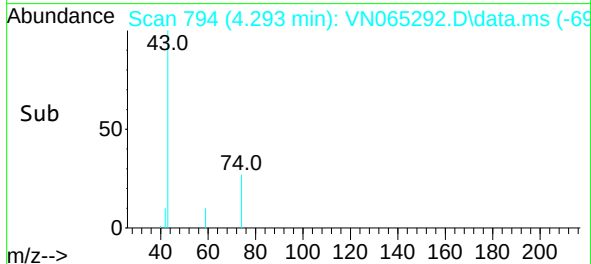

#20
Methylene Chloride
Concen: 1.50 ug/l
RT: 4.509 min Scan# 861
Delta R.T. 0.007 min
Lab File: VN065292.D
Acq: 28 Dec 2020 17:45


Tgt Ion: 84 Resp: 4037
Ion Ratio Lower Upper
84 100
49 121.1 93.4 140.0
51 40.6 28.2 42.4
86 61.6 51.7 77.5

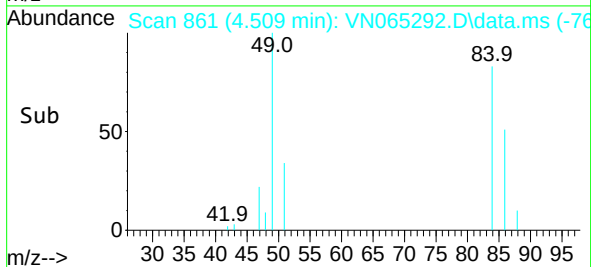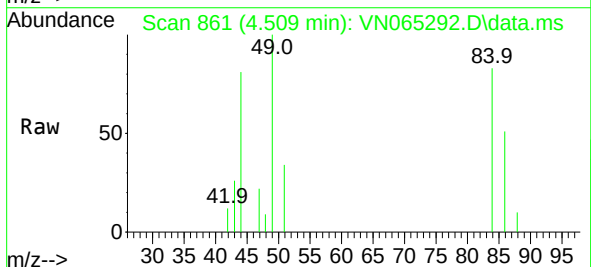






#22
Diisopropyl ether
Concen: 0.30 ug/l
RT: 6.016 min Scan# 1330
Delta R.T. 0.103 min
Lab File: VN065292.D
Acq: 28 Dec 2020 17:45

Instrument :
MSVOA_N
ClientSampled :
COMP-2







Tgt Ion	Ratio	Lower	Upper
45	100		
43	153.6	46.2	69.2#
87	0.0	24.1	36.1#
59	645.7	9.0	13.4#

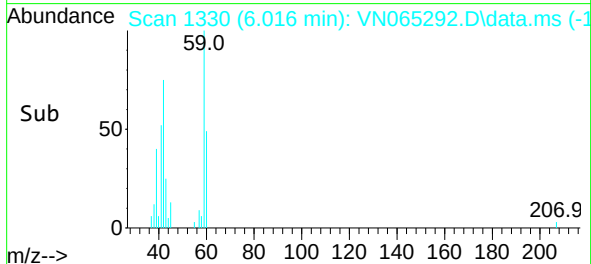

#25
2-Butanone
Concen: 49.97 ug/l
RT: 6.801 min Scan# 1574
Delta R.T. 0.003 min
Lab File: VN065292.D
Acq: 28 Dec 2020 17:45

Tgt Ion	Ratio	Lower	Upper
43	100		
72	27.4	21.0	31.6

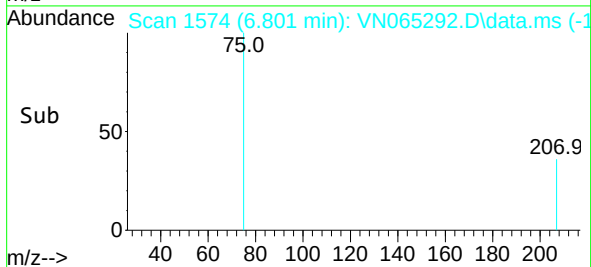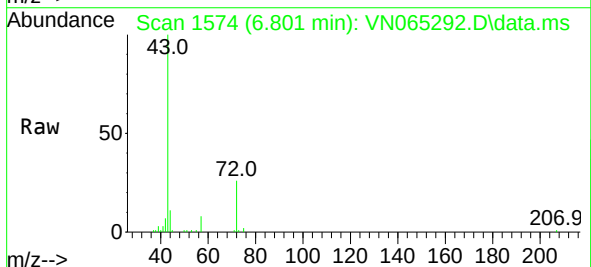

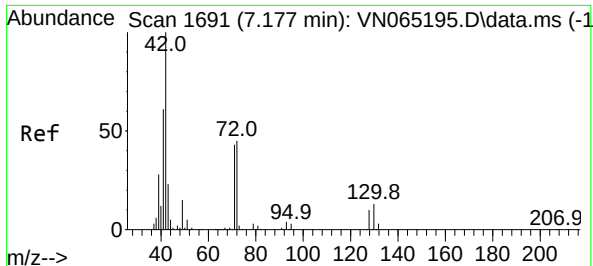

#29

Tetrahydrofuran

Concen: 1.09 ug/l

RT: 7.180 min Scan# 1692





Delta R.T. 0.003 min

Lab File: VN065292.D

Acq: 28 Dec 2020 17:45

Instrument :
MSVOA_N
ClientSampled :
COMP-2

Tgt Ion:	42	Resp:	1092
Ion	Ratio	Lower	Upper
42	100		
72	0.0	36.6	54.8#
71	0.0	33.6	50.4#

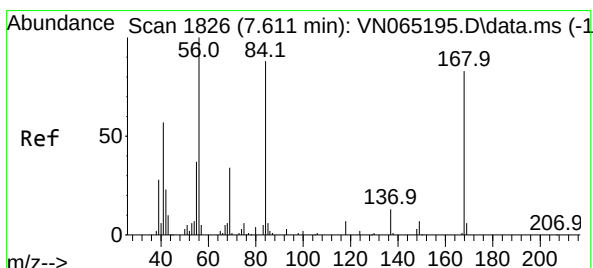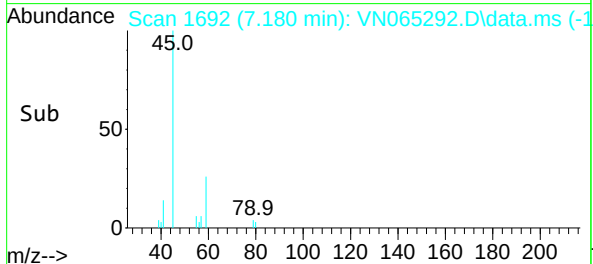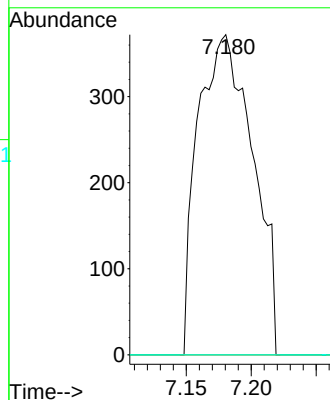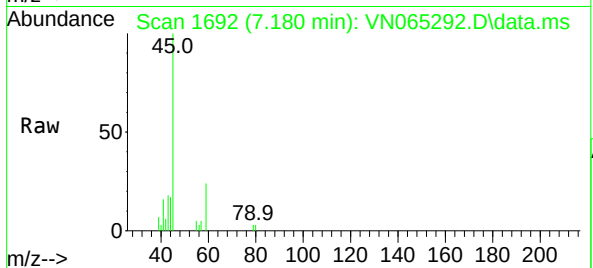

#31

Cyclohexane

Concen: 1.04 ug/l




RT: 7.624 min Scan# 1830


Delta R.T. 0.013 min

Lab File: VN065292.D

Acq: 28 Dec 2020 17:45

Tgt Ion:	56	Resp:	4233
Ion	Ratio	Lower	Upper
56	100		
69	173.5	27.5	41.3#
84	131.3	73.9	110.9#


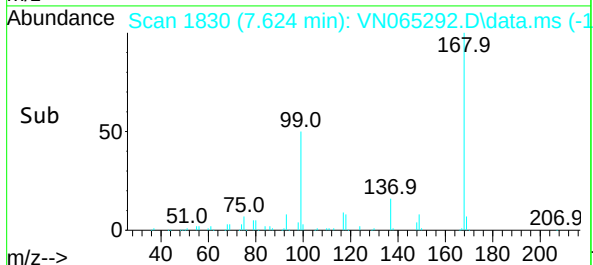
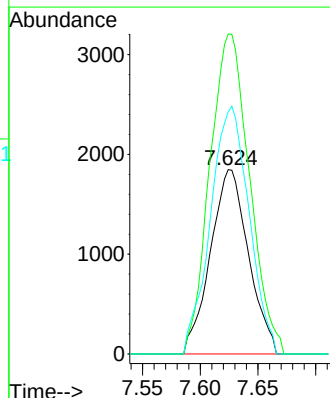
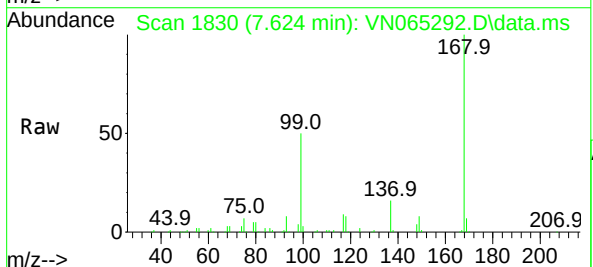


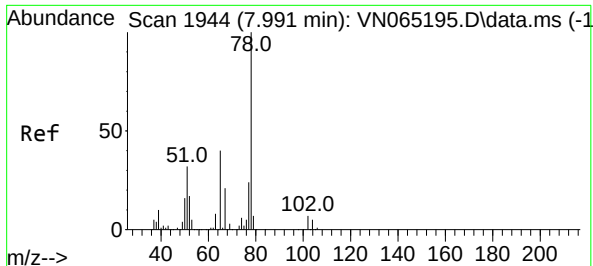

#33
1,2-Dichloroethane-d4
Concen: 50.90 ug/l
RT: 7.991 min Scan# 1944
Delta R.T. -0.000 min
Lab File: VN065292.D
Acq: 28 Dec 2020 17:45




Instrument :
MSVOA_N
ClientSampleId :
COMP-2


Tgt Ion: 65 Resp: 140008
Ion Ratio Lower Upper
65 100
67 51.9 0.0 108.2

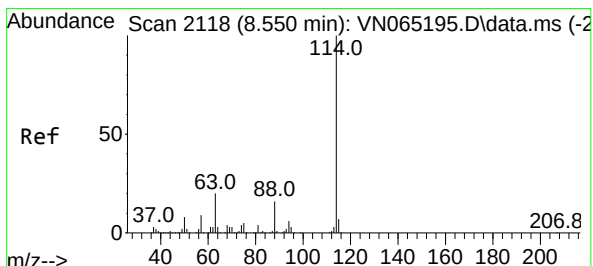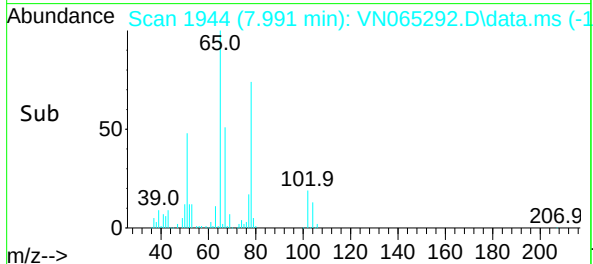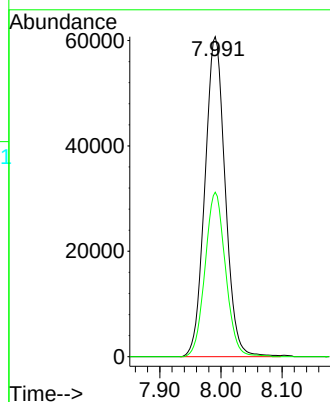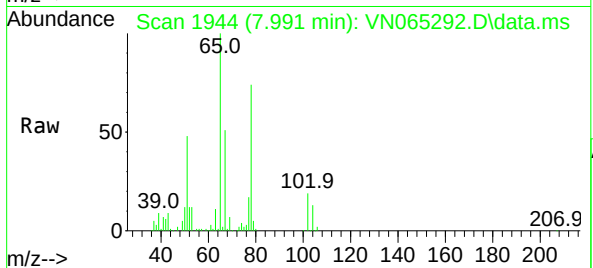

#34
1,4-Difluorobenzene
Concen: 50.00 ug/l
RT: 8.550 min Scan# 2118
Delta R.T. 0.000 min
Lab File: VN065292.D
Acq: 28 Dec 2020 17:45

Tgt Ion: 114 Resp: 403678
Ion Ratio Lower Upper
114 100
63 19.8 0.0 38.6
88 14.8 0.0 32.6

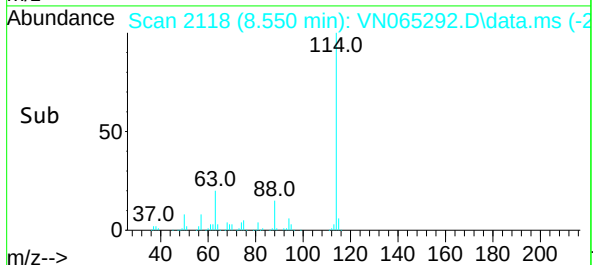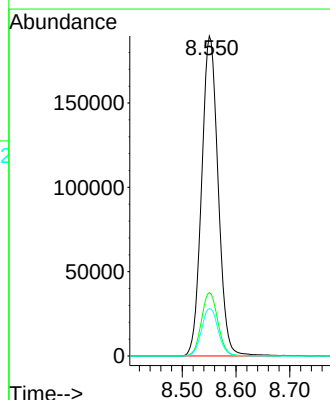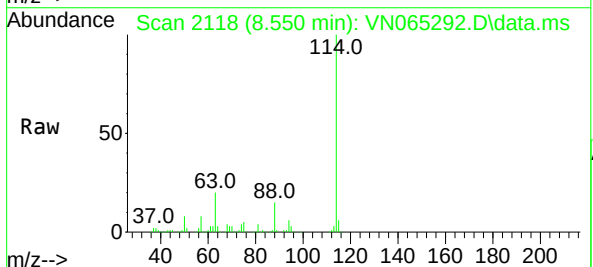

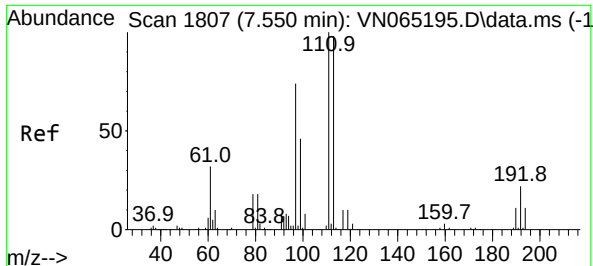

#35

Dibromofluoromethane

Concen: 50.86 ug/l

RT: 7.550 min Scan# 1807

Delta R.T. 0.000 min

Lab File: VN065292.D

Acq: 28 Dec 2020 17:45





Tgt Ion:113 Resp: 123866

Ion Ratio Lower Upper

113 100

111 102.3 81.6 122.4

192 23.2 16.2 24.2

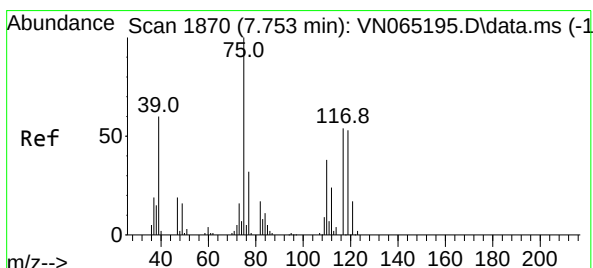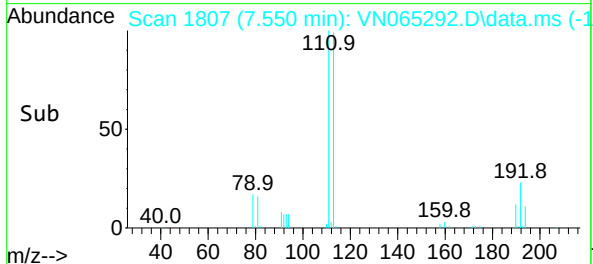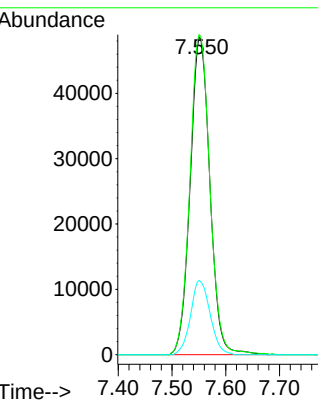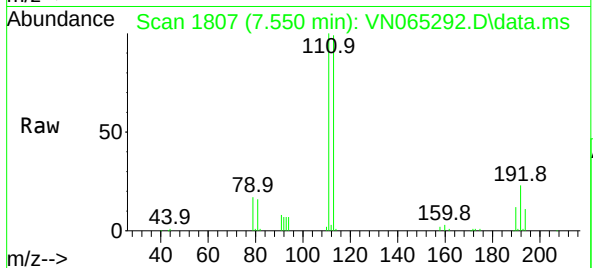

#36

1,1-Dichloropropene

Concen: 4.25 ug/l

RT: 7.624 min Scan# 1830

Delta R.T. -0.129 min

Lab File: VN065292.D

Acq: 28 Dec 2020 17:45




Tgt Ion: 75 Resp: 15597


Ion Ratio Lower Upper

75 100

110 8.1 17.8 53.3#

77 0.0 25.0 37.4#


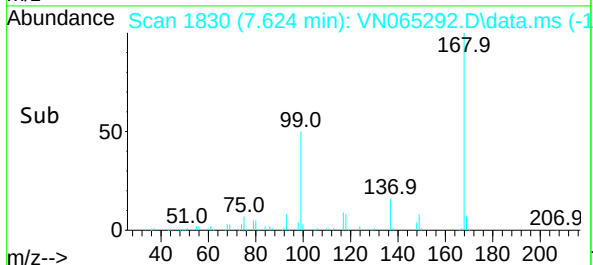
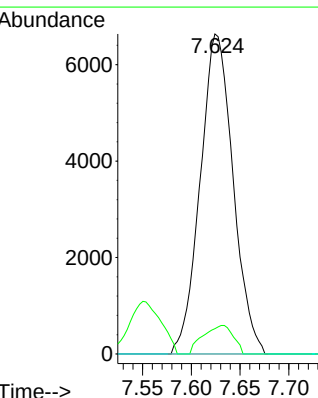
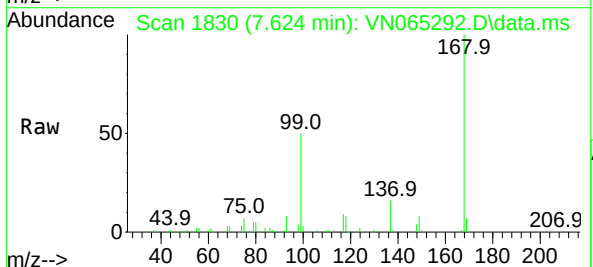


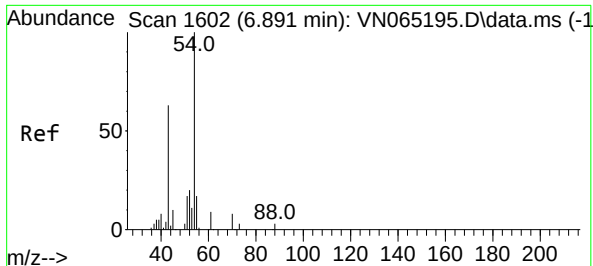

#37
Ethyl Acetate
Concen: 21.21 ug/l
RT: 6.801 min Scan# 1574
Delta R.T. -0.090 min
Lab File: VN065292.D
Acq: 28 Dec 2020 17:45




Instrument :
MSVOA_N
ClientSampled :
COMP-2


Tgt Ion: 43 Resp: 77154
Ion Ratio Lower Upper
43 100
61 0.0 12.8 19.2#
70 0.0 8.8 13.2#

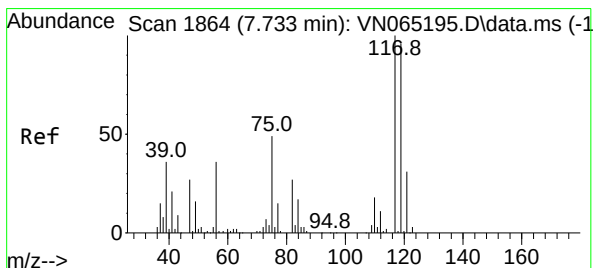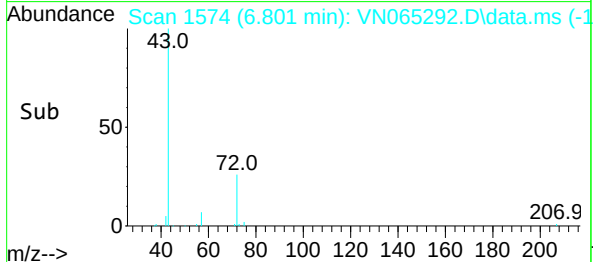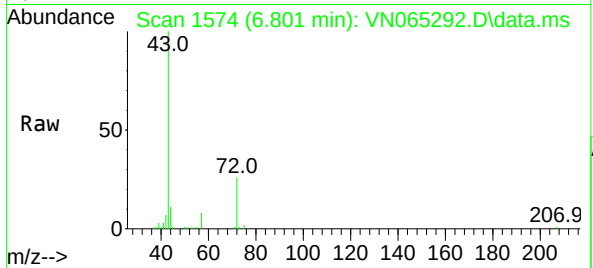

#38
Carbon Tetrachloride
Concen: 5.45 ug/l
RT: 7.627 min Scan# 1831
Delta R.T. -0.106 min
Lab File: VN065292.D
Acq: 28 Dec 2020 17:45

Tgt Ion: 117 Resp: 21000
Ion Ratio Lower Upper
117 100
119 4.7 76.7 115.1#
121 0.0 25.4 38.2#


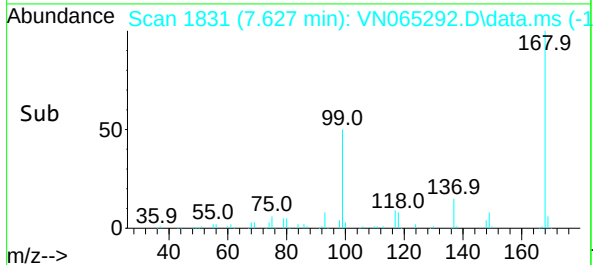

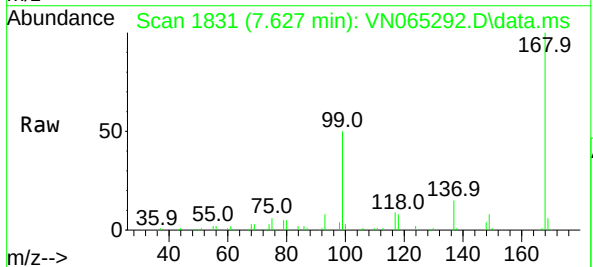




#40
Benzene
Concen: 13.30 ug/l
RT: 8.004 min Scan# 1948
Delta R.T. -0.000 min
Lab File: VN065292.D
Acq: 28 Dec 2020 17:45




Instrument :
MSVOA_N
ClientSampleId :
COMP-2


Tgt Ion: 78 Resp: 145263
Ion Ratio Lower Upper
78 100
77 23.7 17.9 26.9

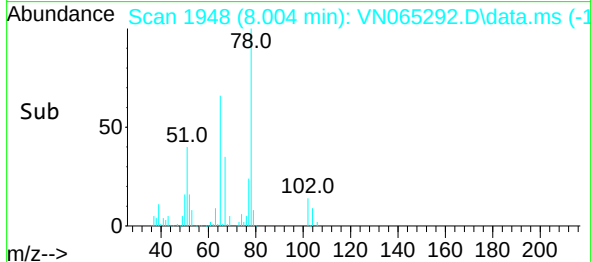

#41
Methacrylonitrile
Concen: 2.02 ug/l
RT: 7.180 min Scan# 1692
Delta R.T. 0.051 min
Lab File: VN065292.D
Acq: 28 Dec 2020 17:45

Tgt Ion: 41 Resp: 3830
Ion Ratio Lower Upper
41 100
39 37.7 51.0 76.6#
67 0.0 79.8 119.8#
52 0.0 31.5 47.3#

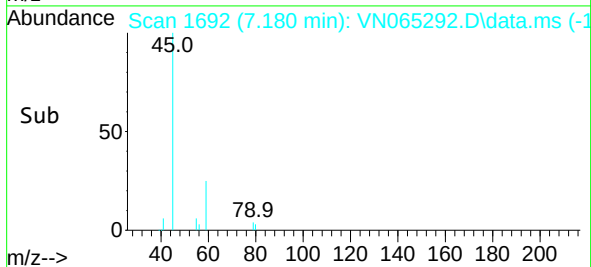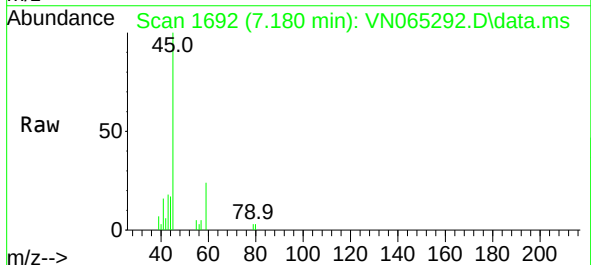




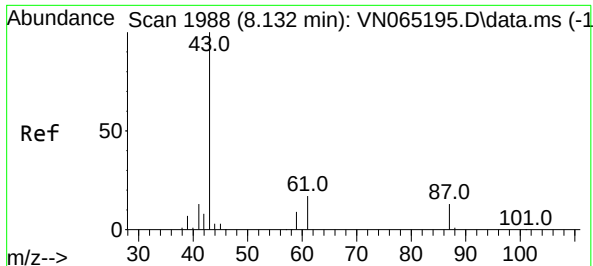


#43

Isopropyl Acetate
 Concen: 0.70 ug/l
 RT: 8.254 min Scan# 2026
 Delta R.T. 0.122 min
 Lab File: VN065292.D
 Acq: 28 Dec 2020 17:45

Instrument :
 MSVOA_N
 ClientSampled :
 COMP-2




Tgt Ion: 43 Resp: 4395
 Ion Ratio Lower Upper
 43 100
 61 0.0 17.2 25.8#
 87 0.0 11.4 17.0#

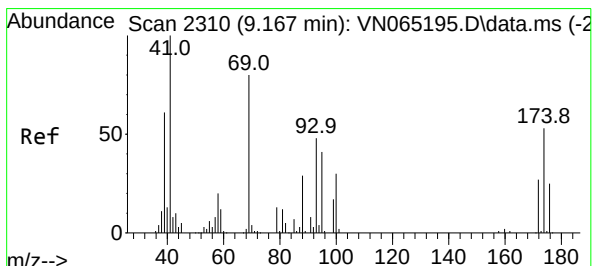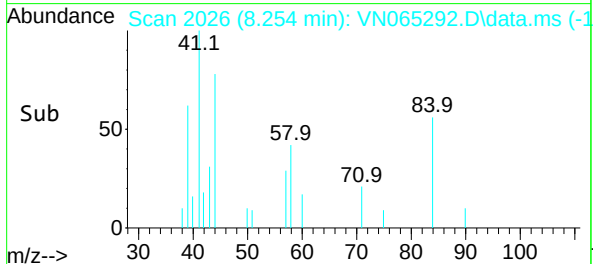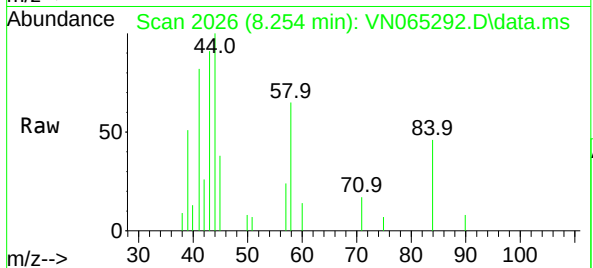


#48

Methyl methacrylate
 Concen: 7.39 ug/l
 RT: 9.135 min Scan# 2300
 Delta R.T. -0.032 min
 Lab File: VN065292.D
 Acq: 28 Dec 2020 17:45

Tgt Ion: 41 Resp: 22508
 Ion Ratio Lower Upper
 41 100
 69 0.0 71.8 107.8#
 39 58.0 44.1 66.1


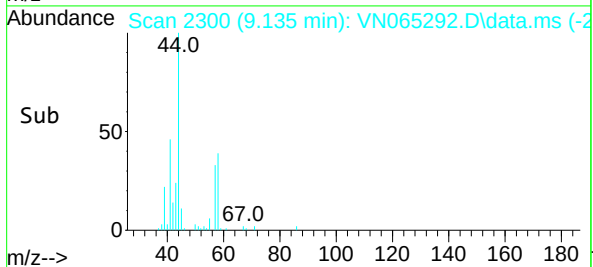

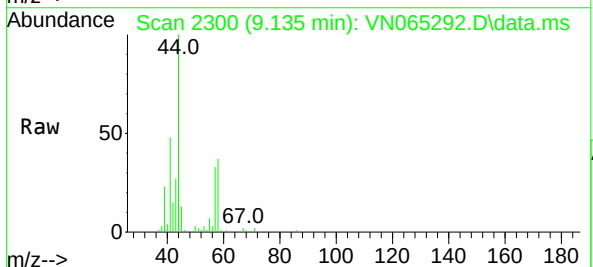




#49
1,4-Dioxane
Concen: 116.74 ug/l
RT: 9.171 min Scan# 2311
Delta R.T. -0.000 min
Lab File: VN065292.D
Acq: 28 Dec 2020 17:45




Instrument :
MSVOA_N
ClientSampled :
COMP-2


Tgt Ion: 88 Resp: 5759
Ion Ratio Lower Upper
88 100
43 0.0 24.2 36.4#
58 0.0 52.5 78.7#

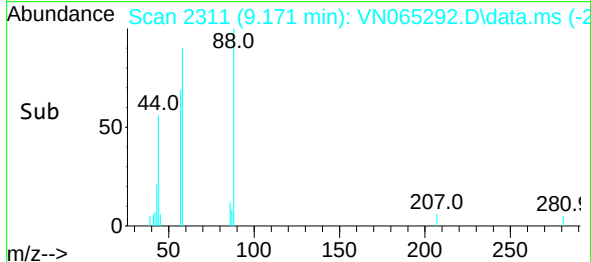

#50
Toluene-d8
Concen: 55.61 ug/l
RT: 10.058 min Scan# 2587
Delta R.T. 0.000 min
Lab File: VN065292.D
Acq: 28 Dec 2020 17:45

Tgt Ion: 98 Resp: 507581
Ion Ratio Lower Upper
98 100
100 64.3 51.7 77.5


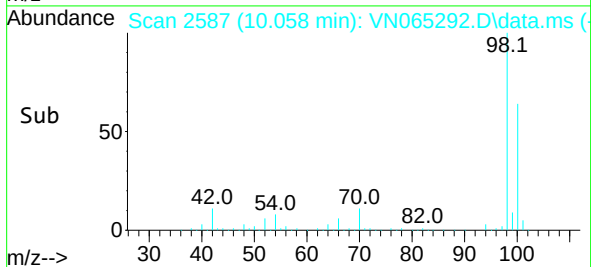

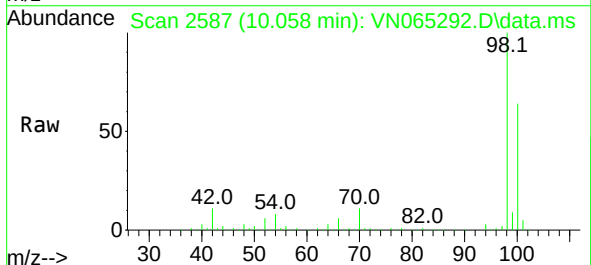




#51
4-Methyl-2-Pentanone
Concen: 208.41 ug/l
RT: 9.955 min Scan# 2555
Delta R.T. 0.000 min
Lab File: VN065292.D
Acq: 28 Dec 2020 17:45




Instrument :
MSVOA_N
ClientSampled :
COMP-2


Tgt Ion: 43 Resp: 734741
Ion Ratio Lower Upper
43 100
58 39.0 32.4 48.6

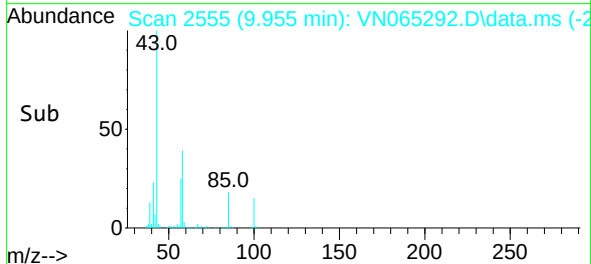

#52
Toluene
Concen: 8.08 ug/l
RT: 10.126 min Scan# 2608
Delta R.T. -0.000 min
Lab File: VN065292.D
Acq: 28 Dec 2020 17:45

Tgt Ion: 92 Resp: 55576
Ion Ratio Lower Upper
92 100
91 177.1 139.1 208.7


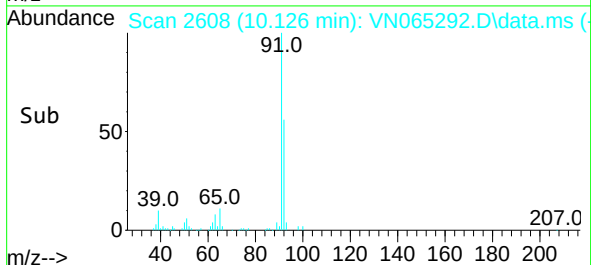

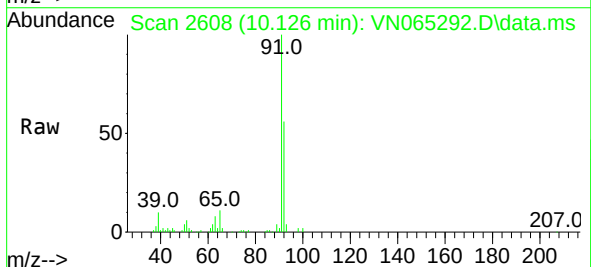




#59
2-Hexanone
Concen: 1.13 ug/l
RT: 10.727 min Scan# 2795
Delta R.T. 0.003 min
Lab File: VN065292.D
Acq: 28 Dec 2020 17:45




Instrument :
MSVOA_N
ClientSampled :
COMP-2


Tgt Ion: 43 Resp: 2929
Ion Ratio Lower Upper
43 100
58 50.3 28.3 84.9

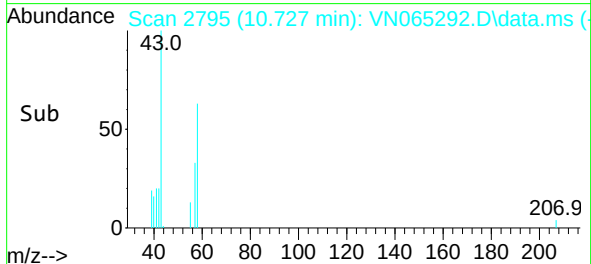

#62
4-Bromofluorobenzene
Concen: 56.37 ug/l
RT: 12.376 min Scan# 3308
Delta R.T. 0.000 min
Lab File: VN065292.D
Acq: 28 Dec 2020 17:45

Tgt Ion: 95 Resp: 206091
Ion Ratio Lower Upper
95 100
174 91.3 0.0 160.4
176 88.7 0.0 158.4


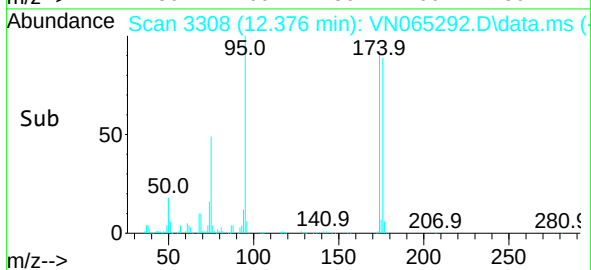

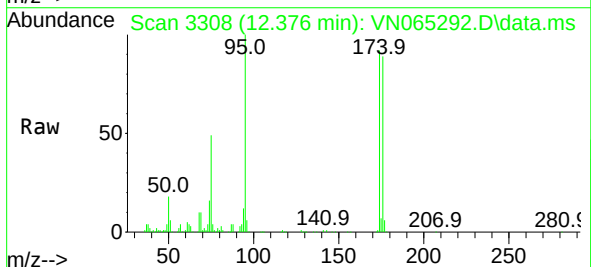


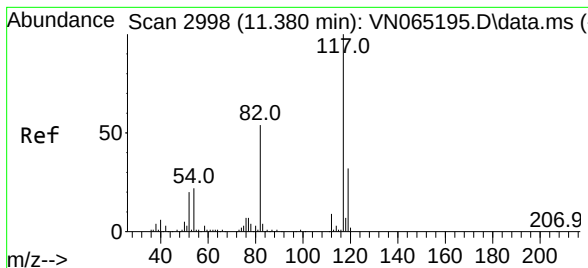

#63
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 11.380 min Scan# 2998
Delta R.T. -0.000 min
Lab File: VN065292.D
Acq: 28 Dec 2020 17:45




Instrument :
MSVOA_N
ClientSampled :
COMP-2


Tgt Ion:117 Resp: 432535
Ion Ratio Lower Upper
117 100
82 53.4 44.2 66.2
119 31.9 25.8 38.6

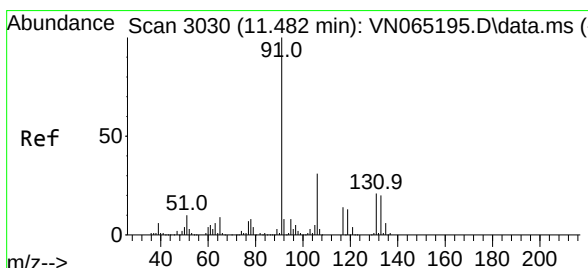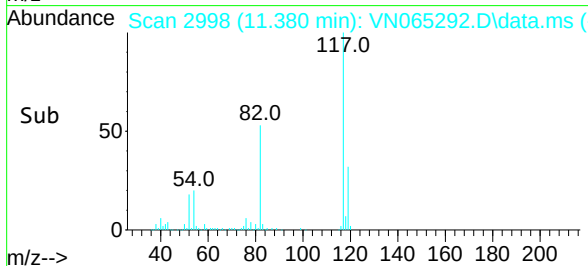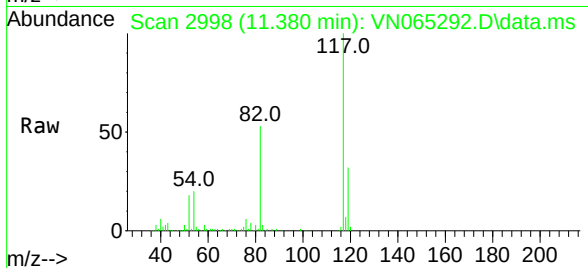

#67
Ethyl Benzene
Concen: 0.47 ug/l
RT: 11.486 min Scan# 3031
Delta R.T. 0.004 min
Lab File: VN065292.D
Acq: 28 Dec 2020 17:45

Tgt Ion: 91 Resp: 7399
Ion Ratio Lower Upper
91 100
106 33.2 25.2 37.8


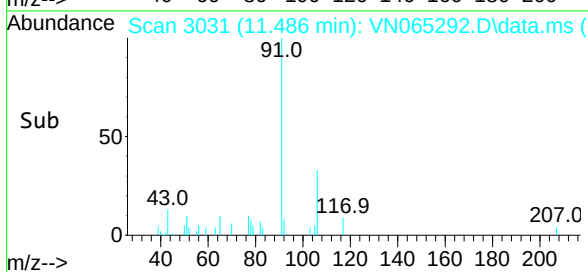

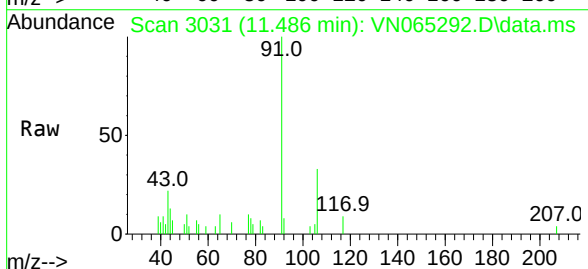


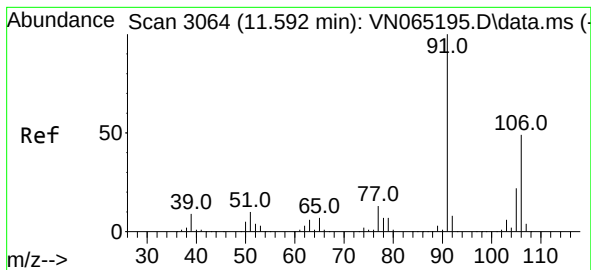

#68
m/p-Xylenes
Concen: 0.99 ug/l
RT: 11.589 min Scan# 3063
Delta R.T. -0.003 min
Lab File: VN065292.D
Acq: 28 Dec 2020 17:45




Instrument :
MSVOA_N
ClientSampled :
COMP-2


Tgt Ion:106 Resp: 5943
Ion Ratio Lower Upper
106 100
91 202.1 161.0 241.4

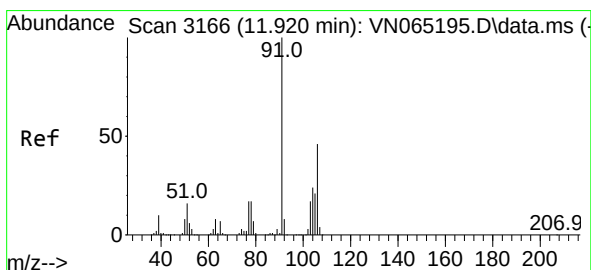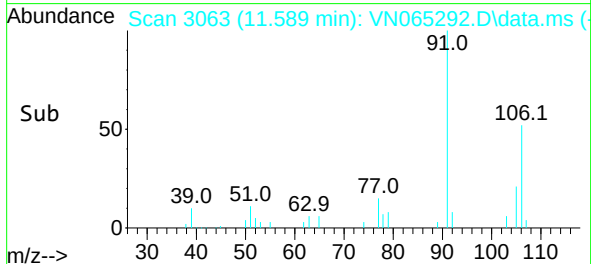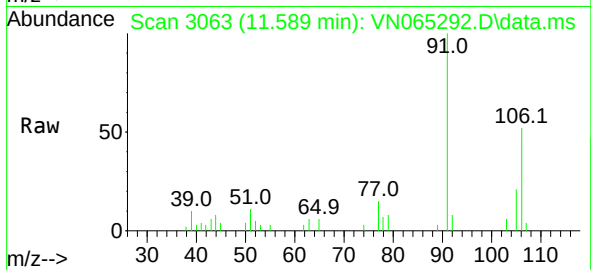

#69
o-Xylene
Concen: 0.65 ug/l
RT: 11.923 min Scan# 3167
Delta R.T. 0.003 min
Lab File: VN065292.D
Acq: 28 Dec 2020 17:45

Tgt Ion:106 Resp: 3788
Ion Ratio Lower Upper
106 100
91 211.5 105.5 316.5

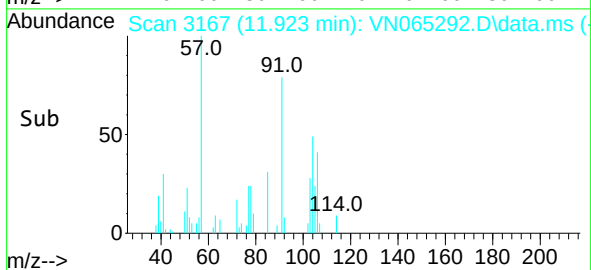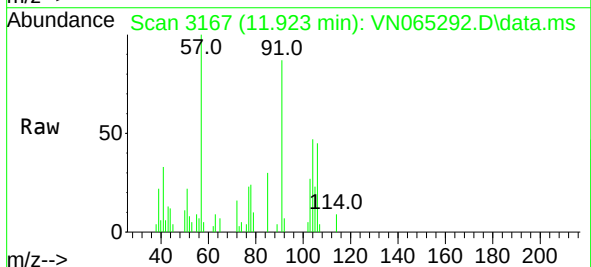

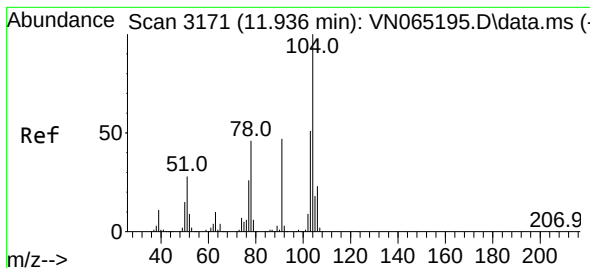

#70

Styrene

Concen: 1.16 ug/l

RT: 11.939 min Scan# 3172

Delta R.T. 0.003 min

Lab File: VN065292.D

Acq: 28 Dec 2020 17:45





Instrument :

MSVOA_N

ClientSampled :

COMP-2

Tgt Ion:	104	Resp:	11246
Ion Ratio	Lower	Upper	
104	100		
78	47.1	39.0	58.6
103	54.6	44.3	66.5

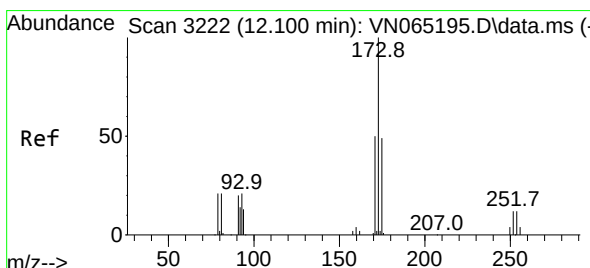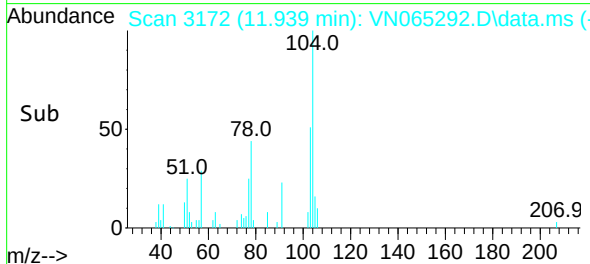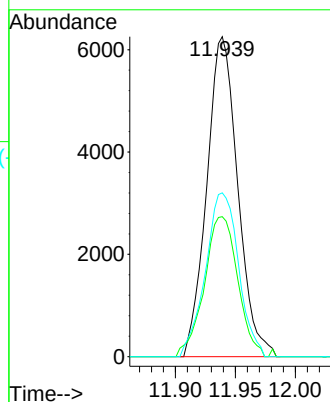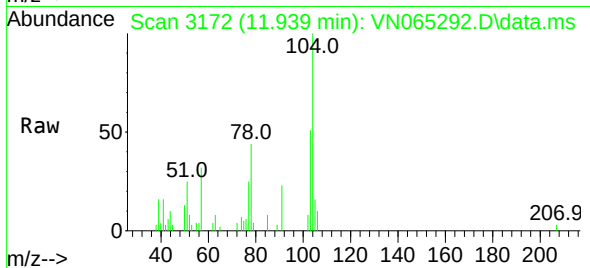

#71

Bromoform

Concen: 0.41 ug/l




RT: 12.376 min Scan# 3308


Delta R.T. 0.276 min

Lab File: VN065292.D

Acq: 28 Dec 2020 17:45

Tgt Ion:	173	Resp:	1207
Ion Ratio	Lower	Upper	
173	100		
175	946.6	24.3	72.8#
254	0.0	0.0	0.0


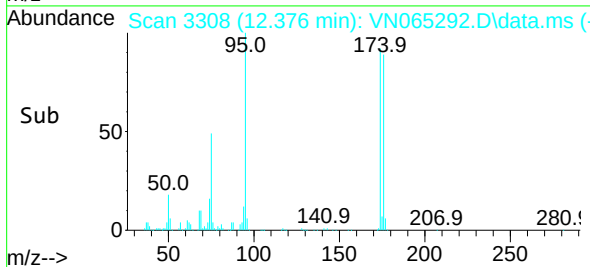
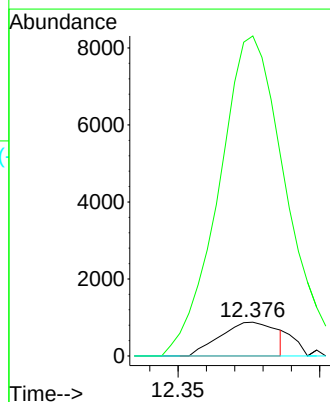
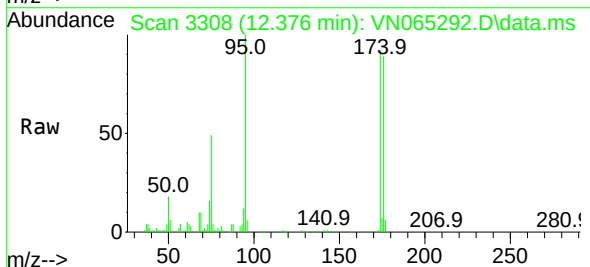


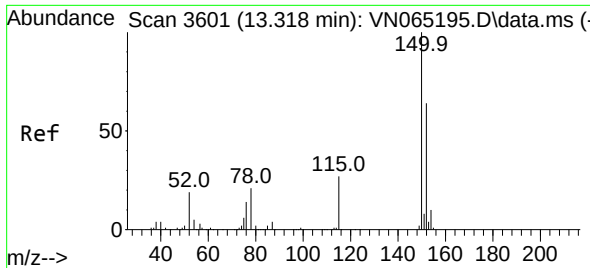

#72
1,4-Dichlorobenzene-d4
Concen: 50.00 ug/l
RT: 13.318 min Scan# 3601
Delta R.T. 0.000 min
Lab File: VN065292.D
Acq: 28 Dec 2020 17:45




Instrument :
MSVOA_N
ClientSampled :
COMP-2


Tgt Ion:152 Resp: 201208
Ion Ratio Lower Upper
152 100
115 55.3 29.7 89.1
150 156.5 0.0 350.6

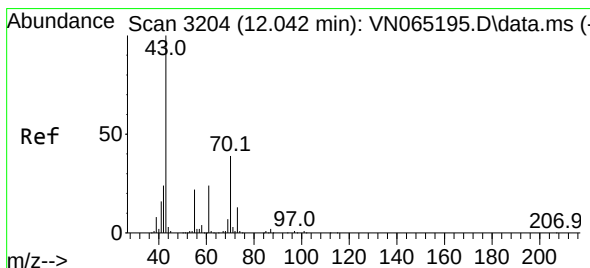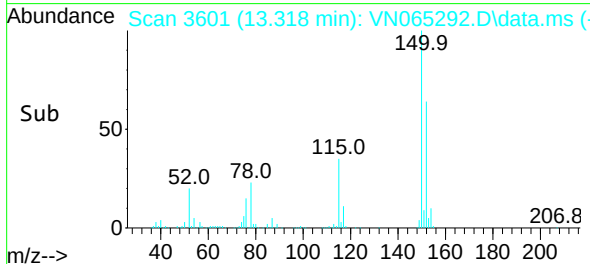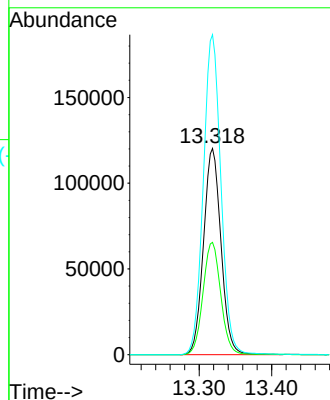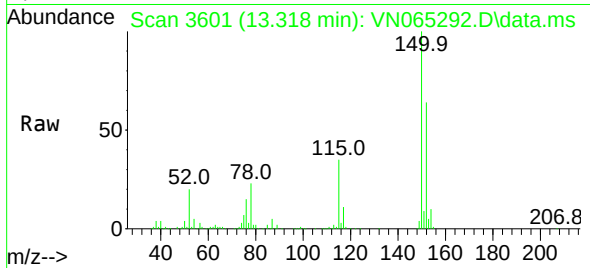

#74
N-ethyl acetate
Concen: 17.23 ug/l
RT: 12.003 min Scan# 3192
Delta R.T. -0.039 min
Lab File: VN065292.D
Acq: 28 Dec 2020 17:45

Tgt Ion: 43 Resp: 105125
Ion Ratio Lower Upper
43 100
70 0.8 34.5 51.7#
55 0.0 20.4 30.6#
61 0.0 20.0 30.0#


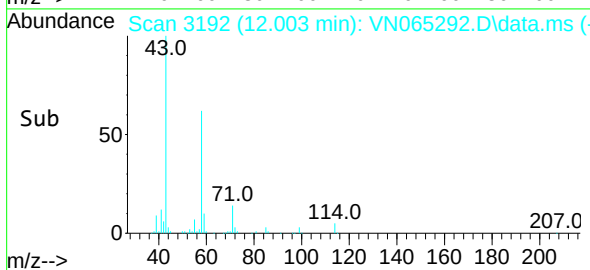
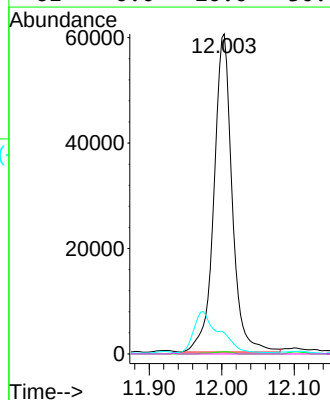
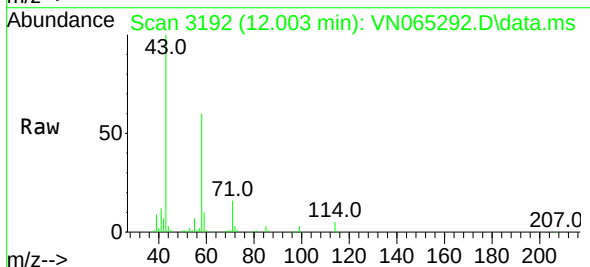




#76
1,2,3-Trichloropropane
Concen: 24.65 ug/l
RT: 12.376 min Scan# 3308
Delta R.T. -0.151 min
Lab File: VN065292.D
Acq: 28 Dec 2020 17:45




Instrument :
MSVOA_N
ClientSampled :
COMP-2


Tgt Ion: 75 Resp: 101170
Ion Ratio Lower Upper
75 100
77 1.2 0.0 0.0#

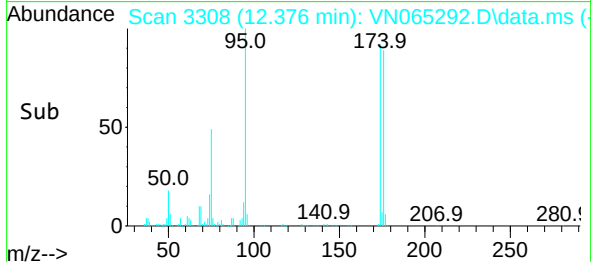

#81
trans-1,4-Dichloro-2-butene
Concen: 62.15 ug/l
RT: 12.376 min Scan# 3308
Delta R.T. 0.103 min
Lab File: VN065292.D
Acq: 28 Dec 2020 17:45

Tgt Ion: 75 Resp: 101170
Ion Ratio Lower Upper
75 100
53 0.0 67.0 100.4#
89 0.0 39.6 59.4#


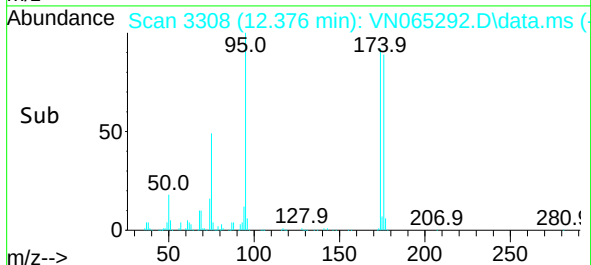

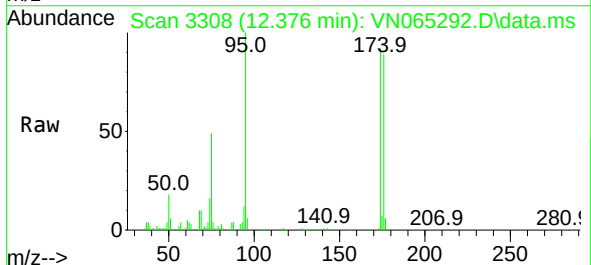




#85
 sec-Butylbenzene
 Concen: 2.50 ug/l
 RT: 13.039 min Scan# 3514
 Delta R.T. -0.106 min
 Lab File: VN065292.D
 Acq: 28 Dec 2020 17:45

Instrument :
 MSVOA_N
 ClientSampled :
 COMP-2

Tgt Ion:105 Resp: 36887
 Ion Ratio Lower Upper
 105 100
 134 0.0 10.1 30.1#



#95
 Naphthalene
 Concen: 6.21 ug/l
 RT: 15.097 min Scan# 4154
 Delta R.T. 0.001 min
 Lab File: VN065292.D
 Acq: 28 Dec 2020 17:45

Tgt Ion:128 Resp: 31707
 Ion Ratio Lower Upper
 128 100
 127 13.1 10.3 15.5
 129 11.6 8.7 13.1

