


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN122820\
 Data File : VN065273.D
 Acq On : 28 Dec 2020 9:27
 Operator : JC/MD
 Sample : BFB
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N122220W.M
 Title : Sw846 8260
 Last Update : Tue Dec 22 15:42:18 2020

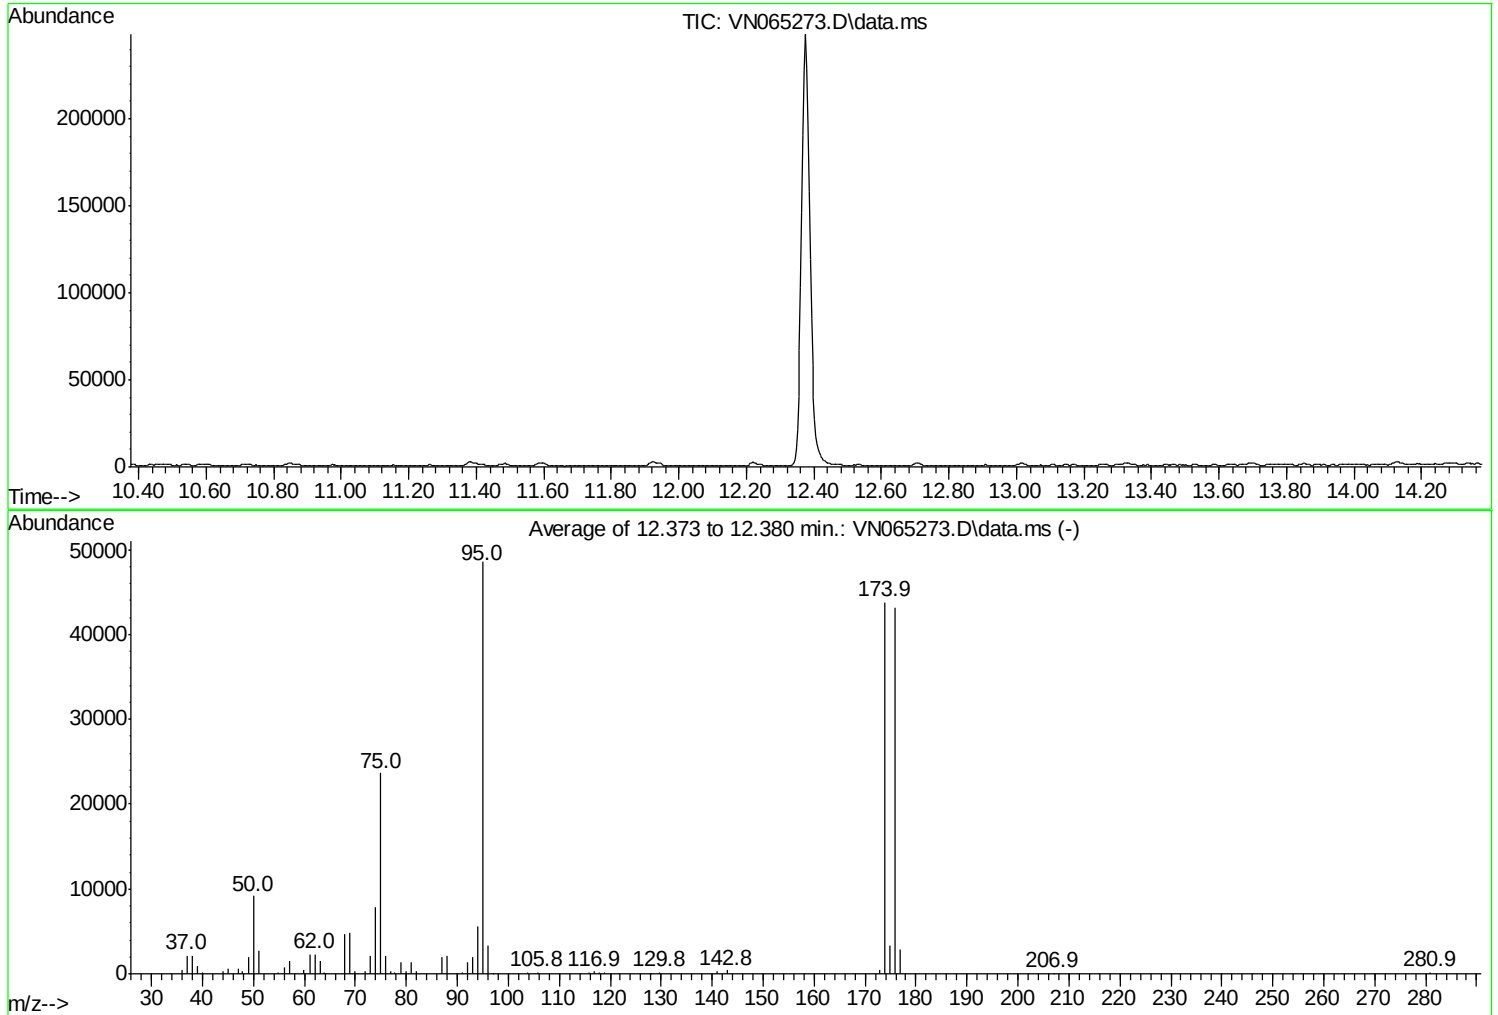

AutoFind: Scans 3307, 3308, 3309; Background Corrected with Scan 3293

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.8	9149	PASS
75	95	30	60	48.6	23621	PASS
95	95	100	100	100.0	48573	PASS
96	95	5	9	6.8	3310	PASS
173	174	0.00	2	1.0	457	PASS
174	95	50	100	90.1	43771	PASS
175	174	5	9	7.4	3252	PASS
176	174	95	101	98.7	43200	PASS
177	176	5	9	6.7	2896	PASS