

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN122822\
 Data File : VN075996.D
 Acq On : 28 Dec 2022 13:45
 Operator : JC\MD
 Sample : N6200-02
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 PL-502A-COMP-3

Quant Time: Dec 29 04:50:15 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N121422W.M
 Quant Title : SW846 8260
 QLast Update : Wed Dec 14 13:03:41 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	8.229	168	324721	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.106	114	516732	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.870	117	468416	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.794	152	202829	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.588	65	171784	48.627	ug/l	0.00
Spiked Amount 50.000	Range 74 - 125		Recovery =	97.260%		
35) Dibromofluoromethane	8.177	113	154540	48.293	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery =	96.580%		
50) Toluene-d8	10.570	98	617065	51.574	ug/l	0.00
Spiked Amount 50.000	Range 86 - 113		Recovery =	103.140%		
62) 4-Bromofluorobenzene	12.853	95	195177	49.252	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery =	98.500%		
Target Compounds						Qvalue
3) Chloromethane	2.365	50	734	0.256	ug/l #	40
11) Tert butyl alcohol	5.536	59	2328	4.657	ug/l #	72
16) Acetone	4.447	43	60533	49.708	ug/l	98
18) Methyl Acetate	5.036	43	2539	0.705	ug/l #	54
20) Methylene Chloride	5.294	84	16128	4.366	ug/l #	90
25) 2-Butanone	7.500	43	19673	11.538	ug/l #	86
29) Tetrahydrofuran	7.859	42	2125	1.989	ug/l	89
31) Cyclohexane	8.235	56	6285	1.242	ug/l #	1
36) 1,1-Dichloropropene	8.235	75	22936	5.396	ug/l #	48
37) Ethyl Acetate	7.571	43	31584	9.250	ug/l	98
38) Carbon Tetrachloride	8.235	117	31992	6.724	ug/l #	16
41) Methacrylonitrile	7.847	41	832	0.469	ug/l #	28
42) 1,2-Dichloroethane	8.694	62	1241	0.285	ug/l #	72
43) Isopropyl Acetate	8.694	43	210687	37.405	ug/l #	79
45) 1,2-Dichloropropane	9.747	63	2097	0.657	ug/l #	43
48) Methyl methacrylate	9.659	41	4487	1.769	ug/l #	6
49) 1,4-Dioxane	9.741	88	118	1.892	ug/l #	1
51) 4-Methyl-2-Pentanone	10.453	43	17755	5.212	ug/l #	81
52) Toluene	10.635	92	3074	0.360	ug/l	99
53) t-1,3-Dichloropropene	10.723	75	1110	0.244	ug/l	95
54) cis-1,3-Dichloropropene	10.365	75	64406	12.909	ug/l #	64
56) Ethyl methacrylate	10.988	69	1582	0.355	ug/l #	1
57) 1,3-Dichloropropane	11.206	76	8469	1.540	ug/l #	42
59) 2-Hexanone	11.176	43	140891	56.716	ug/l #	20
71) Bromoform	12.847	173	1037	0.400	ug/l #	1
74) N-amyl acetate	12.488	43	1307	0.304	ug/l #	44
76) 1,2,3-Trichloropropane	12.853	75	101080	24.723	ug/l #	1
81) trans-1,4-Dichloro-2-b...	12.853	75	101080	88.990	ug/l #	12
95) Naphthalene	15.653	128	2185	2.367	ug/l #	76


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN122822\
Data File : VN075996.D
Acq On : 28 Dec 2022 13:45
Operator : JC\MD
Sample : N6200-02
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
PL-502A-COMP-3

Quant Time: Dec 29 04:50:15 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N121422W.M
Quant Title : SW846 8260
QLast Update : Wed Dec 14 13:03:41 2022
Response via : Initial Calibration




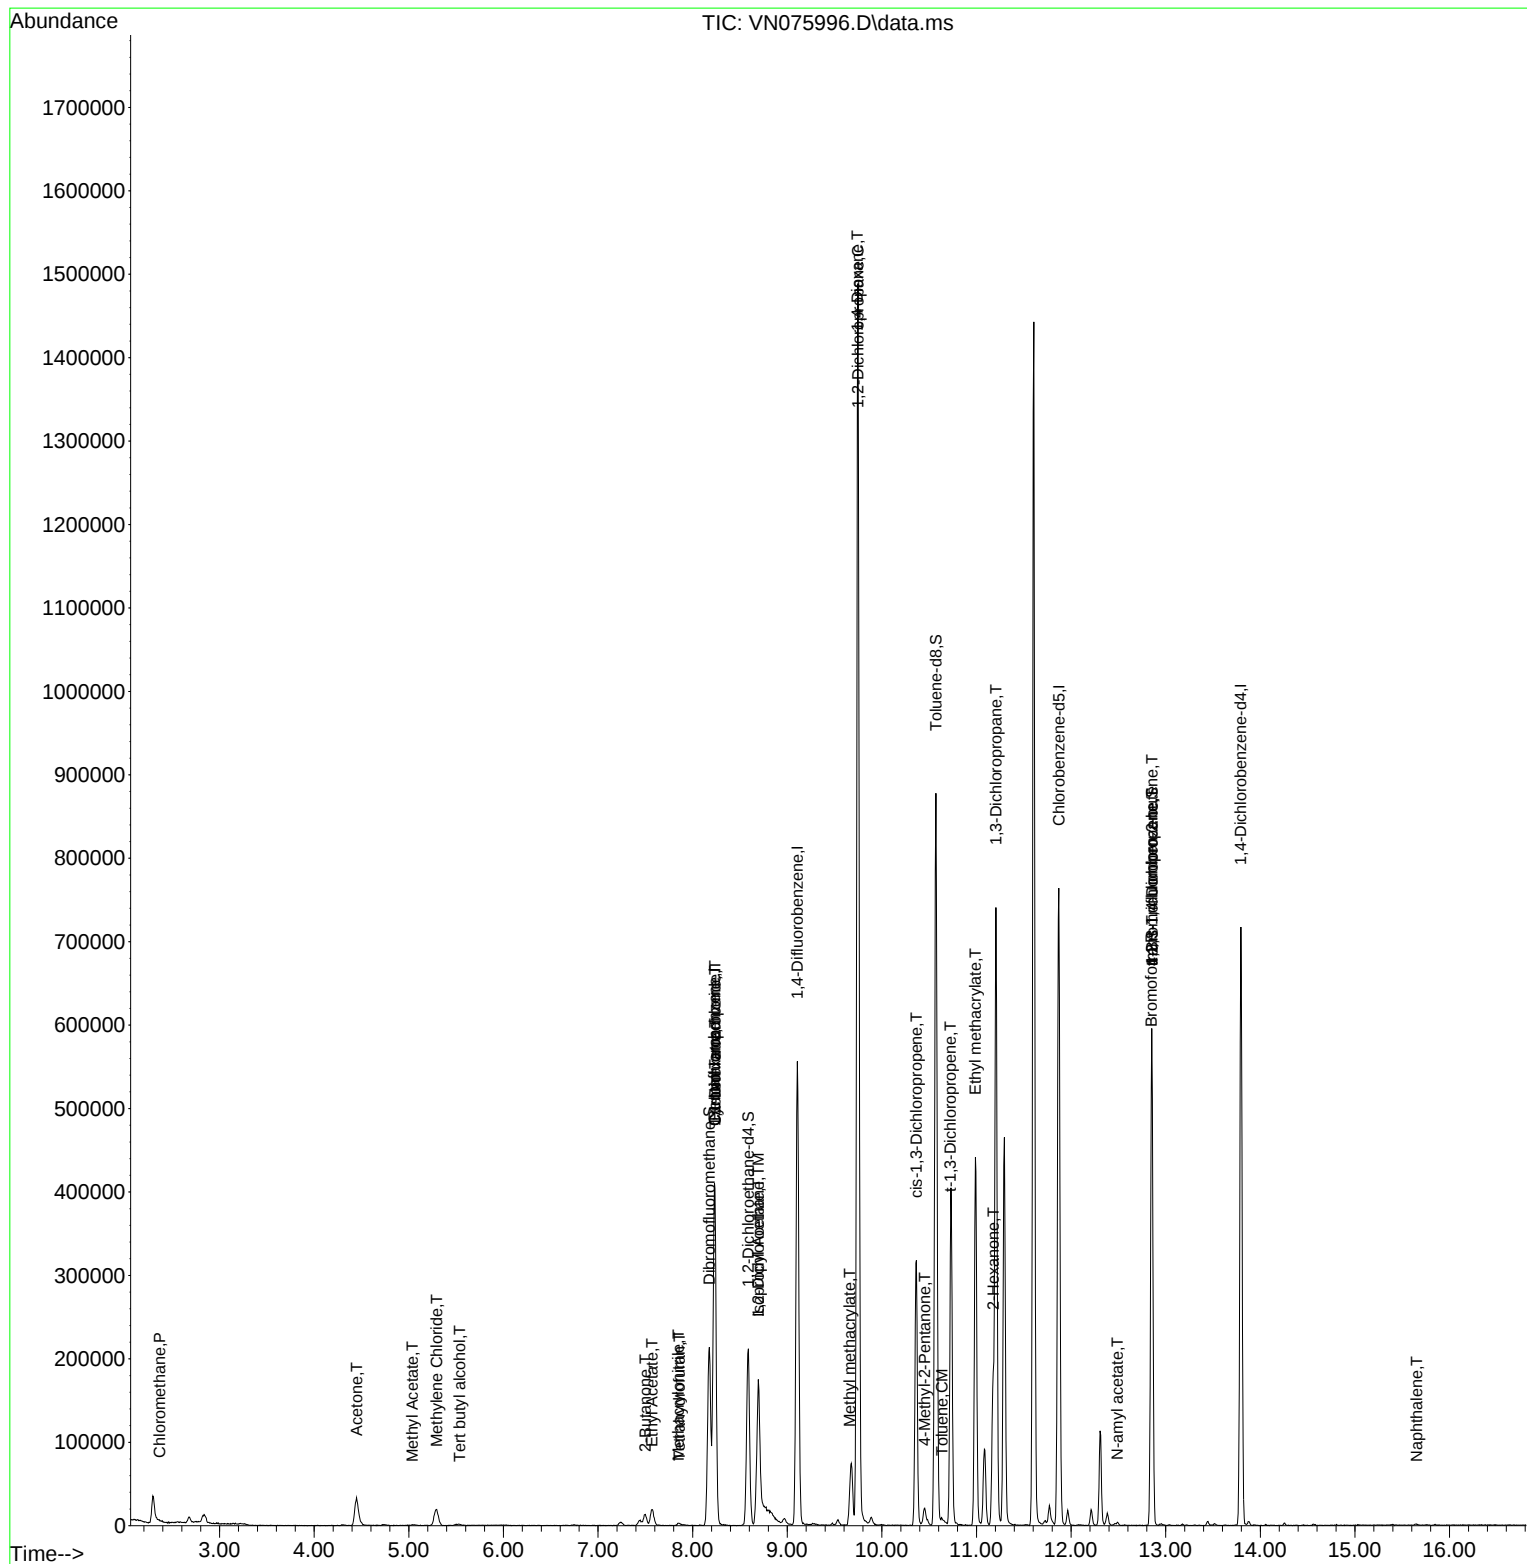




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.229 min Scan# 10
Delta R.T. -0.001 min
Lab File: VN075996.D
Acq: 28 Dec 2022 13:45




Instrument :
MSVOA_N
ClientSampleId :
PL-502A-COMP-3


Tgt Ion:168 Resp: 324721
Ion Ratio Lower Upper
168 100
99 56.1 44.2 66.4



#3
Chloromethane
Concen: 0.256 ug/l
RT: 2.365 min Scan# 53
Delta R.T. -0.006 min
Lab File: VN075996.D
Acq: 28 Dec 2022 13:45

Tgt Ion: 50 Resp: 734
Ion Ratio Lower Upper
50 100
52 0.0 27.7 41.5#




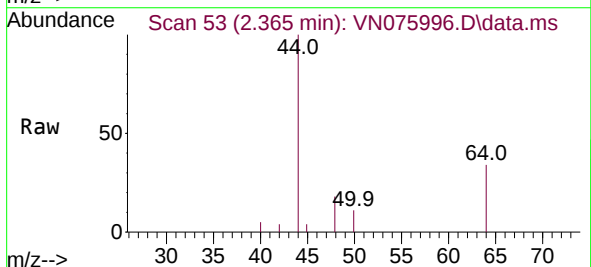




#11
Tert butyl alcohol
Concen: 4.657 ug/l
RT: 5.536 min Scan# 592
Delta R.T. -0.000 min
Lab File: VN075996.D
Acq: 28 Dec 2022 13:45




Instrument :
MSVOA_N
ClientSampleId :
PL-502A-COMP-3


Tgt Ion: 59 Resp: 2328
Ion Ratio Lower Upper
59 100
57 0.0 8.2 12.4#



#16
Acetone
Concen: 49.708 ug/l
RT: 4.447 min Scan# 407
Delta R.T. 0.006 min
Lab File: VN075996.D
Acq: 28 Dec 2022 13:45

Tgt Ion: 43 Resp: 60533
Ion Ratio Lower Upper
43 100
58 36.8 28.6 43.0


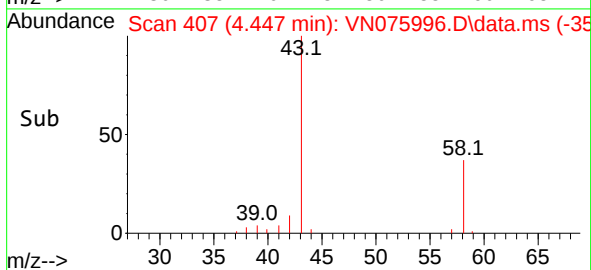






#18
Methyl Acetate
Concen: 0.705 ug/l
RT: 5.036 min Scan# 507
Delta R.T. -0.000 min
Lab File: VN075996.D
Acq: 28 Dec 2022 13:45




Instrument :
MSVOA_N
ClientSampleId :
PL-502A-COMP-3


Tgt Ion: 43 Resp: 2539
Ion Ratio Lower Upper
43 100
74 4.9 23.6 35.4#

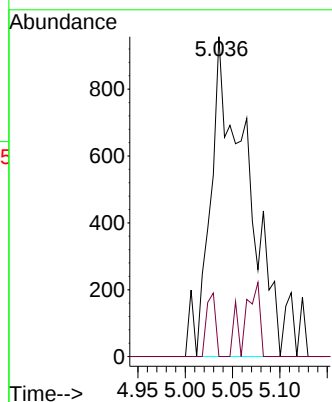

#20
Methylene Chloride
Concen: 4.366 ug/l
RT: 5.294 min Scan# 551
Delta R.T. 0.005 min
Lab File: VN075996.D
Acq: 28 Dec 2022 13:45

Tgt Ion: 84 Resp: 16128
Ion Ratio Lower Upper
84 100
49 89.8 81.8 122.6
51 26.3 26.7 40.1#
86 59.9 51.5 77.3

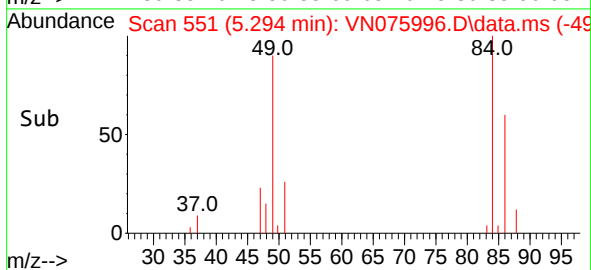



#25

2-Butanone

Concen: 11.538 ug/l

RT: 7.500 min Scan# 91

Delta R.T. 0.012 min

Lab File: VN075996.D

Acq: 28 Dec 2022 13:45

Instrument :

MSVOA_N

ClientSampleId :





PL-502A-COMP-3

Tgt Ion: 43 Resp: 19673

Ion Ratio Lower Upper

43 100

72 26.8 28.0 42.0#

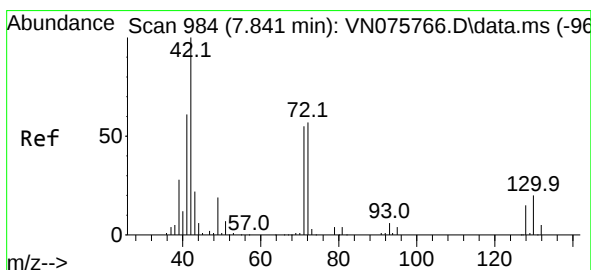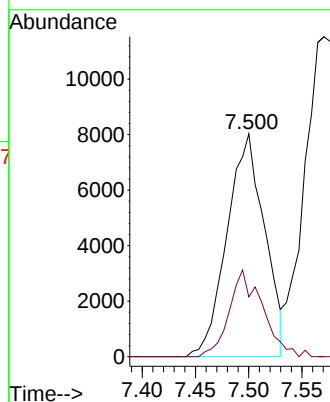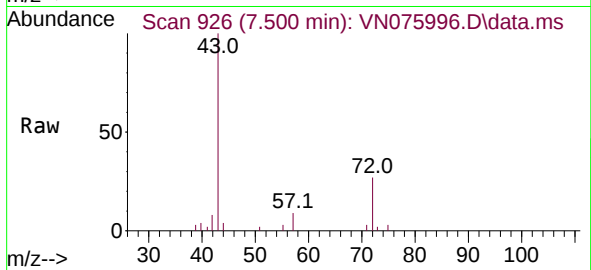

#29

Tetrahydrofuran

Concen: 1.989 ug/l

RT: 7.859 min Scan# 987

Delta R.T. 0.017 min

Lab File: VN075996.D

Acq: 28 Dec 2022 13:45




Tgt Ion: 42 Resp: 2125


Ion Ratio Lower Upper

42 100

72 44.8 44.5 66.7


71 46.6 41.0 61.6

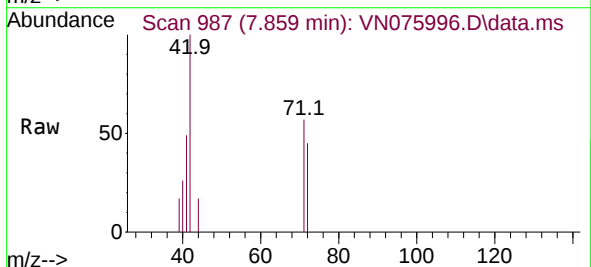



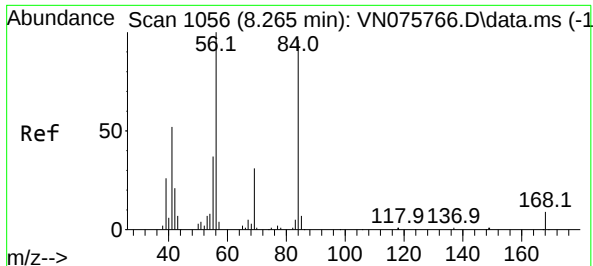


#31
Cyclohexane
Concen: 1.242 ug/l
RT: 8.235 min Scan# 1051
Delta R.T. -0.030 min
Lab File: VN075996.D
Acq: 28 Dec 2022 13:45

Instrument :
MSVOA_N
ClientSampleId :
PL-502A-COMP-3







Tgt Ion: 56 Resp: 6285
Ion Ratio Lower Upper
56 100
69 158.3 24.7 37.1#
84 160.8 76.5 114.7#

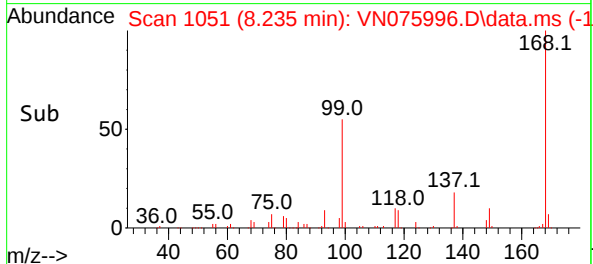

#33
1,2-Dichloroethane-d4
Concen: 48.627 ug/l
RT: 8.588 min Scan# 1111
Delta R.T. 0.006 min
Lab File: VN075996.D
Acq: 28 Dec 2022 13:45

Tgt Ion: 65 Resp: 171784
Ion Ratio Lower Upper
65 100
67 51.9 0.0 103.4

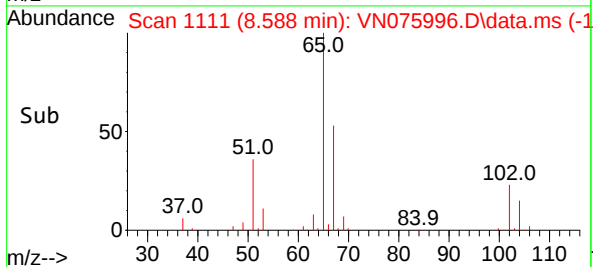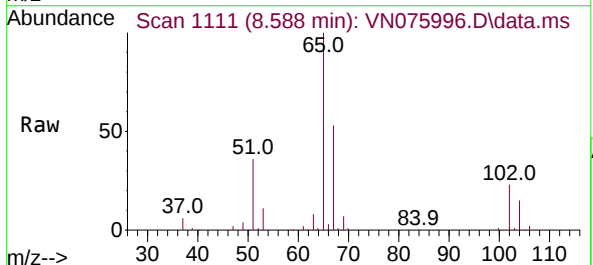

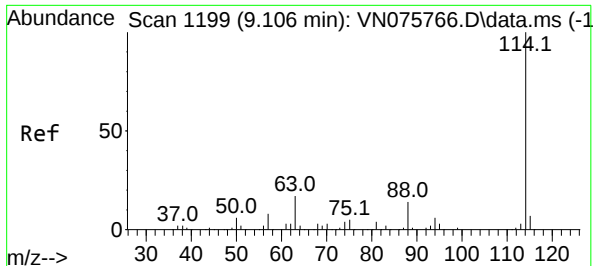

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 9.106 min Scan# 1199

Delta R.T. -0.000 min

Lab File: VN075996.D

Acq: 28 Dec 2022 13:45

Instrument :

MSVOA_N

ClientSampleId :

PL-502A-COMP-3





Tgt Ion:114 Resp: 516732

Ion Ratio Lower Upper

114 100

63 17.2 0.0 34.4

88 14.4 0.0 28.8

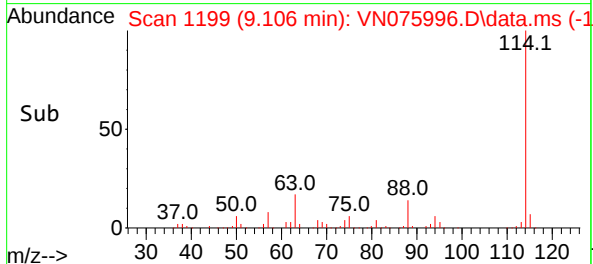

#35

Dibromofluoromethane

Concen: 48.293 ug/l

RT: 8.177 min Scan# 1041

Delta R.T. 0.006 min

Lab File: VN075996.D

Acq: 28 Dec 2022 13:45




Tgt Ion:113 Resp: 154540


Ion Ratio Lower Upper

113 100

111 102.6 83.4 125.2

192 19.8 16.1 24.1


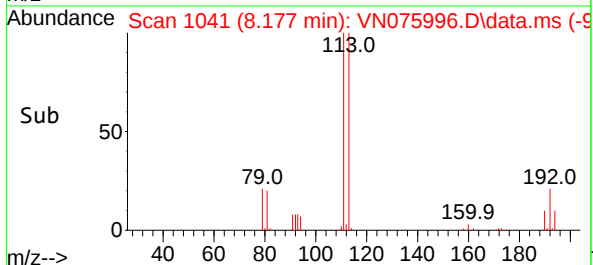
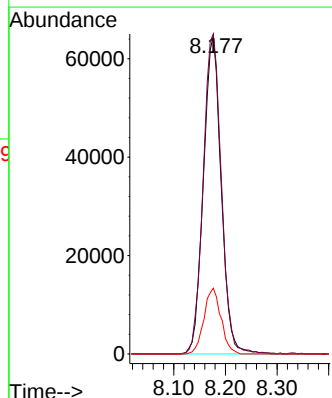
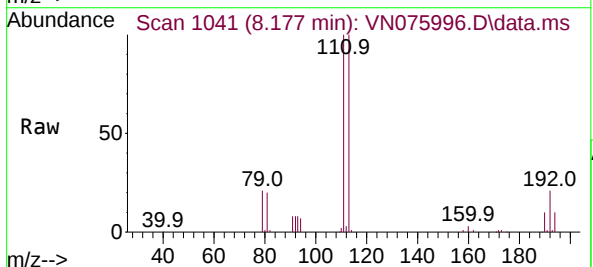


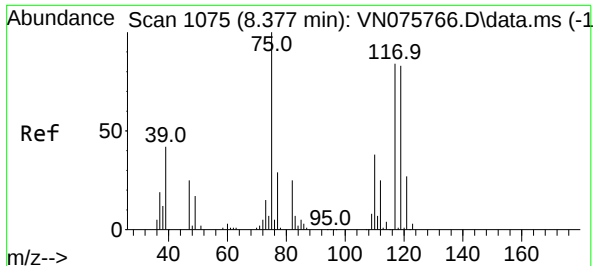

#36
1,1-Dichloropropene
Concen: 5.396 ug/l
RT: 8.235 min Scan# 1075
Delta R.T. -0.141 min
Lab File: VN075996.D
Acq: 28 Dec 2022 13:45




Instrument :
MSVOA_N
ClientSampleId :
PL-502A-COMP-3


Tgt Ion: 75 Resp: 22936
Ion Ratio Lower Upper
75 100
110 8.3 18.8 56.4#
77 0.0 24.1 36.1#

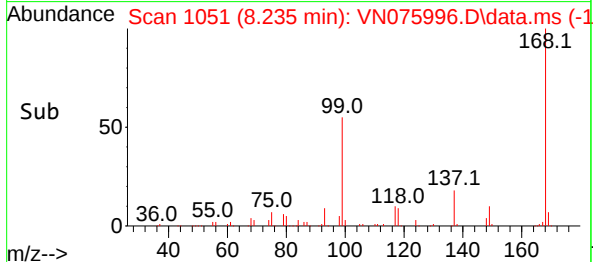

#37
Ethyl Acetate
Concen: 9.250 ug/l
RT: 7.571 min Scan# 938
Delta R.T. 0.006 min
Lab File: VN075996.D
Acq: 28 Dec 2022 13:45


Tgt Ion: 43 Resp: 31584
Ion Ratio Lower Upper
43 100
61 15.1 13.0 19.4
70 11.6 9.4 14.0

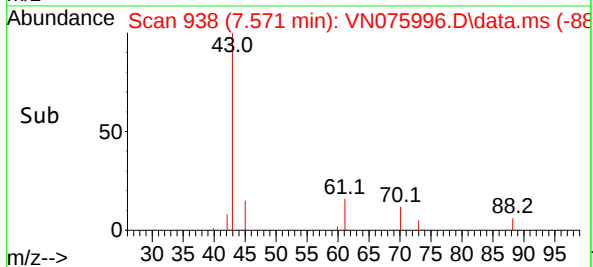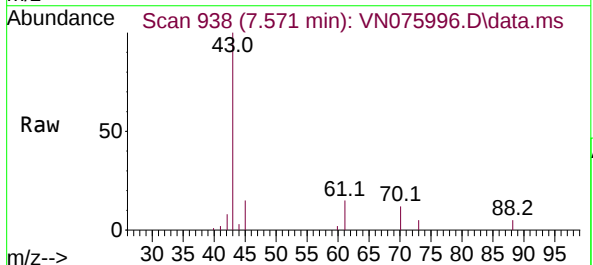



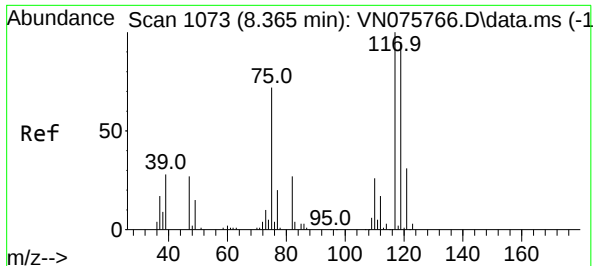


#38
Carbon Tetrachloride
Concen: 6.724 ug/l
RT: 8.235 min Scan# 1051
Delta R.T. -0.130 min
Lab File: VN075996.D
Acq: 28 Dec 2022 13:45

Instrument :
MSVOA_N
ClientSampleId :
PL-502A-COMP-3







Tgt Ion:117 Resp: 31992
Ion Ratio Lower Upper
117 100
119 4.7 76.1 114.1#
121 0.0 24.5 36.7#

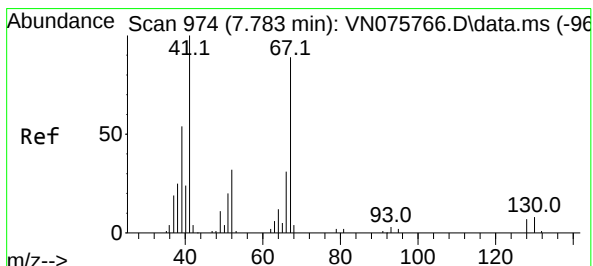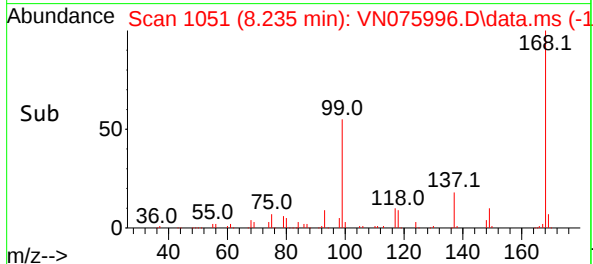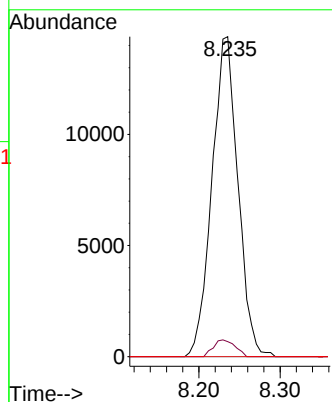

#41
Methacrylonitrile
Concen: 0.469 ug/l
RT: 7.847 min Scan# 985
Delta R.T. 0.065 min
Lab File: VN075996.D
Acq: 28 Dec 2022 13:45

Tgt Ion: 41 Resp: 832
Ion Ratio Lower Upper
41 100
39 22.8 43.1 64.7#
67 0.0 70.7 106.1#
52 0.0 26.7 40.1#

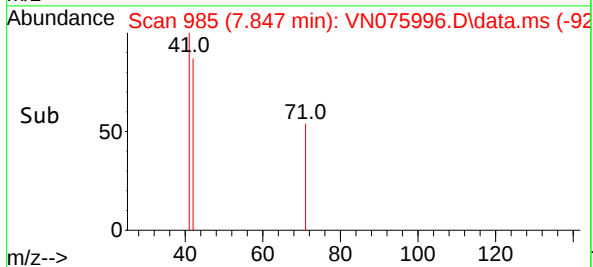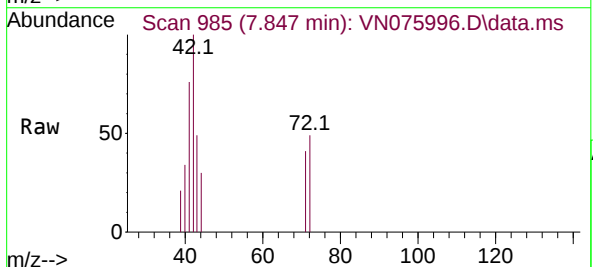

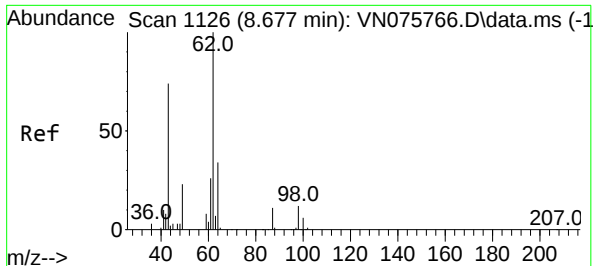

#42

1,2-Dichloroethane

Concen: 0.285 ug/l

RT: 8.694 min Scan# 1129

Delta R.T. 0.018 min

Lab File: VN075996.D

Acq: 28 Dec 2022 13:45

Instrument :

MSVOA_N

ClientSampleId :





PL-502A-COMP-3

Tgt Ion: 62 Resp: 1241

Ion Ratio Lower Upper

62 100

98 0.0 0.0 20.8

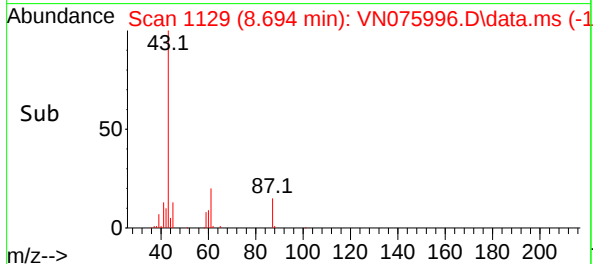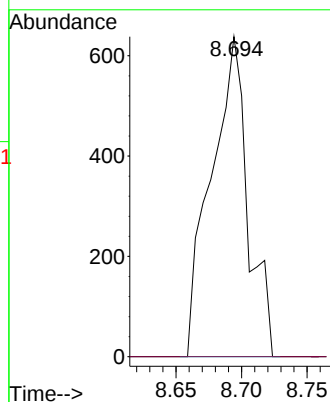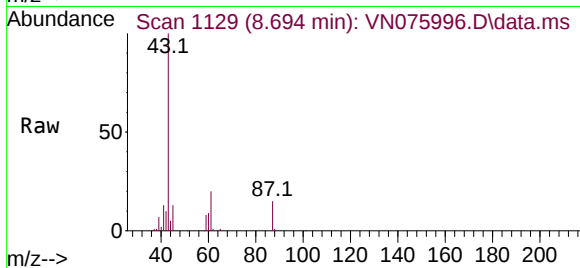

#43

Isopropyl Acetate

Concen: 37.405 ug/l

RT: 8.694 min Scan# 1129

Delta R.T. -0.000 min

Lab File: VN075996.D

Acq: 28 Dec 2022 13:45




Tgt Ion: 43 Resp: 210687


Ion Ratio Lower Upper

43 100

61 16.2 24.2 36.4#

87 11.8 13.3 19.9#

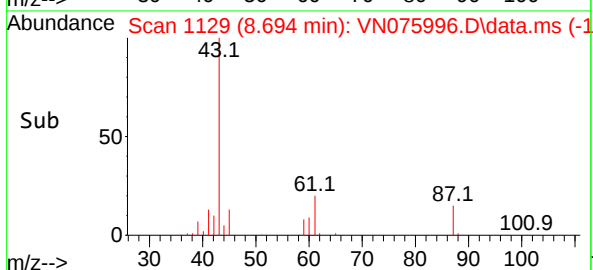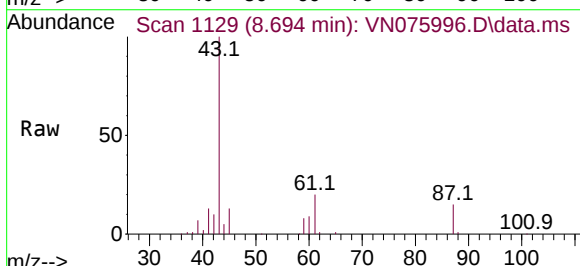

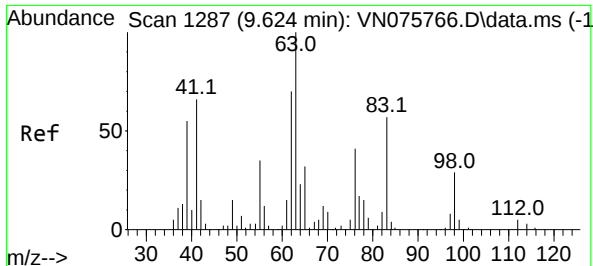

#45

1,2-Dichloropropane

Concen: 0.657 ug/l

RT: 9.747 min Scan# 11

Delta R.T. 0.123 min

Lab File: VN075996.D

Acq: 28 Dec 2022 13:45

Instrument :

MSVOA_N

ClientSampleId :





PL-502A-COMP-3

Tgt Ion: 63 Resp: 2097

Ion Ratio Lower Upper

63 100

65 0.0 25.7 38.5#

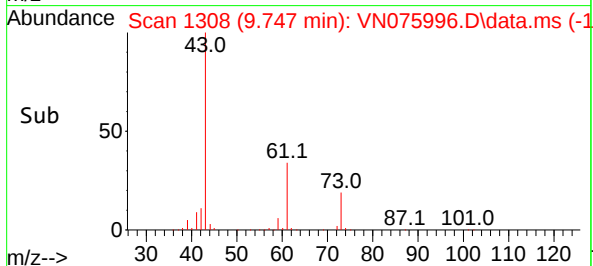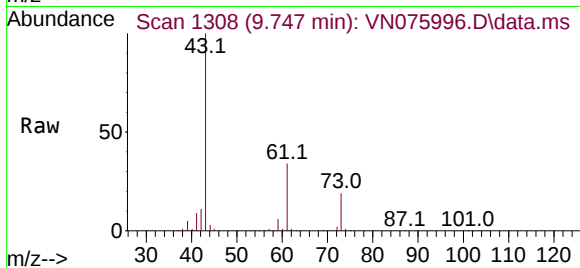

#48

Methyl methacrylate

Concen: 1.769 ug/l

RT: 9.659 min Scan# 1293

Delta R.T. -0.024 min

Lab File: VN075996.D

Acq: 28 Dec 2022 13:45




Tgt Ion: 41 Resp: 4487


Ion Ratio Lower Upper

41 100

69 0.0 81.9 122.9#

39 0.0 51.6 77.4#

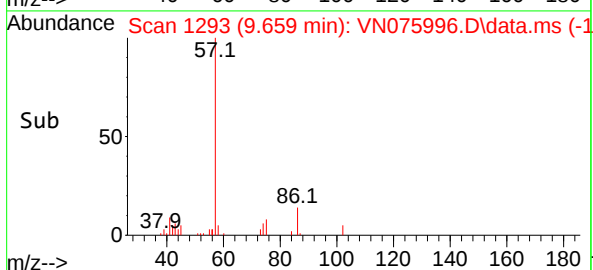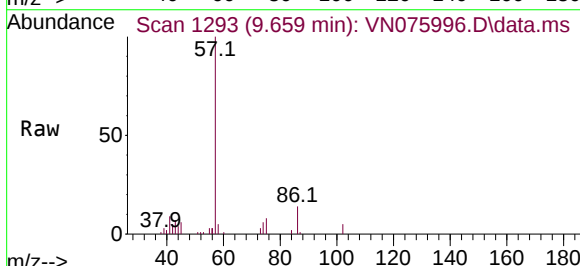

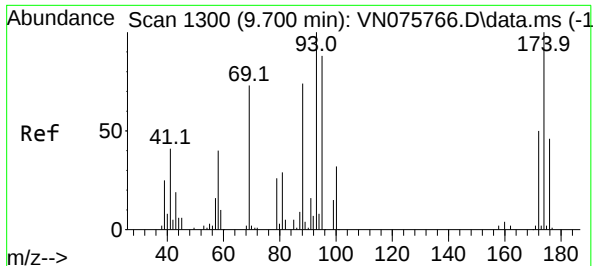

#49

1,4-Dioxane

Concen: 1.892 ug/l

RT: 9.741 min Scan# 1307

Delta R.T. 0.041 min

Lab File: VN075996.D

Acq: 28 Dec 2022 13:45

Instrument :

MSVOA_N

ClientSampleId :

PL-502A-COMP-3





Tgt Ion: 88 Resp: 118

Ion Ratio Lower Upper

88 100

43 1132685.6 17.1 25.7#

58 5350.0 47.8 71.8#

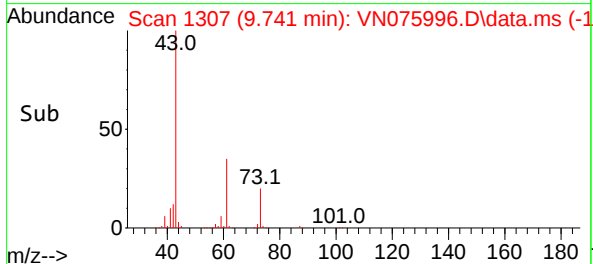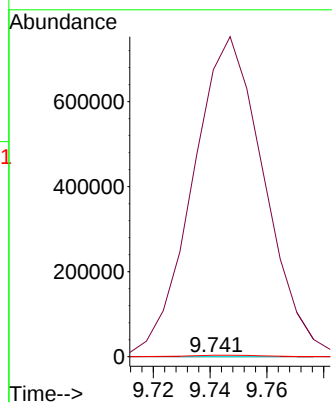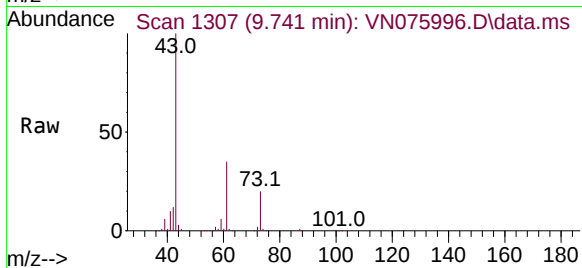

#50

Toluene-d8

Concen: 51.574 ug/l

RT: 10.570 min Scan# 1448

Delta R.T. -0.000 min

Lab File: VN075996.D




Acq: 28 Dec 2022 13:45


Tgt Ion: 98 Resp: 617065

Ion Ratio Lower Upper

98 100

100 64.6 52.1 78.1


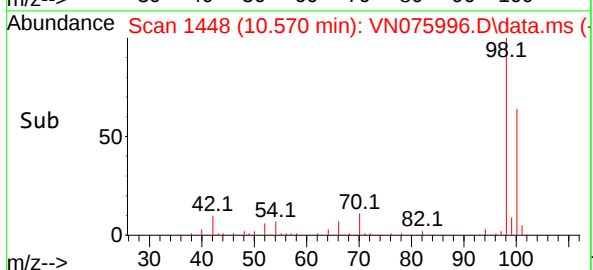

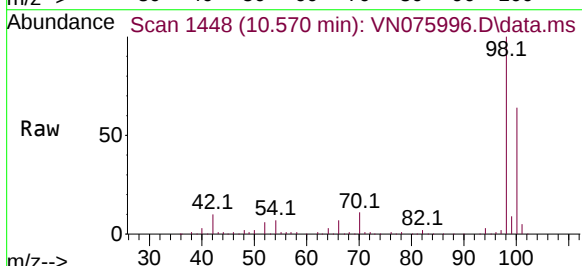




#51
4-Methyl-2-Pentanone
Concen: 5.212 ug/l
RT: 10.453 min Scan# 1428
Delta R.T. 0.006 min
Lab File: VN075996.D
Acq: 28 Dec 2022 13:45




Instrument :
MSVOA_N
ClientSampleId :
PL-502A-COMP-3


Tgt Ion: 43 Resp: 17755
Ion Ratio Lower Upper
43 100
58 32.2 35.5 53.3#



#52
Toluene
Concen: 0.360 ug/l
RT: 10.635 min Scan# 1459
Delta R.T. -0.000 min
Lab File: VN075996.D
Acq: 28 Dec 2022 13:45

Tgt Ion: 92 Resp: 3074
Ion Ratio Lower Upper
92 100
91 170.2 137.3 205.9


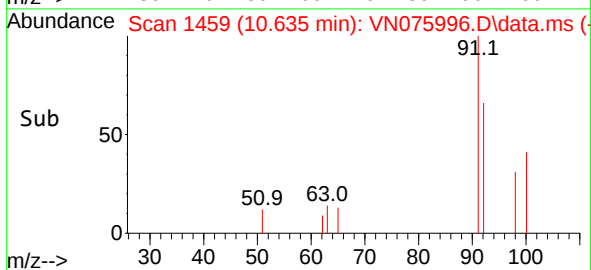

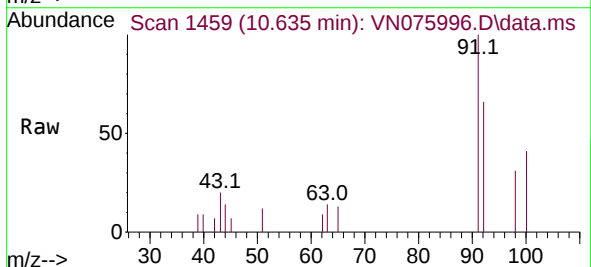




#53
 t-1,3-Dichloropropene
 Concen: 0.244 ug/l
 RT: 10.723 min Scan# 1412
 Delta R.T. -0.112 min
 Lab File: VN075996.D
 Acq: 28 Dec 2022 13:45




Instrument :
 MSVOA_N
 ClientSampleId :
 PL-502A-COMP-3


Tgt Ion: 75 Resp: 1110
 Ion Ratio Lower Upper
 75 100
 77 28.2 24.9 37.3



#54
 cis-1,3-Dichloropropene
 Concen: 12.909 ug/l
 RT: 10.365 min Scan# 1413
 Delta R.T. 0.053 min
 Lab File: VN075996.D
 Acq: 28 Dec 2022 13:45

Tgt Ion: 75 Resp: 64406
 Ion Ratio Lower Upper
 75 100
 77 0.8 25.8 38.8#
 39 29.1 33.4 50.2#


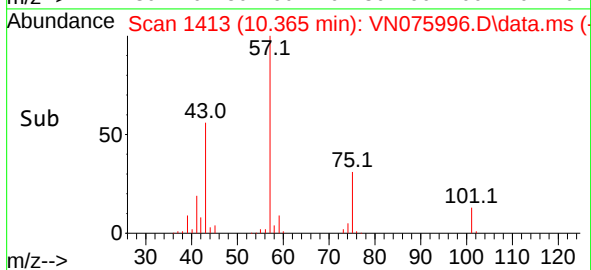

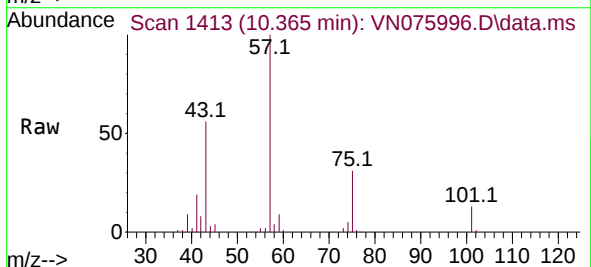




#56
Ethyl methacrylate
Concen: 0.355 ug/l
RT: 10.988 min Scan# 1519
Delta R.T. 0.112 min
Lab File: VN075996.D
Acq: 28 Dec 2022 13:45




Instrument :
MSVOA_N
ClientSampleId :
PL-502A-COMP-3


Tgt Ion: 69 Resp: 1582
Ion Ratio Lower Upper
69 100
41 5159.6 44.2 66.4#
39 2332.6 26.4 39.6#



#57
1,3-Dichloropropane
Concen: 1.540 ug/l
RT: 11.206 min Scan# 1556
Delta R.T. 0.041 min
Lab File: VN075996.D
Acq: 28 Dec 2022 13:45

Tgt Ion: 76 Resp: 8469
Ion Ratio Lower Upper
76 100
78 0.0 26.2 39.2#


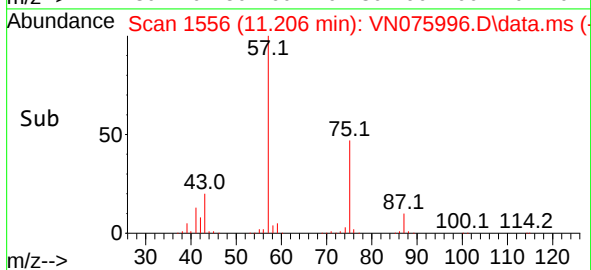

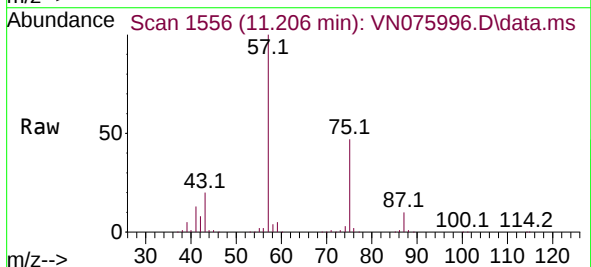




#59
2-Hexanone
Concen: 56.716 ug/l
RT: 11.176 min Scan# 11
Delta R.T. -0.024 min
Lab File: VN075996.D
Acq: 28 Dec 2022 13:45




Instrument :
MSVOA_N
ClientSampleId :
PL-502A-COMP-3


Tgt Ion: 43 Resp: 140891
Ion Ratio Lower Upper
43 100
58 0.0 30.6 92.0#

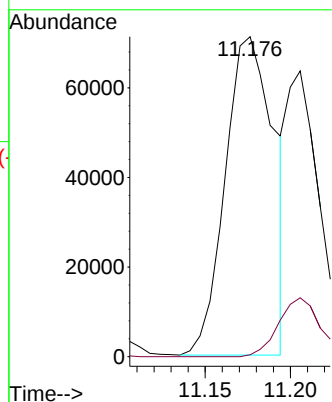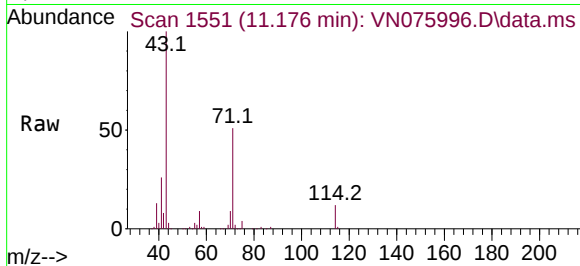

#62
4-Bromofluorobenzene
Concen: 49.252 ug/l
RT: 12.853 min Scan# 1836
Delta R.T. -0.000 min
Lab File: VN075996.D
Acq: 28 Dec 2022 13:45

Tgt Ion: 95 Resp: 195177
Ion Ratio Lower Upper
95 100
174 87.3 0.0 171.6
176 84.2 0.0 169.2


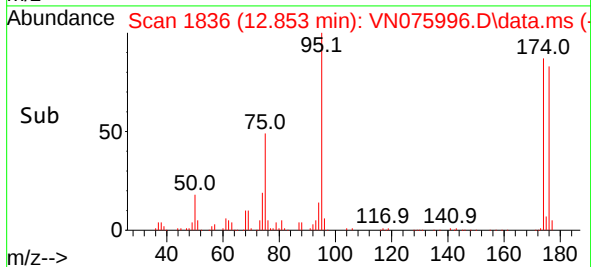
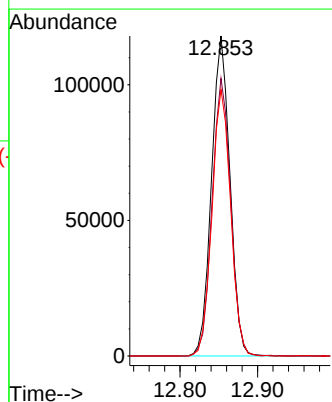
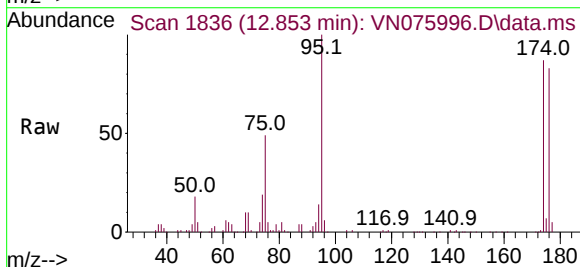




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.870 min Scan# 117
Delta R.T. 0.006 min
Lab File: VN075996.D
Acq: 28 Dec 2022 13:45




Instrument :
MSVOA_N
ClientSampleId :
PL-502A-COMP-3


Tgt Ion:117 Resp: 468416
Ion Ratio Lower Upper
117 100
82 52.5 41.3 61.9
119 32.0 24.6 37.0

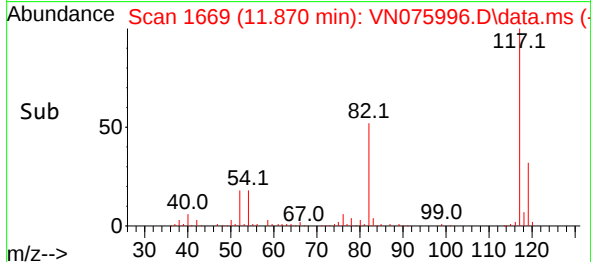

#71
Bromoform
Concen: 0.400 ug/l
RT: 12.847 min Scan# 1835
Delta R.T. 0.265 min
Lab File: VN075996.D
Acq: 28 Dec 2022 13:45

Tgt Ion:173 Resp: 1037
Ion Ratio Lower Upper
173 100
175 1039.3 24.3 72.8#
254 0.0 0.0 0.0


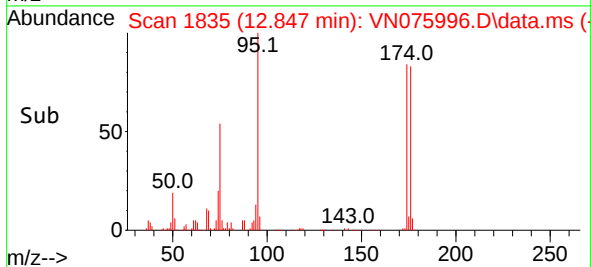

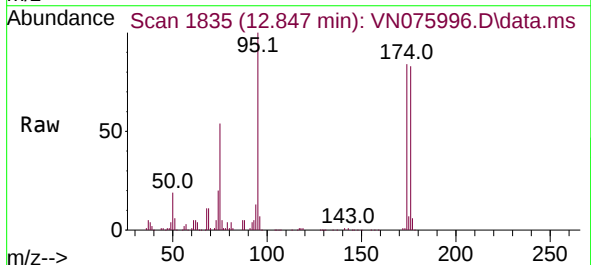


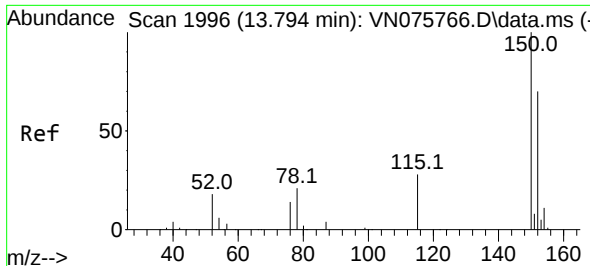

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.794 min Scan# 1996
Delta R.T. -0.000 min
Lab File: VN075996.D
Acq: 28 Dec 2022 13:45




Instrument :
MSVOA_N
ClientSampleId :
PL-502A-COMP-3


Tgt Ion:152 Resp: 202829
Ion Ratio Lower Upper
152 100
115 56.3 29.1 87.4
150 157.1 0.0 347.0

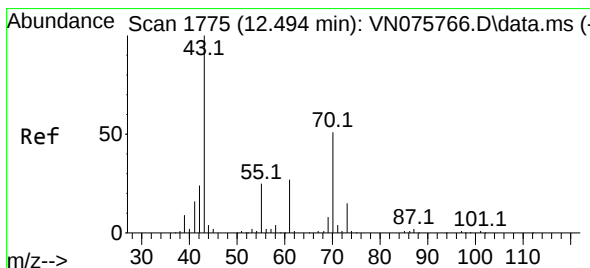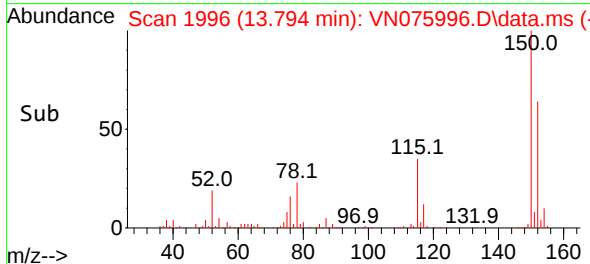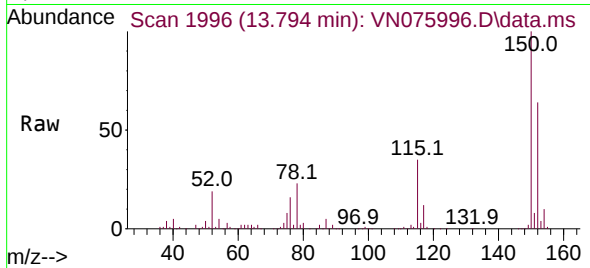

#74
N-ethyl acetate
Concen: 0.304 ug/l
RT: 12.488 min Scan# 1774
Delta R.T. -0.006 min
Lab File: VN075996.D
Acq: 28 Dec 2022 13:45

Tgt Ion: 43 Resp: 1307
Ion Ratio Lower Upper
43 100
70 5.0 41.4 62.0#
55 5.6 21.3 31.9#
61 0.0 21.2 31.8#


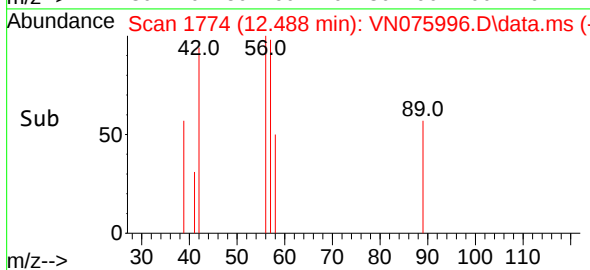

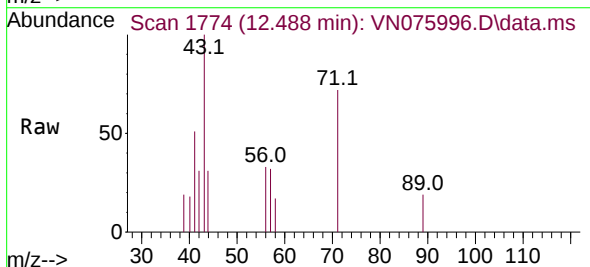




#76
1,2,3-Trichloropropane
Concen: 24.723 ug/l
RT: 12.853 min Scan# 1836
Delta R.T. -0.141 min
Lab File: VN075996.D
Acq: 28 Dec 2022 13:45




Instrument :
MSVOA_N
ClientSampleId :
PL-502A-COMP-3


Tgt Ion: 75 Resp: 101080
Ion Ratio Lower Upper
75 100
77 1.2 82.6 247.8#



#81
trans-1,4-Dichloro-2-butene
Concen: 88.990 ug/l
RT: 12.853 min Scan# 1836
Delta R.T. 0.112 min
Lab File: VN075996.D
Acq: 28 Dec 2022 13:45


Tgt Ion: 75 Resp: 101080
Ion Ratio Lower Upper
75 100
53 0.0 73.8 110.6#
89 0.0 39.5 59.3#

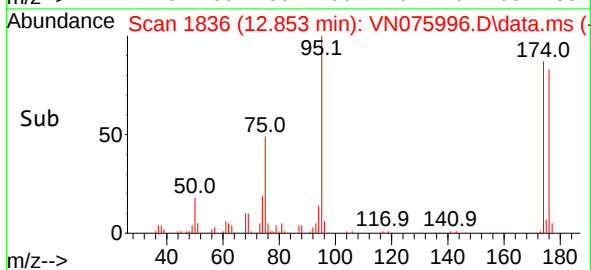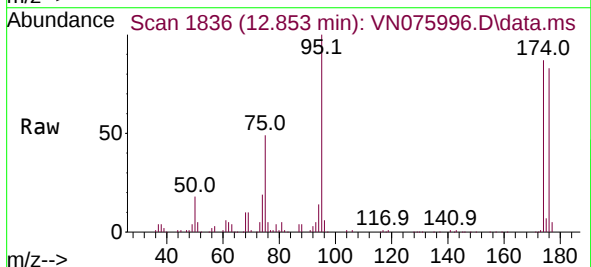

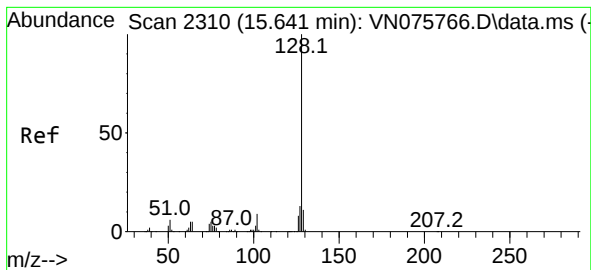

#95
Naphthalene
Concen: 2.367 ug/l
RT: 15.653 min Scan# 21
Delta R.T. 0.011 min
Lab File: VN075996.D
Acq: 28 Dec 2022 13:45

Instrument :
MSVOA_N
ClientSampleId :
PL-502A-COMP-3

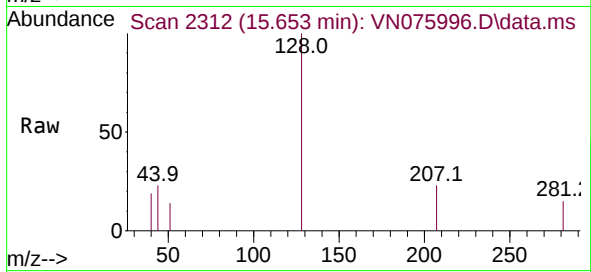

Tgt Ion:128 Resp: 2185
Ion Ratio Lower Upper
128 100
127 2.6 10.4 15.6#
129 2.5 8.7 13.1#

