

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN122822\
 Data File : VN076031.D
 Acq On : 29 Dec 2022 04:31
 Operator : JC\MD
 Sample : PB149923ZHE#12
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 PB149923ZHE#12

Quant Time: Dec 29 07:51:14 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N121422W.M
 Quant Title : SW846 8260
 QLast Update : Wed Dec 14 13:03:41 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	8.235	168	374970	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.106	114	595288	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.871	117	533325	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.794	152	224474	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.588	65	190569	46.716	ug/l	0.00
Spiked Amount 50.000	Range 74 - 125		Recovery =	93.440%		
35) Dibromofluoromethane	8.177	113	173748	47.130	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery =	94.260%		
50) Toluene-d8	10.571	98	702698	50.981	ug/l	0.00
Spiked Amount 50.000	Range 86 - 113		Recovery =	101.960%		
62) 4-Bromofluorobenzene	12.853	95	220379	48.273	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery =	96.540%		
Target Compounds						Qvalue
6) Chloroethane	3.095	64	765	0.262	ug/l #	44
11) Tert butyl alcohol	5.530	59	2607	4.516	ug/l #	72
16) Acetone	4.447	43	66669	47.410	ug/l	92
18) Methyl Acetate	5.042	43	1636	0.394	ug/l	94
20) Methylene Chloride	5.300	84	16915	3.906	ug/l	94
25) 2-Butanone	7.494	43	24380	12.382	ug/l	97
29) Tetrahydrofuran	7.853	42	2514	2.037	ug/l	90
31) Cyclohexane	8.230	56	6912	1.183	ug/l #	24
36) 1,1-Dichloropropene	8.230	75	26802	5.473	ug/l #	48
37) Ethyl Acetate	7.577	43	34551	8.783	ug/l	98
38) Carbon Tetrachloride	8.230	117	37495	6.841	ug/l #	16
41) Methacrylonitrile	7.853	41	1443	0.706	ug/l #	26
42) 1,2-Dichloroethane	8.688	62	1959	0.390	ug/l #	72
43) Isopropyl Acetate	8.694	43	454214	69.999	ug/l #	67
45) 1,2-Dichloropropane	9.741	63	2309	0.628	ug/l #	43
48) Methyl methacrylate	9.665	41	5467	1.871	ug/l #	35
49) 1,4-Dioxane	9.747	88	225	3.132	ug/l #	1
51) 4-Methyl-2-Pentanone	10.447	43	21389	5.451	ug/l #	81
52) Toluene	10.635	92	5951	0.605	ug/l	97
53) t-1,3-Dichloropropene	10.729	75	1294	0.247	ug/l #	76
54) cis-1,3-Dichloropropene	10.359	75	77759	13.528	ug/l #	61
56) Ethyl methacrylate	10.988	69	1851	0.361	ug/l #	1
57) 1,3-Dichloropropane	11.200	76	10179	1.607	ug/l #	42
59) 2-Hexanone	11.176	43	151373	52.895	ug/l #	20
71) Bromoform	12.853	173	1999	0.678	ug/l #	1
74) N-amyl acetate	12.488	43	1413	0.297	ug/l #	40
76) 1,2,3-Trichloropropane	12.853	75	112458	24.853	ug/l #	1
81) trans-1,4-Dichloro-2-b...	12.853	75	112458	89.460	ug/l #	12
95) Naphthalene	15.647	128	2054	2.338	ug/l #	79


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN122822\
Data File : VN076031.D
Acq On : 29 Dec 2022 04:31
Operator : JC\MD
Sample : PB149923ZHE#12
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
PB149923ZHE#12

Quant Time: Dec 29 07:51:14 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N121422W.M
Quant Title : SW846 8260
QLast Update : Wed Dec 14 13:03:41 2022
Response via : Initial Calibration




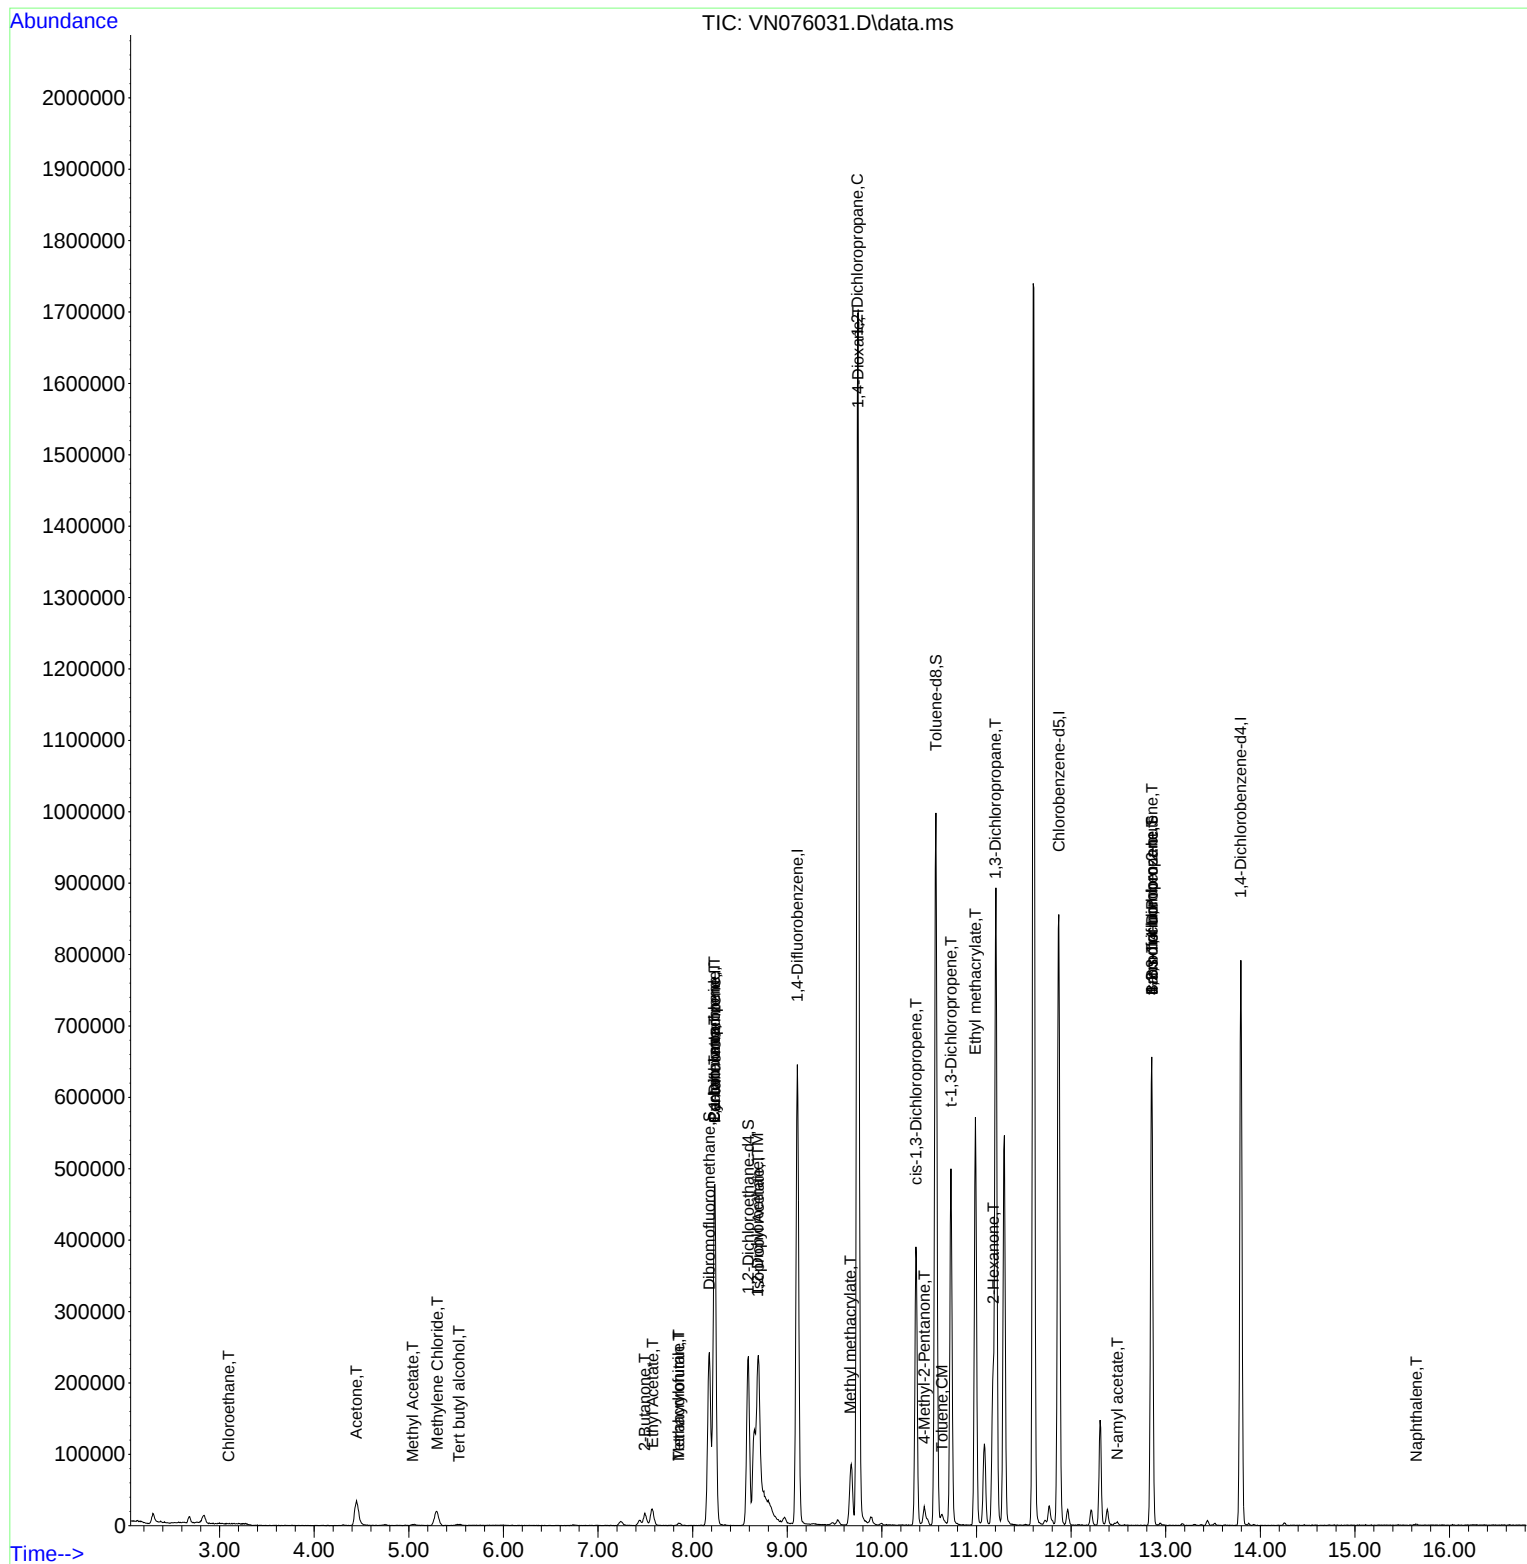


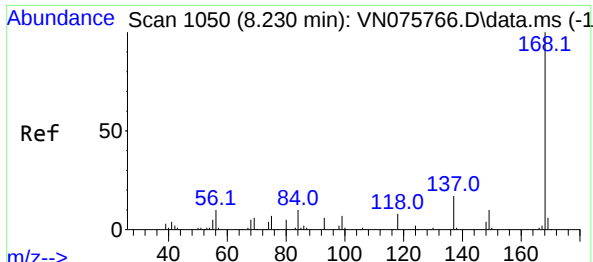

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.235 min Scan# 10
Delta R.T. 0.005 min
Lab File: VN076031.D
Acq: 29 Dec 2022 04:31




Instrument :
MSVOA_N
ClientSampleId :
PB149923ZHE#12


Tgt Ion:168 Resp: 374970
Ion Ratio Lower Upper
168 100
99 54.2 44.2 66.4

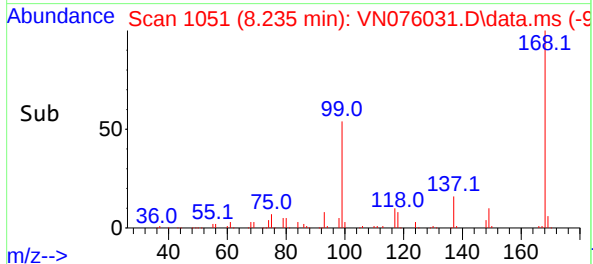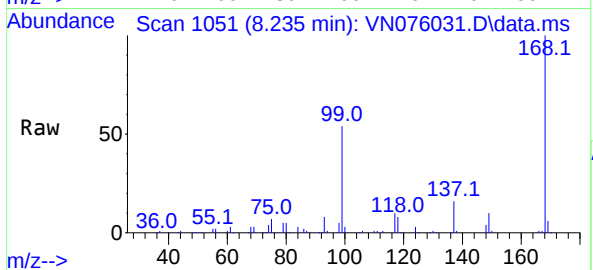

#6
Chloroethane
Concen: 0.262 ug/l
RT: 3.095 min Scan# 177
Delta R.T. -0.024 min
Lab File: VN076031.D
Acq: 29 Dec 2022 04:31

Tgt Ion: 64 Resp: 765
Ion Ratio Lower Upper
64 100
66 0.0 24.6 36.8#


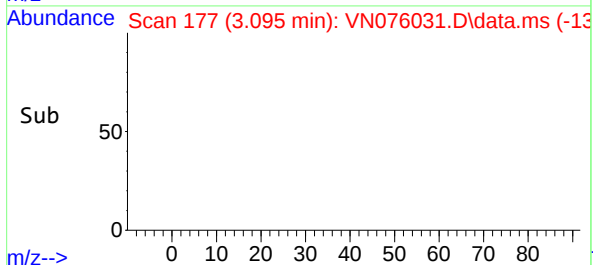

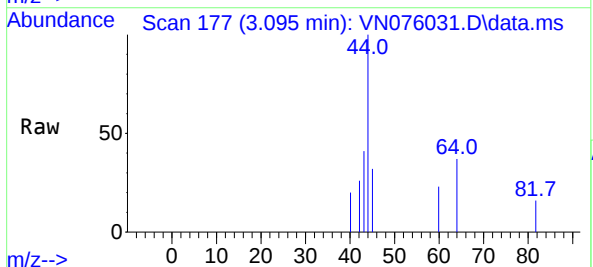




#11
Tert butyl alcohol
Concen: 4.516 ug/l
RT: 5.530 min Scan# 591
Delta R.T. -0.006 min
Lab File: VN076031.D
Acq: 29 Dec 2022 04:31




Instrument :
MSVOA_N
ClientSampleId :
PB149923ZHE#12


Tgt Ion: 59 Resp: 2607
Ion Ratio Lower Upper
59 100
57 0.0 8.2 12.4#



#16
Acetone
Concen: 47.410 ug/l
RT: 4.447 min Scan# 407
Delta R.T. 0.006 min
Lab File: VN076031.D
Acq: 29 Dec 2022 04:31

Tgt Ion: 43 Resp: 66669
Ion Ratio Lower Upper
43 100
58 40.8 28.6 43.0


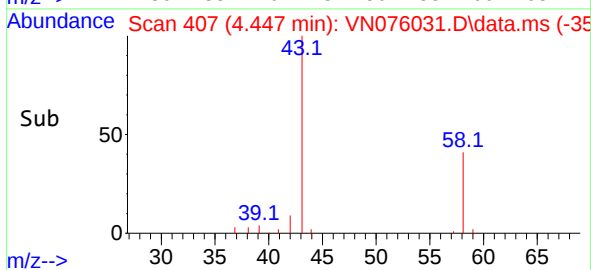






#18
Methyl Acetate
Concen: 0.394 ug/l
RT: 5.042 min Scan# 507
Delta R.T. 0.006 min
Lab File: VN076031.D
Acq: 29 Dec 2022 04:31




Instrument :
MSVOA_N
ClientSampleId :
PB149923ZHE#12


Tgt Ion: 43 Resp: 1636
Ion Ratio Lower Upper
43 100
74 26.2 23.6 35.4



#20
Methylene Chloride
Concen: 3.906 ug/l
RT: 5.300 min Scan# 552
Delta R.T. 0.011 min
Lab File: VN076031.D
Acq: 29 Dec 2022 04:31

Tgt Ion: 84 Resp: 16915
Ion Ratio Lower Upper
84 100
49 108.5 81.8 122.6
51 27.0 26.7 40.1
86 65.8 51.5 77.3

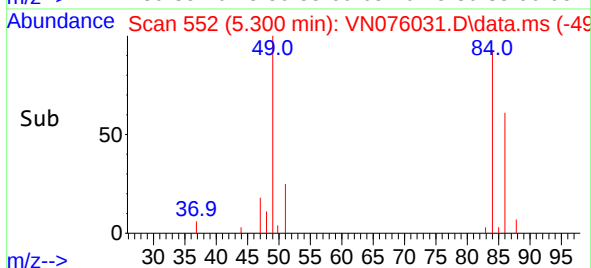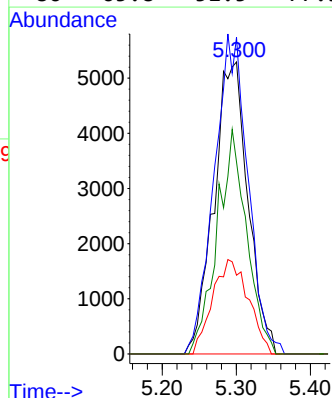



#25

2-Butanone

Concen: 12.382 ug/l

RT: 7.494 min Scan# 91

Delta R.T. 0.006 min

Lab File: VN076031.D

Acq: 29 Dec 2022 04:31

Instrument :

MSVOA_N

ClientSampleId :





PB149923ZHE#12

Tgt Ion: 43 Resp: 24380

Ion Ratio Lower Upper

43 100

72 36.7 28.0 42.0

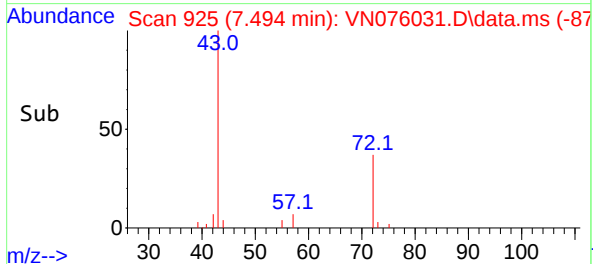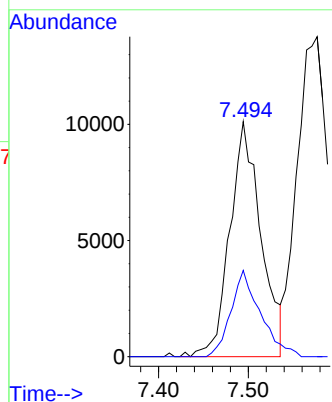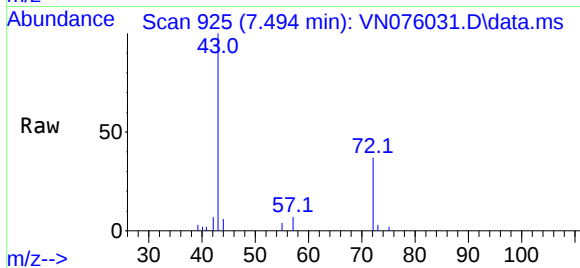

#29

Tetrahydrofuran

Concen: 2.037 ug/l

RT: 7.853 min Scan# 986

Delta R.T. 0.012 min

Lab File: VN076031.D

Acq: 29 Dec 2022 04:31




Tgt Ion: 42 Resp: 2514


Ion Ratio Lower Upper

42 100

72 48.6 44.5 66.7

71 43.4 41.0 61.6


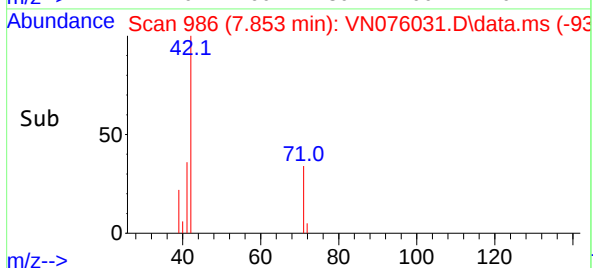

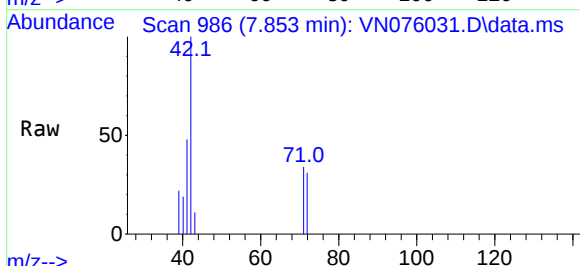




#31
Cyclohexane
Concen: 1.183 ug/l
RT: 8.230 min Scan# 1056
Delta R.T. -0.035 min
Lab File: VN076031.D
Acq: 29 Dec 2022 04:31




Instrument :
MSVOA_N
ClientSampleId :
PB149923ZHE#12


Tgt Ion: 56 Resp: 6912
Ion Ratio Lower Upper
56 100
69 139.8 24.7 37.1#
84 131.1 76.5 114.7#

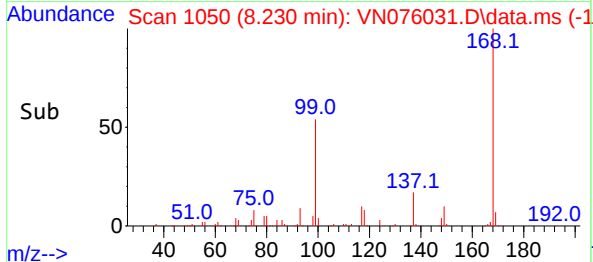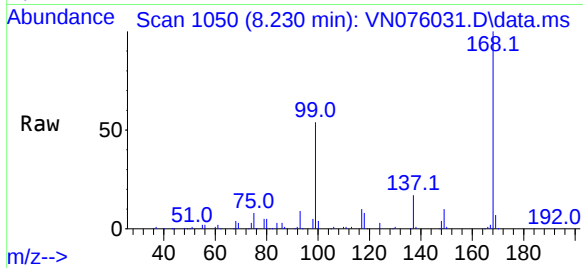

#33
1,2-Dichloroethane-d4
Concen: 46.716 ug/l
RT: 8.588 min Scan# 1111
Delta R.T. 0.006 min
Lab File: VN076031.D
Acq: 29 Dec 2022 04:31

Tgt Ion: 65 Resp: 190569
Ion Ratio Lower Upper
65 100
67 52.2 0.0 103.4


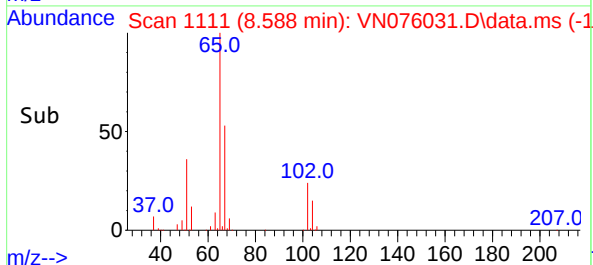
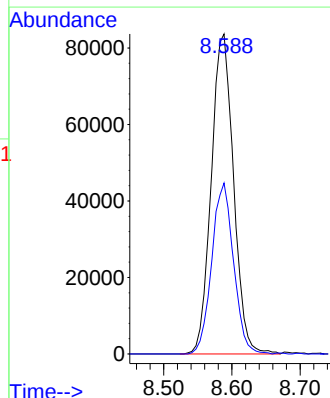
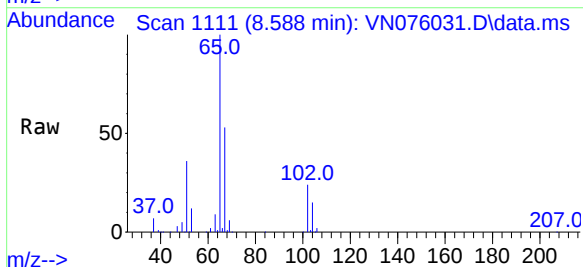


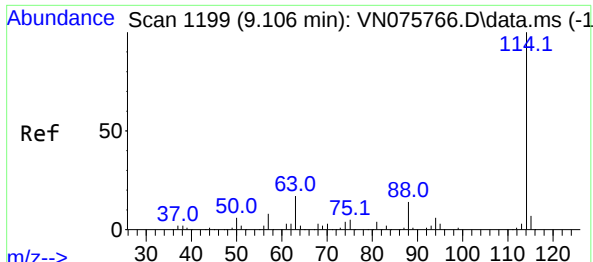

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 9.106 min Scan# 1199
Delta R.T. -0.000 min
Lab File: VN076031.D
Acq: 29 Dec 2022 04:31




Instrument :
MSVOA_N
ClientSampleId :
PB149923ZHE#12


Tgt Ion:114 Resp: 595288
Ion Ratio Lower Upper
114 100
63 17.4 0.0 34.4
88 14.1 0.0 28.8

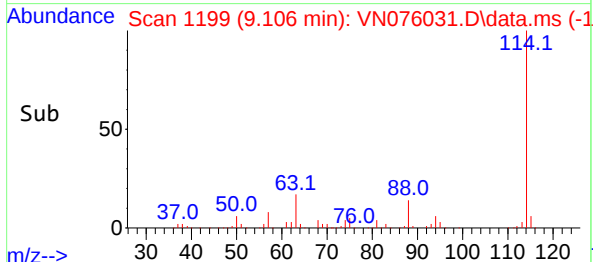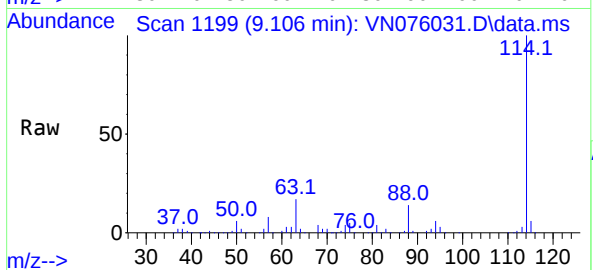

#35
Dibromofluoromethane
Concen: 47.130 ug/l
RT: 8.177 min Scan# 1041
Delta R.T. 0.006 min
Lab File: VN076031.D
Acq: 29 Dec 2022 04:31

Tgt Ion:113 Resp: 173748
Ion Ratio Lower Upper
113 100
111 103.1 83.4 125.2
192 20.1 16.1 24.1


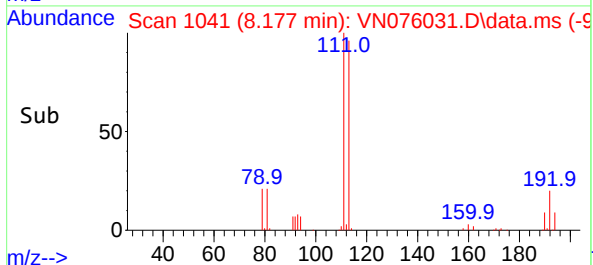

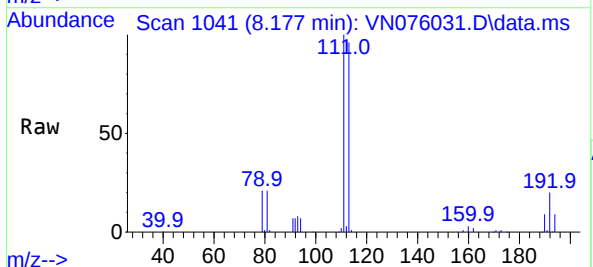




#36
1,1-Dichloropropene
Concen: 5.473 ug/l
RT: 8.230 min Scan# 1075
Delta R.T. -0.147 min
Lab File: VN076031.D
Acq: 29 Dec 2022 04:31




Instrument :
MSVOA_N
ClientSampleId :
PB149923ZHE#12


Tgt Ion: 75 Resp: 26802
Ion Ratio Lower Upper
75 100
110 8.0 18.8 56.4#
77 0.0 24.1 36.1#

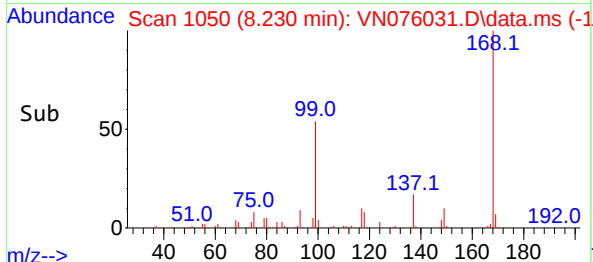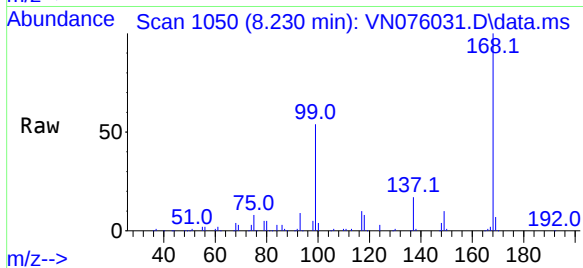

#37
Ethyl Acetate
Concen: 8.783 ug/l
RT: 7.577 min Scan# 939
Delta R.T. 0.012 min
Lab File: VN076031.D
Acq: 29 Dec 2022 04:31

Tgt Ion: 43 Resp: 34551
Ion Ratio Lower Upper
43 100
61 14.7 13.0 19.4
70 12.0 9.4 14.0


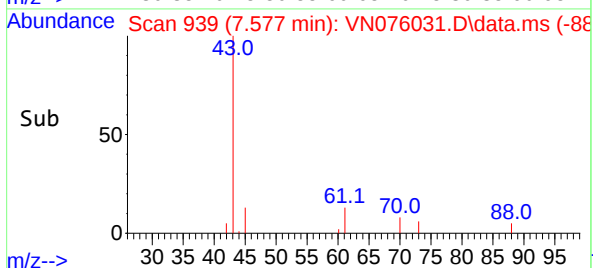

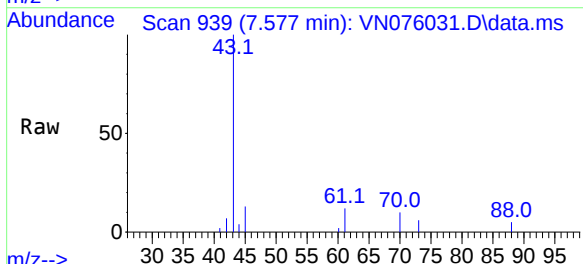




#38
Carbon Tetrachloride
Concen: 6.841 ug/l
RT: 8.230 min Scan# 1073
Delta R.T. -0.135 min
Lab File: VN076031.D
Acq: 29 Dec 2022 04:31




Instrument :
MSVOA_N
ClientSampleId :
PB149923ZHE#12


Tgt Ion:117 Resp: 37495
Ion Ratio Lower Upper
117 100
119 4.7 76.1 114.1#
121 0.0 24.5 36.7#

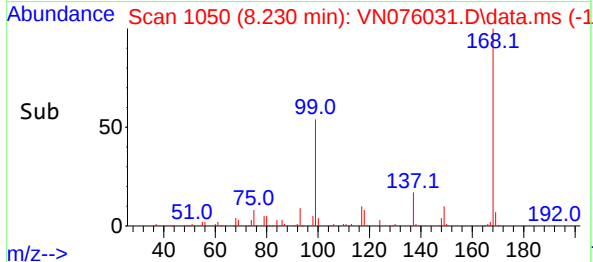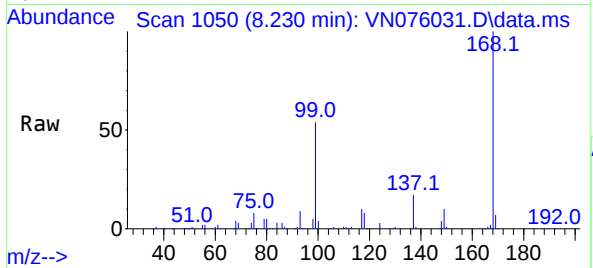

#41
Methacrylonitrile
Concen: 0.706 ug/l
RT: 7.853 min Scan# 986
Delta R.T. 0.071 min
Lab File: VN076031.D
Acq: 29 Dec 2022 04:31

Tgt Ion: 41 Resp: 1443
Ion Ratio Lower Upper
41 100
39 18.5 43.1 64.7#
67 0.0 70.7 106.1#
52 0.0 26.7 40.1#


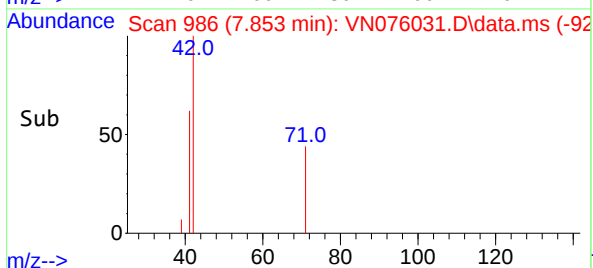
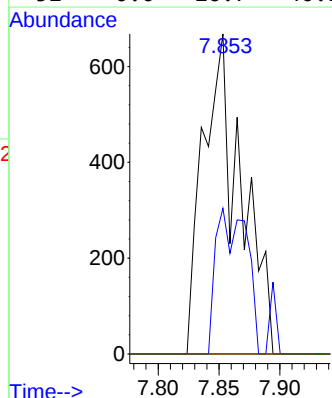
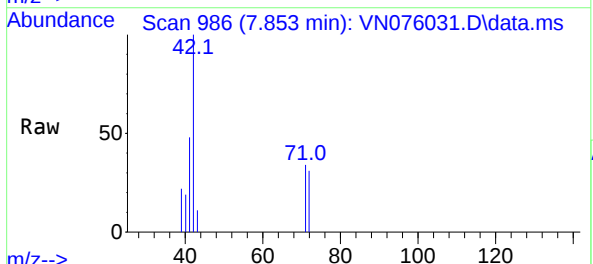




#42
1,2-Dichloroethane
Concen: 0.390 ug/l
RT: 8.688 min Scan# 1126
Delta R.T. 0.012 min
Lab File: VN076031.D
Acq: 29 Dec 2022 04:31




Instrument :
MSVOA_N
ClientSampleId :
PB149923ZHE#12


Tgt Ion: 62 Resp: 1959
Ion Ratio Lower Upper
62 100
98 0.0 0.0 20.8

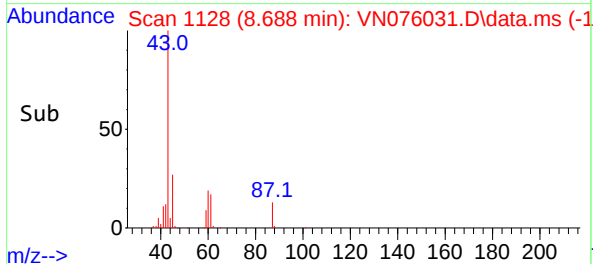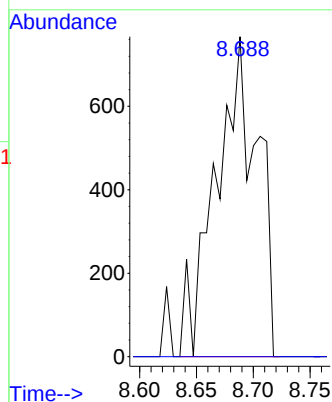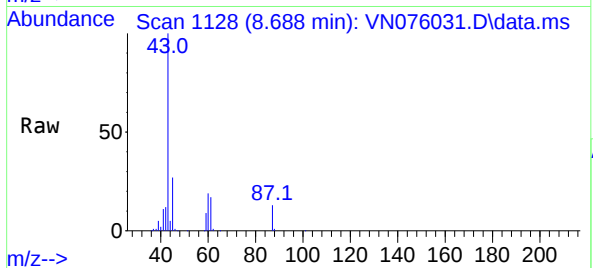

#43
Isopropyl Acetate
Concen: 69.999 ug/l
RT: 8.694 min Scan# 1129
Delta R.T. -0.000 min
Lab File: VN076031.D
Acq: 29 Dec 2022 04:31

Tgt Ion: 43 Resp: 454214
Ion Ratio Lower Upper
43 100
61 9.2 24.2 36.4#
87 6.9 13.3 19.9#

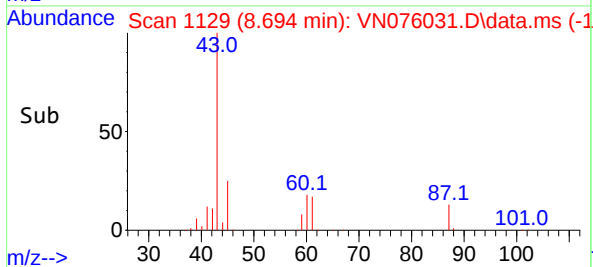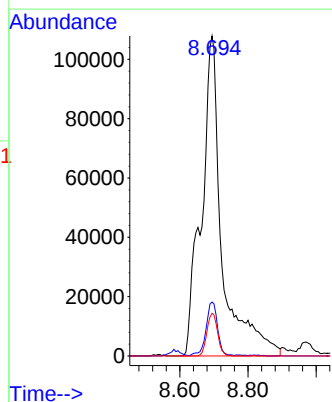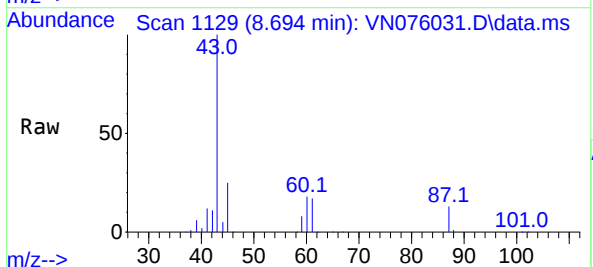

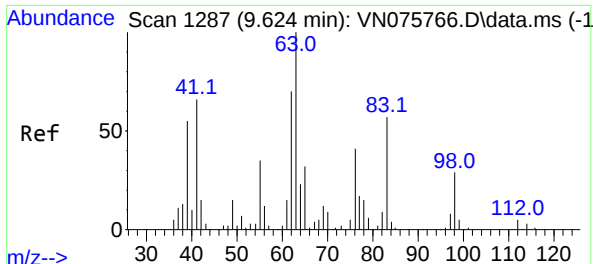

#45

1,2-Dichloropropane

Concen: 0.628 ug/l

RT: 9.741 min Scan# 11

Delta R.T. 0.118 min

Lab File: VN076031.D

Acq: 29 Dec 2022 04:31

Instrument :

MSVOA_N

ClientSampleId :





PB149923ZHE#12

Tgt Ion: 63 Resp: 2309

Ion Ratio Lower Upper

63 100

65 0.0 25.7 38.5#

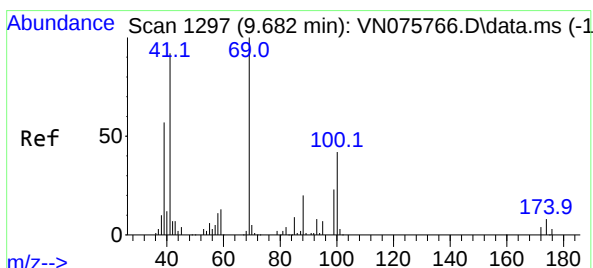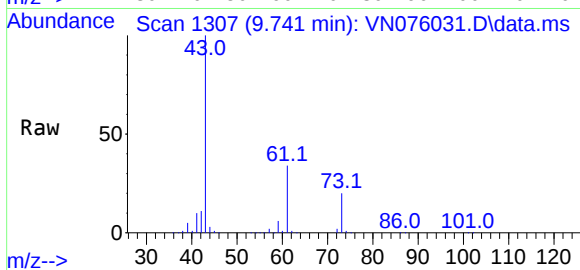

#48

Methyl methacrylate

Concen: 1.871 ug/l

RT: 9.665 min Scan# 1294

Delta R.T. -0.018 min

Lab File: VN076031.D

Acq: 29 Dec 2022 04:31




Tgt Ion: 41 Resp: 5467


Ion Ratio Lower Upper

41 100

69 0.0 81.9 122.9#

39 58.7 51.6 77.4


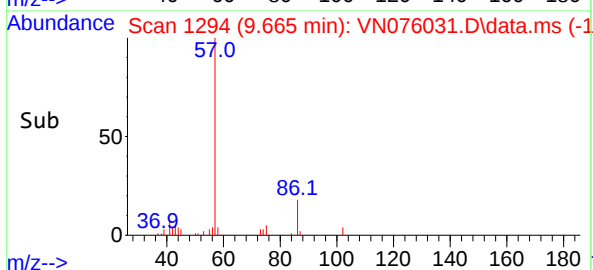

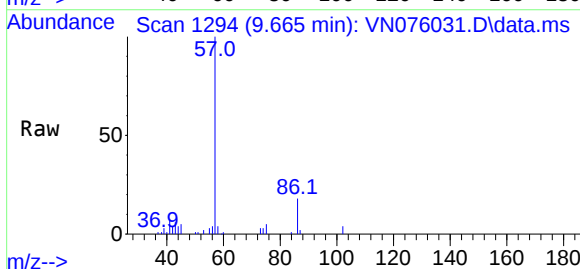


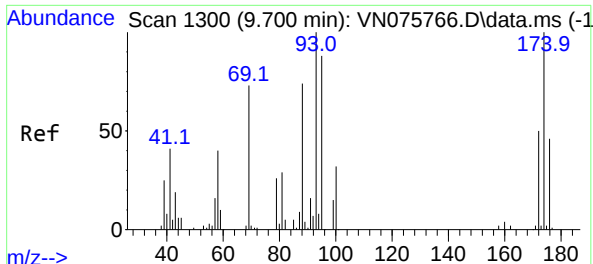

#49
1,4-Dioxane
Concen: 3.132 ug/l
RT: 9.747 min Scan# 11
Delta R.T. 0.047 min
Lab File: VN076031.D
Acq: 29 Dec 2022 04:31




Instrument :
MSVOA_N
ClientSampleId :
PB149923ZHE#12


Tgt Ion: 88 Resp: 225
Ion Ratio Lower Upper
88 100
43 678168.0 17.1 25.7#
58 3200.0 47.8 71.8#

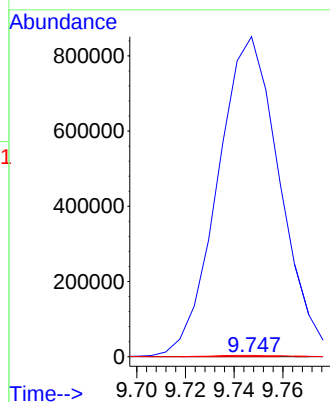

#50
Toluene-d8
Concen: 50.981 ug/l
RT: 10.571 min Scan# 1448
Delta R.T. -0.000 min
Lab File: VN076031.D
Acq: 29 Dec 2022 04:31

Tgt Ion: 98 Resp: 702698
Ion Ratio Lower Upper
98 100
100 64.7 52.1 78.1


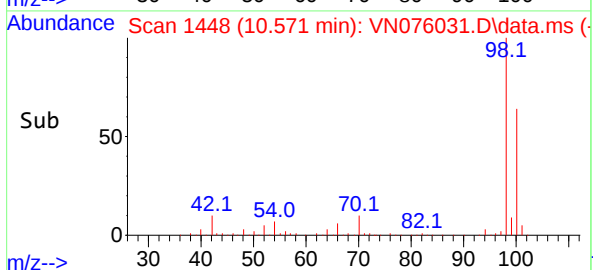

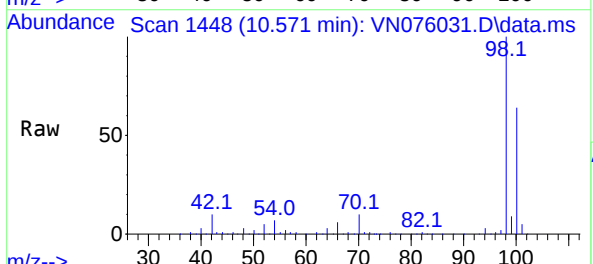




#51
4-Methyl-2-Pentanone
Concen: 5.451 ug/l
RT: 10.447 min Scan# 1427
Delta R.T. -0.000 min
Lab File: VN076031.D
Acq: 29 Dec 2022 04:31




Instrument :
MSVOA_N
ClientSampleId :
PB149923ZHE#12


Tgt Ion: 43 Resp: 21389
Ion Ratio Lower Upper
43 100
58 32.1 35.5 53.3#

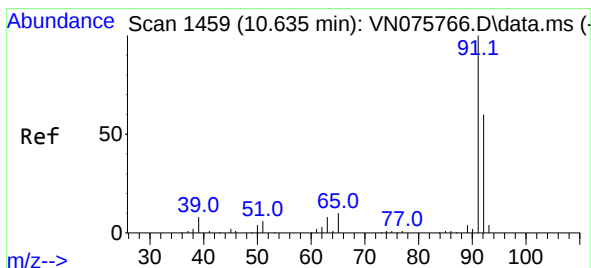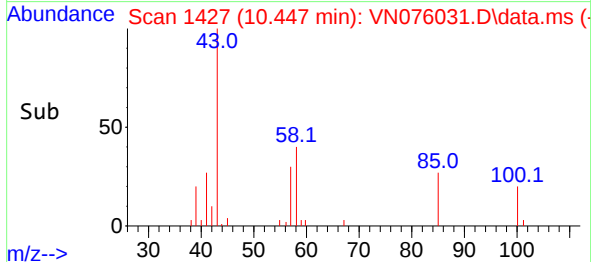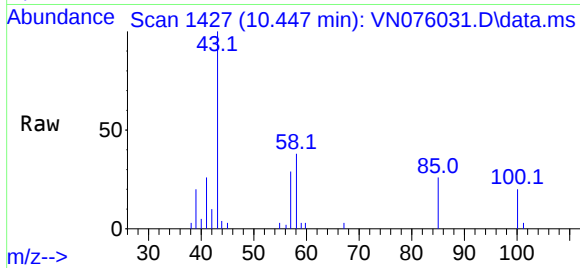

#52
Toluene
Concen: 0.605 ug/l
RT: 10.635 min Scan# 1459
Delta R.T. -0.000 min
Lab File: VN076031.D
Acq: 29 Dec 2022 04:31

Tgt Ion: 92 Resp: 5951
Ion Ratio Lower Upper
92 100
91 175.1 137.3 205.9


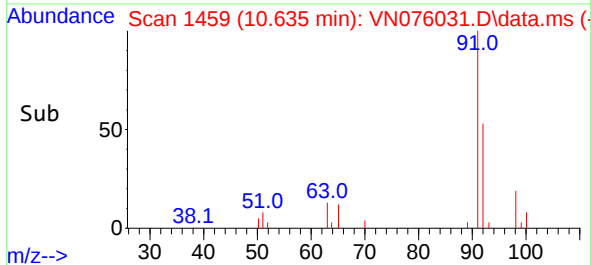

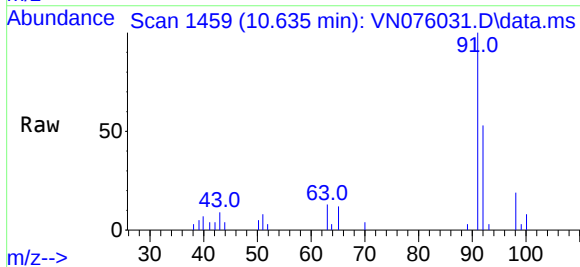


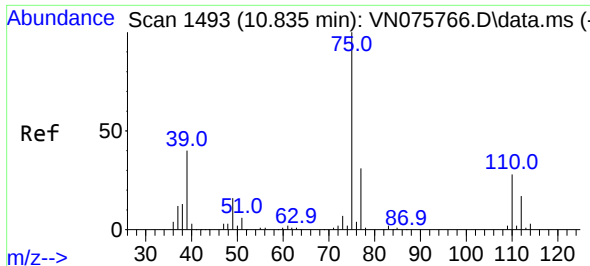

#53
t-1,3-Dichloropropene
Concen: 0.247 ug/l
RT: 10.729 min Scan# 1412
Delta R.T. -0.106 min
Lab File: VN076031.D
Acq: 29 Dec 2022 04:31




Instrument :
MSVOA_N
ClientSampleId :
PB149923ZHE#12


Tgt Ion: 75 Resp: 1294
Ion Ratio Lower Upper
75 100
77 17.9 24.9 37.3#

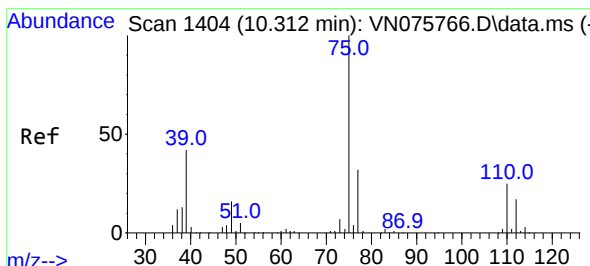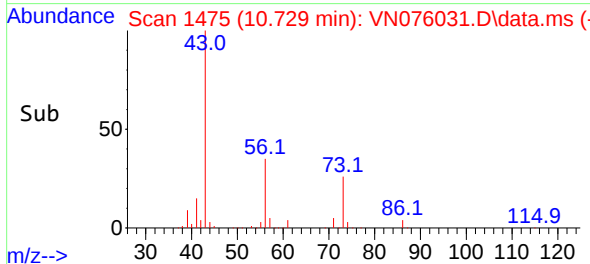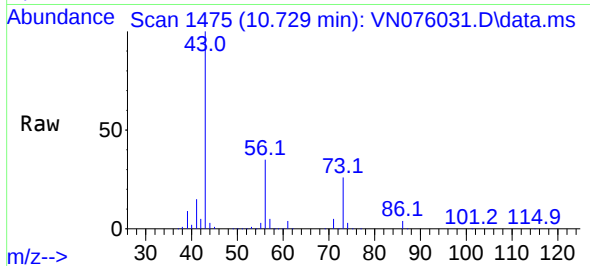

#54
cis-1,3-Dichloropropene
Concen: 13.528 ug/l
RT: 10.359 min Scan# 1412
Delta R.T. 0.047 min
Lab File: VN076031.D
Acq: 29 Dec 2022 04:31

Tgt Ion: 75 Resp: 77759
Ion Ratio Lower Upper
75 100
77 0.6 25.8 38.8#
39 26.3 33.4 50.2#


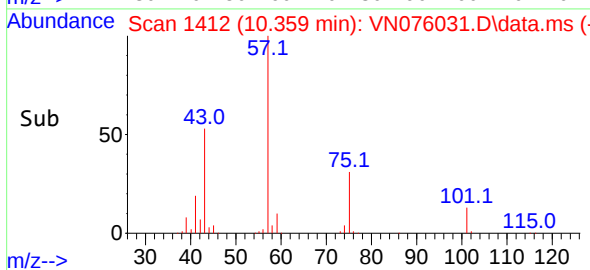

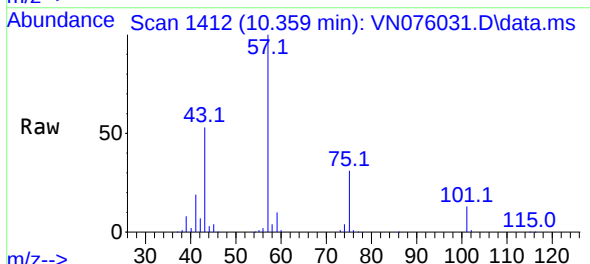




#56
Ethyl methacrylate
Concen: 0.361 ug/l
RT: 10.988 min Scan# 11
Delta R.T. 0.112 min
Lab File: VN076031.D
Acq: 29 Dec 2022 04:31




Instrument :
MSVOA_N
ClientSampleId :
PB149923ZHE#12


Tgt Ion: 69 Resp: 1851
Ion Ratio Lower Upper
69 100
41 5460.1 44.2 66.4#
39 2507.8 26.4 39.6#



#57
1,3-Dichloropropane
Concen: 1.607 ug/l
RT: 11.200 min Scan# 1555
Delta R.T. 0.035 min
Lab File: VN076031.D
Acq: 29 Dec 2022 04:31

Tgt Ion: 76 Resp: 10179
Ion Ratio Lower Upper
76 100
78 0.0 26.2 39.2#


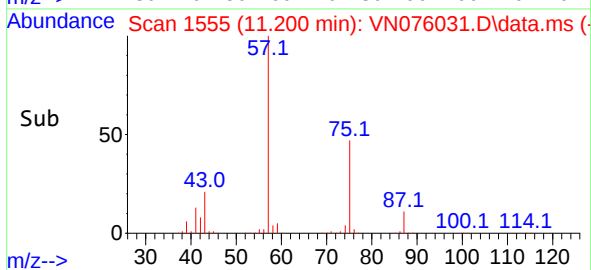






#59
2-Hexanone
Concen: 52.895 ug/l
RT: 11.176 min Scan# 1551
Delta R.T. -0.024 min
Lab File: VN076031.D
Acq: 29 Dec 2022 04:31




Instrument :
MSVOA_N
ClientSampleId :
PB149923ZHE#12


Tgt Ion: 43 Resp: 151373
Ion Ratio Lower Upper
43 100
58 0.0 30.6 92.0#

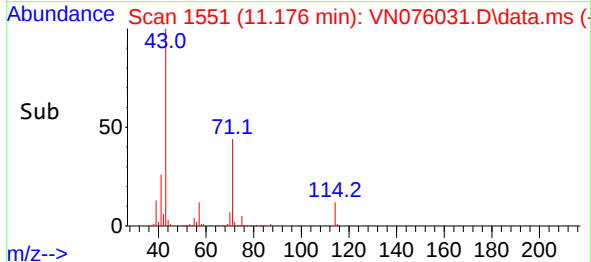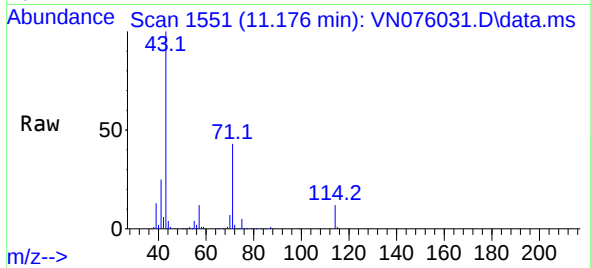

#62
4-Bromofluorobenzene
Concen: 48.273 ug/l
RT: 12.853 min Scan# 1836
Delta R.T. -0.000 min
Lab File: VN076031.D
Acq: 29 Dec 2022 04:31

Tgt Ion: 95 Resp: 220379
Ion Ratio Lower Upper
95 100
174 87.8 0.0 171.6
176 85.4 0.0 169.2


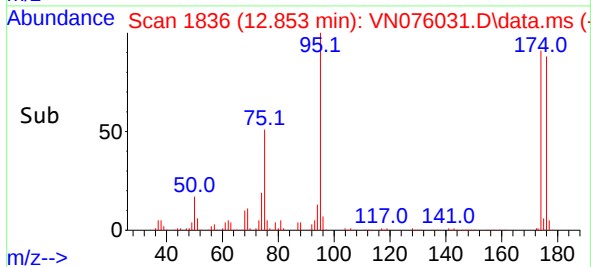

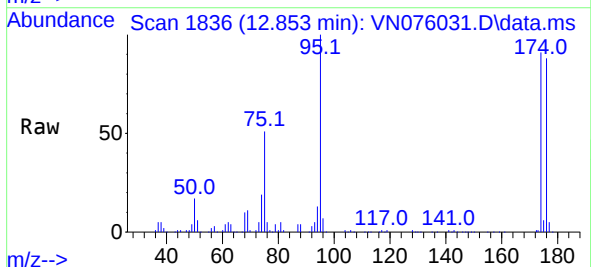




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.871 min Scan# 11
Delta R.T. 0.006 min
Lab File: VN076031.D
Acq: 29 Dec 2022 04:31




Instrument :
MSVOA_N
ClientSampleId :
PB149923ZHE#12


Tgt Ion:117 Resp: 533325
Ion Ratio Lower Upper
117 100
82 51.0 41.3 61.9
119 32.2 24.6 37.0

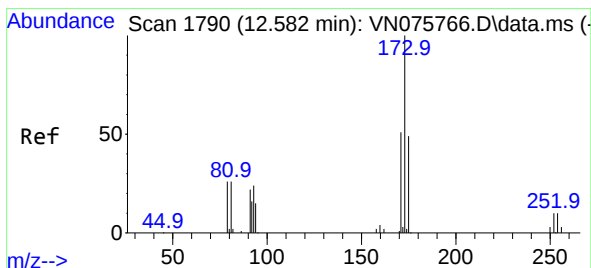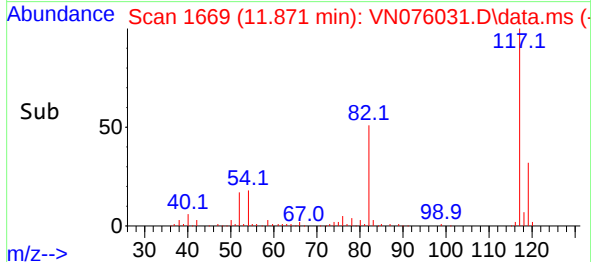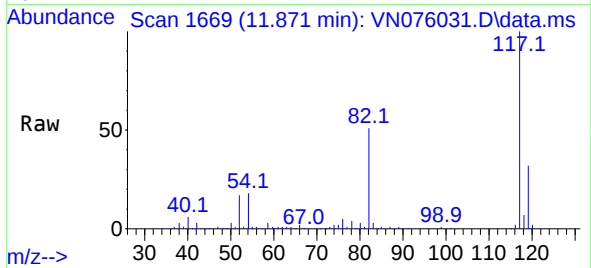

#71
Bromoform
Concen: 0.678 ug/l
RT: 12.853 min Scan# 1836
Delta R.T. 0.271 min
Lab File: VN076031.D
Acq: 29 Dec 2022 04:31

Tgt Ion:173 Resp: 1999
Ion Ratio Lower Upper
173 100
175 569.3 24.3 72.8#
254 0.0 0.0 0.0


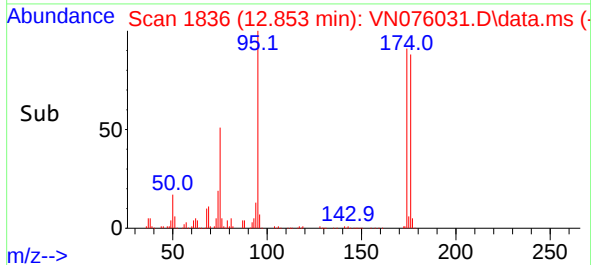

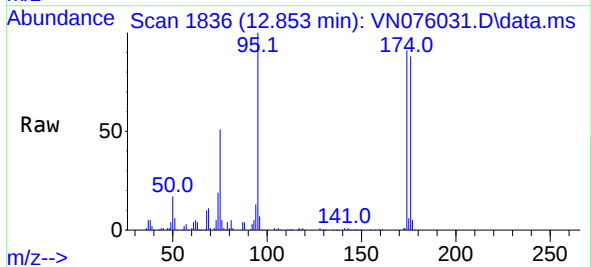




#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.794 min Scan# 1996
Delta R.T. -0.000 min
Lab File: VN076031.D
Acq: 29 Dec 2022 04:31




Instrument :
MSVOA_N
ClientSampleId :
PB149923ZHE#12


Tgt Ion:152 Resp: 224474
Ion Ratio Lower Upper
152 100
115 57.4 29.1 87.4
150 156.0 0.0 347.0

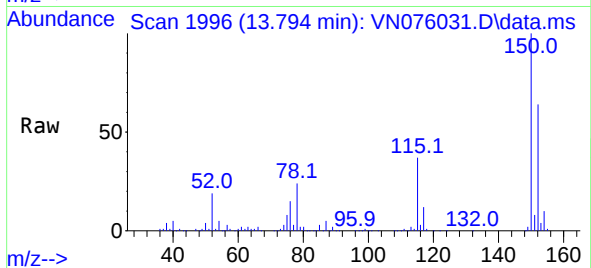

#74
N-ethyl acetate
Concen: 0.297 ug/l
RT: 12.488 min Scan# 1774
Delta R.T. -0.006 min
Lab File: VN076031.D
Acq: 29 Dec 2022 04:31

Tgt Ion: 43 Resp: 1413
Ion Ratio Lower Upper
43 100
70 3.9 41.4 62.0#
55 0.0 21.3 31.9#
61 0.0 21.2 31.8#


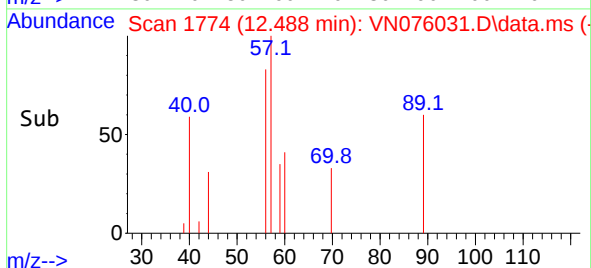
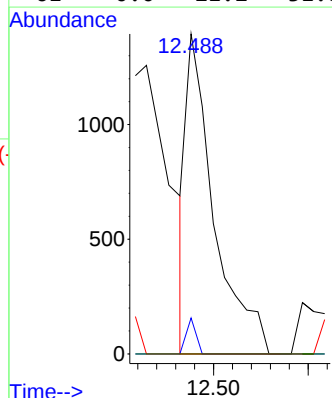





#76
1,2,3-Trichloropropane
Concen: 24.853 ug/l
RT: 12.853 min Scan# 1836
Delta R.T. -0.141 min
Lab File: VN076031.D
Acq: 29 Dec 2022 04:31




Instrument :
MSVOA_N
ClientSampleId :
PB149923ZHE#12


Tgt Ion: 75 Resp: 112458
Ion Ratio Lower Upper
75 100
77 1.3 82.6 247.8#



#81
trans-1,4-Dichloro-2-butene
Concen: 89.460 ug/l
RT: 12.853 min Scan# 1836
Delta R.T. 0.112 min
Lab File: VN076031.D
Acq: 29 Dec 2022 04:31

Tgt Ion: 75 Resp: 112458
Ion Ratio Lower Upper
75 100
53 0.0 73.8 110.6#
89 0.0 39.5 59.3#

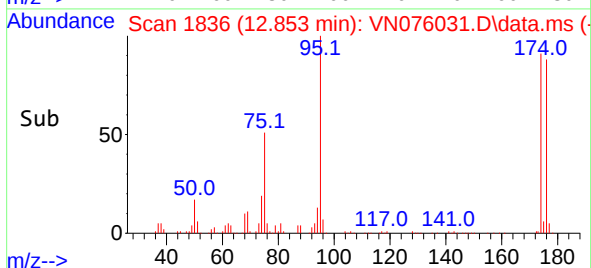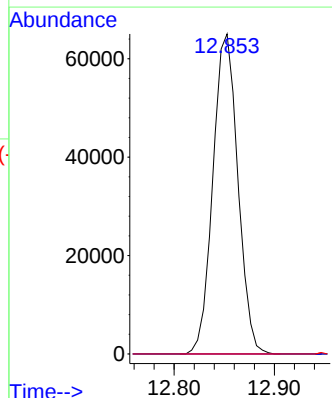



#95

Naphthalene

Concen: 2.338 ug/l

RT: 15.647 min Scan# 21

Delta R.T. 0.006 min

Lab File: VN076031.D


Acq: 29 Dec 2022 04:31

Instrument :

MSVOA_N

ClientSampleId :

PB149923ZHE#12

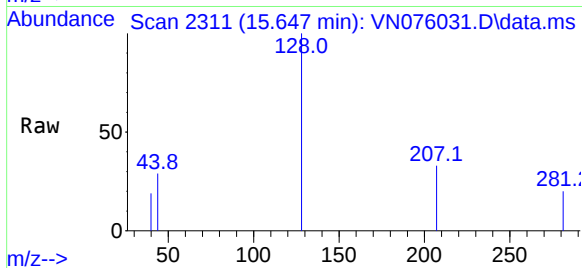

Tgt Ion:128 Resp: 2054

Ion Ratio Lower Upper

128 100

127 0.0 10.4 15.6#

129 8.3 8.7 13.1#

