
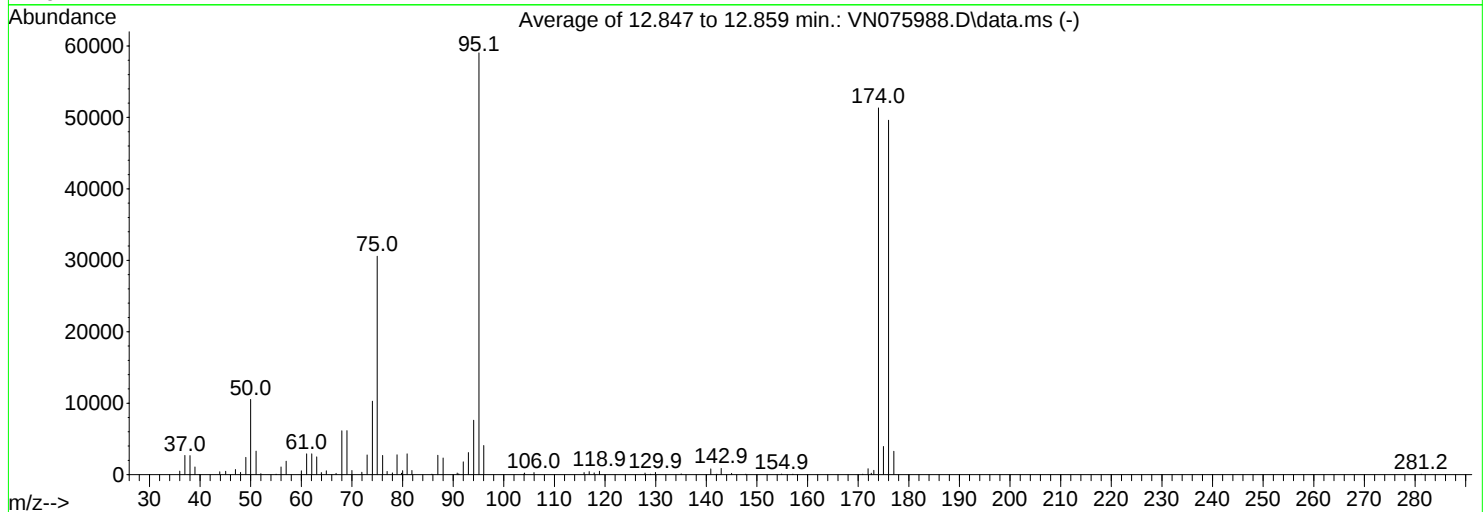


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN122822\
Data File : VN075988.D
Acq On : 28 Dec 2022 09:25
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N121422W.M
Title : SW846 8260
Last Update : Wed Dec 14 13:03:41 2022

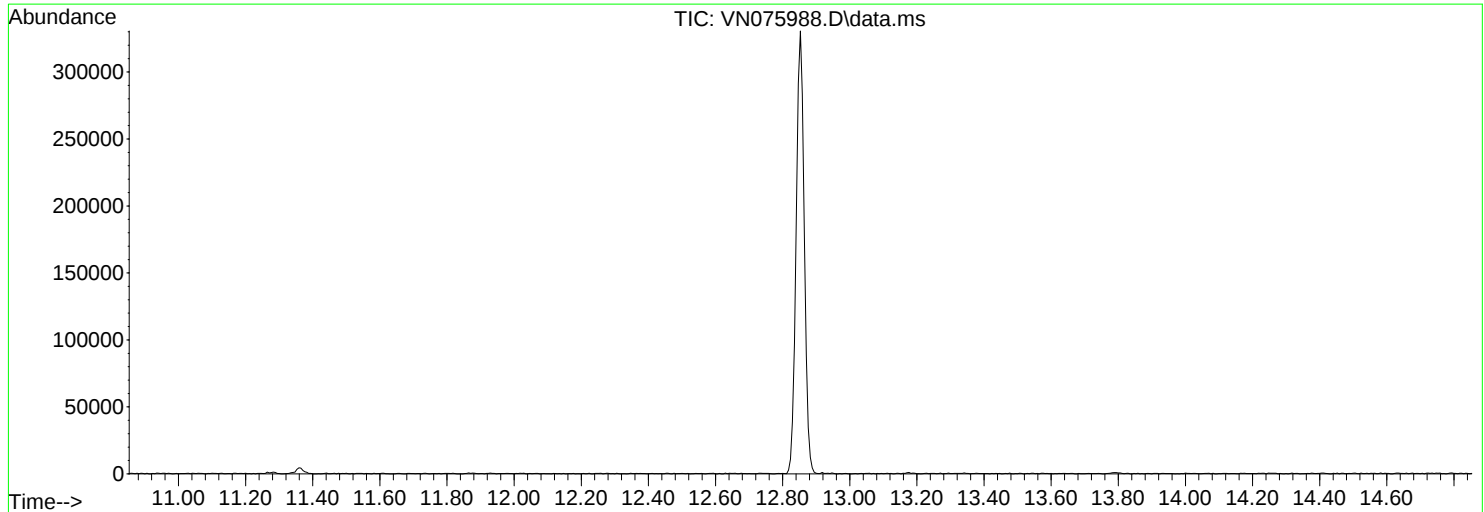

AutoFind: Scans 1835, 1836, 1837; Background Corrected with Scan 1827

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.8	10517	PASS
75	95	30	60	51.8	30571	PASS
95	95	100	100	100.0	59040	PASS
96	95	5	9	6.9	4073	PASS
173	174	0.00	2	1.2	597	PASS
174	95	50	100	87.0	51341	PASS
175	174	5	9	7.7	3953	PASS
176	174	95	101	96.6	49600	PASS
177	176	5	9	6.6	3279	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.00	502	51.05	3304	66.85	184	78.90	277
37.00	2687	52.00	130	68.00	6144	79.80	20
38.00	2671	55.00	60	69.00	6162	80.00	56
39.00	1067	56.00	1074	70.00	594	80.90	290
39.90	29	57.00	1883	71.95	346	81.85	577
43.90	412	60.00	532	73.00	2754	85.80	72
45.05	478	61.05	2922	74.05	10278	86.95	2702
47.00	718	62.05	2918	75.00	30571	88.00	2328
48.00	324	63.05	2495	76.05	2689	90.80	227
49.05	2419	63.95	290	76.95	457	91.10	115
50.00	10517	64.95	535	78.00	242	92.00	1800

Average of 12.847 to 12.859 min.: VN075988.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
93.00	3101	127.90	214	170.90	61		
94.05	7607	129.00	71	171.95	840		
95.10	59040	129.95	306	172.60	195		
96.05	4073	135.05	115	173.10	597		
103.90	78	140.90	800	174.00	51341		
104.10	225	142.10	63	175.00	3953		
105.95	302	142.95	875	176.00	49600		
115.85	287	145.00	172	177.05	3279		
116.85	423	147.80	79	281.20	68		
117.85	255	154.90	93				
118.90	460	157.10	66				

Instrument :

MSVOA_N

ClientSampleId :

BFB