


BFB

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_N\Data\VN122822\  
Data File : VN076015.D  
Acq On : 28 Dec 2022 21:45  
Operator : JC\MD  
Sample : BFB  
Misc : 5.0mL/MSVOA\_N/WATER  
ALS Vial : 29 Sample Multiplier: 1

Instrument :  
MSVOA\_N  
ClientSampleId :  
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA\_N\methods\82N121422W.M  
Title : SW846 8260  
Last Update : Wed Dec 14 13:03:41 2022

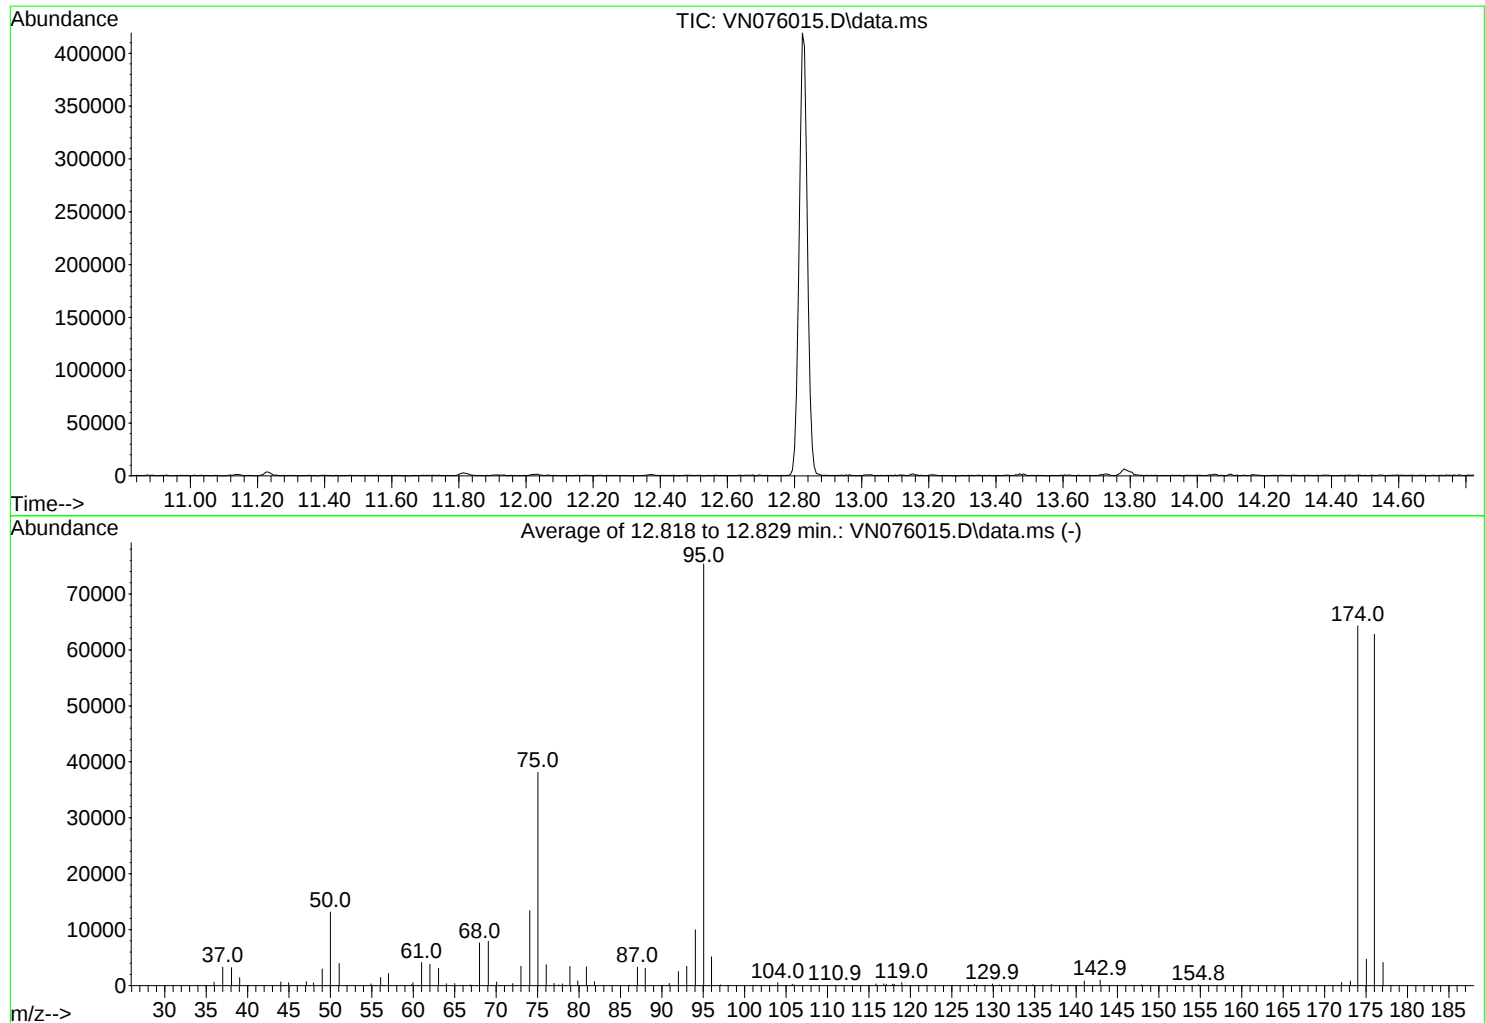

AutoFind: Scans 1830, 1831, 1832; Background Corrected with Scan 1822

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 50             | 95              | 15              | 40              | 17.4         | 13148      | PASS                |
| 75             | 95              | 30              | 60              | 50.6         | 38125      | PASS                |
| 95             | 95              | 100             | 100             | 100.0        | 75387      | PASS                |
| 96             | 95              | 5               | 9               | 6.8          | 5155       | PASS                |
| 173            | 174             | 0.00            | 2               | 1.2          | 791        | PASS                |
| 174            | 95              | 50              | 100             | 85.3         | 64328      | PASS                |
| 175            | 174             | 5               | 9               | 7.3          | 4717       | PASS                |
| 176            | 174             | 95              | 101             | 97.6         | 62797      | PASS                |
| 177            | 176             | 5               | 9               | 6.6          | 4159       | PASS                |

BFB

Modified:subtracted

| m/z   | abund. | m/z   | abund. | m/z   | abund. | m/z   | abund. |
|-------|--------|-------|--------|-------|--------|-------|--------|
| 35.95 | 622    | 51.05 | 3970   | 65.00 | 368    | 77.00 | 401    |
| 37.00 | 3334   | 51.90 | 53     | 66.80 | 54     | 77.55 | 144    |
| 38.05 | 3216   | 54.90 | 309    | 66.95 | 133    | 78.00 | 311    |
| 39.05 | 1432   | 56.05 | 1459   | 68.00 | 7647   | 78.90 | 3441   |
| 39.95 | 8      | 57.00 | 2160   | 69.05 | 7911   | 79.85 | 874    |
| 44.00 | 654    | 59.80 | 179    | 70.05 | 662    | 80.90 | 3341   |
| 44.95 | 525    | 59.95 | 537    | 72.00 | 386    | 81.85 | 707    |
| 47.10 | 700    | 61.00 | 4110   | 73.00 | 3457   | 83.00 | 69     |
| 47.95 | 490    | 62.00 | 3844   | 74.05 | 13417  | 86.10 | 82     |
| 49.00 | 2977   | 63.05 | 3108   | 75.05 | 38125  | 87.05 | 3319   |
| 50.00 | 13148  | 64.00 | 340    | 76.05 | 3762   | 88.00 | 3124   |

Average of 12.818 to 12.829 min.: VN076015.D\data.ms

BFB

Modified:subtracted

| m/z    | abund. | m/z    | abund. | m/z    | abund. | m/z    | abund. |
|--------|--------|--------|--------|--------|--------|--------|--------|
| 90.90  | 403    | 113.00 | 50     | 129.90 | 289    | 156.70 | 63     |
| 92.00  | 2525   | 114.90 | 64     | 130.80 | 149    | 157.10 | 62     |
| 93.00  | 3467   | 115.85 | 327    | 134.80 | 163    | 172.05 | 571    |
| 94.05  | 9975   | 116.80 | 331    | 137.05 | 216    | 173.10 | 791    |
| 95.05  | 75387  | 117.10 | 251    | 141.00 | 835    | 174.00 | 64328  |
| 96.00  | 5155   | 117.85 | 250    | 141.90 | 69     | 175.05 | 4717   |
| 97.10  | 135    | 118.05 | 249    | 142.90 | 1013   | 176.00 | 62797  |
| 104.00 | 552    | 118.95 | 548    | 145.00 | 57     | 177.05 | 4159   |
| 105.75 | 246    | 127.75 | 243    | 147.90 | 152    | 178.00 | 64     |
| 106.00 | 132    | 128.10 | 82     | 153.90 | 60     |        |        |
| 110.90 | 63     | 128.90 | 57     | 154.80 | 145    |        |        |

Instrument :

MSVOA\_N

ClientSampleId :

BFB