

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN122921\
 Data File : VN070346.D
 Acq On : 29 Dec 2021 14:08
 Operator : JC/MD
 Sample : M5115-01
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :

Quant Time: Dec 30 01:50:06 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N122721W.M
 Quant Title : SW846 8260
 QLast Update : Mon Dec 27 18:47:12 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	8.085	168	959946	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.968	114	1622829	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.746	117	1459155	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.675	152	479087	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.437	65	695576	50.396	ug/l	0.00
Spiked Amount	50.000	Range	61 - 141	Recovery	= 100.800%	
35) Dibromofluoromethane	8.021	113	491599	50.066	ug/l	0.00
Spiked Amount	50.000	Range	69 - 133	Recovery	= 100.140%	
50) Toluene-d8	10.443	98	1874047	46.721	ug/l	0.00
Spiked Amount	50.000	Range	65 - 126	Recovery	= 93.440%	
62) 4-Bromofluorobenzene	12.731	95	647124	44.668	ug/l	0.00
Spiked Amount	50.000	Range	58 - 135	Recovery	= 89.340%	
Target Compounds						
					Qvalue	
3) Chloromethane	2.303	50	4332	0.293	ug/l	96
13) Acrolein	4.044	56	2460	1.319	ug/l #	74
15) Acrylonitrile	5.559	53	2014	0.281	ug/l #	76
16) Acetone	4.301	43	20579	2.297	ug/l #	86
17) Carbon Disulfide	4.535	76	7747	0.290	ug/l	99
18) Methyl Acetate	4.867	43	6602	0.255	ug/l #	59
25) 2-Butanone	7.343	43	2703	0.240	ug/l	98
29) Tetrahydrofuran	7.707	42	2478	0.368	ug/l #	54
31) Cyclohexane	8.085	56	23058	1.059	ug/l #	3
36) 1,1-Dichloropropene	8.085	75	81430	5.013	ug/l #	43
38) Carbon Tetrachloride	8.085	117	94392	6.086	ug/l #	16
49) 1,4-Dioxane	9.577	88	554	2.390	ug/l #	74
51) 4-Methyl-2-Pentanone	10.336	43	11134	0.534	ug/l	92
58) 2-Chloroethyl Vinyl ether	10.046	63	151	18.541	ug/l #	45
59) 2-Hexanone	11.089	43	21270	1.398	ug/l	96
65) Chlorobenzene	11.771	112	21444	0.693	ug/l	99
74) N-amyl acetate	12.390	43	12018	0.642	ug/l	92
75) 1,1,2,2-Tetrachloroethane	12.825	83	3006	0.631	ug/l #	60
76) 1,2,3-Trichloropropane	12.731	75	340987	25.461	ug/l #	1
81) trans-1,4-Dichloro-2-b...	12.731	75	340987	86.959	ug/l #	5
82) 4-Chlorotoluene	13.109	91	7844	0.265	ug/l	91
84) 1,2,4-Trimethylbenzene	13.369	105	7474	0.218	ug/l	92
87) 1,3-Dichlorobenzene	13.616	146	6004	0.351	ug/l	92
88) 1,4-Dichlorobenzene	13.616	146	6004	0.356	ug/l	92
89) n-Butylbenzene	13.946	91	14642	0.524	ug/l	96
91) 1,2-Dichlorobenzene	13.989	146	8063	0.481	ug/l	98
92) 1,2-Dibromo-3-Chloropr...	14.600	75	2489	0.966	ug/l	58
93) 1,2,4-Trichlorobenzene	15.262	180	11870	1.503	ug/l	92
94) Hexachlorobutadiene	15.372	225	1646	0.359	ug/l	91
95) Naphthalene	15.507	128	47404	3.891	ug/l	99
96) 1,2,3-Trichlorobenzene	15.700	180	13906	2.636	ug/l	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN122921\
Data File : VN070346.D
Acq On : 29 Dec 2021 14:08
Operator : JC/MD
Sample : M5115-01
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :

Quant Time: Dec 30 01:50:06 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N122721W.M
Quant Title : SW846 8260
QLast Update : Mon Dec 27 18:47:12 2021
Response via : Initial Calibration




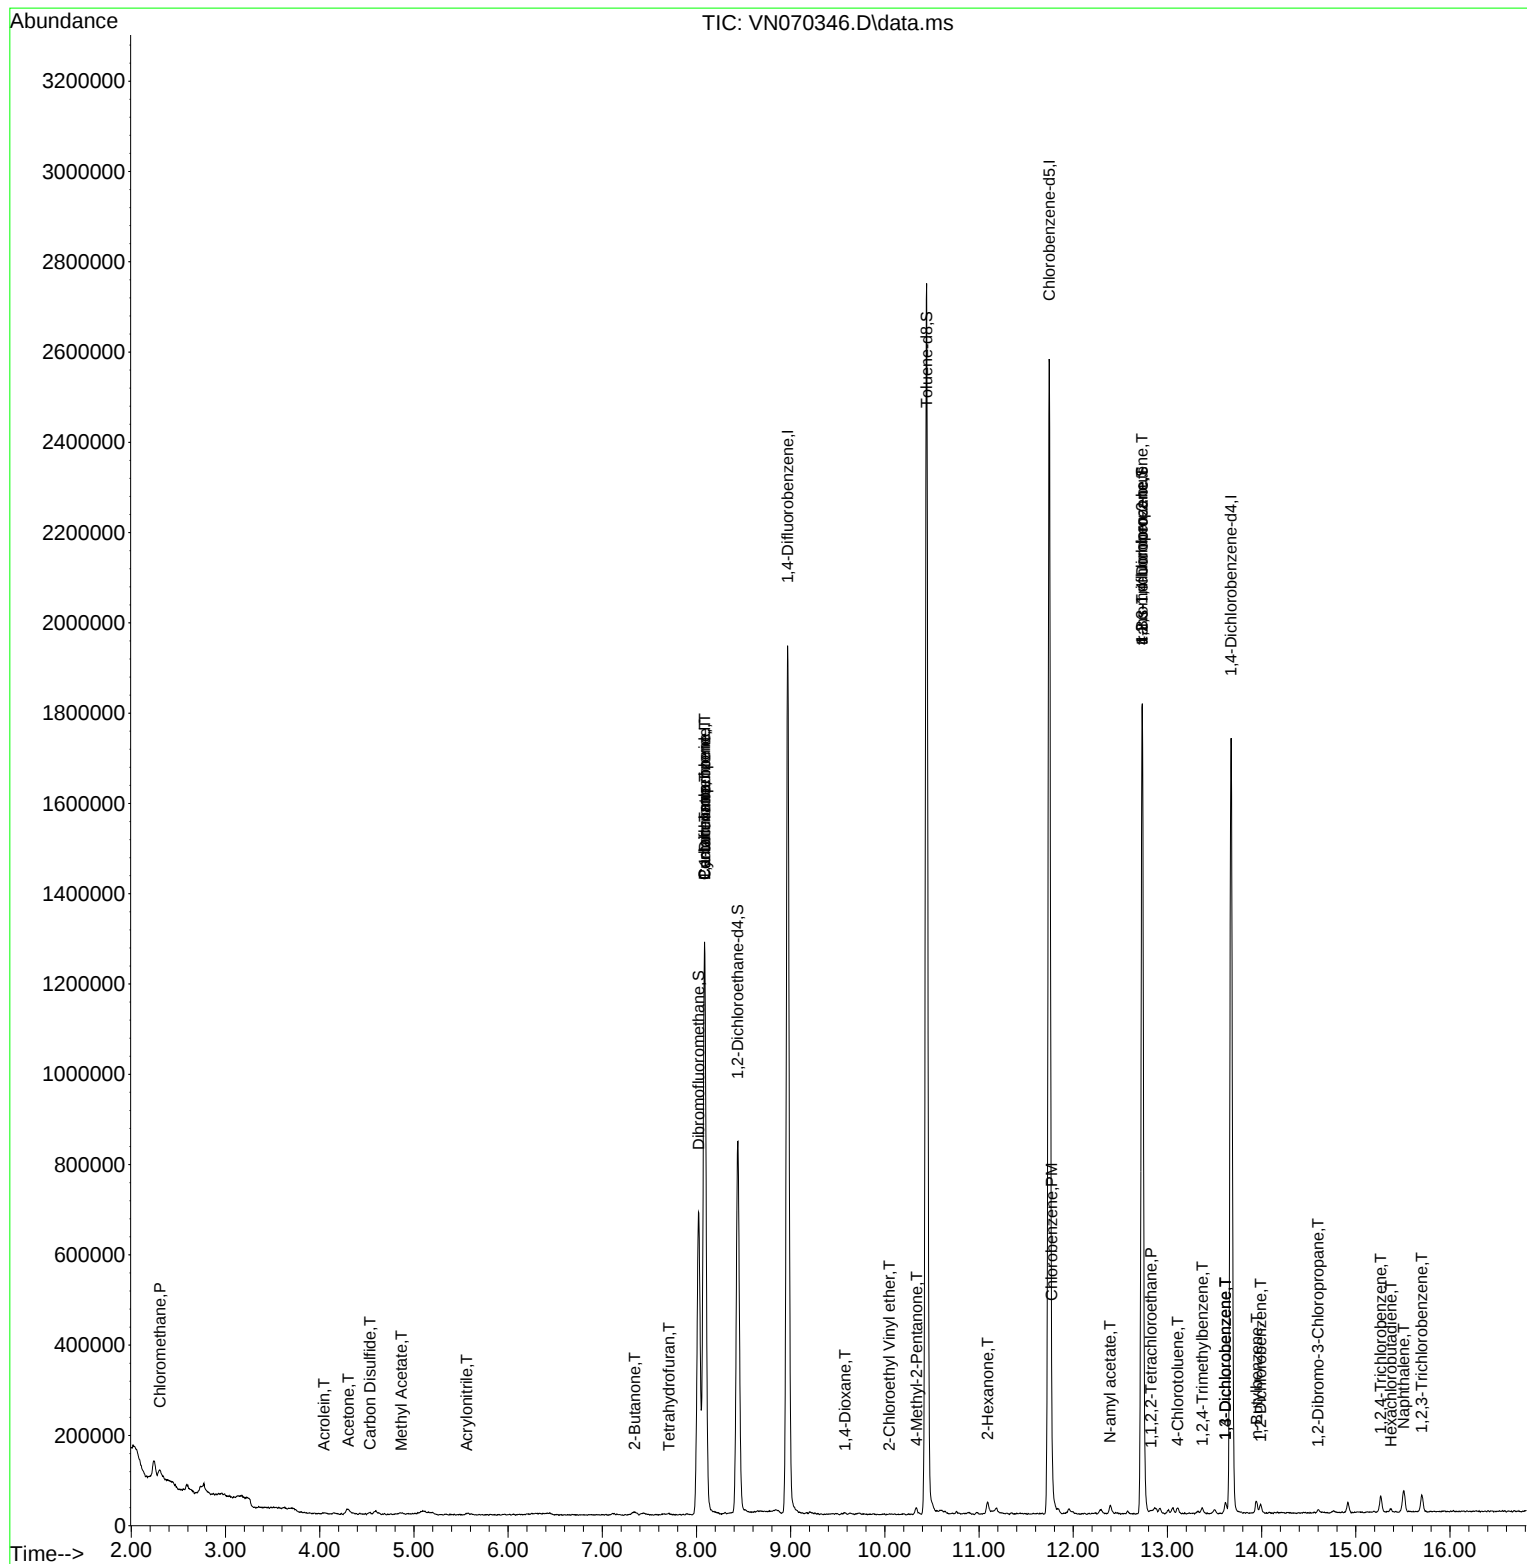




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.085 min Scan# 21
Delta R.T. -0.001 min
Lab File: VN070346.D
Acq: 29 Dec 2021 14:08




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion:168 Resp: 959946
Ion Ratio Lower Upper
168 100
99 58.6 41.3 61.9

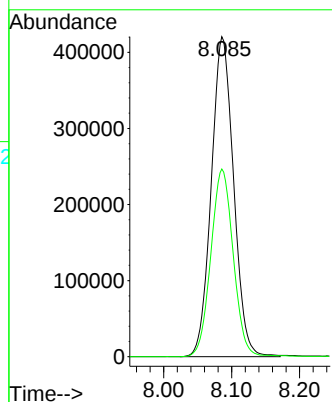

#3
Chloromethane
Concen: 0.293 ug/l
RT: 2.303 min Scan# 117
Delta R.T. 0.000 min
Lab File: VN070346.D
Acq: 29 Dec 2021 14:08

Tgt Ion: 50 Resp: 4332
Ion Ratio Lower Upper
50 100
52 33.8 25.4 38.0


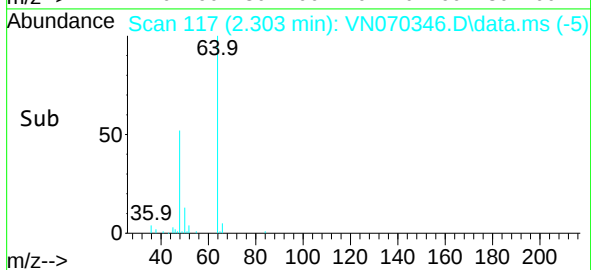
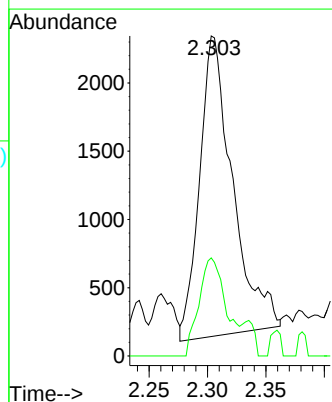
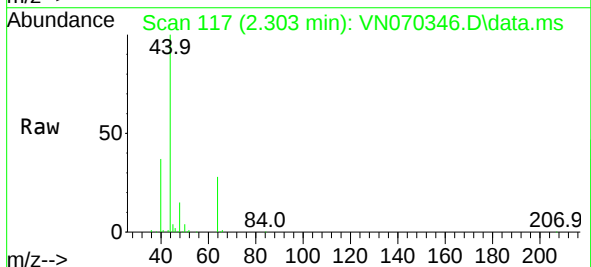


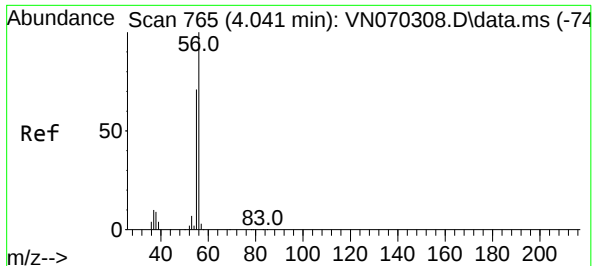

#13
Acrolein
Concen: 1.319 ug/l
RT: 4.044 min Scan# 765
Delta R.T. 0.003 min
Lab File: VN070346.D
Acq: 29 Dec 2021 14:08




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 56 Resp: 2460
Ion Ratio Lower Upper
56 100
55 92.4 56.6 85.0#

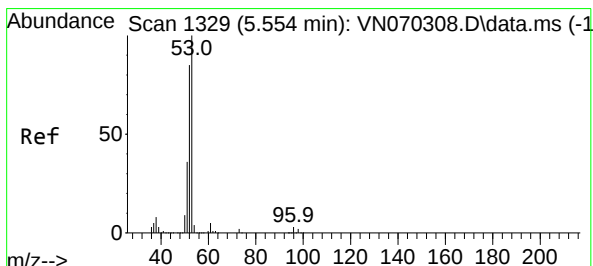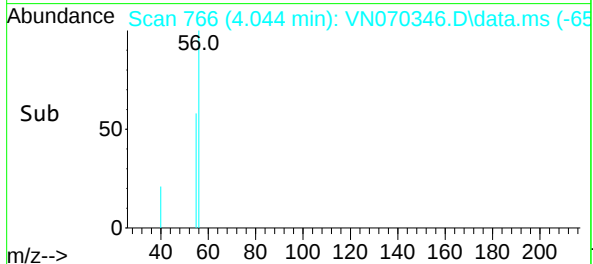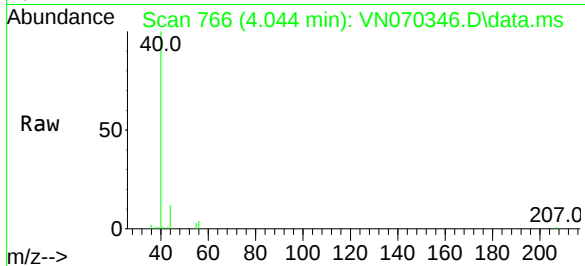

#15
Acrylonitrile
Concen: 0.281 ug/l
RT: 5.559 min Scan# 1331
Delta R.T. 0.005 min
Lab File: VN070346.D
Acq: 29 Dec 2021 14:08

Tgt Ion: 53 Resp: 2014
Ion Ratio Lower Upper
53 100
52 70.1 66.2 99.2
51 10.0 29.6 44.4#


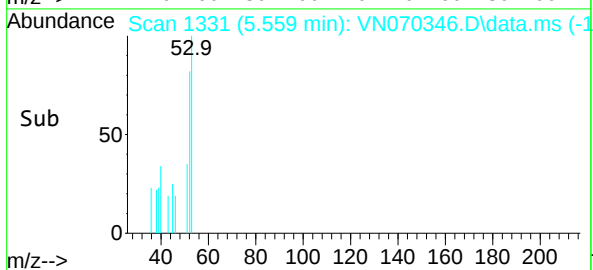

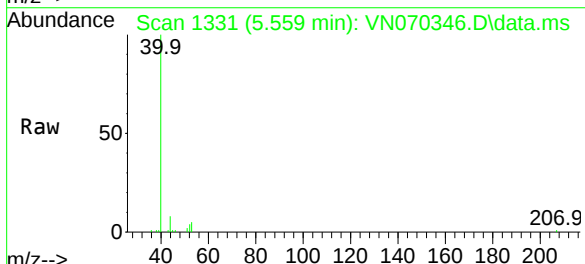




#16
Acetone
Concen: 2.297 ug/l
RT: 4.301 min Scan# 80
Delta R.T. 0.016 min
Lab File: VN070346.D
Acq: 29 Dec 2021 14:08




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 43 Resp: 20579
Ion Ratio Lower Upper
43 100
58 21.2 23.1 34.7#

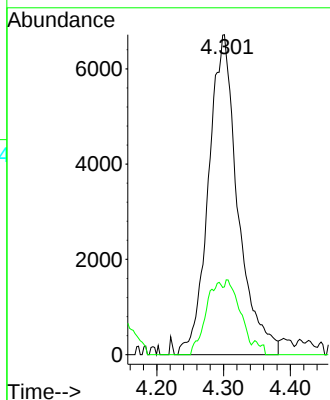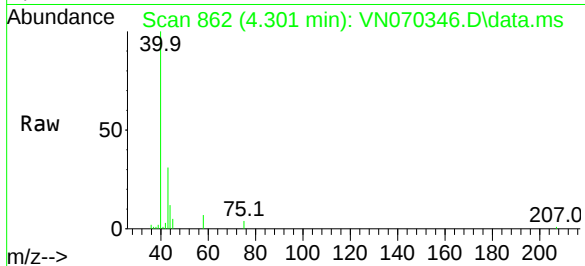

#17
Carbon Disulfide
Concen: 0.290 ug/l
RT: 4.535 min Scan# 949
Delta R.T. 0.006 min
Lab File: VN070346.D
Acq: 29 Dec 2021 14:08

Tgt Ion: 76 Resp: 7747
Ion Ratio Lower Upper
76 100
78 9.6 7.5 11.3

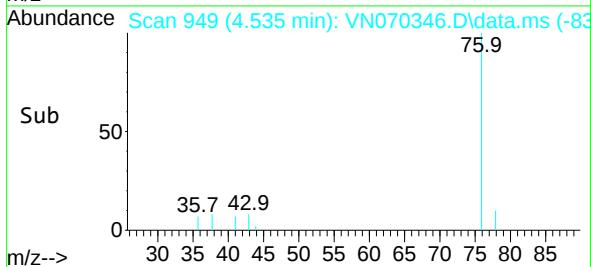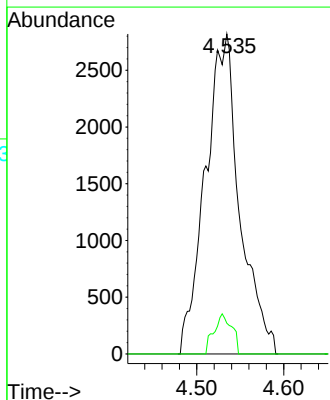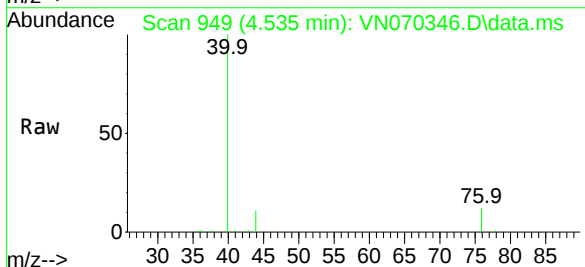

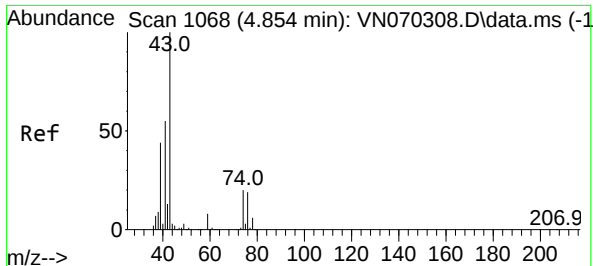

#18

Methyl Acetate

Concen: 0.255 ug/l

RT: 4.867 min Scan# 1

Delta R.T. 0.013 min

Lab File: VN070346.D

Acq: 29 Dec 2021 14:08

Instrument :

MSVOA_N





ClientSampleId :

Tgt Ion: 43 Resp: 6602

Ion Ratio Lower Upper

43 100

74 4.1 19.4 29.2#

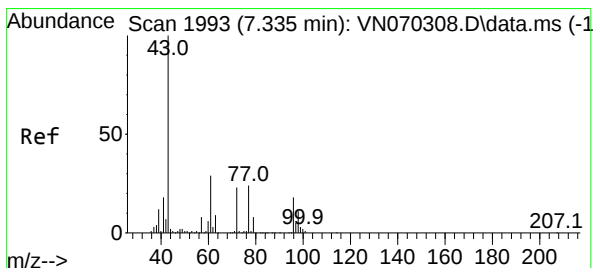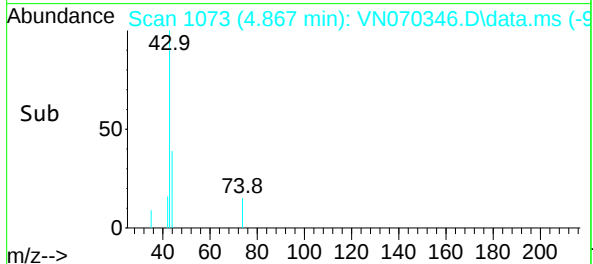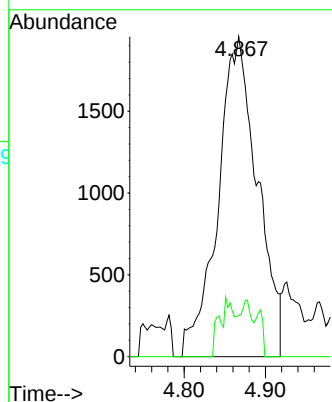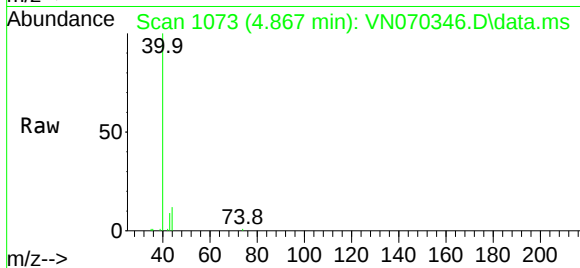

#25

2-Butanone

Concen: 0.240 ug/l

RT: 7.343 min Scan# 1996

Delta R.T. 0.008 min

Lab File: VN070346.D




Acq: 29 Dec 2021 14:08


Tgt Ion: 43 Resp: 2703

Ion Ratio Lower Upper

43 100

72 28.3 21.7 32.5

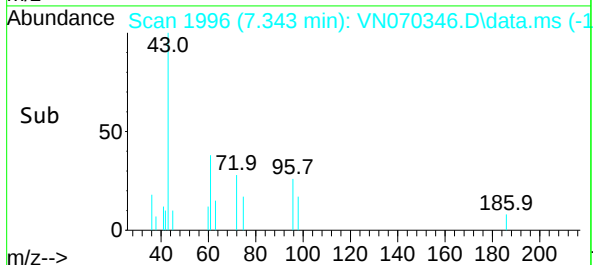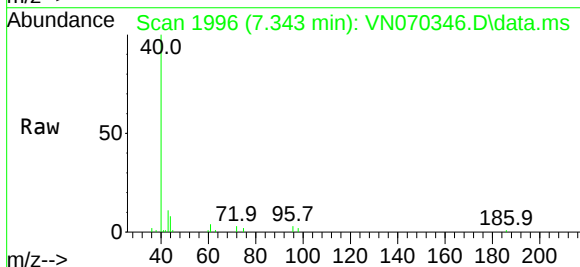



#29

Tetrahydrofuran

Concen: 0.368 ug/l

RT: 7.707 min Scan# 21

Delta R.T. 0.024 min


Lab File: VN070346.D

Acq: 29 Dec 2021 14:08

Instrument :

MSVOA_N

ClientSampleId :

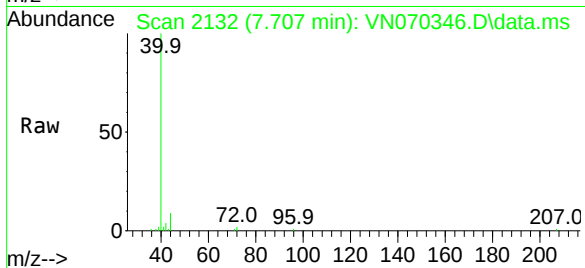




Tgt Ion: 42 Resp: 2478

Ion Ratio Lower Upper

42 100

72 17.2 36.3 54.5#

71 12.0 34.7 52.1#

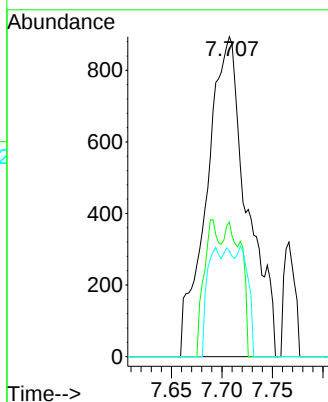

#31

Cyclohexane

Concen: 1.059 ug/l

RT: 8.085 min Scan# 2273

Delta R.T. -0.008 min

Lab File: VN070346.D

Acq: 29 Dec 2021 14:08




Tgt Ion: 56 Resp: 23058


Ion Ratio Lower Upper

56 100

69 169.6 27.1 40.7#

84 134.5 73.4 110.0#

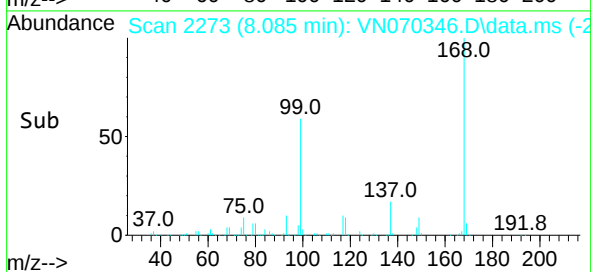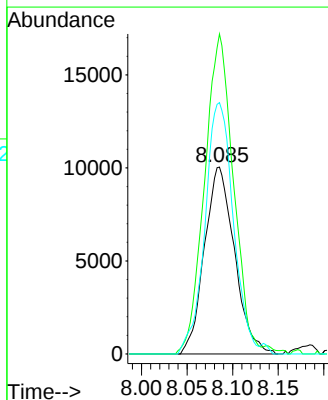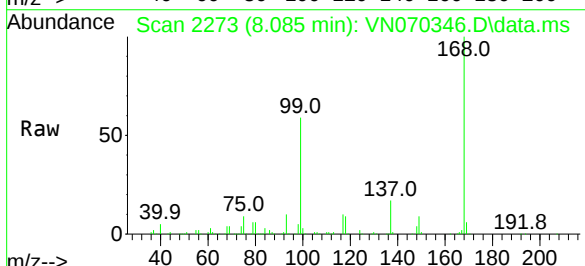



#33

1,2-Dichloroethane-d4

Concen: 50.396 ug/l

RT: 8.437 min Scan# 2404

Delta R.T. -0.000 min

Lab File: VN070346.D

Acq: 29 Dec 2021 14:08

Instrument :

MSVOA_N





ClientSampleId :

Tgt Ion: 65 Resp: 695576

Ion Ratio Lower Upper

65 100

67 53.4 0.0 103.0

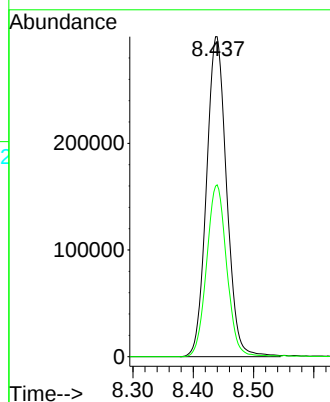

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.968 min Scan# 2602

Delta R.T. -0.000 min

Lab File: VN070346.D

Acq: 29 Dec 2021 14:08




Tgt Ion: 114 Resp: 1622829


Ion Ratio Lower Upper

114 100

63 23.2 0.0 37.8


88 16.2 0.0 27.4

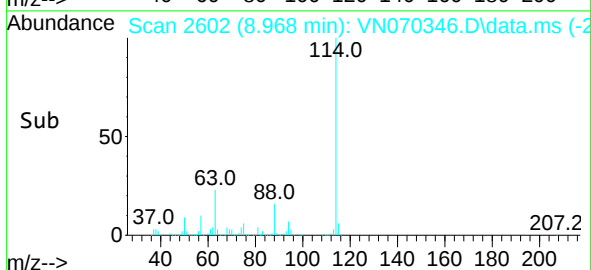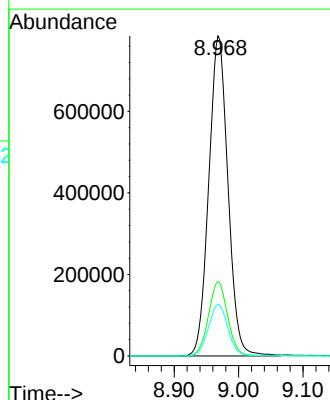






#35
Dibromofluoromethane
Concen: 50.066 ug/l
RT: 8.021 min Scan# 21
Delta R.T. 0.000 min
Lab File: VN070346.D
Acq: 29 Dec 2021 14:08

Instrument :
MSVOA_N
ClientSampleId :







Tgt Ion:113 Resp: 491599
Ion Ratio Lower Upper
113 100
111 102.5 82.2 123.2
192 19.6 16.9 25.3

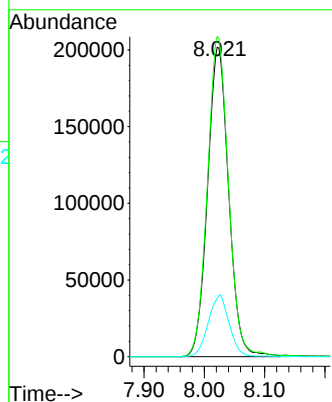

#36
1,1-Dichloropropene
Concen: 5.013 ug/l
RT: 8.085 min Scan# 2273
Delta R.T. -0.135 min
Lab File: VN070346.D
Acq: 29 Dec 2021 14:08


Tgt Ion: 75 Resp: 81430
Ion Ratio Lower Upper
75 100
110 2.2 18.4 55.2#
77 0.0 24.4 36.6#

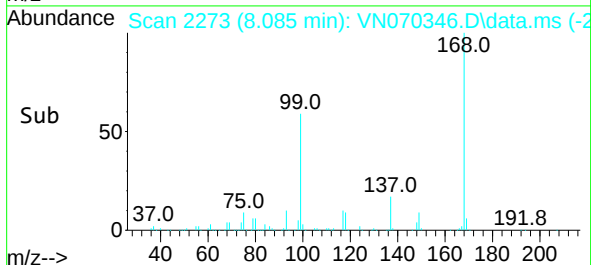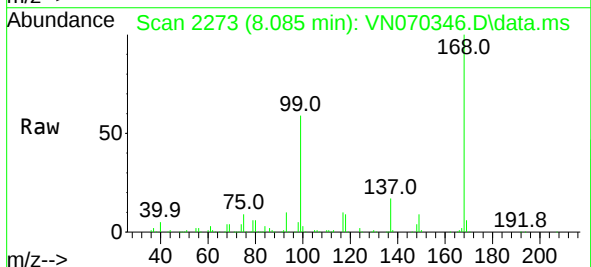






#38
Carbon Tetrachloride
Concen: 6.086 ug/l
RT: 8.085 min Scan# 21
Delta R.T. -0.120 min
Lab File: VN070346.D
Acq: 29 Dec 2021 14:08

Instrument :
MSVOA_N
ClientSampleId :







Tgt Ion:117 Resp: 94392
Ion Ratio Lower Upper
117 100
119 5.0 76.1 114.1#
121 0.0 24.2 36.2#

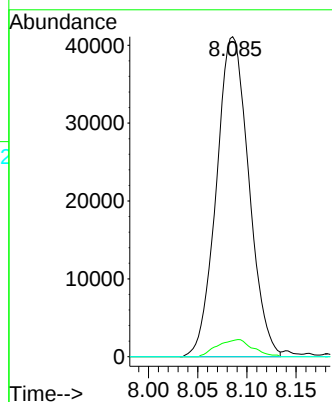

#49
1,4-Dioxane
Concen: 2.390 ug/l
RT: 9.577 min Scan# 2829
Delta R.T. 0.008 min
Lab File: VN070346.D
Acq: 29 Dec 2021 14:08

Tgt Ion: 88 Resp: 554
Ion Ratio Lower Upper
88 100
43 24.7 23.4 35.2
58 89.4 50.6 75.8#

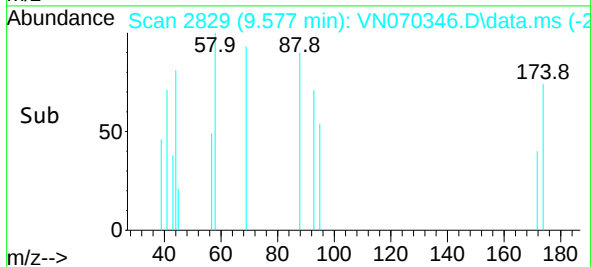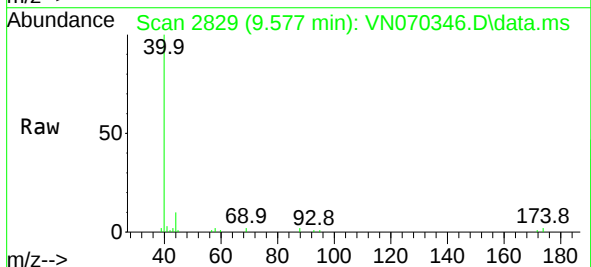



#50

Toluene-d8

Concen: 46.721 ug/l

RT: 10.443 min Scan# 3151

Delta R.T. 0.003 min

Lab File: VN070346.D

Acq: 29 Dec 2021 14:08

Instrument :

MSVOA_N





ClientSampleId :

Tgt Ion: 98 Resp: 1874047

Ion Ratio Lower Upper

98 100

100 64.4 50.4 75.6



#51

4-Methyl-2-Pentanone

Concen: 0.534 ug/l

RT: 10.336 min Scan# 3112

Delta R.T. 0.006 min

Lab File: VN070346.D




Acq: 29 Dec 2021 14:08


Tgt Ion: 43 Resp: 11134

Ion Ratio Lower Upper

43 100

58 33.4 30.4 45.6


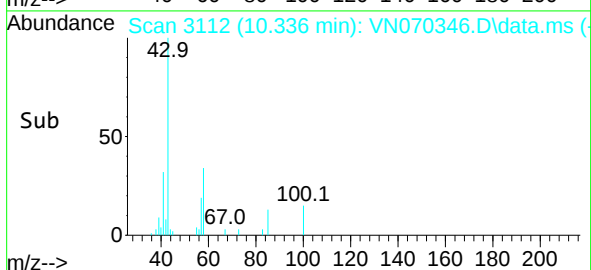






#58
2-Chloroethyl Vinyl ether
Concen: 18.541 ug/l
RT: 10.046 min Scan# 3004
Delta R.T. 0.005 min
Lab File: VN070346.D
Acq: 29 Dec 2021 14:08




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 63 Resp: 151
Ion Ratio Lower Upper
63 100
106 0.0 23.9 35.9#

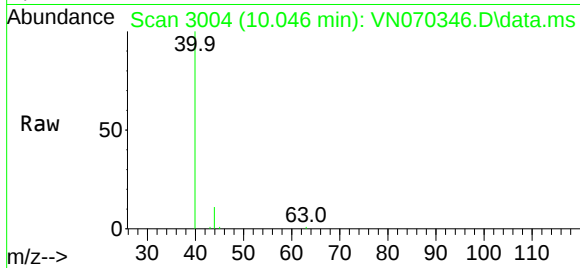

#59
2-Hexanone
Concen: 1.398 ug/l
RT: 11.089 min Scan# 3393
Delta R.T. 0.005 min
Lab File: VN070346.D
Acq: 29 Dec 2021 14:08

Tgt Ion: 43 Resp: 21270
Ion Ratio Lower Upper
43 100
58 50.7 26.9 80.7


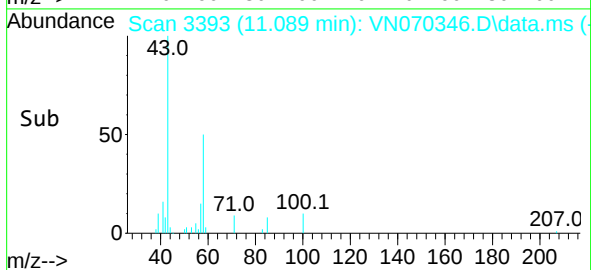

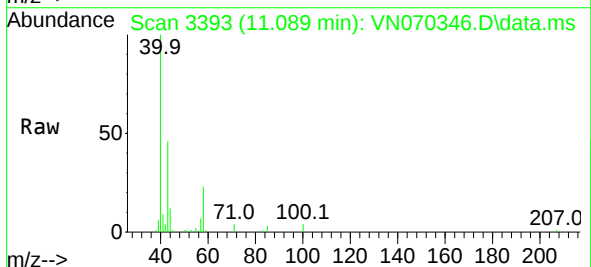


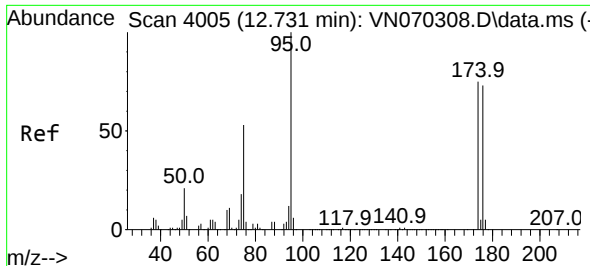

#62
4-Bromofluorobenzene
Concen: 44.668 ug/l
RT: 12.731 min Scan# 4005
Delta R.T. -0.000 min
Lab File: VN070346.D
Acq: 29 Dec 2021 14:08




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 95 Resp: 647124
Ion Ratio Lower Upper
95 100
174 76.7 0.0 187.2
176 73.5 0.0 181.4

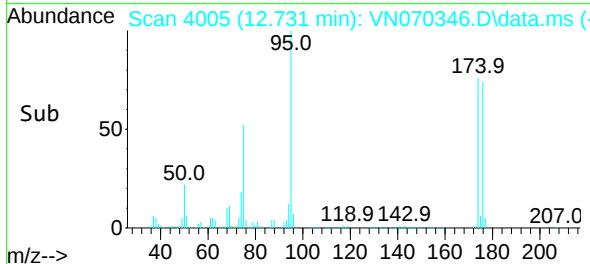

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.746 min Scan# 3638
Delta R.T. 0.002 min
Lab File: VN070346.D
Acq: 29 Dec 2021 14:08

Tgt Ion: 117 Resp: 1459155
Ion Ratio Lower Upper
117 100
82 59.4 42.4 63.6
119 31.7 25.4 38.2


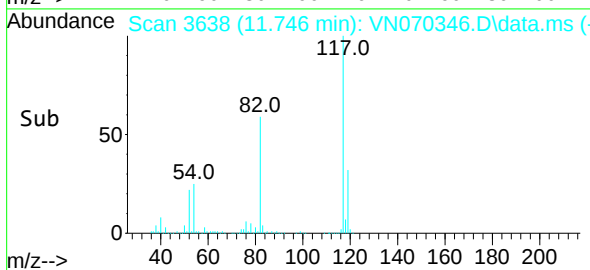

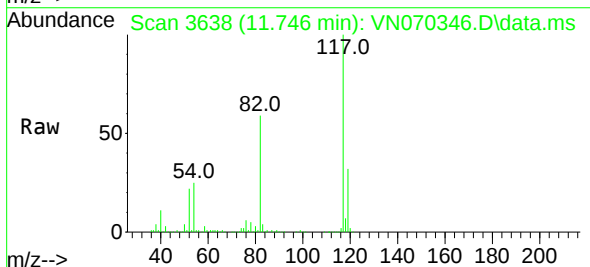




#65
Chlorobenzene
Concen: 0.693 ug/l
RT: 11.771 min Scan# 30
Delta R.T. 0.003 min
Lab File: VN070346.D
Acq: 29 Dec 2021 14:08




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion:112 Resp: 21444
Ion Ratio Lower Upper
112 100
114 32.5 25.4 38.0

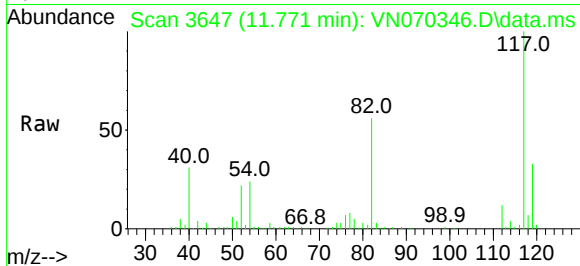

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.675 min Scan# 4357
Delta R.T. 0.003 min
Lab File: VN070346.D
Acq: 29 Dec 2021 14:08


Tgt Ion:152 Resp: 479087
Ion Ratio Lower Upper
152 100
115 60.7 27.5 82.5
150 156.6 0.0 344.4

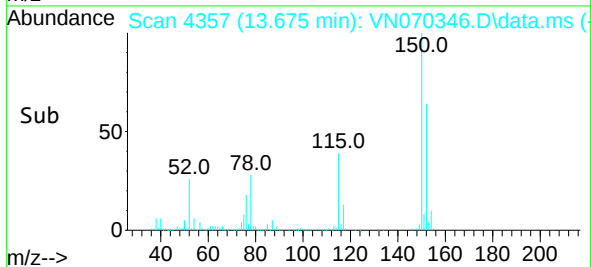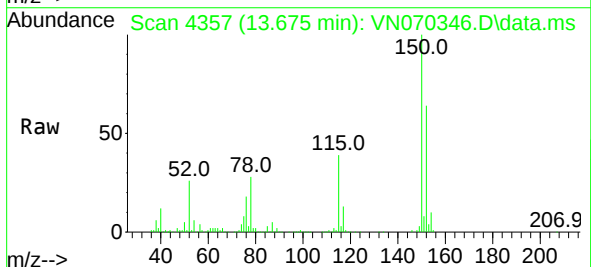






#74
N-amy1 acetate
Concen: 0.642 ug/l
RT: 12.390 min Scan# 3876
Delta R.T. 0.005 min
Lab File: VN070346.D
Acq: 29 Dec 2021 14:08

Instrument :
MSVOA_N
ClientSampleId :







Tgt Ion: 43	Resp: 12018
Ion Ratio	Lower Upper
43 100	
70 33.7	33.4 50.0
55 21.4	19.3 28.9
61 21.3	18.5 27.7



#75
1,1,2,2-Tetrachloroethane
Concen: 0.631 ug/l
RT: 12.825 min Scan# 4040
Delta R.T. -0.000 min
Lab File: VN070346.D
Acq: 29 Dec 2021 14:08


Tgt Ion: 83	Resp: 3006
Ion Ratio	Lower Upper
83 100	
131 1.8	5.5 16.5#
85 31.3	32.4 97.2#

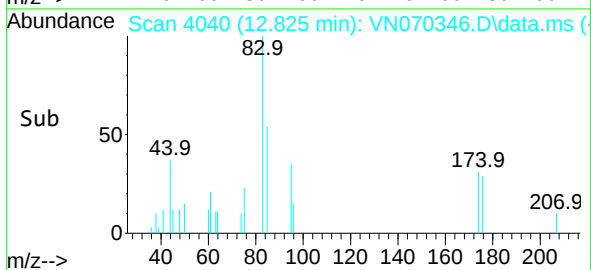



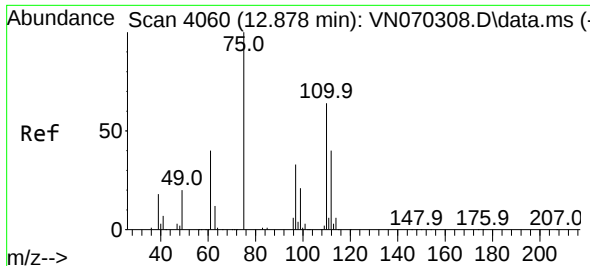


#76
1,2,3-Trichloropropane
Concen: 25.461 ug/l
RT: 12.731 min Scan# 4005
Delta R.T. -0.147 min
Lab File: VN070346.D
Acq: 29 Dec 2021 14:08

Instrument :
MSVOA_N
ClientSampleId :







Tgt Ion: 75 Resp: 340987
Ion Ratio Lower Upper
75 100
77 1.1 82.6 247.8#

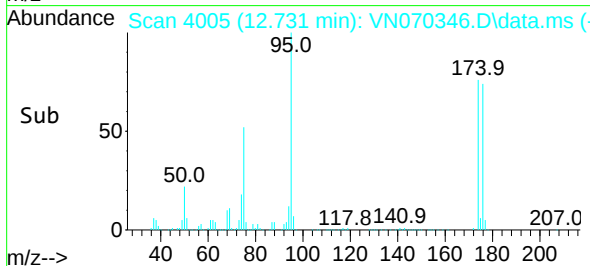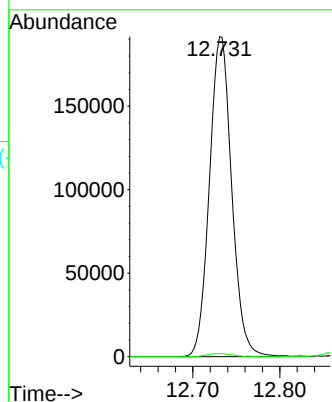

#81
trans-1,4-Dichloro-2-butene
Concen: 86.959 ug/l
RT: 12.731 min Scan# 4005
Delta R.T. 0.107 min
Lab File: VN070346.D
Acq: 29 Dec 2021 14:08

Tgt Ion: 75 Resp: 340987
Ion Ratio Lower Upper
75 100
53 0.2 90.5 135.7#
89 0.0 38.2 57.4#


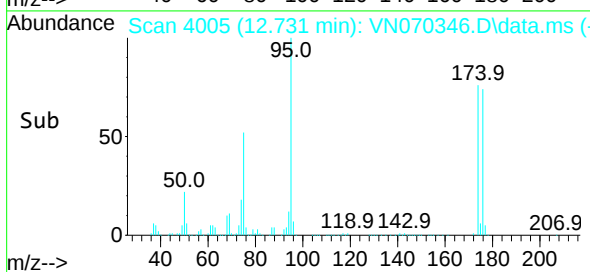
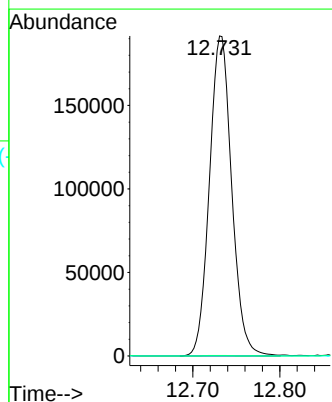
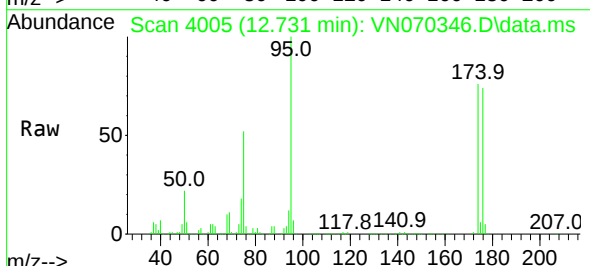


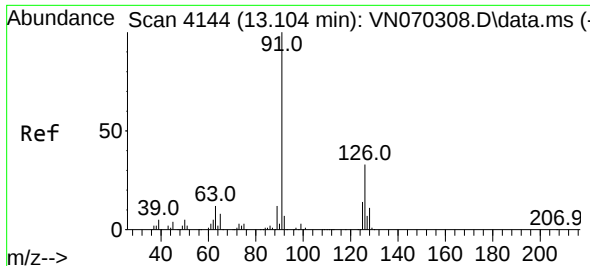

#82
4-Chlorotoluene
Concen: 0.265 ug/l
RT: 13.109 min Scan# 4144
Delta R.T. 0.005 min
Lab File: VN070346.D
Acq: 29 Dec 2021 14:08




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 91 Resp: 7844
Ion Ratio Lower Upper
91 100
126 31.3 18.2 54.6

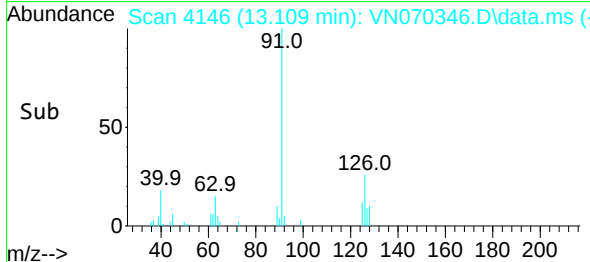

#84
1,2,4-Trimethylbenzene
Concen: 0.218 ug/l
RT: 13.369 min Scan# 4243
Delta R.T. 0.003 min
Lab File: VN070346.D
Acq: 29 Dec 2021 14:08


Tgt Ion: 105 Resp: 7474
Ion Ratio Lower Upper
105 100
120 40.3 22.8 68.4

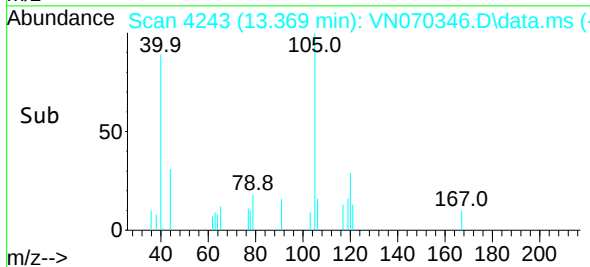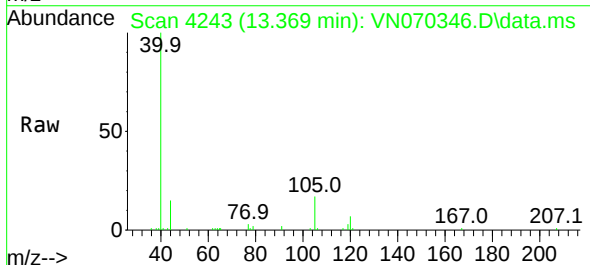



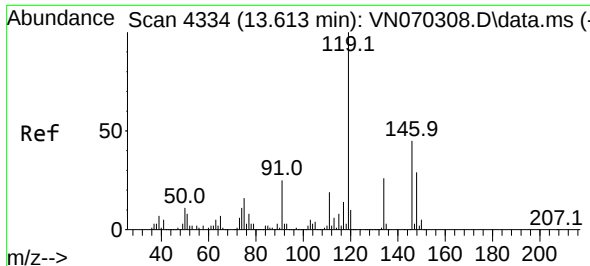


#87
 1,3-Dichlorobenzene
 Concen: 0.351 ug/l
 RT: 13.616 min Scan# 41
 Delta R.T. 0.003 min
 Lab File: VN070346.D
 Acq: 29 Dec 2021 14:08


Instrument :
 MSVOA_N
 ClientSampleId :





Tgt Ion:146 Resp: 6004
 Ion Ratio Lower Upper
 146 100
 111 42.8 18.6 55.6
 148 68.7 31.6 95.0

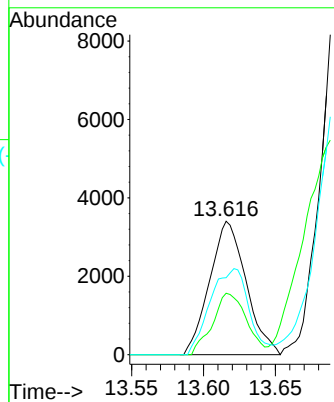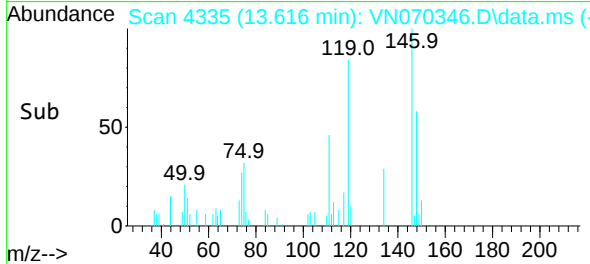


#88
 1,4-Dichlorobenzene
 Concen: 0.356 ug/l
 RT: 13.616 min Scan# 4335
 Delta R.T. -0.078 min
 Lab File: VN070346.D
 Acq: 29 Dec 2021 14:08

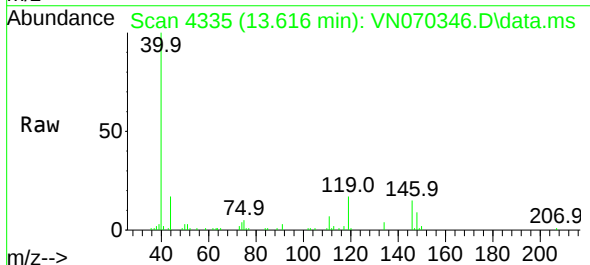

Tgt Ion:146 Resp: 6004
 Ion Ratio Lower Upper
 146 100
 111 42.8 18.3 54.8
 148 68.7 31.8 95.4



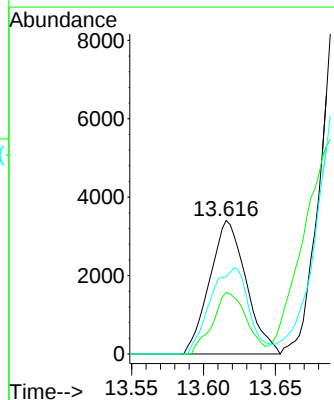
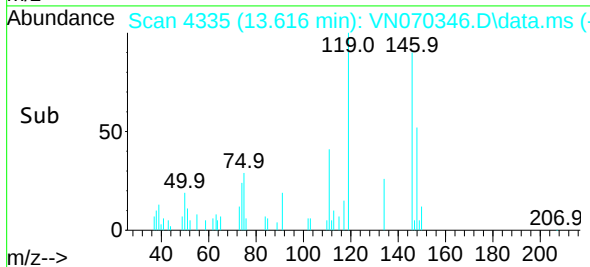


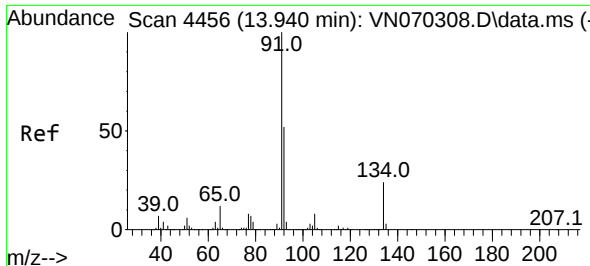

#89
n-Butylbenzene
Concen: 0.524 ug/l
RT: 13.946 min Scan# 4456
Delta R.T. 0.006 min
Lab File: VN070346.D
Acq: 29 Dec 2021 14:08




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 91 Resp: 14642
Ion Ratio Lower Upper
91 100
92 51.6 25.4 76.0
134 22.2 13.6 40.8

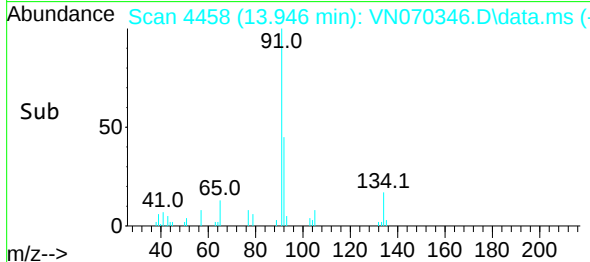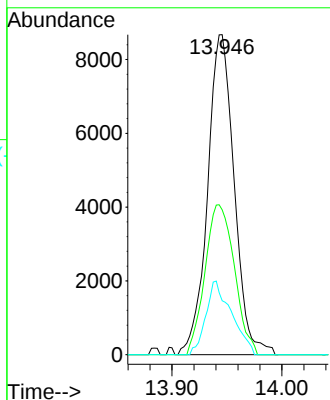

#91
1,2-Dichlorobenzene
Concen: 0.481 ug/l
RT: 13.989 min Scan# 4474
Delta R.T. 0.003 min
Lab File: VN070346.D
Acq: 29 Dec 2021 14:08

Tgt Ion: 146 Resp: 8063
Ion Ratio Lower Upper
146 100
111 41.8 19.1 57.3
148 63.9 32.1 96.3


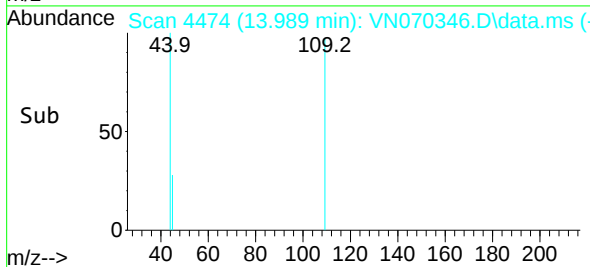
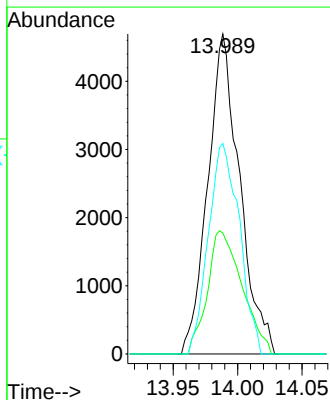
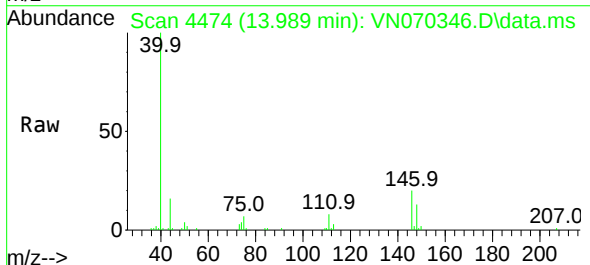




#92
1,2-Dibromo-3-Chloropropane
Concen: 0.966 ug/l
RT: 14.600 min Scan# 41
Delta R.T. 0.000 min
Lab File: VN070346.D
Acq: 29 Dec 2021 14:08




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 75 Resp: 2489
Ion Ratio Lower Upper
75 100
155 58.6 46.9 140.7
157 69.7 60.6 181.7

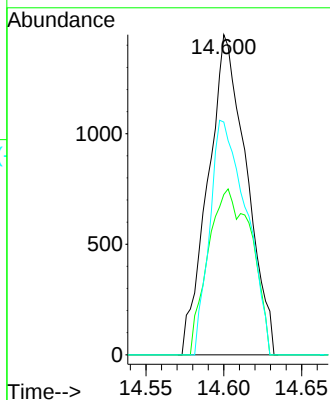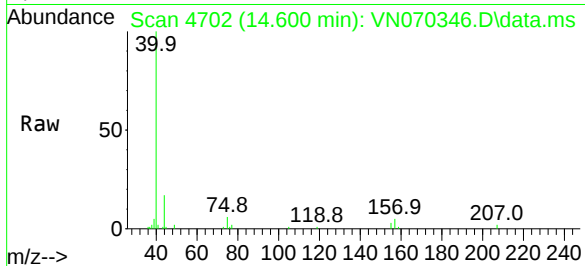

#93
1,2,4-Trichlorobenzene
Concen: 1.503 ug/l
RT: 15.262 min Scan# 4949
Delta R.T. -0.001 min
Lab File: VN070346.D
Acq: 29 Dec 2021 14:08

Tgt Ion: 180 Resp: 11870
Ion Ratio Lower Upper
180 100
182 89.0 48.3 144.9
145 32.7 14.5 43.5


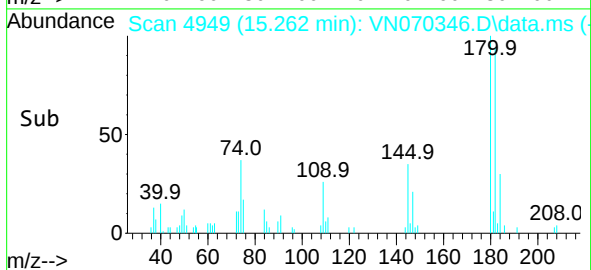
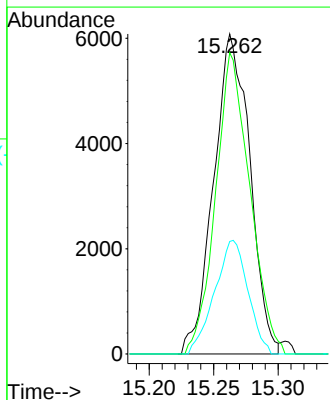
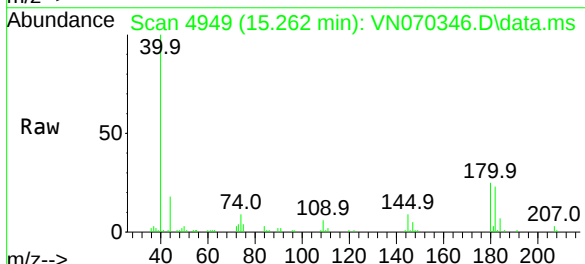




#94
Hexachlorobutadiene
Concen: 0.359 ug/l
RT: 15.372 min Scan# 4988
Delta R.T. 0.005 min
Lab File: VN070346.D
Acq: 29 Dec 2021 14:08




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion:225 Resp: 1646
Ion Ratio Lower Upper
225 100
223 69.7 31.9 95.7
227 72.1 32.1 96.3

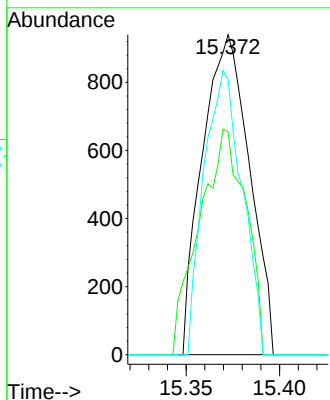

#95
Naphthalene
Concen: 3.891 ug/l
RT: 15.507 min Scan# 5040
Delta R.T. 0.003 min
Lab File: VN070346.D
Acq: 29 Dec 2021 14:08


Tgt Ion:128 Resp: 47404
Ion Ratio Lower Upper
128 100
127 12.8 10.5 15.7
129 10.8 8.7 13.1

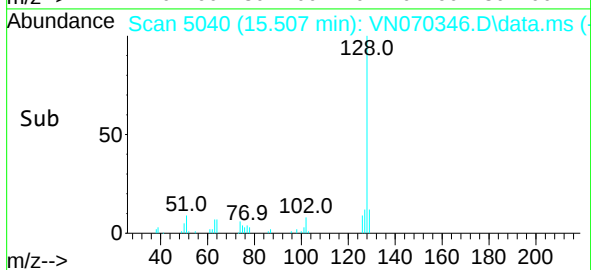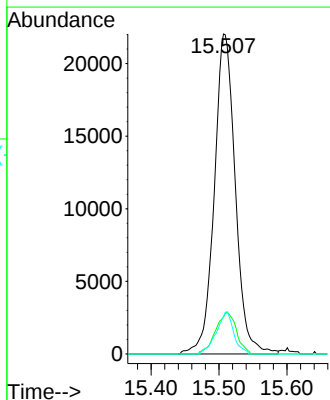



#96
 1,2,3-Trichlorobenzene
 Concen: 2.636 ug/l
 RT: 15.700 min Scan# 51
 Delta R.T. -0.000 min
 Lab File: VN070346.D
 Acq: 29 Dec 2021 14:08

Instrument :
 MSVOA_N
 ClientSampleId :

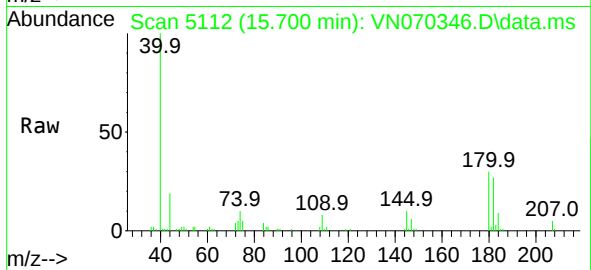

Tgt Ion:	180	Resp:	13906
Ion Ratio	Lower	Upper	
180	100		
182	97.1	47.4	142.2
145	31.8	15.0	45.1

