
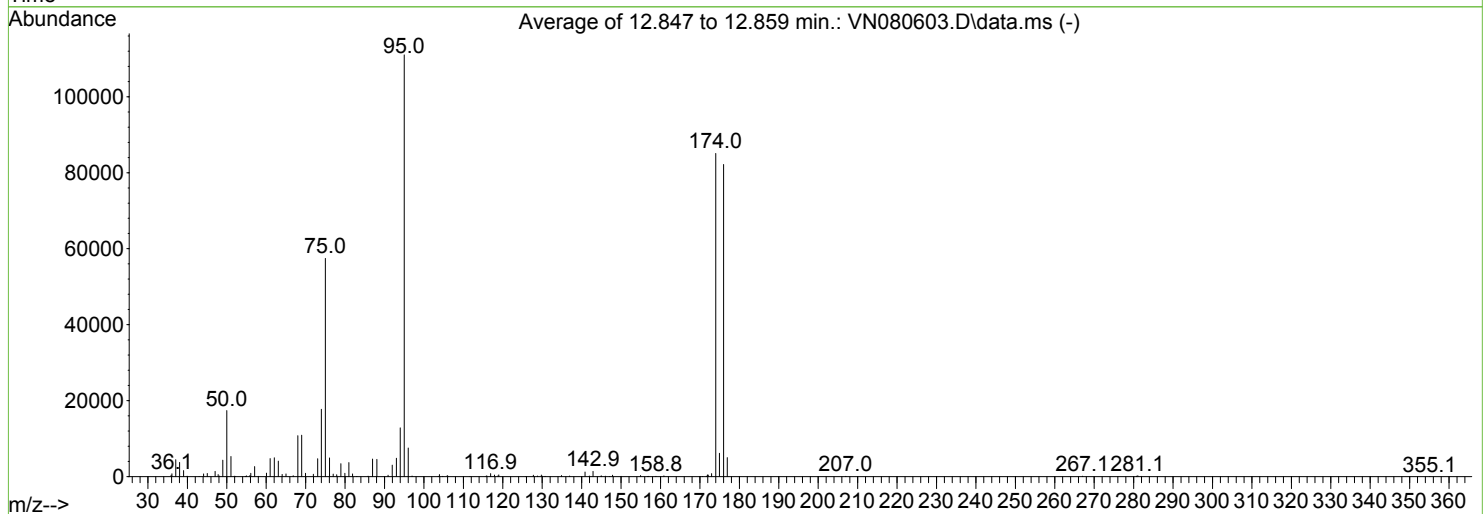


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN122923\
Data File : VN080603.D
Acq On : 29 Dec 2023 09:13
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N122723W.M
Title : SW846 8260
Last Update : Thu Dec 28 03:07:01 2023

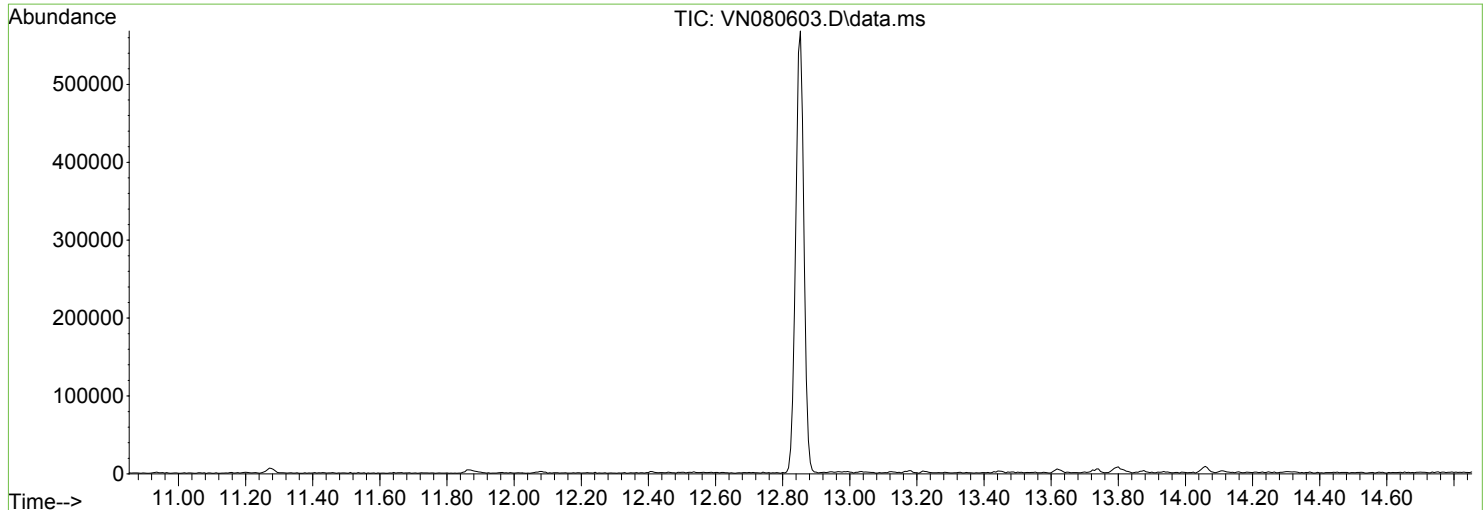

AutoFind: Scans 1852, 1853, 1854; Background Corrected with Scan 1843

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.7	17386	PASS
75	95	30	60	51.8	57459	PASS
95	95	100	100	100.0	111029	PASS
96	95	5	9	6.8	7538	PASS
173	174	0.00	2	1.0	822	PASS
174	95	50	100	76.6	85099	PASS
175	174	5	9	7.2	6148	PASS
176	174	95	101	96.5	82155	PASS
177	176	5	9	6.1	5029	PASS

Average of 12.847 to 12.859 min.: VN080603.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.90	368	48.10	164	58.00	103	71.95	621
36.10	765	49.00	4359	60.05	926	73.05	470
37.05	4469	50.00	17386	61.00	4755	74.00	1773
38.05	3765	51.05	5316	62.05	4957	75.00	5745
39.05	1590	51.90	115	63.05	4074	76.05	4941
39.95	123	52.10	106	64.05	575	77.00	669
43.00	60	54.70	88	65.00	706	77.90	526
44.10	708	55.00	229	66.85	265	78.95	3423
45.05	846	55.90	321	68.00	10781	79.95	892
47.05	1410	56.10	871	69.00	10908	80.95	3693
47.80	568	57.05	2657	69.95	905	81.90	725

Average of 12.847 to 12.859 min.: VN080603.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
83.00	56	103.60	92	119.00	483	142.90	1411
85.85	138	103.95	542	125.90	58	144.90	166
86.95	4632	104.80	98	127.75	369	145.05	182
88.05	4565	105.90	293	128.80	174	146.00	128
90.90	391	106.10	144	129.80	419	147.10	53
91.95	3020	111.70	51	130.10	110	147.85	395
93.00	4867	115.80	121	130.70	71	150.00	85
94.00	12837	115.95	231	134.90	316	154.95	293
95.00	111029	116.90	800	136.95	158	156.70	61
96.00	7538	117.90	406	140.85	1240	157.00	75
97.00	184	118.80	221	141.95	182	158.85	104

Average of 12.847 to 12.859 min.: VN080603.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
160.85	209	207.00	89				
170.00	51	267.05	128				
170.70	59	280.75	120				
171.60	135	281.05	254				
171.90	459	281.90	71				
172.10	440	355.10	52				
172.95	822						
174.00	85099						
174.95	6148						
176.00	82155						
176.95	5029						