


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN123020\
Data File : VN065310.D
Acq On : 30 Dec 2020 10:37
Operator : JC/MD
Sample : BFB
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N122220W.M
Title : Sw846 8260
Last Update : Tue Dec 22 15:42:18 2020

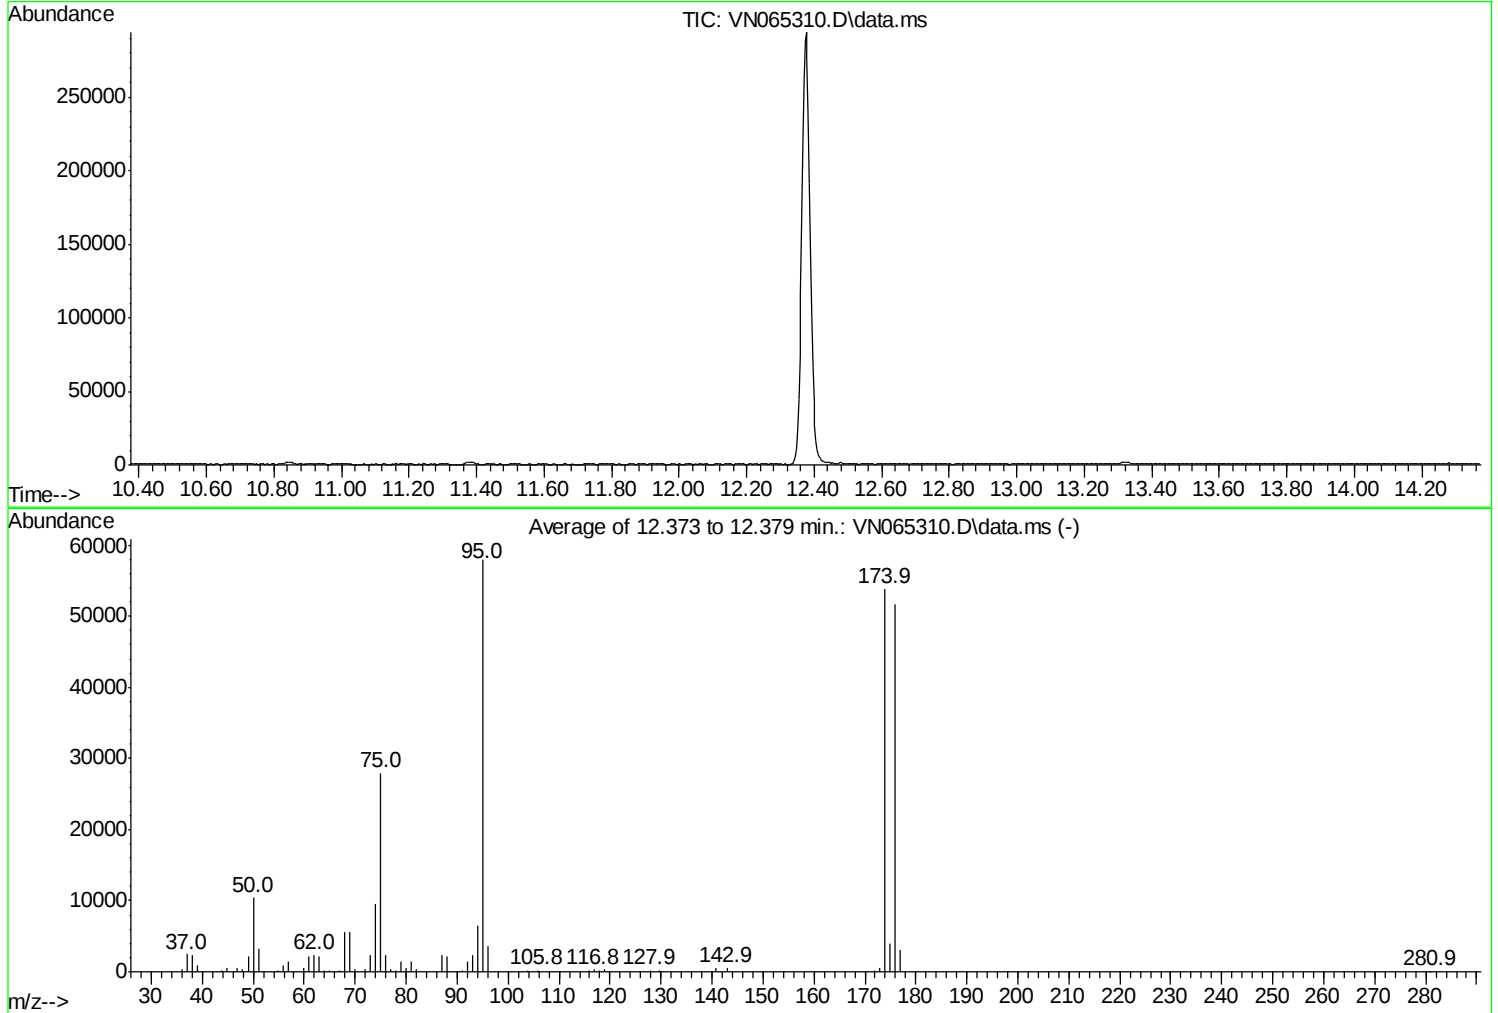

AutoFind: Scans 3307, 3308, 3309; Background Corrected with Scan 3293

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	17.9	10390	PASS
75	95	30	60	48.2	27907	PASS
95	95	100	100	100.0	57933	PASS
96	95	5	9	6.4	3692	PASS
173	174	0.00	2	1.0	555	PASS
174	95	50	100	93.0	53867	PASS
175	174	5	9	7.4	3972	PASS
176	174	95	101	96.1	51741	PASS
177	176	5	9	6.0	3126	PASS