

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN123021\
 Data File : VN070416.D
 Acq On : 30 Dec 2021 23:39
 Operator : JC/MD
 Sample : VN1230MBL02
 Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_N/MEOH
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 VN1230MBL02

Quant Time: Dec 31 05:26:33 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N122721W.M
 Quant Title : SW846 8260
 QLast Update : Mon Dec 27 18:47:12 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	8.086	168	910081	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.971	114	1563648	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.747	117	1439485	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.678	152	449119	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.440	65	668727	51.105	ug/l	0.00
Spiked Amount 50.000	Range 61 - 141		Recovery = 102.220%			
35) Dibromofluoromethane	8.024	113	485862	51.355	ug/l	0.00
Spiked Amount 50.000	Range 69 - 133		Recovery = 102.700%			
50) Toluene-d8	10.443	98	1839676	47.600	ug/l	0.00
Spiked Amount 50.000	Range 65 - 126		Recovery = 95.200%			
62) 4-Bromofluorobenzene	12.734	95	637854	45.695	ug/l	0.00
Spiked Amount 50.000	Range 58 - 135		Recovery = 91.380%			
Target Compounds						Qvalue
3) Chloromethane	2.306	50	4272	0.304	ug/l	89
11) Tert butyl alcohol	5.315	59	4868	2.234	ug/l #	71
13) Acrolein	4.039	56	779	0.441	ug/l #	51
16) Acetone	4.291	43	3940	0.464	ug/l	90
17) Carbon Disulfide	4.524	76	7643	0.302	ug/l #	74
18) Methyl Acetate	4.862	43	5325	0.217	ug/l #	81
20) Methylene Chloride	5.087	84	3173	0.270	ug/l	89
25) 2-Butanone	7.346	43	4452	0.416	ug/l	90
31) Cyclohexane	8.088	56	22445	1.087	ug/l #	35
36) 1,1-Dichloropropene	8.086	75	73864	4.720	ug/l #	49
38) Carbon Tetrachloride	8.086	117	90446	6.052	ug/l #	16
49) 1,4-Dioxane	9.572	88	148	0.663	ug/l #	1
51) 4-Methyl-2-Pentanone	10.331	43	7958	0.396	ug/l	88
58) 2-Chloroethyl Vinyl ether	10.038	63	269	18.564	ug/l #	45
59) 2-Hexanone	11.090	43	13132	0.896	ug/l	87
74) N-amyl acetate	12.393	43	6704	0.382	ug/l #	89
75) 1,1,2,2-Tetrachloroethane	12.836	83	1928	0.573	ug/l #	91
76) 1,2,3-Trichloropropane	12.734	75	338065	26.769	ug/l #	1
77) Bromobenzene	12.865	156	1925	0.201	ug/l	76
81) trans-1,4-Dichloro-2-b...	12.734	75	338065	91.966	ug/l #	5
87) 1,3-Dichlorobenzene	13.619	146	4721	0.295	ug/l	93
88) 1,4-Dichlorobenzene	13.619	146	4721	0.299	ug/l	93
89) n-Butylbenzene	13.943	91	8641	0.330	ug/l	94
91) 1,2-Dichlorobenzene	13.986	146	4424	0.282	ug/l	94
92) 1,2-Dibromo-3-Chloropr...	14.606	75	1084	0.449	ug/l	76
93) 1,2,4-Trichlorobenzene	15.268	180	6380	0.862	ug/l	95
94) Hexachlorobutadiene	15.367	225	1166	0.271	ug/l	69
95) Naphthalene	15.507	128	29652	3.194	ug/l	99
96) 1,2,3-Trichlorobenzene	15.703	180	7856	1.917	ug/l	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN123021\
Data File : VN070416.D
Acq On : 30 Dec 2021 23:39
Operator : JC/MD
Sample : VN1230MBL02
Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_N/MEOH
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
VN1230MBL02

Quant Time: Dec 31 05:26:33 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N122721W.M
Quant Title : SW846 8260
QLast Update : Mon Dec 27 18:47:12 2021
Response via : Initial Calibration




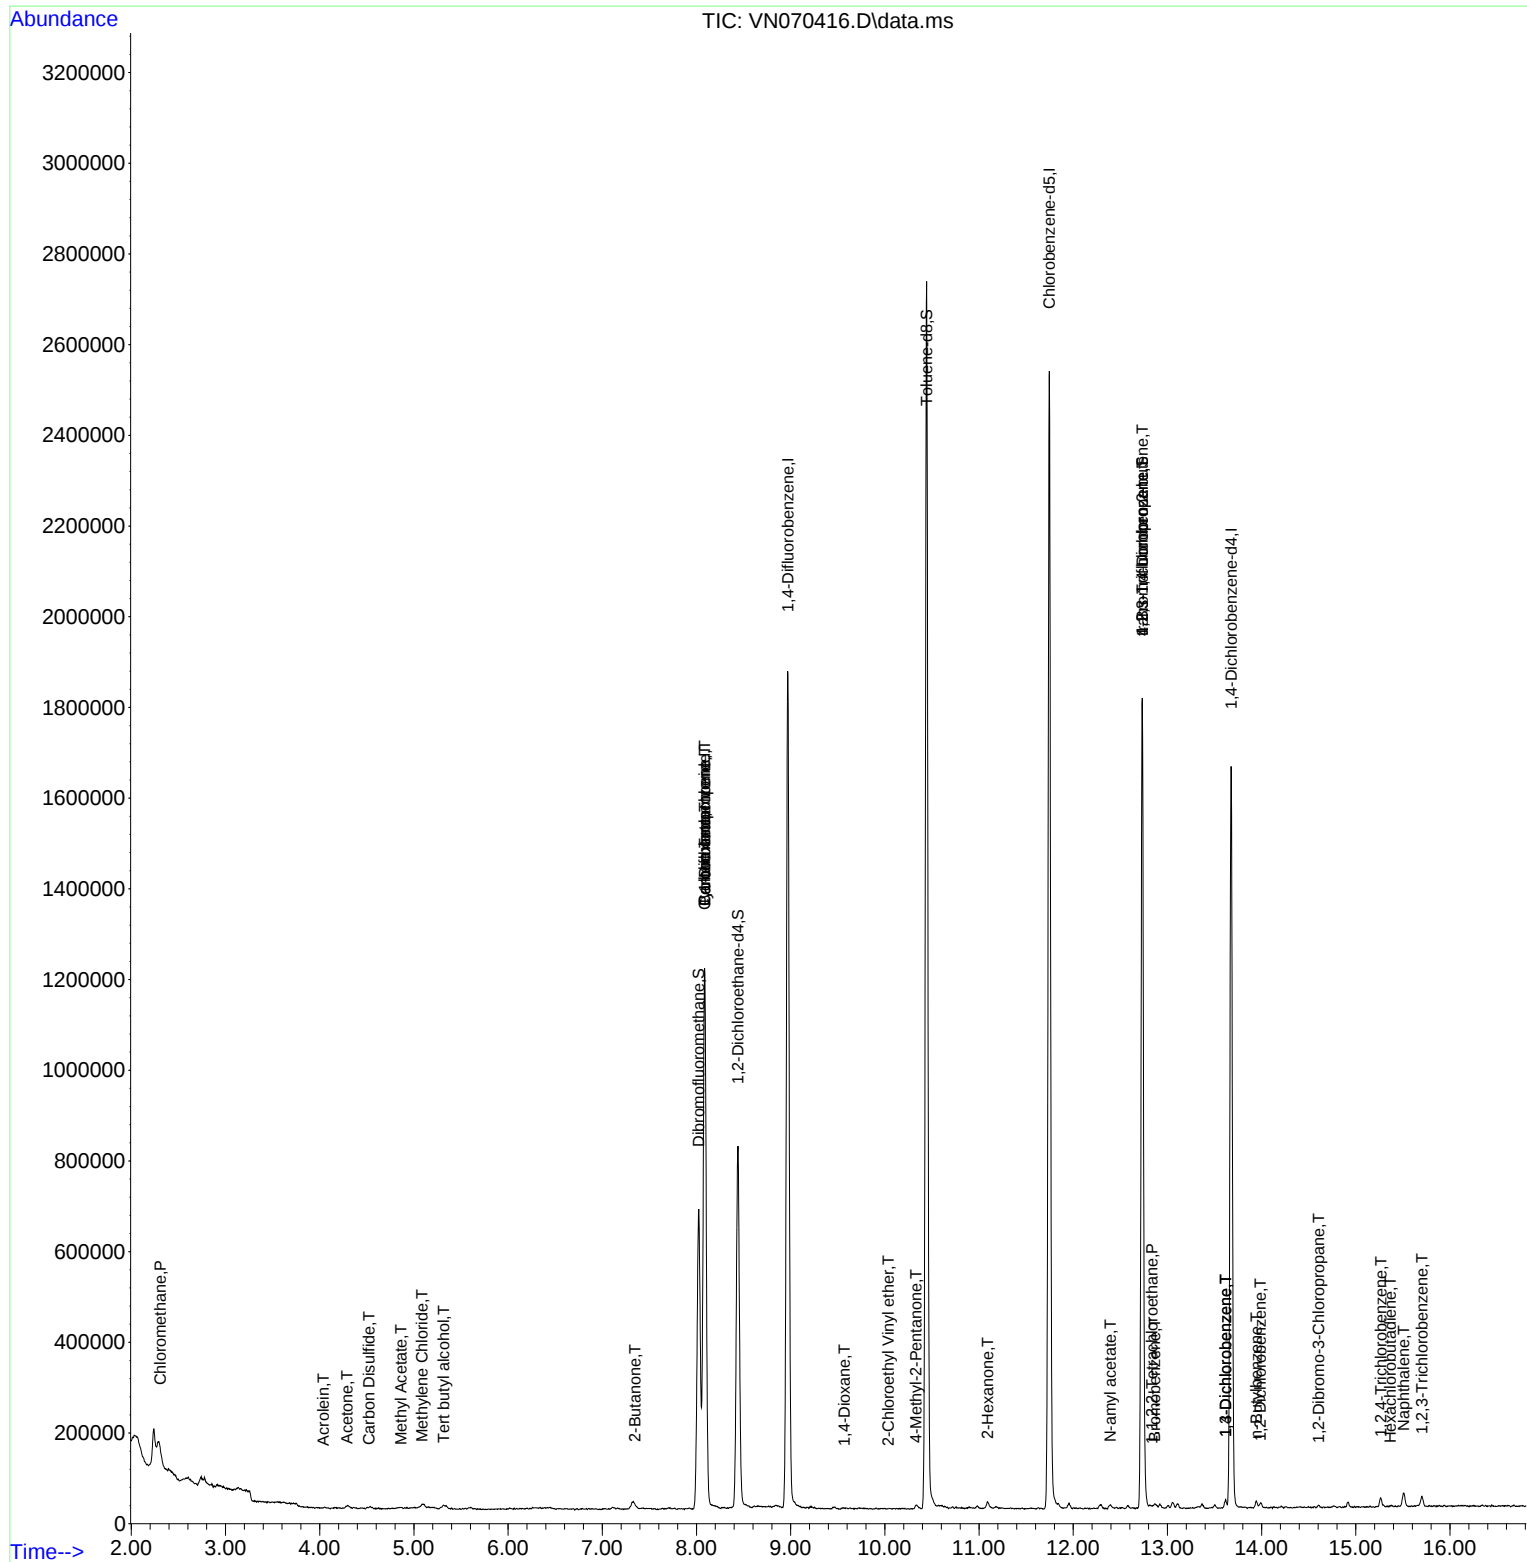




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.086 min Scan# 21
Delta R.T. -0.000 min
Lab File: VN070416.D
Acq: 30 Dec 2021 23:39




Instrument :
MSVOA_N
ClientSampleId :
VN1230MBL02


Tgt Ion:168 Resp: 910081
Ion Ratio Lower Upper
168 100
99 57.9 41.3 61.9

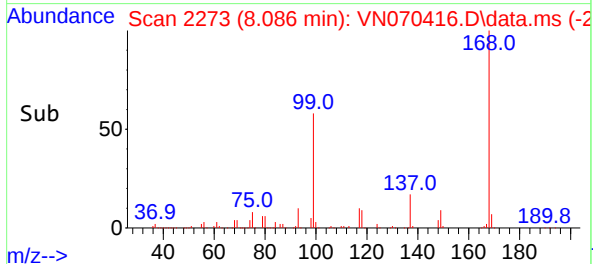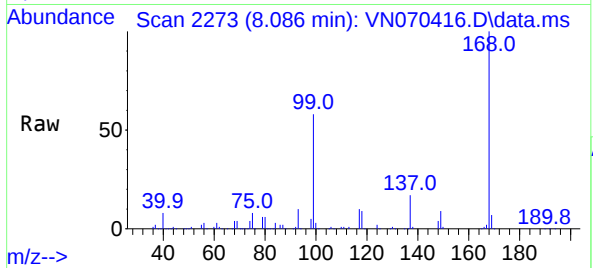

#3
Chloromethane
Concen: 0.304 ug/l
RT: 2.306 min Scan# 118
Delta R.T. 0.003 min
Lab File: VN070416.D
Acq: 30 Dec 2021 23:39

Tgt Ion: 50 Resp: 4272
Ion Ratio Lower Upper
50 100
52 37.9 25.4 38.0


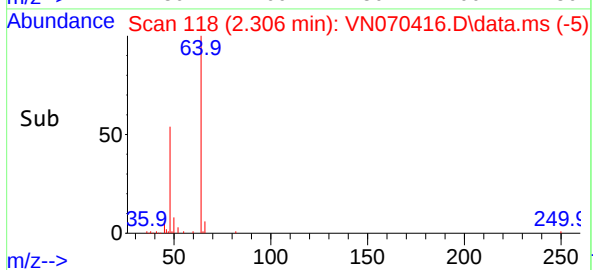

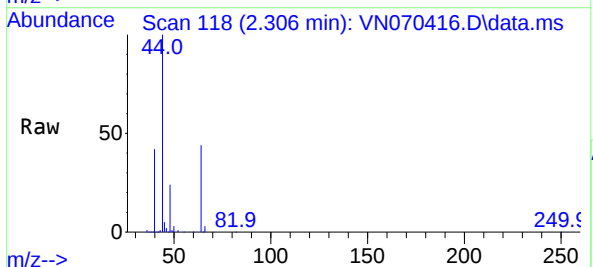


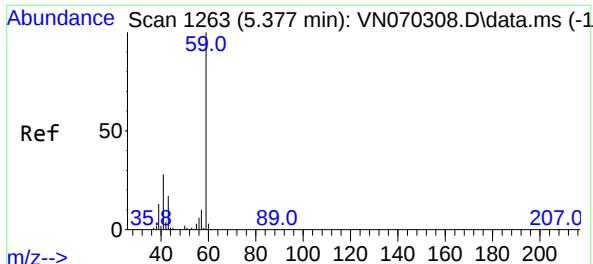

#11
Tert butyl alcohol
Concen: 2.234 ug/l
RT: 5.315 min Scan# 11
Delta R.T. -0.062 min
Lab File: VN070416.D
Acq: 30 Dec 2021 23:39




Instrument :
MSVOA_N
ClientSampleId :
VN1230MBL02


Tgt Ion: 59 Resp: 4868
Ion Ratio Lower Upper
59 100
57 0.0 8.7 13.1#

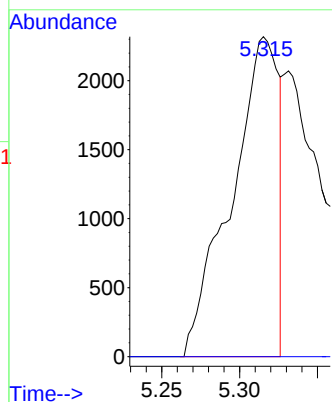

#13
Acrolein
Concen: 0.441 ug/l
RT: 4.039 min Scan# 764
Delta R.T. -0.002 min
Lab File: VN070416.D
Acq: 30 Dec 2021 23:39

Tgt Ion: 56 Resp: 779
Ion Ratio Lower Upper
56 100
55 30.0 56.6 85.0#


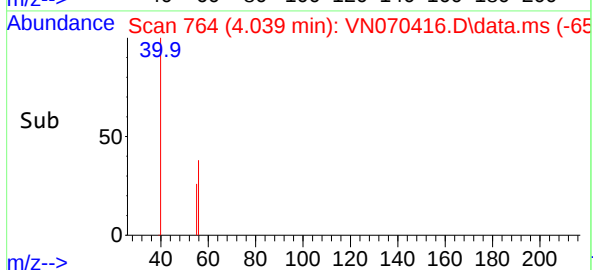

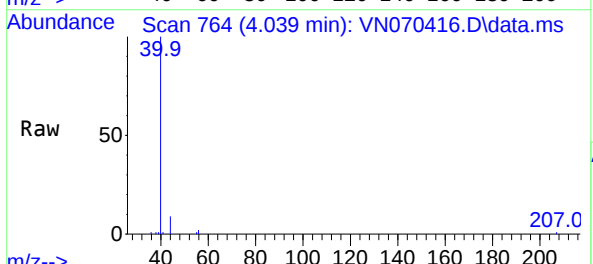




#16
Acetone
Concen: 0.464 ug/l
RT: 4.291 min Scan# 856
Delta R.T. 0.006 min
Lab File: VN070416.D
Acq: 30 Dec 2021 23:39




Instrument :
MSVOA_N
ClientSampleId :
VN1230MBL02


Tgt Ion: 43 Resp: 3940
Ion Ratio Lower Upper
43 100
58 23.5 23.1 34.7

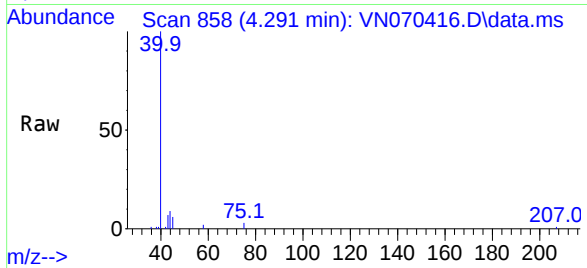

#17
Carbon Disulfide
Concen: 0.302 ug/l
RT: 4.524 min Scan# 945
Delta R.T. -0.005 min
Lab File: VN070416.D
Acq: 30 Dec 2021 23:39

Tgt Ion: 76 Resp: 7643
Ion Ratio Lower Upper
76 100
78 0.0 7.5 11.3#

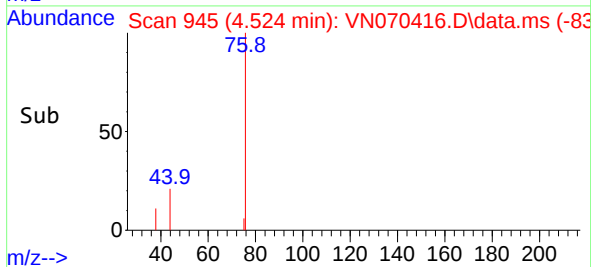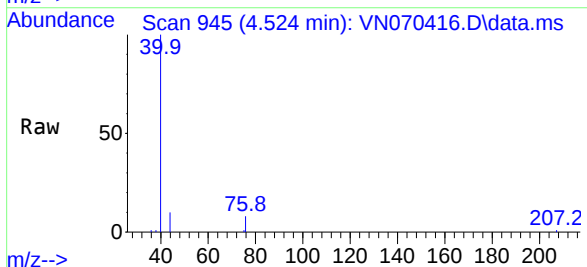



#18

Methyl Acetate

Concen: 0.217 ug/l

RT: 4.862 min Scan# 110

Delta R.T. 0.008 min

Lab File: VN070416.D

Acq: 30 Dec 2021 23:39

Instrument :

MSVOA_N

ClientSampleId :





VN1230MBL02

Tgt Ion: 43 Resp: 5325

Ion Ratio Lower Upper

43 100

74 15.0 19.4 29.2#

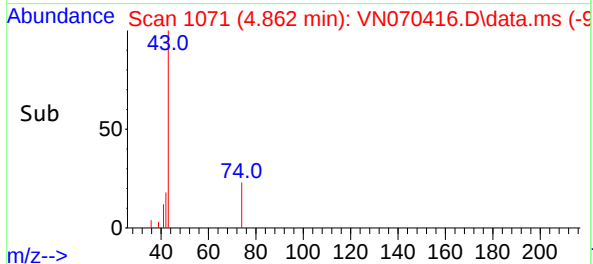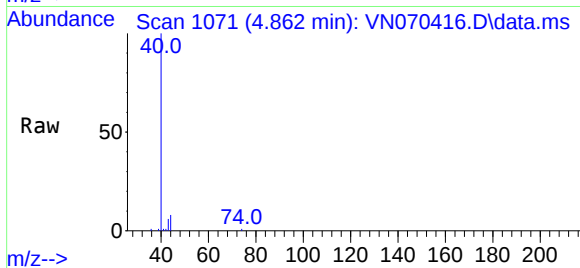

#20

Methylene Chloride

Concen: 0.270 ug/l

RT: 5.087 min Scan# 1155

Delta R.T. -0.008 min

Lab File: VN070416.D

Acq: 30 Dec 2021 23:39

Tgt Ion: 84 Resp: 3173




Ion Ratio Lower Upper


84 100

49 131.9 93.5 140.3

51 38.3 29.4 44.2

86 57.7 53.0 79.4


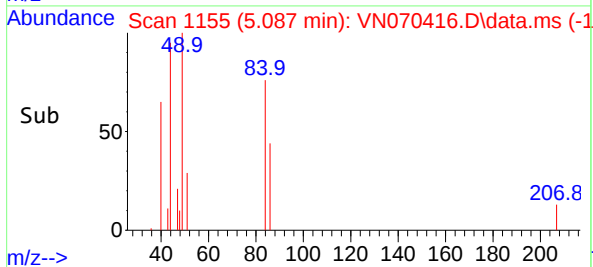

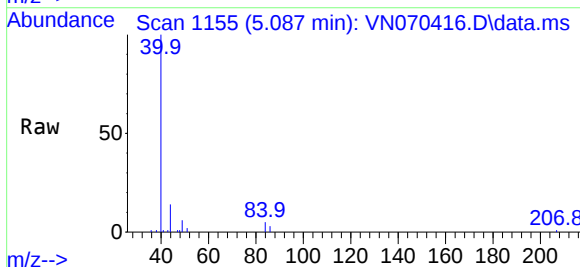




#25
2-Butanone
Concen: 0.416 ug/l
RT: 7.346 min Scan# 1997
Delta R.T. 0.011 min
Lab File: VN070416.D
Acq: 30 Dec 2021 23:39




Instrument :
MSVOA_N
ClientSampleId :
VN1230MBL02


Tgt Ion: 43 Resp: 4452
Ion Ratio Lower Upper
43 100
72 21.9 21.7 32.5

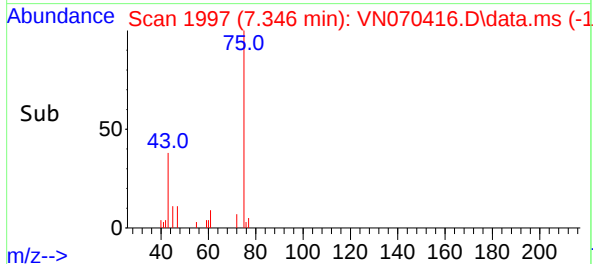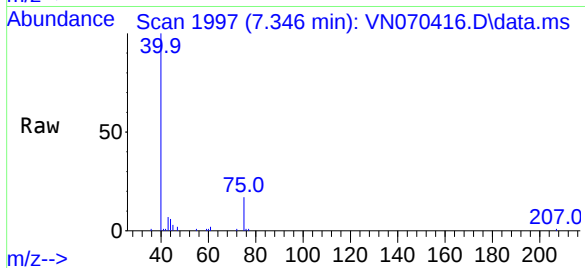

#31
Cyclohexane
Concen: 1.087 ug/l
RT: 8.088 min Scan# 2274
Delta R.T. -0.006 min
Lab File: VN070416.D
Acq: 30 Dec 2021 23:39

Tgt Ion: 56 Resp: 22445
Ion Ratio Lower Upper
56 100
69 146.6 27.1 40.7#
84 106.5 73.4 110.0

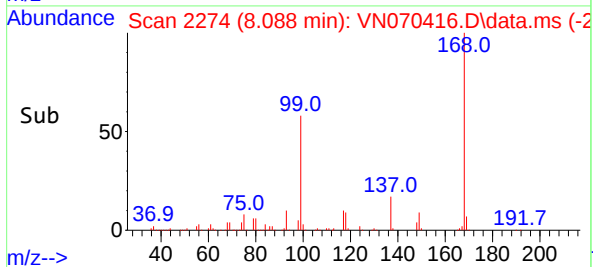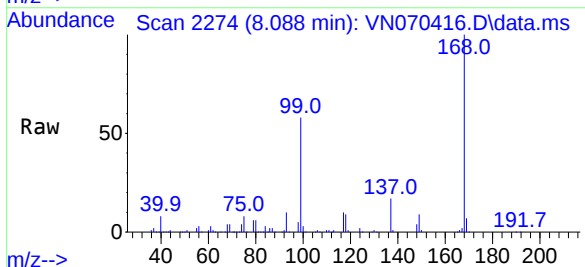



#33

1,2-Dichloroethane-d4

Concen: 51.105 ug/l

RT: 8.440 min Scan# 24

Delta R.T. 0.003 min

Lab File: VN070416.D

Acq: 30 Dec 2021 23:39

Instrument :

MSVOA_N

ClientSampleId :





VN1230MBL02

Tgt Ion: 65 Resp: 668727

Ion Ratio Lower Upper

65 100

67 52.5 0.0 103.0

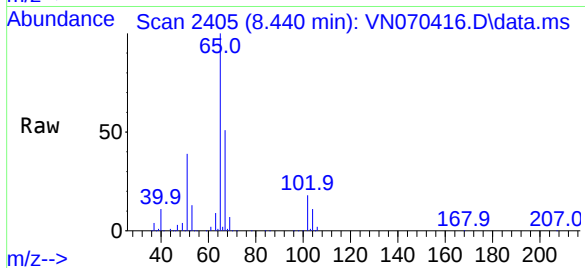

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.971 min Scan# 2603

Delta R.T. 0.003 min

Lab File: VN070416.D

Acq: 30 Dec 2021 23:39




Tgt Ion:114 Resp: 1563648


Ion Ratio Lower Upper

114 100

63 23.5 0.0 37.8

88 16.3 0.0 27.4


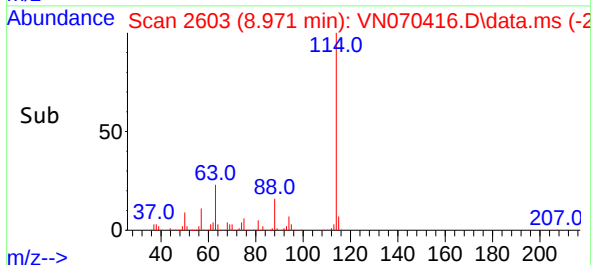
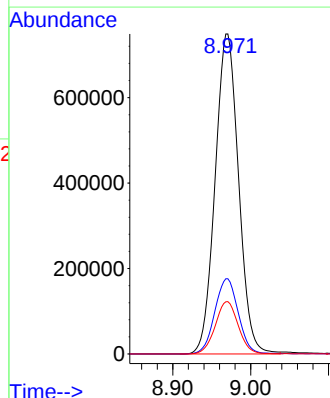
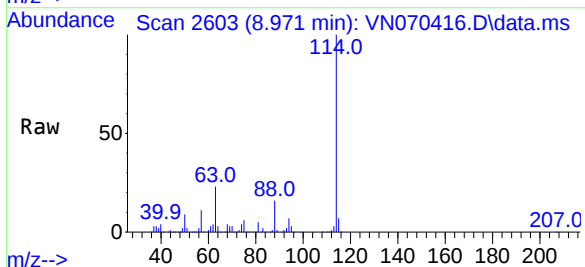




#35
Dibromofluoromethane
Concen: 51.355 ug/l
RT: 8.024 min Scan# 211
Delta R.T. 0.003 min
Lab File: VN070416.D
Acq: 30 Dec 2021 23:39




Instrument :
MSVOA_N
ClientSampleId :
VN1230MBL02


Tgt Ion:113 Resp: 485862
Ion Ratio Lower Upper
113 100
111 103.4 82.2 123.2
192 19.6 16.9 25.3

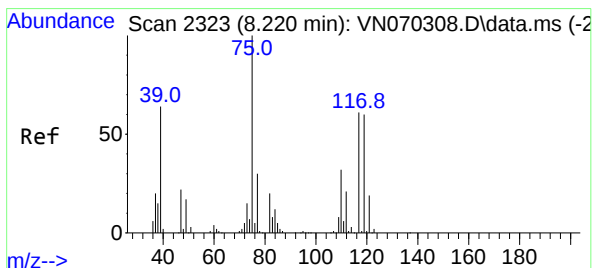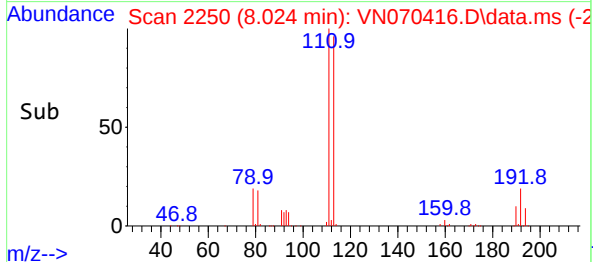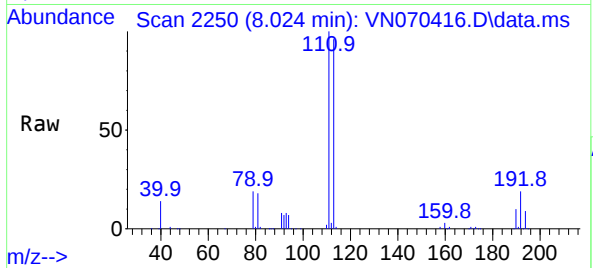

#36
1,1-Dichloropropene
Concen: 4.720 ug/l
RT: 8.086 min Scan# 2273
Delta R.T. -0.134 min
Lab File: VN070416.D
Acq: 30 Dec 2021 23:39

Tgt Ion: 75 Resp: 73864
Ion Ratio Lower Upper
75 100
110 8.6 18.4 55.2#
77 0.0 24.4 36.6#


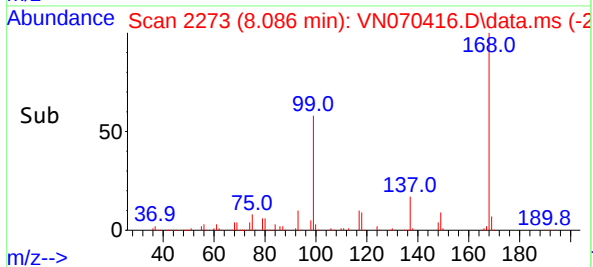

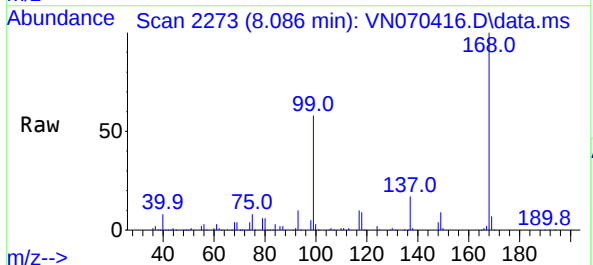




#38
Carbon Tetrachloride
Concen: 6.052 ug/l
RT: 8.086 min Scan# 21
Delta R.T. -0.120 min
Lab File: VN070416.D
Acq: 30 Dec 2021 23:39




Instrument :
MSVOA_N
ClientSampleId :
VN1230MBL02


Tgt Ion:117 Resp: 90446
Ion Ratio Lower Upper
117 100
119 4.9 76.1 114.1#
121 0.0 24.2 36.2#

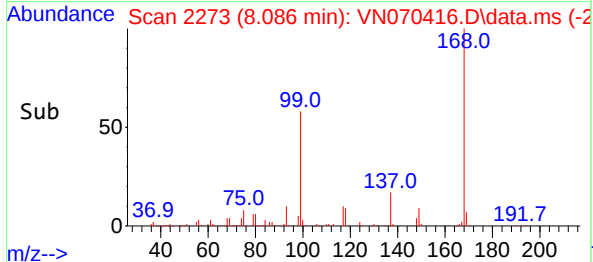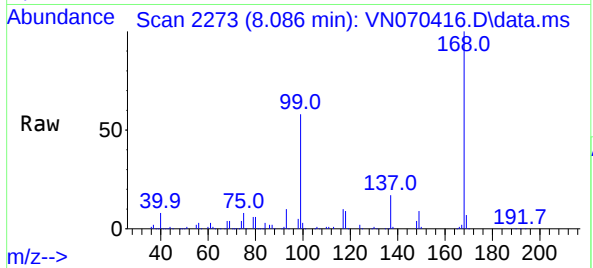

#49
1,4-Dioxane
Concen: 0.663 ug/l
RT: 9.572 min Scan# 2827
Delta R.T. 0.003 min
Lab File: VN070416.D
Acq: 30 Dec 2021 23:39

Tgt Ion: 88 Resp: 148
Ion Ratio Lower Upper
88 100
43 164.2 23.4 35.2#
58 0.0 50.6 75.8#


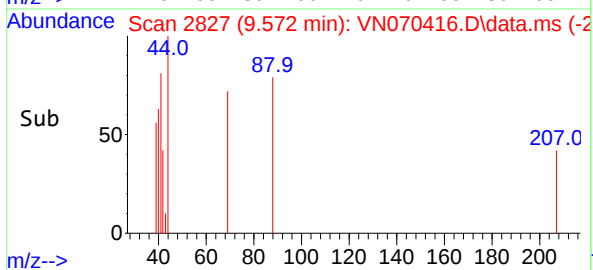

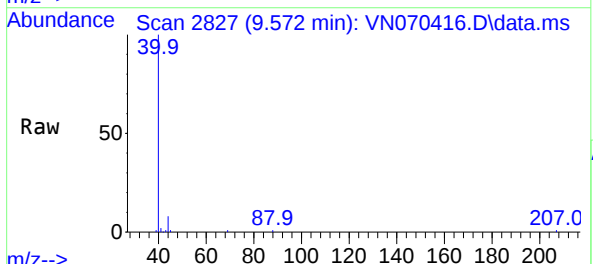




#50
Toluene-d8
Concen: 47.600 ug/l
RT: 10.443 min Scan# 3151
Delta R.T. 0.003 min
Lab File: VN070416.D
Acq: 30 Dec 2021 23:39




Instrument :
MSVOA_N
ClientSampleId :
VN1230MBL02


Tgt Ion: 98 Resp: 1839676
Ion Ratio Lower Upper
98 100
100 64.1 50.4 75.6

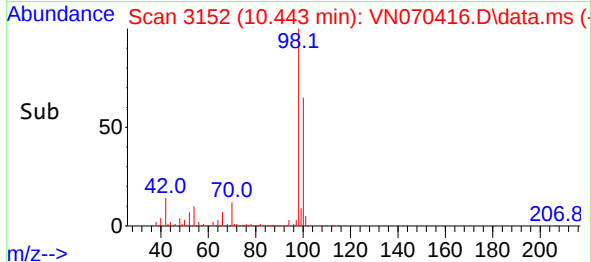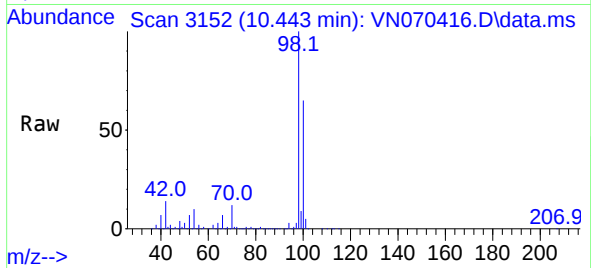

#51
4-Methyl-2-Pentanone
Concen: 0.396 ug/l
RT: 10.331 min Scan# 3110
Delta R.T. 0.001 min
Lab File: VN070416.D
Acq: 30 Dec 2021 23:39

Tgt Ion: 43 Resp: 7958
Ion Ratio Lower Upper
43 100
58 30.9 30.4 45.6


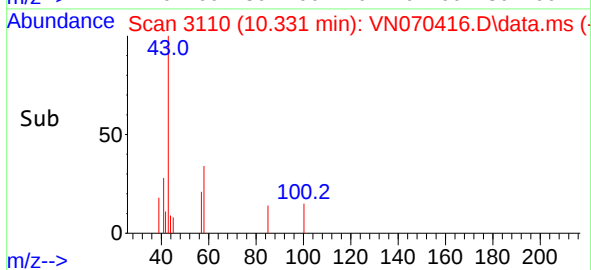






#58
2-Chloroethyl Vinyl ether
Concen: 18.564 ug/l
RT: 10.038 min Scan# 3002
Delta R.T. -0.003 min
Lab File: VN070416.D
Acq: 30 Dec 2021 23:39




Instrument :
MSVOA_N
ClientSampleId :
VN1230MBL02


Tgt Ion: 63 Resp: 269
Ion Ratio Lower Upper
63 100
106 0.0 23.9 35.9#

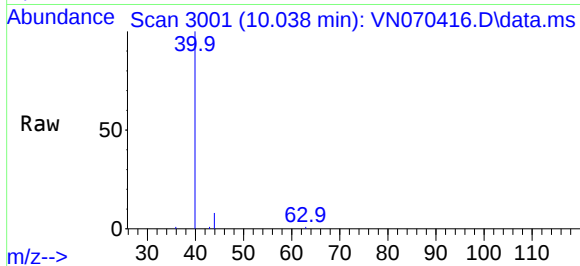

#59
2-Hexanone
Concen: 0.896 ug/l
RT: 11.090 min Scan# 3393
Delta R.T. 0.006 min
Lab File: VN070416.D
Acq: 30 Dec 2021 23:39

Tgt Ion: 43 Resp: 13132
Ion Ratio Lower Upper
43 100
58 44.2 26.9 80.7


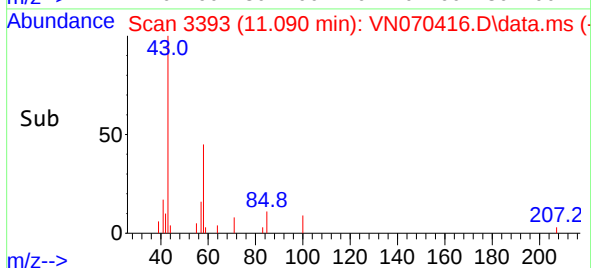
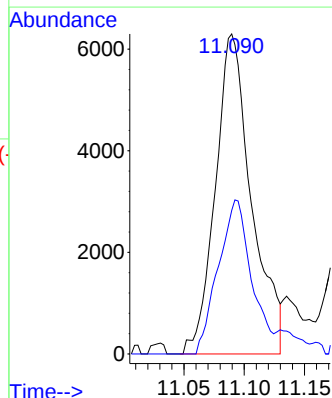
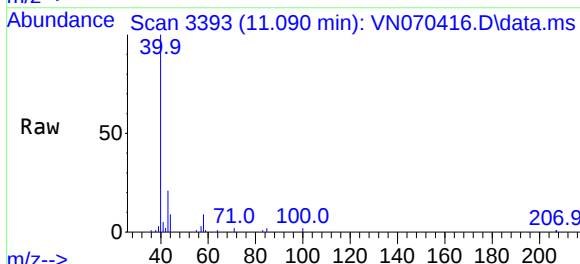




#62
4-Bromofluorobenzene
Concen: 45.695 ug/l
RT: 12.734 min Scan# 4005
Delta R.T. 0.003 min
Lab File: VN070416.D
Acq: 30 Dec 2021 23:39




Instrument :
MSVOA_N
ClientSampleId :
VN1230MBL02


Tgt Ion: 95 Resp: 637854
Ion Ratio Lower Upper
95 100
174 78.3 0.0 187.2
176 74.0 0.0 181.4



#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.747 min Scan# 3638
Delta R.T. 0.003 min
Lab File: VN070416.D
Acq: 30 Dec 2021 23:39

Tgt Ion: 117 Resp: 1439485
Ion Ratio Lower Upper
117 100
82 59.2 42.4 63.6
119 32.5 25.4 38.2


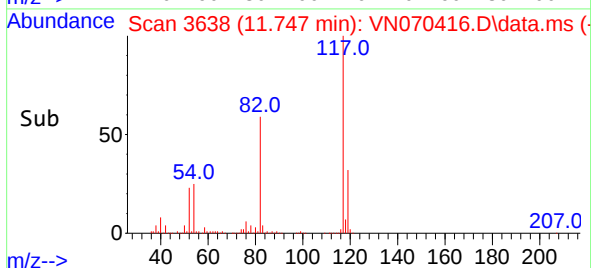
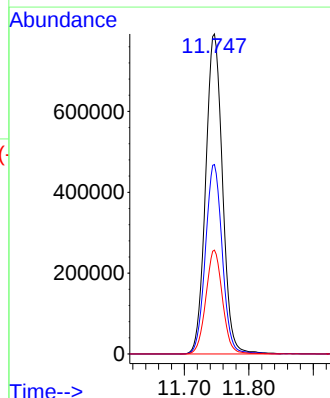





#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.678 min Scan# 41
Delta R.T. 0.006 min
Lab File: VN070416.D
Acq: 30 Dec 2021 23:39




Instrument :
MSVOA_N
ClientSampleId :
VN1230MBL02


Tgt Ion:152 Resp: 449119
Ion Ratio Lower Upper
152 100
115 60.0 27.5 82.5
150 157.9 0.0 344.4

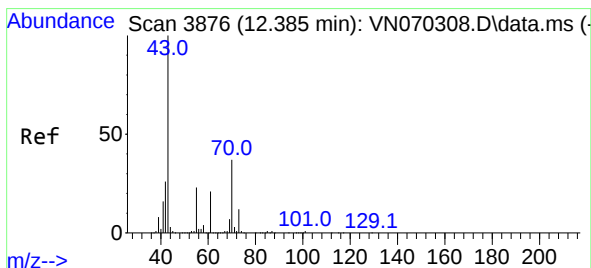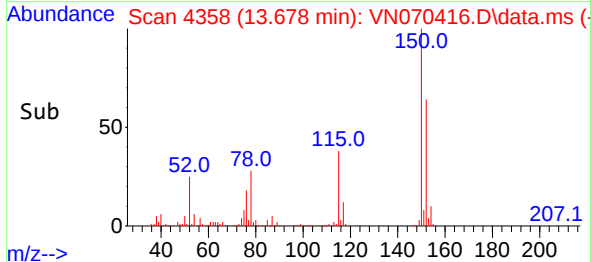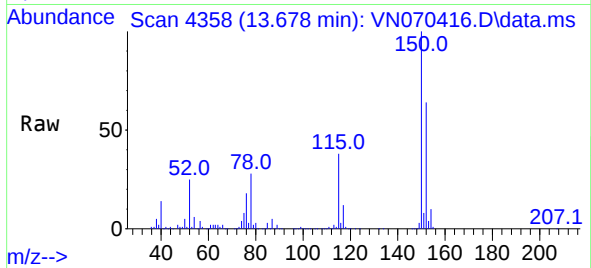

#74
N-ethyl acetate
Concen: 0.382 ug/l
RT: 12.393 min Scan# 3879
Delta R.T. 0.008 min
Lab File: VN070416.D
Acq: 30 Dec 2021 23:39

Tgt Ion: 43 Resp: 6704
Ion Ratio Lower Upper
43 100
70 28.7 33.4 50.0#
55 23.1 19.3 28.9
61 23.8 18.5 27.7


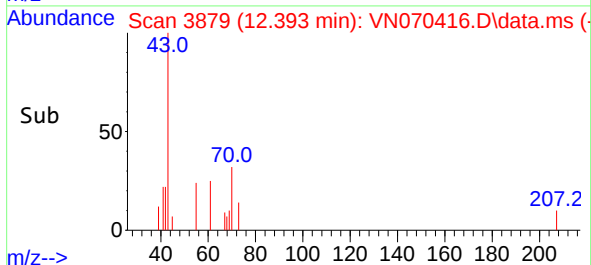
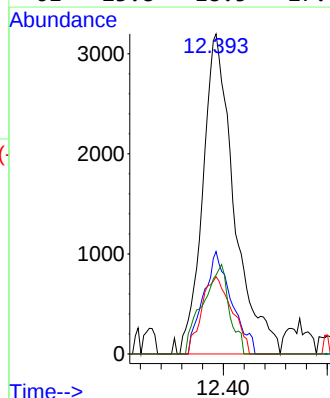
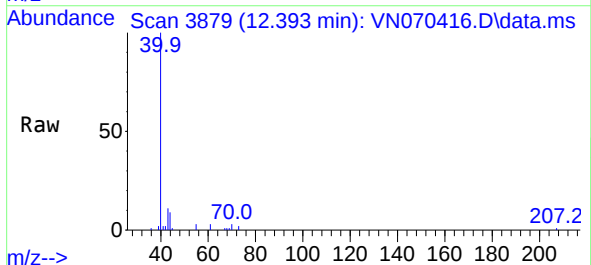




#75
1,1,2,2-Tetrachloroethane
Concen: 0.573 ug/l
RT: 12.836 min Scan# 4040
Delta R.T. 0.011 min
Lab File: VN070416.D
Acq: 30 Dec 2021 23:39




Instrument :
MSVOA_N
ClientSampleId :
VN1230MBL02


Tgt Ion: 83 Resp: 1928
Ion Ratio Lower Upper
83 100
131 0.0 5.5 16.5#
85 68.8 32.4 97.2

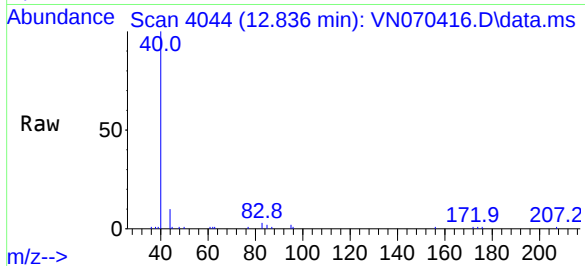

#76
1,2,3-Trichloropropane
Concen: 26.769 ug/l
RT: 12.734 min Scan# 4006
Delta R.T. -0.144 min
Lab File: VN070416.D
Acq: 30 Dec 2021 23:39

Tgt Ion: 75 Resp: 338065
Ion Ratio Lower Upper
75 100
77 1.2 82.6 247.8#


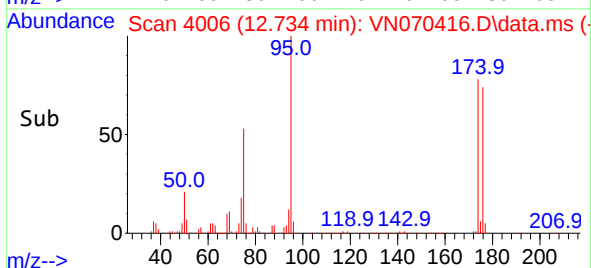
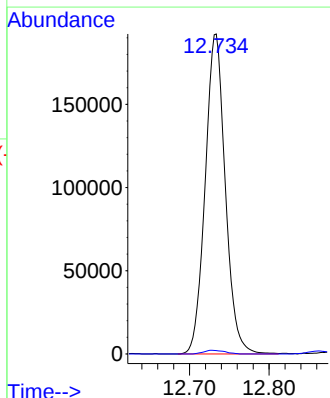
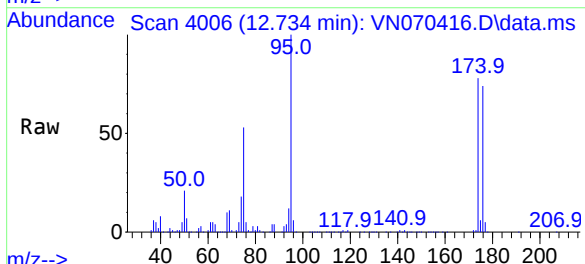




#77
Bromobenzene
Concen: 0.201 ug/l
RT: 12.865 min Scan# 4053
Delta R.T. 0.005 min
Lab File: VN070416.D
Acq: 30 Dec 2021 23:39




Instrument :
MSVOA_N
ClientSampleId :
VN1230MBL02


Tgt Ion:156 Resp: 1925
Ion Ratio Lower Upper
156 100
77 215.7 90.6 271.8
158 75.2 48.9 146.7

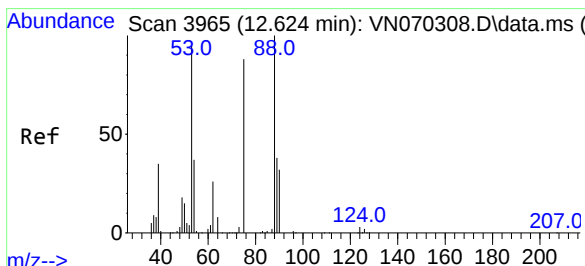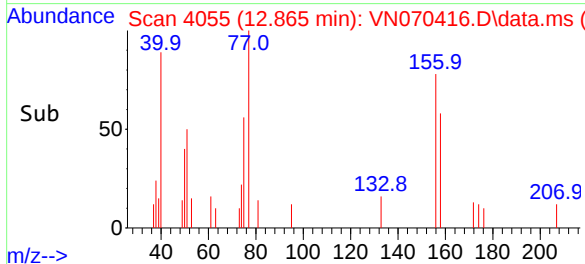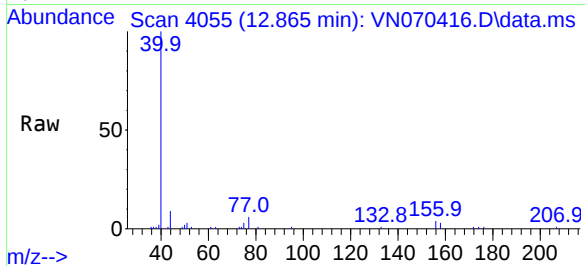

#81
trans-1,4-Dichloro-2-butene
Concen: 91.966 ug/l
RT: 12.734 min Scan# 4006
Delta R.T. 0.110 min
Lab File: VN070416.D
Acq: 30 Dec 2021 23:39

Tgt Ion: 75 Resp: 338065
Ion Ratio Lower Upper
75 100
53 0.1 90.5 135.7#
89 0.0 38.2 57.4#

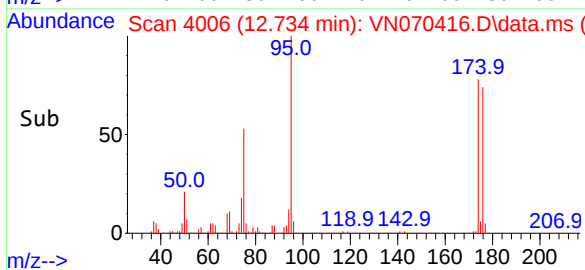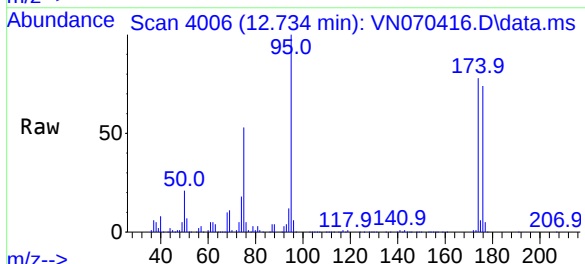



#87

1,3-Dichlorobenzene

Concen: 0.295 ug/l

RT: 13.619 min Scan# 4336

Delta R.T. 0.006 min

Lab File: VN070416.D

Acq: 30 Dec 2021 23:39

Instrument :

MSVOA_N

ClientSampleId :

VN1230MBL02





Tgt Ion:146 Resp: 4721

Ion Ratio Lower Upper

146 100

111 42.1 18.6 55.6

148 58.7 31.6 95.0

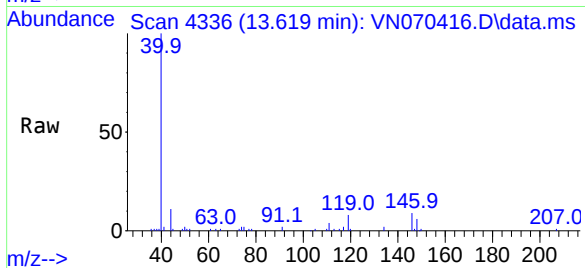

#88

1,4-Dichlorobenzene

Concen: 0.299 ug/l

RT: 13.619 min Scan# 4336

Delta R.T. -0.075 min

Lab File: VN070416.D

Acq: 30 Dec 2021 23:39




Tgt Ion:146 Resp: 4721


Ion Ratio Lower Upper

146 100

111 42.1 18.3 54.8

148 58.7 31.8 95.4


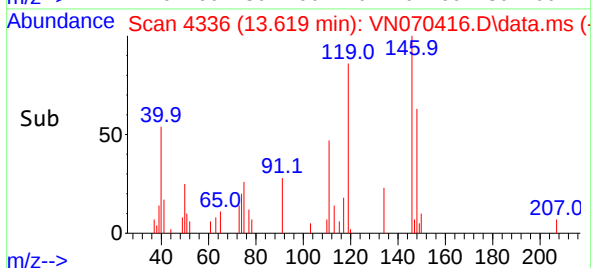

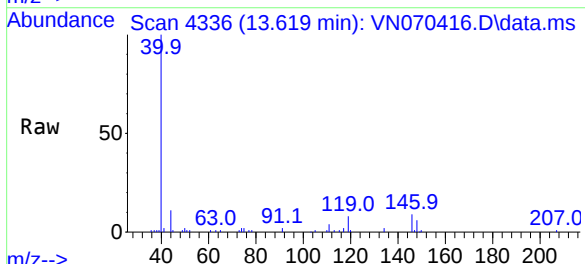




#89
n-Butylbenzene
Concen: 0.330 ug/l
RT: 13.943 min Scan# 4456
Delta R.T. 0.003 min
Lab File: VN070416.D
Acq: 30 Dec 2021 23:39




Instrument :
MSVOA_N
ClientSampleId :
VN1230MBL02


Tgt Ion: 91	Resp:	8641
Ion Ratio	Lower	Upper
91	100	
92	49.1	25.4 76.0
134	21.1	13.6 40.8

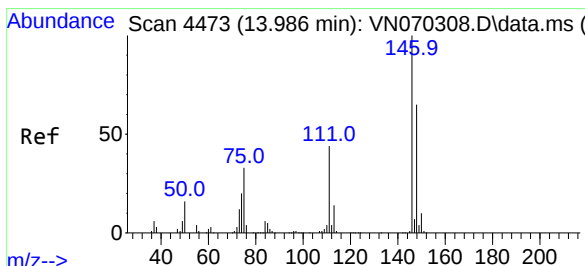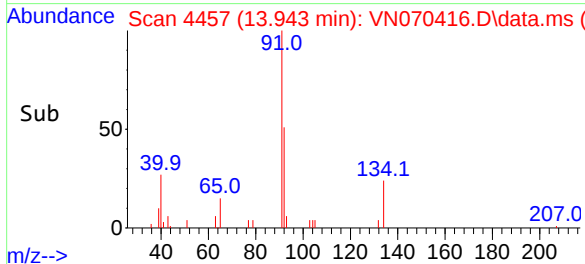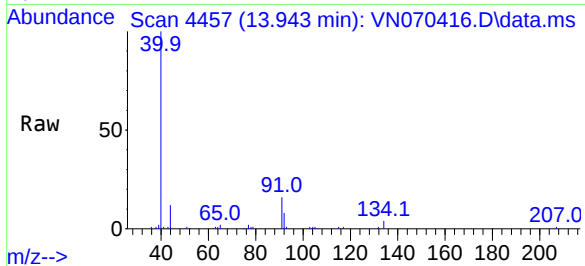

#91
1,2-Dichlorobenzene
Concen: 0.282 ug/l
RT: 13.986 min Scan# 4473
Delta R.T. 0.000 min
Lab File: VN070416.D
Acq: 30 Dec 2021 23:39

Tgt Ion: 146	Resp:	4424
Ion Ratio	Lower	Upper
146	100	
111	39.0	19.1 57.3
148	56.9	32.1 96.3

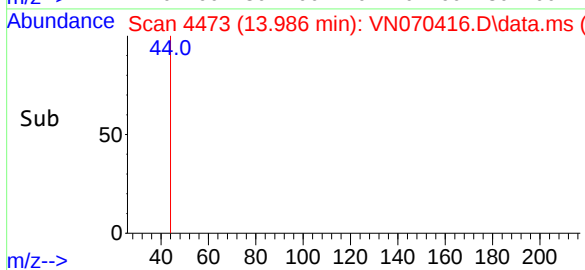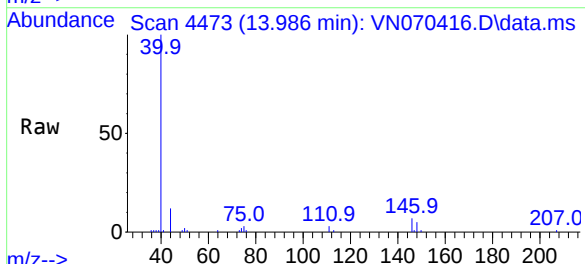



#92

1,2-Dibromo-3-Chloropropane

Concen: 0.449 ug/l

RT: 14.606 min Scan# 41

Delta R.T. 0.006 min

Lab File: VN070416.D

Acq: 30 Dec 2021 23:39

Instrument :

MSVOA_N

ClientSampleId :

VN1230MBL02





Tgt Ion: 75 Resp: 1084

Ion Ratio Lower Upper

75 100

155 82.7 46.9 140.7

157 84.2 60.6 181.7

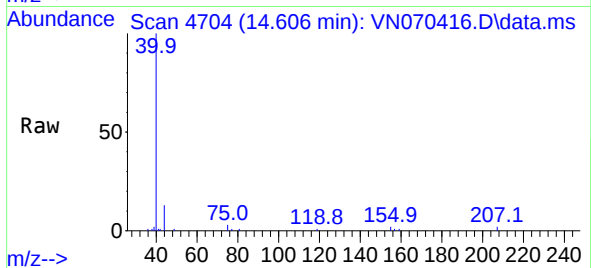

#93

1,2,4-Trichlorobenzene

Concen: 0.862 ug/l

RT: 15.268 min Scan# 4951

Delta R.T. 0.005 min

Lab File: VN070416.D

Acq: 30 Dec 2021 23:39




Tgt Ion:180 Resp: 6380


Ion Ratio Lower Upper

180 100

182 100.8 48.3 144.9

145 31.9 14.5 43.5


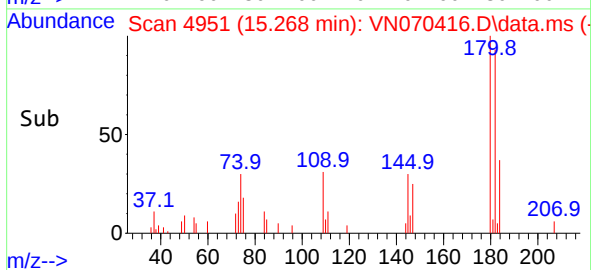






#94
Hexachlorobutadiene
Concen: 0.271 ug/l
RT: 15.367 min Scan# 4988
Delta R.T. 0.000 min
Lab File: VN070416.D
Acq: 30 Dec 2021 23:39




Instrument :
MSVOA_N
ClientSampleId :
VN1230MBL02


Tgt Ion:225 Resp: 1166
Ion Ratio Lower Upper
225 100
223 43.0 31.9 95.7
227 37.2 32.1 96.3



#95
Naphthalene
Concen: 3.194 ug/l
RT: 15.507 min Scan# 5040
Delta R.T. 0.003 min
Lab File: VN070416.D
Acq: 30 Dec 2021 23:39


Tgt Ion:128 Resp: 29652
Ion Ratio Lower Upper
128 100
127 12.7 10.5 15.7
129 11.0 8.7 13.1

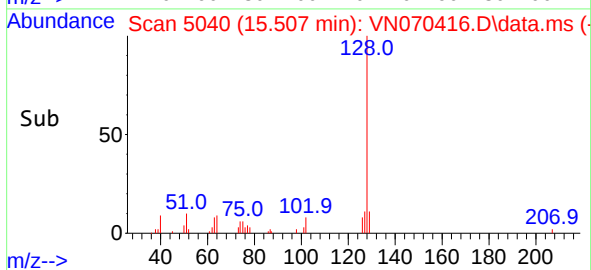



#96
1,2,3-Trichlorobenzene
Concen: 1.917 ug/l
RT: 15.703 min Scan# 5113
Delta R.T. 0.003 min
Lab File: VN070416.D
Acq: 30 Dec 2021 23:39

Instrument :
MSVOA_N
ClientSampleId :
VN1230MBL02

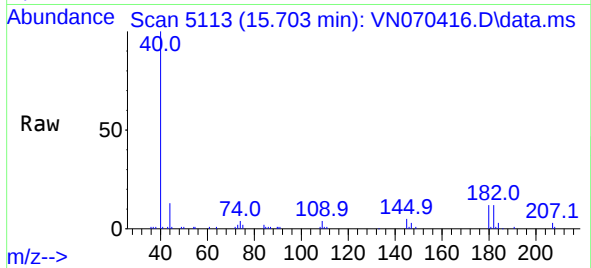

Tgt Ion:	180	Resp:	7856
Ion	Ratio	Lower	Upper
180	100		
182	93.4	47.4	142.2
145	35.7	15.0	45.1

