

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN123021\
 Data File : VN070411.D
 Acq On : 30 Dec 2021 20:14
 Operator : JC/MD
 Sample : M5234-03
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 TB-12-23-21

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N122721W.M

Title : SW846 8260

Signal : TIC: VN070411.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.234	82	91	102	rBV2	142762	286466	5.27%	1.101%
2	4.299	840	861	878	rBV2	31497	95591	1.76%	0.367%
3	5.095	1137	1158	1180	rBV4	31822	109534	2.01%	0.421%
4	8.024	2226	2250	2261	rBV2	709505	1699021	31.25%	6.527%
5	8.086	2262	2273	2296	rVB	1129150	2558453	47.06%	9.829%
6	8.440	2379	2405	2434	rBV	865569	2000099	36.79%	7.684%
7	8.968	2583	2602	2624	rBV	1768929	3673842	67.57%	14.114%
8	10.443	3132	3152	3183	rBV	2886521	5437125	100.00%	20.888%
9	11.747	3618	3638	3669	rBV	2329297	4250232	78.17%	16.328%
10	12.734	3989	4006	4033	rBV	1817999	3251368	59.80%	12.491%
11	13.678	4341	4358	4381	rBV	1489660	2668412	49.08%	10.251%




Sum of corrected areas: 26030143

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN123021\
Data File : VN070411.D
Acq On : 30 Dec 2021 20:14
Operator : JC/MD
Sample : M5234-03
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
TB-12-23-21

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N122721W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

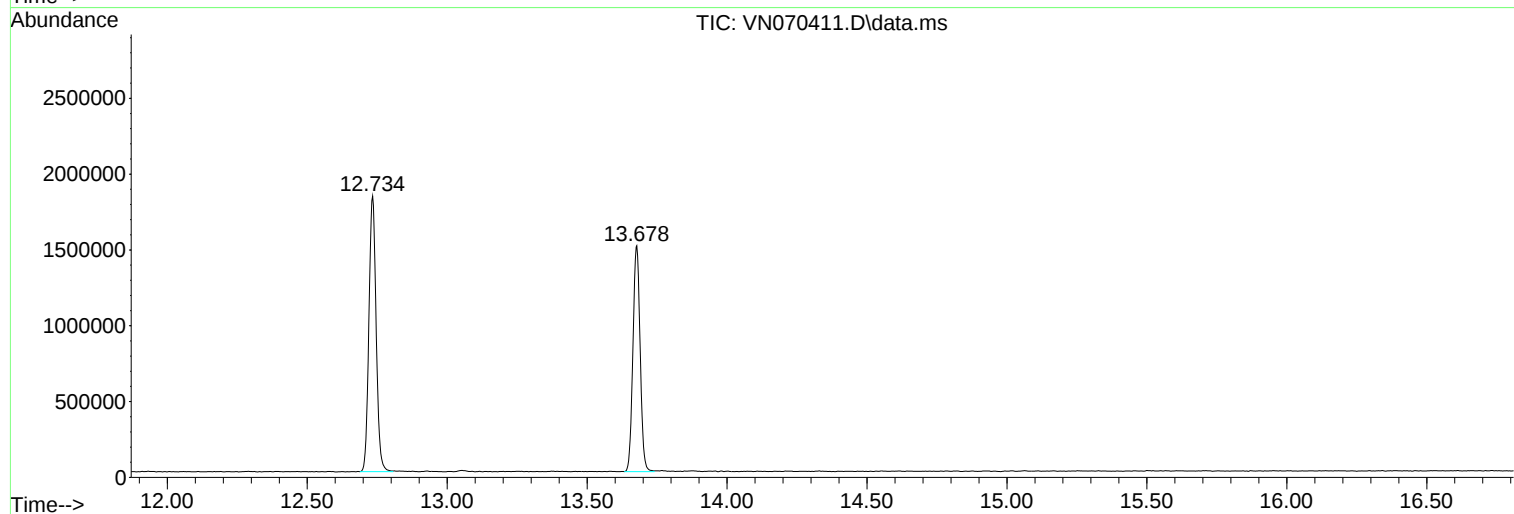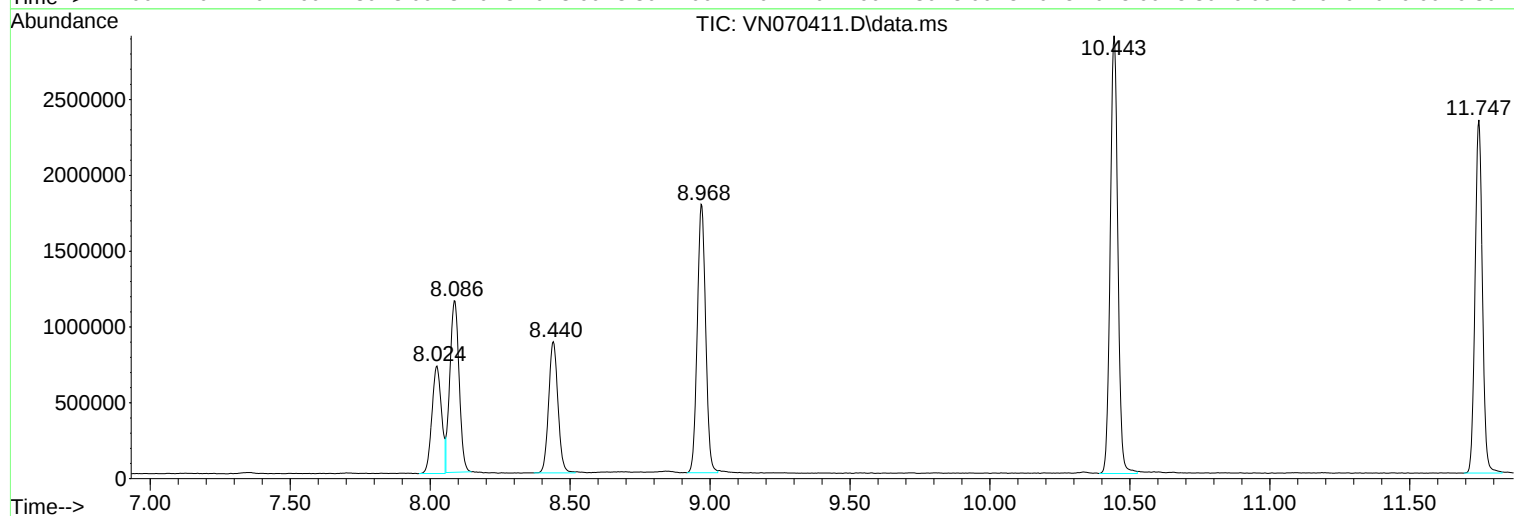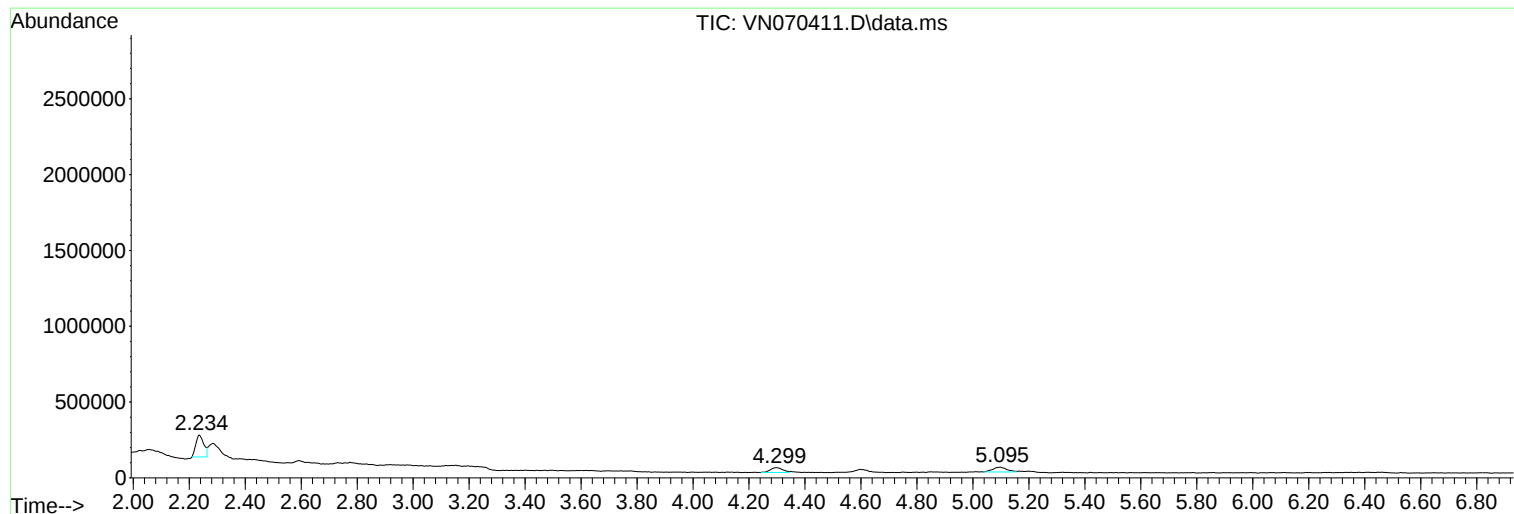

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN123021\
Data File : VN070411.D
Acq On : 30 Dec 2021 20:14
Operator : JC/MD
Sample : M5234-03
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
TB-12-23-21

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N122721W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Sulfur dioxide	2.234	5.6	ug/l	286466	1	8.088	2558450	50.0