
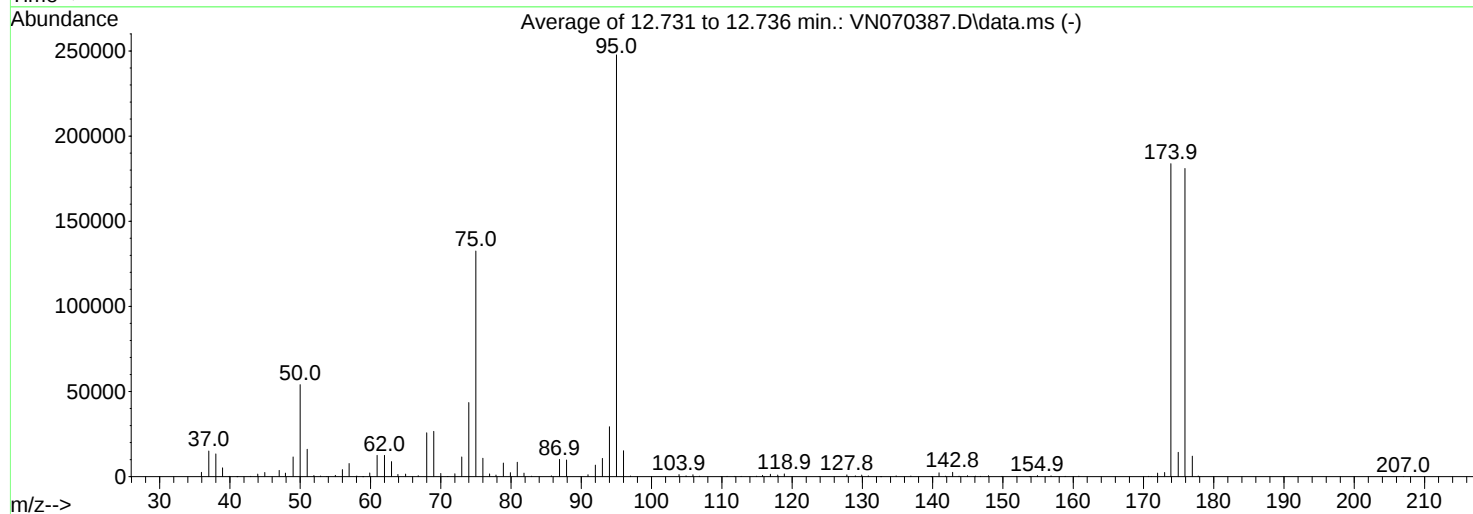


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN123021\
 Data File : VN070387.D
 Acq On : 30 Dec 2021 9:24
 Operator : JC/MD
 Sample : BFB
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N122721W.M
 Title : SW846 8260
 Last Update : Mon Dec 27 18:47:12 2021

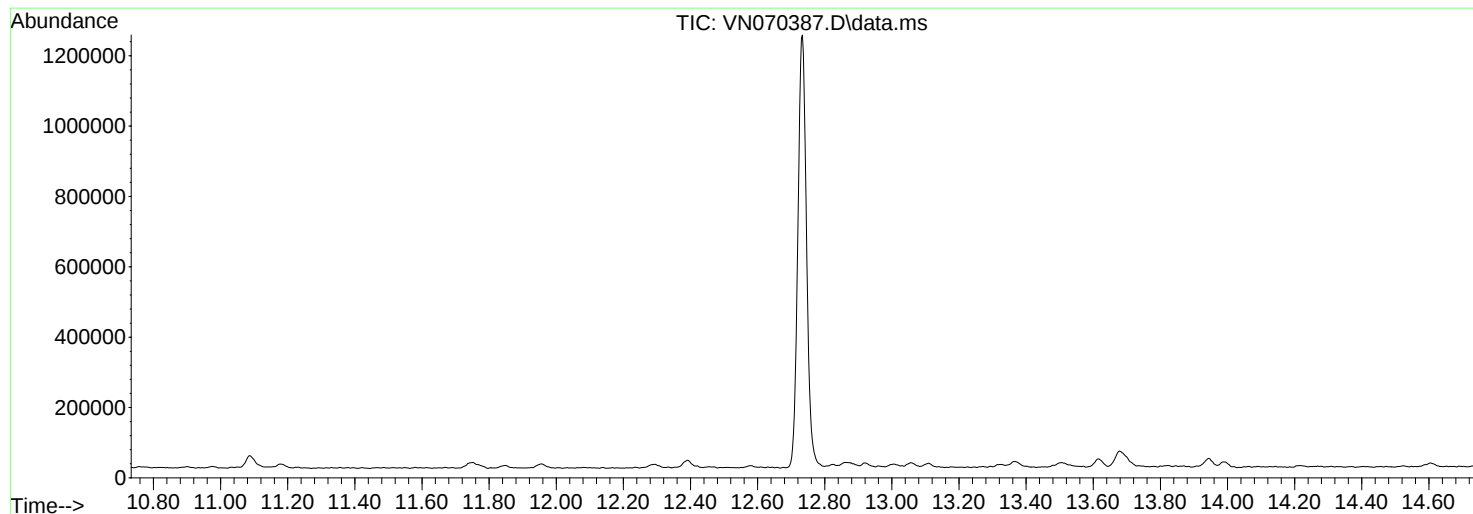

AutoFind: Scans 4005, 4006, 4007; Background Corrected with Scan 3986

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.8	54045	PASS
75	95	30	60	53.5	132507	PASS
95	95	100	100	100.0	247723	PASS
96	95	5	9	6.1	15214	PASS
173	174	0.00	2	1.4	2486	PASS
174	95	50	100	74.2	183765	PASS
175	174	5	9	7.8	14253	PASS
176	174	95	101	98.5	181013	PASS
177	176	5	9	6.6	12008	PASS