
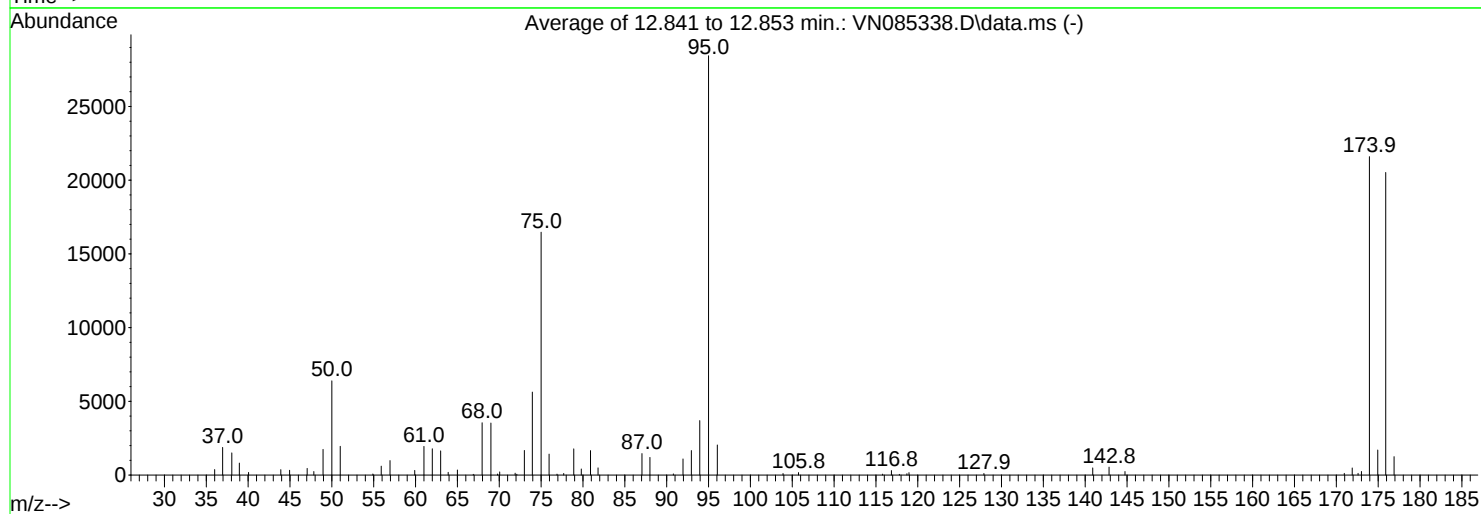


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN123024\
Data File : VN085338.D
Acq On : 30 Dec 2024 10:39
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N122724W.M
Title : SW846 8260
Last Update : Sat Dec 28 01:36:16 2024

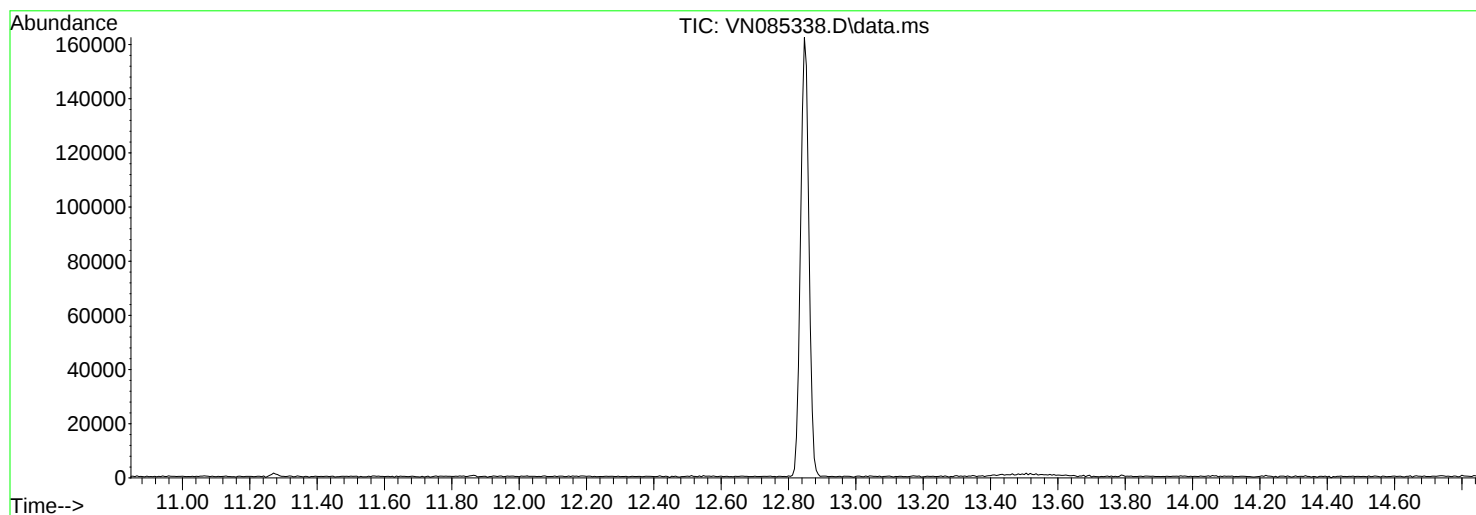

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1843

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.5	6392	PASS
75	95	30	60	57.9	16474	PASS
95	95	100	100	100.0	28440	PASS
96	95	5	9	7.2	2042	PASS
173	174	0.00	2	1.1	243	PASS
174	95	50	100	75.9	21597	PASS
175	174	5	9	7.9	1698	PASS
176	174	95	101	95.0	20523	PASS
177	176	5	9	6.1	1250	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.00	373	51.00	1951	67.95	3548	77.70	111
36.95	1874	54.90	76	69.00	3528	78.90	1779
38.05	1503	55.90	604	69.80	72	79.80	415
38.95	813	56.95	984	70.05	215	80.90	1659
40.05	178	59.90	317	71.90	129	81.80	488
43.90	367	61.00	1944	72.10	58	87.05	1457
44.95	325	62.00	1783	73.00	1670	88.00	1198
47.05	451	63.00	1640	73.95	5630	90.80	82
47.85	242	63.90	185	75.00	16474	91.95	1094
48.95	1743	65.00	346	75.95	1422	92.95	1664
50.00	6392	66.90	52	76.90	65	93.95	3694

Average of 12.841 to 12.853 min.: VN085338.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
95.00	28440	142.85	539				
96.05	2042	144.75	240				
103.90	108	170.95	117				
105.75	170	171.90	482				
115.80	66	172.60	118				
116.85	306	173.00	243				
117.80	50	173.95	21597				
118.70	96	174.95	1698				
118.95	166	175.90	20523				
127.90	111	176.90	1250				
140.90	485						

Instrument :

MSVOA_N

ClientSampleId :

BFB