

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_N\Data\VN123120\  
 Data File : VN065358.D  
 Acq On : 31 Dec 2020 20:28  
 Operator : JC/MD  
 Sample : L5242-15  
 Misc : 5.00mL/MSVOA\_N/WATER  
 ALS Vial : 25 Sample Multiplier: 1

Instrument :  
 MSVOA\_N  
 ClientSampleId :  
 SAMPLE-1(494+26)

Quant Time: Jan 01 01:54:29 2021  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_N\methods\82N122220W.M  
 Quant Title : SW846 8260  
 QLast Update : Tue Dec 22 15:42:18 2020  
 Response via : Initial Calibration


| Compound                      | R.T.           | QIon | Response           | Conc  | Units  | Dev(Min) |
|-------------------------------|----------------|------|--------------------|-------|--------|----------|
| -----                         |                |      |                    |       |        |          |
| Internal Standards            |                |      |                    |       |        |          |
| 1) Pentafluorobenzene         | 7.631          | 168  | 259185             | 50.00 | ug/l   | 0.00     |
| 34) 1,4-Difluorobenzene       | 8.553          | 114  | 438573             | 50.00 | ug/l   | 0.00     |
| 63) Chlorobenzene-d5          | 11.380         | 117  | 470130             | 50.00 | ug/l   | 0.00     |
| 72) 1,4-Dichlorobenzene-d4    | 13.318         | 152  | 197088             | 50.00 | ug/l   | 0.00     |
|                               |                |      |                    |       |        |          |
| System Monitoring Compounds   |                |      |                    |       |        |          |
| 33) 1,2-Dichloroethane-d4     | 7.991          | 65   | 149213             | 51.00 | ug/l   | 0.00     |
| Spiked Amount 50.000          | Range 61 - 141 |      | Recovery = 102.00% |       |        |          |
| 35) Dibromofluoromethane      | 7.557          | 113  | 133888             | 50.60 | ug/l   | 0.00     |
| Spiked Amount 50.000          | Range 69 - 133 |      | Recovery = 101.20% |       |        |          |
| 50) Toluene-d8                | 10.061         | 98   | 548100             | 55.27 | ug/l   | 0.00     |
| Spiked Amount 50.000          | Range 65 - 126 |      | Recovery = 110.54% |       |        |          |
| 62) 4-Bromofluorobenzene      | 12.376         | 95   | 213496             | 53.98 | ug/l   | 0.00     |
| Spiked Amount 50.000          | Range 58 - 135 |      | Recovery = 107.96% |       |        |          |
|                               |                |      |                    |       |        |          |
| Target Compounds              |                |      |                    |       |        | Qvalue   |
| 3) Chloromethane              | 2.158          | 50   | 667                | 0.24  | ug/l # | 41       |
| 8) Diethyl Ether              | 3.386          | 74   | 1002               | 0.60  | ug/l # | 35       |
| 11) Tert butyl alcohol        | 4.772          | 59   | 96                 | 0.20  | ug/l # | 73       |
| 13) Acrolein                  | 3.570          | 56   | 29                 | 2.50  | ug/l # | 1        |
| 16) Acetone                   | 3.792          | 43   | 18175              | 4.22  | ug/l   | 97       |
| 18) Methyl Acetate            | 4.300          | 43   | 2966               | 1.13  | ug/l # | 61       |
| 20) Methylene Chloride        | 4.512          | 84   | 11903              | 4.17  | ug/l   | 99       |
| 25) 2-Butanone                | 6.814          | 43   | 5707               | 3.47  | ug/l   | 93       |
| 29) Tetrahydrofuran           | 7.184          | 42   | 504                | 0.47  | ug/l # | 76       |
| 31) Cyclohexane               | 7.627          | 56   | 4363               | 1.01  | ug/l # | 1        |
| 36) 1,1-Dichloropropene       | 7.631          | 75   | 16405              | 4.11  | ug/l # | 50       |
| 38) Carbon Tetrachloride      | 7.631          | 117  | 22755              | 5.43  | ug/l # | 16       |
| 43) Isopropyl Acetate         | 8.135          | 43   | 22657              | 3.33  | ug/l   | 96       |
| 45) 1,2-Dichloropropane       | 9.241          | 63   | 1213               | 0.39  | ug/l # | 43       |
| 48) Methyl methacrylate       | 9.148          | 41   | 5955               | 1.80  | ug/l # | 12       |
| 51) 4-Methyl-2-Pentanone      | 9.958          | 43   | 5211               | 1.36  | ug/l   | 98       |
| 54) cis-1,3-Dichloropropene   | 9.875          | 75   | 42692              | 8.07  | ug/l # | 62       |
| 57) 1,3-Dichloropropane       | 10.737         | 76   | 20252              | 4.15  | ug/l # | 42       |
| 59) 2-Hexanone                | 10.737         | 43   | 277864             | 98.68 | ug/l # | 49       |
| 71) Bromoform                 | 12.380         | 173  | 1405               | 0.44  | ug/l # | 1        |
| 74) N-amyl acetate            | 12.010         | 43   | 1210               | 0.20  | ug/l # | 42       |
| 76) 1,2,3-Trichloropropane    | 12.376         | 75   | 104951             | 26.10 | ug/l # | 100      |
| 81) trans-1,4-Dichloro-2-b... | 12.376         | 75   | 104951             | 65.82 | ug/l # | 15       |
| 95) Naphthalene               | 15.109         | 128  | 158                | 3.39  | ug/l # | 69       |
| -----                         |                |      |                    |       |        |          |


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_N\Data\VN123120\  
Data File : VN065358.D  
Acq On : 31 Dec 2020 20:28  
Operator : JC/MD  
Sample : L5242-15  
Misc : 5.00mL/MSVOA\_N/WATER  
ALS Vial : 25 Sample Multiplier: 1

Instrument :  
MSVOA\_N  
ClientSampleId :  
SAMPLE-1(494+26)

Quant Time: Jan 01 01:54:29 2021  
Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_N\methods\82N122220W.M  
Quant Title : SW846 8260  
QLast Update : Tue Dec 22 15:42:18 2020  
Response via : Initial Calibration




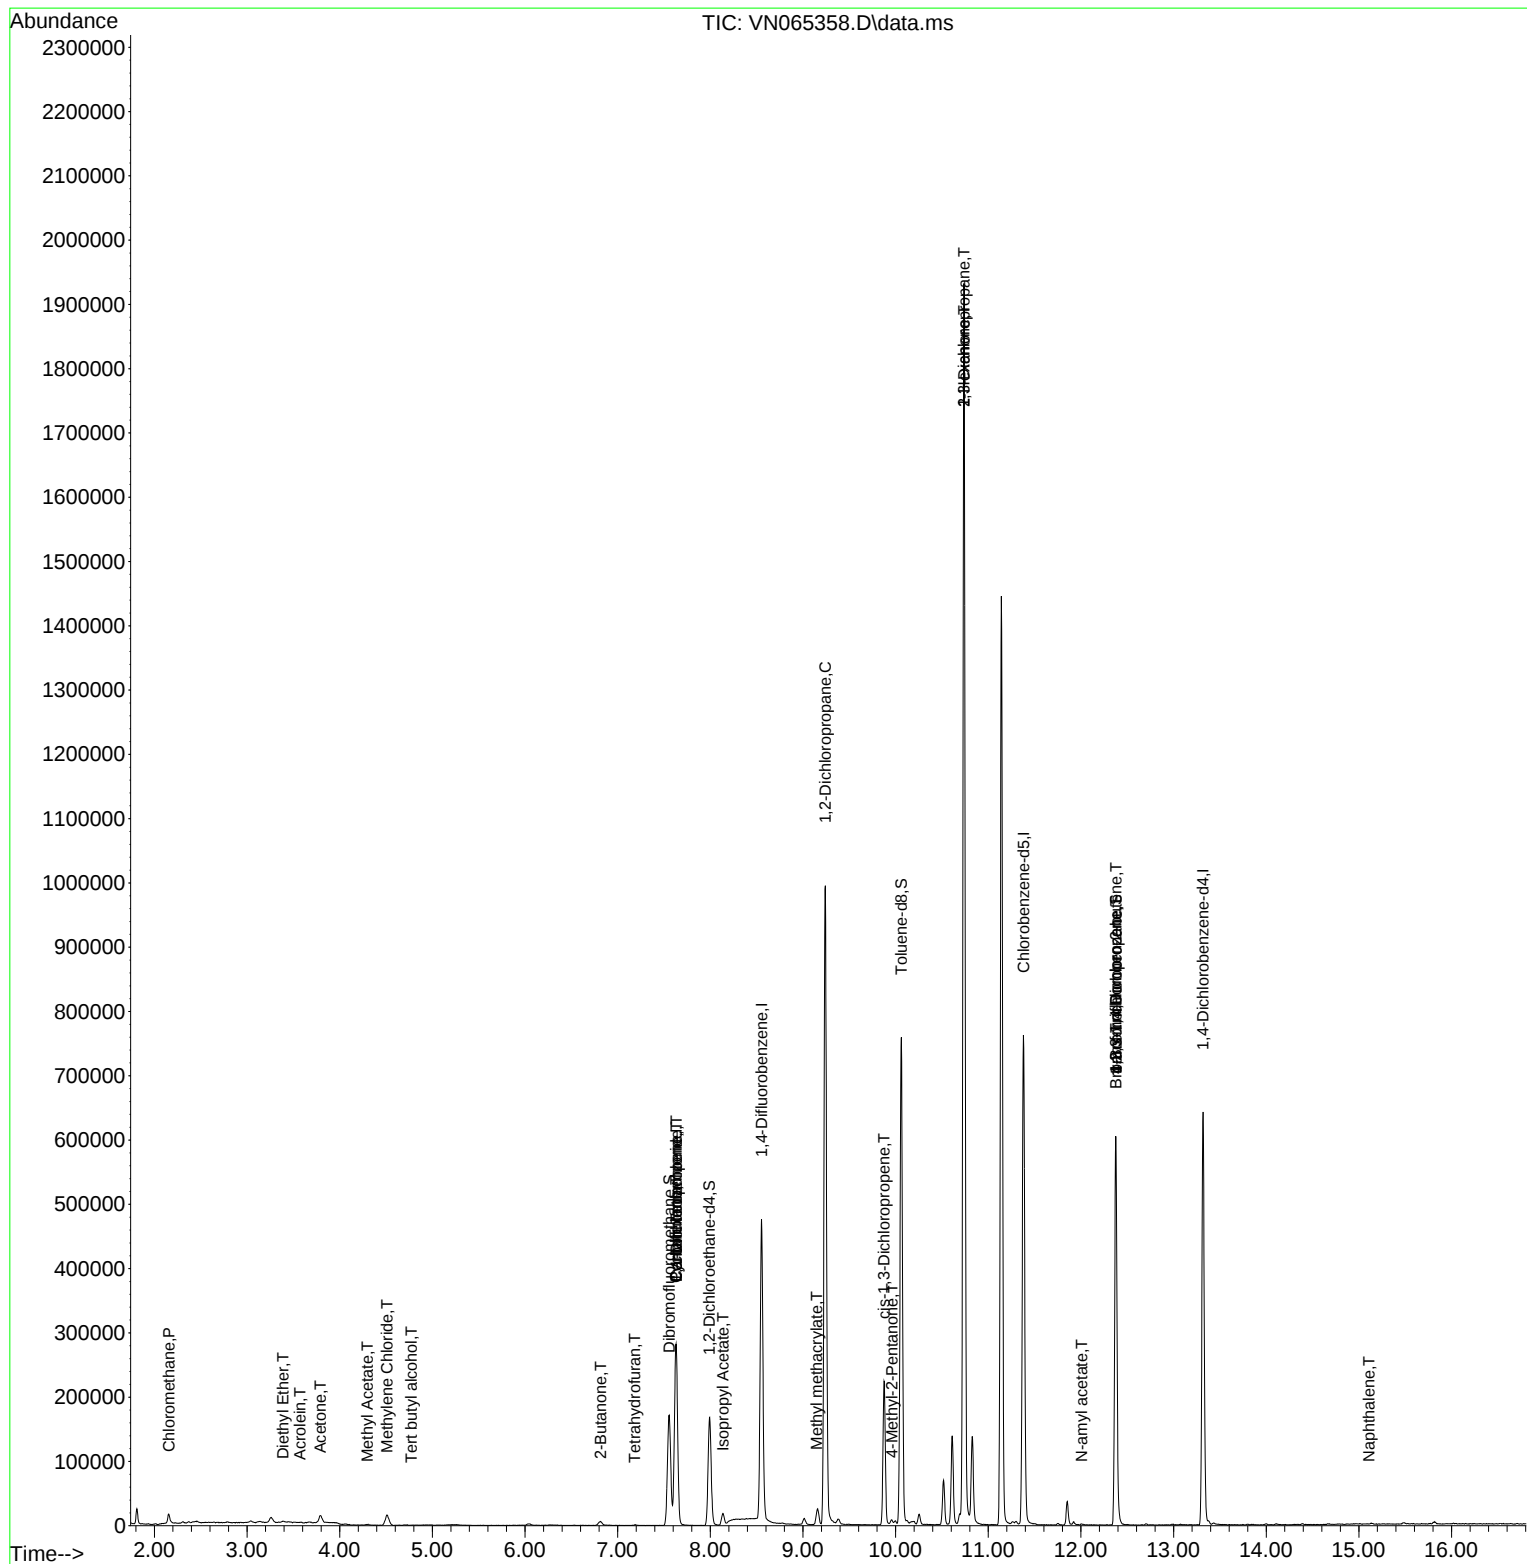




#1  
Pentafluorobenzene  
Concen: 50.00 ug/l  
RT: 7.631 min Scan# 1832  
Delta R.T. 0.004 min  
Lab File: VN065358.D  
Acq: 31 Dec 2020 20:28




Instrument :  
MSVOA\_N  
ClientSampleId :  
SAMPLE-1(494+26)


Tgt Ion:168 Resp: 259185  
Ion Ratio Lower Upper  
168 100  
99 48.8 43.0 64.4

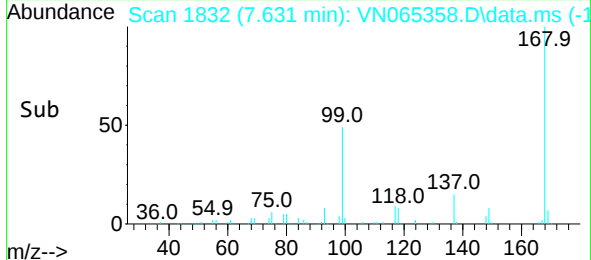

#3  
Chloromethane  
Concen: 0.24 ug/l  
RT: 2.158 min Scan# 130  
Delta R.T. 0.112 min  
Lab File: VN065358.D  
Acq: 31 Dec 2020 20:28

Tgt Ion: 50 Resp: 667  
Ion Ratio Lower Upper  
50 100  
52 0.0 26.6 39.8#

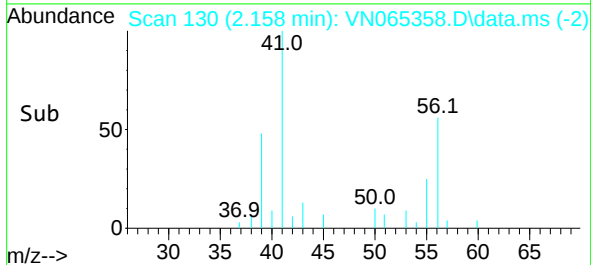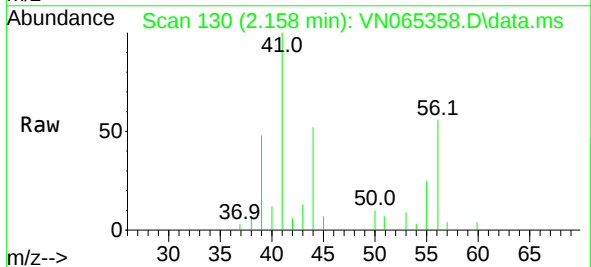

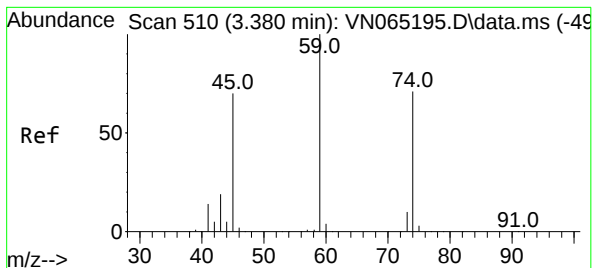

#8

Diethyl Ether

Concen: 0.60 ug/l

RT: 3.386 min Scan# 512

Delta R.T. 0.006 min

Lab File: VN065358.D





Acq: 31 Dec 2020 20:28

Tgt Ion: 74 Resp: 1002

Ion Ratio Lower Upper

74 100

45 33.9 48.9 146.8#

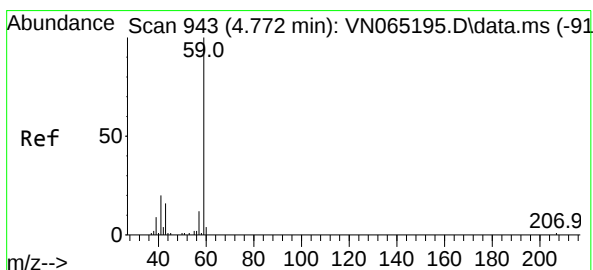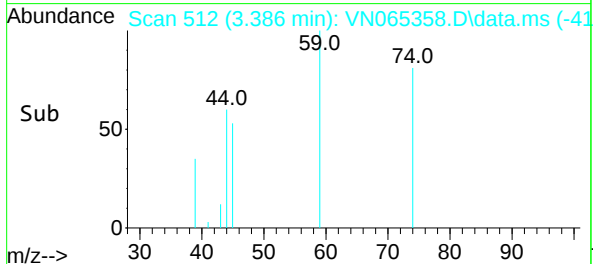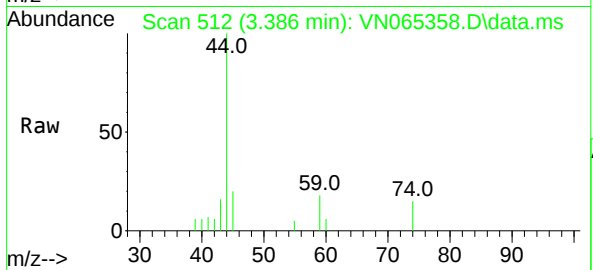

#11

Tert butyl alcohol

Concen: 0.20 ug/l

RT: 4.772 min Scan# 943

Delta R.T. 0.000 min

Lab File: VN065358.D




Acq: 31 Dec 2020 20:28


Tgt Ion: 59 Resp: 96

Ion Ratio Lower Upper

59 100

57 0.0 7.9 11.9#


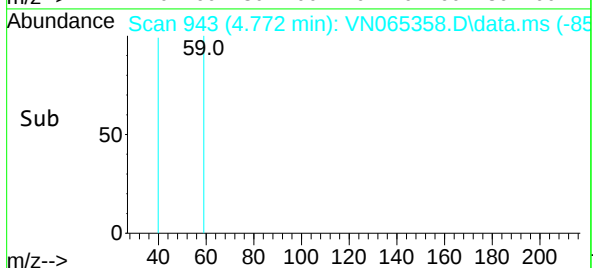

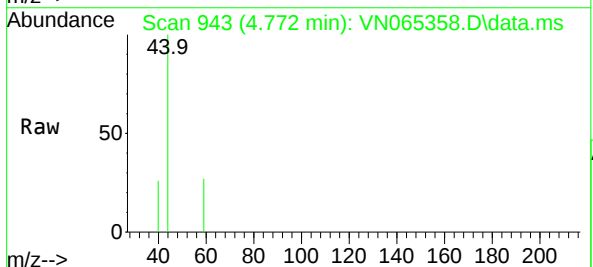




#13  
Acrolein  
Concen: 2.50 ug/l  
RT: 3.570 min Scan# 569  
Delta R.T. -0.003 min  
Lab File: VN065358.D  
Acq: 31 Dec 2020 20:28




Instrument :  
MSVOA\_N  
ClientSampleId :  
SAMPLE-1(494+26)


Tgt Ion: 56 Resp: 29  
Ion Ratio Lower Upper  
56 100  
55 206.9 56.5 84.7#

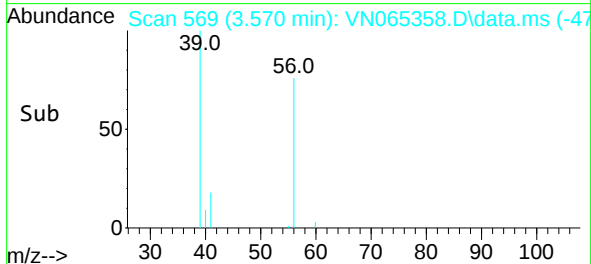

#16  
Acetone  
Concen: 4.22 ug/l  
RT: 3.792 min Scan# 638  
Delta R.T. 0.007 min  
Lab File: VN065358.D  
Acq: 31 Dec 2020 20:28


Tgt Ion: 43 Resp: 18175  
Ion Ratio Lower Upper  
43 100  
58 33.8 25.7 38.5

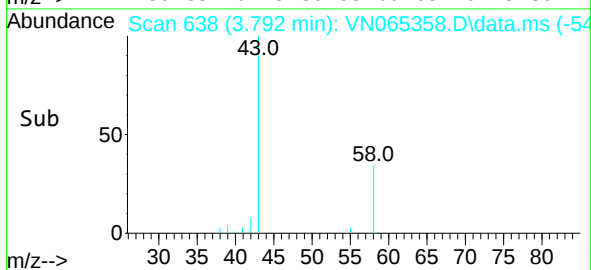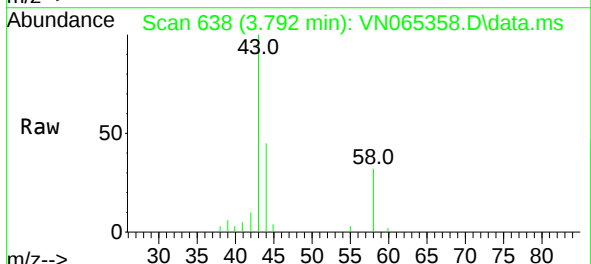






#18  
Methyl Acetate  
Concen: 1.13 ug/l  
RT: 4.300 min Scan# 796  
Delta R.T. 0.013 min  
Lab File: VN065358.D  
Acq: 31 Dec 2020 20:28

Instrument :  
MSVOA\_N  
ClientSampleId :  
SAMPLE-1(494+26)







Tgt Ion: 43 Resp: 2966  
Ion Ratio Lower Upper  
43 100  
74 5.7 20.2 30.2#



#20  
Methylene Chloride  
Concen: 4.17 ug/l  
RT: 4.512 min Scan# 862  
Delta R.T. 0.010 min  
Lab File: VN065358.D  
Acq: 31 Dec 2020 20:28

Tgt Ion: 84 Resp: 11903  
Ion Ratio Lower Upper  
84 100  
49 116.2 93.4 140.0  
51 36.2 28.2 42.4  
86 63.3 51.7 77.5


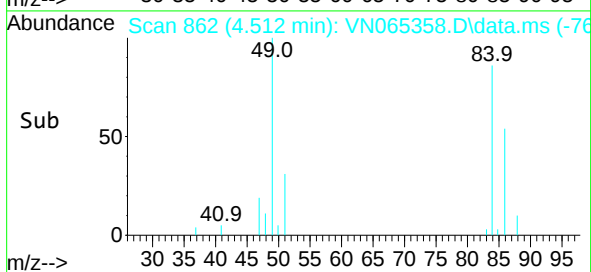




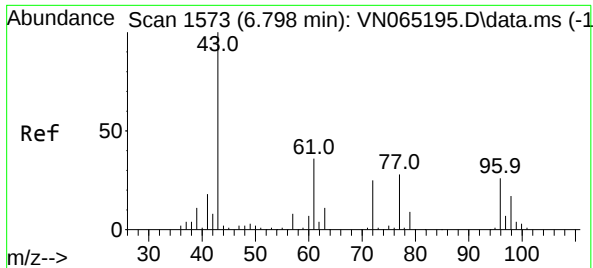

#25  
2-Butanone  
Concen: 3.47 ug/l  
RT: 6.814 min Scan# 1578  
Delta R.T. 0.016 min  
Lab File: VN065358.D  
Acq: 31 Dec 2020 20:28




Instrument :  
MSVOA\_N  
ClientSampleId :  
SAMPLE-1(494+26)


Tgt Ion: 43 Resp: 5707  
Ion Ratio Lower Upper  
43 100  
72 30.0 21.0 31.6

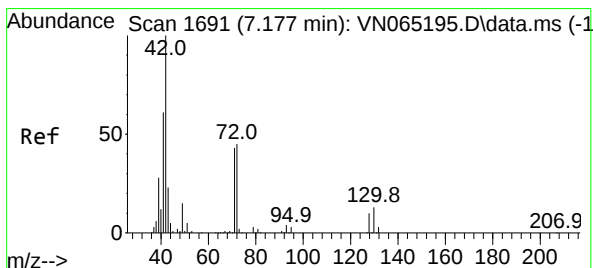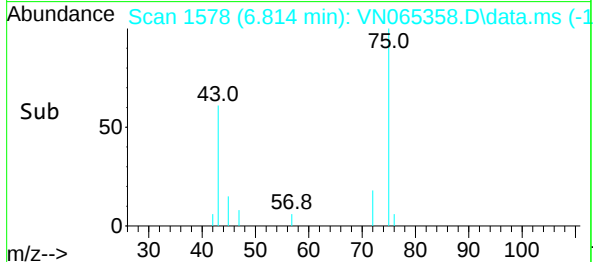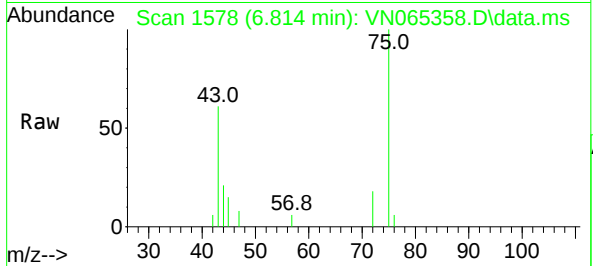

#29  
Tetrahydrofuran  
Concen: 0.47 ug/l  
RT: 7.184 min Scan# 1693  
Delta R.T. 0.007 min  
Lab File: VN065358.D  
Acq: 31 Dec 2020 20:28

Tgt Ion: 42 Resp: 504  
Ion Ratio Lower Upper  
42 100  
72 38.1 36.6 54.8  
71 17.9 33.6 50.4#


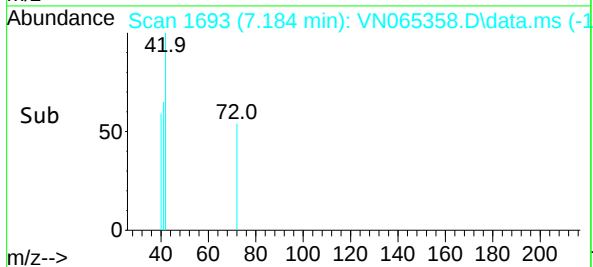

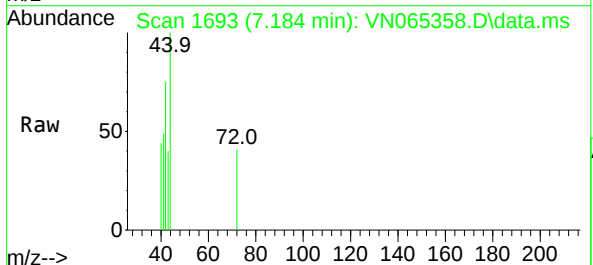




#31  
Cyclohexane  
Concen: 1.01 ug/l  
RT: 7.627 min Scan# 1831  
Delta R.T. 0.016 min  
Lab File: VN065358.D  
Acq: 31 Dec 2020 20:28




Instrument :  
MSVOA\_N  
ClientSampleId :  
SAMPLE-1(494+26)


Tgt Ion: 56 Resp: 4363  
Ion Ratio Lower Upper  
56 100  
69 171.7 27.5 41.3#  
84 151.4 73.9 110.9#

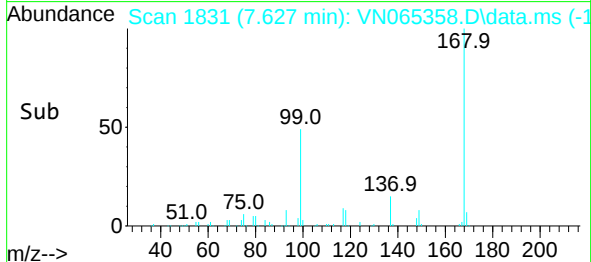

#33  
1,2-Dichloroethane-d4  
Concen: 51.00 ug/l  
RT: 7.991 min Scan# 1944  
Delta R.T. -0.000 min  
Lab File: VN065358.D  
Acq: 31 Dec 2020 20:28

Tgt Ion: 65 Resp: 149213  
Ion Ratio Lower Upper  
65 100  
67 52.4 0.0 108.2

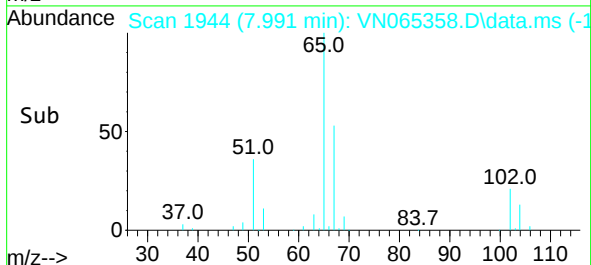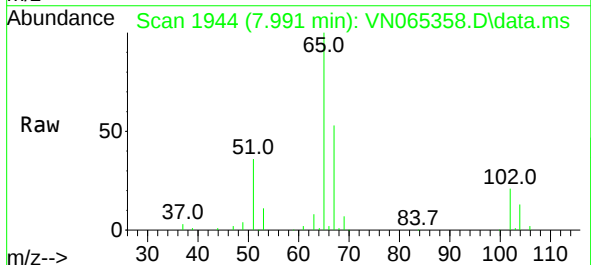



#34

1,4-Difluorobenzene

Concen: 50.00 ug/l

RT: 8.553 min Scan# 2119

Delta R.T. 0.003 min

Lab File: VN065358.D

Acq: 31 Dec 2020 20:28





Tgt Ion:114 Resp: 438573

Ion Ratio Lower Upper

114 100

63 19.2 0.0 38.6

88 15.3 0.0 32.6

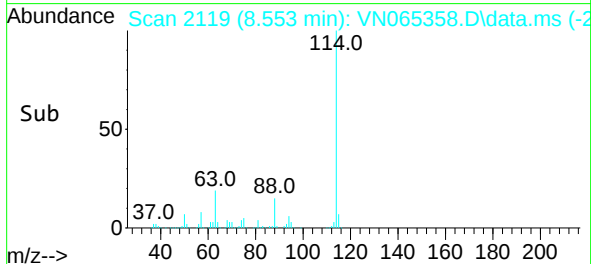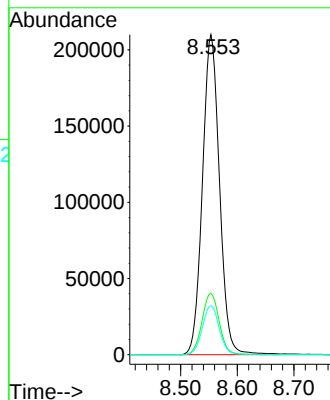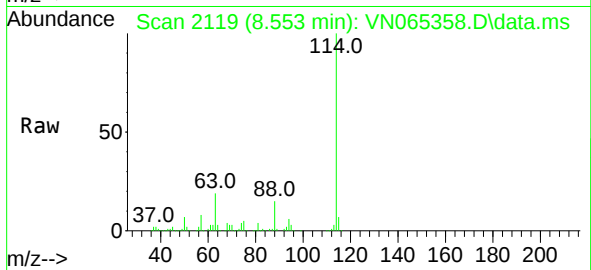

#35

Dibromofluoromethane

Concen: 50.60 ug/l

RT: 7.557 min Scan# 1809

Delta R.T. 0.007 min

Lab File: VN065358.D

Acq: 31 Dec 2020 20:28




Tgt Ion:113 Resp: 133888


Ion Ratio Lower Upper

113 100

111 102.1 81.6 122.4

192 23.3 16.2 24.2


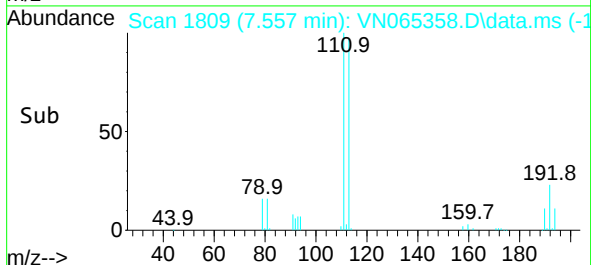
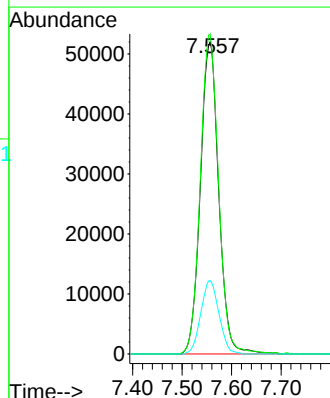
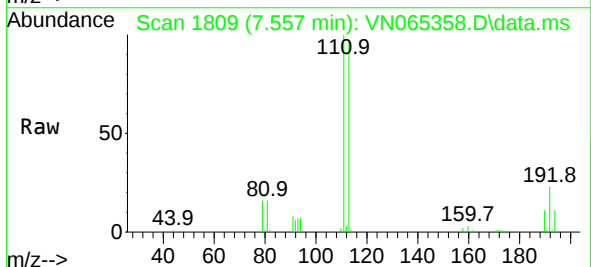


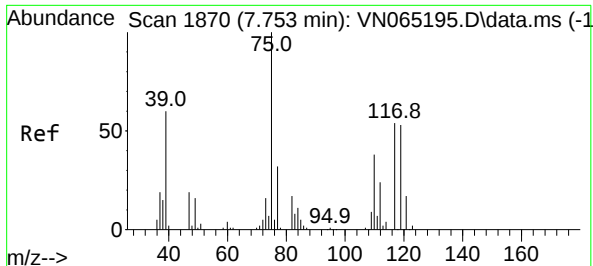

#36  
1,1-Dichloropropene  
Concen: 4.11 ug/l  
RT: 7.631 min Scan# 1832  
Delta R.T. -0.122 min  
Lab File: VN065358.D  
Acq: 31 Dec 2020 20:28




Instrument :  
MSVOA\_N  
ClientSampleId :  
SAMPLE-1(494+26)


Tgt Ion: 75 Resp: 16405  
Ion Ratio Lower Upper  
75 100  
110 9.2 17.8 53.3#  
77 0.0 25.0 37.4#

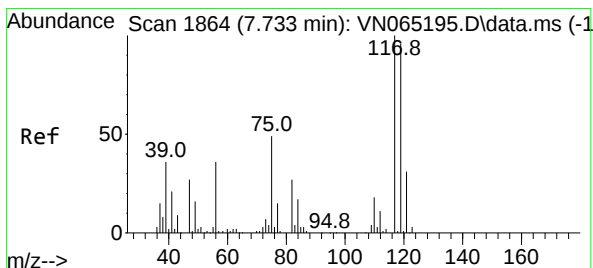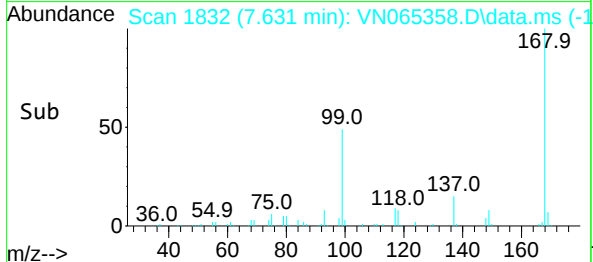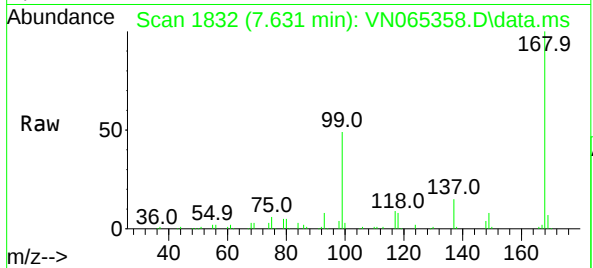

#38  
Carbon Tetrachloride  
Concen: 5.43 ug/l  
RT: 7.631 min Scan# 1832  
Delta R.T. -0.102 min  
Lab File: VN065358.D  
Acq: 31 Dec 2020 20:28

Tgt Ion: 117 Resp: 22755  
Ion Ratio Lower Upper  
117 100  
119 5.2 76.7 115.1#  
121 0.0 25.4 38.2#


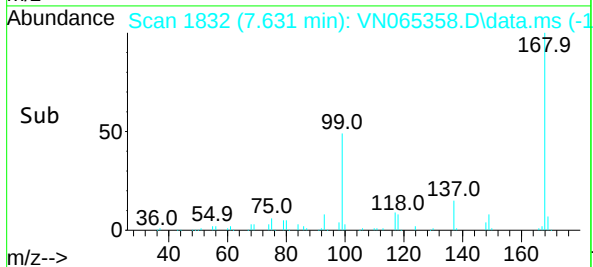

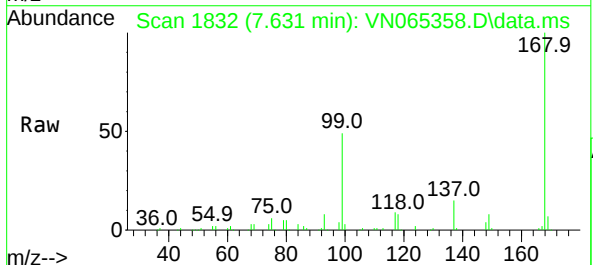


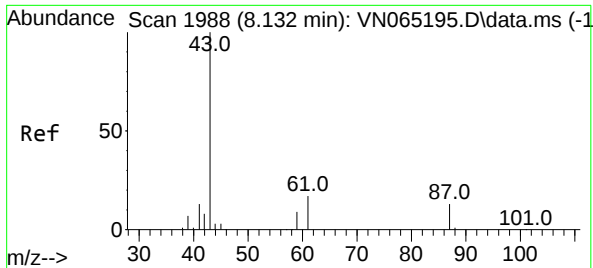

#43  
Isopropyl Acetate  
Concen: 3.33 ug/l  
RT: 8.135 min Scan# 1989  
Delta R.T. 0.003 min  
Lab File: VN065358.D  
Acq: 31 Dec 2020 20:28




Instrument :  
MSVOA\_N  
ClientSampleId :  
SAMPLE-1(494+26)


|          |       |       |       |
|----------|-------|-------|-------|
| Tgt Ion: | 43    | Resp: | 22657 |
| Ion      | Ratio | Lower | Upper |
| 43       | 100   |       |       |
| 61       | 19.6  | 17.2  | 25.8  |
| 87       | 12.9  | 11.4  | 17.0  |

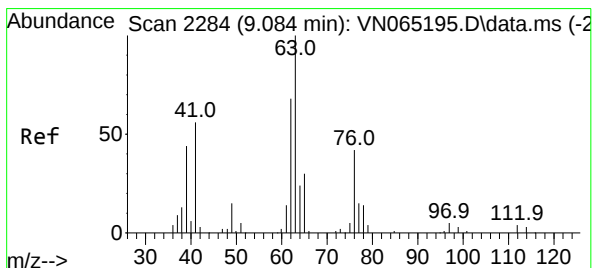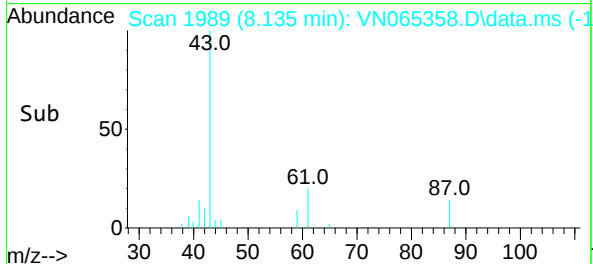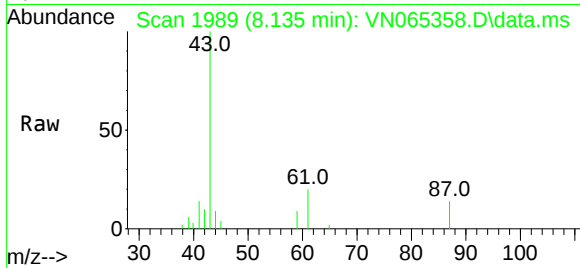

#45  
1,2-Dichloropropane  
Concen: 0.39 ug/l  
RT: 9.241 min Scan# 2333  
Delta R.T. 0.157 min  
Lab File: VN065358.D  
Acq: 31 Dec 2020 20:28

|          |       |       |       |
|----------|-------|-------|-------|
| Tgt Ion: | 63    | Resp: | 1213  |
| Ion      | Ratio | Lower | Upper |
| 63       | 100   |       |       |
| 65       | 0.0   | 25.0  | 37.4# |


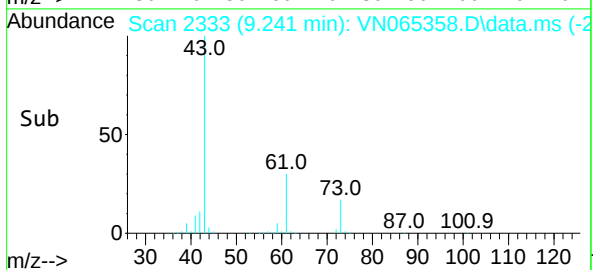

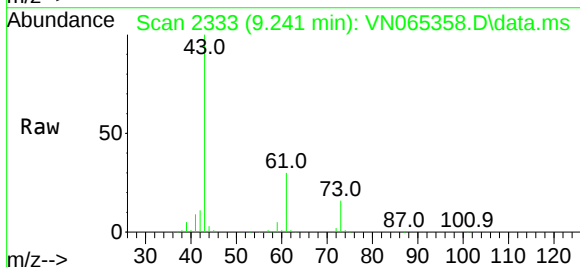




#48  
Methyl methacrylate  
Concen: 1.80 ug/l  
RT: 9.148 min Scan# 2304  
Delta R.T. -0.019 min  
Lab File: VN065358.D  
Acq: 31 Dec 2020 20:28




Instrument :  
MSVOA\_N  
ClientSampleId :  
SAMPLE-1(494+26)


Tgt Ion: 41 Resp: 5955  
Ion Ratio Lower Upper  
41 100  
69 0.0 71.8 107.8#  
39 0.0 44.1 66.1#

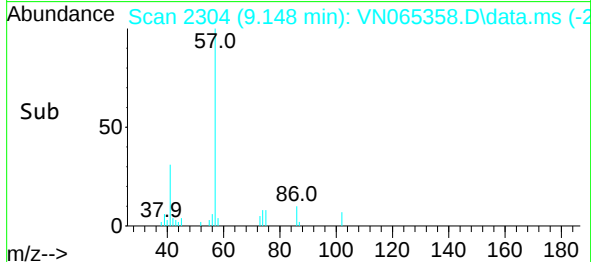

#50  
Toluene-d8  
Concen: 55.27 ug/l  
RT: 10.061 min Scan# 2588  
Delta R.T. 0.003 min  
Lab File: VN065358.D  
Acq: 31 Dec 2020 20:28

Tgt Ion: 98 Resp: 548100  
Ion Ratio Lower Upper  
98 100  
100 64.3 51.7 77.5


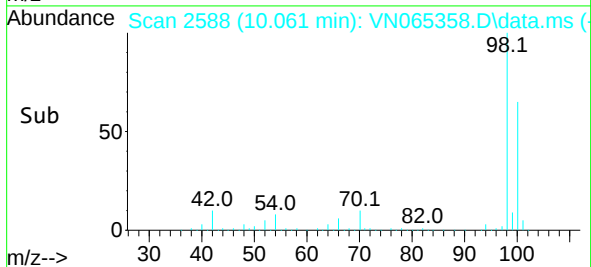

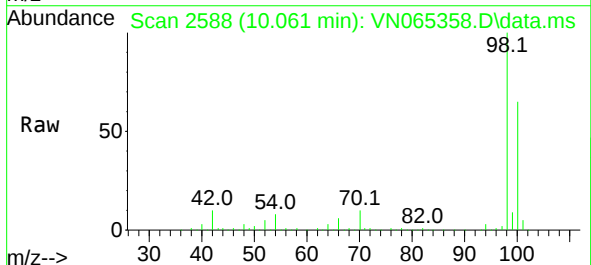




#51  
4-Methyl-2-Pentanone  
Concen: 1.36 ug/l  
RT: 9.958 min Scan# 2556  
Delta R.T. 0.003 min  
Lab File: VN065358.D  
Acq: 31 Dec 2020 20:28




Instrument :  
MSVOA\_N  
ClientSampleId :  
SAMPLE-1(494+26)


Tgt Ion: 43 Resp: 5211  
Ion Ratio Lower Upper  
43 100  
58 39.3 32.4 48.6

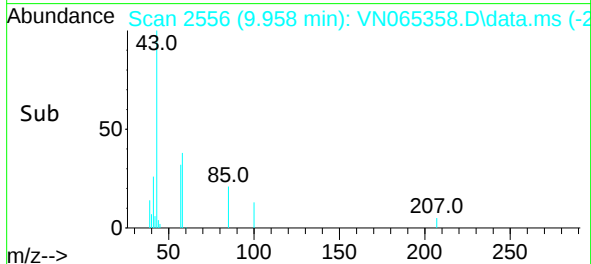

#54  
cis-1,3-Dichloropropene  
Concen: 8.07 ug/l  
RT: 9.875 min Scan# 2530  
Delta R.T. 0.068 min  
Lab File: VN065358.D  
Acq: 31 Dec 2020 20:28

Tgt Ion: 75 Resp: 42692  
Ion Ratio Lower Upper  
75 100  
77 0.7 25.5 38.3#  
39 27.7 35.6 53.4#


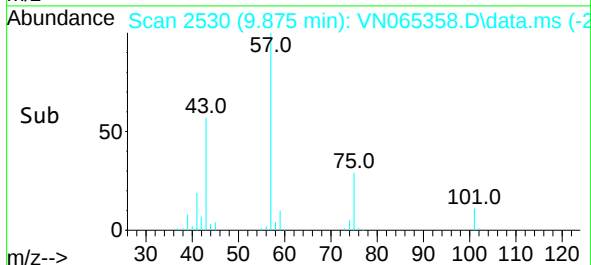

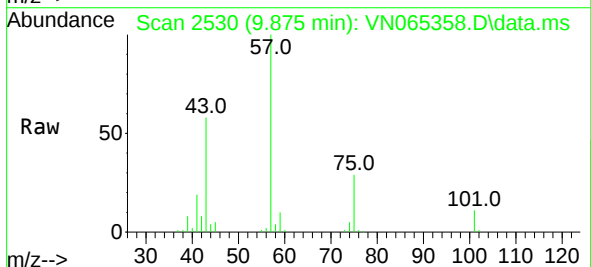




#57  
1,3-Dichloropropane  
Concen: 4.15 ug/l  
RT: 10.737 min Scan# 2798  
Delta R.T. 0.058 min  
Lab File: VN065358.D  
Acq: 31 Dec 2020 20:28




Instrument :  
MSVOA\_N  
ClientSampleId :  
SAMPLE-1(494+26)


Tgt Ion: 76 Resp: 20252  
Ion Ratio Lower Upper  
76 100  
78 0.0 26.1 39.1#

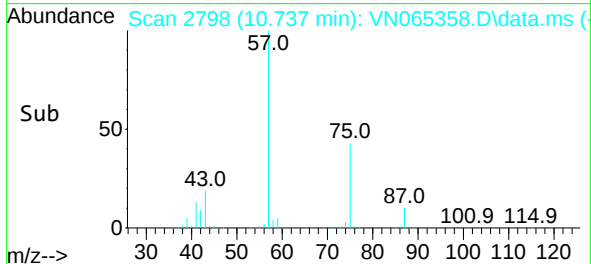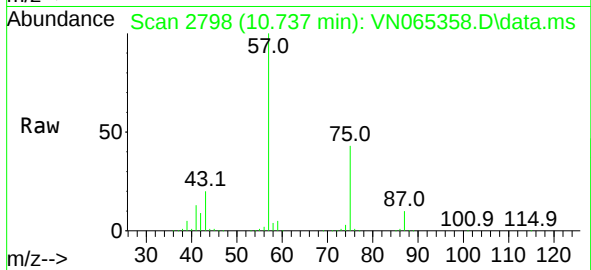

#59  
2-Hexanone  
Concen: 98.68 ug/l  
RT: 10.737 min Scan# 2798  
Delta R.T. 0.013 min  
Lab File: VN065358.D  
Acq: 31 Dec 2020 20:28

Tgt Ion: 43 Resp: 277864  
Ion Ratio Lower Upper  
43 100  
58 19.3 28.3 84.9#


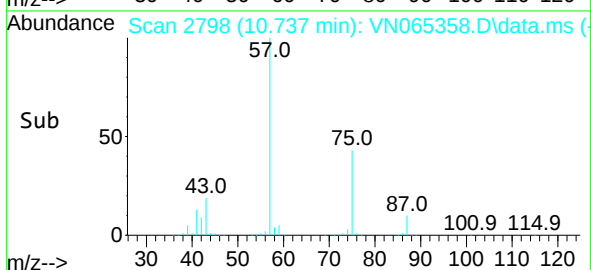




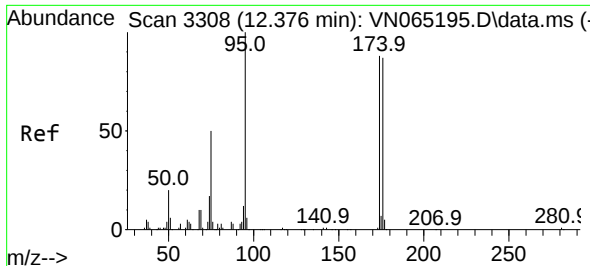

#62  
4-Bromofluorobenzene  
Concen: 53.98 ug/l  
RT: 12.376 min Scan# 3308  
Delta R.T. 0.000 min  
Lab File: VN065358.D  
Acq: 31 Dec 2020 20:28




Instrument :  
MSVOA\_N  
ClientSampleId :  
SAMPLE-1(494+26)


Tgt Ion: 95 Resp: 213496  
Ion Ratio Lower Upper  
95 100  
174 92.8 0.0 160.4  
176 89.1 0.0 158.4

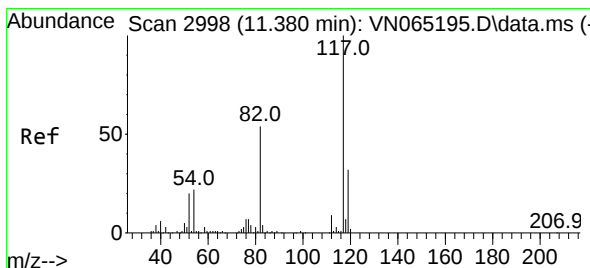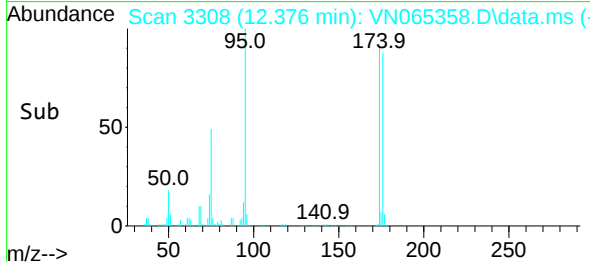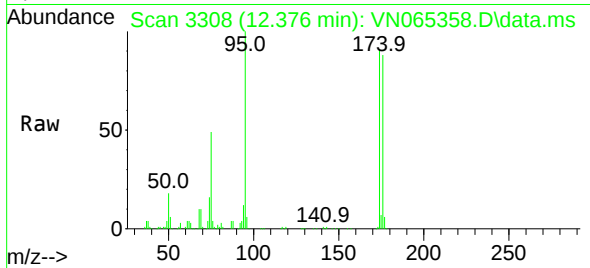

#63  
Chlorobenzene-d5  
Concen: 50.00 ug/l  
RT: 11.380 min Scan# 2998  
Delta R.T. -0.000 min  
Lab File: VN065358.D  
Acq: 31 Dec 2020 20:28

Tgt Ion: 117 Resp: 470130  
Ion Ratio Lower Upper  
117 100  
82 52.7 44.2 66.2  
119 31.8 25.8 38.6

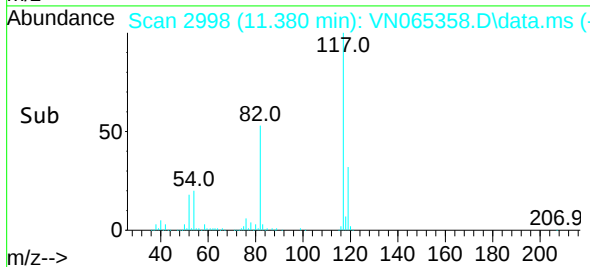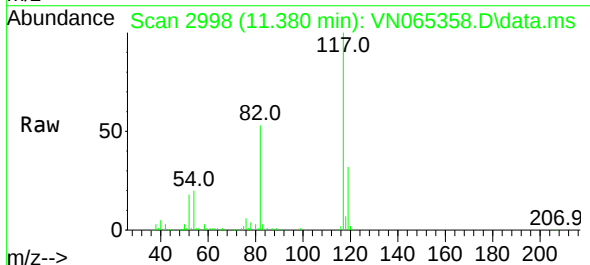

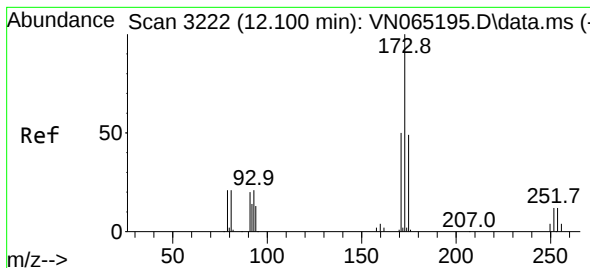

#71

Bromoform

Concen: 0.44 ug/l

RT: 12.380 min Scan# 3309

Delta R.T. 0.280 min





Lab File: VN065358.D

Acq: 31 Dec 2020 20:28

Tgt Ion:173 Resp: 1405

| Ion | Ratio | Lower | Upper |
|-----|-------|-------|-------|
| 173 | 100   |       |       |
| 175 | 822.1 | 24.3  | 72.8# |
| 254 | 0.0   | 0.0   | 0.0   |

Instrument :  
MSVOA\_N  
ClientSampleId :  
SAMPLE-1(494+26)

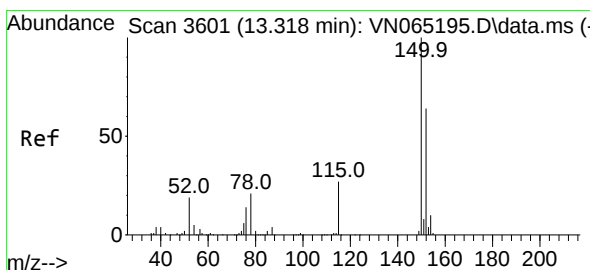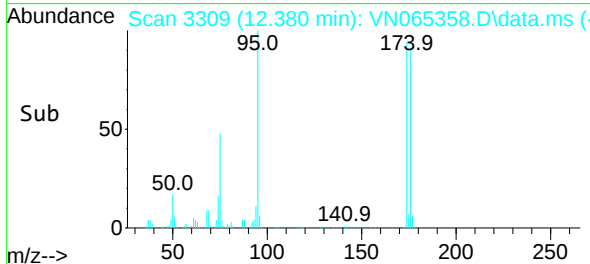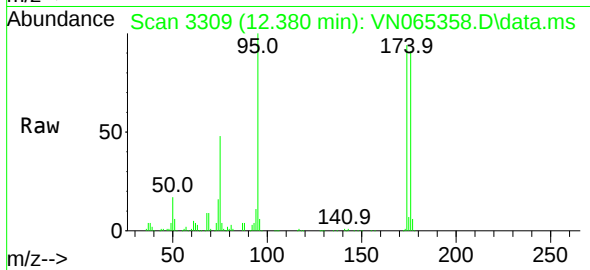

#72

1,4-Dichlorobenzene-d4

Concen: 50.00 ug/l

RT: 13.318 min Scan# 3601




Delta R.T. 0.000 min


Lab File: VN065358.D

Acq: 31 Dec 2020 20:28

Tgt Ion:152 Resp: 197088


| Ion | Ratio | Lower | Upper |
|-----|-------|-------|-------|
| 152 | 100   |       |       |
| 115 | 54.4  | 29.7  | 89.1  |
| 150 | 155.7 | 0.0   | 350.6 |

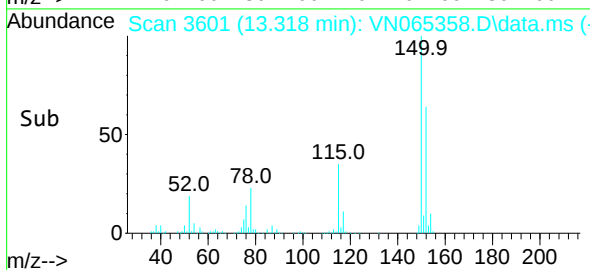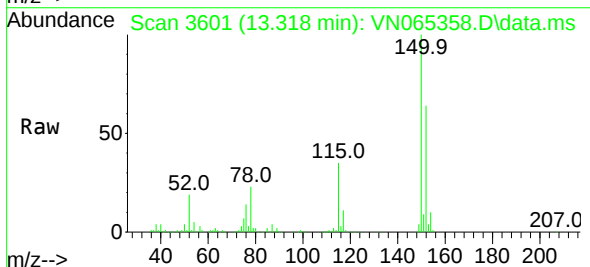



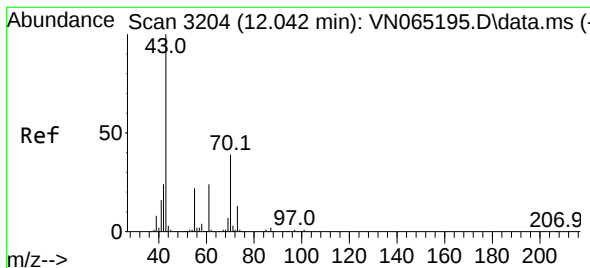


#74  
N-amy1 acetate  
Concen: 0.20 ug/l  
RT: 12.010 min Scan# 3194  
Delta R.T. -0.032 min  
Lab File: VN065358.D  
Acq: 31 Dec 2020 20:28

Instrument :  
MSVOA\_N  
ClientSampleId :  
SAMPLE-1(494+26)



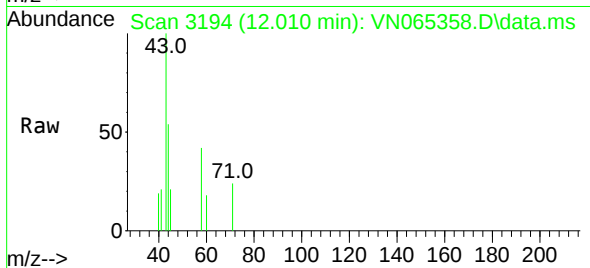



|             |                |
|-------------|----------------|
| Tgt Ion: 43 | Resp: 1210     |
| Ion Ratio   | Lower Upper    |
| 43          | 100            |
| 70          | 0.0 34.5 51.7# |
| 55          | 0.0 20.4 30.6# |
| 61          | 0.0 20.0 30.0# |

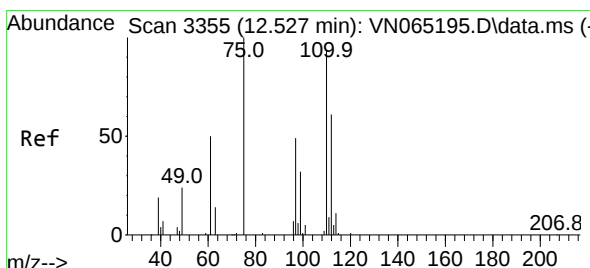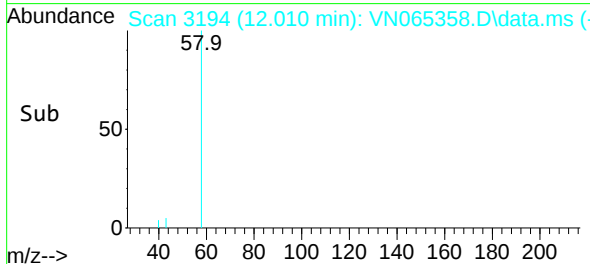

#76  
1,2,3-Trichloropropane  
Concen: 26.10 ug/l  
RT: 12.376 min Scan# 3308  
Delta R.T. -0.151 min  
Lab File: VN065358.D  
Acq: 31 Dec 2020 20:28


|             |              |
|-------------|--------------|
| Tgt Ion: 75 | Resp: 104951 |
| Ion Ratio   | Lower Upper  |
| 75          | 100          |
| 77          | 1.1 0.0 0.0# |

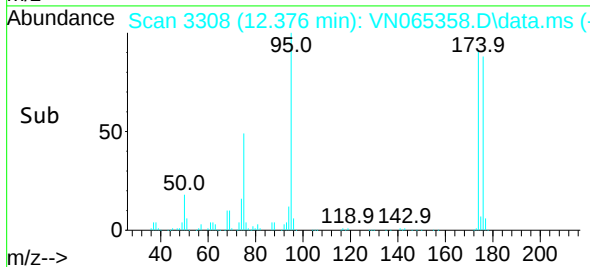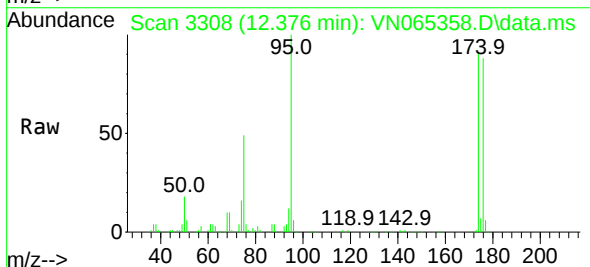



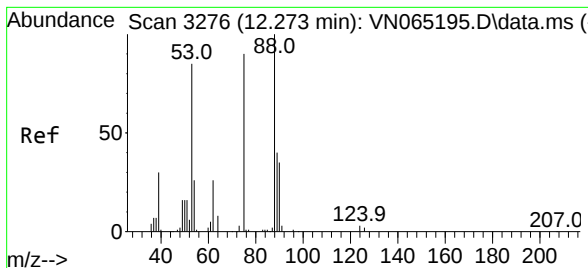


#81  
trans-1,4-Dichloro-2-butene  
Concen: 65.82 ug/l  
RT: 12.376 min Scan# 3308  
Delta R.T. 0.103 min  
Lab File: VN065358.D  
Acq: 31 Dec 2020 20:28


Instrument :  
MSVOA\_N  
ClientSampleId :  
SAMPLE-1(494+26)

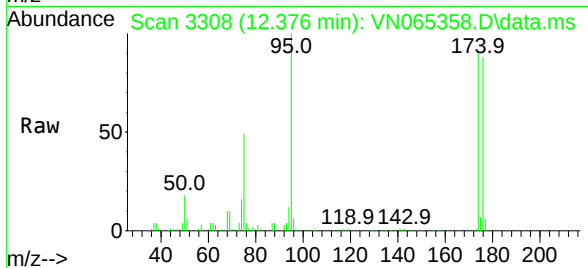

Tgt Ion: 75 Resp: 104951  
Ion Ratio Lower Upper  
75 100  
53 0.0 67.0 100.4#  
89 0.0 39.6 59.4#

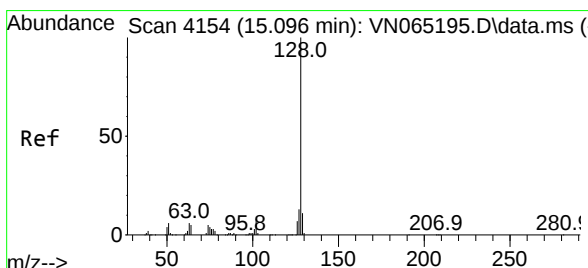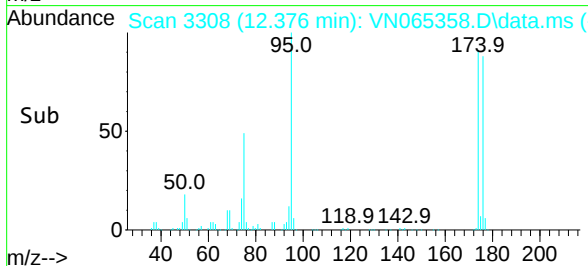

#95  
Naphthalene  
Concen: 3.39 ug/l  
RT: 15.109 min Scan# 4158  
Delta R.T. 0.013 min  
Lab File: VN065358.D  
Acq: 31 Dec 2020 20:28

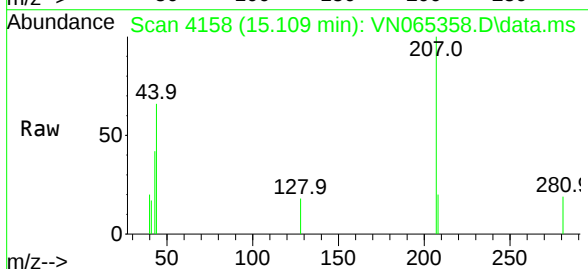

Tgt Ion: 128 Resp: 158  
Ion Ratio Lower Upper  
128 100  
127 0.0 10.3 15.5#  
129 0.0 8.7 13.1#

