
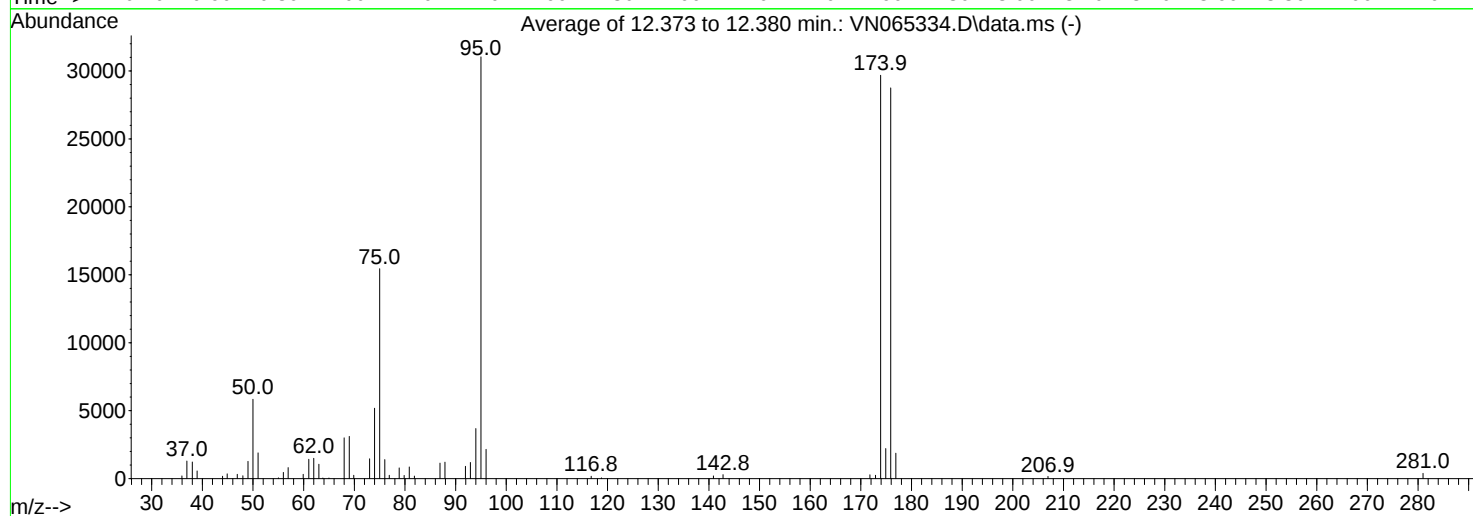


Data Path : Z:\voasrv\HPCHEM1\MSVOA\_N\Data\VN123120\  
 Data File : VN065334.D  
 Acq On : 31 Dec 2020 9:00  
 Operator : JC/MD  
 Sample : BFB  
 Misc : 5.00mL/MSVOA\_N/WATER  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 MSVOA\_N  
 ClientSampleId :  
 BFB

Integration File: RTEINT3.P

Method : Z:\voasrv\HPCHEM1\MSVOA\_N\methods\624N122120W.M  
 Title : METHOD 624 VOLATILE ORGANIC ANALYSIS  
 Last Update : Mon Dec 21 13:17:58 2020

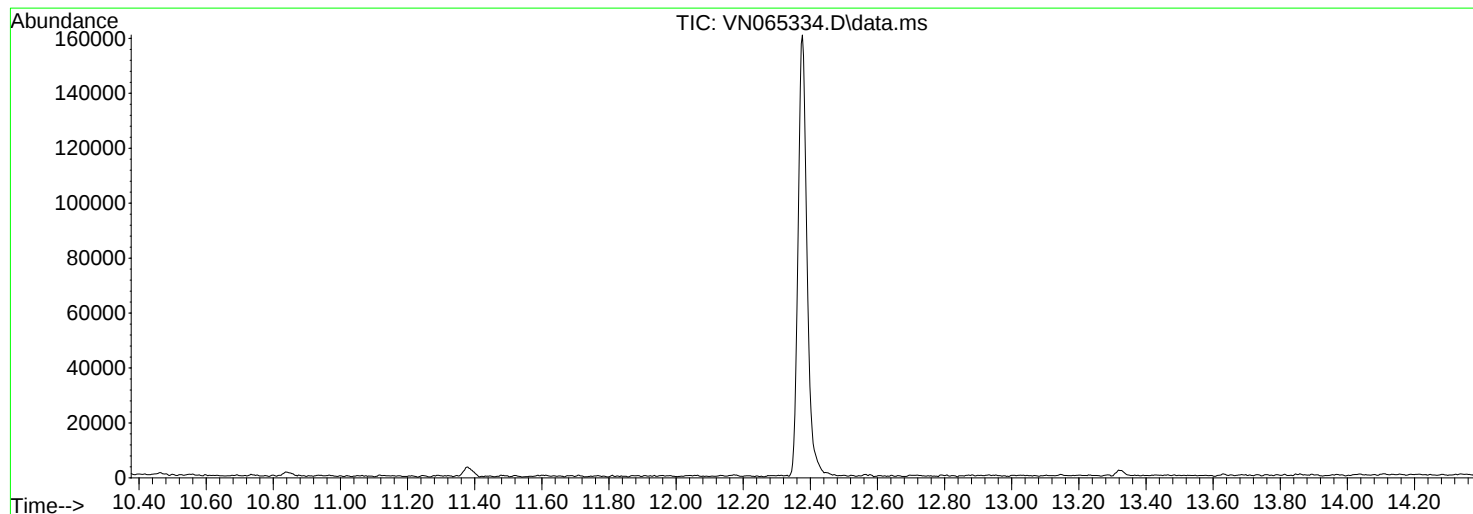

AutoFind: Scans 3307, 3308, 3309; Background Corrected with Scan 3295

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 50             | 95              | 15              | 40              | 18.8         | 5836       | PASS                |
| 75             | 95              | 30              | 60              | 49.8         | 15452      | PASS                |
| 95             | 95              | 100             | 100             | 100.0        | 31040      | PASS                |
| 96             | 95              | 5               | 9               | 6.9          | 2157       | PASS                |
| 173            | 174             | 0.00            | 2               | 0.9          | 253        | PASS                |
| 174            | 95              | 50              | 100             | 95.6         | 29680      | PASS                |
| 175            | 174             | 5               | 9               | 7.5          | 2212       | PASS                |
| 176            | 174             | 95              | 101             | 96.9         | 28757      | PASS                |
| 177            | 176             | 5               | 9               | 6.5          | 1872       | PASS                |