


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN123120\
Data File : VN065341.D
Acq On : 31 Dec 2020 12:37
Operator : JC/MD
Sample : BFB
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N122220W.M
Title : SW846 8260
Last Update : Tue Dec 22 15:42:18 2020

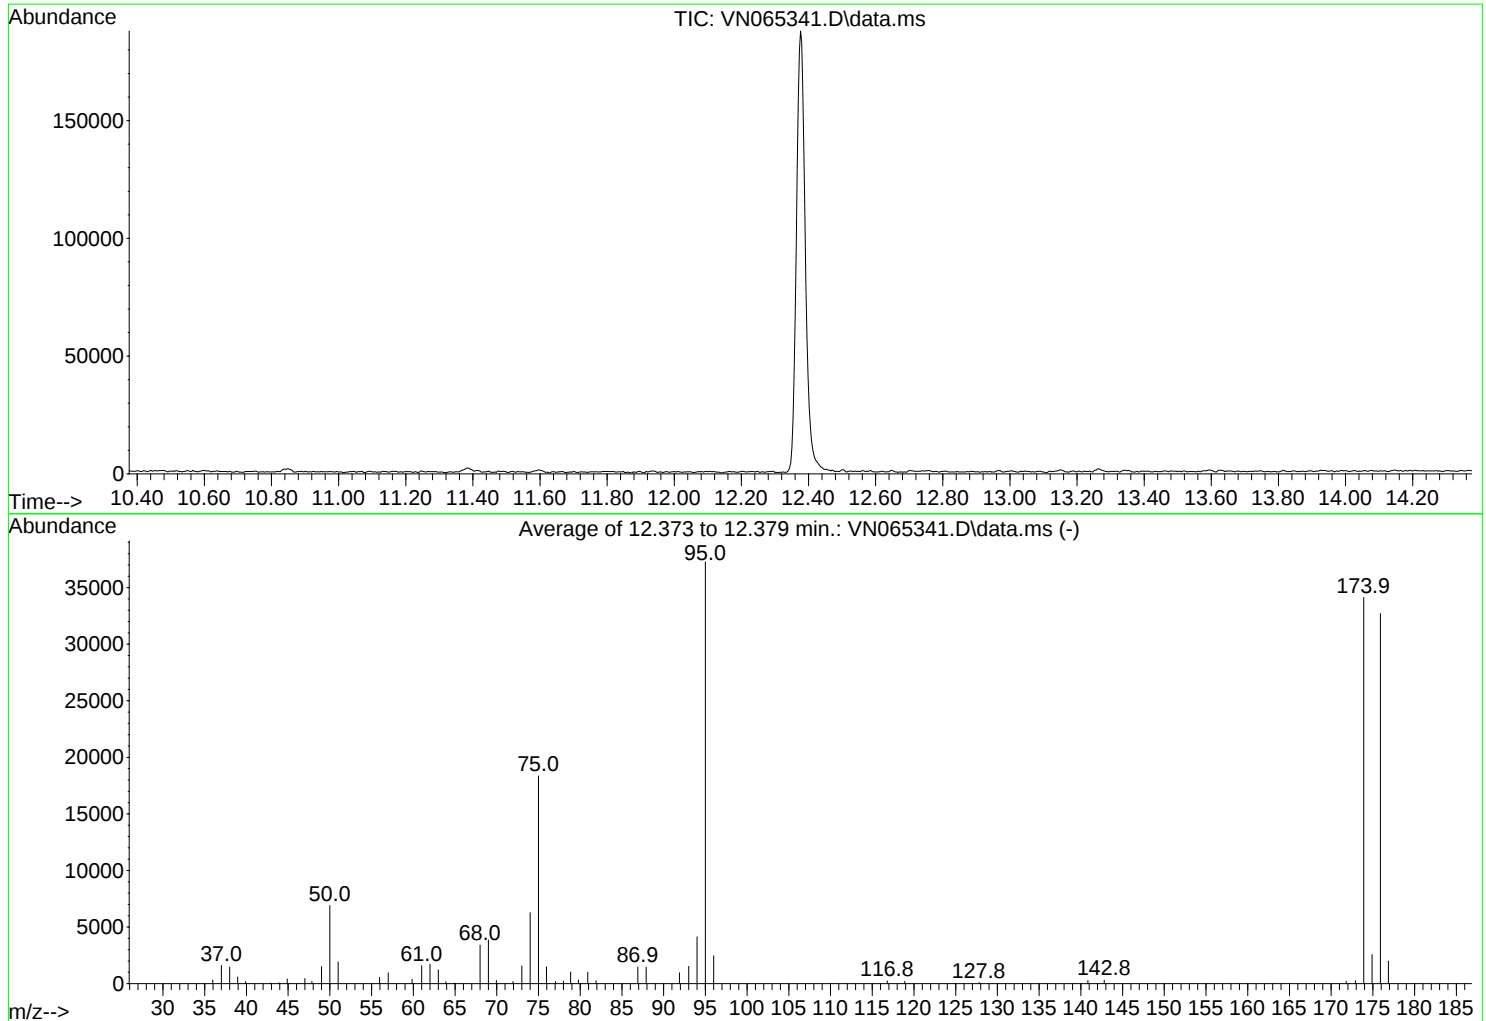

AutoFind: Scans 3307, 3308, 3309; Background Corrected with Scan 3294

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	18.5	6894	PASS
75	95	30	60	49.2	18357	PASS
95	95	100	100	100.0	37277	PASS
96	95	5	9	6.6	2454	PASS
173	174	0.00	2	0.8	266	PASS
174	95	50	100	91.6	34128	PASS
175	174	5	9	7.5	2570	PASS
176	174	95	101	95.8	32709	PASS
177	176	5	9	6.1	1988	PASS