

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN123124\
 Data File : VN085361.D
 Acq On : 31 Dec 2024 09:55
 Operator : JC\MD
 Sample : VN1231MBL01
 Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_N/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 VN1231MBL01

Quant Time: Jan 01 02:01:30 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N122724W.M
 Quant Title : SW846 8260
 QLast Update : Sat Dec 28 01:36:16 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.224	168	137413	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.100	114	259828	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.865	117	227401	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.788	152	89672	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.577	65	120959	61.717	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	=	123.440%
35) Dibromofluoromethane	8.165	113	93008	57.379	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	114.760%
50) Toluene-d8	10.565	98	316346	53.184	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	=	106.360%
62) 4-Bromofluorobenzene	12.847	95	95116	48.149	ug/l	0.00
Spiked Amount	50.000	Range	77 - 121	Recovery	=	96.300%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN123124\
Data File : VN085361.D
Acq On : 31 Dec 2024 09:55
Operator : JC\MD
Sample : VN1231MBL01
Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_N/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
VN1231MBL01


Quant Time: Jan 01 02:01:30 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N122724W.M
Quant Title : SW846 8260
QLast Update : Sat Dec 28 01:36:16 2024
Response via : Initial Calibration

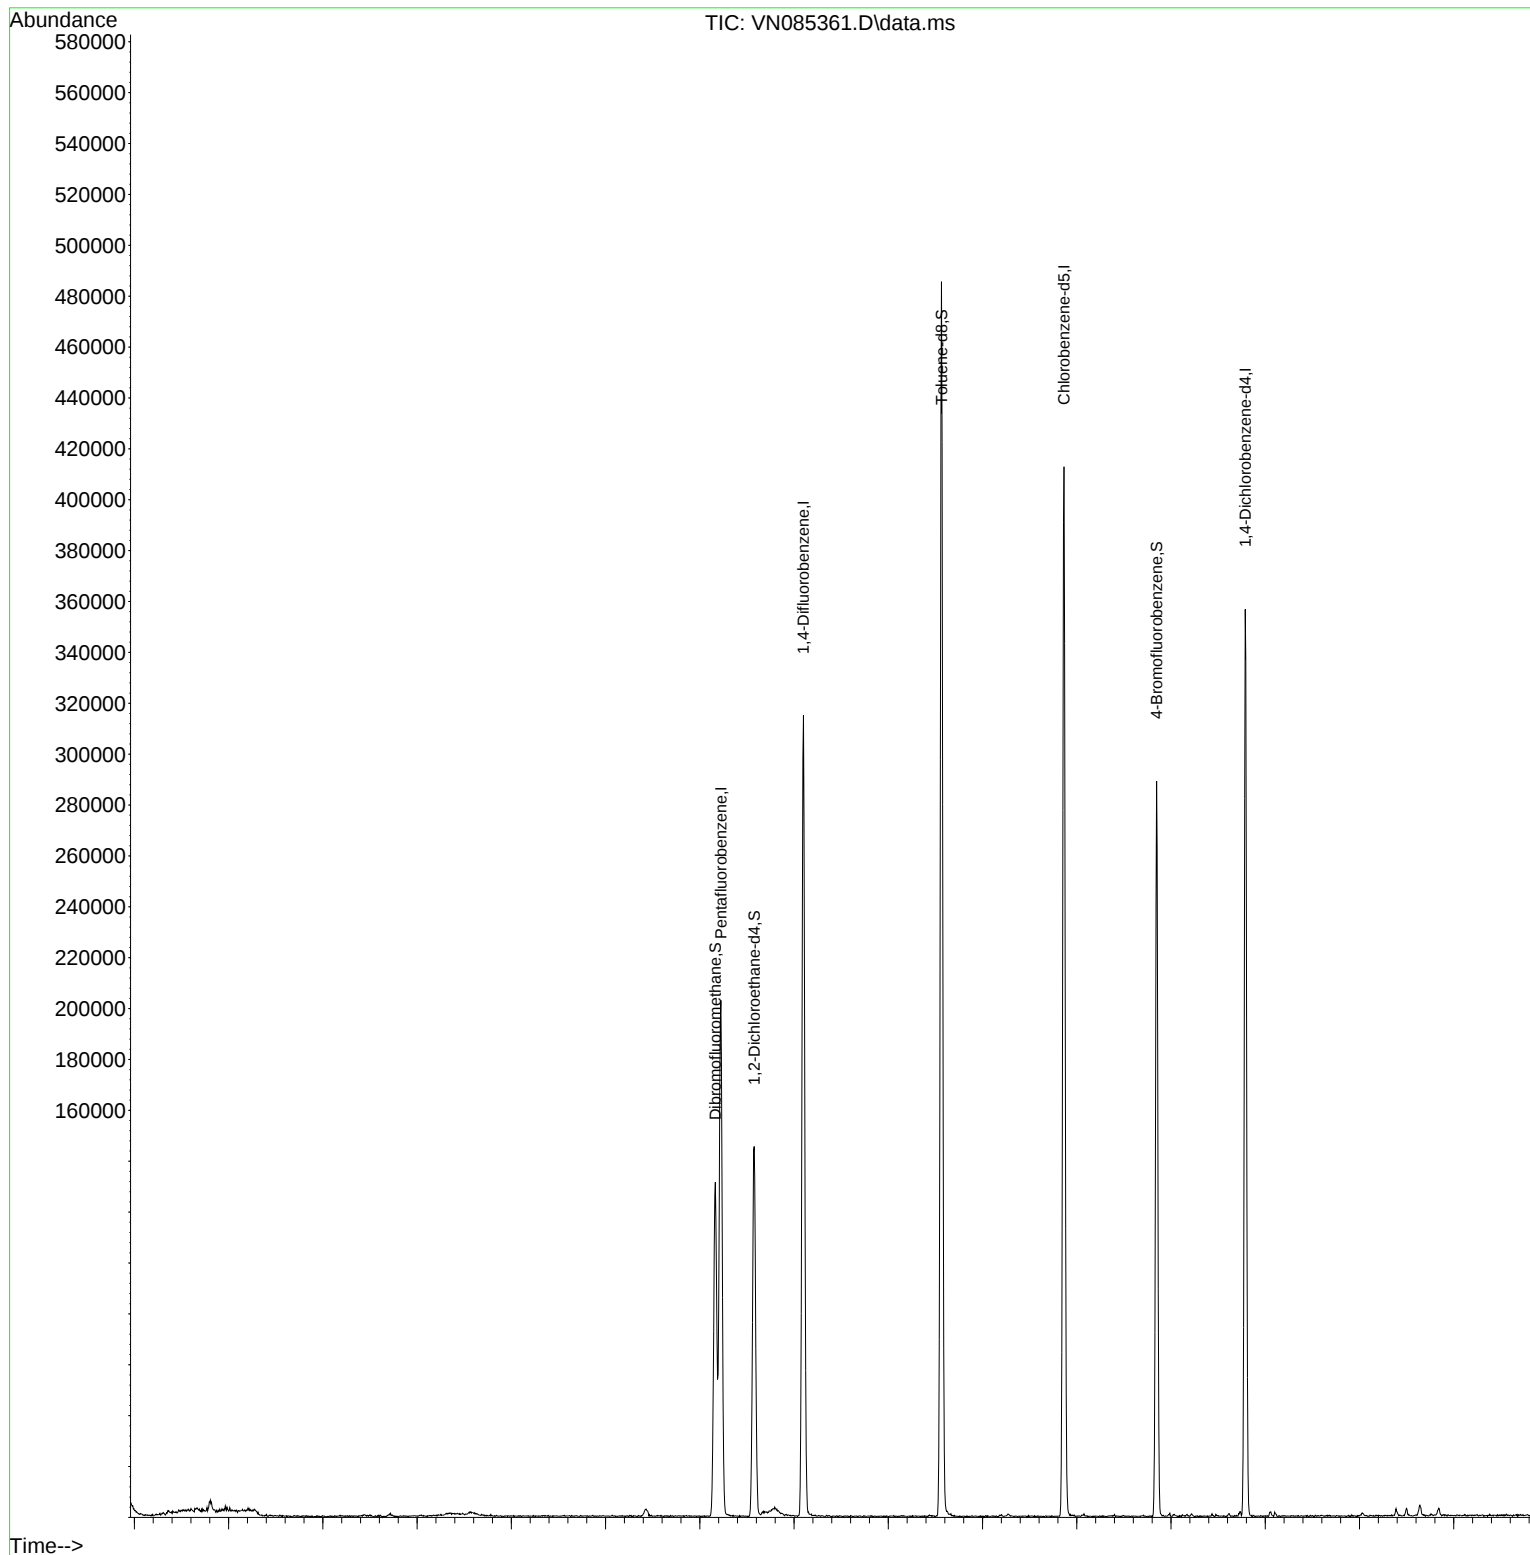



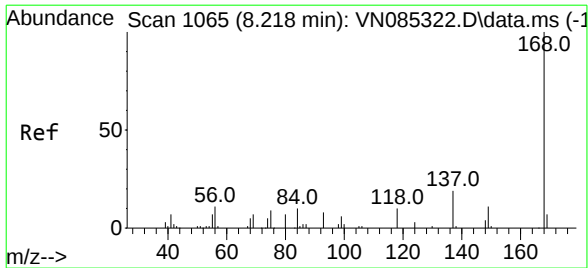


#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.224 min Scan# 1066
Delta R.T. 0.006 min
Lab File: VN085361.D
Acq: 31 Dec 2024 09:55

Instrument :
MSVOA_N
ClientSampleId :
VN1231MBL01



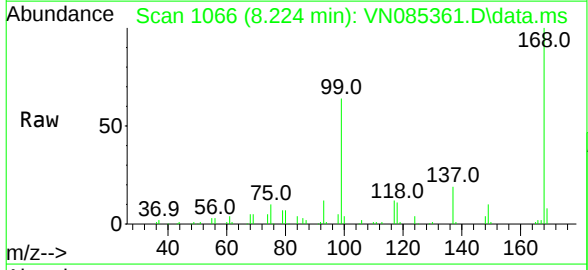



Tgt Ion:168 Resp: 137413
Ion Ratio Lower Upper
168 100
99 63.5 51.0 76.4

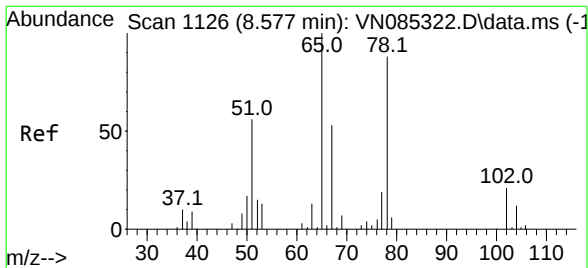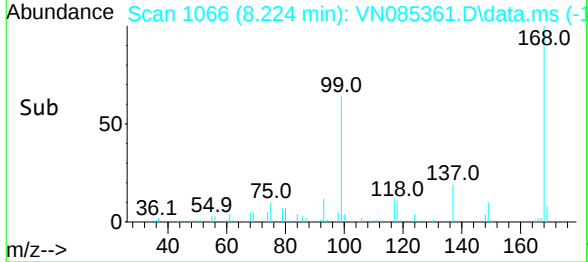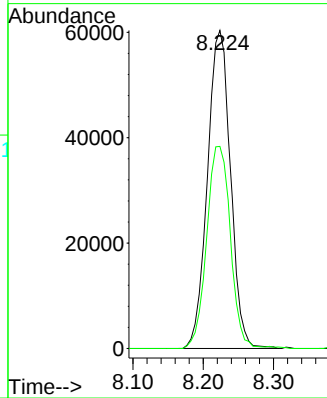

#33
1,2-Dichloroethane-d4
Concen: 61.717 ug/l
RT: 8.577 min Scan# 1126
Delta R.T. 0.000 min
Lab File: VN085361.D
Acq: 31 Dec 2024 09:55

Tgt Ion: 65 Resp: 120959
Ion Ratio Lower Upper
65 100
67 51.4 0.0 104.0


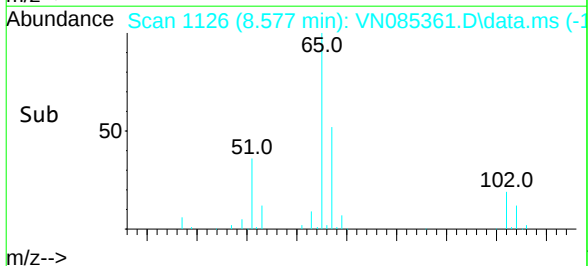
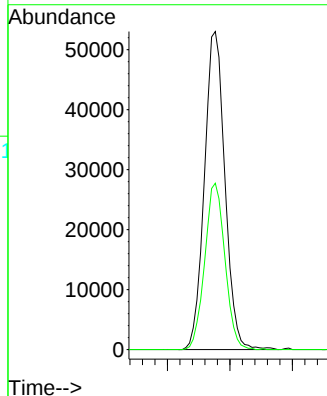
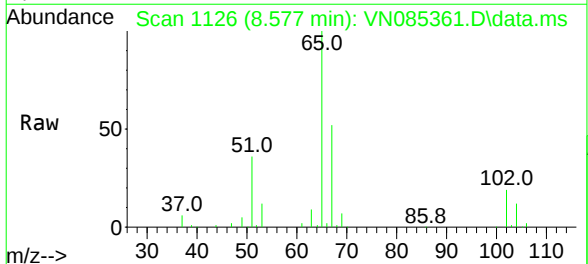


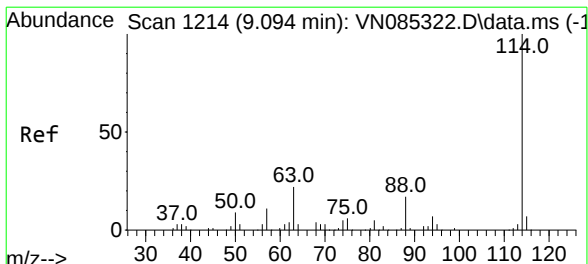

#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 9.100 min Scan# 1215
 Delta R.T. 0.006 min
 Lab File: VN085361.D
 Acq: 31 Dec 2024 09:55




Instrument :
 MSVOA_N
 ClientSampleId :
 VN1231MBL01


Tgt Ion:	114	Resp:	259828
Ion	Ratio	Lower	Upper
114	100		
63	21.6	0.0	43.4
88	15.1	0.0	33.6

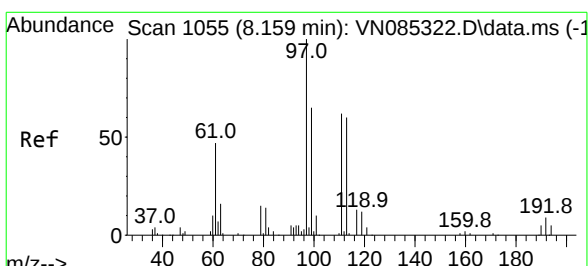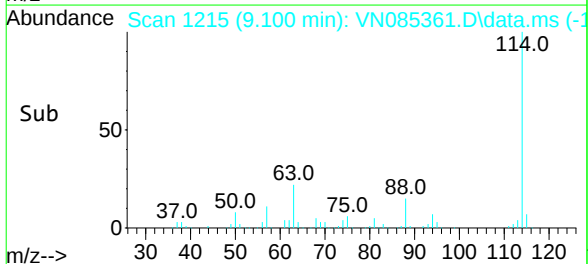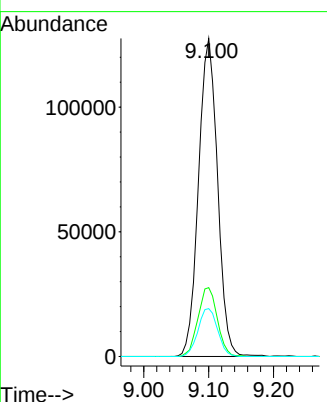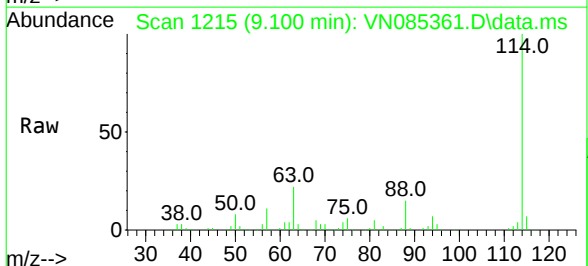

#35
 Dibromofluoromethane
 Concen: 57.379 ug/l
 RT: 8.165 min Scan# 1056
 Delta R.T. 0.006 min
 Lab File: VN085361.D
 Acq: 31 Dec 2024 09:55

Tgt Ion:	113	Resp:	93008
Ion	Ratio	Lower	Upper
113	100		
111	102.9	80.5	120.7
192	16.8	12.9	19.3

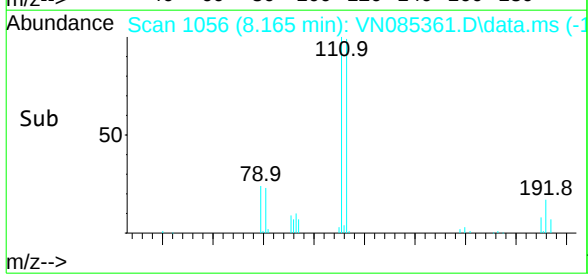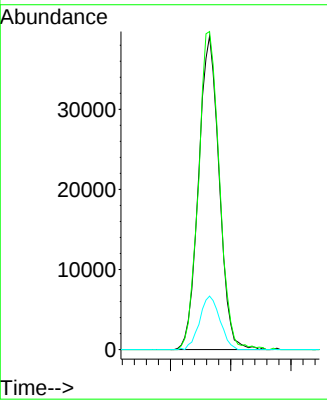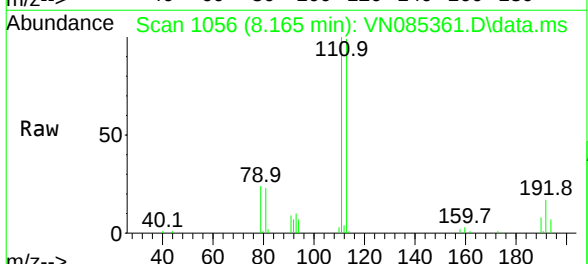

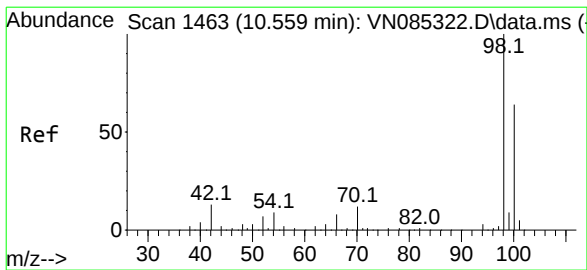

#50

Toluene-d8

Concen: 53.184 ug/l

RT: 10.565 min Scan# 1464

Delta R.T. 0.006 min

Lab File: VN085361.D

Acq: 31 Dec 2024 09:55

Instrument :

MSVOA_N

ClientSampleId :





VN1231MBL01

Tgt Ion: 98 Resp: 316346

Ion Ratio Lower Upper

98 100

100 63.9 51.5 77.3

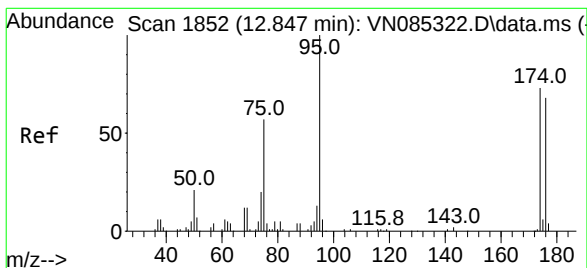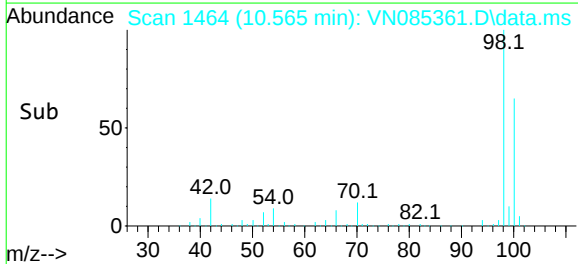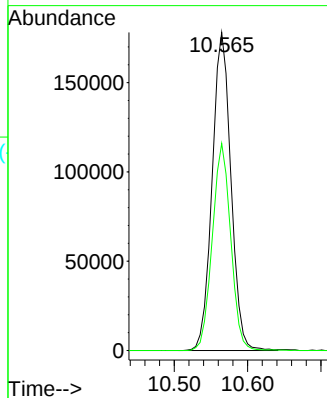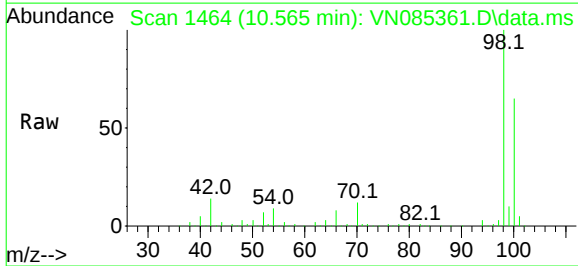

#62

4-Bromofluorobenzene

Concen: 48.149 ug/l

RT: 12.847 min Scan# 1852

Delta R.T. 0.000 min

Lab File: VN085361.D

Acq: 31 Dec 2024 09:55




Tgt Ion: 95 Resp: 95116


Ion Ratio Lower Upper

95 100

174 74.1 0.0 143.2

176 69.2 0.0 135.8


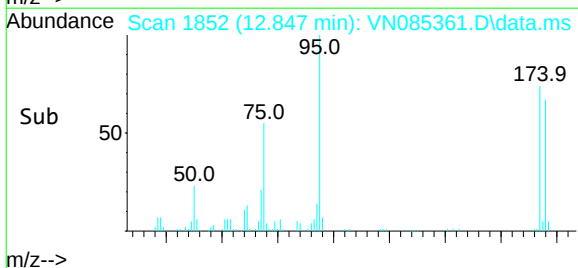
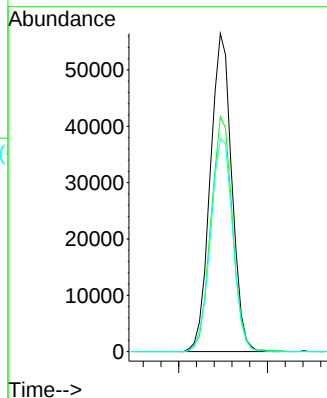
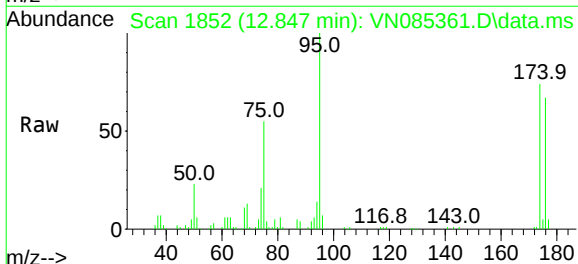


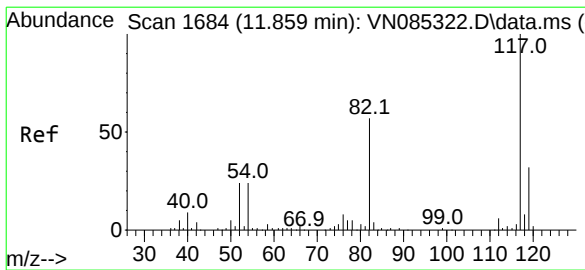

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.865 min Scan# 1684
Delta R.T. 0.006 min
Lab File: VN085361.D
Acq: 31 Dec 2024 09:55

Instrument :
MSVOA_N
ClientSampleId :
VN1231MBL01

Tgt Ion:117 Resp: 227401
Ion Ratio Lower Upper
117 100
82 57.2 45.7 68.5
119 31.3 25.8 38.8

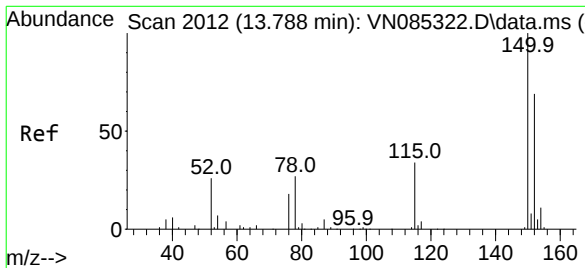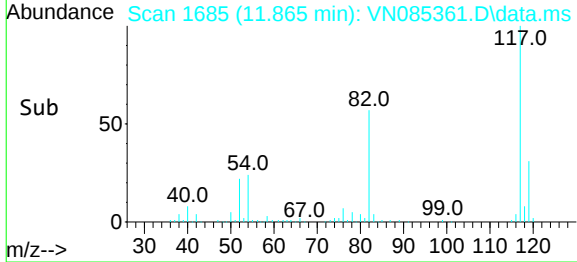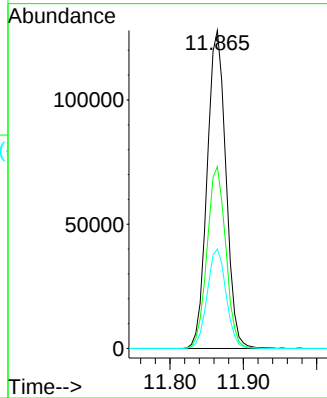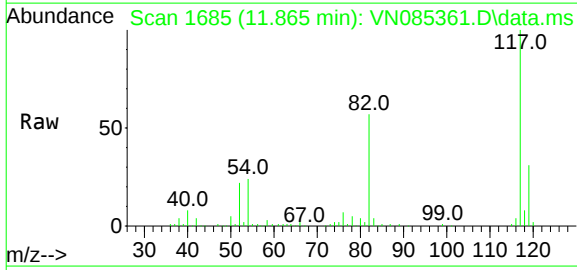

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.788 min Scan# 2012
Delta R.T. 0.000 min
Lab File: VN085361.D
Acq: 31 Dec 2024 09:55

Tgt Ion:152 Resp: 89672
Ion Ratio Lower Upper
152 100
115 62.0 30.4 91.3
150 159.8 0.0 345.0

