
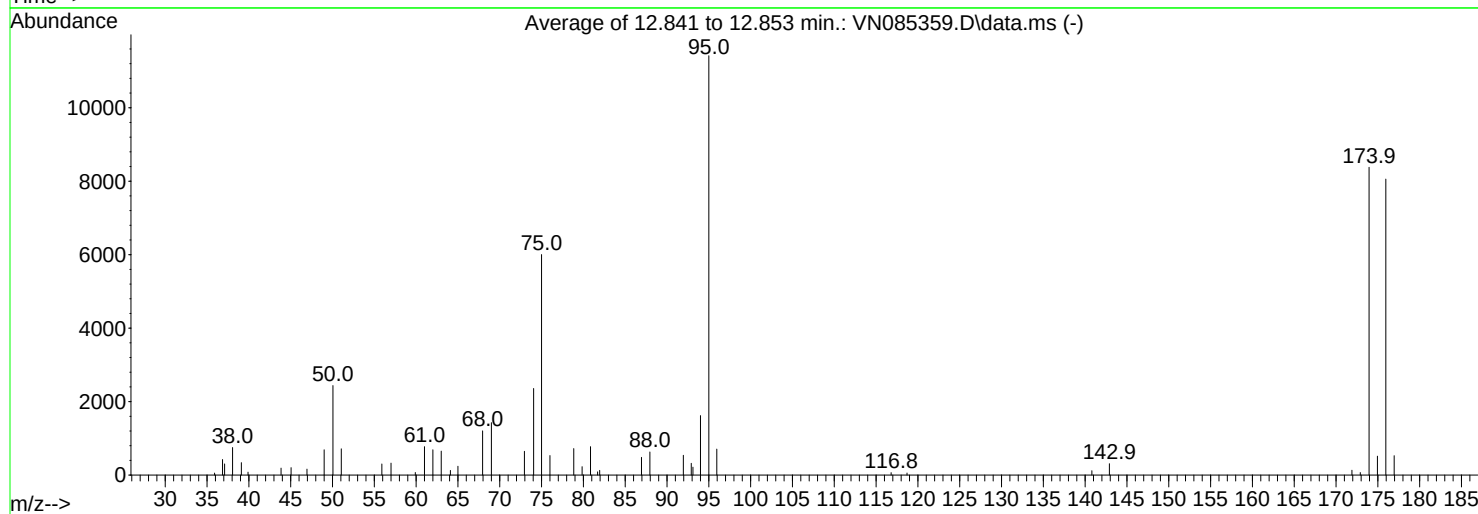


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN123124\
Data File : VN085359.D
Acq On : 31 Dec 2024 08:44
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N122724W.M
Title : SW846 8260
Last Update : Sat Dec 28 01:36:16 2024

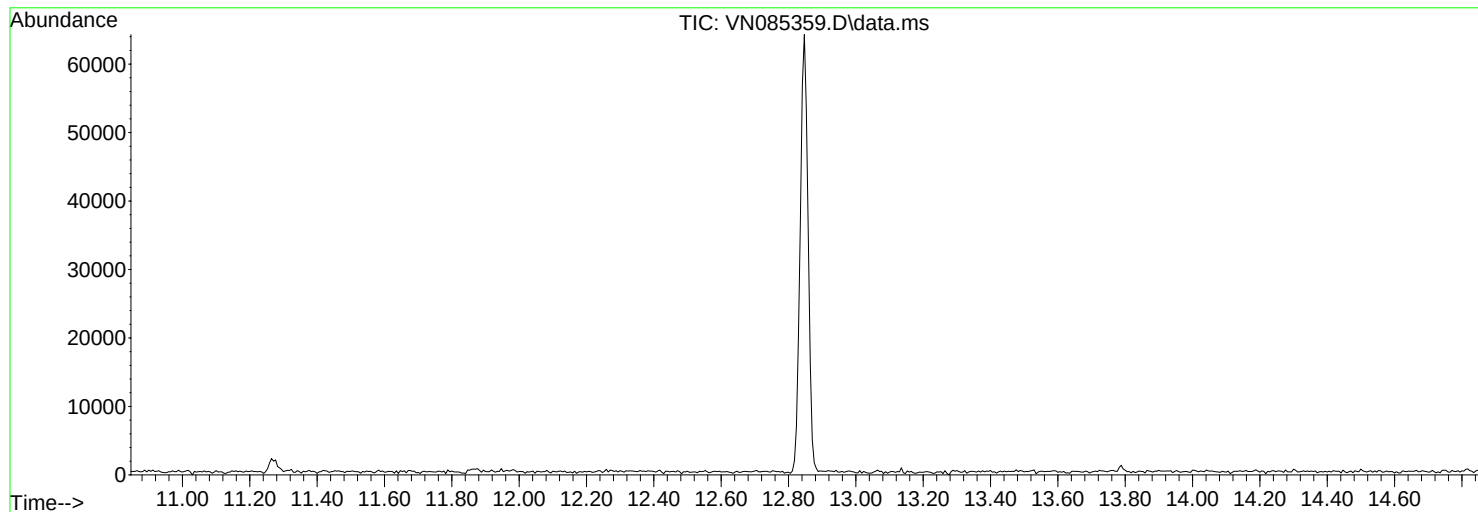

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1844

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.3	2437	PASS
75	95	30	60	52.6	6003	PASS
95	95	100	100	100.0	11416	PASS
96	95	5	9	6.2	707	PASS
173	174	0.00	2	0.8	69	PASS
174	95	50	100	73.4	8379	PASS
175	174	5	9	6.1	515	PASS
176	174	95	101	96.2	8058	PASS
177	176	5	9	6.6	528	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.90	55	51.05	715	72.95	647	91.95	539
36.85	423	55.90	302	74.05	2357	92.90	320
37.10	303	57.00	325	75.00	6003	93.10	216
38.05	750	59.90	70	76.00	532	94.00	1619
39.10	339	61.00	774	78.85	721	95.00	11416
39.90	80	62.00	689	79.85	229	95.95	707
43.85	190	63.00	652	80.85	774	116.80	67
45.05	202	64.10	127	81.70	88	118.70	56
46.95	162	65.00	241	81.95	128	140.80	119
49.00	689	67.95	1203	86.95	482	142.90	310
50.05	2437	69.00	1427	87.95	629	171.90	132

Average of 12.841 to 12.853 min.: VN085359.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
172.90	69						
173.95	8379						
174.95	515						
175.95	8058						
176.95	528						

Instrument :

MSVOA_N

ClientSampleId :

BFB