

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN032223\
 Data File : VN077097.D
 Acq On : 22 Mar 2023 10:40
 Operator : JC\MD
 Sample : VN0322MBL01
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 VN0322MBL01

Quant Time: Mar 22 23:19:15 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N031723W.M
 Quant Title : SW846 8260
 QLast Update : Mon Mar 20 08:50:30 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	8.230	168	342546	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.107	114	630503	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.866	117	547598	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.795	152	202247	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.583	65	276746	50.579	ug/l	0.00
Spiked Amount 50.000	Range 74 - 125		Recovery = 101.160%			
35) Dibromofluoromethane	8.172	113	202365	45.831	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery = 91.660%			
50) Toluene-d8	10.571	98	755620	47.907	ug/l	0.00
Spiked Amount 50.000	Range 86 - 113		Recovery = 95.820%			
62) 4-Bromofluorobenzene	12.854	95	249029	44.681	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery = 89.360%			
Target Compounds						Qvalue
5) Bromomethane	2.984	94	1748	0.695	ug/l	99
6) Chloroethane	3.148	64	510	0.216	ug/l #	42
10) Methyl Iodide	4.613	142	2465	0.481	ug/l #	91
11) Tert butyl alcohol	5.501	59	173	0.217	ug/l #	72
13) Acrolein	4.195	56	968	0.982	ug/l #	62
15) Acrylonitrile	5.742	53	1710	0.638	ug/l #	80
16) Acetone	4.454	43	1075	0.441	ug/l	97
17) Carbon Disulfide	4.737	76	4240	0.350	ug/l #	84
20) Methylene Chloride	5.289	84	1119	0.211	ug/l #	77
25) 2-Butanone	7.501	43	1339	0.375	ug/l #	84
31) Cyclohexane	8.230	56	8904	0.995	ug/l #	1
36) 1,1-Dichloropropene	8.236	75	33238	4.819	ug/l #	51
38) Carbon Tetrachloride	8.225	117	39716	5.912	ug/l #	16
43) Isopropyl Acetate	8.777	43	6266	0.544	ug/l #	56
51) 4-Methyl-2-Pentanone	10.442	43	2073	0.289	ug/l #	61
59) 2-Hexanone	11.207	43	4863	0.934	ug/l	88
74) N-amyl acetate	12.501	43	2310	0.294	ug/l #	78
76) 1,2,3-Trichloropropane	12.854	75	134277	25.668	ug/l #	1
77) Bromobenzene	12.983	156	844	0.208	ug/l	77
81) trans-1,4-Dichloro-2-b...	12.854	75	134277	70.651	ug/l #	10
82) 4-Chlorotoluene	13.224	91	3170	0.250	ug/l	94
87) 1,3-Dichlorobenzene	13.736	146	2221	0.289	ug/l	96
88) 1,4-Dichlorobenzene	13.736	146	2221	0.291	ug/l	96
89) n-Butylbenzene	14.059	91	3297	0.259	ug/l	91
91) 1,2-Dichlorobenzene	14.112	146	2674	0.350	ug/l	86
92) 1,2-Dibromo-3-Chloropr...	14.724	75	397	0.326	ug/l #	74
93) 1,2,4-Trichlorobenzene	15.406	180	2863	0.828	ug/l	94
95) Naphthalene	15.648	128	12448	2.803	ug/l	98
96) 1,2,3-Trichlorobenzene	15.842	180	3712	1.070	ug/l	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN032223\
Data File : VN077097.D
Acq On : 22 Mar 2023 10:40
Operator : JC\MD
Sample : VN0322MBL01
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
VN0322MBL01

Quant Time: Mar 22 23:19:15 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N031723W.M
Quant Title : SW846 8260
QLast Update : Mon Mar 20 08:50:30 2023
Response via : Initial Calibration

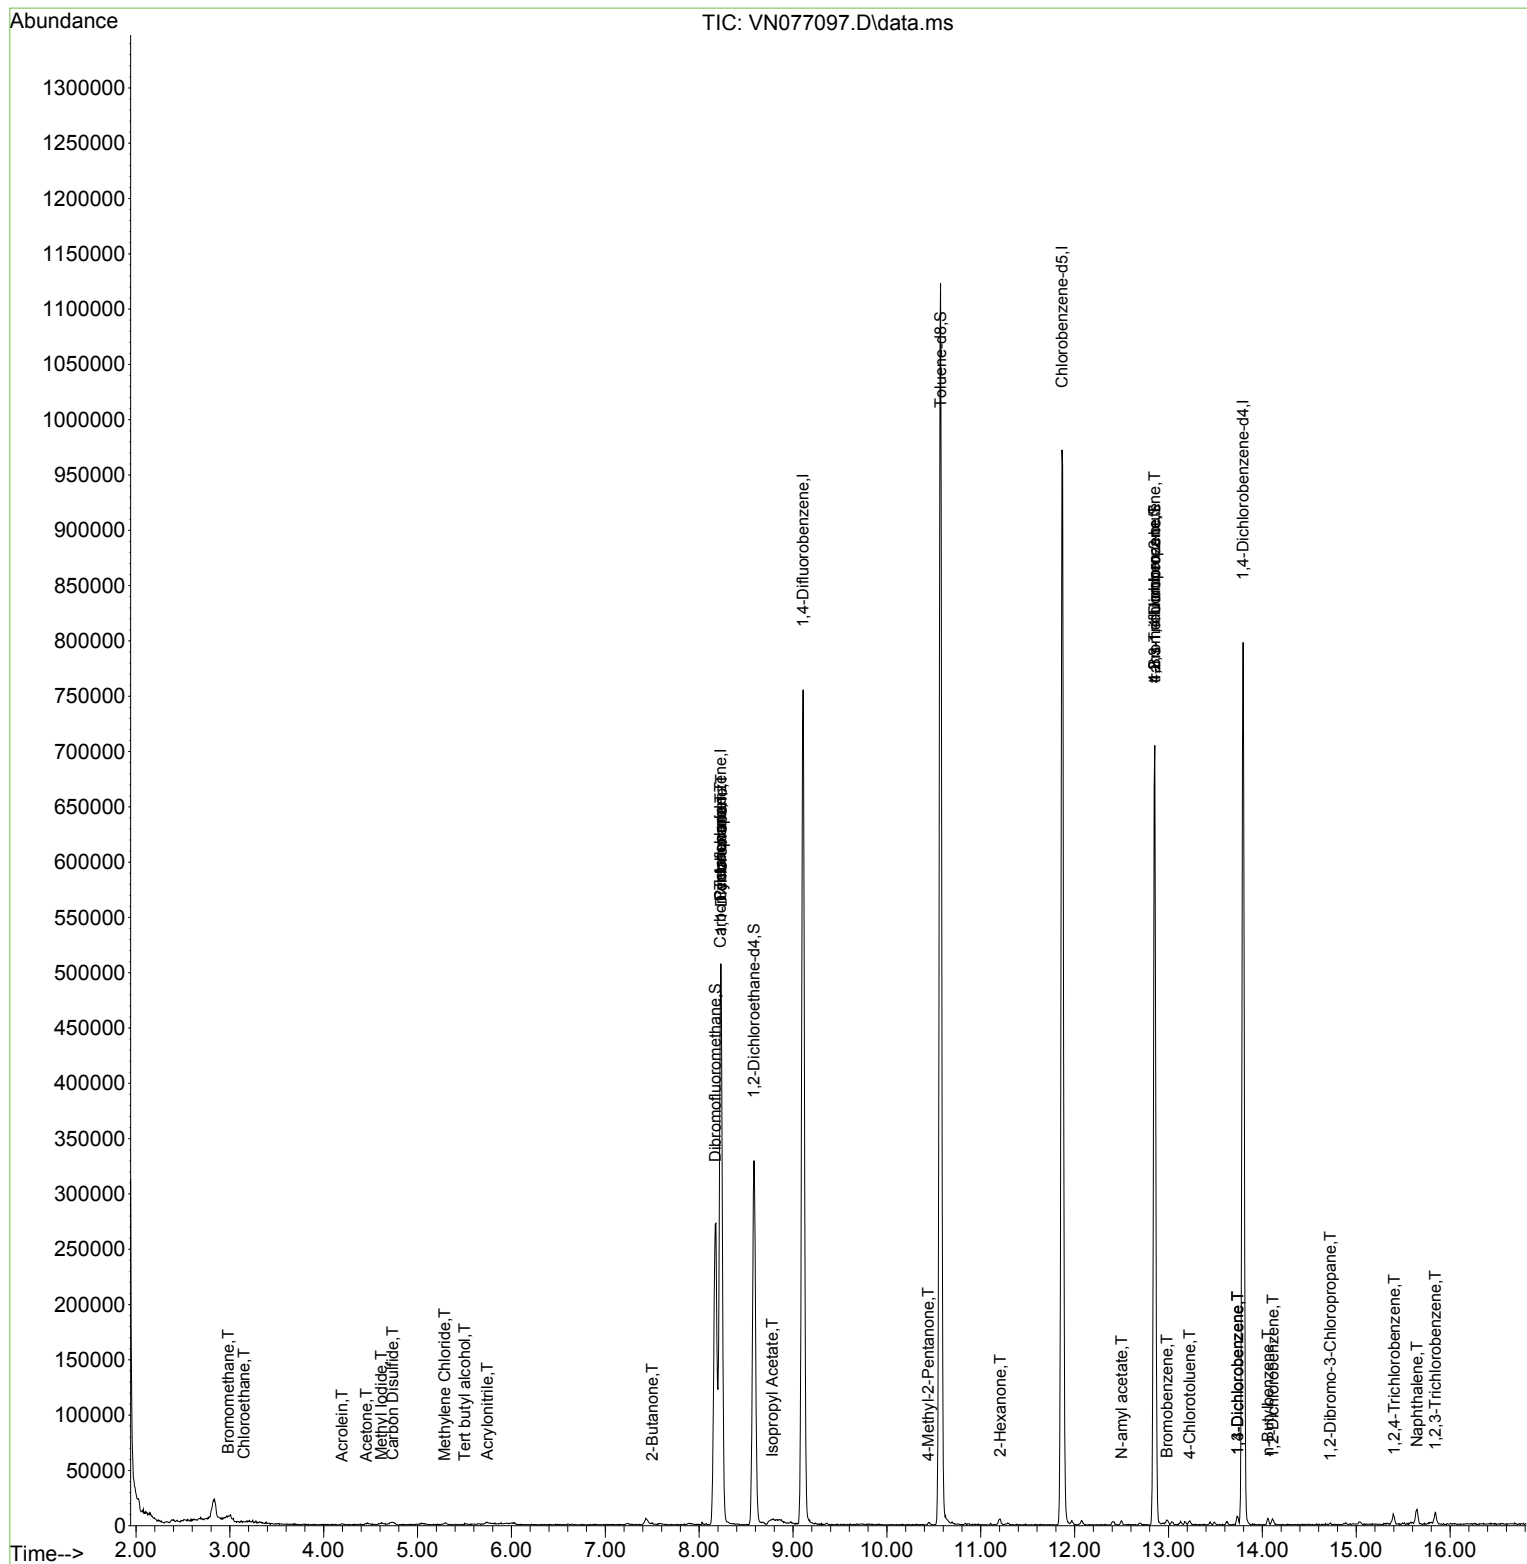



#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 8.230 min Scan# 1

Delta R.T. -0.001 min

Lab File: VN077097.D

Acq: 22 Mar 2023 10:40

Instrument :

MSVOA_N

ClientSampleId :





VN0322MBL01

Tgt Ion:168 Resp: 342546

Ion Ratio Lower Upper

168 100

99 66.9 53.9 80.9

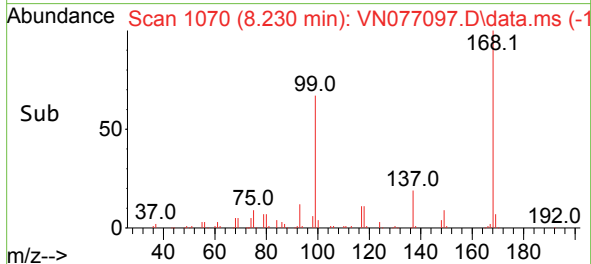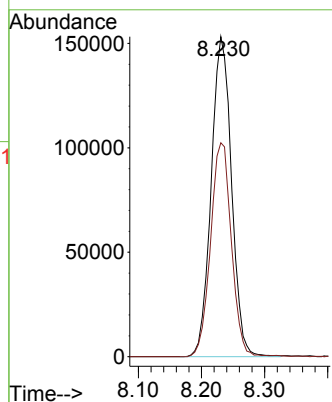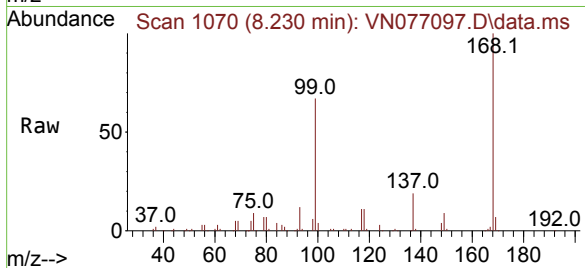

#5

Bromomethane

Concen: 0.695 ug/l

RT: 2.984 min Scan# 178

Delta R.T. 0.035 min

Lab File: VN077097.D




Acq: 22 Mar 2023 10:40


Tgt Ion: 94 Resp: 1748

Ion Ratio Lower Upper

94 100

96 93.8 74.1 111.1


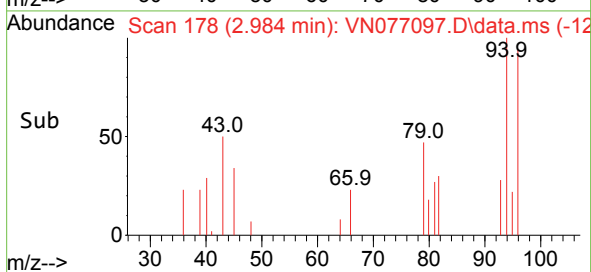
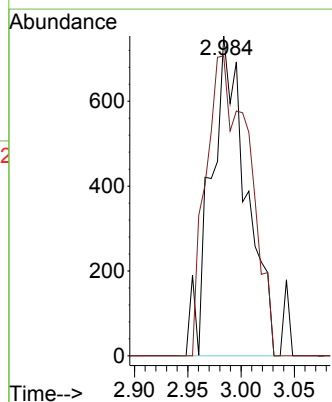
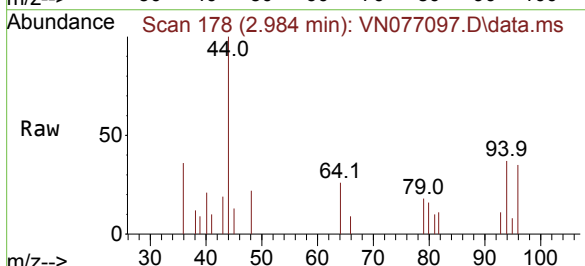


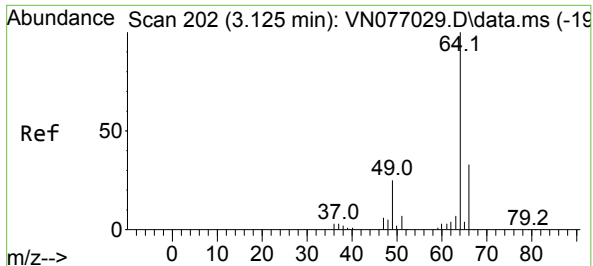

#6
Chloroethane
Concen: 0.216 ug/l
RT: 3.148 min Scan# 206
Delta R.T. 0.023 min
Lab File: VN077097.D
Acq: 22 Mar 2023 10:40




Instrument :
MSVOA_N
ClientSampleId :
VN0322MBL01


Tgt Ion: 64 Resp: 510
Ion Ratio Lower Upper
64 100
66 0.0 26.3 39.5#

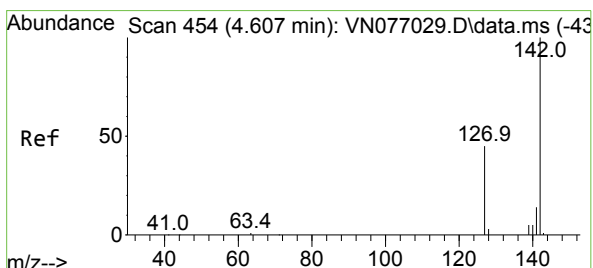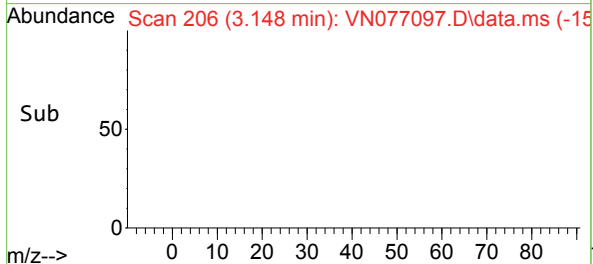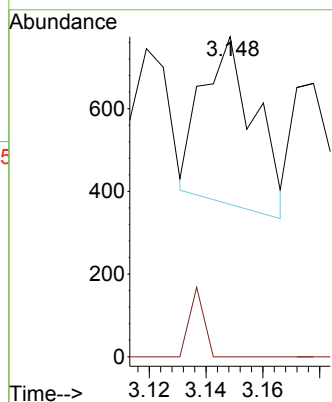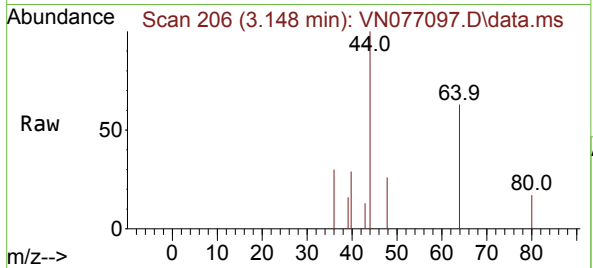

#10
Methyl Iodide
Concen: 0.481 ug/l
RT: 4.613 min Scan# 455
Delta R.T. 0.006 min
Lab File: VN077097.D
Acq: 22 Mar 2023 10:40

Tgt Ion: 142 Resp: 2465
Ion Ratio Lower Upper
142 100
127 50.9 36.1 54.1
141 17.2 10.8 16.2#


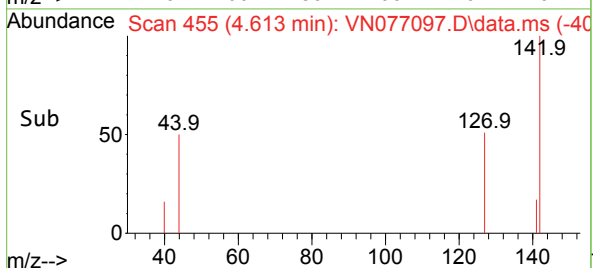

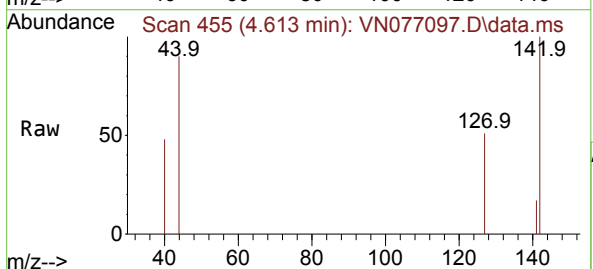




#11
Tert butyl alcohol
Concen: 0.217 ug/l
RT: 5.501 min Scan# 60
Delta R.T. -0.036 min
Lab File: VN077097.D
Acq: 22 Mar 2023 10:40




Instrument :
MSVOA_N
ClientSampleId :
VN0322MBL01


Tgt Ion: 59 Resp: 173
Ion Ratio Lower Upper
59 100
57 0.0 8.6 12.8#

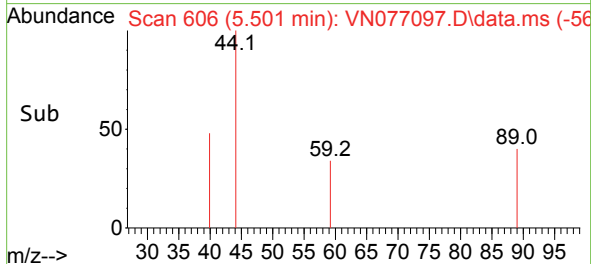

#13
Acrolein
Concen: 0.982 ug/l
RT: 4.195 min Scan# 384
Delta R.T. 0.005 min
Lab File: VN077097.D
Acq: 22 Mar 2023 10:40

Tgt Ion: 56 Resp: 968
Ion Ratio Lower Upper
56 100
55 39.7 57.0 85.6#


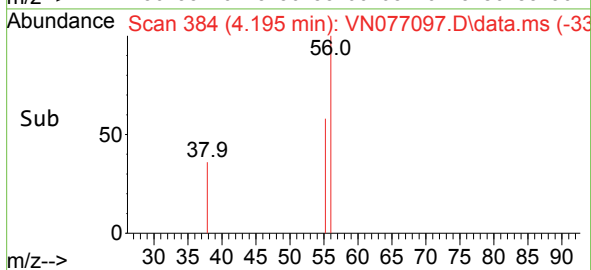

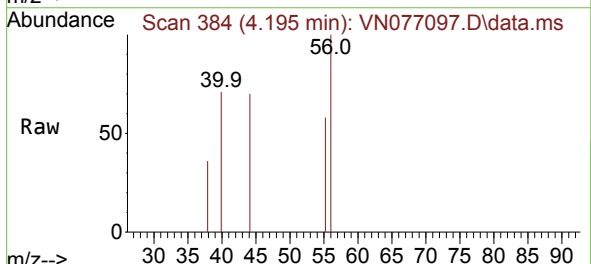




#15
Acrylonitrile
Concen: 0.638 ug/l
RT: 5.742 min Scan# 645
Delta R.T. 0.011 min
Lab File: VN077097.D
Acq: 22 Mar 2023 10:40




Instrument :
MSVOA_N
ClientSampleId :
VN0322MBL01


Tgt Ion: 53 Resp: 1710
Ion Ratio Lower Upper
53 100
52 94.1 64.6 97.0
51 17.1 28.3 42.5#

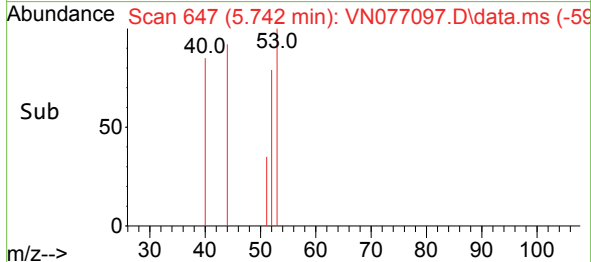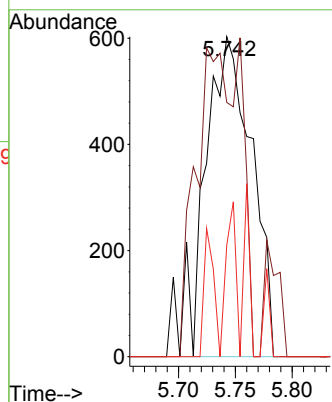

#16
Acetone
Concen: 0.441 ug/l
RT: 4.454 min Scan# 428
Delta R.T. 0.017 min
Lab File: VN077097.D
Acq: 22 Mar 2023 10:40

Tgt Ion: 43 Resp: 1075
Ion Ratio Lower Upper
43 100
58 30.1 25.4 38.0


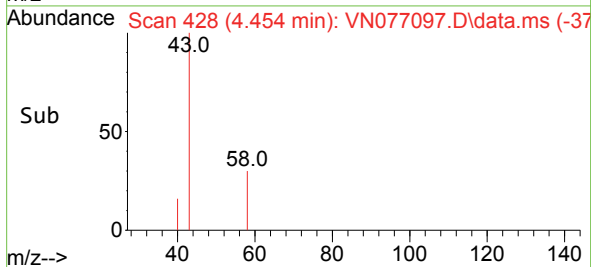

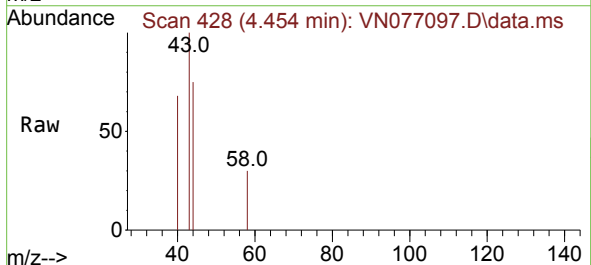




#17
Carbon Disulfide
Concen: 0.350 ug/l
RT: 4.737 min Scan# 41
Delta R.T. 0.012 min
Lab File: VN077097.D
Acq: 22 Mar 2023 10:40




Instrument :
MSVOA_N
ClientSampleId :
VN0322MBL01


Tgt Ion: 76 Resp: 4240
Ion Ratio Lower Upper
76 100
78 13.9 6.6 10.0#

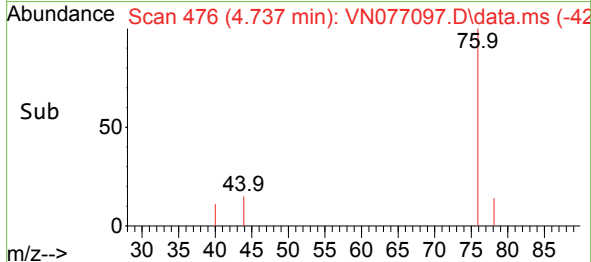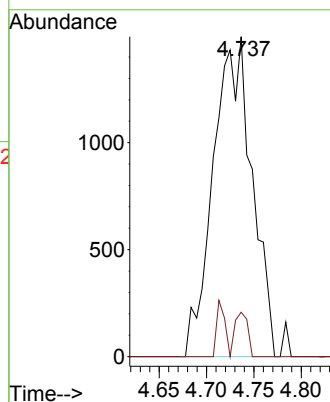

#20
Methylene Chloride
Concen: 0.211 ug/l
RT: 5.289 min Scan# 570
Delta R.T. -0.001 min
Lab File: VN077097.D
Acq: 22 Mar 2023 10:40

Tgt Ion: 84 Resp: 1119
Ion Ratio Lower Upper
84 100
49 146.4 103.8 155.6
51 0.0 32.3 48.5#
86 51.3 49.9 74.9


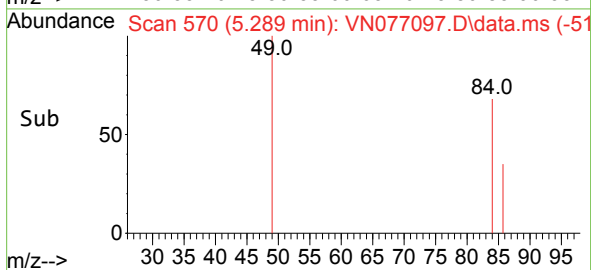

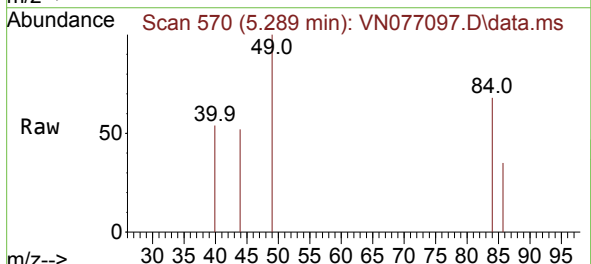


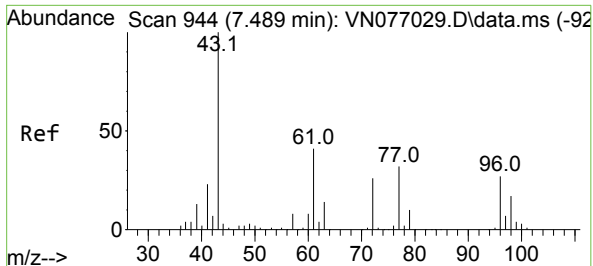

#25
2-Butanone
Concen: 0.375 ug/l
RT: 7.501 min Scan# 94
Delta R.T. 0.012 min
Lab File: VN077097.D
Acq: 22 Mar 2023 10:40




Instrument :
MSVOA_N
ClientSampleId :
VN0322MBL01


Tgt Ion: 43 Resp: 1339
Ion Ratio Lower Upper
43 100
72 34.1 20.7 31.1#

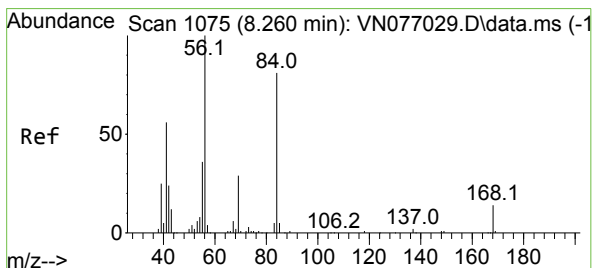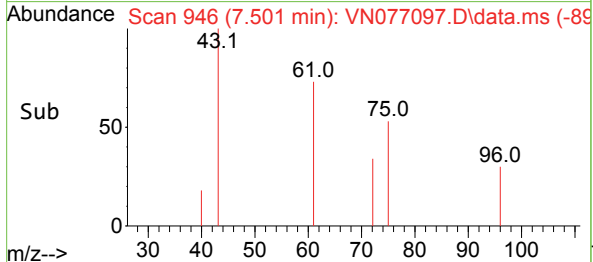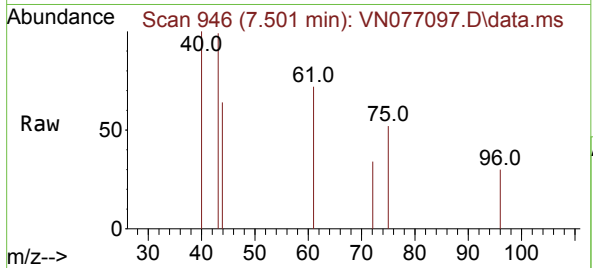

#31
Cyclohexane
Concen: 0.995 ug/l
RT: 8.230 min Scan# 1070
Delta R.T. -0.030 min
Lab File: VN077097.D
Acq: 22 Mar 2023 10:40

Tgt Ion: 56 Resp: 8904
Ion Ratio Lower Upper
56 100
69 189.7 22.8 34.2#
84 148.9 64.7 97.1#

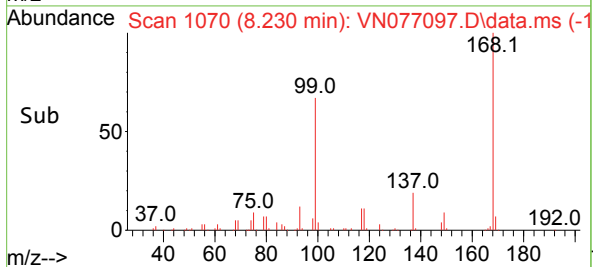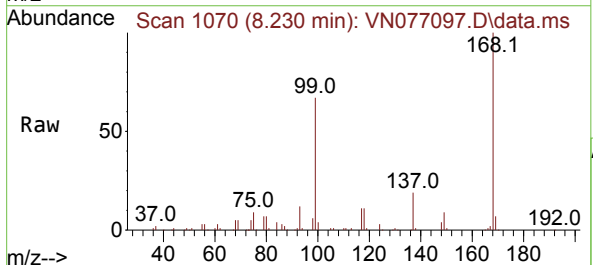



#33

1,2-Dichloroethane-d4

Concen: 50.579 ug/l

RT: 8.583 min Scan# 1130

Delta R.T. 0.000 min

Lab File: VN077097.D

Acq: 22 Mar 2023 10:40

Instrument :

MSVOA_N

ClientSampleId :





VN0322MBL01

Tgt Ion: 65 Resp: 276746

Ion Ratio Lower Upper

65 100

67 51.9 0.0 105.2

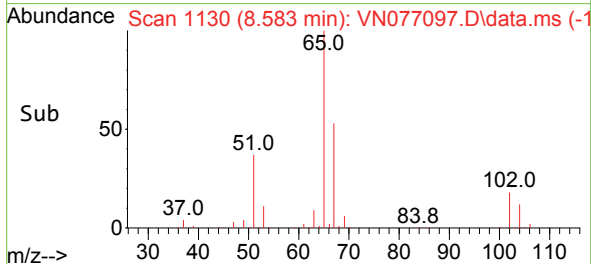

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 9.107 min Scan# 1219

Delta R.T. -0.000 min

Lab File: VN077097.D

Acq: 22 Mar 2023 10:40




Tgt Ion: 114 Resp: 630503


Ion Ratio Lower Upper

114 100

63 24.4 0.0 44.6

88 17.9 0.0 33.8


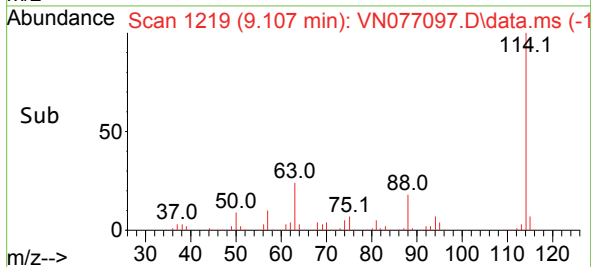

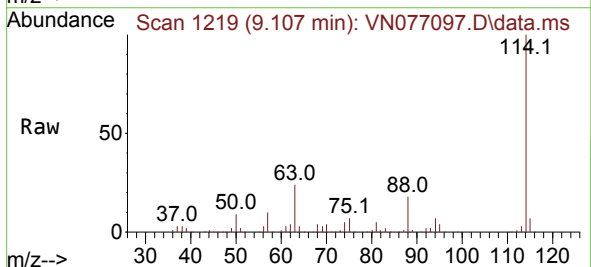




#35
Dibromofluoromethane
Concen: 45.831 ug/l
RT: 8.172 min Scan# 1070
Delta R.T. -0.000 min
Lab File: VN077097.D
Acq: 22 Mar 2023 10:40




Instrument :
MSVOA_N
ClientSampleId :
VN0322MBL01


Tgt Ion:113 Resp: 202365
Ion Ratio Lower Upper
113 100
111 103.2 82.2 123.2
192 16.0 13.0 19.6

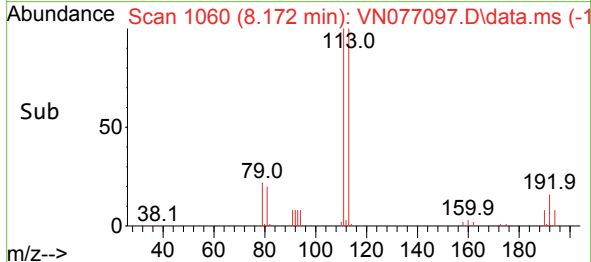

#36
1,1-Dichloropropene
Concen: 4.819 ug/l
RT: 8.236 min Scan# 1071
Delta R.T. -0.141 min
Lab File: VN077097.D
Acq: 22 Mar 2023 10:40

Tgt Ion: 75 Resp: 33238
Ion Ratio Lower Upper
75 100
110 8.1 15.9 47.7#
77 0.0 24.3 36.5#

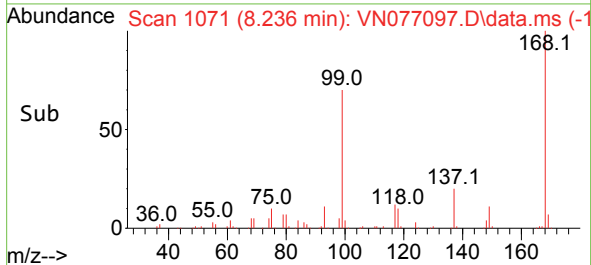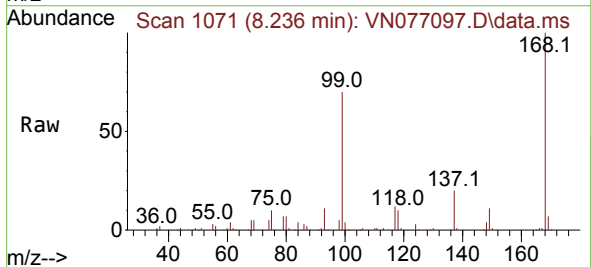



#38

Carbon Tetrachloride

Concen: 5.912 ug/l

RT: 8.225 min Scan# 1106

Delta R.T. -0.141 min

Lab File: VN077097.D


Acq: 22 Mar 2023 10:40

Instrument :

MSVOA_N

ClientSampleId :

VN0322MBL01






Tgt Ion:117 Resp: 39716

Ion Ratio Lower Upper

117 100

119 6.0 78.2 117.2#

121 0.0 23.2 34.8#

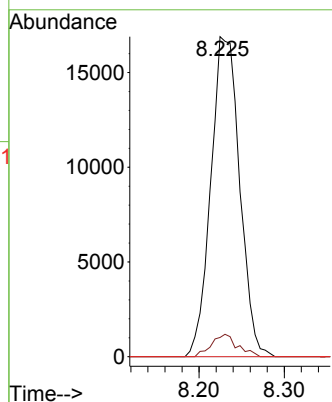

#43

Isopropyl Acetate

Concen: 0.544 ug/l

RT: 8.777 min Scan# 1163

Delta R.T. 0.082 min

Lab File: VN077097.D

Acq: 22 Mar 2023 10:40




Tgt Ion: 43 Resp: 6266


Ion Ratio Lower Upper

43 100

61 0.0 20.6 30.8#

87 0.0 10.0 15.0#


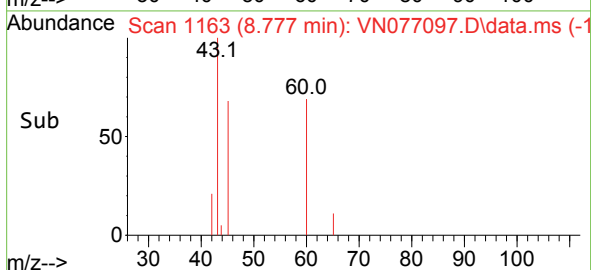






#50
Toluene-d8
Concen: 47.907 ug/l
RT: 10.571 min Scan# 1468
Delta R.T. -0.000 min
Lab File: VN077097.D
Acq: 22 Mar 2023 10:40




Instrument :
MSVOA_N
ClientSampleId :
VN0322MBL01


Tgt Ion: 98 Resp: 755620
Ion Ratio Lower Upper
98 100
100 65.5 51.6 77.4

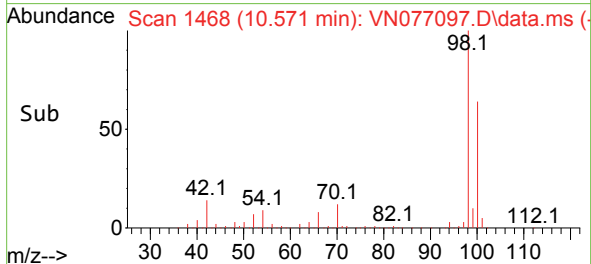

#51
4-Methyl-2-Pentanone
Concen: 0.289 ug/l
RT: 10.442 min Scan# 1446
Delta R.T. -0.006 min
Lab File: VN077097.D
Acq: 22 Mar 2023 10:40

Tgt Ion: 43 Resp: 2073
Ion Ratio Lower Upper
43 100
58 15.3 31.1 46.7#


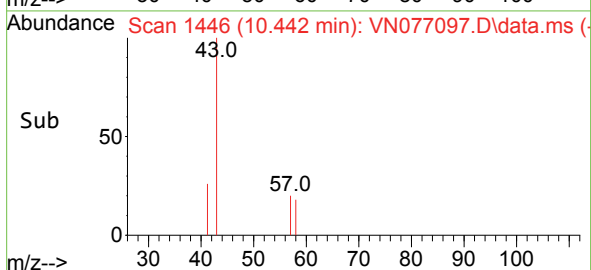




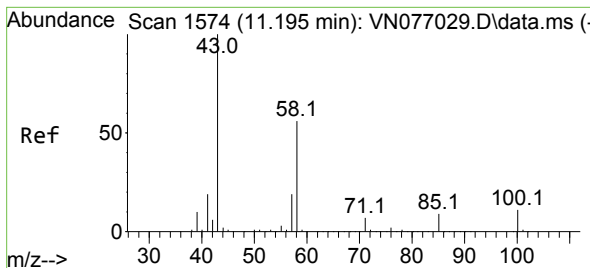

#59
2-Hexanone
Concen: 0.934 ug/l
RT: 11.207 min Scan# 1576
Delta R.T. 0.012 min
Lab File: VN077097.D
Acq: 22 Mar 2023 10:40




Instrument :
MSVOA_N
ClientSampleId :
VN0322MBL01


Tgt Ion: 43 Resp: 4863
Ion Ratio Lower Upper
43 100
58 46.9 27.7 83.1

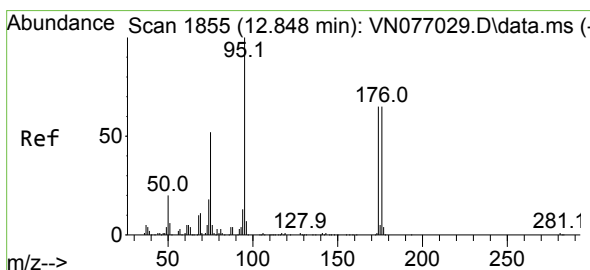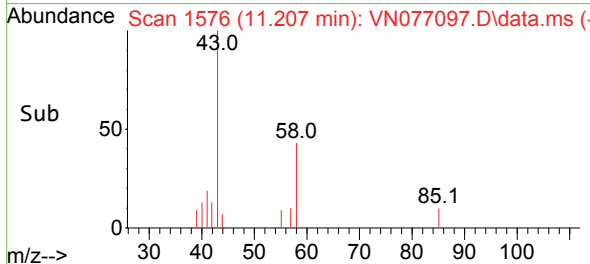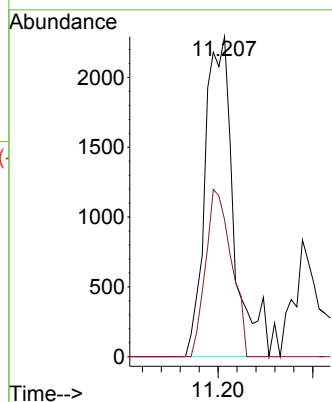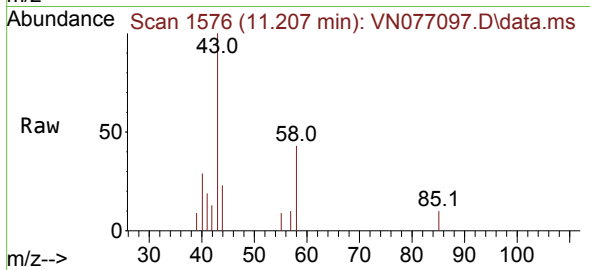

#62
4-Bromofluorobenzene
Concen: 44.681 ug/l
RT: 12.854 min Scan# 1856
Delta R.T. 0.006 min
Lab File: VN077097.D
Acq: 22 Mar 2023 10:40

Tgt Ion: 95 Resp: 249029
Ion Ratio Lower Upper
95 100
174 67.6 0.0 136.6
176 65.2 0.0 130.0


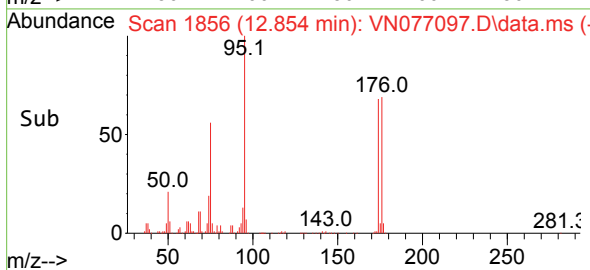
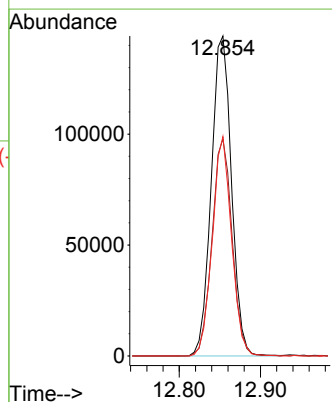
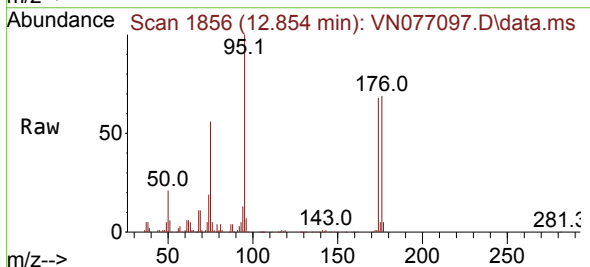




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.866 min Scan# 117
Delta R.T. -0.000 min
Lab File: VN077097.D
Acq: 22 Mar 2023 10:40




Instrument :
MSVOA_N
ClientSampleId :
VN0322MBL01


Tgt Ion:117 Resp: 547598
Ion Ratio Lower Upper
117 100
82 62.1 49.4 74.0
119 32.9 26.5 39.7

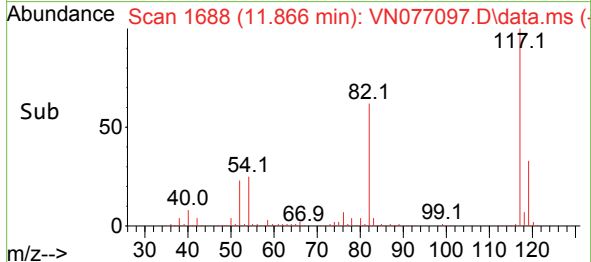

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.795 min Scan# 2016
Delta R.T. -0.000 min
Lab File: VN077097.D
Acq: 22 Mar 2023 10:40

Tgt Ion:152 Resp: 202247
Ion Ratio Lower Upper
152 100
115 65.4 31.9 95.7
150 158.9 0.0 348.0

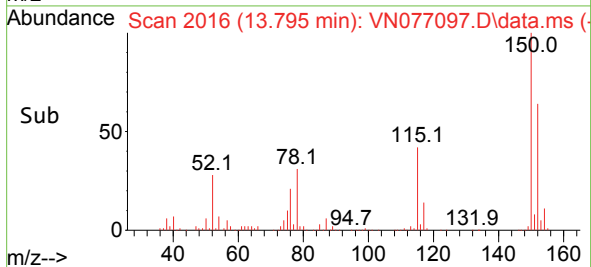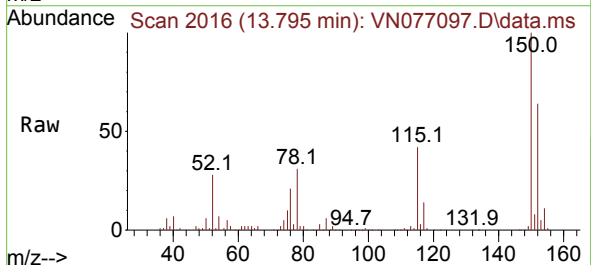

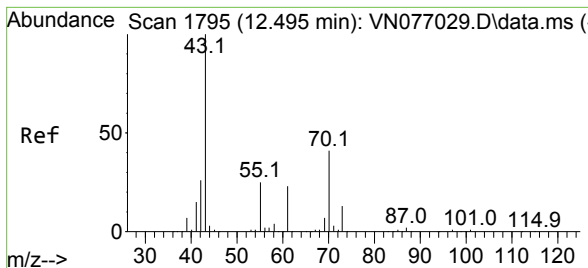

#74

N-ethyl acetate

Concen: 0.294 ug/l

RT: 12.501 min Scan# 1

Delta R.T. 0.006 min

Lab File: VN077097.D

Acq: 22 Mar 2023 10:40

Instrument :

MSVOA_N

ClientSampleId :

VN0322MBL01

Tgt Ion: 43 Resp: 2310





Ion Ratio Lower Upper

43 100

70 27.9 33.6 50.4#

55 17.8 20.3 30.5#

61 9.0 18.9 28.3#

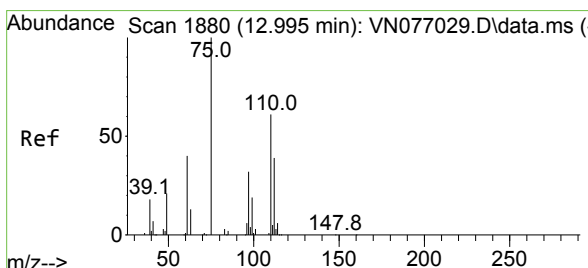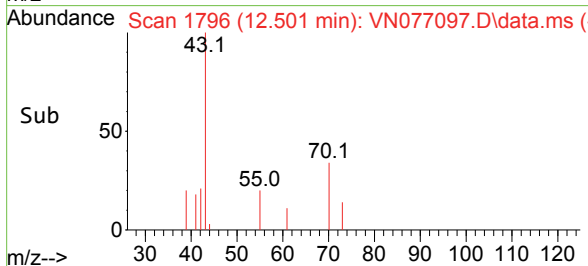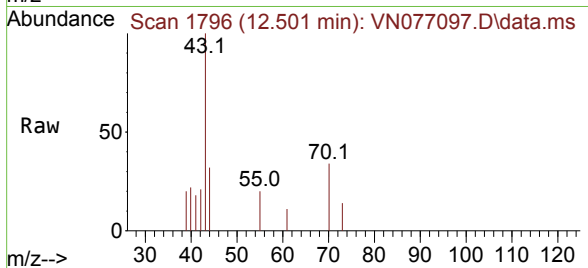

#76

1,2,3-Trichloropropane

Concen: 25.668 ug/l

RT: 12.854 min Scan# 1856

Delta R.T. -0.141 min

Lab File: VN077097.D




Acq: 22 Mar 2023 10:40


Tgt Ion: 75 Resp: 134277

Ion Ratio Lower Upper

75 100

77 1.2 107.3 322.0#


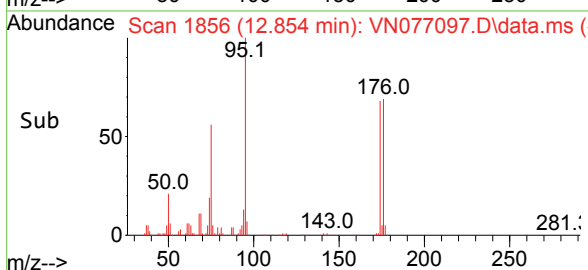

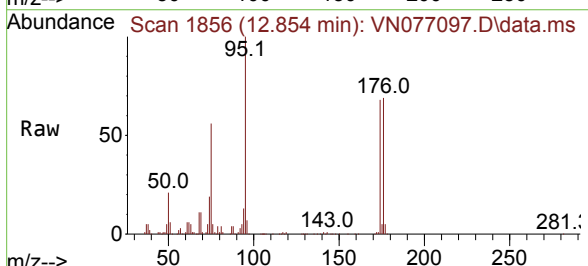




#77
Bromobenzene
Concen: 0.208 ug/l
RT: 12.983 min Scan# 1878
Delta R.T. 0.000 min
Lab File: VN077097.D
Acq: 22 Mar 2023 10:40




Instrument :
MSVOA_N
ClientSampleId :
VN0322MBL01


Tgt Ion:156 Resp: 844
Ion Ratio Lower Upper
156 100
77 285.2 124.8 374.3
158 126.3 48.6 145.9

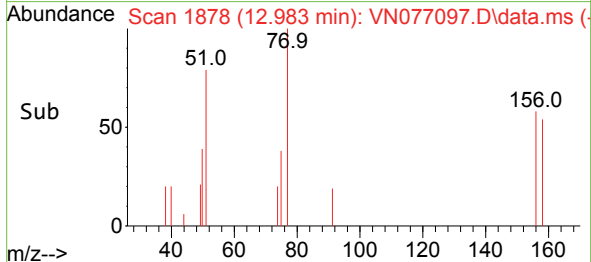

#81
trans-1,4-Dichloro-2-butene
Concen: 70.651 ug/l
RT: 12.854 min Scan# 1856
Delta R.T. 0.118 min
Lab File: VN077097.D
Acq: 22 Mar 2023 10:40

Tgt Ion: 75 Resp: 134277
Ion Ratio Lower Upper
75 100
53 0.0 80.8 121.2#
89 0.1 34.2 51.4#


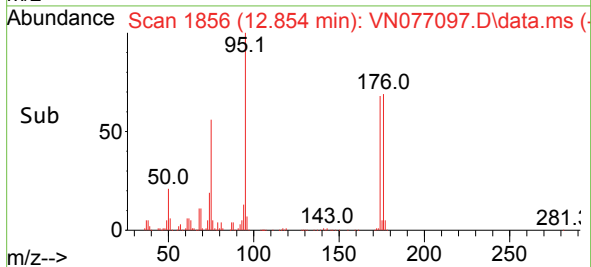

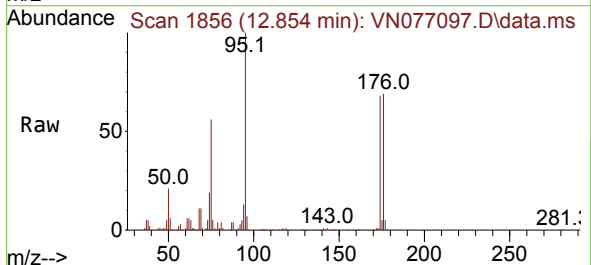




#82
4-Chlorotoluene
Concen: 0.250 ug/l
RT: 13.224 min Scan# 1919
Delta R.T. -0.000 min
Lab File: VN077097.D
Acq: 22 Mar 2023 10:40




Instrument :
MSVOA_N
ClientSampleId :
VN0322MBL01


Tgt Ion: 91 Resp: 3170
Ion Ratio Lower Upper
91 100
126 34.4 15.5 46.5

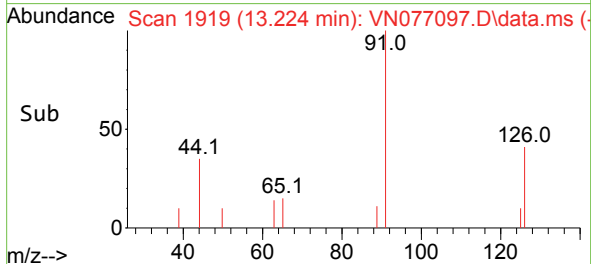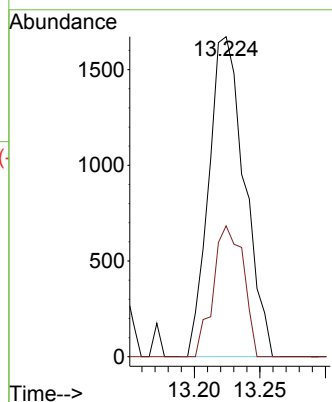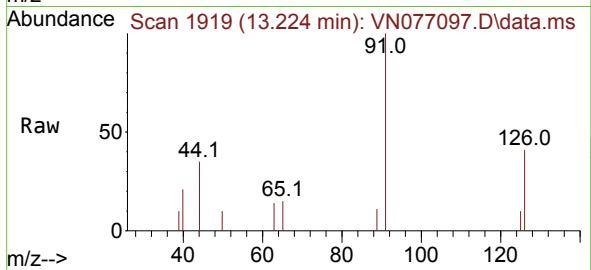

#87
1,3-Dichlorobenzene
Concen: 0.289 ug/l
RT: 13.736 min Scan# 2006
Delta R.T. -0.000 min
Lab File: VN077097.D
Acq: 22 Mar 2023 10:40

Tgt Ion: 146 Resp: 2221
Ion Ratio Lower Upper
146 100
111 42.7 21.9 65.5
148 68.8 32.1 96.5


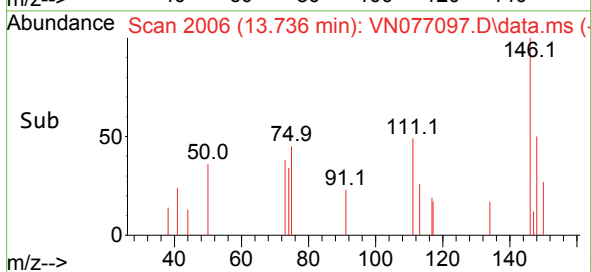
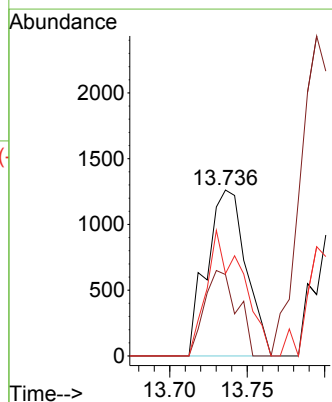
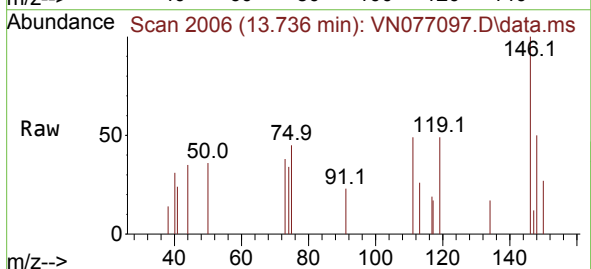




#88
1,4-Dichlorobenzene
Concen: 0.291 ug/l
RT: 13.736 min Scan# 2006
Delta R.T. -0.077 min
Lab File: VN077097.D
Acq: 22 Mar 2023 10:40




Instrument :
MSVOA_N
ClientSampleId :
VN0322MBL01


Tgt Ion:146 Resp: 2221
Ion Ratio Lower Upper
146 100
111 42.7 21.5 64.5
148 68.8 31.9 95.9

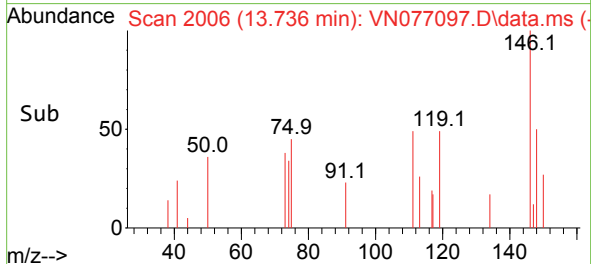

#89
n-Butylbenzene
Concen: 0.259 ug/l
RT: 14.059 min Scan# 2061
Delta R.T. -0.001 min
Lab File: VN077097.D
Acq: 22 Mar 2023 10:40

Tgt Ion: 91 Resp: 3297
Ion Ratio Lower Upper
91 100
92 56.3 26.5 79.5
134 32.8 11.7 35.1


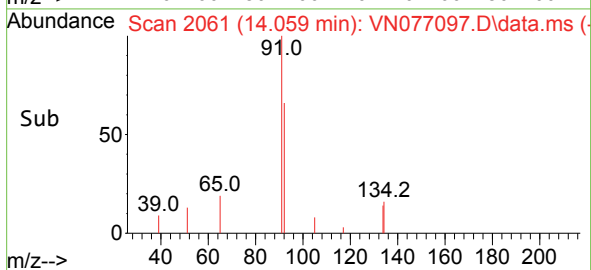

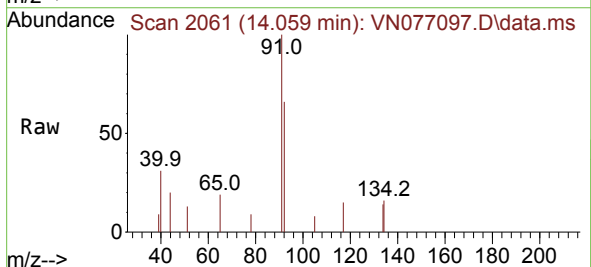




#91
1,2-Dichlorobenzene
Concen: 0.350 ug/l
RT: 14.112 min Scan# 2069
Delta R.T. 0.005 min
Lab File: VN077097.D
Acq: 22 Mar 2023 10:40




Instrument :
MSVOA_N
ClientSampleId :
VN0322MBL01


Tgt Ion:146 Resp: 2674
Ion Ratio Lower Upper
146 100
111 41.4 22.6 67.7
148 47.8 31.6 95.0

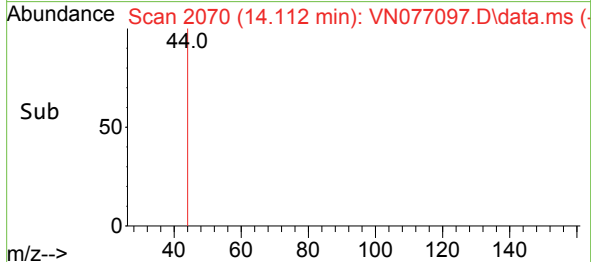

#92
1,2-Dibromo-3-Chloropropane
Concen: 0.326 ug/l
RT: 14.724 min Scan# 2174
Delta R.T. 0.000 min
Lab File: VN077097.D
Acq: 22 Mar 2023 10:40

Tgt Ion: 75 Resp: 397
Ion Ratio Lower Upper
75 100
155 30.7 36.1 108.3#
157 98.2 45.8 137.3

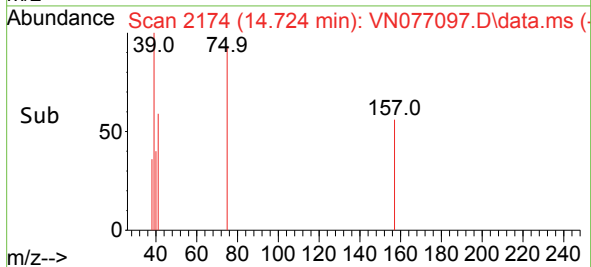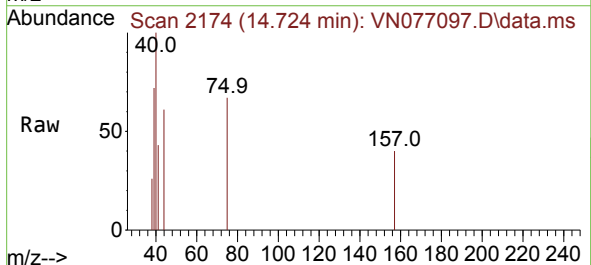

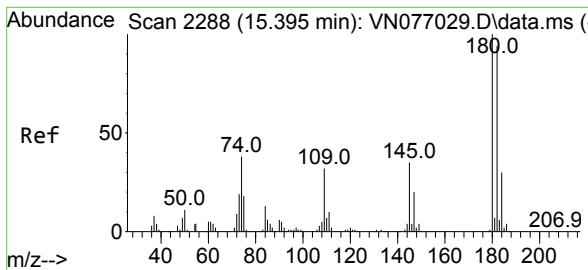

#93

1,2,4-Trichlorobenzene

Concen: 0.828 ug/l

RT: 15.406 min Scan# 21

Delta R.T. 0.011 min

Lab File: VN077097.D

Acq: 22 Mar 2023 10:40

Instrument :

MSVOA_N

ClientSampleId :

VN0322MBL01





Tgt Ion:180 Resp: 2863

Ion Ratio Lower Upper

180 100

182 101.3 47.3 141.9

145 36.4 16.9 50.7

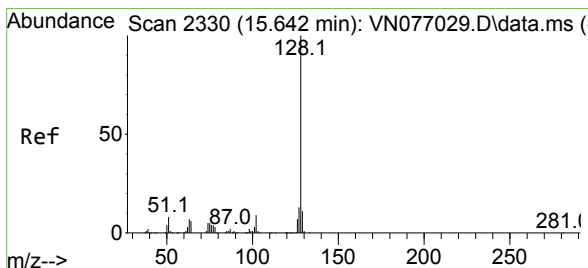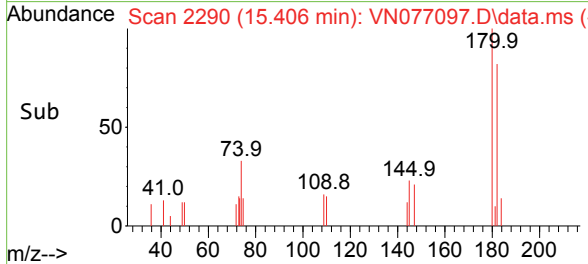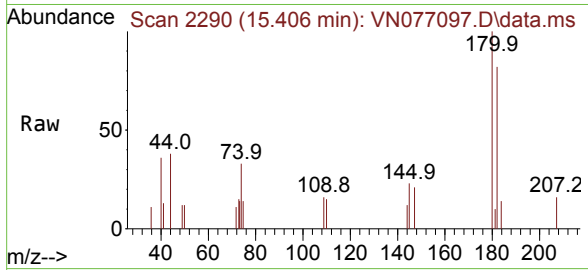

#95

Naphthalene

Concen: 2.803 ug/l

RT: 15.648 min Scan# 2331

Delta R.T. 0.006 min

Lab File: VN077097.D

Acq: 22 Mar 2023 10:40




Tgt Ion:128 Resp: 12448


Ion Ratio Lower Upper

128 100

127 13.8 10.0 15.0


129 10.9 8.6 13.0

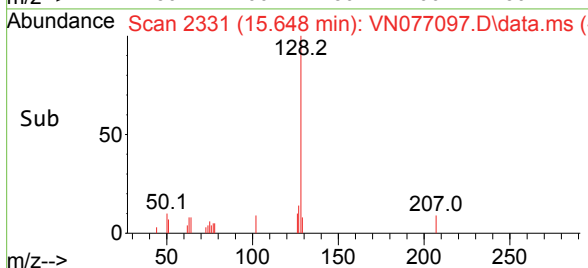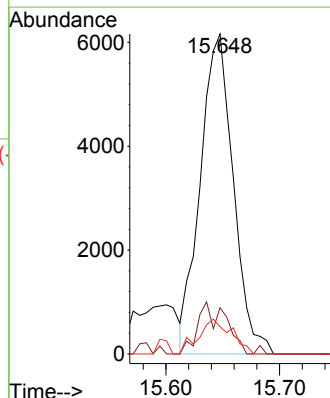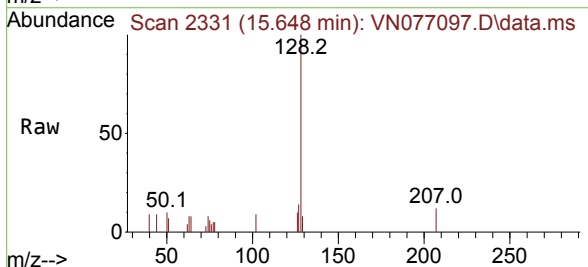



#96
 1,2,3-Trichlorobenzene
 Concen: 1.070 ug/l
 RT: 15.842 min Scan# 21
 Delta R.T. -0.000 min
 Lab File: VN077097.D
 Acq: 22 Mar 2023 10:40

Instrument :
 MSVOA_N
 ClientSampleId :
 VN0322MBL01

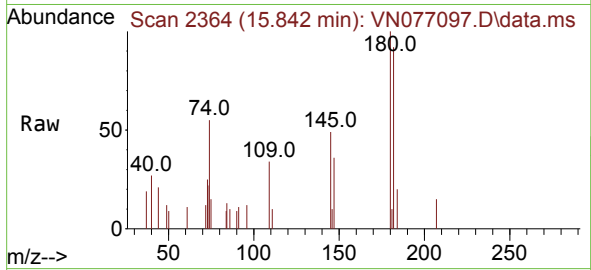

Tgt Ion:	180	Resp:	3712
Ion	Ratio	Lower	Upper
180	100		
182	86.8	47.4	142.2
145	40.3	17.9	53.8

