
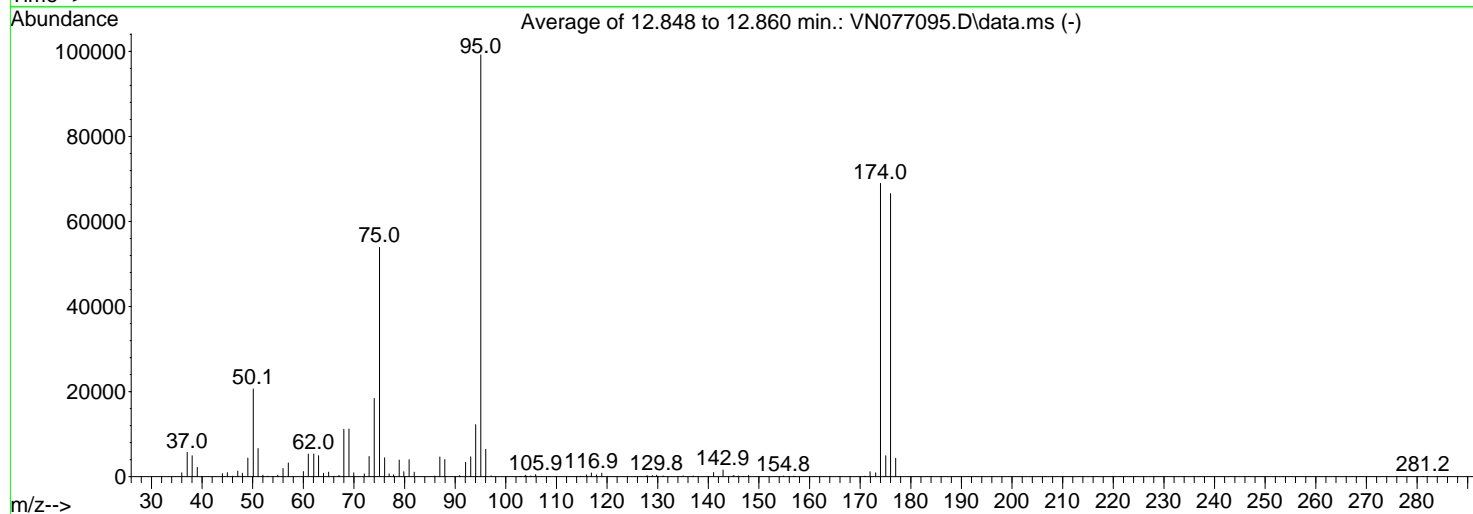


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN032223\
 Data File : VN077095.D
 Acq On : 22 Mar 2023 08:34
 Operator : JC\MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N031723W.M
 Title : SW846 8260
 Last Update : Mon Mar 20 08:50:30 2023

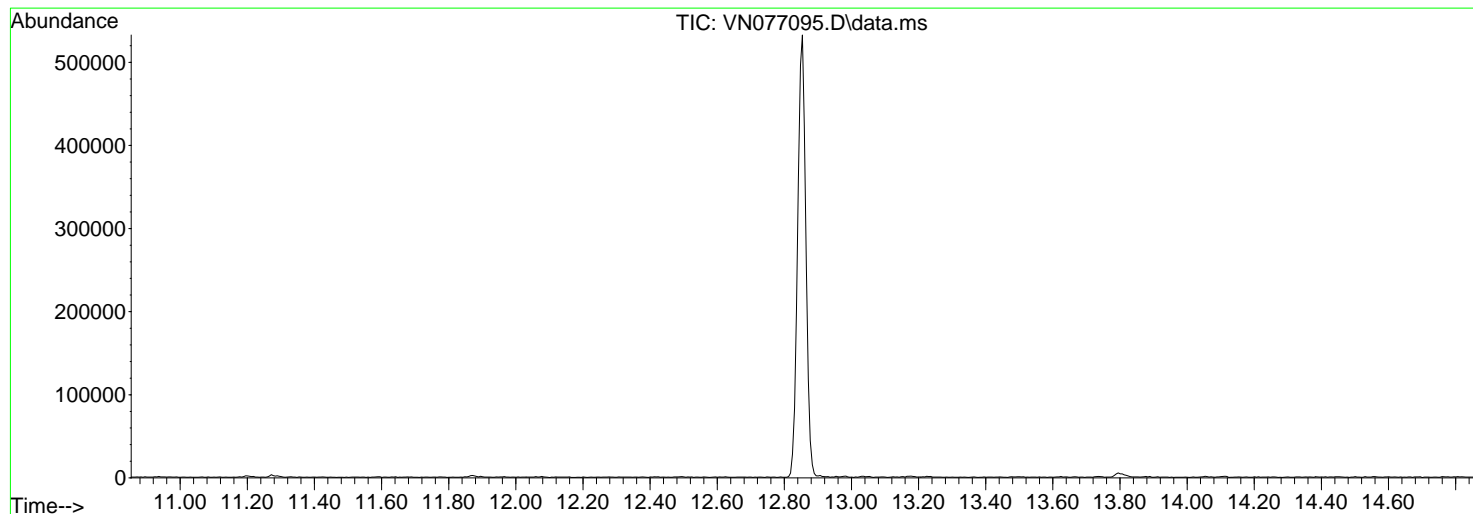

AutoFind: Scans 1855, 1856, 1857; Background Corrected with Scan 1846

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result
50	95	15	40	20.8	20637	PASS
75	95	30	60	54.4	53931	PASS
95	95	100	100	100.0	99192	PASS
96	95	5	9	6.5	6447	PASS
173	174	0.00	2	1.3	893	PASS
174	95	50	100	69.5	68971	PASS
175	174	5	9	7.1	4926	PASS
176	174	95	101	96.5	66552	PASS
177	176	5	9	6.5	4321	PASS

Average of 12.848 to 12.860 min.: VN077095.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.00	923	50.10	20637	64.00	791	75.05	5393
37.05	5709	51.05	6636	65.00	1072	76.05	444
38.05	4935	52.00	328	66.00	84	76.95	66
39.05	2178	53.00	105	66.90	116	77.80	45
39.95	94	54.95	331	67.05	297	78.10	110
44.00	722	56.00	1905	68.00	11133	78.95	3919
45.00	934	57.05	3251	69.00	11206	79.85	1177
46.00	133	60.00	1200	69.95	895	80.90	3978
47.05	1317	61.00	5319	72.05	625	81.90	1075
47.95	776	62.05	5353	73.00	4739	85.95	141
49.05	4375	63.00	4919	74.00	18398	86.95	4637

Average of 12.848 to 12.860 min.: VN077095.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
87.95	4018	103.95	338	118.95	812	142.90	1592
90.85	236	104.20	78	127.80	136	144.90	176
91.10	123	104.95	190	127.95	193	145.05	257
92.05	3376	105.90	509	128.95	257	145.70	79
93.05	4683	107.00	69	129.80	344	146.00	144
94.05	12230	109.90	51	131.05	195	146.90	75
95.05	99192	112.00	62	134.70	53	147.95	291
96.05	6447	114.80	130	135.05	177	154.85	144
97.10	193	115.95	423	136.90	61	156.80	101
102.90	60	116.90	861	137.05	159	157.10	50
103.70	125	117.90	418	141.05	994	160.90	57

Average of 12.848 to 12.860 min.: VN077095.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
170.90	104						
171.10	54						
171.95	1164						
173.05	893						
174.00	68971						
175.05	4926						
176.00	66552						
177.00	4321						
281.20	82						

Instrument :

MSVOA_N

ClientSampleId :

BFB