
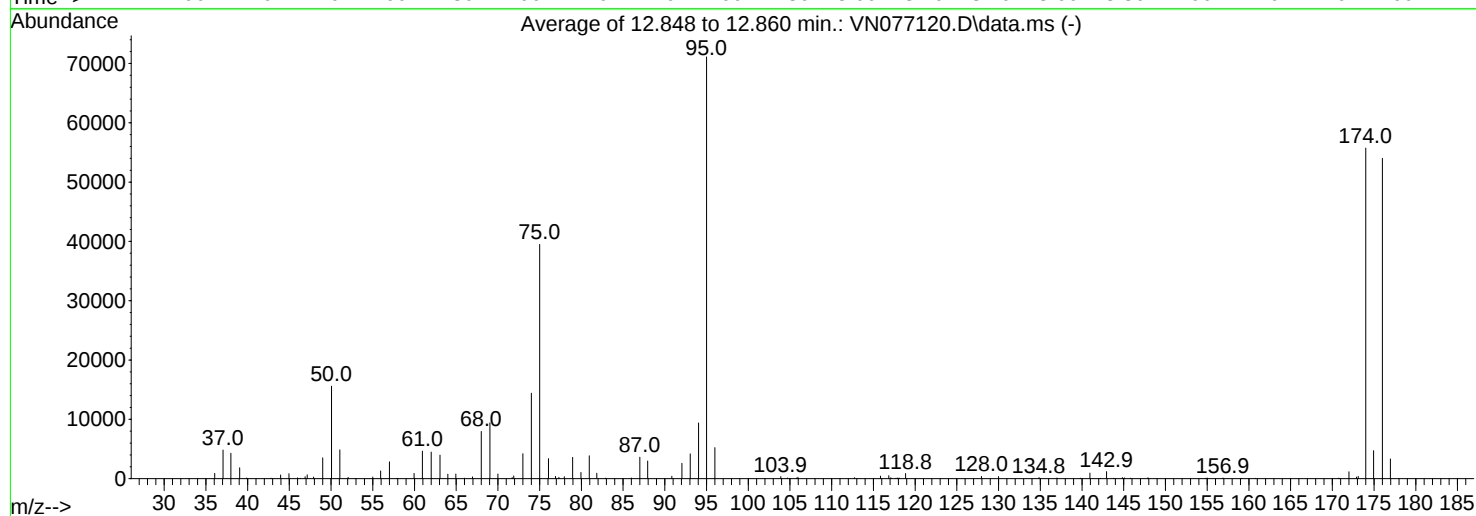


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN032223\
Data File : VN077120.D
Acq On : 23 Mar 2023 01:02
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N031723W.M
Title : SW846 8260
Last Update : Mon Mar 20 08:50:30 2023

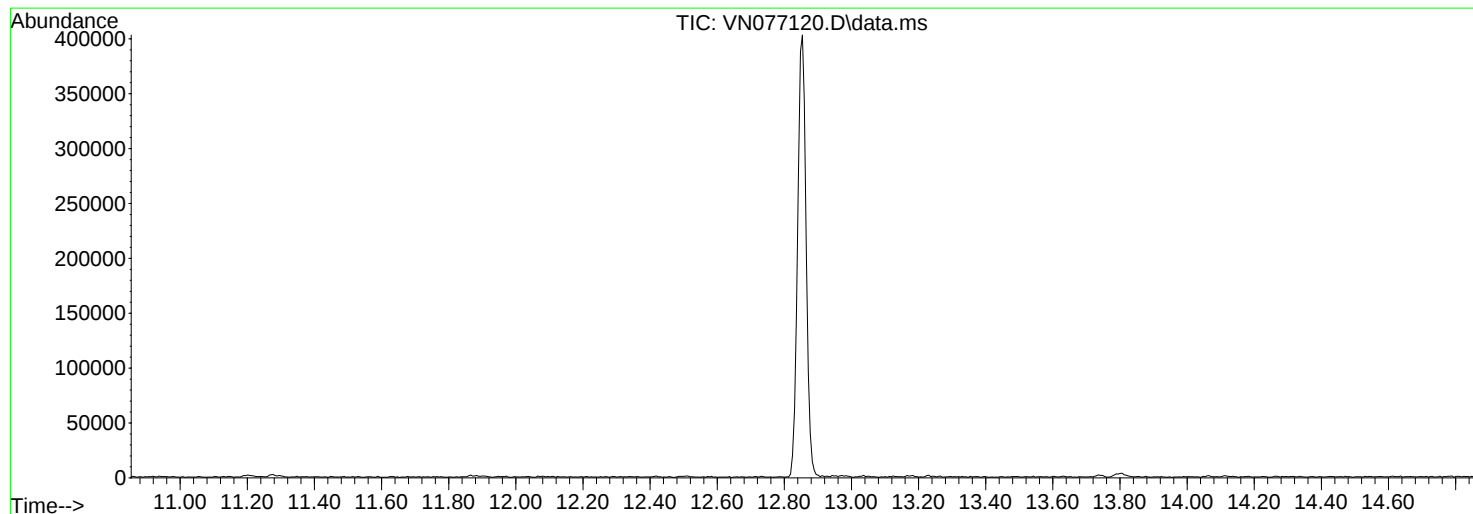

AutoFind: Scans 1855, 1856, 1857; Background Corrected with Scan 1847

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	21.9	15602	PASS
75	95	30	60	55.5	39507	PASS
95	95	100	100	100.0	71123	PASS
96	95	5	9	7.4	5248	PASS
173	174	0.00	2	0.7	381	PASS
174	95	50	100	78.4	55733	PASS
175	174	5	9	8.5	4731	PASS
176	174	95	101	96.9	54021	PASS
177	176	5	9	6.2	3330	PASS

Average of 12.848 to 12.860 min.: VN077120.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.05	896	47.15	655	59.95	886	71.70	181
37.05	4831	47.90	278	60.95	4642	71.90	45
38.00	4280	49.00	3500	62.00	4483	73.00	421
39.05	1841	50.05	15602	63.05	3982	74.00	1441
39.90	119	51.05	4851	64.00	753	75.00	39507
42.80	81	52.05	222	64.95	776	76.05	3387
43.95	627	52.90	59	66.00	86	76.90	389
44.95	831	55.00	284	66.95	309	77.30	208
46.00	124	55.95	1303	68.00	7963	77.95	324
46.30	66	57.00	2843	69.05	9404	78.95	3601
46.90	339	57.90	56	70.00	783	79.95	1048

Instrument :

MSVOA_N

ClientSampleId :

BFB

Average of 12.848 to 12.860 min.: VN077120.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
80.95	3849	96.00	5248	118.10	98	144.85	202
81.85	925	103.90	366	118.85	855	145.10	138
82.90	85	104.70	103	127.95	389	145.80	80
86.00	118	105.80	123	130.00	362	147.90	161
87.00	3612	105.95	258	134.85	184	154.80	70
87.95	2956	112.75	159	137.00	108	155.00	107
90.85	416	115.85	429	139.80	83	156.90	110
92.05	2607	116.85	520	140.95	956	159.10	52
93.05	4173	117.10	177	142.20	51	160.80	53
94.05	9383	117.70	90	142.95	1202	170.70	81
95.00	71123	117.90	121	143.80	83	170.90	55

Average of 12.848 to 12.860 min.: VN077120.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
172.00	1173						
172.90	286						
173.10	381						
174.00	55733						
174.95	4731						
176.00	54021						
176.95	3330						