
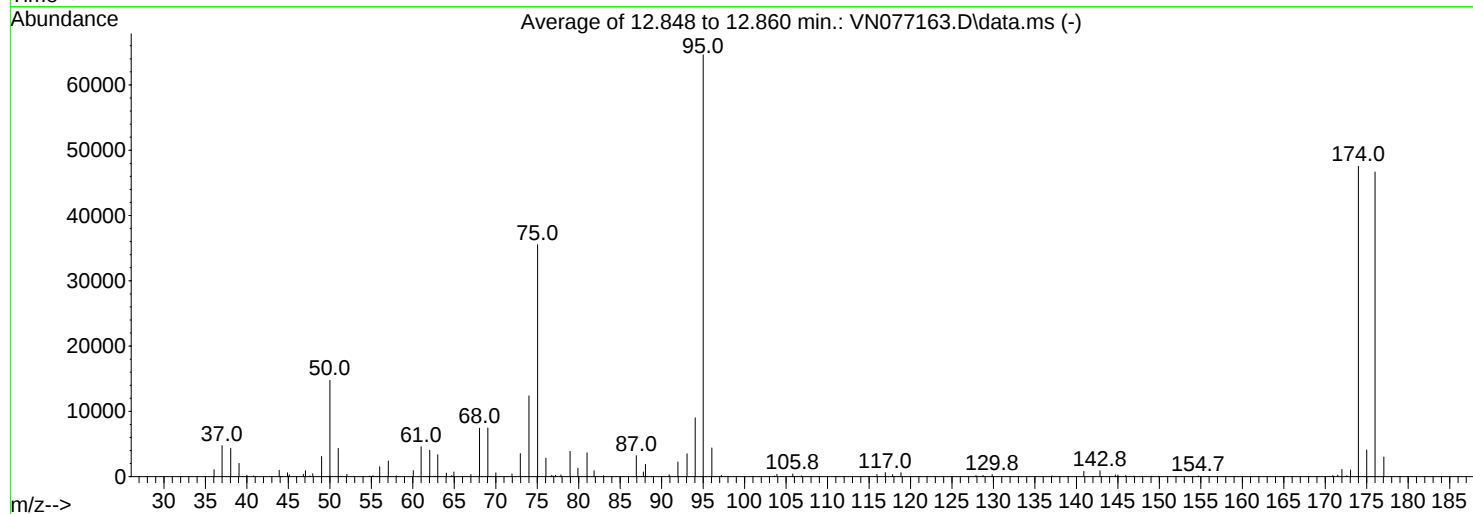


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN032423\
Data File : VN077163.D
Acq On : 23 Mar 2023 21:09
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT3.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\624N032423W.M
Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
Last Update : Fri Mar 24 05:55:38 2023

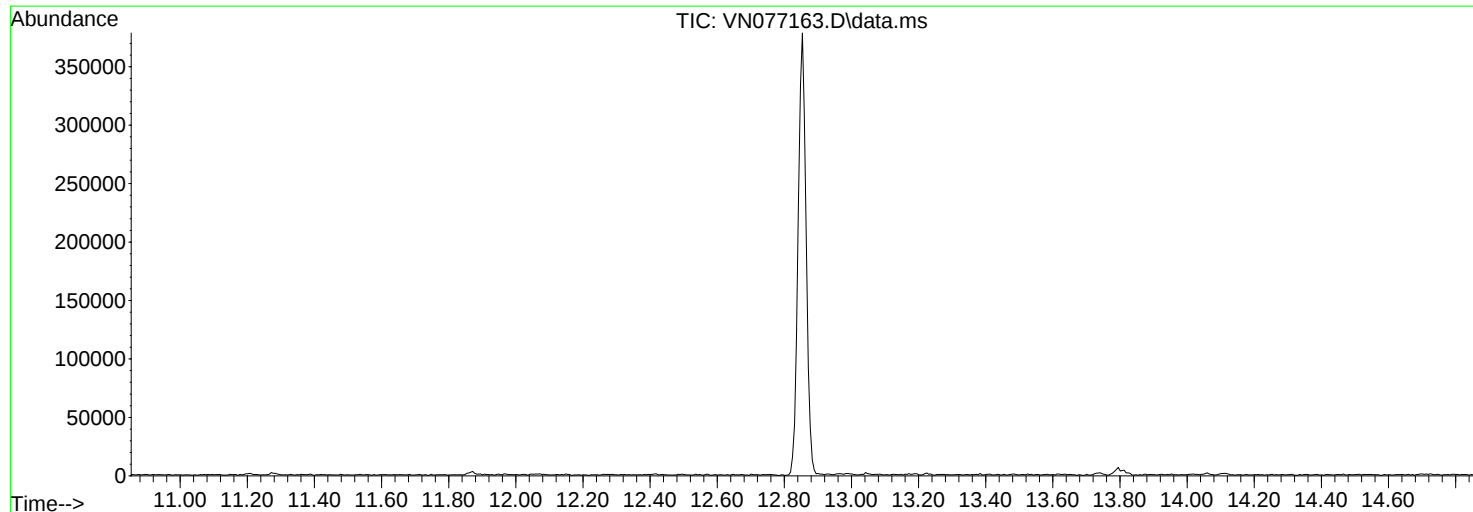

AutoFind: Scans 1855, 1856, 1857; Background Corrected with Scan 1848

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	22.8	14757	PASS
75	95	30	60	55.0	35541	PASS
95	95	100	100	100.0	64611	PASS
96	95	5	9	6.8	4383	PASS
173	174	0.00	2	2.2	1024	FAIL*
174	95	50	100	73.6	47552	PASS
175	174	5	9	8.6	4095	PASS
176	174	95	101	98.1	46656	PASS
177	176	5	9	6.5	3025	PASS