
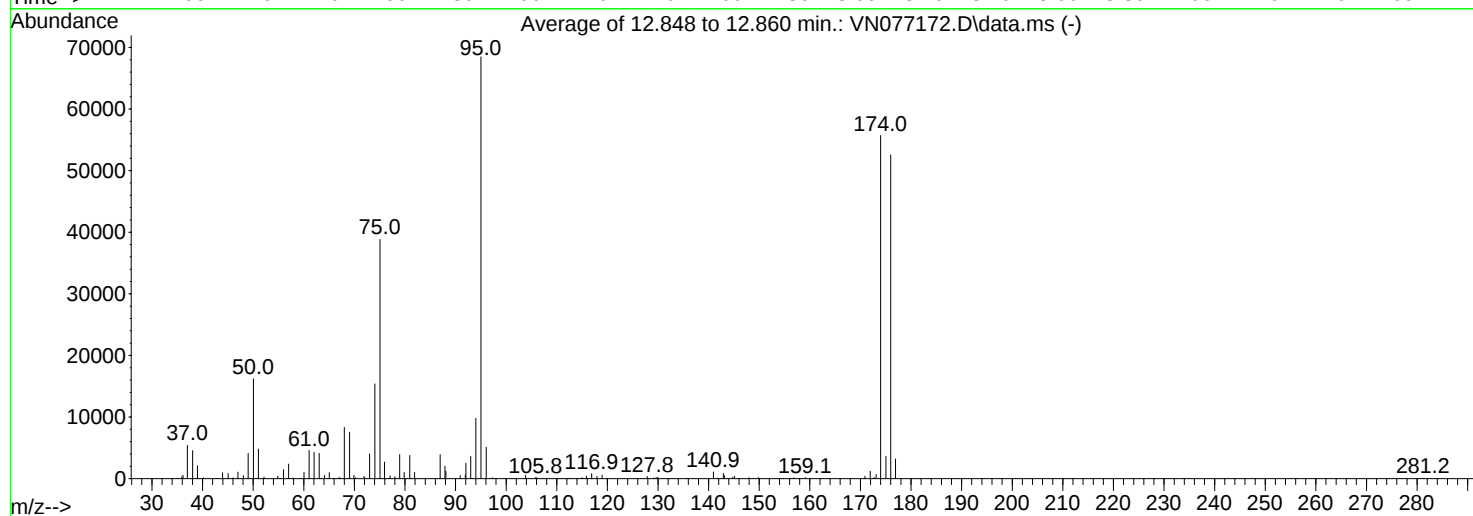


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN032423\
Data File : VN077172.D
Acq On : 24 Mar 2023 10:05
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT3.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\624N032423W.M
Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
Last Update : Fri Mar 24 05:55:38 2023

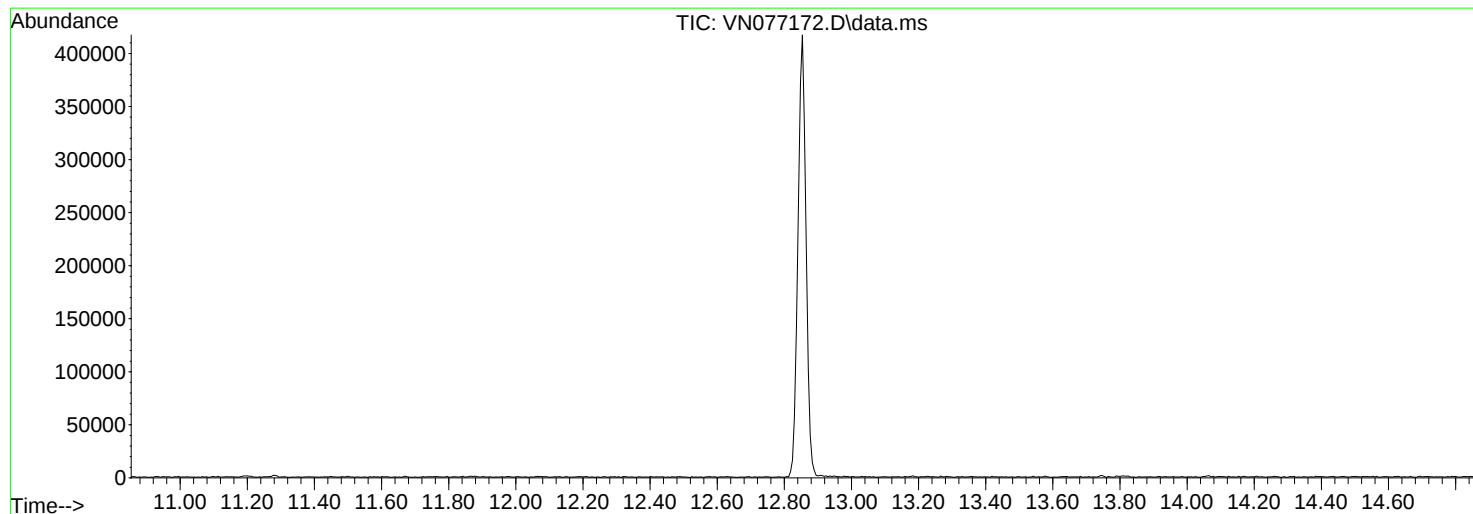

AutoFind: Scans 1855, 1856, 1857; Background Corrected with Scan 1847

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.7	16201	PASS
75	95	30	60	56.7	38837	PASS
95	95	100	100	100.0	68483	PASS
96	95	5	9	7.4	5081	PASS
173	174	0.00	2	1.2	642	PASS
174	95	50	100	81.4	55712	PASS
175	174	5	9	6.5	3615	PASS
176	174	95	101	94.3	52557	FAIL*
177	176	5	9	6.1	3208	PASS