

Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN033019\
 Data File : VN054820.D
 Acq On : 30 Mar 2019 23:58
 Operator : JC/SP
 Sample : VN0330WBL02
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 VN0330WBL02

Quant Time: Mar 31 04:55:53 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N032919W.M
 Quant Title : SW846 8260
 QLast Update : Sat Mar 30 00:48:18 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.67	168	527706	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.59	114	863404	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.41	117	713039	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.35	152	252270	50.00	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.03	65	356825	50.16	ug/l	0.00
Spiked Amount	50.000		Recovery	=	100.32%	
35) Dibromofluoromethane	7.59	113	274232	47.64	ug/l	0.00
Spiked Amount	50.000		Recovery	=	95.28%	
50) Toluene-d8	10.09	98	1031229	48.19	ug/l	0.00
Spiked Amount	50.000		Recovery	=	96.38%	
62) 4-Bromofluorobenzene	12.40	95	308320	43.32	ug/l	0.00
Spiked Amount	50.000		Recovery	=	86.64%	


Target Compounds	Qvalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA N\DATA\VN033019\
Data File : VN054820.D
Acq On : 30 Mar 2019 23:58
Operator : JC/SP
Sample : VN0330WBL02
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
VN0330WBL02

Quant Time: Mar 31 04:55:53 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_N\METHODS\82N032919W.M
Quant Title : SW846 8260
QLast Update : Sat Mar 30 00:48:18 2019
Response via : Initial Calibration

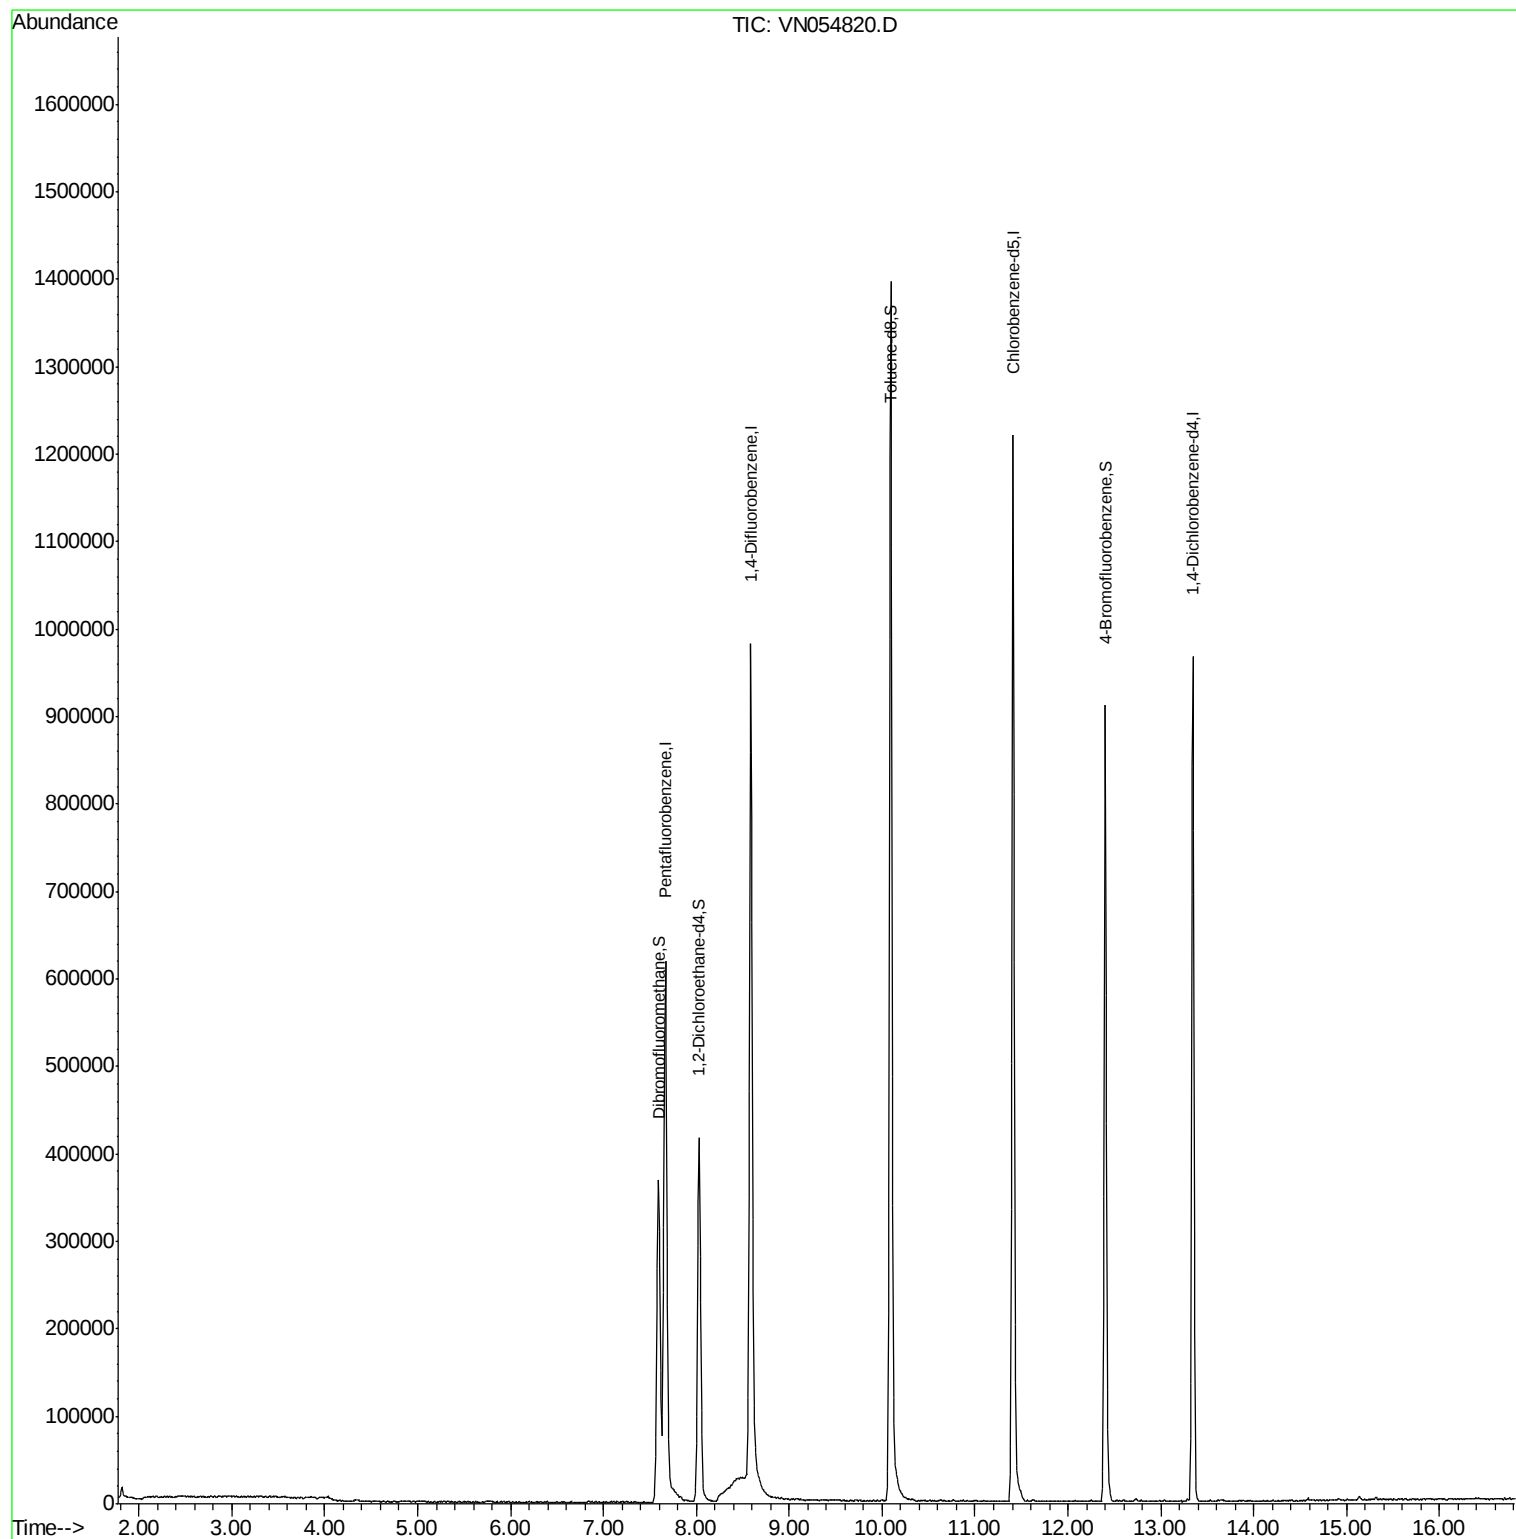

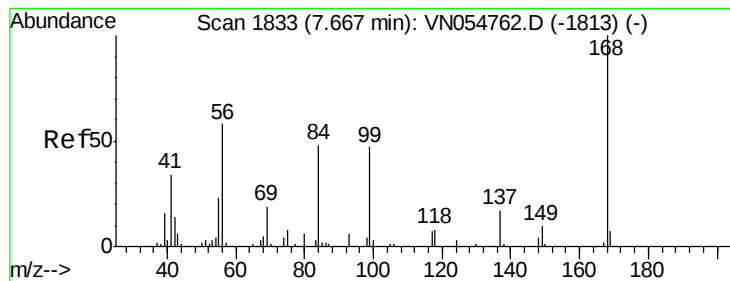

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.67 min Scan# 1833

Delta R.T. -0.00 min

Lab File: VN054820.D

Acq: 30 Mar 2019 23:58

Instrument :

MSVOA_N

ClientSampleId :


VN0330WBL02

Tot Ion:168 Resp: 527706

Ion Ratio Lower Upper

168 100

99 55.1 37.1 55.7

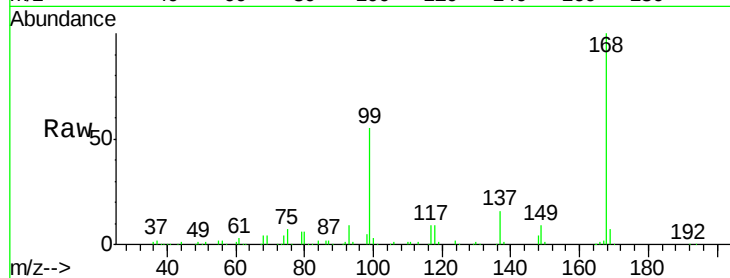

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VN0

7.67

250000

200000



150000

100000

50000

0

Time-->

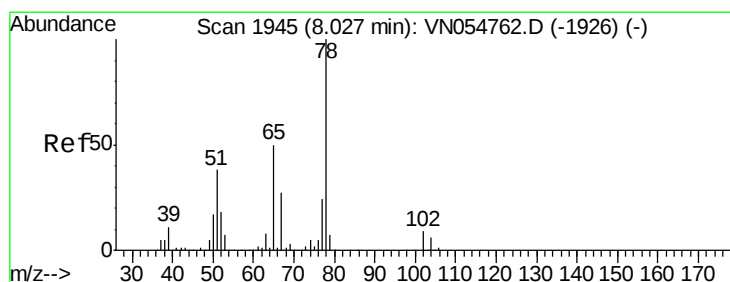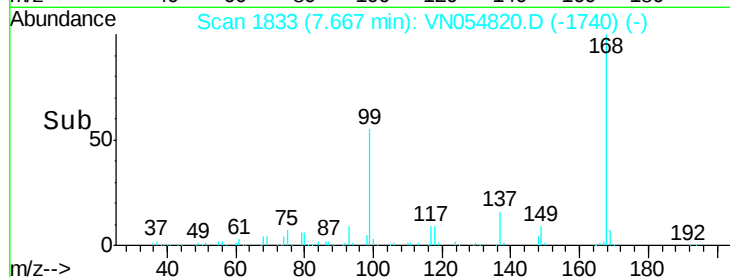

#33

1,2-Dichloroethane-d4

Concen: 50.161 ug/l

RT: 8.03 min Scan# 1946

Delta R.T. 0.00 min

Lab File: VN054820.D


Acq: 30 Mar 2019 23:58

Tgt Ion: 65 Resp: 356825

Ion Ratio Lower Upper

65 100

67 52.5 0.0 104.6

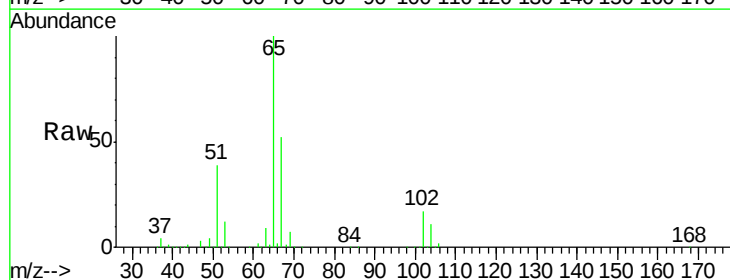

Abundance Ion 64.90 (64.60 to 65.60): VN0

Ion 66.90 (66.60 to 67.60): VN0

8.03


150000


100000

50000

0

Time-->

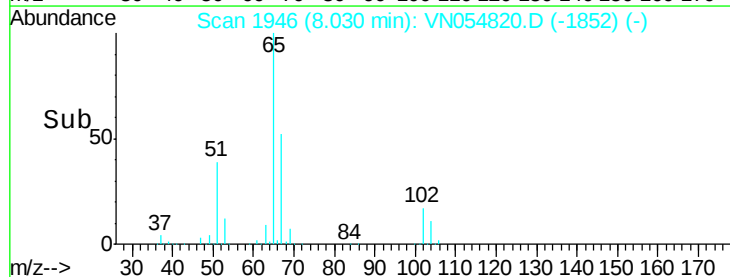

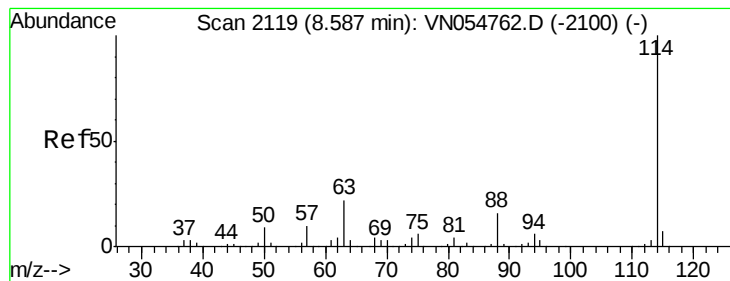

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.59 min Scan# 2119

Delta R.T. -0.00 min

Lab File: VN054820.D

Acq: 30 Mar 2019 23:58

Instrument :

MSVOA_N

ClientSampled :

VN0330WBL02


Tot Ion:114 Resp: 863404

Ion Ratio Lower Upper

114 100

63 22.0 0.0 35.2




88 16.3 0.0 30.2

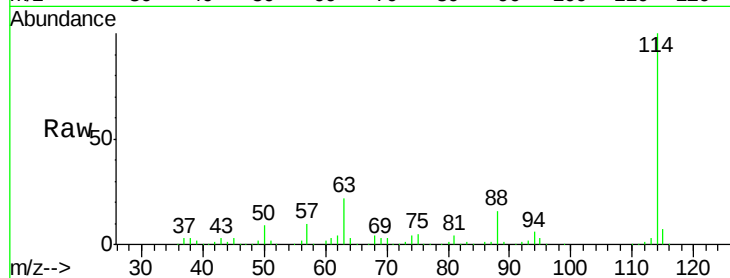

Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): VN0

Ion 87.90 (87.60 to 88.60): VN0

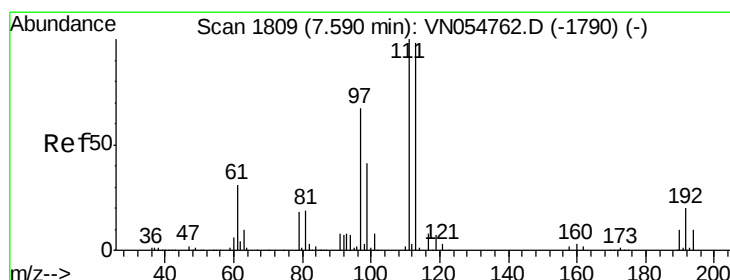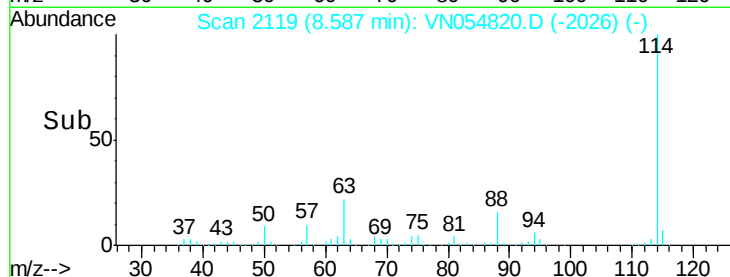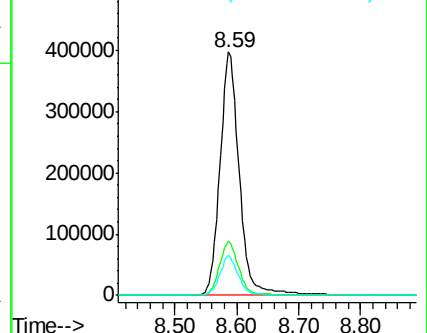

#35

Dibromofluoromethane

Concen: 47.641 ug/l

RT: 7.59 min Scan# 1810

Delta R.T. 0.00 min

Lab File: VN054820.D

Acq: 30 Mar 2019 23:58


Tgt Ion:113 Resp: 274232

Ion Ratio Lower Upper

113 100

111 105.2 82.2 123.4



192 20.5 19.2 28.8

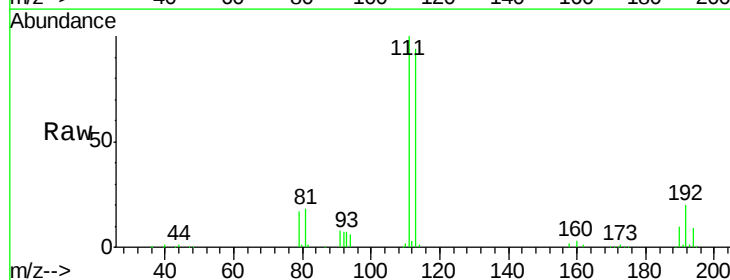


Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V

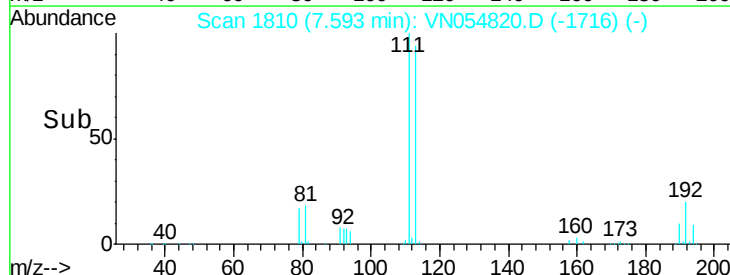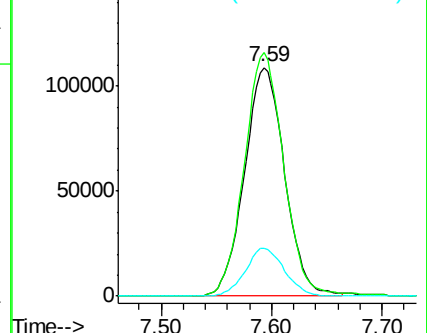

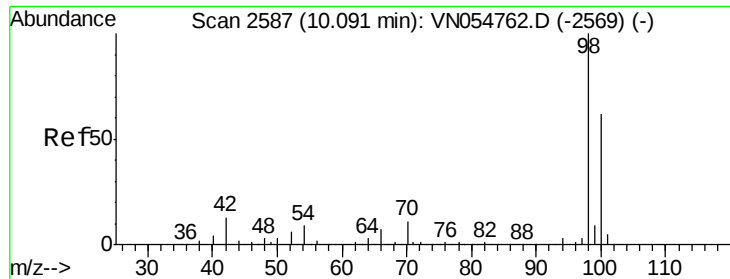

#50

Toluene-d8

Concen: 48.187 ug/l

RT: 10.09 min Scan# 2587

Delta R.T. -0.00 min

Lab File: VN054820.D

Acq: 30 Mar 2019 23:58

Instrument :

MSVOA_N

ClientSampleId :


VN0330WBL02

Tot Ion: 98 Resp: 1031229

Ion Ratio Lower Upper

98 100

100 63.7 51.2 76.8

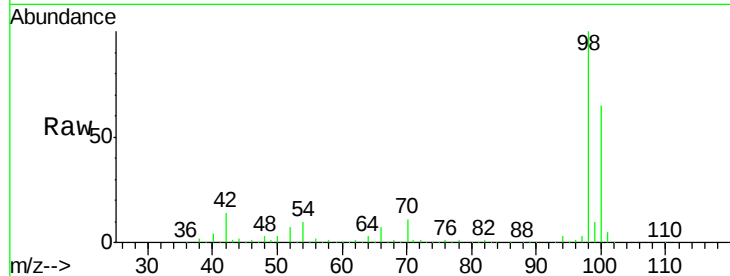

Abundance Ion 98.00 (97.70 to 98.70): VN0

Ion 100.00 (99.70 to 100.70): VN

10.09

500000

400000



300000

200000

100000

0

Time-->

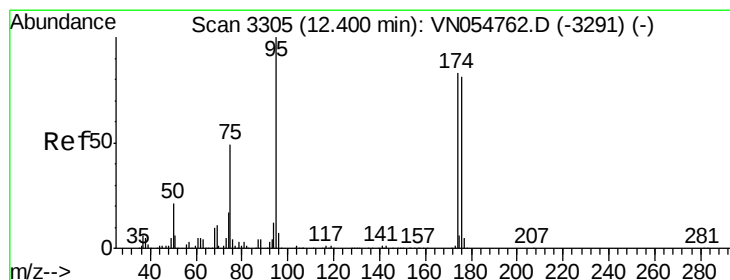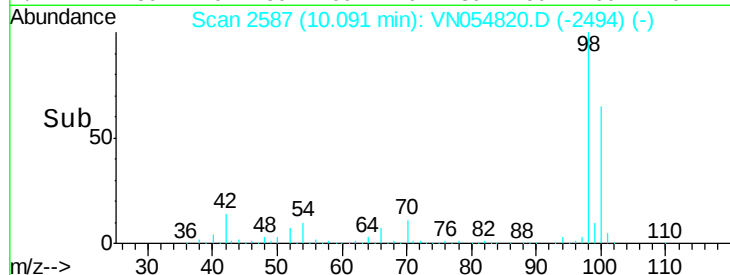

#62

4-Bromofluorobenzene

Concen: 43.320 ug/l

RT: 12.40 min Scan# 3306

Delta R.T. 0.00 min

Lab File: VN054820.D

Acq: 30 Mar 2019 23:58


Tgt Ion: 95 Resp: 308320

Ion Ratio Lower Upper

95 100

174 84.5 0.0 191.0

176 80.2 0.0 187.4

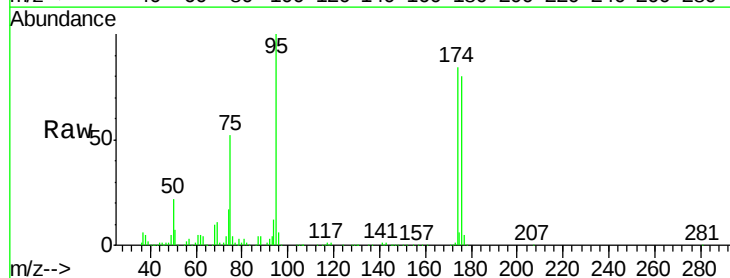

Abundance Ion 94.90 (94.60 to 95.60): VN0

Ion 173.80 (173.50 to 174.50): V

Ion 175.80 (175.50 to 176.50): V

250000

200000


150000


100000

50000

0

Time-->

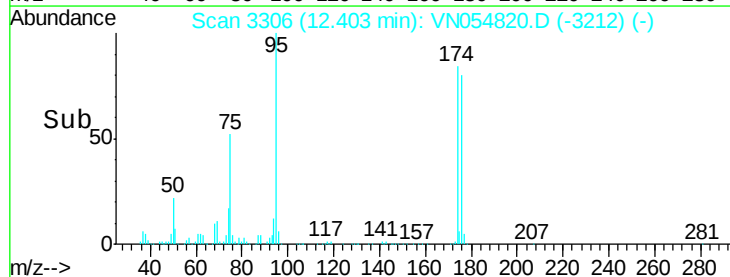

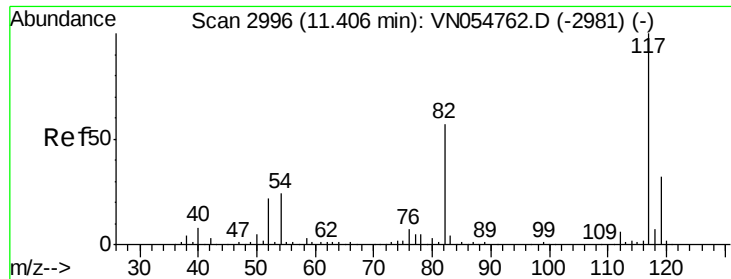

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 11.41 min Scan# 2997

Delta R.T. 0.00 min

Lab File: VN054820.D

Acq: 30 Mar 2019 23:58

Instrument :

MSVOA_N

ClientSampled :

VN0330WBL02


Tot Ion:117 Resp: 713039

Ion Ratio Lower Upper

117 100

82 55.5 40.0 60.0




119 31.9 25.8 38.6

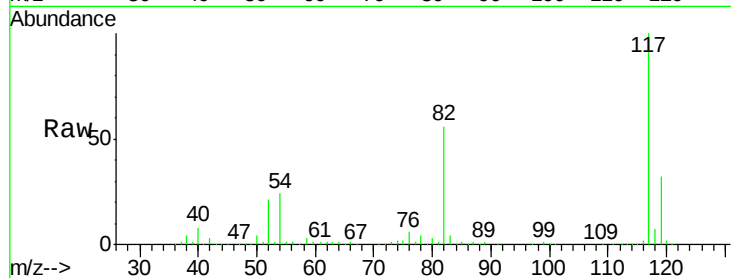

Abundance Ion 116.90 (116.60 to 117.60): V

Ion 82.00 (81.70 to 82.70): VN

Ion 118.90 (118.60 to 119.60): V

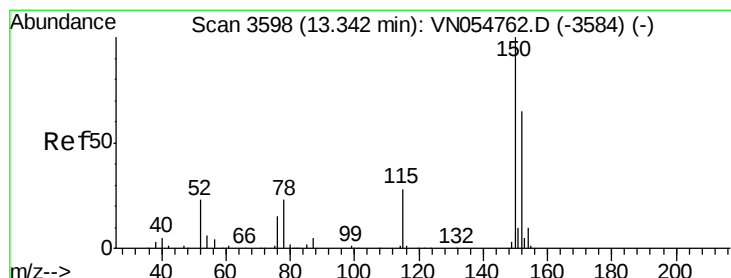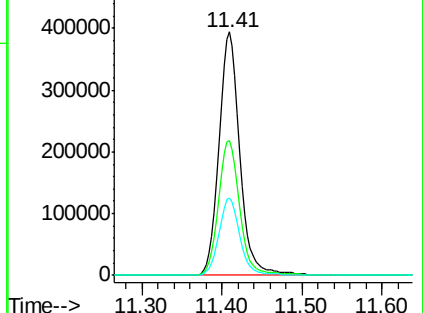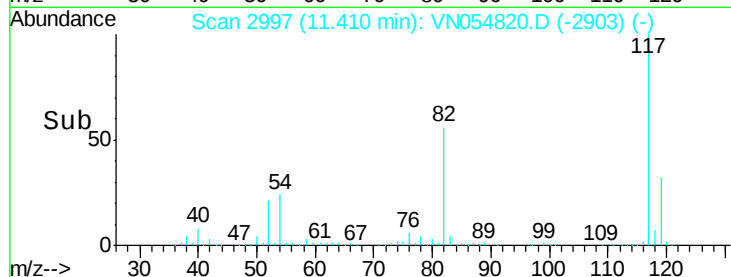

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.35 min Scan# 3599

Delta R.T. 0.00 min

Lab File: VN054820.D

Acq: 30 Mar 2019 23:58


Tgt Ion:152 Resp: 252270

Ion Ratio Lower Upper

152 100

115 57.7 27.2 81.6

150 159.0 0.0 349.2

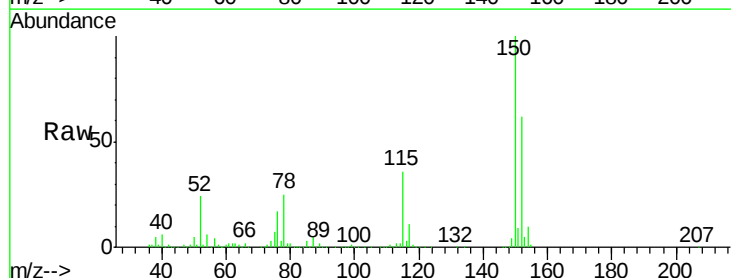

Abundance Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

