


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN033019\
Data File : VN054818.D
Acq On : 30 Mar 2019 22:38
Operator : JC/SP
Sample : BFB
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N032919W.M
Title : SW846 8260
Last Update : Sat Mar 30 00:48:18 2019

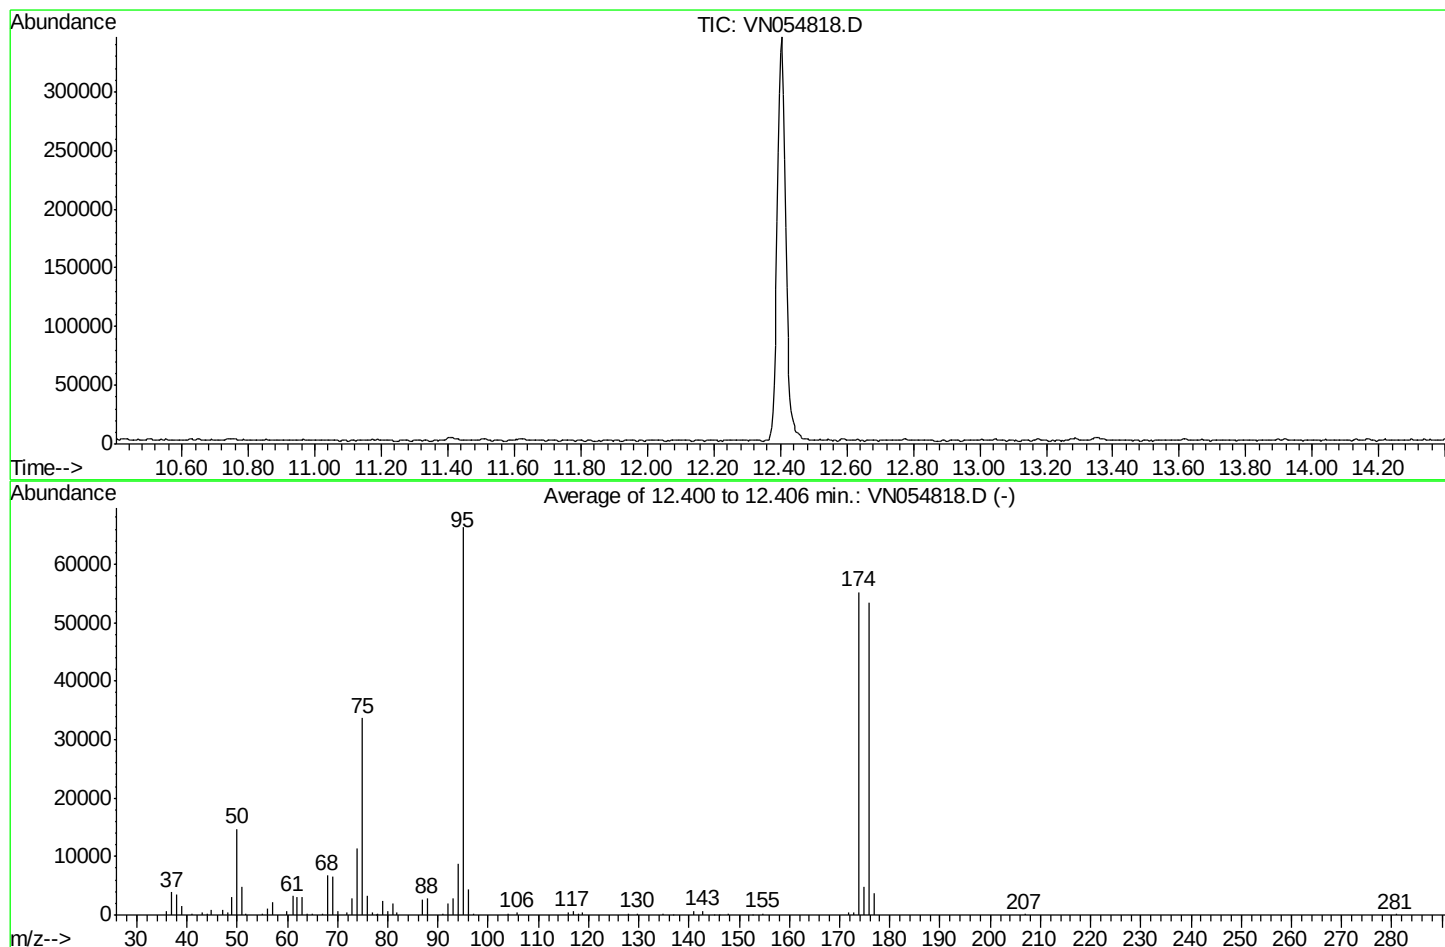

AutoFind: Scans 3305, 3306, 3307; Background Corrected with Scan 3291

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.2	14725	PASS
75	95	30	60	50.8	33701	PASS
95	95	100	100	100.0	66317	PASS
96	95	5	9	6.6	4379	PASS
173	174	0.00	2	0.9	478	PASS
174	95	50	100	83.3	55226	PASS
175	174	5	9	8.6	4757	PASS
176	174	95	101	97.0	53544	PASS
177	176	5	9	7.0	3766	PASS