
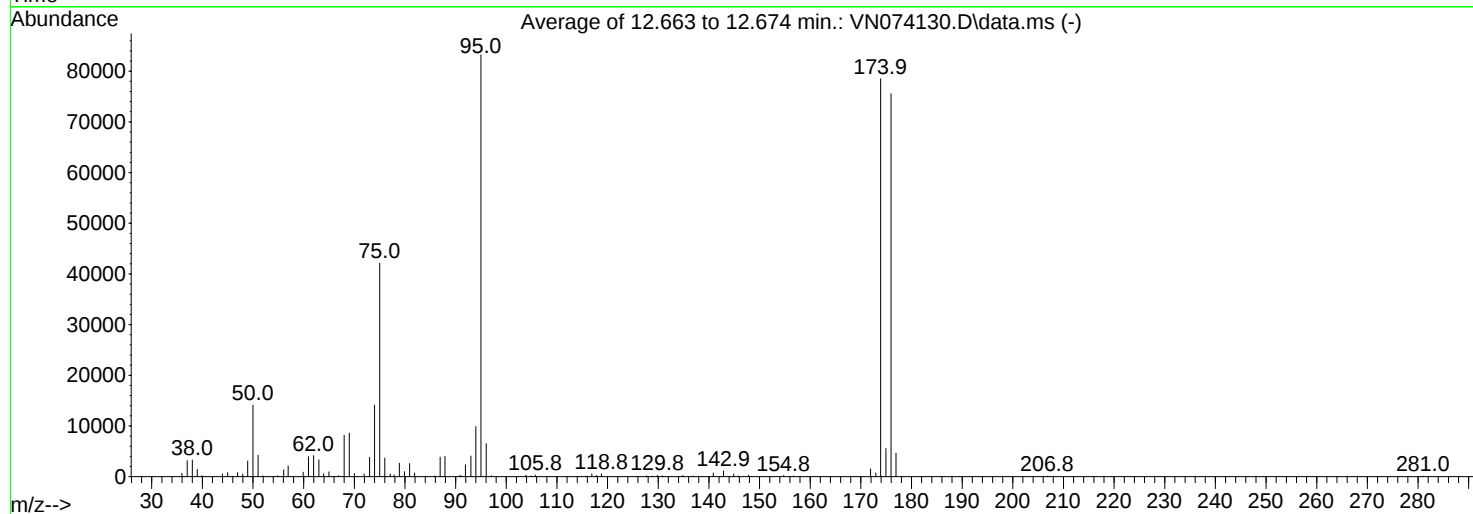


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN082622\
Data File : VN074130.D
Acq On : 26 Aug 2022 09:12
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N081522W.M
Title : SW846 8260
Last Update : Fri Aug 26 06:44:47 2022

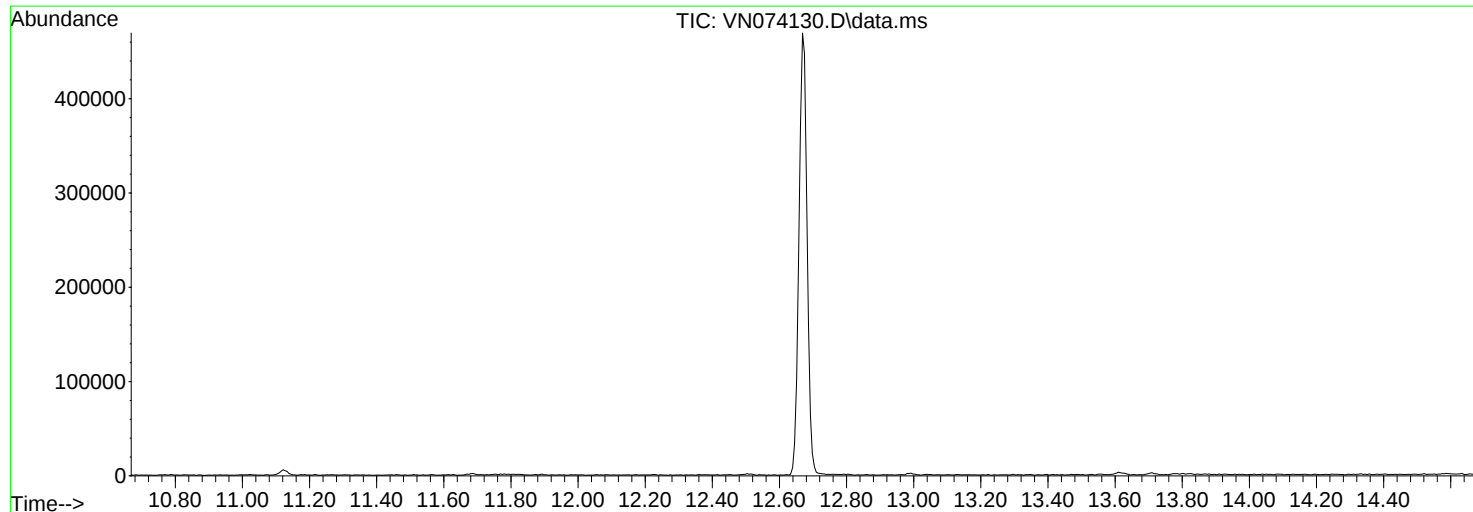

AutoFind: Scans 1832, 1833, 1834; Background Corrected with Scan 1824

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.0	14120	PASS
75	95	30	60	50.6	42115	PASS
95	95	100	100	100.0	83229	PASS
96	95	5	9	7.8	6513	PASS
173	174	0.00	2	0.9	720	PASS
174	95	50	100	94.3	78515	PASS
175	174	5	9	7.1	5560	PASS
176	174	95	101	96.2	75563	PASS
177	176	5	9	6.2	4648	PASS