

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN120522\
 Data File : VN075559.D
 Acq On : 05 Dec 2022 15:19
 Operator : JC\MD
 Sample : N5809-01ME
 Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_N/MEOH
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 HOWE-DRUM-A-1129

Quant Time: Dec 06 03:25:00 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N112122W.M
 Quant Title : SW846 8260
 QLast Update : Wed Nov 23 00:18:03 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	8.224	168	158358	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.100	114	254494	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.870	117	214529	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.794	152	94987	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.582	65	50825	59.791	ug/l	0.00
Spiked Amount 50.000	Range 74 - 125		Recovery = 119.580%			
35) Dibromofluoromethane	8.171	113	63199	63.216	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery = 126.440%#			
50) Toluene-d8	10.565	98	131395	58.354	ug/l	0.00
Spiked Amount 50.000	Range 86 - 113		Recovery = 116.700%#			
62) 4-Bromofluorobenzene	12.853	95	90587	54.505	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery = 109.020%			
Target Compounds						Qvalue
3) Chloromethane	2.359	50	358	0.238	ug/l #	42
5) Bromomethane	2.906	94	483	0.289	ug/l	85
6) Chloroethane	3.071	64	13378	9.298	ug/l #	56
11) Tert butyl alcohol	5.500	59	3952	11.075	ug/l #	72
16) Acetone	4.459	43	760	0.959	ug/l #	43
18) Methyl Acetate	5.036	43	991	Below Cal	#	59
20) Methylene Chloride	5.265	84	2045	Below Cal	#	82
23) Vinyl Acetate	6.612	43	1028	0.299	ug/l #	67
25) 2-Butanone	7.518	43	1124	1.015	ug/l #	43
27) cis-1,2-Dichloroethene	7.488	96	1104	0.584	ug/l	77
29) Tetrahydrofuran	7.859	42	359	0.533	ug/l #	51
31) Cyclohexane	8.229	56	2934	1.086	ug/l #	19
36) 1,1-Dichloropropene	8.224	75	10745	4.928	ug/l #	51
38) Carbon Tetrachloride	8.224	117	14890	6.217	ug/l #	17
43) Isopropyl Acetate	8.794	43	3570	1.133	ug/l #	53
44) Trichloroethene	9.359	130	884	0.484	ug/l	76
51) 4-Methyl-2-Pentanone	10.447	43	843	0.420	ug/l #	57
58) 2-Chloroethyl Vinyl ether	10.165	63	676	0.792	ug/l #	58
59) 2-Hexanone	11.206	43	1224	0.812	ug/l	91
68) m/p-Xylenes	12.076	106	946	0.308	ug/l	87
76) 1,2,3-Trichloropropane	12.853	75	46352	25.809	ug/l #	1
77) Bromobenzene	12.976	156	474	0.277	ug/l	68
81) trans-1,4-Dichloro-2-b...	12.853	75	46352	76.363	ug/l #	10
87) 1,3-Dichlorobenzene	13.735	146	960	0.296	ug/l	82
88) 1,4-Dichlorobenzene	13.735	146	960	0.291	ug/l	83
89) n-Butylbenzene	14.053	91	1541	0.304	ug/l	81
91) 1,2-Dichlorobenzene	14.111	146	1102	0.348	ug/l	87
93) 1,2,4-Trichlorobenzene	15.400	180	1275	0.786	ug/l	67
95) Naphthalene	15.647	128	7406	1.452	ug/l	99
96) 1,2,3-Trichlorobenzene	15.841	180	1697	1.065	ug/l	88


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN120522\
Data File : VN075559.D
Acq On : 05 Dec 2022 15:19
Operator : JC\MD
Sample : N5809-01ME
Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_N/MEOH
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
HOWE-DRUM-A-1129

Quant Time: Dec 06 03:25:00 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N112122W.M
Quant Title : SW846 8260
QLast Update : Wed Nov 23 00:18:03 2022
Response via : Initial Calibration




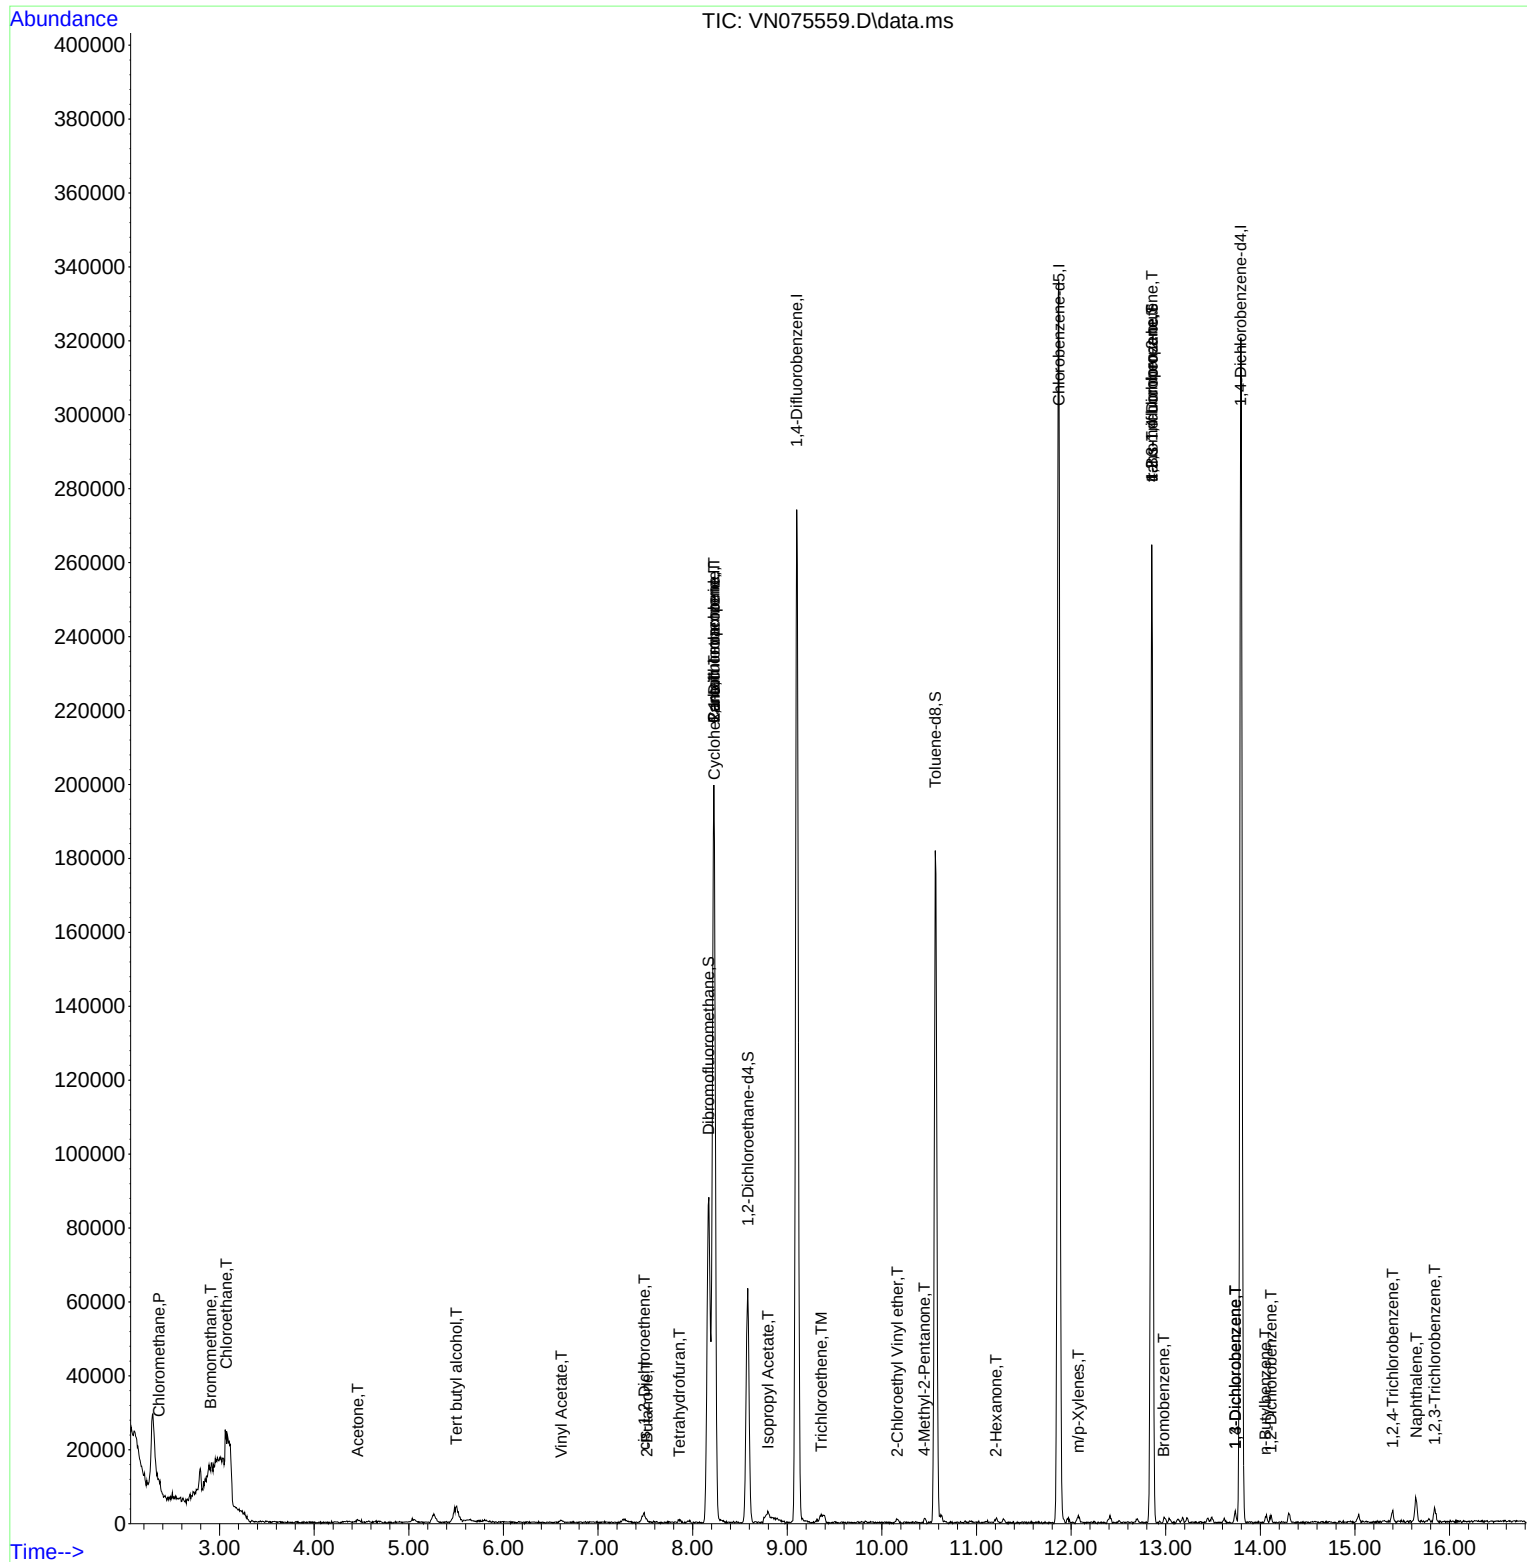


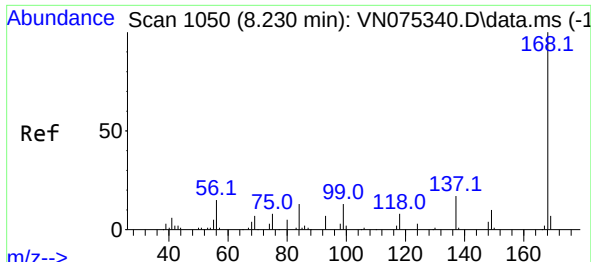

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.224 min Scan# 10
Delta R.T. -0.006 min
Lab File: VN075559.D
Acq: 05 Dec 2022 15:19




Instrument :
MSVOA_N
ClientSampleId :
HOWE-DRUM-A-1129


Tgt Ion:168 Resp: 158358
Ion Ratio Lower Upper
168 100
99 54.2 51.6 77.4

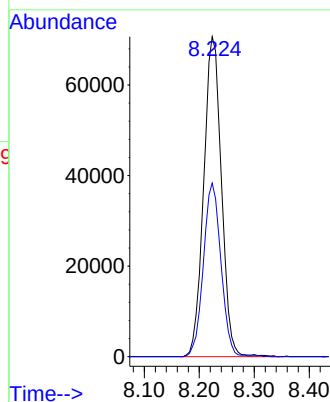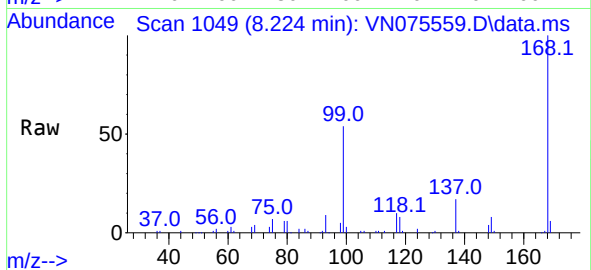

#3
Chloromethane
Concen: 0.238 ug/l
RT: 2.359 min Scan# 52
Delta R.T. -0.012 min
Lab File: VN075559.D
Acq: 05 Dec 2022 15:19

Tgt Ion: 50 Resp: 358
Ion Ratio Lower Upper
50 100
52 0.0 25.8 38.6#


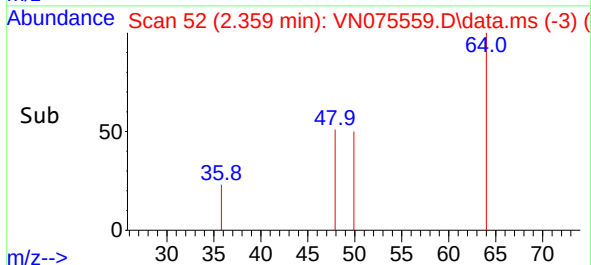

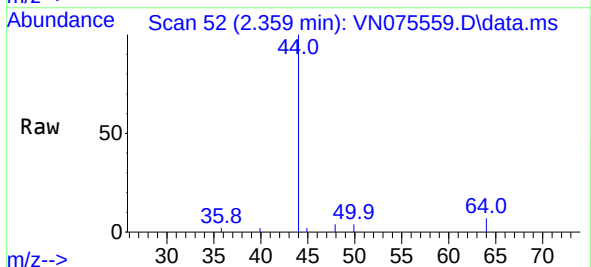


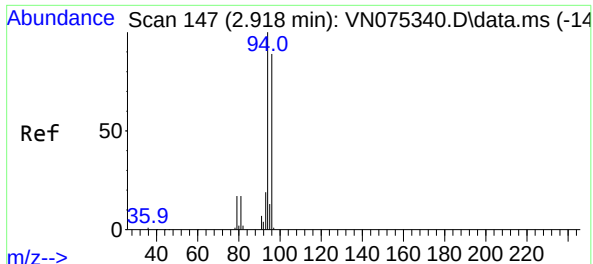

#5
Bromomethane
Concen: 0.289 ug/l
RT: 2.906 min Scan# 147
Delta R.T. -0.012 min
Lab File: VN075559.D
Acq: 05 Dec 2022 15:19




Instrument :
MSVOA_N
ClientSampleId :
HOWE-DRUM-A-1129


Tgt Ion: 94 Resp: 483
Ion Ratio Lower Upper
94 100
96 75.8 71.8 107.6



#6
Chloroethane
Concen: 9.298 ug/l
RT: 3.071 min Scan# 173
Delta R.T. -0.036 min
Lab File: VN075559.D
Acq: 05 Dec 2022 15:19

Tgt Ion: 64 Resp: 13378
Ion Ratio Lower Upper
64 100
66 6.0 23.8 35.8#


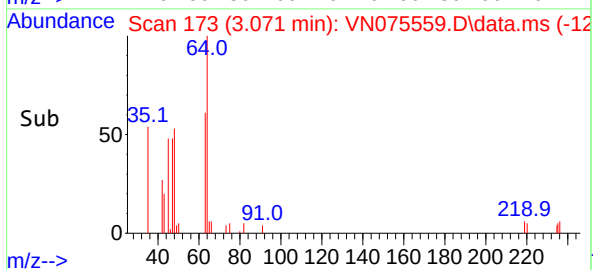

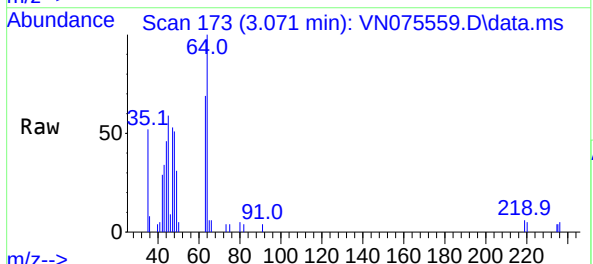




#11
Tert butyl alcohol
Concen: 11.075 ug/l
RT: 5.500 min Scan# 51
Delta R.T. -0.042 min
Lab File: VN075559.D
Acq: 05 Dec 2022 15:19




Instrument :
MSVOA_N
ClientSampleId :
HOWE-DRUM-A-1129


Tgt Ion: 59 Resp: 3952
Ion Ratio Lower Upper
59 100
57 0.0 8.5 12.7#



#16
Acetone
Concen: 0.959 ug/l
RT: 4.459 min Scan# 409
Delta R.T. 0.023 min
Lab File: VN075559.D
Acq: 05 Dec 2022 15:19

Tgt Ion: 43 Resp: 760
Ion Ratio Lower Upper
43 100
58 0.0 25.5 38.3#


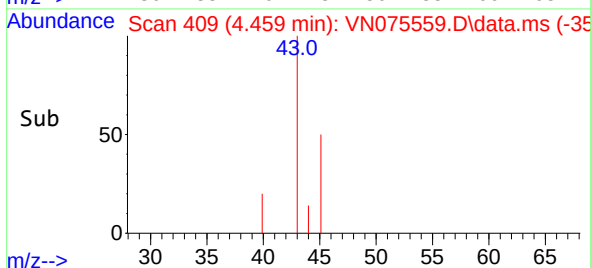
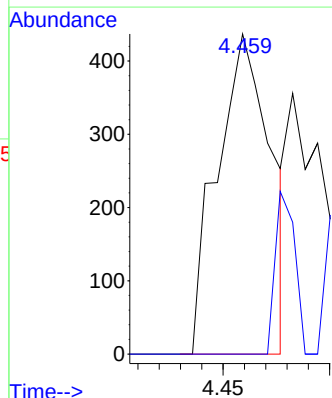





#18
Methyl Acetate
Concen: Below Cal
RT: 5.036 min Scan# 507
Delta R.T. -0.000 min
Lab File: VN075559.D
Acq: 05 Dec 2022 15:19




Instrument :
MSVOA_N
ClientSampleId :
HOWE-DRUM-A-1129


Tgt Ion: 43 Resp: 991
Ion Ratio Lower Upper
43 100
74 6.4 22.0 33.0#

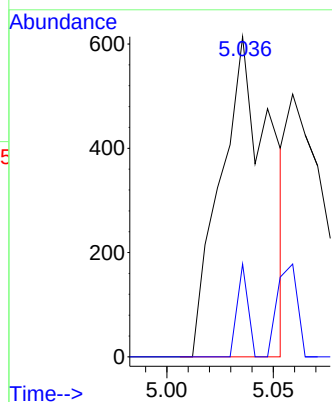

#23
Vinyl Acetate
Concen: 0.299 ug/l
RT: 6.612 min Scan# 775
Delta R.T. -0.000 min
Lab File: VN075559.D
Acq: 05 Dec 2022 15:19

Tgt Ion: 43 Resp: 1028
Ion Ratio Lower Upper
43 100
86 0.0 10.7 16.1#

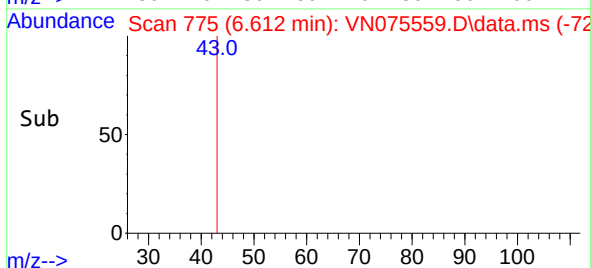



#25

2-Butanone

Concen: 1.015 ug/l

RT: 7.518 min Scan# 91

Delta R.T. 0.029 min

Lab File: VN075559.D

Acq: 05 Dec 2022 15:19

Instrument :

MSVOA_N

ClientSampleId :





HOWE-DRUM-A-1129

Tgt Ion: 43 Resp: 1124

Ion Ratio Lower Upper

43 100

72 0.0 25.5 38.3#

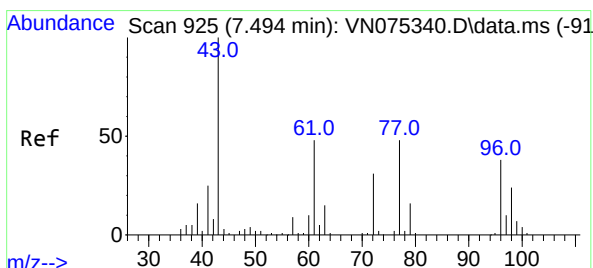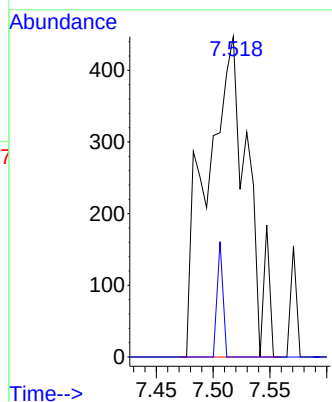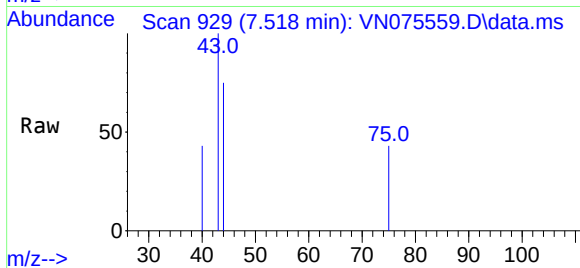

#27

cis-1,2-Dichloroethene

Concen: 0.584 ug/l

RT: 7.488 min Scan# 924

Delta R.T. -0.006 min

Lab File: VN075559.D

Acq: 05 Dec 2022 15:19




Tgt Ion: 96 Resp: 1104


Ion Ratio Lower Upper

96 100

61 110.4 0.0 278.8

98 46.6 0.0 128.4


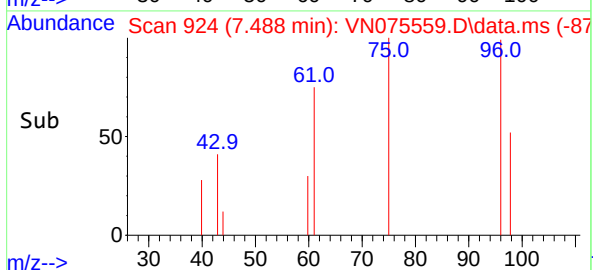

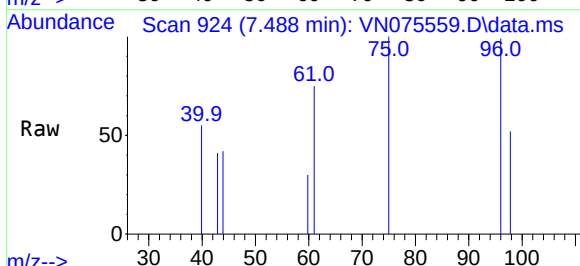


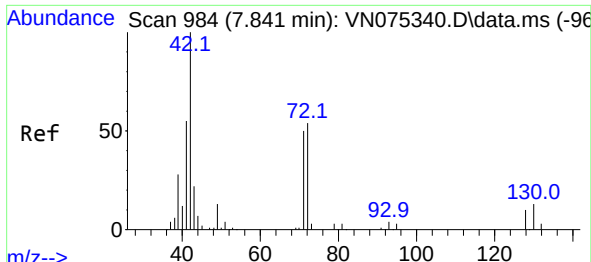

#29
Tetrahydrofuran
Concen: 0.533 ug/l
RT: 7.859 min Scan# 91
Delta R.T. 0.018 min
Lab File: VN075559.D
Acq: 05 Dec 2022 15:19




Instrument :
MSVOA_N
ClientSampleId :
HOWE-DRUM-A-1129


Tgt Ion: 42 Resp: 359
Ion Ratio Lower Upper
42 100
72 73.5 43.0 64.6#
71 0.0 39.9 59.9#

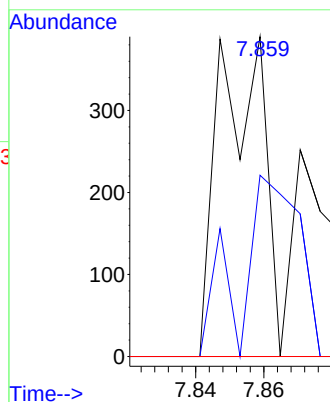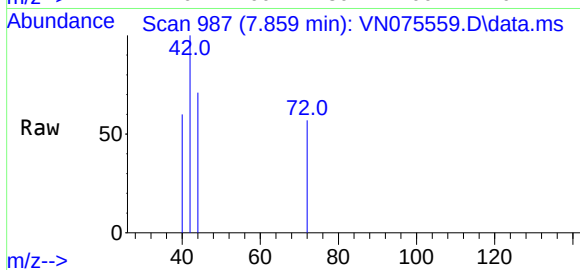

#31
Cyclohexane
Concen: 1.086 ug/l
RT: 8.229 min Scan# 1050
Delta R.T. -0.030 min
Lab File: VN075559.D
Acq: 05 Dec 2022 15:19

Tgt Ion: 56 Resp: 2934
Ion Ratio Lower Upper
56 100
69 138.2 25.2 37.8#
84 141.8 77.8 116.8#


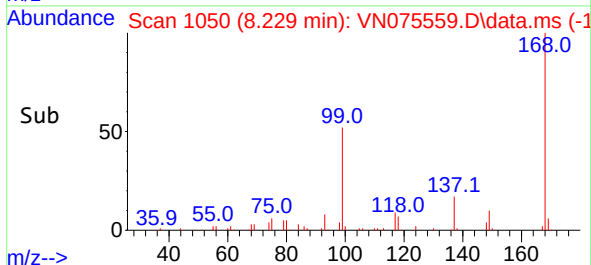

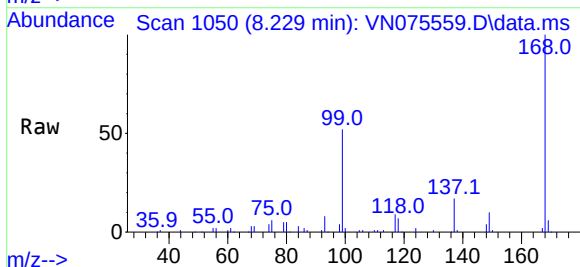




#33
1,2-Dichloroethane-d4
Concen: 59.791 ug/l
RT: 8.582 min Scan# 1110
Delta R.T. -0.001 min
Lab File: VN075559.D
Acq: 05 Dec 2022 15:19




Instrument :
MSVOA_N
ClientSampleId :
HOWE-DRUM-A-1129


Tgt Ion: 65 Resp: 50825
Ion Ratio Lower Upper
65 100
67 51.4 0.0 102.0

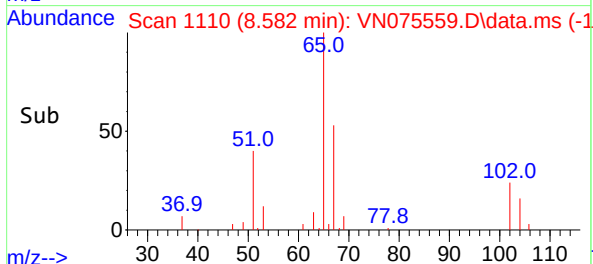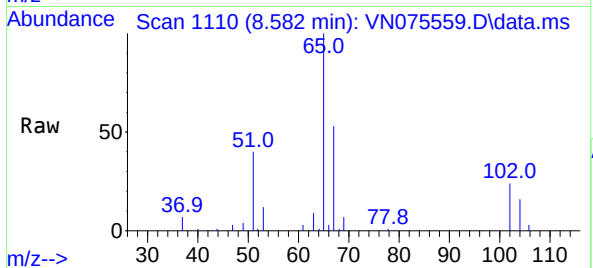

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 9.100 min Scan# 1198
Delta R.T. -0.006 min
Lab File: VN075559.D
Acq: 05 Dec 2022 15:19

Tgt Ion: 114 Resp: 254494
Ion Ratio Lower Upper
114 100
63 17.1 0.0 39.6
88 15.5 0.0 29.0


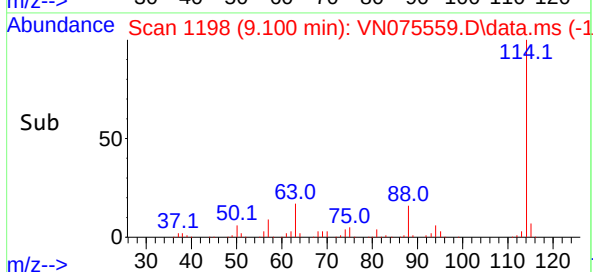

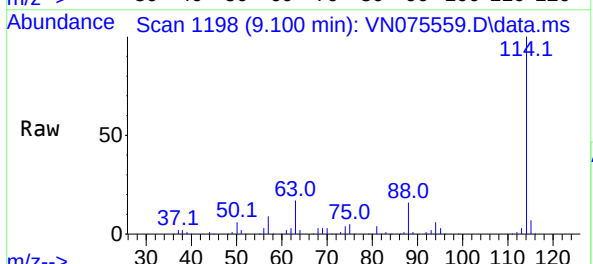


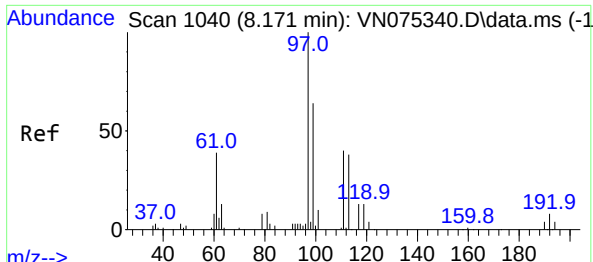

#35
Dibromofluoromethane
Concen: 63.216 ug/l
RT: 8.171 min Scan# 1040
Delta R.T. -0.000 min
Lab File: VN075559.D
Acq: 05 Dec 2022 15:19




Instrument :
MSVOA_N
ClientSampleId :
HOWE-DRUM-A-1129


Tgt Ion:113 Resp: 63199
Ion Ratio Lower Upper
113 100
111 102.9 80.5 120.7
192 19.7 13.2 19.8

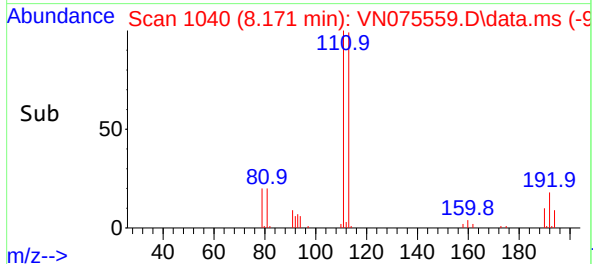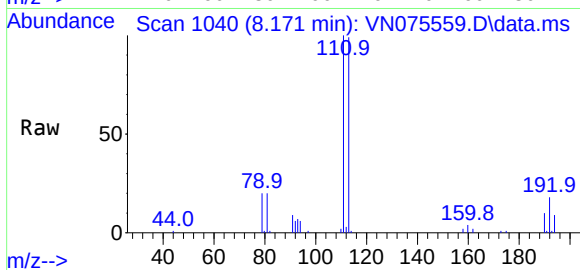

#36
1,1-Dichloropropene
Concen: 4.928 ug/l
RT: 8.224 min Scan# 1049
Delta R.T. -0.147 min
Lab File: VN075559.D
Acq: 05 Dec 2022 15:19


Tgt Ion: 75 Resp: 10745
Ion Ratio Lower Upper
75 100
110 10.0 17.8 53.3#
77 0.0 24.6 37.0#

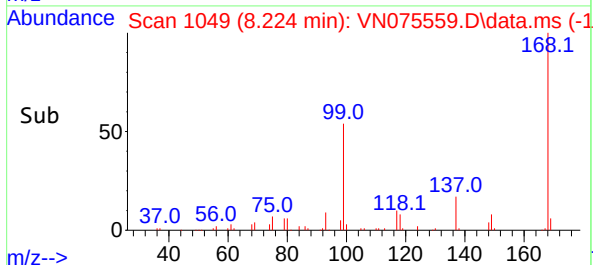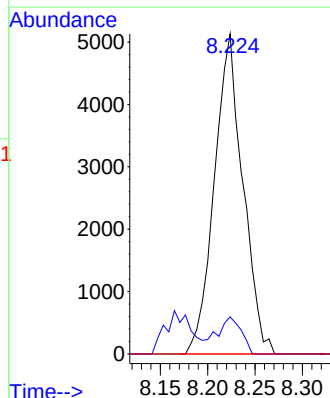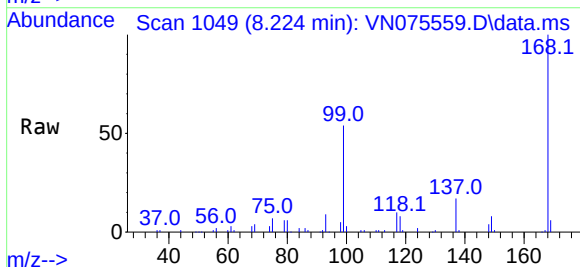



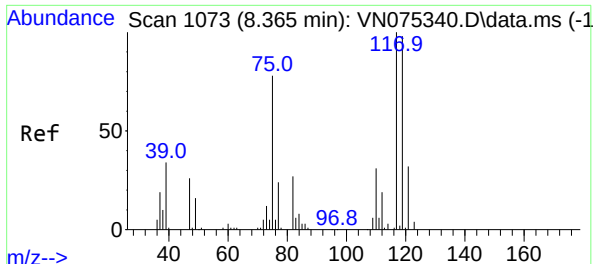


#38
Carbon Tetrachloride
Concen: 6.217 ug/l
RT: 8.224 min Scan# 1107
Delta R.T. -0.141 min
Lab File: VN075559.D
Acq: 05 Dec 2022 15:19

Instrument :
MSVOA_N
ClientSampleId :
HOWE-DRUM-A-1129



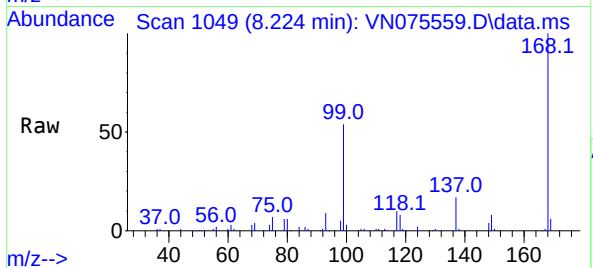



Tgt Ion:117 Resp: 14890
Ion Ratio Lower Upper
117 100
119 6.1 76.7 115.1#
121 0.0 23.9 35.9#

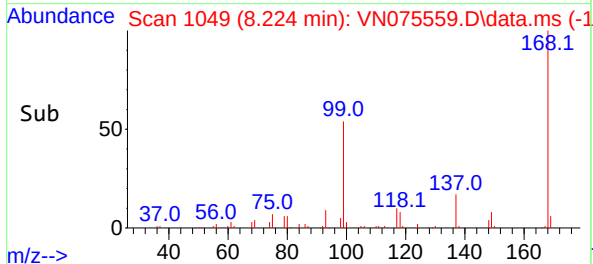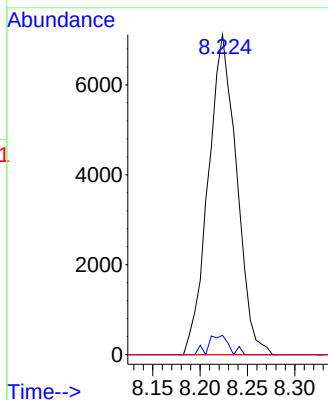

#43
Isopropyl Acetate
Concen: 1.133 ug/l
RT: 8.794 min Scan# 1146
Delta R.T. 0.106 min
Lab File: VN075559.D
Acq: 05 Dec 2022 15:19

Tgt Ion: 43 Resp: 3570
Ion Ratio Lower Upper
43 100
61 0.0 22.4 33.6#
87 0.0 12.5 18.7#

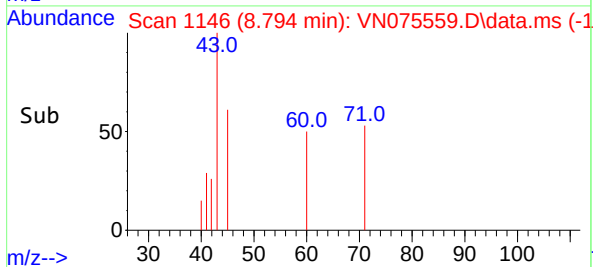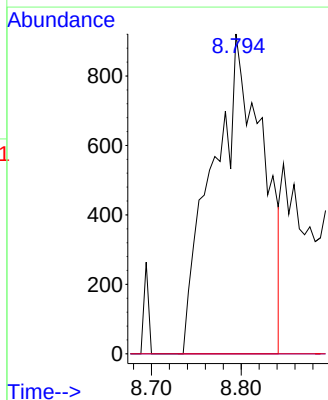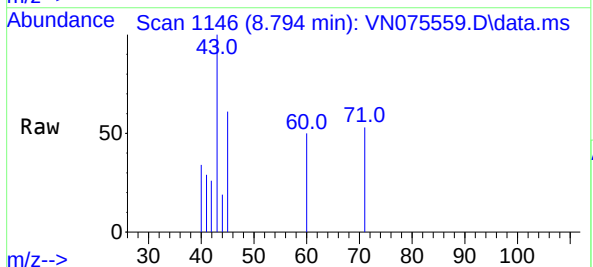



#44

Trichloroethene

Concen: 0.484 ug/l

RT: 9.359 min Scan# 11

Delta R.T. 0.006 min

Lab File: VN075559.D

Acq: 05 Dec 2022 15:19

Instrument :

MSVOA_N

ClientSampleId :





HOWE-DRUM-A-1129

Tgt Ion:130 Resp: 884

Ion Ratio Lower Upper

130 100

95 74.8 0.0 198.4

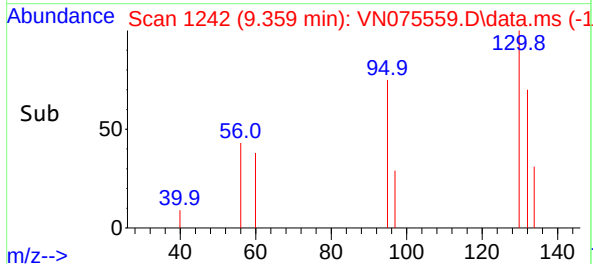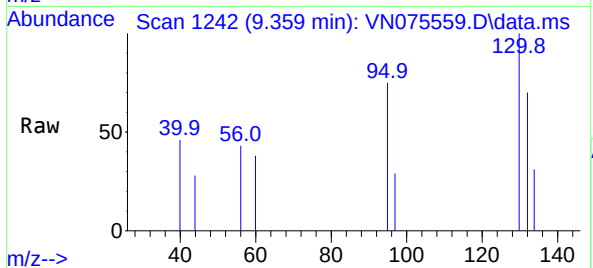

#50

Toluene-d8

Concen: 58.354 ug/l

RT: 10.565 min Scan# 1447

Delta R.T. -0.000 min

Lab File: VN075559.D




Acq: 05 Dec 2022 15:19


Tgt Ion: 98 Resp: 131395

Ion Ratio Lower Upper

98 100

100 66.1 53.0 79.6


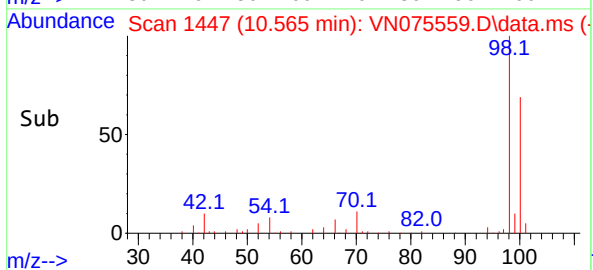

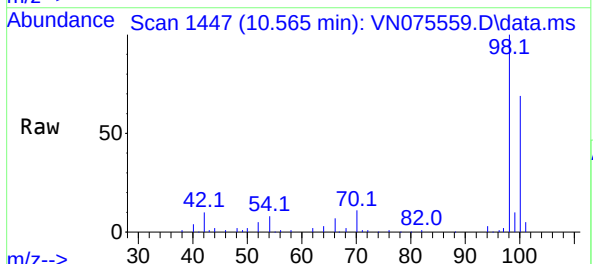




#51
4-Methyl-2-Pentanone
Concen: 0.420 ug/l
RT: 10.447 min Scan# 1427
Delta R.T. -0.000 min
Lab File: VN075559.D
Acq: 05 Dec 2022 15:19




Instrument :
MSVOA_N
ClientSampleId :
HOWE-DRUM-A-1129


Tgt Ion: 43 Resp: 843
Ion Ratio Lower Upper
43 100
58 15.1 33.6 50.4#

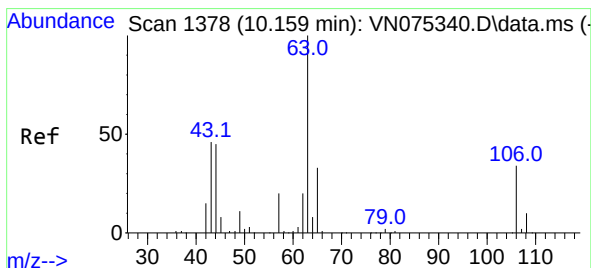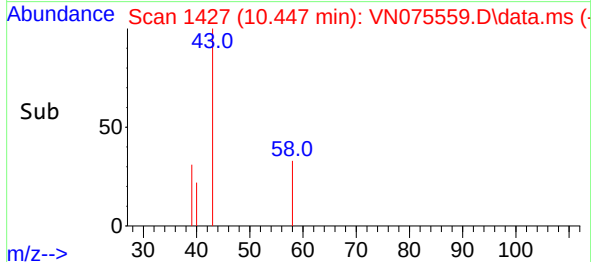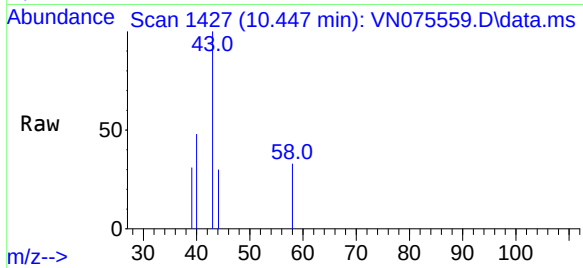

#58
2-Chloroethyl Vinyl ether
Concen: 0.792 ug/l
RT: 10.165 min Scan# 1379
Delta R.T. 0.006 min
Lab File: VN075559.D
Acq: 05 Dec 2022 15:19

Tgt Ion: 63 Resp: 676
Ion Ratio Lower Upper
63 100
106 7.8 24.8 37.2#


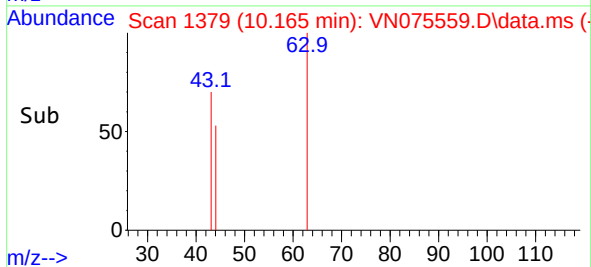

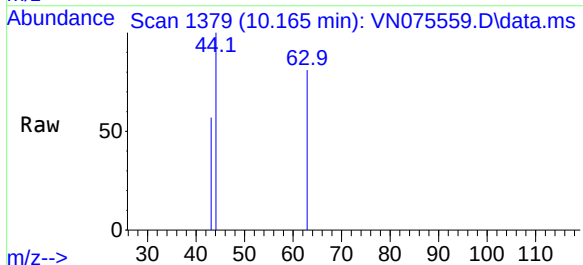




#59
2-Hexanone
Concen: 0.812 ug/l
RT: 11.206 min Scan# 11
Delta R.T. 0.012 min
Lab File: VN075559.D
Acq: 05 Dec 2022 15:19




Instrument :
MSVOA_N
ClientSampleId :
HOWE-DRUM-A-1129


Tgt Ion: 43 Resp: 1224
Ion Ratio Lower Upper
43 100
58 52.1 29.6 88.8

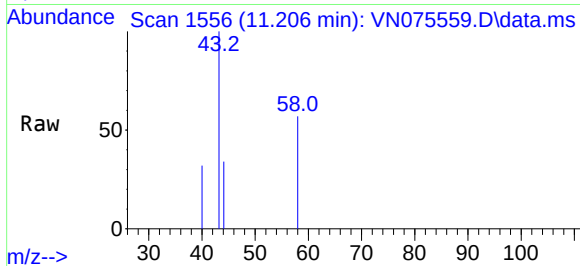

#62
4-Bromofluorobenzene
Concen: 54.505 ug/l
RT: 12.853 min Scan# 1836
Delta R.T. 0.006 min
Lab File: VN075559.D
Acq: 05 Dec 2022 15:19

Tgt Ion: 95 Resp: 90587
Ion Ratio Lower Upper
95 100
174 83.7 0.0 147.4
176 82.1 0.0 142.2


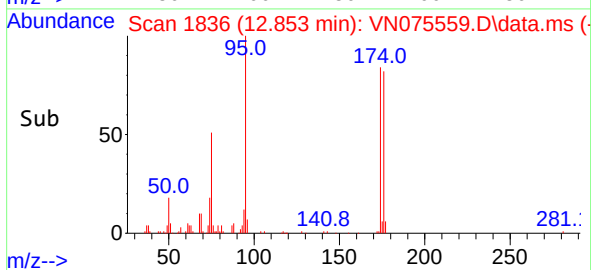

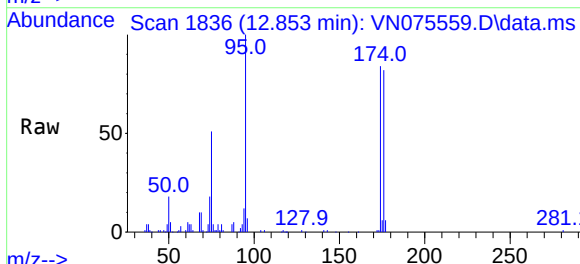




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.870 min Scan# 1170
Delta R.T. 0.005 min
Lab File: VN075559.D
Acq: 05 Dec 2022 15:19




Instrument :
MSVOA_N
ClientSampleId :
HOWE-DRUM-A-1129


Tgt Ion:117 Resp: 214529
Ion Ratio Lower Upper
117 100
82 53.6 43.1 64.7
119 32.5 25.5 38.3

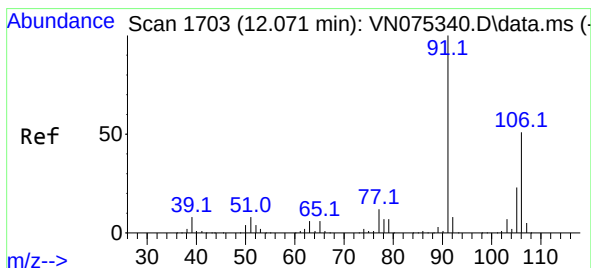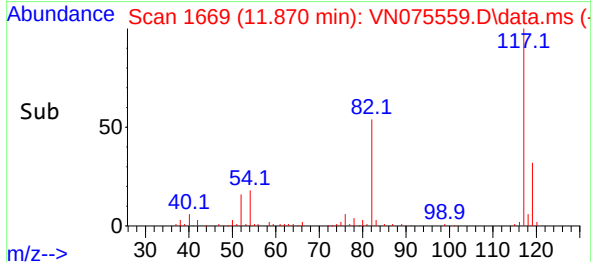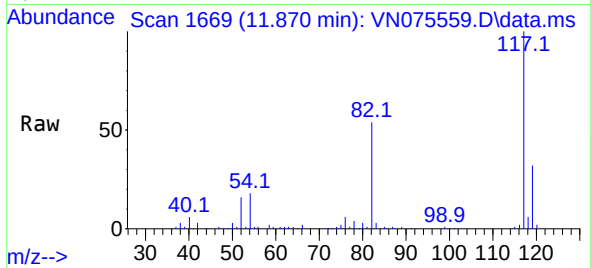

#68
m/p-Xylenes
Concen: 0.308 ug/l
RT: 12.076 min Scan# 1704
Delta R.T. 0.005 min
Lab File: VN075559.D
Acq: 05 Dec 2022 15:19

Tgt Ion:106 Resp: 946
Ion Ratio Lower Upper
106 100
91 214.0 156.0 234.0


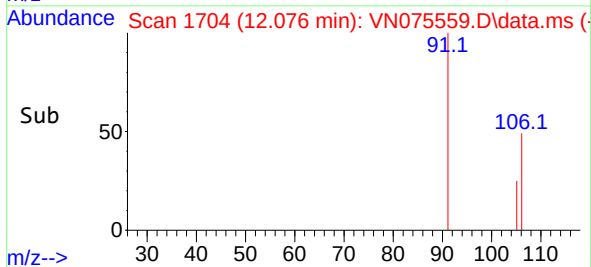

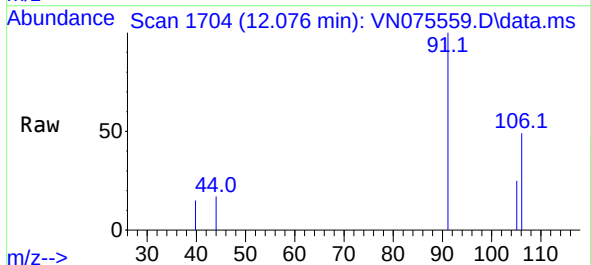




#72
 1,4-Dichlorobenzene-d4
 Concen: 50.000 ug/l
 RT: 13.794 min Scan# 1996
 Delta R.T. -0.000 min
 Lab File: VN075559.D
 Acq: 05 Dec 2022 15:19




Instrument :
 MSVOA_N
 ClientSampleId :
 HOWE-DRUM-A-1129


Tgt Ion:152 Resp: 94987
 Ion Ratio Lower Upper
 152 100
 115 56.7 30.2 90.6
 150 154.1 0.0 348.4

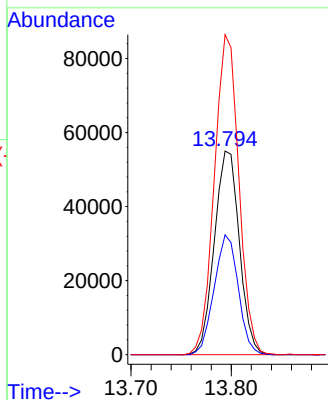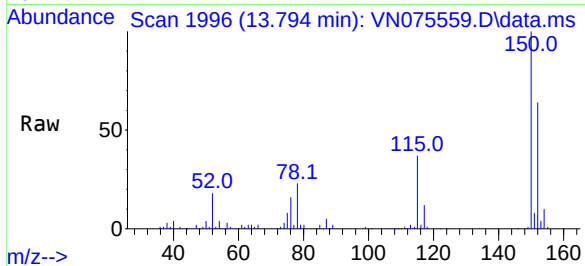

#76
 1,2,3-Trichloropropane
 Concen: 25.809 ug/l
 RT: 12.853 min Scan# 1836
 Delta R.T. -0.141 min
 Lab File: VN075559.D
 Acq: 05 Dec 2022 15:19

Tgt Ion: 75 Resp: 46352
 Ion Ratio Lower Upper
 75 100
 77 1.2 75.6 226.8#


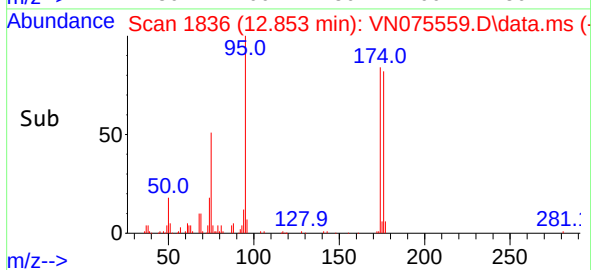
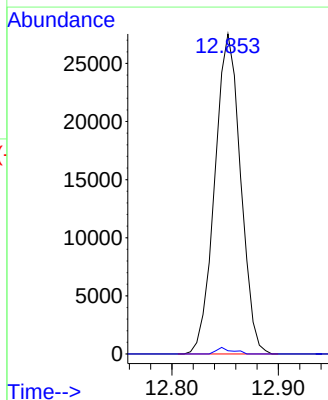
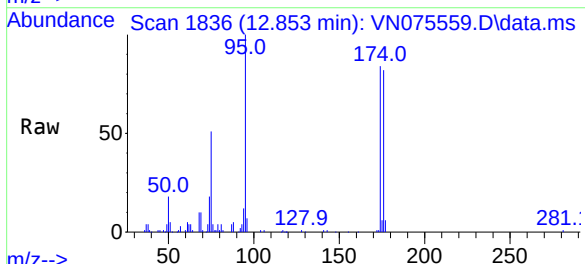




#77
Bromobenzene
Concen: 0.277 ug/l
RT: 12.976 min Scan# 1857
Delta R.T. -0.006 min
Lab File: VN075559.D
Acq: 05 Dec 2022 15:19




Instrument :
MSVOA_N
ClientSampleId :
HOWE-DRUM-A-1129


Tgt Ion:	156	Resp:	474
Ion	Ratio	Lower	Upper
156	100		
77	152.3	108.5	325.5
158	83.3	47.7	143.1

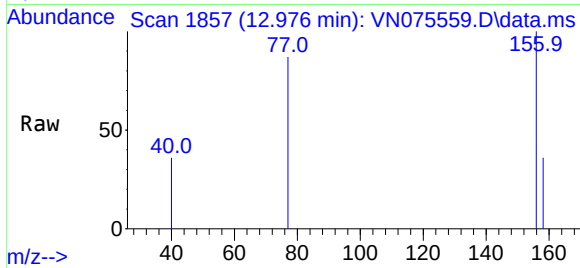

#81
trans-1,4-Dichloro-2-butene
Concen: 76.363 ug/l
RT: 12.853 min Scan# 1836
Delta R.T. 0.118 min
Lab File: VN075559.D
Acq: 05 Dec 2022 15:19

Tgt Ion:	75	Resp:	46352
Ion	Ratio	Lower	Upper
75	100		
53	0.0	78.5	117.7#
89	0.0	37.7	56.5#

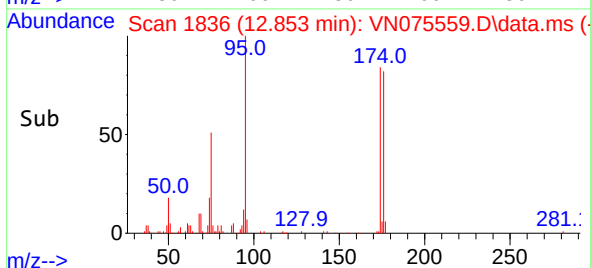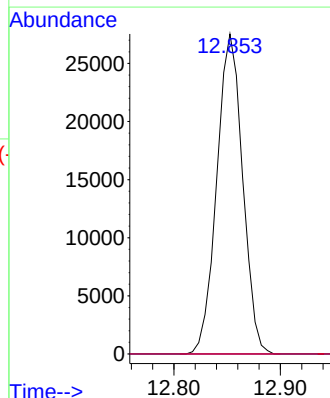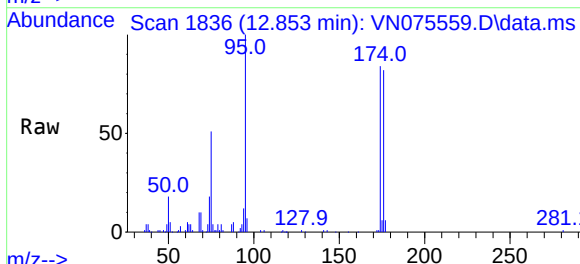



#87

1,3-Dichlorobenzene

Concen: 0.296 ug/l

RT: 13.735 min Scan# 1986

Delta R.T. -0.000 min

Lab File: VN075559.D


Acq: 05 Dec 2022 15:19

Instrument :

MSVOA_N




ClientSampleId :

HOWE-DRUM-A-1129

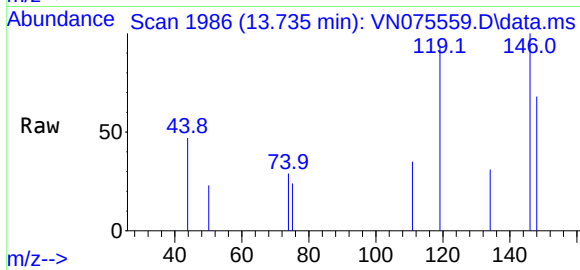

Tgt Ion:146 Resp: 960

Ion	Ratio	Lower	Upper
146	100		
111	41.1	20.8	62.5
148	85.2	31.1	93.5

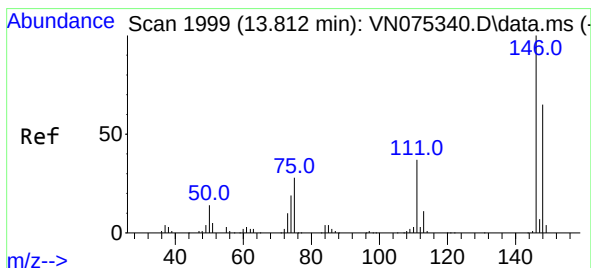

#88

1,4-Dichlorobenzene

Concen: 0.291 ug/l

RT: 13.735 min Scan# 1986




Delta R.T. -0.077 min


Lab File: VN075559.D

Acq: 05 Dec 2022 15:19

Tgt Ion:146 Resp: 960

Ion	Ratio	Lower	Upper
146	100		
111	41.1	20.1	60.3
148	85.2	31.9	95.7

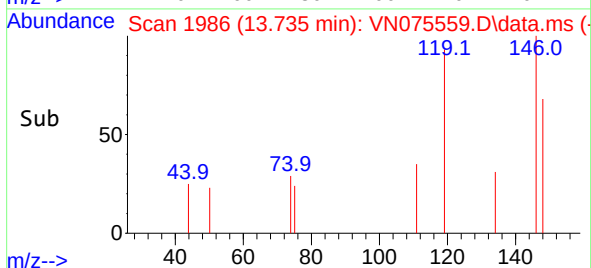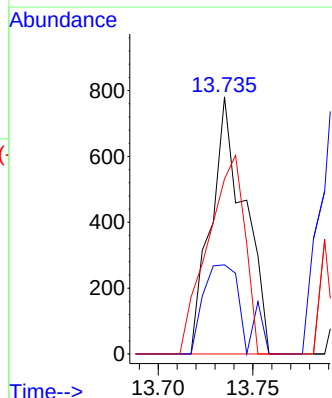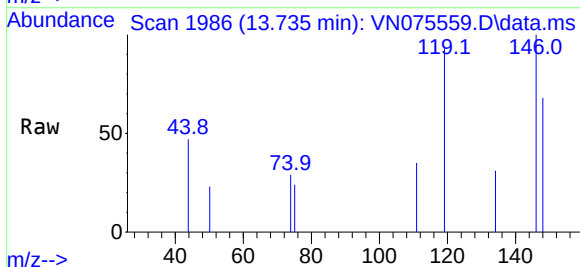



#89

n-Butylbenzene

Concen: 0.304 ug/l

RT: 14.053 min Scan# 2040

Delta R.T. -0.006 min

Lab File: VN075559.D

Acq: 05 Dec 2022 15:19





Instrument :

MSVOA_N

ClientSampleId :

HOWE-DRUM-A-1129

Tgt Ion: 91	Resp:	1541
Ion	Ratio	Lower Upper
91	100	
92	38.0	26.5 79.4
134	18.2	13.0 39.0

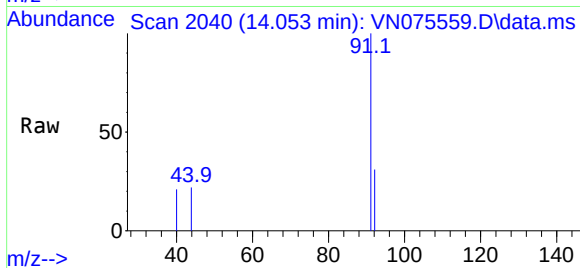

#91

1,2-Dichlorobenzene

Concen: 0.348 ug/l




RT: 14.111 min Scan# 2050


Delta R.T. 0.005 min

Lab File: VN075559.D

Acq: 05 Dec 2022 15:19

Tgt Ion: 146	Resp:	1102
Ion	Ratio	Lower Upper
146	100	
111	37.6	21.3 63.9
148	75.0	31.4 94.2


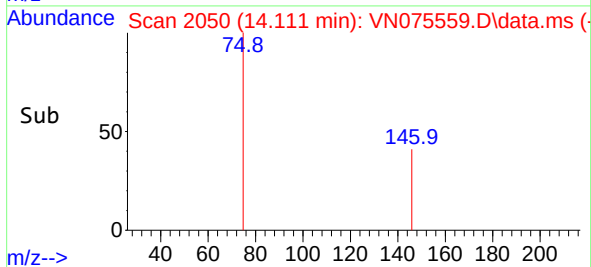

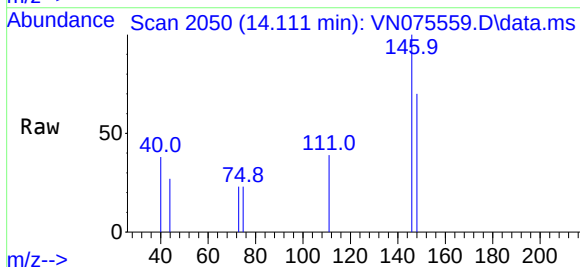


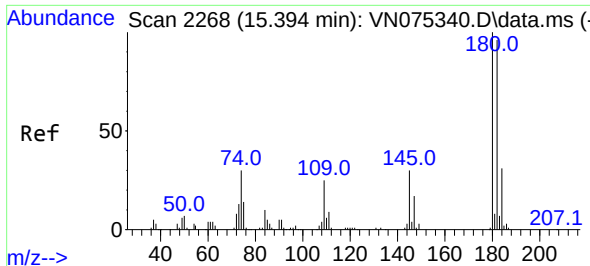

#93
1,2,4-Trichlorobenzene
Concen: 0.786 ug/l
RT: 15.400 min Scan# 211
Delta R.T. 0.006 min
Lab File: VN075559.D
Acq: 05 Dec 2022 15:19




Instrument :
MSVOA_N
ClientSampleId :
HOWE-DRUM-A-1129


Tgt Ion:	180	Resp:	1275
Ion	Ratio	Lower	Upper
180	100		
182	132.6	47.8	143.4
145	22.6	16.8	50.3

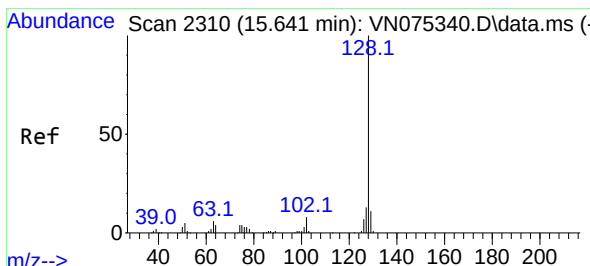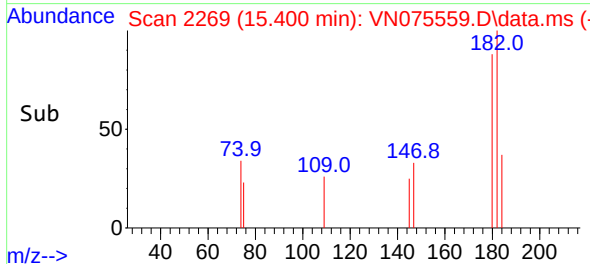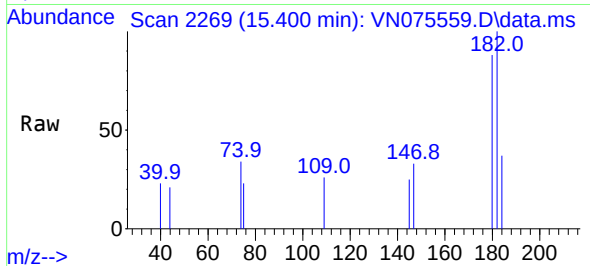

#95
Naphthalene
Concen: 1.452 ug/l
RT: 15.647 min Scan# 2311
Delta R.T. 0.006 min
Lab File: VN075559.D
Acq: 05 Dec 2022 15:19

Tgt Ion:	128	Resp:	7406
Ion	Ratio	Lower	Upper
128	100		
127	13.2	10.4	15.6
129	9.7	8.6	12.8

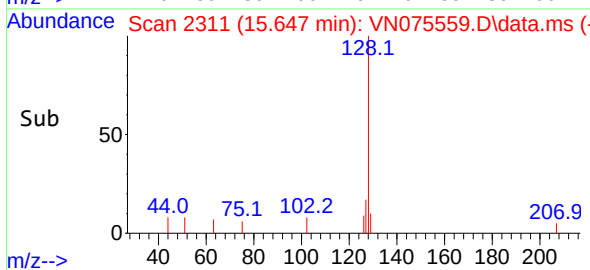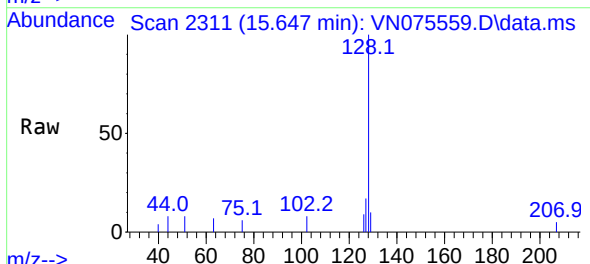



#96

1,2,3-Trichlorobenzene

Concen: 1.065 ug/l

RT: 15.841 min Scan# 21

Delta R.T. -0.000 min

Lab File: VN075559.D


Acq: 05 Dec 2022 15:19

Instrument :

MSVOA_N

ClientSampleId :

HOWE-DRUM-A-1129

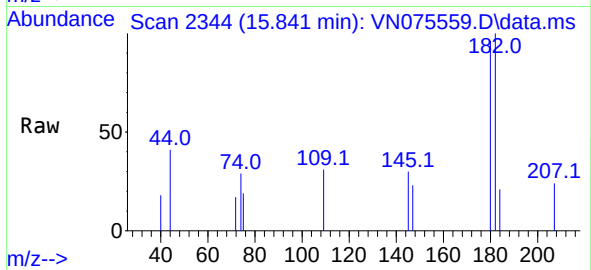

Tgt Ion:180 Resp: 1697

Ion Ratio Lower Upper

180 100

182 105.0 47.3 141.8

145 26.2 17.6 52.9

