

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN120522\
 Data File : VN075563.D
 Acq On : 05 Dec 2022 16:55
 Operator : JC\MD
 Sample : N5836-01 400X
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 JAM-VRG-1201DL

Quant Time: Dec 06 03:25:45 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N112122W.M
 Quant Title : SW846 8260
 QLast Update : Wed Nov 23 00:18:03 2022
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.230	168	167506	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.106	114	279675	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.871	117	244994	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.794	152	106538	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.589	65	45158	50.223	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	= 100.440%	
35) Dibromofluoromethane	8.171	113	56883	51.775	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	= 103.560%	
50) Toluene-d8	10.571	98	114993	46.472	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	= 92.940%	
62) 4-Bromofluorobenzene	12.853	95	83947	45.962	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	= 91.920%	
Target Compounds						
					Qvalue	
6) Chloroethane	3.124	64	430	0.283	ug/l #	45
8) Diethyl Ether	3.971	74	2045	2.033	ug/l	98
11) Tert butyl alcohol	5.530	59	8379	22.199	ug/l #	78
16) Acetone	4.448	43	13975	16.663	ug/l	96
18) Methyl Acetate	5.042	43	7080	2.108	ug/l	94
19) Methyl tert-butyl Ether	5.818	73	16509	3.004	ug/l	98
20) Methylene Chloride	5.283	84	1543	Below Cal	#	72
22) Diisopropyl ether	6.683	45	5715	1.248	ug/l #	1
25) 2-Butanone	7.494	43	8044	6.870	ug/l	89
27) cis-1,2-Dichloroethene	7.494	96	558	0.279	ug/l	71
31) Cyclohexane	8.224	56	3892	1.362	ug/l #	39
36) 1,1-Dichloropropene	8.230	75	11697	4.882	ug/l #	51
37) Ethyl Acetate	7.494	43	8044	3.729	ug/l #	78
38) Carbon Tetrachloride	8.224	117	16062	6.103	ug/l #	16
40) Benzene	8.612	78	208144	28.375	ug/l	99
42) 1,2-Dichloroethane	8.612	62	1718	0.699	ug/l #	75
51) 4-Methyl-2-Pentanone	10.447	43	962	0.436	ug/l #	75
52) Toluene	10.630	92	175069	37.035	ug/l	99
53) t-1,3-Dichloropropene	10.741	75	826	0.321	ug/l #	83
59) 2-Hexanone	11.206	43	403	0.243	ug/l #	21
67) Ethyl Benzene	11.965	91	11958	1.385	ug/l	96
68) m/p-Xylenes	12.071	106	24026	6.854	ug/l	95
69) o-Xylene	12.406	106	8995	2.583	ug/l	94
71) Bromoform	12.847	173	583	0.406	ug/l #	28
76) 1,2,3-Trichloropropane	12.853	75	42928	21.311	ug/l #	1
80) 1,3,5-Trimethylbenzene	13.176	105	4092	0.633	ug/l	99
81) trans-1,4-Dichloro-2-b...	12.853	75	42928	63.055	ug/l #	10
84) 1,2,4-Trimethylbenzene	13.488	105	7151	1.102	ug/l	99
90) Hexachloroethane	14.447	117	237	0.204	ug/l #	19
95) Naphthalene	15.653	128	1367	0.239	ug/l #	69

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Quant Time: Dec 06 03:25:45 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N112122W.M
Quant Title : SW846 8260
QLast Update : Wed Nov 23 00:18:03 2022
Response via : Initial Calibration







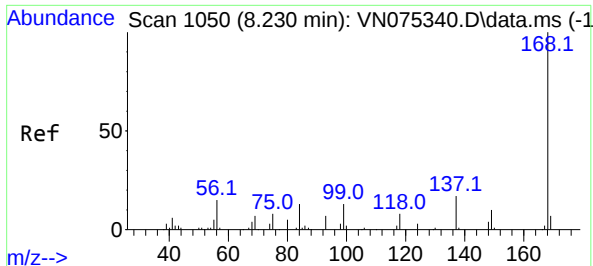

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.230 min Scan# 1050
Delta R.T. -0.000 min
Lab File: VN075563.D
Acq: 05 Dec 2022 16:55



Instrument :
MSVOA_N
ClientSampleId :
JAM-VRG-1201DL


Tgt Ion:168 Resp: 167506
Ion Ratio Lower Upper
168 100
99 55.6 51.6 77.4



#6
Chloroethane
Concen: 0.283 ug/l
RT: 3.124 min Scan# 182
Delta R.T. 0.017 min
Lab File: VN075563.D
Acq: 05 Dec 2022 16:55

Tgt Ion: 64 Resp: 430
Ion Ratio Lower Upper
64 100
66 0.0 23.8 35.8#





#8
Diethyl Ether

Concen: 2.033 ug/l

RT: 3.971 min Scan# 31

Delta R.T. 0.006 min

Lab File: VN075563.D

Acq: 05 Dec 2022 16:55

Instrument :

MSVOA_N

ClientSampleId :





JAM-VRG-1201DL

Tgt Ion: 74 Resp: 2045

Ion Ratio Lower Upper

74 100

45 80.6 39.3 117.9



#11

Tert butyl alcohol

Concen: 22.199 ug/l

RT: 5.530 min Scan# 591

Delta R.T. -0.012 min

Lab File: VN075563.D




Acq: 05 Dec 2022 16:55


Tgt Ion: 59 Resp: 8379

Ion Ratio Lower Upper

59 100

57 2.2 8.5 12.7#









#16
Acetone
Concen: 16.663 ug/l
RT: 4.448 min Scan# 405
Delta R.T. 0.012 min
Lab File: VN075563.D
Acq: 05 Dec 2022 16:55




Instrument :
MSVOA_N
ClientSampleId :
JAM-VRG-1201DL


Tgt Ion: 43 Resp: 13975
Ion Ratio Lower Upper
43 100
58 33.9 25.5 38.3



#18
Methyl Acetate
Concen: 2.108 ug/l
RT: 5.042 min Scan# 508
Delta R.T. 0.006 min
Lab File: VN075563.D
Acq: 05 Dec 2022 16:55

Tgt Ion: 43 Resp: 7080
Ion Ratio Lower Upper
43 100
74 24.2 22.0 33.0





#19

Methyl tert-butyl Ether

Concen: 3.004 ug/l

RT: 5.818 min Scan# 64

Delta R.T. 0.012 min

Lab File: VN075563.D

Acq: 05 Dec 2022 16:55

Instrument :

MSVOA_N

ClientSampleId :





JAM-VRG-1201DL

Tgt Ion: 73 Resp: 16509

Ion Ratio Lower Upper

73 100

57 21.2 16.3 24.5



#20

Methylene Chloride

Concen: Below Cal

RT: 5.283 min Scan# 549

Delta R.T. -0.006 min

Lab File: VN075563.D

Acq: 05 Dec 2022 16:55

Tgt Ion: 84 Resp: 1543




Ion Ratio Lower Upper


84 100

49 99.2 94.9 142.3

51 0.0 26.8 40.2#

86 43.6 53.7 80.5#









#22
Diisopropyl ether
Concen: 1.248 ug/l
RT: 6.683 min Scan# 71
Delta R.T. 0.006 min
Lab File: VN075563.D
Acq: 05 Dec 2022 16:55




Instrument :
MSVOA_N
ClientSampleId :
JAM-VRG-1201DL


Tgt Ion:	45	Resp:	5715
Ion	Ratio	Lower	Upper
45	100		
43	0.0	42.8	64.2#
87	0.0	28.4	42.6#
59	164.8	10.4	15.6#



#25
2-Butanone
Concen: 6.870 ug/l
RT: 7.494 min Scan# 925
Delta R.T. 0.005 min
Lab File: VN075563.D
Acq: 05 Dec 2022 16:55

Tgt Ion:	43	Resp:	8044
Ion	Ratio	Lower	Upper
43	100		
72	37.9	25.5	38.3









#27
cis-1,2-Dichloroethene
Concen: 0.279 ug/l
RT: 7.494 min Scan# 91
Delta R.T. 0.000 min
Lab File: VN075563.D
Acq: 05 Dec 2022 16:55




Instrument :
MSVOA_N
ClientSampleId :
JAM-VRG-1201DL


Tgt Ion: 96 Resp: 558
Ion Ratio Lower Upper
96 100
61 124.2 0.0 278.8
98 14.2 0.0 128.4



#31
Cyclohexane
Concen: 1.362 ug/l
RT: 8.224 min Scan# 1049
Delta R.T. -0.035 min
Lab File: VN075563.D
Acq: 05 Dec 2022 16:55

Tgt Ion: 56 Resp: 3892
Ion Ratio Lower Upper
56 100
69 146.8 25.2 37.8#
84 110.7 77.8 116.8









#33
1,2-Dichloroethane-d4
Concen: 50.223 ug/l
RT: 8.589 min Scan# 1110
Delta R.T. 0.006 min
Lab File: VN075563.D
Acq: 05 Dec 2022 16:55




Instrument :
MSVOA_N
ClientSampleId :
JAM-VRG-1201DL


Tgt Ion: 65 Resp: 45158
Ion Ratio Lower Upper
65 100
67 52.2 0.0 102.0



#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 9.106 min Scan# 1199
Delta R.T. 0.000 min
Lab File: VN075563.D
Acq: 05 Dec 2022 16:55


Tgt Ion: 114 Resp: 279675
Ion Ratio Lower Upper
114 100
63 17.7 0.0 39.6
88 13.9 0.0 29.0








#35
Dibromofluoromethane
Concen: 51.775 ug/l
RT: 8.171 min Scan# 1040
Delta R.T. -0.000 min
Lab File: VN075563.D
Acq: 05 Dec 2022 16:55


Instrument :
MSVOA_N
ClientSampleId :
JAM-VRG-1201DL





Tgt Ion:113 Resp: 56883
Ion Ratio Lower Upper
113 100
111 101.3 80.5 120.7
192 19.3 13.2 19.8




#36
1,1-Dichloropropene
Concen: 4.882 ug/l
RT: 8.230 min Scan# 1050
Delta R.T. -0.141 min
Lab File: VN075563.D
Acq: 05 Dec 2022 16:55



Tgt Ion: 75 Resp: 11697
Ion Ratio Lower Upper
75 100
110 10.3 17.8 53.3#
77 0.0 24.6 37.0#









#37
Ethyl Acetate
Concen: 3.729 ug/l
RT: 7.494 min Scan# 91
Delta R.T. -0.071 min
Lab File: VN075563.D
Acq: 05 Dec 2022 16:55




Instrument :
MSVOA_N
ClientSampleId :
JAM-VRG-1201DL


Tgt Ion: 43 Resp: 8044
Ion Ratio Lower Upper
43 100
61 8.6 12.2 18.4#
70 0.0 9.4 14.2#



#38
Carbon Tetrachloride
Concen: 6.103 ug/l
RT: 8.224 min Scan# 1049
Delta R.T. -0.141 min
Lab File: VN075563.D
Acq: 05 Dec 2022 16:55

Tgt Ion: 117 Resp: 16062
Ion Ratio Lower Upper
117 100
119 5.6 76.7 115.1#
121 0.0 23.9 35.9#









#40
Benzene
Concen: 28.375 ug/l
RT: 8.612 min Scan# 1115
Delta R.T. 0.006 min
Lab File: VN075563.D
Acq: 05 Dec 2022 16:55




Instrument :
MSVOA_N
ClientSampleId :
JAM-VRG-1201DL


Tgt Ion: 78 Resp: 208144
Ion Ratio Lower Upper
78 100
77 23.8 19.4 29.0



#42
1,2-Dichloroethane
Concen: 0.699 ug/l
RT: 8.612 min Scan# 1115
Delta R.T. -0.059 min
Lab File: VN075563.D
Acq: 05 Dec 2022 16:55

Tgt Ion: 62 Resp: 1718
Ion Ratio Lower Upper
62 100
98 0.0 0.0 18.2









#50
Toluene-d8
Concen: 46.472 ug/l
RT: 10.571 min Scan# 1447
Delta R.T. 0.006 min
Lab File: VN075563.D
Acq: 05 Dec 2022 16:55




Instrument :
MSVOA_N
ClientSampleId :
JAM-VRG-1201DL


Tgt Ion: 98 Resp: 114993
Ion Ratio Lower Upper
98 100
100 66.2 53.0 79.6



#51
4-Methyl-2-Pentanone
Concen: 0.436 ug/l
RT: 10.447 min Scan# 1427
Delta R.T. 0.000 min
Lab File: VN075563.D
Acq: 05 Dec 2022 16:55

Tgt Ion: 43 Resp: 962
Ion Ratio Lower Upper
43 100
58 26.2 33.6 50.4#









#52
Toluene
Concen: 37.035 ug/l
RT: 10.630 min Scan# 1458
Delta R.T. -0.000 min
Lab File: VN075563.D
Acq: 05 Dec 2022 16:55




Instrument :
MSVOA_N
ClientSampleId :
JAM-VRG-1201DL


Tgt Ion: 92 Resp: 175069
Ion Ratio Lower Upper
92 100
91 168.0 135.4 203.2



#53
t-1,3-Dichloropropene
Concen: 0.321 ug/l
RT: 10.741 min Scan# 1477
Delta R.T. -0.094 min
Lab File: VN075563.D
Acq: 05 Dec 2022 16:55

Tgt Ion: 75 Resp: 826
Ion Ratio Lower Upper
75 100
77 41.3 25.4 38.2#









#59
2-Hexanone
Concen: 0.243 ug/l
RT: 11.206 min Scan# 11
Delta R.T. 0.012 min
Lab File: VN075563.D
Acq: 05 Dec 2022 16:55




Instrument :
MSVOA_N
ClientSampleId :
JAM-VRG-1201DL


Tgt Ion: 43 Resp: 403
Ion Ratio Lower Upper
43 100
58 0.0 29.6 88.8#



#62
4-Bromofluorobenzene
Concen: 45.962 ug/l
RT: 12.853 min Scan# 1836
Delta R.T. 0.006 min
Lab File: VN075563.D
Acq: 05 Dec 2022 16:55

Tgt Ion: 95 Resp: 83947
Ion Ratio Lower Upper
95 100
174 86.4 0.0 147.4
176 84.3 0.0 142.2









#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.871 min Scan# 117
Delta R.T. 0.006 min
Lab File: VN075563.D
Acq: 05 Dec 2022 16:55




Instrument :
MSVOA_N
ClientSampleId :
JAM-VRG-1201DL


Tgt Ion:117 Resp: 244994
Ion Ratio Lower Upper
117 100
82 49.7 43.1 64.7
119 30.8 25.5 38.3



#67
Ethyl Benzene
Concen: 1.385 ug/l
RT: 11.965 min Scan# 1685
Delta R.T. -0.000 min
Lab File: VN075563.D
Acq: 05 Dec 2022 16:55

Tgt Ion: 91 Resp: 11958
Ion Ratio Lower Upper
91 100
106 33.3 24.9 37.3









#68
m/p-Xylenes
Concen: 6.854 ug/l
RT: 12.071 min Scan# 11
Delta R.T. -0.000 min
Lab File: VN075563.D
Acq: 05 Dec 2022 16:55




Instrument :
MSVOA_N
ClientSampleId :
JAM-VRG-1201DL


Tgt Ion:106 Resp: 24026
Ion Ratio Lower Upper
106 100
91 203.2 156.0 234.0



#69
o-Xylene
Concen: 2.583 ug/l
RT: 12.406 min Scan# 1760
Delta R.T. 0.006 min
Lab File: VN075563.D
Acq: 05 Dec 2022 16:55

Tgt Ion:106 Resp: 8995
Ion Ratio Lower Upper
106 100
91 201.6 105.2 315.5









#71
Bromoform
Concen: 0.406 ug/l
RT: 12.847 min Scan# 11
Delta R.T. 0.271 min
Lab File: VN075563.D
Acq: 05 Dec 2022 16:55




Instrument :
MSVOA_N
ClientSampleId :
JAM-VRG-1201DL


Tgt Ion:173 Resp: 583
Ion Ratio Lower Upper
173 100
175 0.0 24.6 74.0#
254 0.0 0.0 0.0



#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.794 min Scan# 1996
Delta R.T. 0.000 min
Lab File: VN075563.D
Acq: 05 Dec 2022 16:55

Tgt Ion:152 Resp: 106538
Ion Ratio Lower Upper
152 100
115 57.7 30.2 90.6
150 154.8 0.0 348.4









#76
1,2,3-Trichloropropane
Concen: 21.311 ug/l
RT: 12.853 min Scan# 1836
Delta R.T. -0.141 min
Lab File: VN075563.D
Acq: 05 Dec 2022 16:55




Instrument :
MSVOA_N
ClientSampleId :
JAM-VRG-1201DL


Tgt Ion: 75 Resp: 42928
Ion Ratio Lower Upper
75 100
77 0.5 75.6 226.8#



#80
1,3,5-Trimethylbenzene
Concen: 0.633 ug/l
RT: 13.176 min Scan# 1891
Delta R.T. 0.000 min
Lab File: VN075563.D
Acq: 05 Dec 2022 16:55

Tgt Ion: 105 Resp: 4092
Ion Ratio Lower Upper
105 100
120 49.9 24.7 74.1









#81
trans-1,4-Dichloro-2-butene
Concen: 63.055 ug/l
RT: 12.853 min Scan# 1836
Delta R.T. 0.118 min
Lab File: VN075563.D
Acq: 05 Dec 2022 16:55




Instrument :
MSVOA_N
ClientSampleId :
JAM-VRG-1201DL


Tgt Ion: 75 Resp: 42928
Ion Ratio Lower Upper
75 100
53 0.0 78.5 117.7#
89 0.0 37.7 56.5#



#84
1,2,4-Trimethylbenzene
Concen: 1.102 ug/l
RT: 13.488 min Scan# 1944
Delta R.T. 0.006 min
Lab File: VN075563.D
Acq: 05 Dec 2022 16:55


Tgt Ion: 105 Resp: 7151
Ion Ratio Lower Upper
105 100
120 44.9 22.7 68.1








#90
Hexachloroethane
Concen: 0.204 ug/l
RT: 14.447 min Scan# 2107
Delta R.T. 0.112 min
Lab File: VN075563.D
Acq: 05 Dec 2022 16:55

Instrument :
MSVOA_N
ClientSampleId :
JAM-VRG-1201DL



Tgt Ion:117 Resp: 237
Ion Ratio Lower Upper
117 100
201 0.0 31.5 94.5#



#95
Naphthalene
Concen: 0.239 ug/l
RT: 15.653 min Scan# 2312
Delta R.T. 0.012 min
Lab File: VN075563.D
Acq: 05 Dec 2022 16:55

Tgt Ion:128 Resp: 1367
Ion Ratio Lower Upper
128 100
127 0.0 10.4 15.6#
129 0.0 8.6 12.8#

