
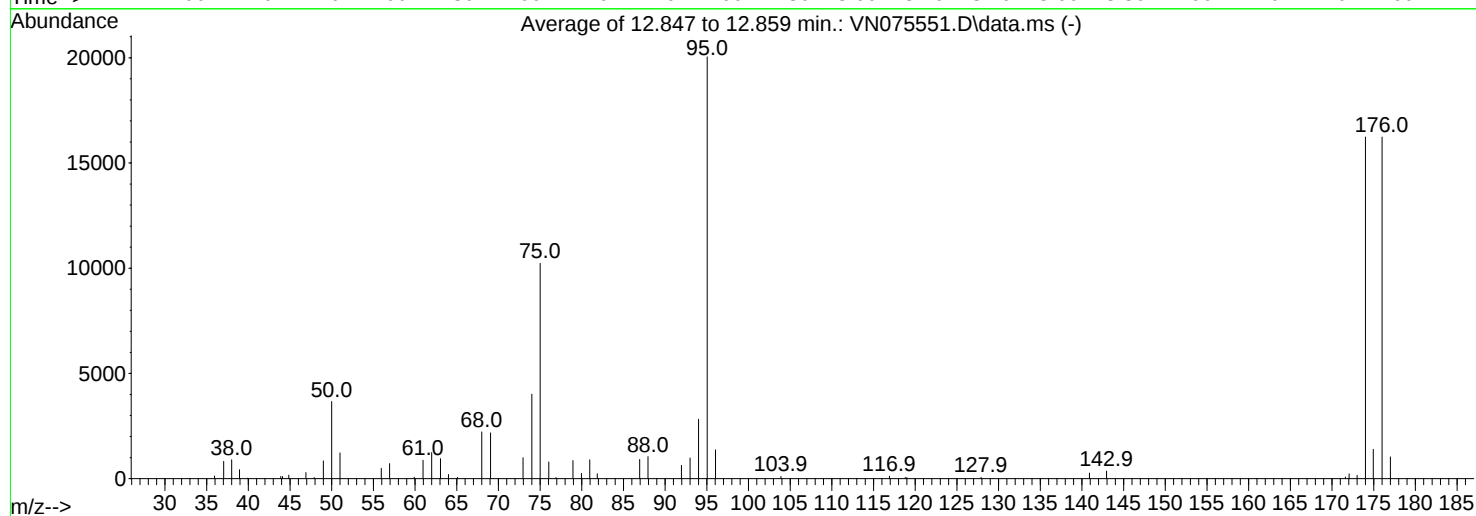


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN120522\
 Data File : VN075551.D
 Acq On : 05 Dec 2022 10:23
 Operator : JC\MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N112122W.M
 Title : SW846 8260
 Last Update : Wed Nov 23 00:18:03 2022

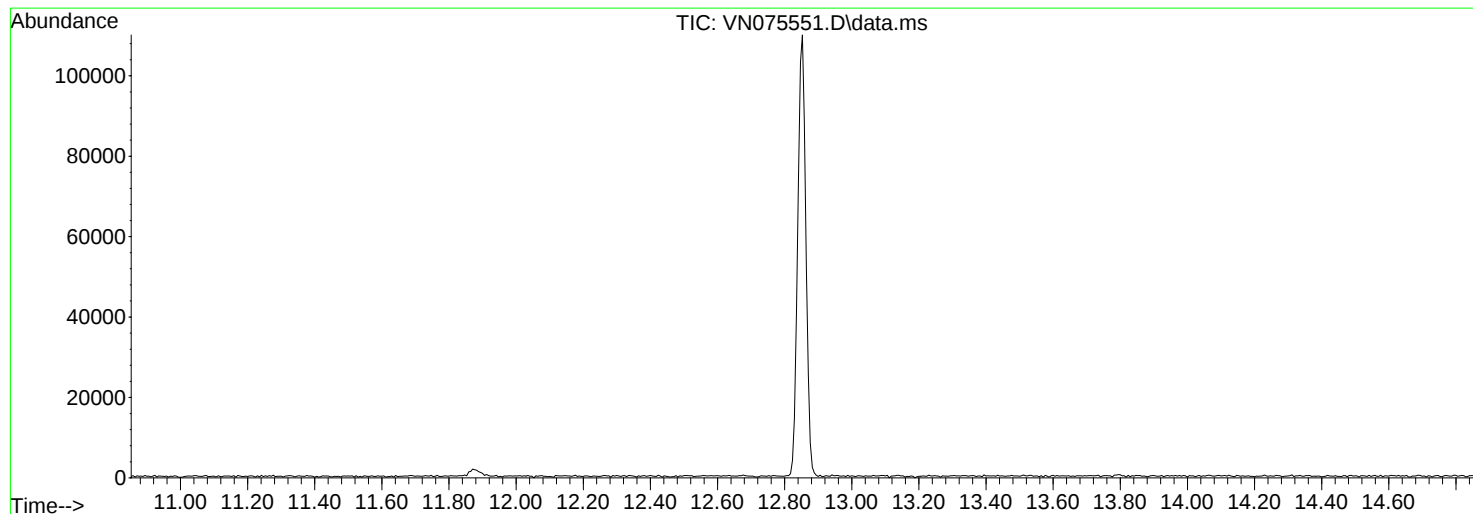

AutoFind: Scans 1835, 1836, 1837; Background Corrected with Scan 1827

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.3	3669	PASS
75	95	30	60	51.1	10235	PASS
95	95	100	100	100.0	20045	PASS
96	95	5	9	6.8	1366	PASS
173	174	0.00	2	1.0	160	PASS
174	95	50	100	81.0	16231	PASS
175	174	5	9	8.6	1390	PASS
176	174	95	101	100.0	16231	PASS
177	176	5	9	6.4	1032	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.95	128	50.00	3669	69.05	2174	87.95	1051
37.05	824	51.00	1225	72.95	996	91.95	631
38.00	895	55.95	494	74.00	4014	93.00	981
38.95	425	56.95	717	75.00	10235	94.00	2821
39.90	21	59.90	70	76.05	792	95.05	20045
43.90	104	60.95	874	76.90	57	96.05	1366
44.10	99	62.00	1240	78.95	863	103.90	107
44.85	167	63.05	949	79.95	253	116.90	116
46.90	290	64.00	200	80.95	899	118.80	57
47.90	51	65.10	61	81.85	236	119.00	54
49.00	845	68.00	2224	86.95	911	127.90	61

Average of 12.847 to 12.859 min.: VN075551.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
140.90	269						
142.95	357						
171.60	76						
172.05	230						
173.00	160						
174.00	16231						
174.95	1390						
176.00	16231						
177.00	1032						