
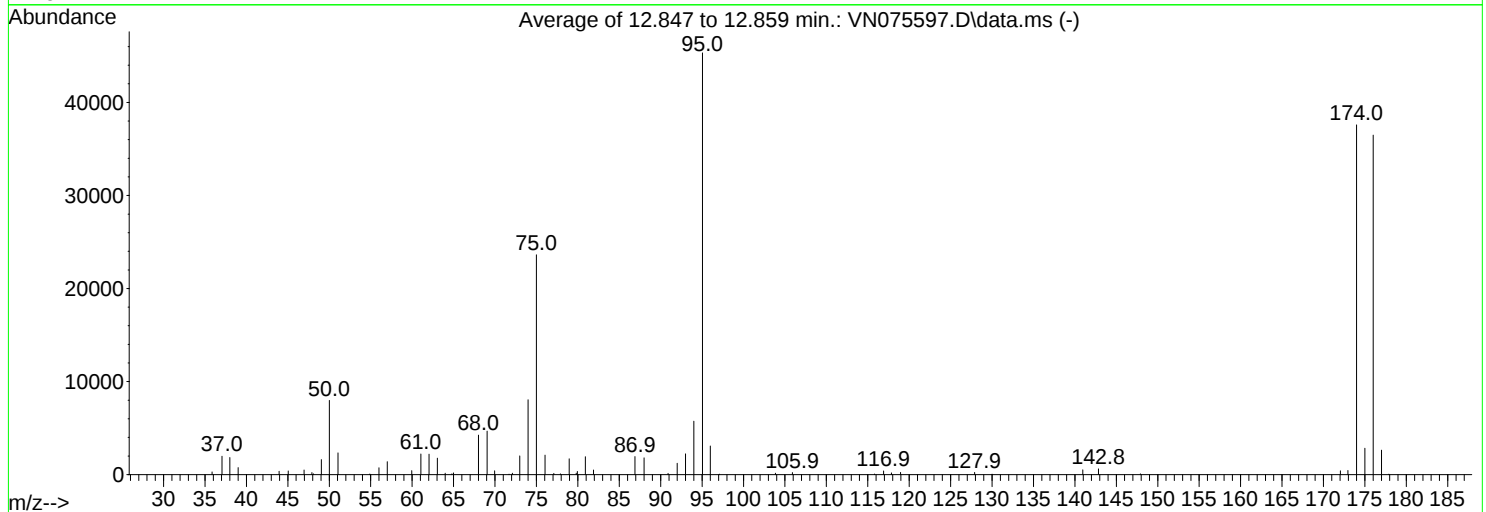


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN120722\
 Data File : VN075597.D
 Acq On : 07 Dec 2022 09:25
 Operator : JC\MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N112122W.M
 Title : SW846 8260
 Last Update : Wed Nov 23 00:18:03 2022

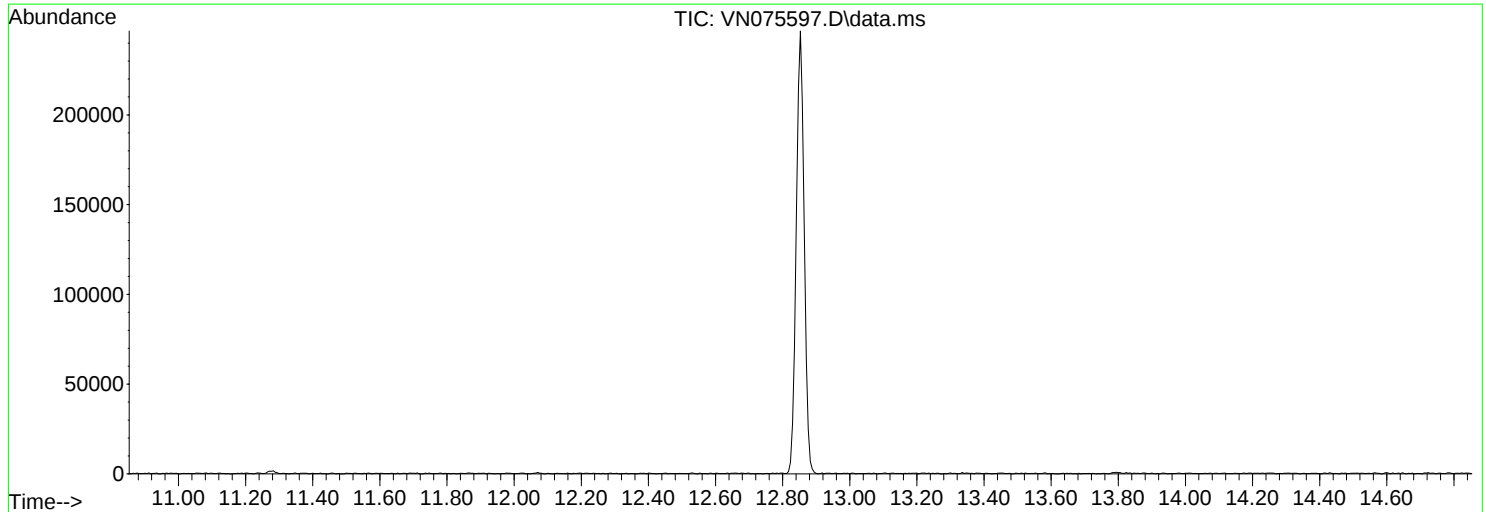

AutoFind: Scans 1835, 1836, 1837; Background Corrected with Scan 1827

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.6	7974	PASS
75	95	30	60	52.1	23635	PASS
95	95	100	100	100.0	45328	PASS
96	95	5	9	6.8	3076	PASS
173	174	0.00	2	1.2	446	PASS
174	95	50	100	82.9	37597	PASS
175	174	5	9	7.5	2834	PASS
176	174	95	101	97.1	36493	PASS
177	176	5	9	7.2	2637	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.85	297	51.05	2340	68.00	4247	78.95	1691
37.05	1976	54.90	67	69.05	4687	79.80	151
38.00	1849	56.00	733	69.95	408	79.95	33
39.00	762	57.00	1393	71.70	55	80.90	192
43.95	371	59.95	433	72.10	153	81.90	494
45.05	393	61.05	2216	73.00	2008	86.90	1948
46.95	497	62.05	2209	74.00	8045	88.00	1810
47.90	232	63.05	1777	75.00	23635	90.90	138
48.10	84	64.00	156	76.05	2106	92.00	1217
49.05	1615	64.80	80	77.10	136	93.00	2231
50.00	7974	65.00	185	77.90	94	94.00	5738

Average of 12.847 to 12.859 min.: VN075597.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
95.05	45328	140.95	515				
96.00	3076	142.85	619				
97.10	60	147.90	84				
103.85	159	172.05	406				
105.90	216	172.95	446				
115.80	77	174.00	37597				
116.90	394	175.00	2834				
117.85	188	176.00	36493				
118.95	238	177.00	2637				
127.90	236	177.90	55				
130.00	50						

Instrument :

MSVOA_N

ClientSampleId :

BFB