


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN120722\
 Data File : VN075623.D
 Acq On : 07 Dec 2022 21:57
 Operator : JC\MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N112122W.M
 Title : SW846 8260
 Last Update : Wed Nov 23 00:18:03 2022

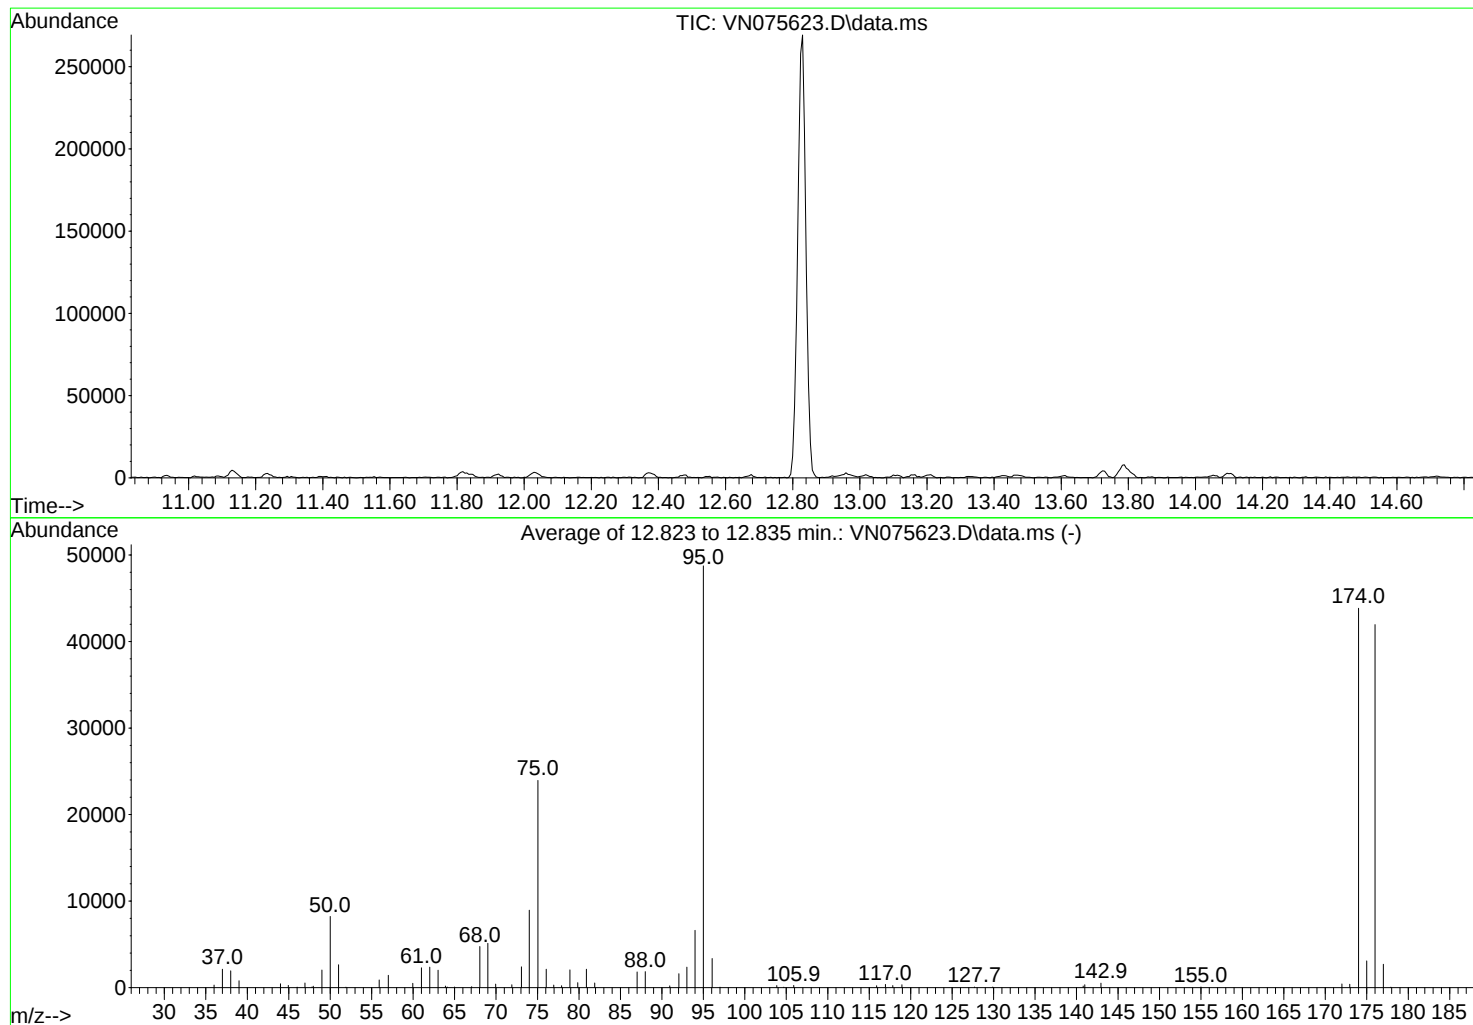

AutoFind: Scans 1831, 1832, 1833; Background Corrected with Scan 1822

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.9	8222	PASS
75	95	30	60	49.1	23955	PASS
95	95	100	100	100.0	48749	PASS
96	95	5	9	6.9	3361	PASS
173	174	0.00	2	0.9	397	PASS
174	95	50	100	89.9	43848	PASS
175	174	5	9	7.0	3087	PASS
176	174	95	101	95.7	41952	PASS
177	176	5	9	6.4	2692	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.00	288	50.00	8222	65.00	72	77.90	23
37.00	2132	51.00	2652	67.05	113	78.90	206
38.00	1951	51.90	59	68.05	4752	79.85	57
39.00	798	55.90	884	69.00	5122	80.90	212
44.00	437	57.00	1426	69.95	404	81.90	547
44.95	266	59.95	507	71.90	336	87.00	1813
46.00	53	61.00	2290	73.05	2410	88.00	1854
46.95	536	62.00	2366	74.00	8942	90.95	212
47.80	76	63.00	2014	75.05	23955	92.05	1611
47.95	158	63.90	180	76.05	2121	93.00	2375
49.00	2026	64.10	77	76.95	299	94.00	6615

Average of 12.823 to 12.835 min.: VN075623.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
95.00	48749	129.90	66	177.90	60		
96.05	3361	140.80	194				
97.00	57	141.00	330				
103.85	244	142.95	512				
104.70	50	155.00	68				
105.90	256	172.00	434				
115.90	227	172.95	397				
116.95	368	174.00	43848				
117.85	239	175.00	3087				
118.95	339	176.00	41952				
127.70	77	177.00	2692				

Instrument :

MSVOA_N

ClientSampleId :

BFB