

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN100722\
 Data File : VN074800.D
 Acq On : 07 Oct 2022 10:22
 Operator : JC\MD
 Sample : VN1007WBL01
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 VN1007WBL01

Quant Time: Oct 07 10:40:13 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N100522W.M
 Quant Title : SW846 8260
 QLast Update : Thu Oct 06 05:37:50 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.236	168	285500	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.112	114	541551	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.871	117	542721	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.794	152	250013	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.583	65	366771	54.219	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	=	108.440%
35) Dibromofluoromethane	8.177	113	295540	54.014	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	108.020%
50) Toluene-d8	10.571	98	1187749	50.590	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	=	101.180%
62) 4-Bromofluorobenzene	12.853	95	296260	41.511	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	83.020%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN100722\
Data File : VN074800.D
Acq On : 07 Oct 2022 10:22
Operator : JC\MD
Sample : VN1007WBL01
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
VN1007WBL01

Quant Time: Oct 07 10:40:13 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N100522W.M
Quant Title : SW846 8260
QLast Update : Thu Oct 06 05:37:50 2022
Response via : Initial Calibration




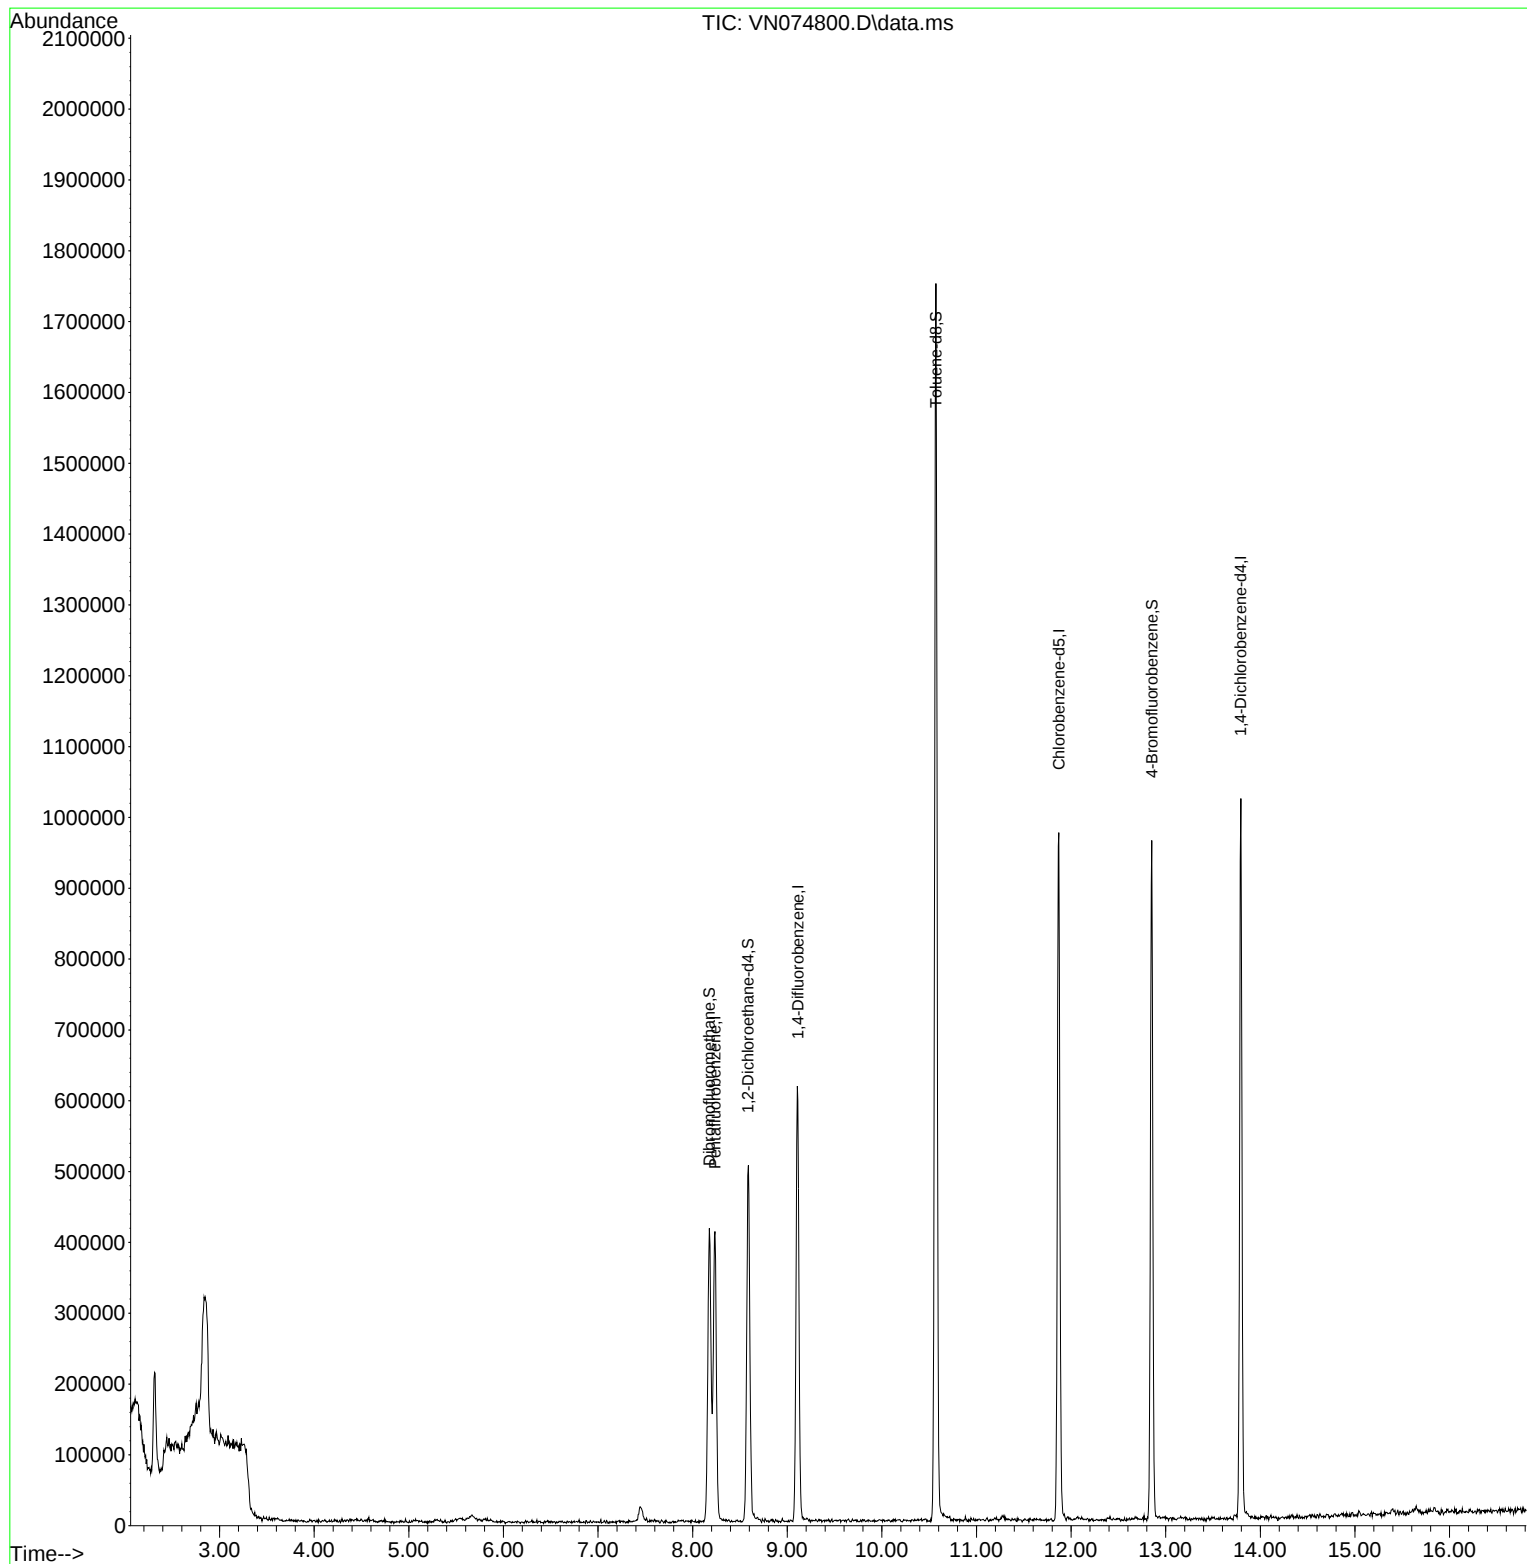


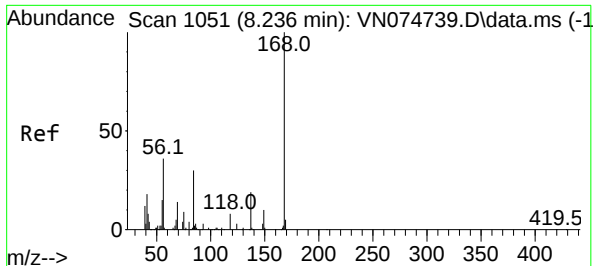

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.236 min Scan# 1105
Delta R.T. -0.001 min
Lab File: VN074800.D
Acq: 07 Oct 2022 10:22




Instrument :
MSVOA_N
ClientSampleId :
VN1007WBL01


Tgt Ion:168 Resp: 285500
Ion Ratio Lower Upper
168 100
99 55.1 42.8 64.2

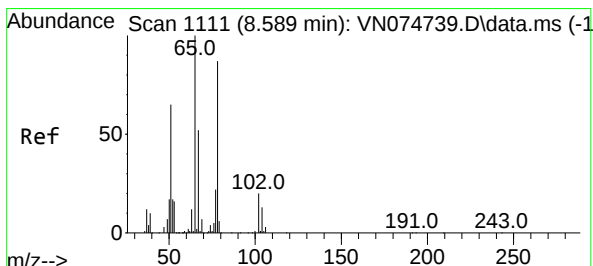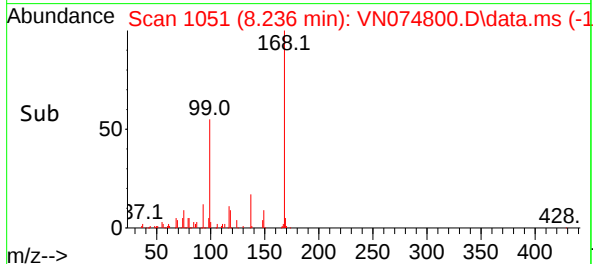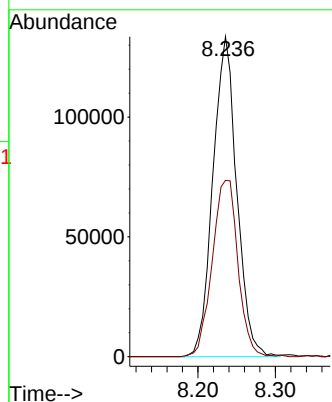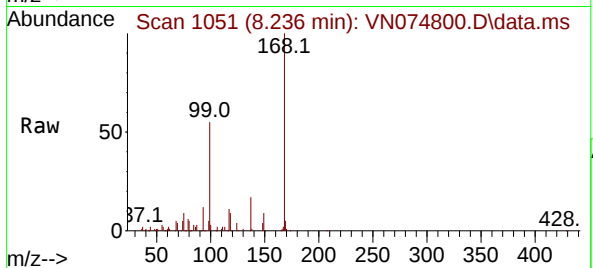

#33
1,2-Dichloroethane-d4
Concen: 54.219 ug/l
RT: 8.583 min Scan# 1110
Delta R.T. -0.006 min
Lab File: VN074800.D
Acq: 07 Oct 2022 10:22

Tgt Ion: 65 Resp: 366771
Ion Ratio Lower Upper
65 100
67 55.9 0.0 109.0

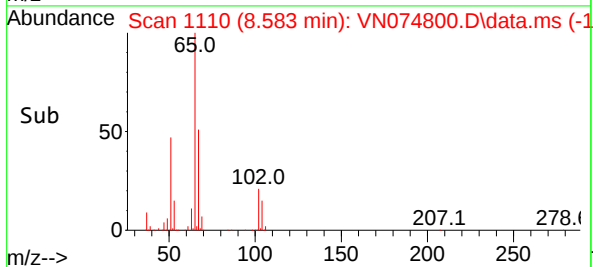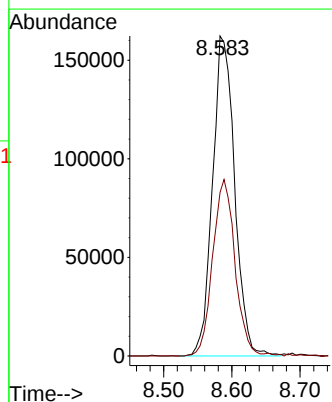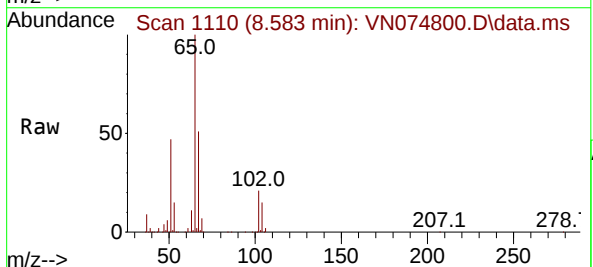

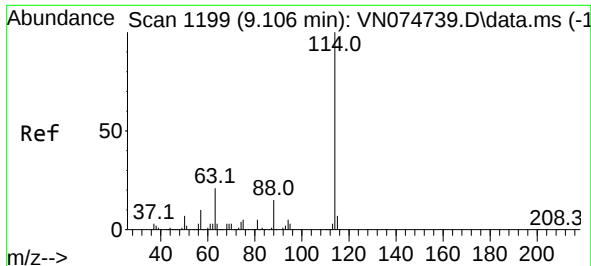

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 9.112 min Scan# 1199

Delta R.T. 0.006 min

Lab File: VN074800.D

Acq: 07 Oct 2022 10:22

Instrument :

MSVOA_N

ClientSampleId :

VN1007WBL01





Tgt Ion:114 Resp: 541551

Ion Ratio Lower Upper

114 100

63 19.1 0.0 41.2

88 13.7 0.0 30.2

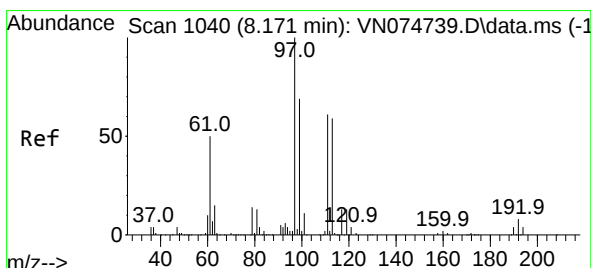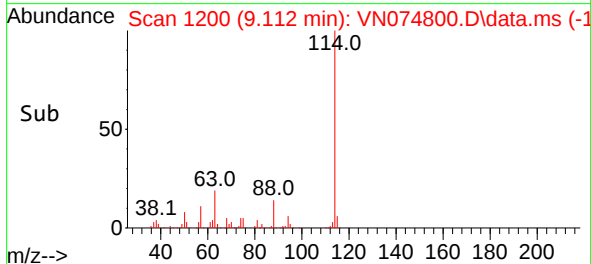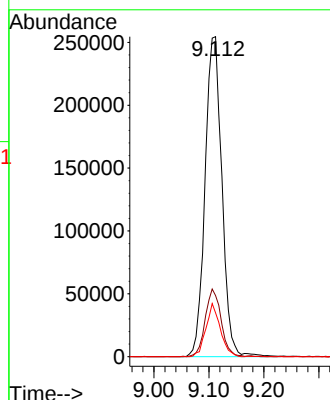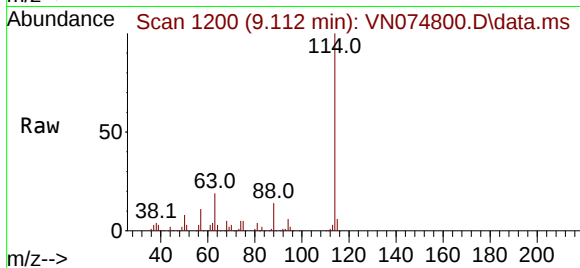

#35

Dibromofluoromethane

Concen: 54.014 ug/l

RT: 8.177 min Scan# 1041

Delta R.T. 0.006 min

Lab File: VN074800.D

Acq: 07 Oct 2022 10:22




Tgt Ion:113 Resp: 295540


Ion Ratio Lower Upper

113 100

111 102.7 83.0 124.6

192 15.6 12.6 18.8


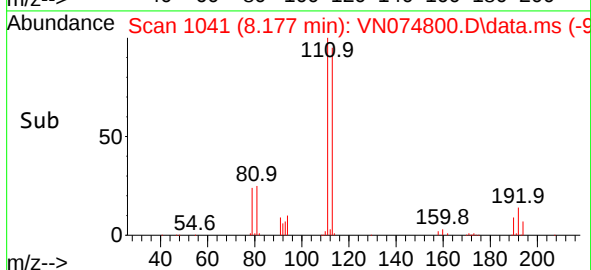
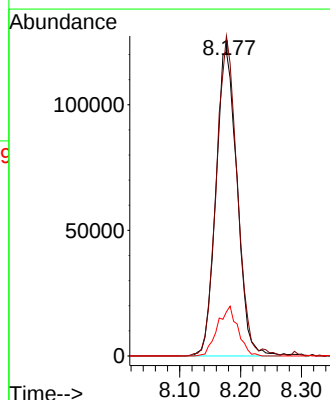
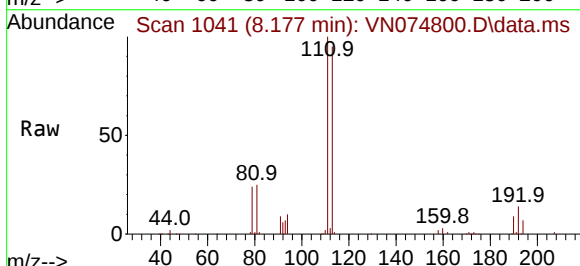


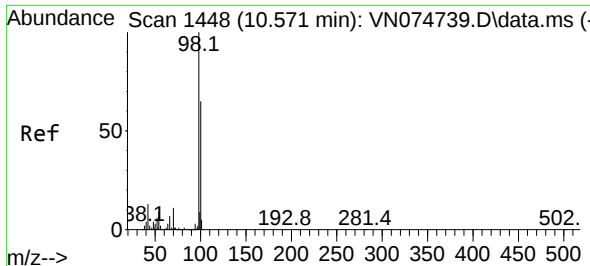

#50
Toluene-d8
Concen: 50.590 ug/l
RT: 10.571 min Scan# 1448
Delta R.T. -0.000 min
Lab File: VN074800.D
Acq: 07 Oct 2022 10:22




Instrument :
MSVOA_N
ClientSampleId :
VN1007WBL01


Tgt Ion: 98 Resp: 1187749
Ion Ratio Lower Upper
98 100
100 63.7 50.7 76.1

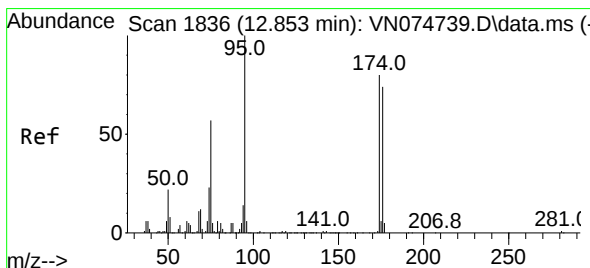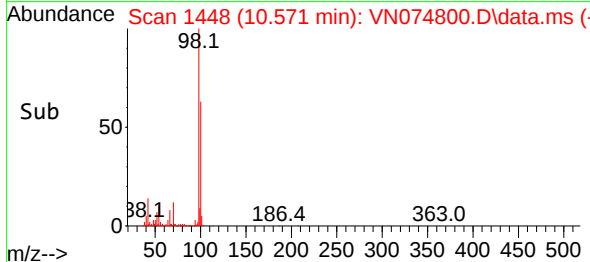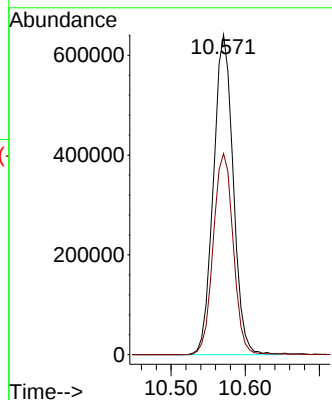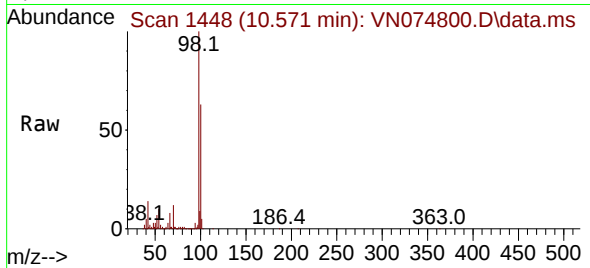

#62
4-Bromofluorobenzene
Concen: 41.511 ug/l
RT: 12.853 min Scan# 1836
Delta R.T. -0.000 min
Lab File: VN074800.D
Acq: 07 Oct 2022 10:22

Tgt Ion: 95 Resp: 296260
Ion Ratio Lower Upper
95 100
174 79.6 0.0 149.4
176 74.9 0.0 142.0


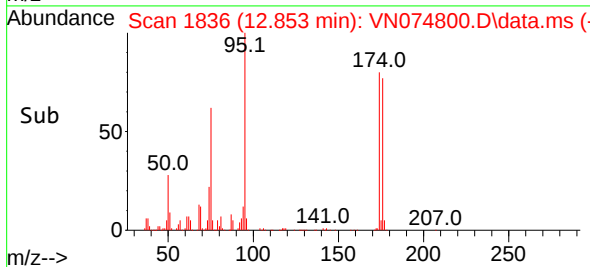
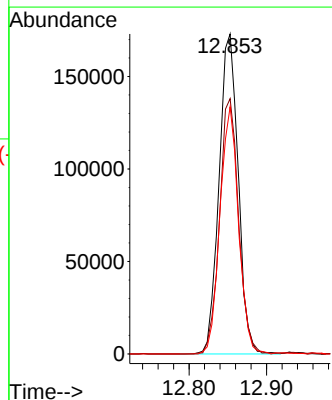
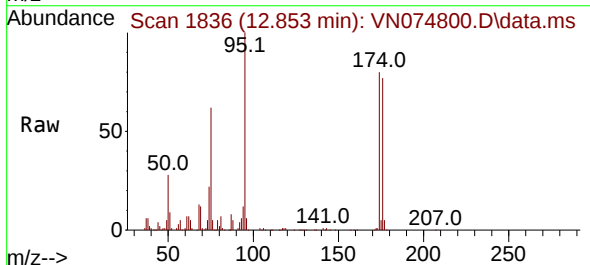


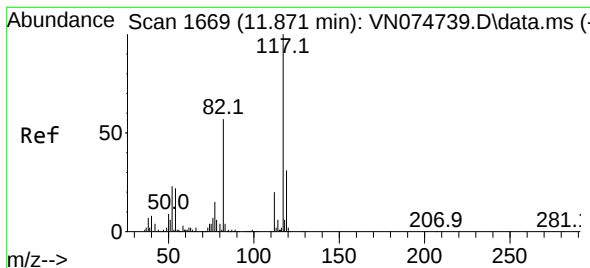

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.871 min Scan# 117
Delta R.T. -0.000 min
Lab File: VN074800.D
Acq: 07 Oct 2022 10:22

Instrument :
MSVOA_N
ClientSampleId :
VN1007WBL01

Tgt Ion:117 Resp: 542721
Ion Ratio Lower Upper
117 100
82 64.0 45.4 68.2
119 30.9 25.1 37.7

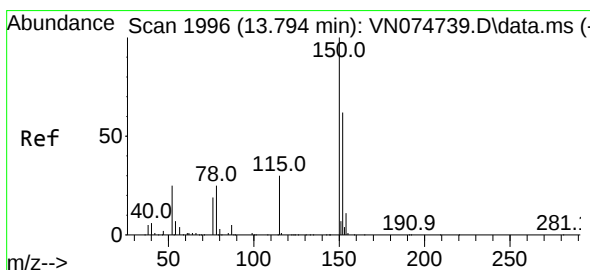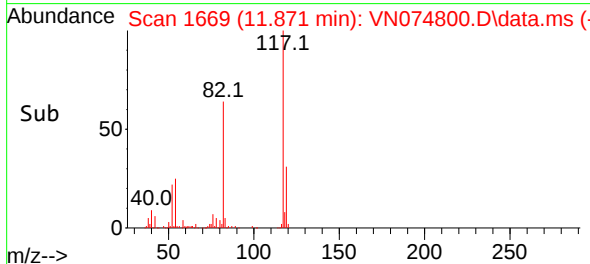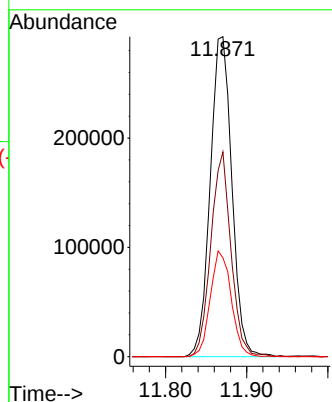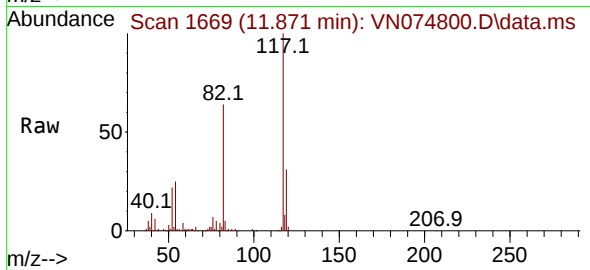

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.794 min Scan# 1996
Delta R.T. -0.000 min
Lab File: VN074800.D
Acq: 07 Oct 2022 10:22

Tgt Ion:152 Resp: 250013
Ion Ratio Lower Upper
152 100
115 60.7 30.0 90.0
150 160.9 0.0 356.4

