

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN100722\
 Data File : VN074819.D
 Acq On : 07 Oct 2022 18:21
 Operator : JC\MD
 Sample : N5014-18
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 TRIP-BLANK-1

Quant Time: Oct 08 03:55:23 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N100522W.M
 Quant Title : SW846 8260
 QLast Update : Thu Oct 06 05:37:50 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.236	168	239850	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.112	114	441590	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.871	117	451887	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.794	152	204447	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.588	65	344792	60.670	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	=	121.340%
35) Dibromofluoromethane	8.177	113	263239	59.001	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	118.000%
50) Toluene-d8	10.571	98	1062638	55.507	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	=	111.020%
62) 4-Bromofluorobenzene	12.853	95	271508	46.654	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	93.300%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN100722\
Data File : VN074819.D
Acq On : 07 Oct 2022 18:21
Operator : JC\MD
Sample : N5014-18
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
TRIP-BLANK-1

Quant Time: Oct 08 03:55:23 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N100522W.M
Quant Title : SW846 8260
QLast Update : Thu Oct 06 05:37:50 2022
Response via : Initial Calibration




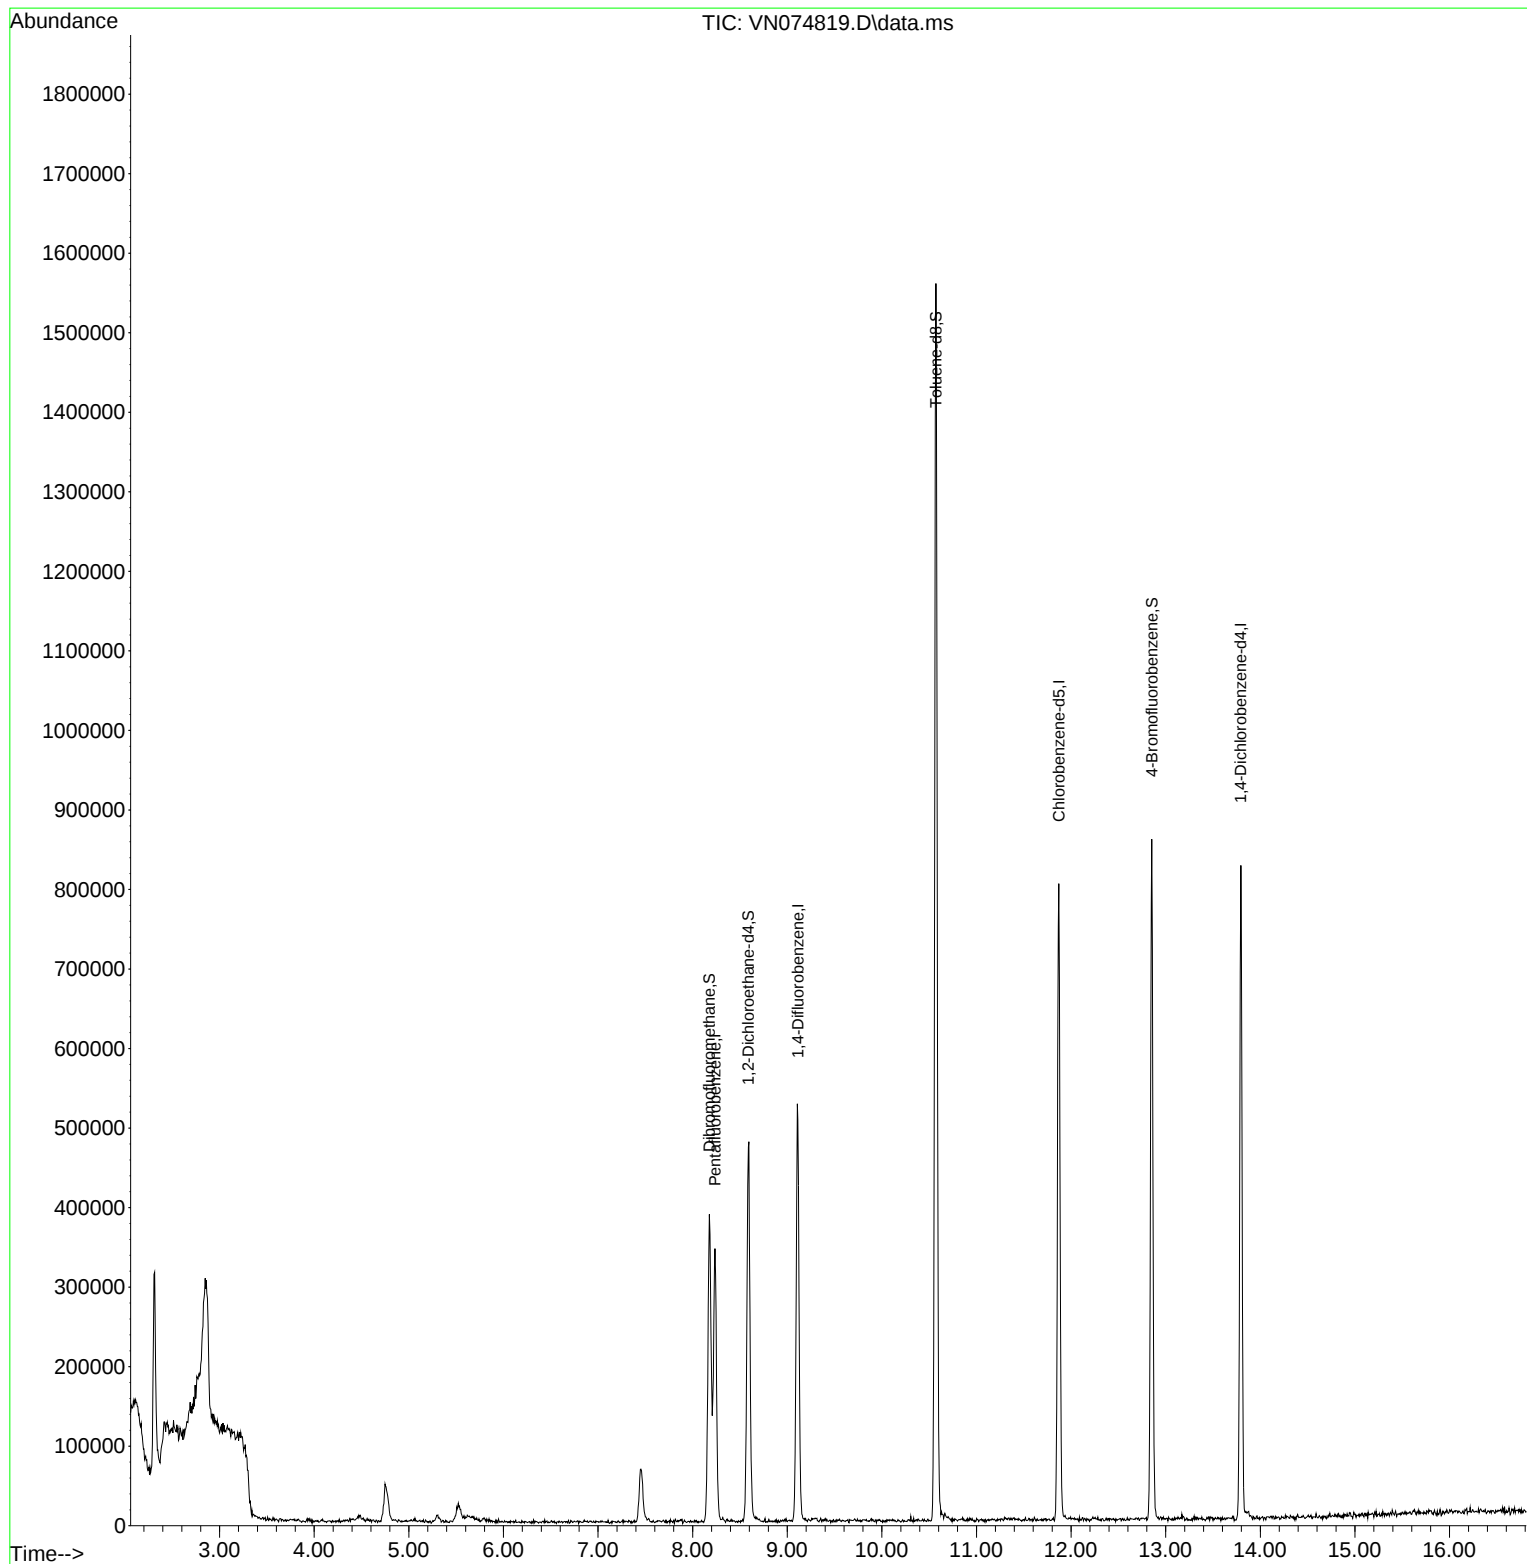


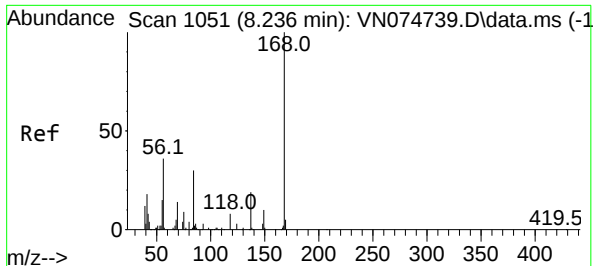

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.236 min Scan# 1051
Delta R.T. -0.000 min
Lab File: VN074819.D
Acq: 07 Oct 2022 18:21




Instrument :
MSVOA_N
ClientSampleId :
TRIP-BLANK-1


Tgt Ion:168 Resp: 239850
Ion Ratio Lower Upper
168 100
99 63.4 42.8 64.2

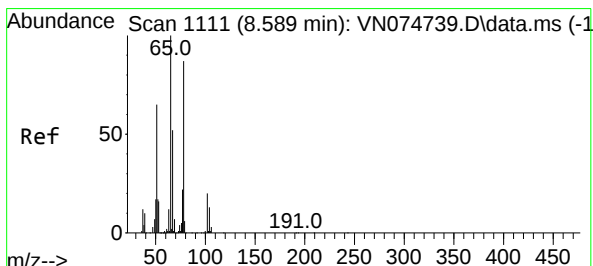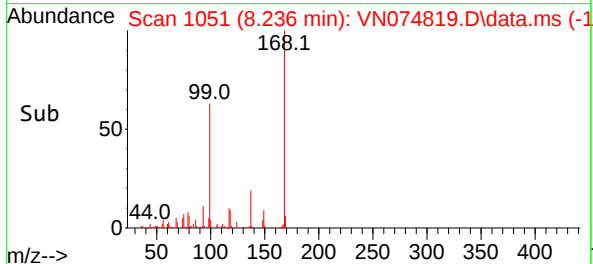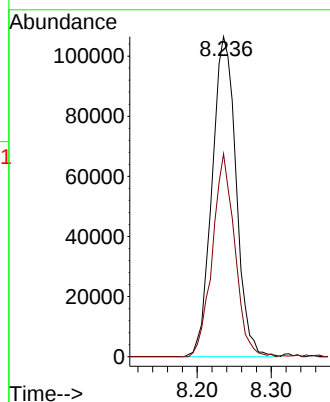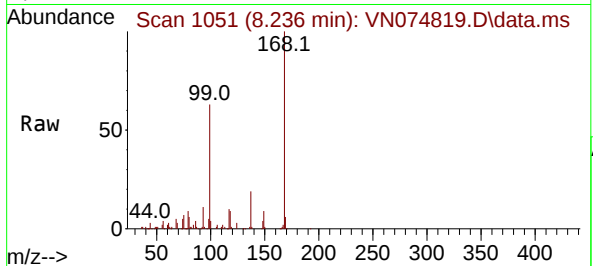

#33
1,2-Dichloroethane-d4
Concen: 60.670 ug/l
RT: 8.588 min Scan# 1111
Delta R.T. -0.000 min
Lab File: VN074819.D
Acq: 07 Oct 2022 18:21

Tgt Ion: 65 Resp: 344792
Ion Ratio Lower Upper
65 100
67 55.4 0.0 109.0

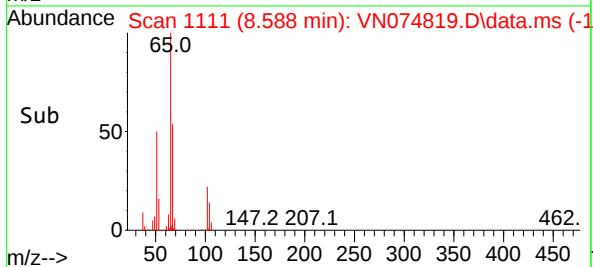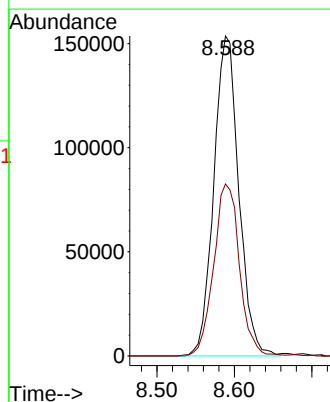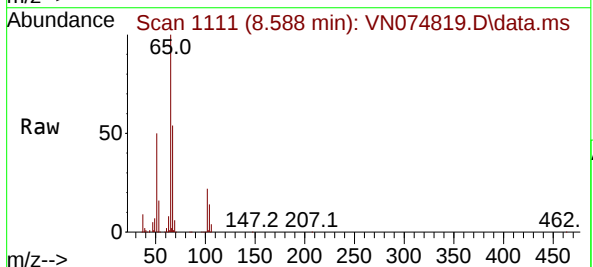

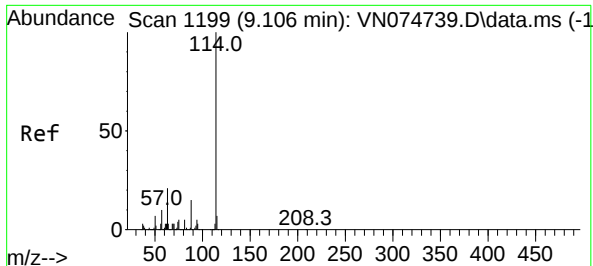

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 9.112 min Scan# 1199

Delta R.T. 0.006 min

Lab File: VN074819.D

Acq: 07 Oct 2022 18:21

Instrument :

MSVOA_N

ClientSampleId :

TRIP-BLANK-1





Tgt Ion:114 Resp: 441590

Ion Ratio Lower Upper

114 100

63 22.5 0.0 41.2

88 12.8 0.0 30.2

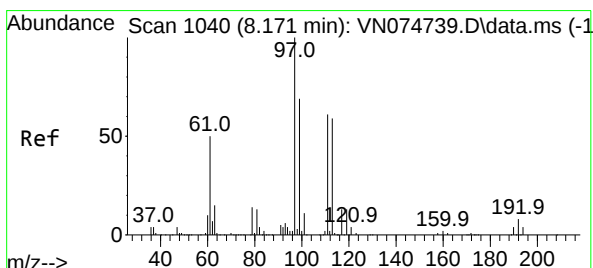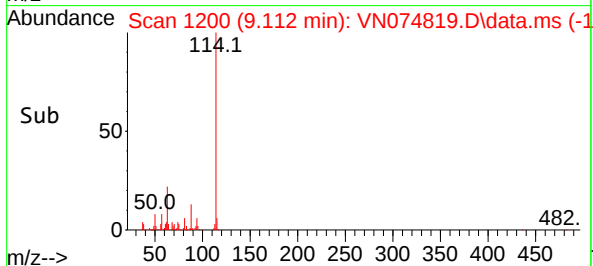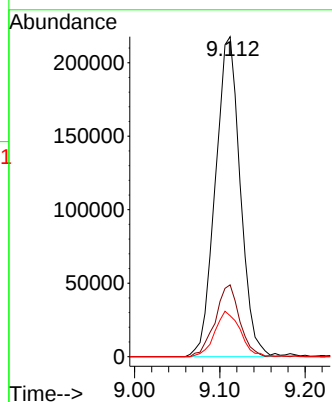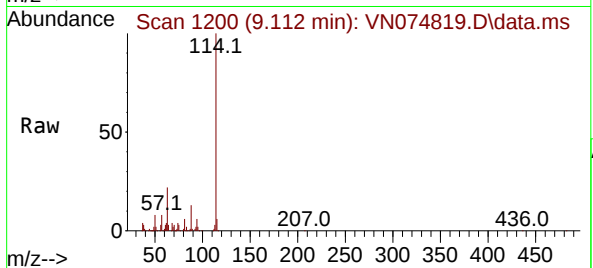

#35

Dibromofluoromethane

Concen: 59.001 ug/l

RT: 8.177 min Scan# 1041

Delta R.T. 0.006 min

Lab File: VN074819.D

Acq: 07 Oct 2022 18:21




Tgt Ion:113 Resp: 263239


Ion Ratio Lower Upper

113 100

111 106.5 83.0 124.6

192 16.6 12.6 18.8


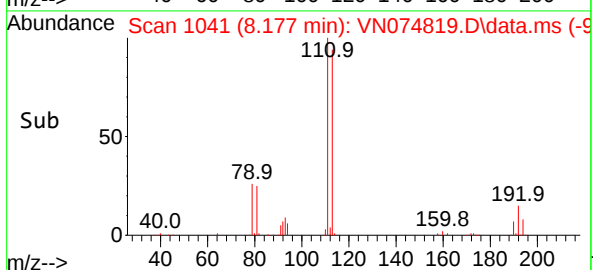
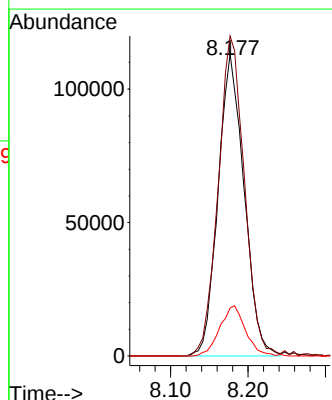
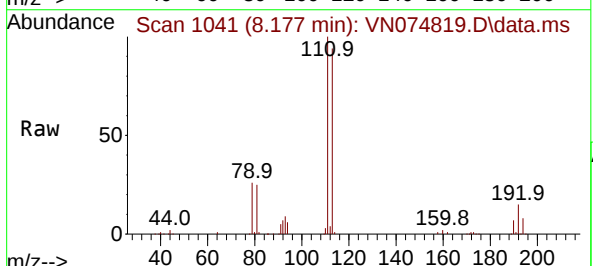


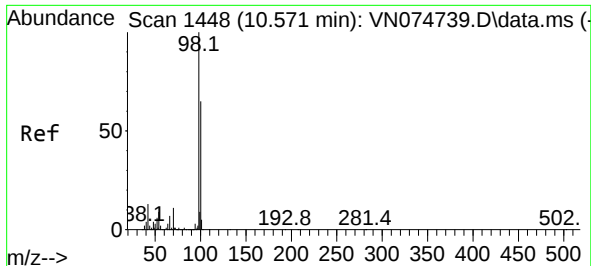

#50
Toluene-d8
Concen: 55.507 ug/l
RT: 10.571 min Scan# 1448
Delta R.T. -0.000 min
Lab File: VN074819.D
Acq: 07 Oct 2022 18:21




Instrument :
MSVOA_N
ClientSampleId :
TRIP-BLANK-1


Tgt Ion: 98 Resp: 1062638
Ion Ratio Lower Upper
98 100
100 64.2 50.7 76.1

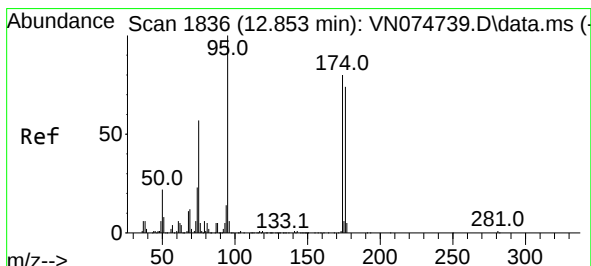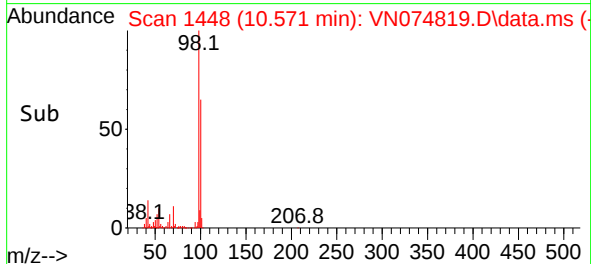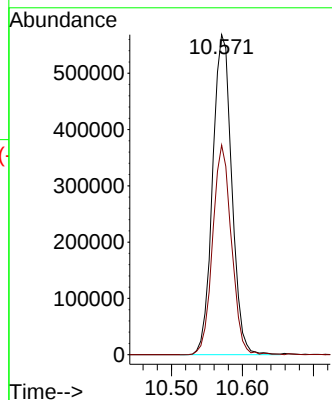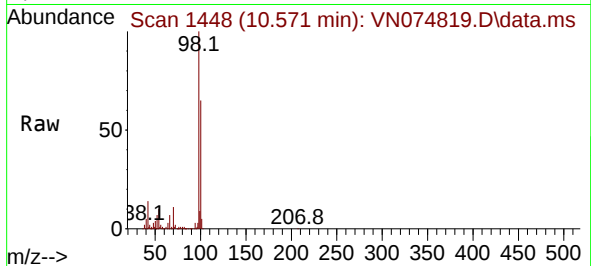

#62
4-Bromofluorobenzene
Concen: 46.654 ug/l
RT: 12.853 min Scan# 1836
Delta R.T. -0.000 min
Lab File: VN074819.D
Acq: 07 Oct 2022 18:21

Tgt Ion: 95 Resp: 271508
Ion Ratio Lower Upper
95 100
174 78.8 0.0 149.4
176 73.1 0.0 142.0


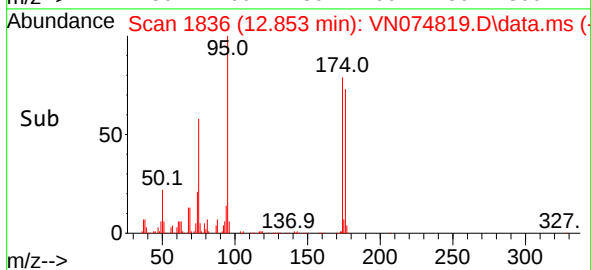
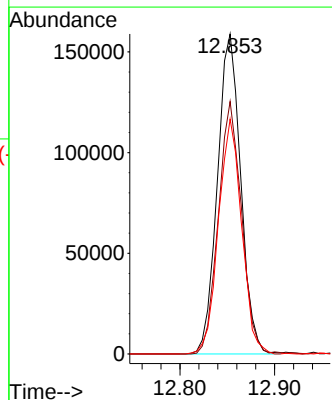
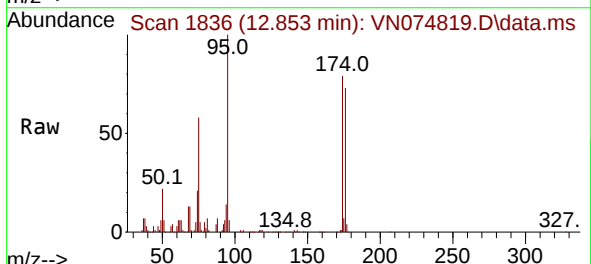


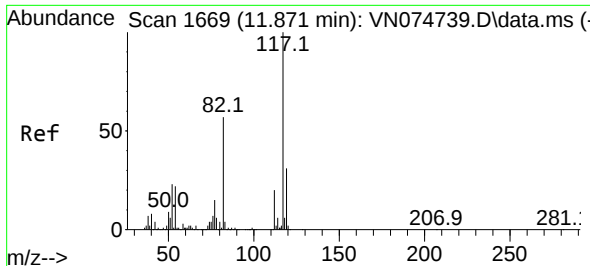

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.871 min Scan# 1669
Delta R.T. -0.000 min
Lab File: VN074819.D
Acq: 07 Oct 2022 18:21

Instrument :
MSVOA_N
ClientSampleId :
TRIP-BLANK-1

Tgt Ion:117 Resp: 451887
Ion Ratio Lower Upper
117 100
82 57.5 45.4 68.2
119 30.9 25.1 37.7

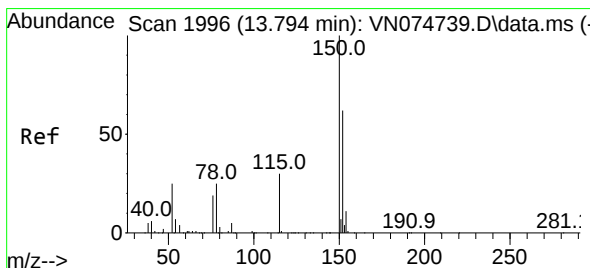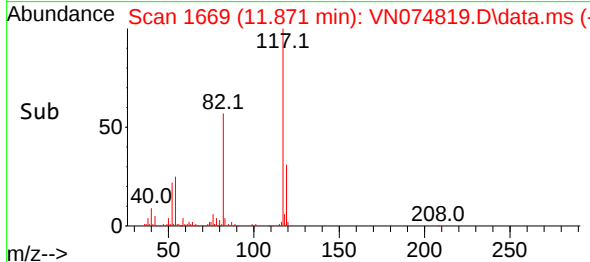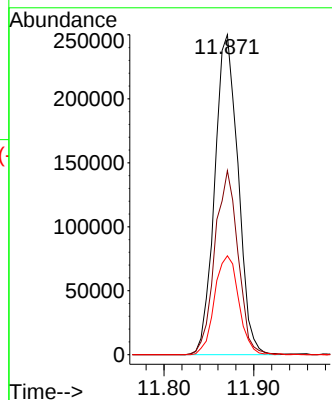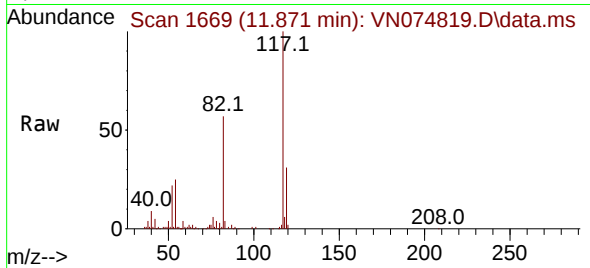

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.794 min Scan# 1996
Delta R.T. -0.000 min
Lab File: VN074819.D
Acq: 07 Oct 2022 18:21

Tgt Ion:152 Resp: 204447
Ion Ratio Lower Upper
152 100
115 59.7 30.0 90.0
150 159.4 0.0 356.4

