
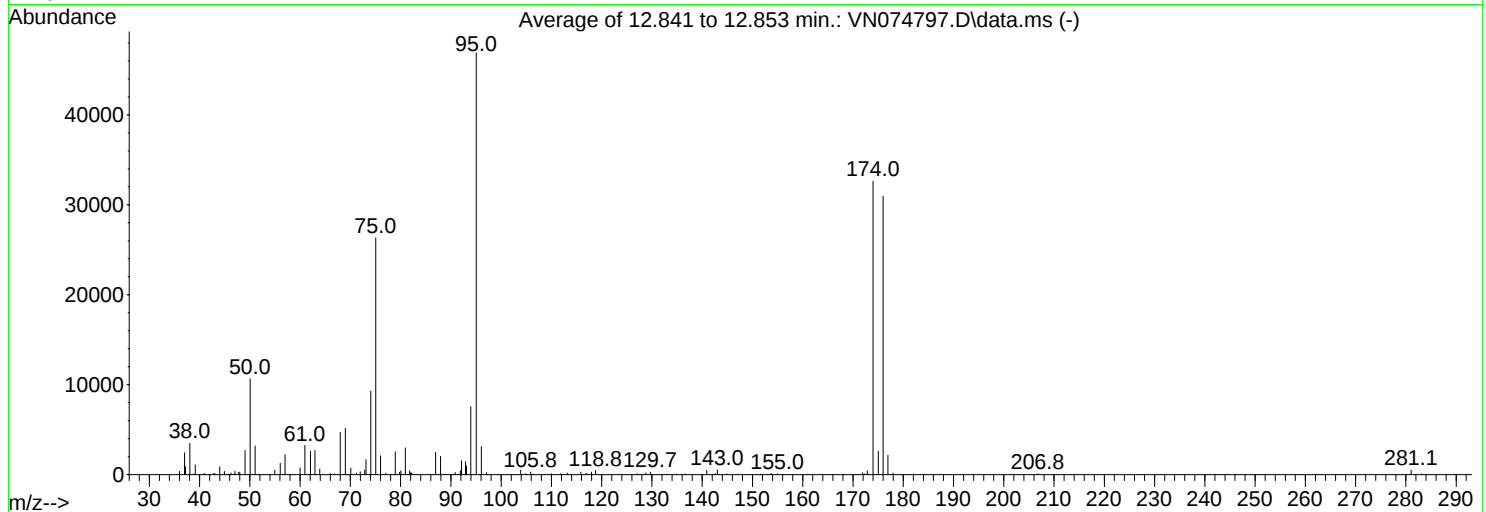


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN100722\
Data File : VN074797.D
Acq On : 07 Oct 2022 08:12
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N100522W.M
Title : SW846 8260
Last Update : Thu Oct 06 05:37:50 2022

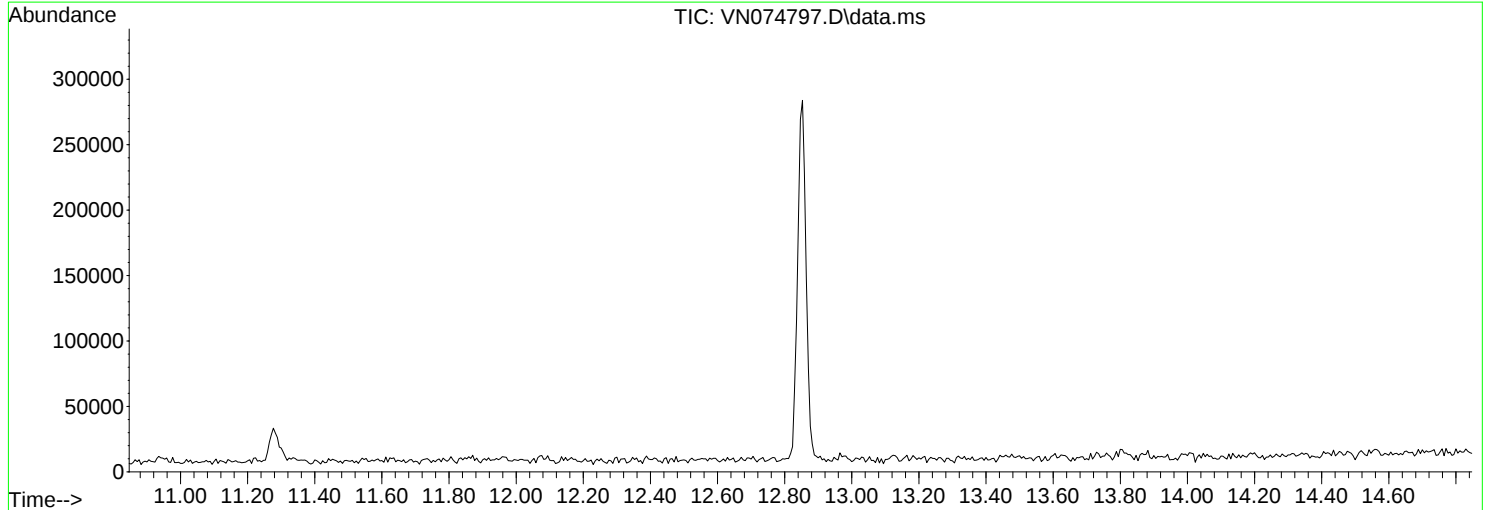

AutoFind: Scans 1834, 1835, 1836; Background Corrected with Scan 1827

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.7	10661	PASS
75	95	30	60	56.1	26331	PASS
95	95	100	100	100.0	46901	PASS
96	95	5	9	6.7	3121	PASS
173	174	0.00	2	1.3	410	PASS
174	95	50	100	69.6	32627	PASS
175	174	5	9	8.0	2595	PASS
176	174	95	101	94.9	30971	PASS
177	176	5	9	6.9	2147	PASS