


Data Path : W:\HPCHEM1\MSVOA_N\DATA\VN010518\
Data File : VN046326.D
Acq On : 5 Jan 2018 9:45
Operator : MD\SY
Sample : BFB
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT3.P

Method : W:\HPCHEM1\MSVOA_N\METHODS\624N121917W.M
Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
Last Update : Tue Dec 19 04:09:09 2017

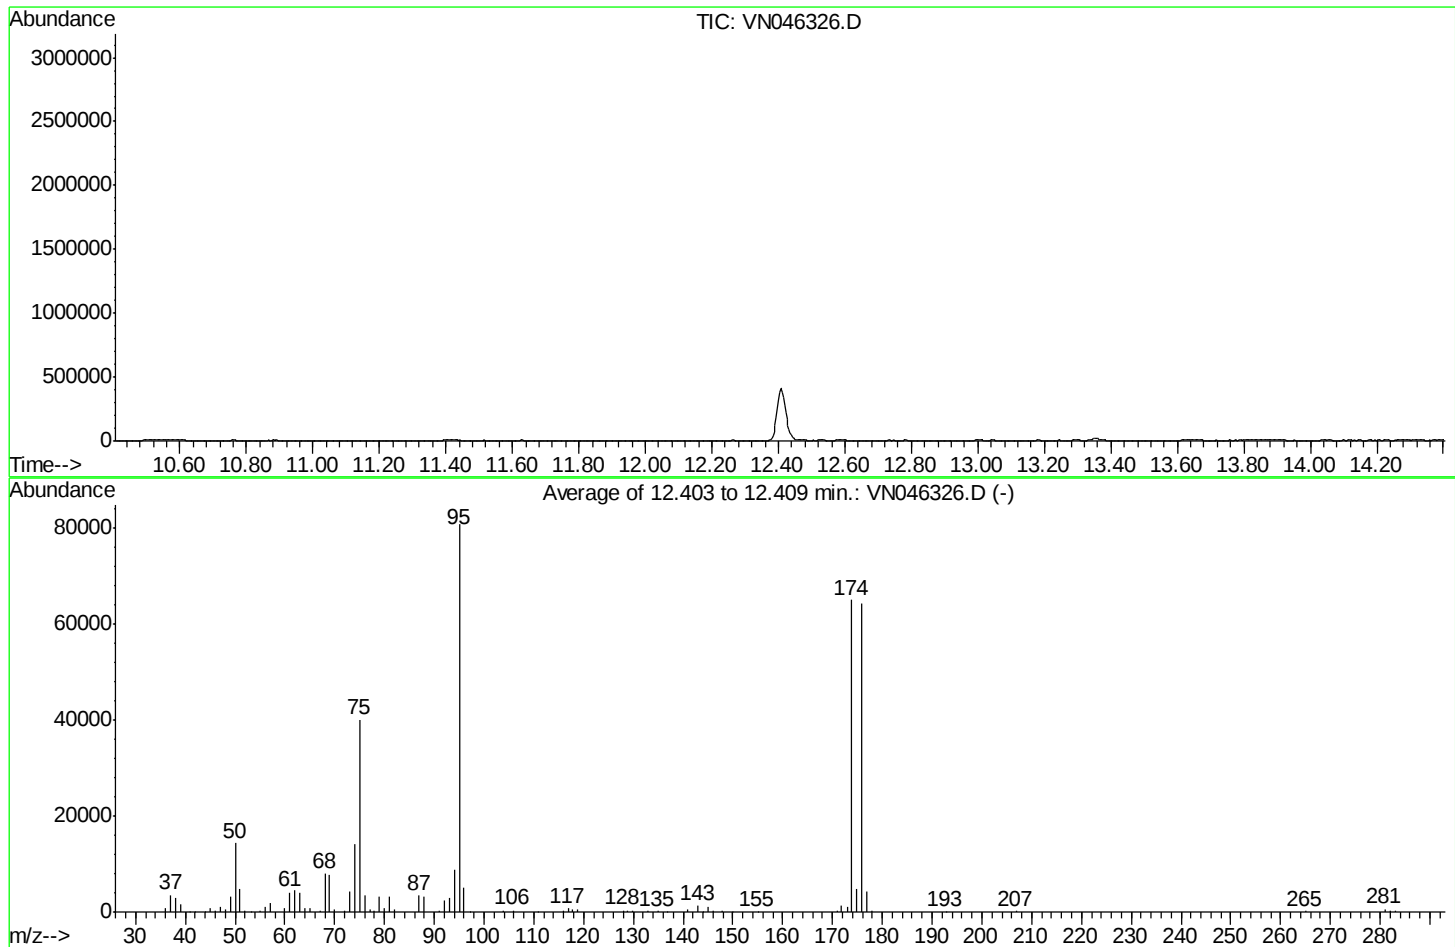

AutoFind: Scans 3363, 3364, 3365; Background Corrected with Scan 3350

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.8	14346	PASS
75	95	30	60	49.6	40082	PASS
95	95	100	100	100.0	80818	PASS
96	95	5	9	6.1	4969	PASS
173	174	0.00	2	1.8	1160	PASS
174	95	50	100	80.5	65066	PASS
175	174	5	9	7.3	4729	PASS
176	174	95	101	98.7	64221	PASS
177	176	5	9	6.8	4362	PASS