

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN011023\
 Data File : VN076188.D
 Acq On : 10 Jan 2023 17:36
 Operator : JC\MD
 Sample : 01061-03
 Misc : 5.00gr/10mL/100uL/5.0mL/MSVOA_N/MeOH
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :

Quant Time: Jan 11 01:08:18 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N121422W.M
 Quant Title : SW846 8260
 QLast Update : Wed Dec 14 13:03:41 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.224	168	374513	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.100	114	581702	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.865	117	505726	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.794	152	234743	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.582	65	192871	47.338	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	=	94.680%
35) Dibromofluoromethane	8.171	113	164564	45.682	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	91.360%
50) Toluene-d8	10.565	98	681437	50.593	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	=	101.180%
62) 4-Bromofluorobenzene	12.853	95	220105	49.339	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	98.680%


Target Compounds				Qvalue		
6) Chloroethane	3.083	64	2219	0.760	ug/l #	68
11) Tert butyl alcohol	5.506	59	4869	8.446	ug/l #	72
16) Acetone	4.465	43	9100	6.479	ug/l #	85
18) Methyl Acetate	5.059	43	1443	0.348	ug/l #	54
20) Methylene Chloride	5.271	84	11756	2.521	ug/l	91
25) 2-Butanone	7.500	43	1957	0.995	ug/l	95
31) Cyclohexane	8.224	56	8695	1.490	ug/l #	17
36) 1,1-Dichloropropene	8.224	75	26813	5.603	ug/l #	50
38) Carbon Tetrachloride	8.224	117	37302	6.965	ug/l #	17
39) Methylcyclohexane	9.594	83	2709	0.469	ug/l	94
48) Methyl methacrylate	9.647	41	1059	0.371	ug/l #	22
51) 4-Methyl-2-Pentanone	10.453	43	1120	0.292	ug/l #	32
52) Toluene	10.629	92	6370	0.662	ug/l	88
55) 1,1,2-Trichloroethane	11.012	97	2393	0.634	ug/l #	27
59) 2-Hexanone	11.170	43	3282	1.174	ug/l #	20
67) Ethyl Benzene	11.965	91	10586	0.604	ug/l	97
68) m/p-Xylenes	12.070	106	18089	2.609	ug/l	99
69) o-Xylene	12.406	106	11297	1.646	ug/l	92
73) Isopropylbenzene	12.700	105	5626	0.332	ug/l	88
74) N-amyl acetate	12.482	43	5701	1.146	ug/l #	69
76) 1,2,3-Trichloropropane	12.853	75	112352	23.744	ug/l #	1
78) n-propylbenzene	13.035	91	5652	0.302	ug/l #	39
79) 2-Chlorotoluene	13.106	91	2361	0.202	ug/l #	40
80) 1,3,5-Trimethylbenzene	13.176	105	10342	0.728	ug/l	90
81) trans-1,4-Dichloro-2-b...	12.853	75	112352	85.466	ug/l #	12
82) 4-Chlorotoluene	13.106	91	2361	0.202	ug/l #	40
83) tert-Butylbenzene	13.488	119	4689	0.375	ug/l #	54
84) 1,2,4-Trimethylbenzene	13.488	105	35357	2.510	ug/l	99
85) sec-Butylbenzene	13.611	105	8226	0.476	ug/l	87
86) p-Isopropyltoluene	13.729	119	38738	2.695	ug/l #	78
90) Hexachloroethane	14.329	117	929	0.361	ug/l #	11
95) Naphthalene	15.641	128	9123	2.861	ug/l #	84


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN011023\
Data File : VN076188.D
Acq On : 10 Jan 2023 17:36
Operator : JC\MD
Sample : 01061-03
Misc : 5.00gr/10mL/100uL/5.0mL/MSVOA_N/MeOH
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :

Quant Time: Jan 11 01:08:18 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N121422W.M
Quant Title : SW846 8260
QLast Update : Wed Dec 14 13:03:41 2022
Response via : Initial Calibration




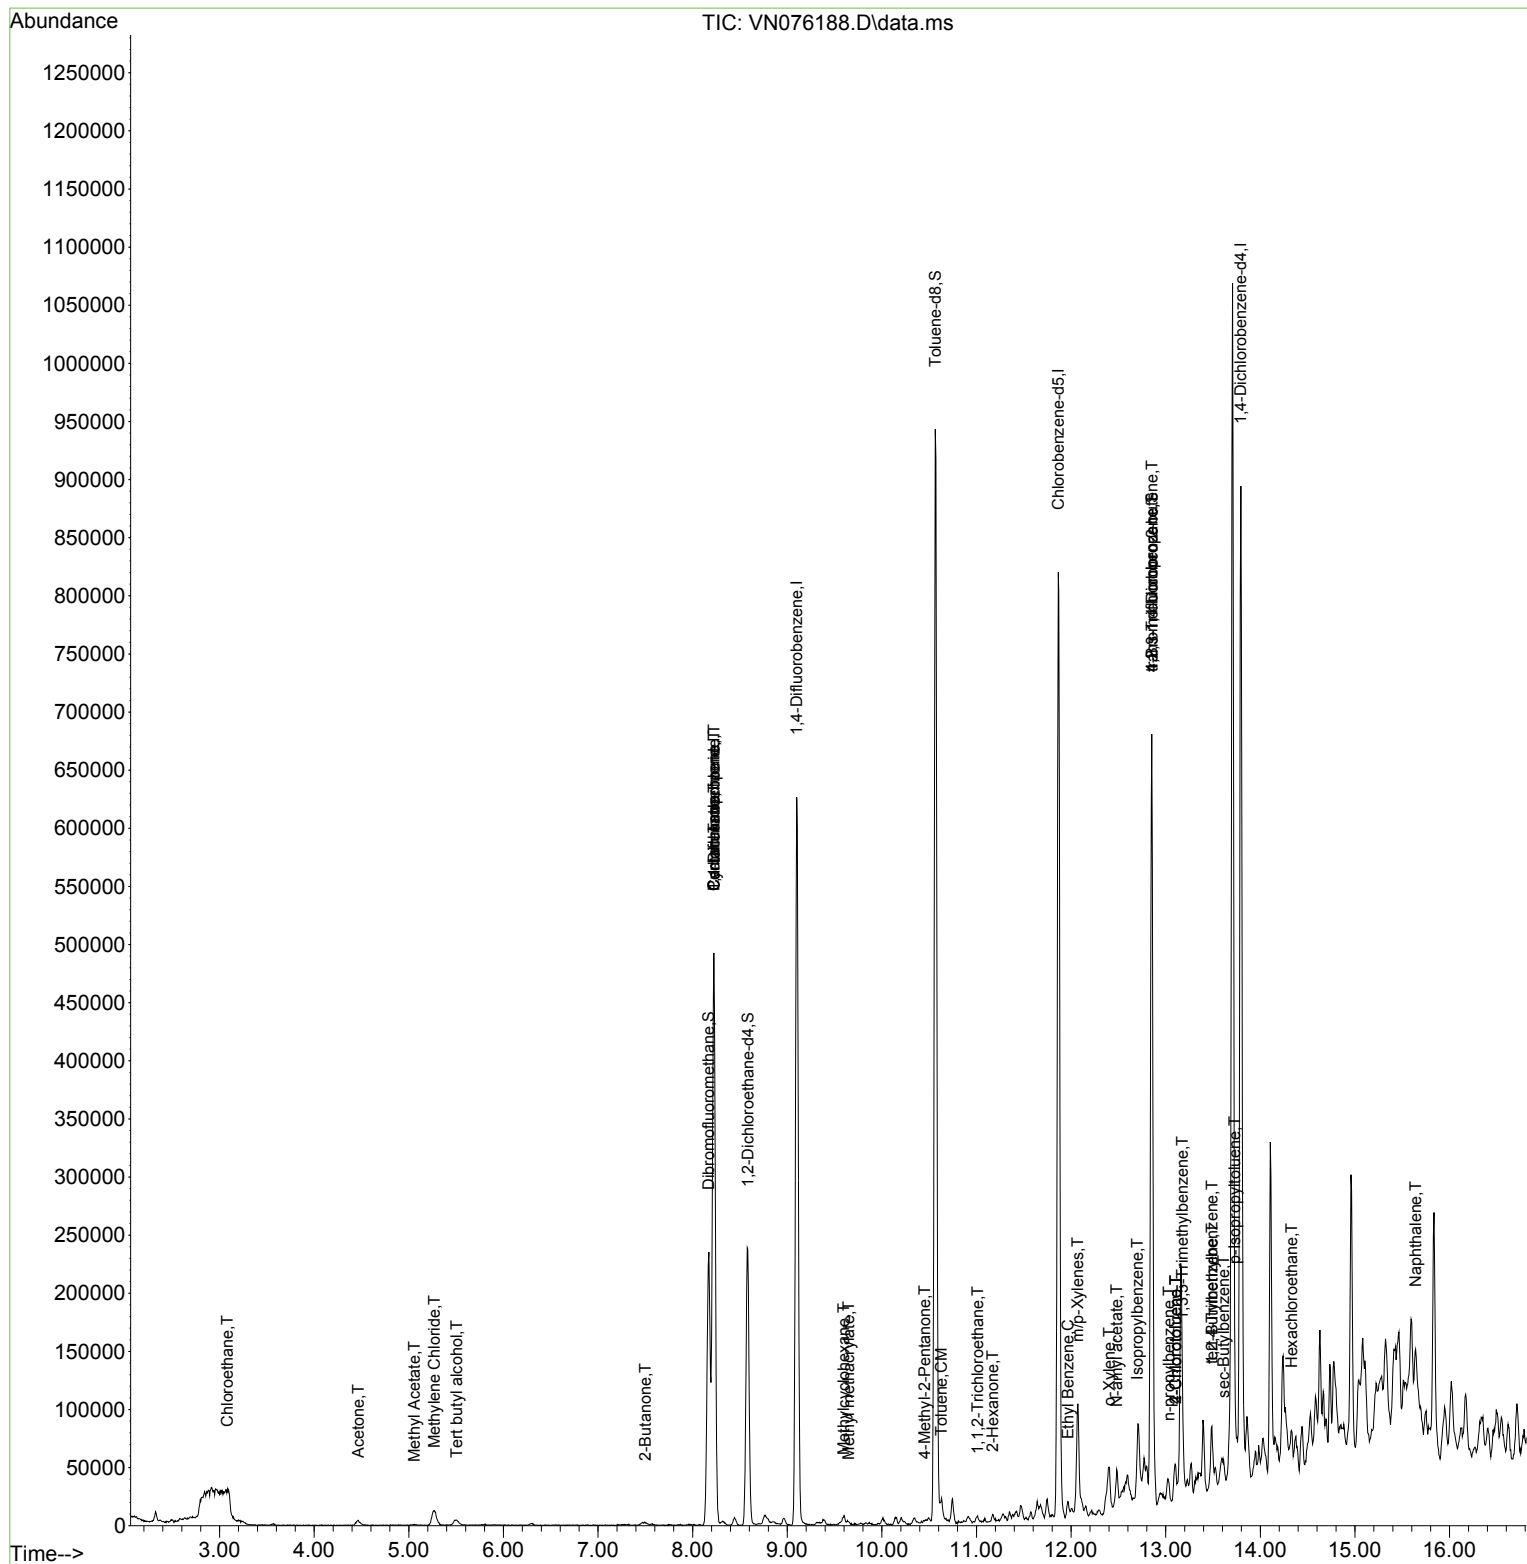




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.224 min Scan# 10
Delta R.T. -0.006 min
Lab File: VN076188.D
Acq: 10 Jan 2023 17:36




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion:168 Resp: 374513
Ion Ratio Lower Upper
168 100
99 53.1 44.2 66.4

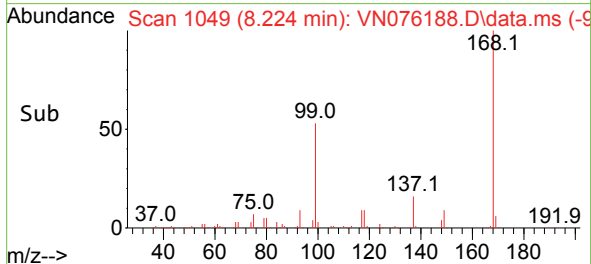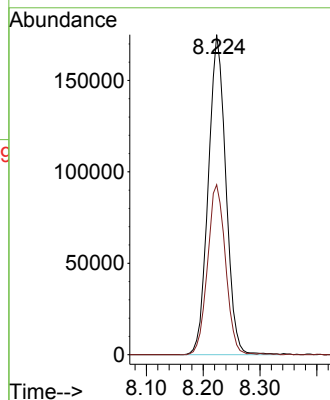

#6
Chloroethane
Concen: 0.760 ug/l
RT: 3.083 min Scan# 175
Delta R.T. -0.035 min
Lab File: VN076188.D
Acq: 10 Jan 2023 17:36


Tgt Ion: 64 Resp: 2219
Ion Ratio Lower Upper
64 100
66 13.4 24.6 36.8#

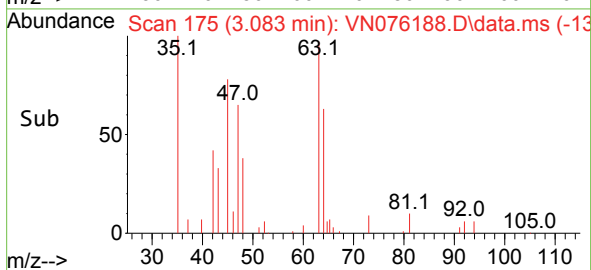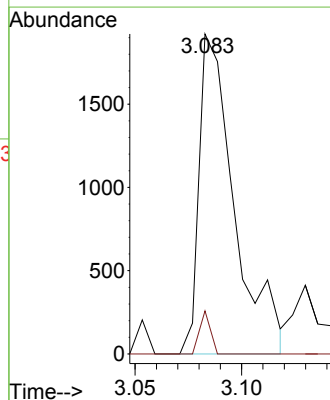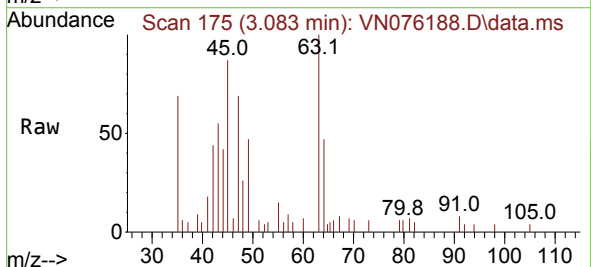






#11
Tert butyl alcohol
Concen: 8.446 ug/l
RT: 5.506 min Scan# 51
Delta R.T. -0.030 min
Lab File: VN076188.D
Acq: 10 Jan 2023 17:36


Instrument :
MSVOA_N
ClientSampleId :

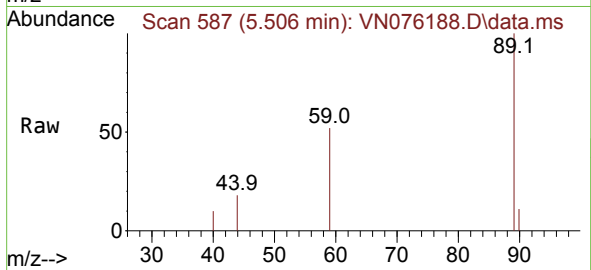



Tgt Ion: 59 Resp: 4869
Ion Ratio Lower Upper
59 100
57 0.0 8.2 12.4#

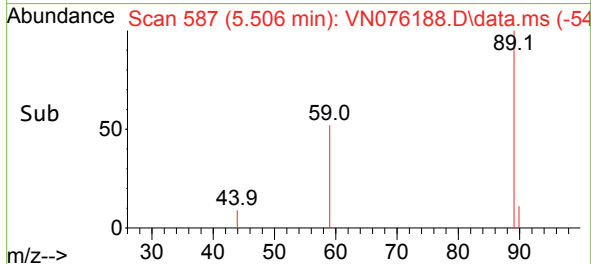


#16
Acetone
Concen: 6.479 ug/l
RT: 4.465 min Scan# 410
Delta R.T. 0.023 min
Lab File: VN076188.D
Acq: 10 Jan 2023 17:36

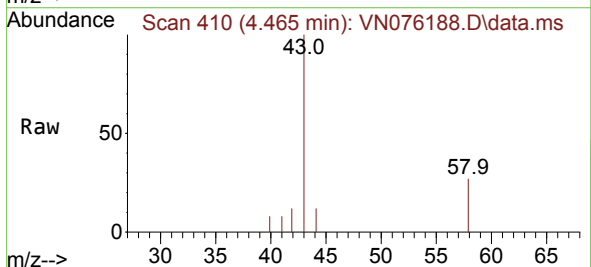

Tgt Ion: 43 Resp: 9100
Ion Ratio Lower Upper
43 100
58 27.0 28.6 43.0#



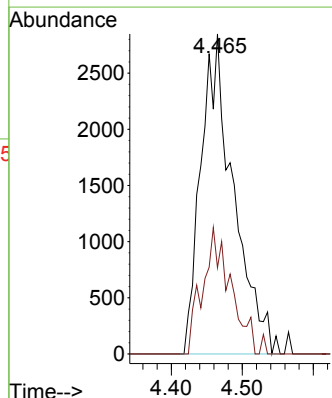





#18
Methyl Acetate
Concen: 0.348 ug/l
RT: 5.059 min Scan# 511
Delta R.T. 0.023 min
Lab File: VN076188.D
Acq: 10 Jan 2023 17:36




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 43 Resp: 1443
Ion Ratio Lower Upper
43 100
74 4.6 23.6 35.4#

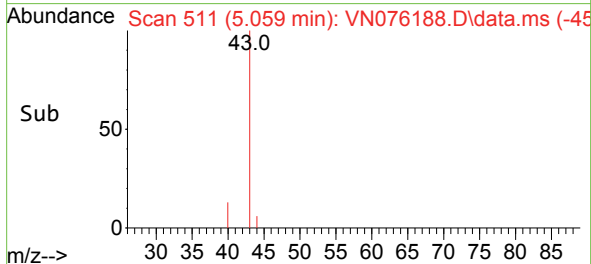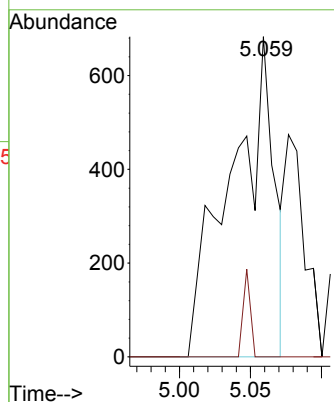

#20
Methylene Chloride
Concen: 2.521 ug/l
RT: 5.271 min Scan# 547
Delta R.T. -0.018 min
Lab File: VN076188.D
Acq: 10 Jan 2023 17:36

Tgt Ion: 84 Resp: 11756
Ion Ratio Lower Upper
84 100
49 111.7 81.8 122.6
51 36.9 26.7 40.1
86 72.9 51.5 77.3


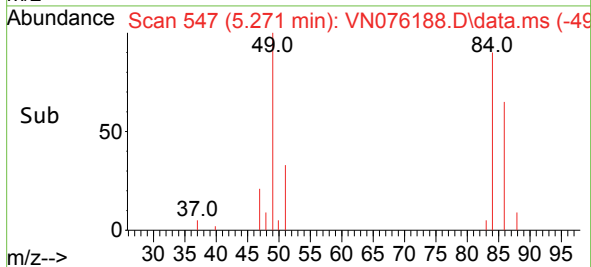
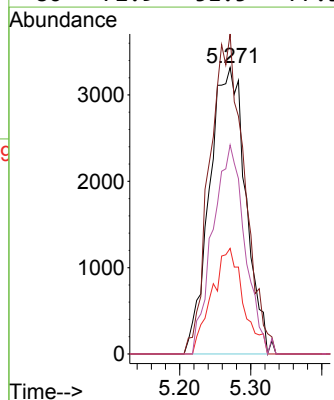
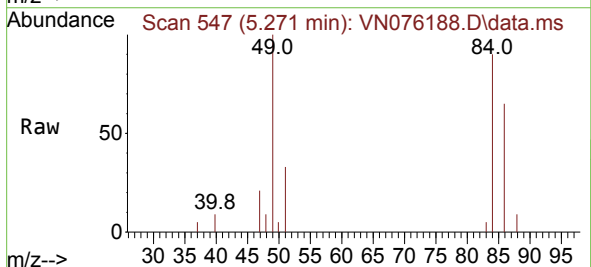




#25
2-Butanone
Concen: 0.995 ug/l
RT: 7.500 min Scan# 91
Delta R.T. 0.012 min
Lab File: VN076188.D
Acq: 10 Jan 2023 17:36




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 43 Resp: 1957
Ion Ratio Lower Upper
43 100
72 37.8 28.0 42.0

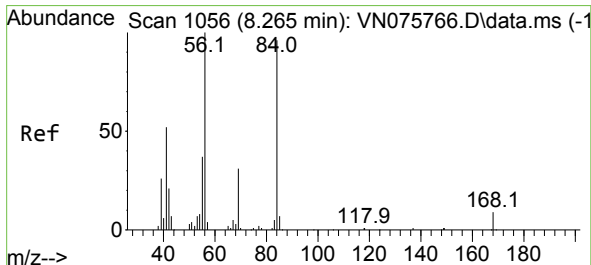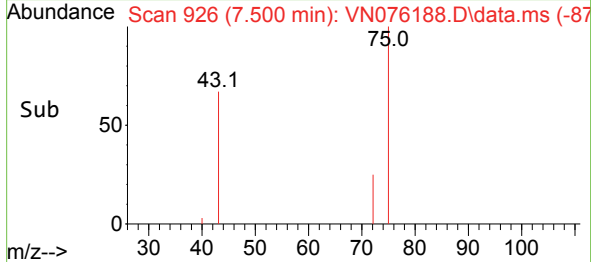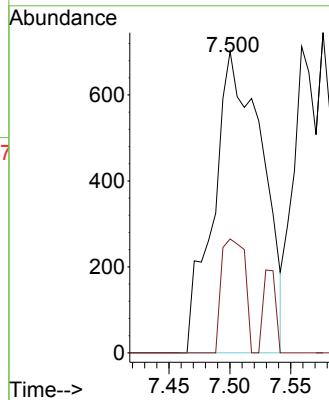

#31
Cyclohexane
Concen: 1.490 ug/l
RT: 8.224 min Scan# 1049
Delta R.T. -0.041 min
Lab File: VN076188.D
Acq: 10 Jan 2023 17:36

Tgt Ion: 56 Resp: 8695
Ion Ratio Lower Upper
56 100
69 168.6 24.7 37.1#
84 123.0 76.5 114.7#

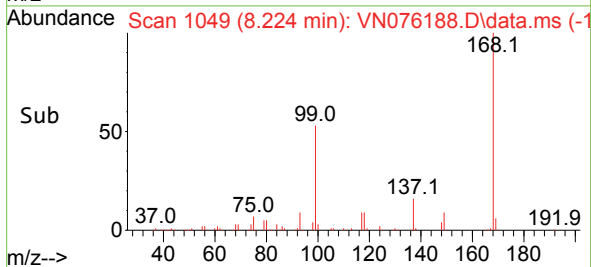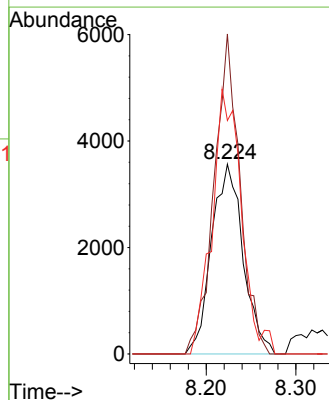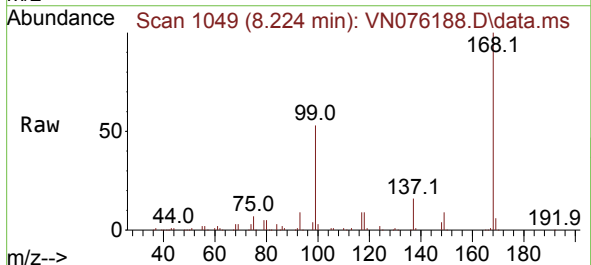



#33

1,2-Dichloroethane-d4

Concen: 47.338 ug/l

RT: 8.582 min Scan# 1110

Delta R.T. -0.000 min

Lab File: VN076188.D

Acq: 10 Jan 2023 17:36

Instrument :

MSVOA_N





ClientSampleId :

Tgt Ion: 65 Resp: 192871

Ion Ratio Lower Upper

65 100

67 52.7 0.0 103.4

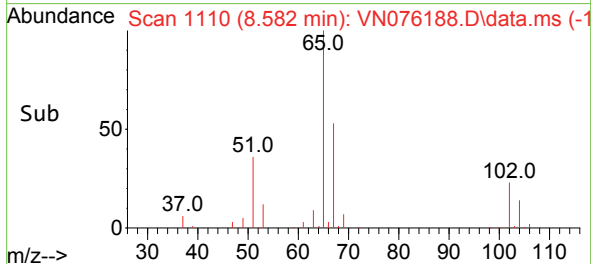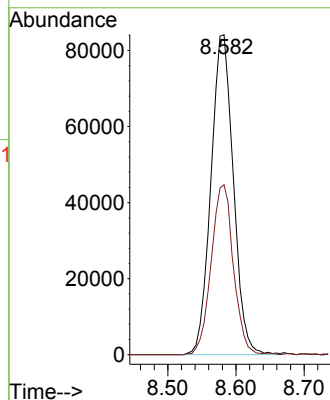

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 9.100 min Scan# 1198

Delta R.T. -0.006 min

Lab File: VN076188.D

Acq: 10 Jan 2023 17:36




Tgt Ion: 114 Resp: 581702


Ion Ratio Lower Upper

114 100

63 19.1 0.0 34.4

88 15.8 0.0 28.8

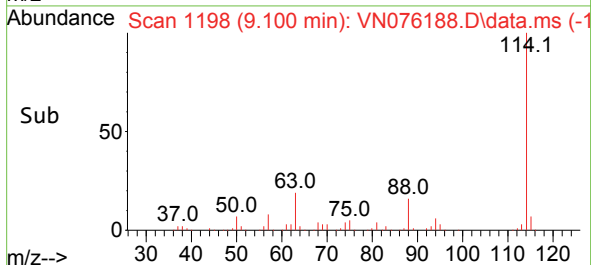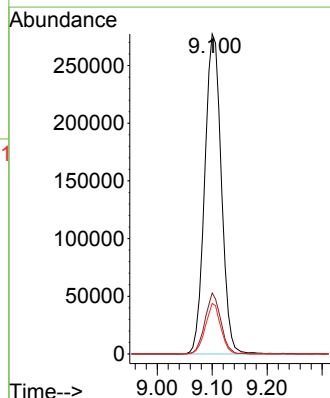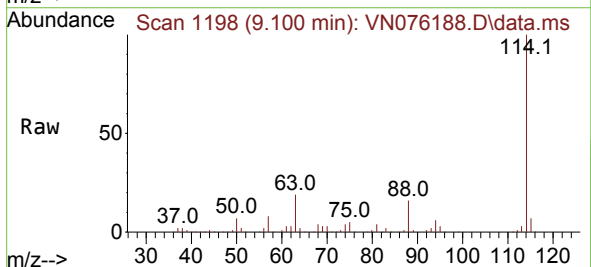



#35

Dibromofluoromethane

Concen: 45.682 ug/l

RT: 8.171 min Scan# 1040

Delta R.T. -0.000 min

Lab File: VN076188.D

Acq: 10 Jan 2023 17:36

Instrument :

MSVOA_N

ClientSampleId :





Tgt Ion:113 Resp: 164564

Ion Ratio Lower Upper

113 100

111 103.3 83.4 125.2

192 19.9 16.1 24.1

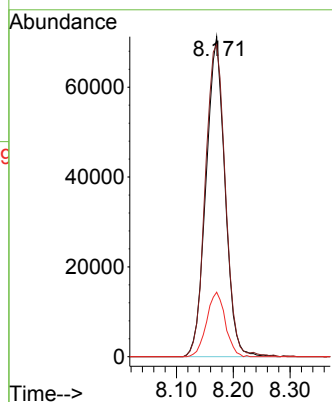

#36

1,1-Dichloropropene

Concen: 5.603 ug/l

RT: 8.224 min Scan# 1049

Delta R.T. -0.153 min

Lab File: VN076188.D

Acq: 10 Jan 2023 17:36




Tgt Ion: 75 Resp: 26813


Ion Ratio Lower Upper

75 100

110 9.8 18.8 56.4#


77 0.0 24.1 36.1#

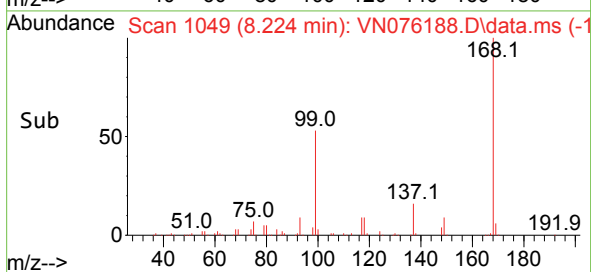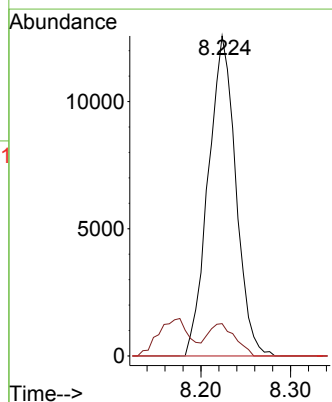






#38
Carbon Tetrachloride
Concen: 6.965 ug/l
RT: 8.224 min Scan# 1049
Delta R.T. -0.141 min
Lab File: VN076188.D
Acq: 10 Jan 2023 17:36

Instrument :
MSVOA_N
ClientSampleId :







Tgt Ion:117 Resp: 37302
Ion Ratio Lower Upper
117 100
119 5.5 76.1 114.1#
121 0.0 24.5 36.7#

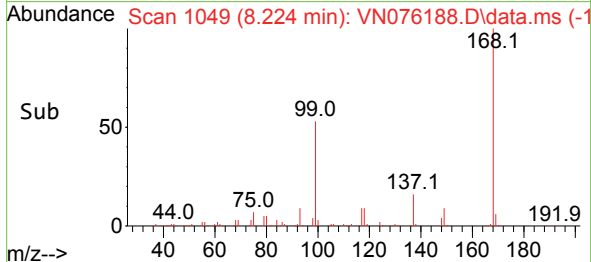

#39
Methylcyclohexane
Concen: 0.469 ug/l
RT: 9.594 min Scan# 1282
Delta R.T. -0.012 min
Lab File: VN076188.D
Acq: 10 Jan 2023 17:36

Tgt Ion: 83 Resp: 2709
Ion Ratio Lower Upper
83 100
55 59.3 51.4 77.0
98 45.6 39.8 59.8

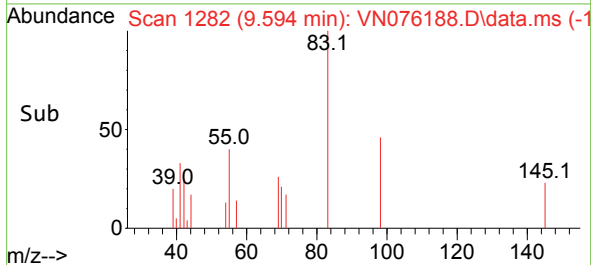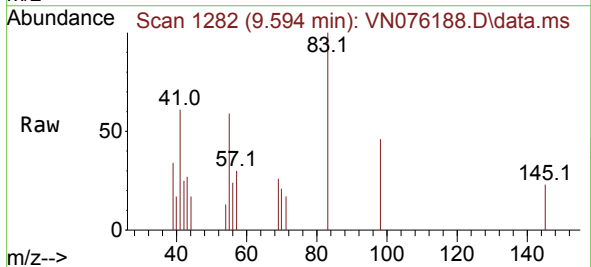



#48

Methyl methacrylate

Concen: 0.371 ug/l

RT: 9.647 min Scan# 11

Delta R.T. -0.035 min


Lab File: VN076188.D

Acq: 10 Jan 2023 17:36

Instrument :

MSVOA_N

ClientSampleId :






Tgt Ion: 41 Resp: 1059

Ion Ratio Lower Upper

41 100

69 11.9 81.9 122.9#

39 18.1 51.6 77.4#

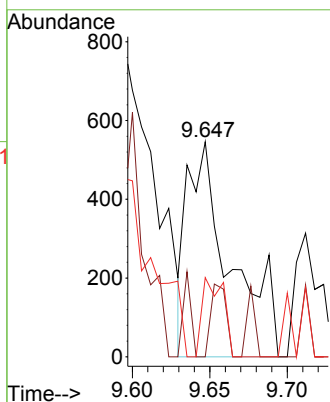

#50

Toluene-d8

Concen: 50.593 ug/l

RT: 10.565 min Scan# 1447

Delta R.T. -0.006 min

Lab File: VN076188.D




Acq: 10 Jan 2023 17:36


Tgt Ion: 98 Resp: 681437

Ion Ratio Lower Upper

98 100

100 65.1 52.1 78.1


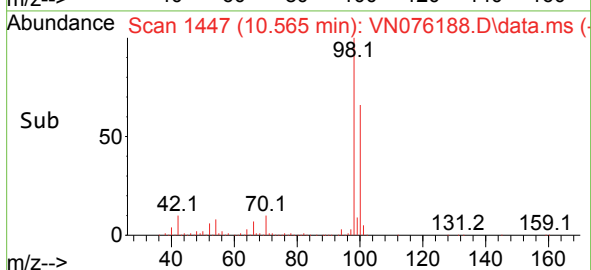
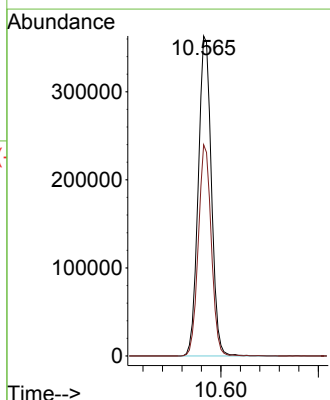





#51
4-Methyl-2-Pentanone
Concen: 0.292 ug/l
RT: 10.453 min Scan# 1428
Delta R.T. 0.006 min
Lab File: VN076188.D
Acq: 10 Jan 2023 17:36




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 43 Resp: 1120
Ion Ratio Lower Upper
43 100
58 0.0 35.5 53.3#

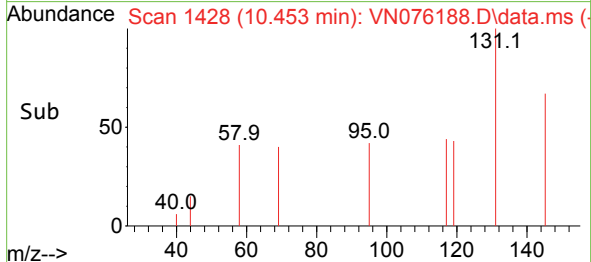

#52
Toluene
Concen: 0.662 ug/l
RT: 10.629 min Scan# 1458
Delta R.T. -0.006 min
Lab File: VN076188.D
Acq: 10 Jan 2023 17:36


Tgt Ion: 92 Resp: 6370
Ion Ratio Lower Upper
92 100
91 187.9 137.3 205.9

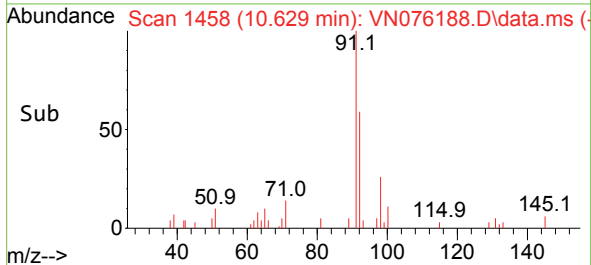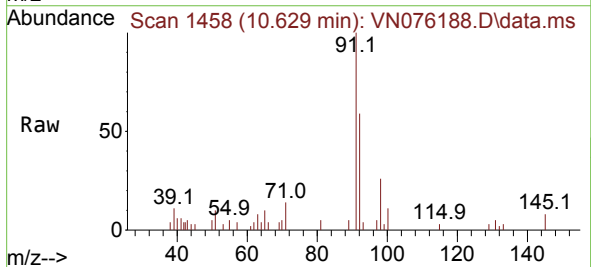



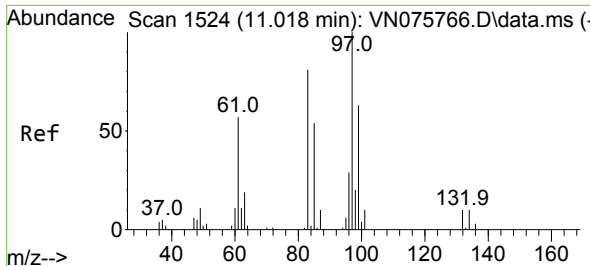


#55
 1,1,2-Trichloroethane
 Concen: 0.634 ug/l
 RT: 11.012 min Scan# 1523
 Delta R.T. -0.006 min
 Lab File: VN076188.D
 Acq: 10 Jan 2023 17:36

Instrument :
 MSVOA_N
 ClientSampleId :



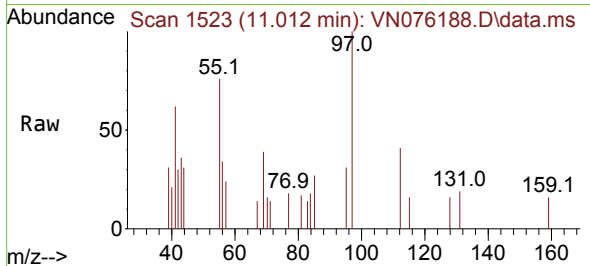



Tgt Ion: 97	Resp: 2393
Ion Ratio	Lower Upper
97 100	
83 0.0	65.0 97.4#
85 27.4	43.0 64.6#
99 0.0	50.2 75.2#

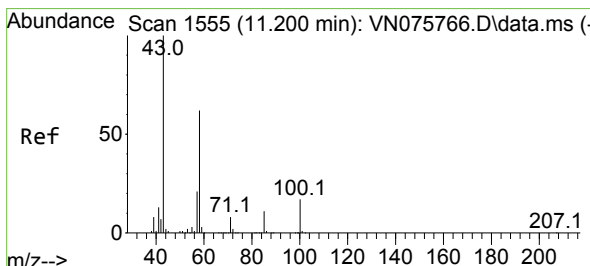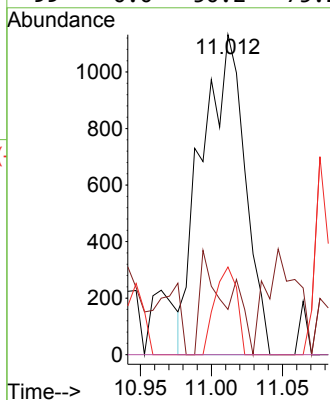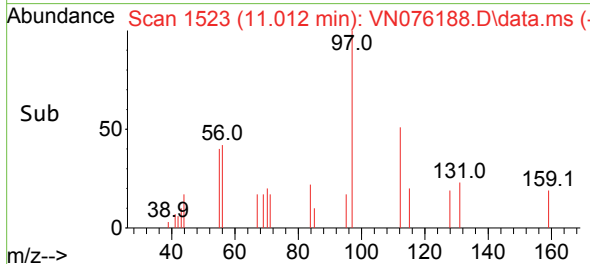

#59
 2-Hexanone
 Concen: 1.174 ug/l
 RT: 11.170 min Scan# 1550
 Delta R.T. -0.030 min
 Lab File: VN076188.D
 Acq: 10 Jan 2023 17:36

Tgt Ion: 43	Resp: 3282
Ion Ratio	Lower Upper
43 100	
58 0.0	30.6 92.0#


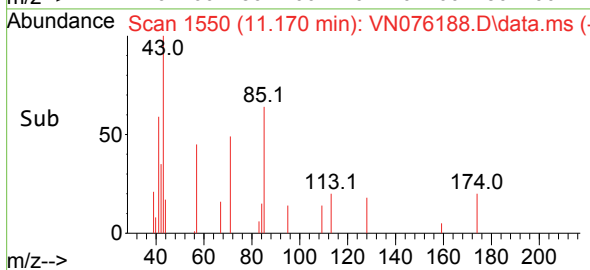
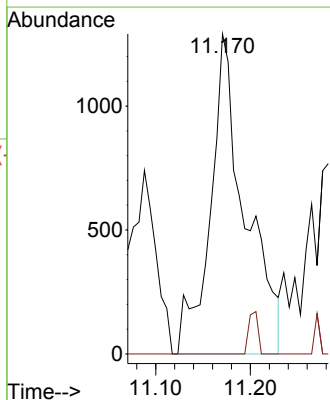
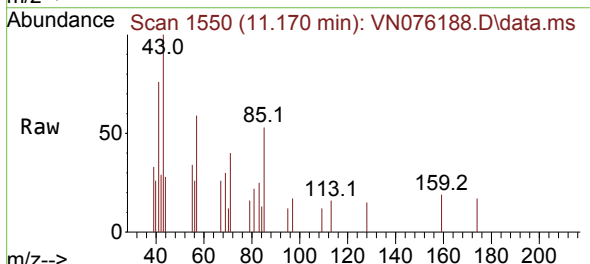


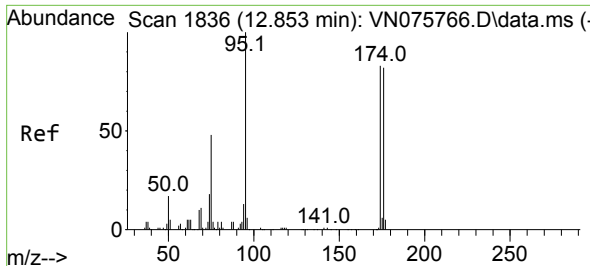

#62
4-Bromofluorobenzene
Concen: 49.339 ug/l
RT: 12.853 min Scan# 1836
Delta R.T. -0.000 min
Lab File: VN076188.D
Acq: 10 Jan 2023 17:36




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 95 Resp: 220105
Ion Ratio Lower Upper
95 100
174 85.5 0.0 171.6
176 82.7 0.0 169.2

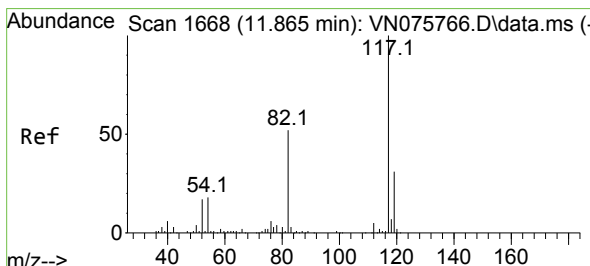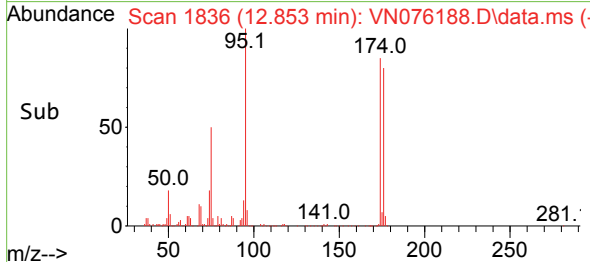

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.865 min Scan# 1668
Delta R.T. -0.000 min
Lab File: VN076188.D
Acq: 10 Jan 2023 17:36

Tgt Ion: 117 Resp: 505726
Ion Ratio Lower Upper
117 100
82 52.3 41.3 61.9
119 30.6 24.6 37.0


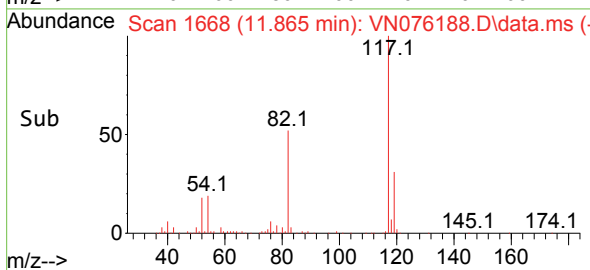

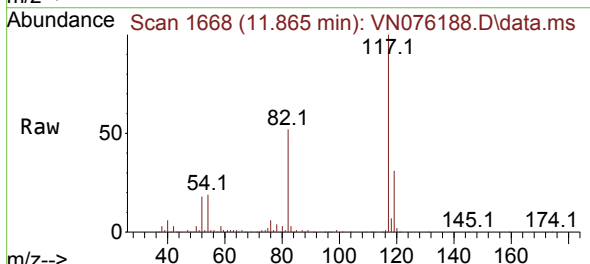




#67
Ethyl Benzene
Concen: 0.604 ug/l
RT: 11.965 min Scan# 1190
Delta R.T. -0.000 min
Lab File: VN076188.D
Acq: 10 Jan 2023 17:36




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 91 Resp: 10586
Ion Ratio Lower Upper
91 100
106 30.2 25.7 38.5

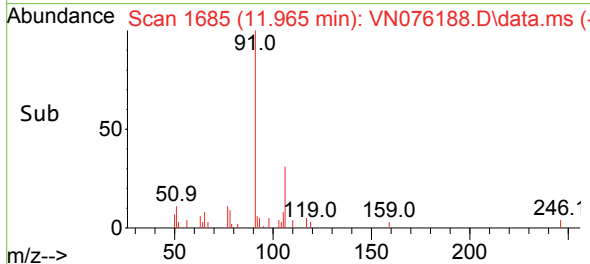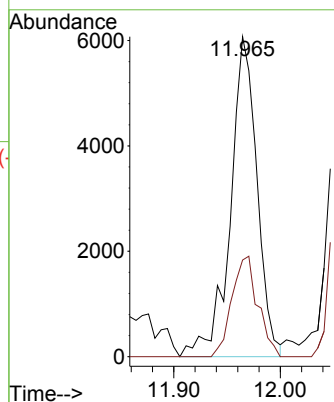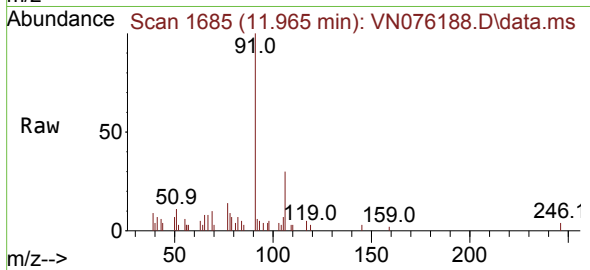

#68
m/p-Xylenes
Concen: 2.609 ug/l
RT: 12.070 min Scan# 1703
Delta R.T. -0.006 min
Lab File: VN076188.D
Acq: 10 Jan 2023 17:36

Tgt Ion:106 Resp: 18089
Ion Ratio Lower Upper
106 100
91 194.7 156.6 235.0


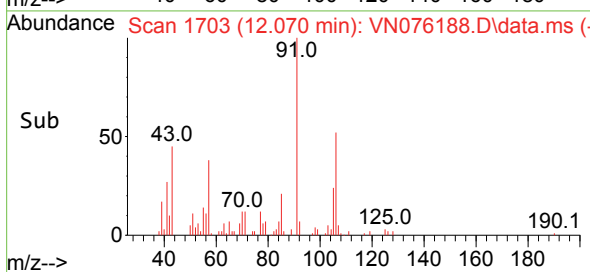
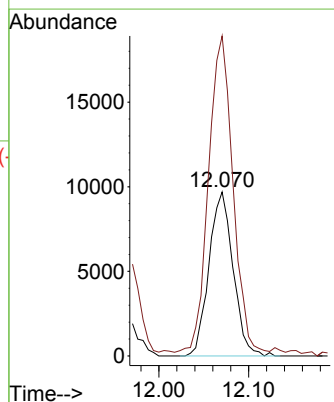
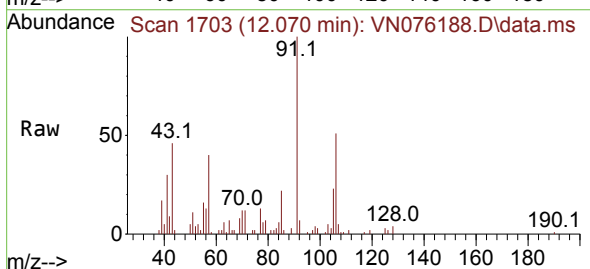




#69
o-Xylene
Concen: 1.646 ug/l
RT: 12.406 min Scan# 11
Delta R.T. 0.006 min
Lab File: VN076188.D
Acq: 10 Jan 2023 17:36




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion:106 Resp: 11297
Ion Ratio Lower Upper
106 100
91 195.0 103.8 311.6

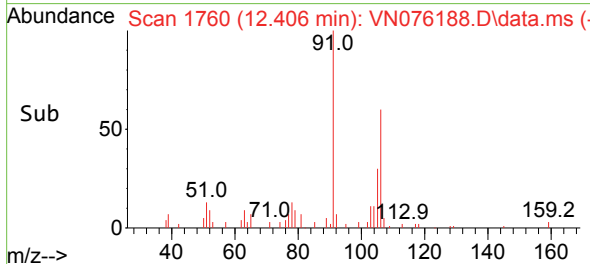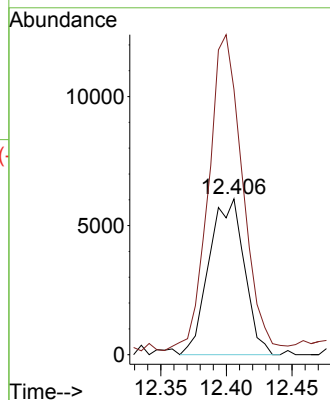

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.794 min Scan# 1996
Delta R.T. -0.000 min
Lab File: VN076188.D
Acq: 10 Jan 2023 17:36


Tgt Ion:152 Resp: 234743
Ion Ratio Lower Upper
152 100
115 58.0 29.1 87.4
150 156.0 0.0 347.0

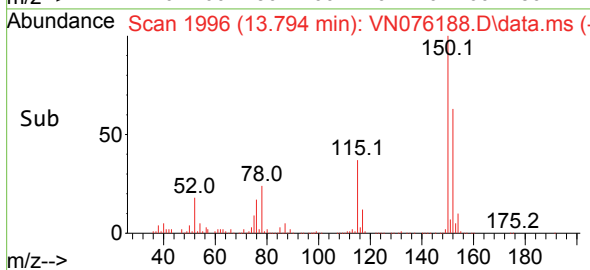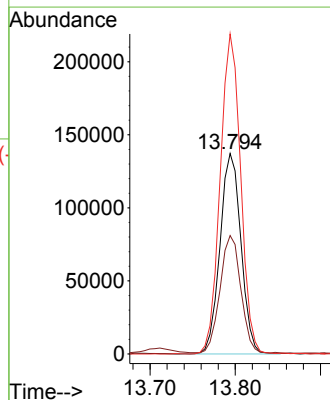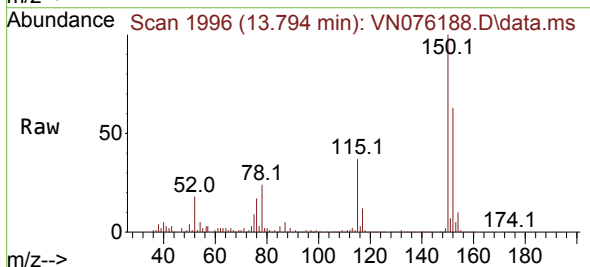






#73
Isopropylbenzene
Concen: 0.332 ug/l
RT: 12.700 min Scan# 11
Delta R.T. -0.000 min
Lab File: VN076188.D
Acq: 10 Jan 2023 17:36


Instrument :
MSVOA_N
ClientSampleId :





Tgt Ion:105 Resp: 5626
Ion Ratio Lower Upper
105 100
120 20.7 13.4 40.2

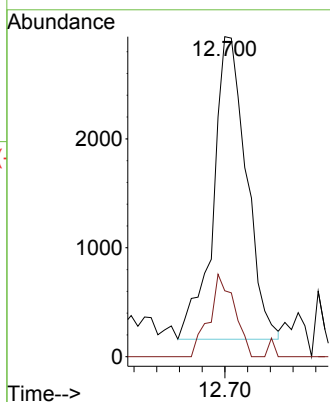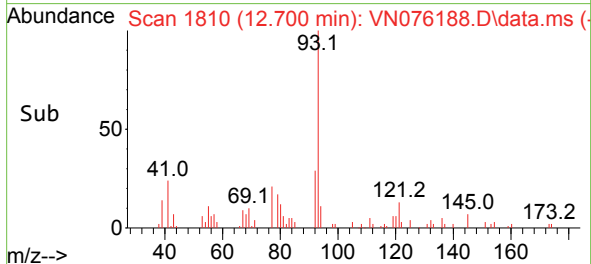


#74
N-ethyl acetate
Concen: 1.146 ug/l
RT: 12.482 min Scan# 1773
Delta R.T. -0.012 min
Lab File: VN076188.D
Acq: 10 Jan 2023 17:36

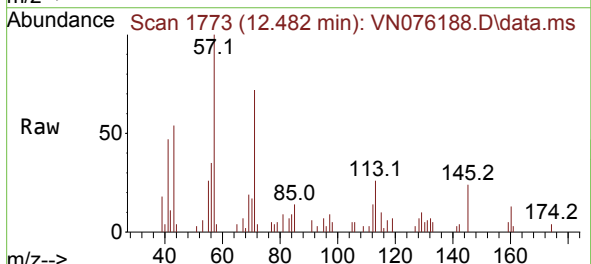

Tgt Ion: 43 Resp: 5701
Ion Ratio Lower Upper
43 100
70 31.5 41.4 62.0#
55 34.6 21.3 31.9#
61 0.0 21.2 31.8#

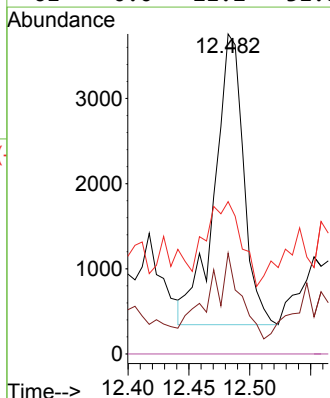



#76

1,2,3-Trichloropropane

Concen: 23.744 ug/l

RT: 12.853 min Scan# 1836

Delta R.T. -0.141 min

Lab File: VN076188.D

Acq: 10 Jan 2023 17:36

Instrument :

MSVOA_N





ClientSampleId :

Tgt Ion: 75 Resp: 112352

Ion Ratio Lower Upper

75 100

77 1.3 82.6 247.8#

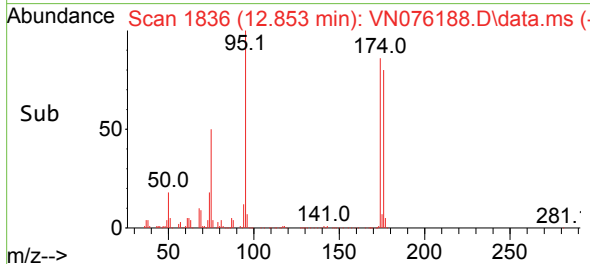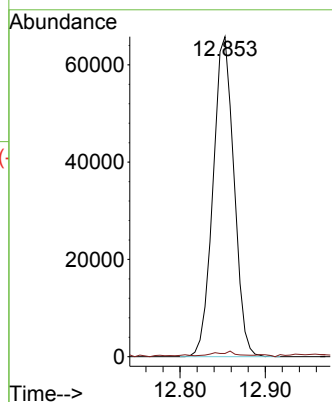

#78

n-propylbenzene

Concen: 0.302 ug/l

RT: 13.035 min Scan# 1867

Delta R.T. -0.006 min

Lab File: VN076188.D




Acq: 10 Jan 2023 17:36


Tgt Ion: 91 Resp: 5652

Ion Ratio Lower Upper

91 100

120 54.5 12.0 36.1#

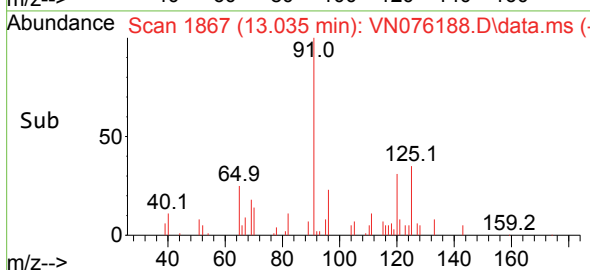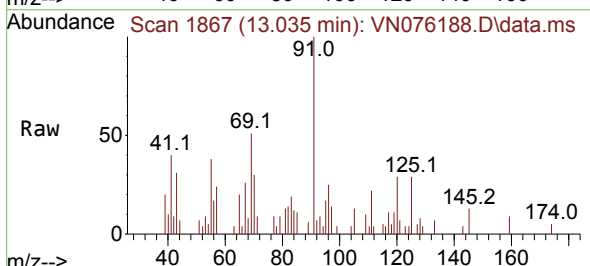



#79

2-Chlorotoluene

Concen: 0.202 ug/l

RT: 13.106 min Scan# 1879

Delta R.T. -0.024 min

Lab File: VN076188.D

Acq: 10 Jan 2023 17:36

Instrument :

MSVOA_N





ClientSampleId :

Tgt Ion: 91 Resp: 2361

Ion Ratio Lower Upper

91 100

126 0.0 17.5 52.5#

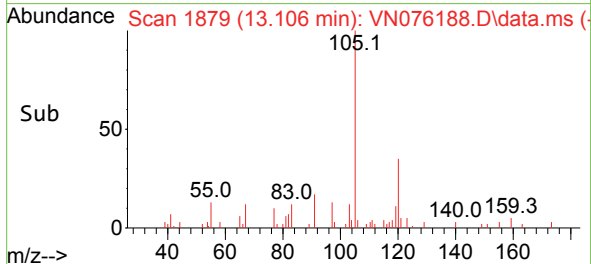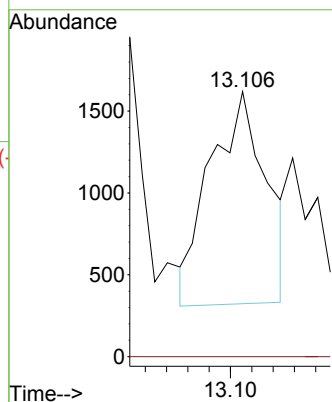

#80

1,3,5-Trimethylbenzene

Concen: 0.728 ug/l

RT: 13.176 min Scan# 1891

Delta R.T. -0.000 min

Lab File: VN076188.D




Acq: 10 Jan 2023 17:36


Tgt Ion: 105 Resp: 10342

Ion Ratio Lower Upper

105 100

120 56.5 24.7 74.1


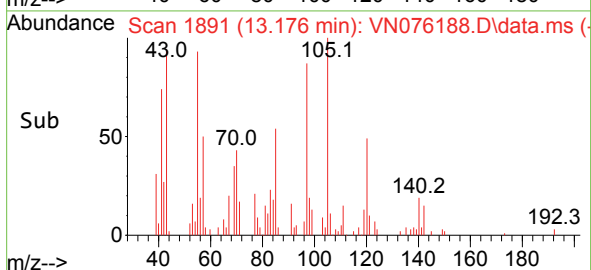






#81
trans-1,4-Dichloro-2-butene
Concen: 85.466 ug/l
RT: 12.853 min Scan# 1836
Delta R.T. 0.112 min
Lab File: VN076188.D
Acq: 10 Jan 2023 17:36




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 75 Resp: 112352
Ion Ratio Lower Upper
75 100
53 0.2 73.8 110.6#
89 0.1 39.5 59.3#

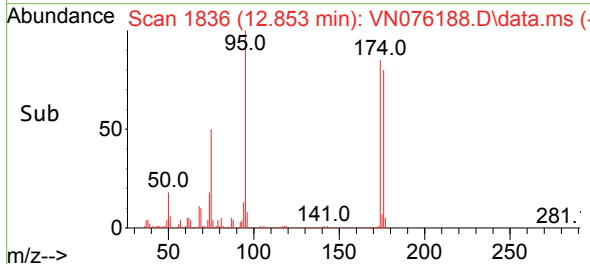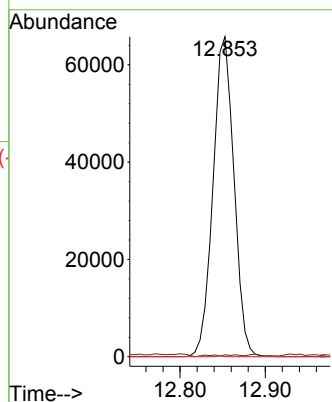

#82
4-Chlorotoluene
Concen: 0.202 ug/l
RT: 13.106 min Scan# 1879
Delta R.T. -0.024 min
Lab File: VN076188.D
Acq: 10 Jan 2023 17:36

Tgt Ion: 91 Resp: 2361
Ion Ratio Lower Upper
91 100
126 0.0 17.5 52.5#

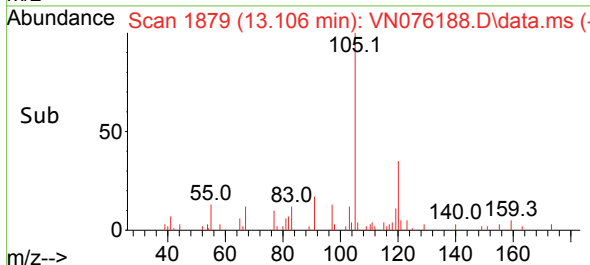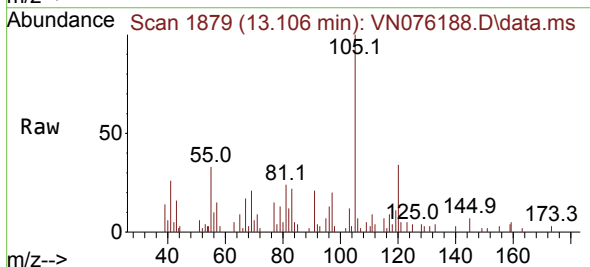



#83

tert-Butylbenzene

Concen: 0.375 ug/l

RT: 13.488 min Scan# 1936

Delta R.T. 0.047 min

Lab File: VN076188.D





Acq: 10 Jan 2023 17:36

Instrument :

MSVOA_N

ClientSampleId :

Tgt Ion:119	Resp:	4689
Ion Ratio	Lower	Upper
119	100	
91	99.6	31.9 95.5#
134	4.3	13.8 41.4#

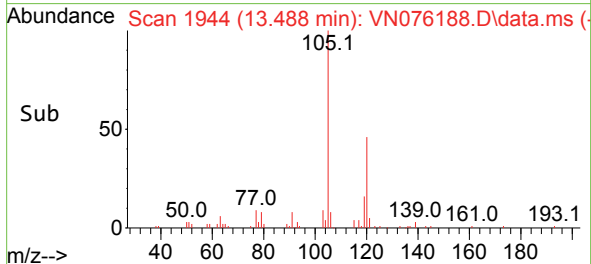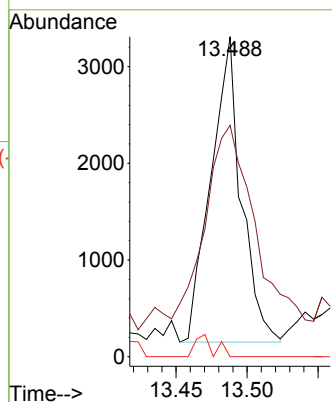

#84

1,2,4-Trimethylbenzene

Concen: 2.510 ug/l




RT: 13.488 min Scan# 1944


Delta R.T. 0.006 min

Lab File: VN076188.D

Acq: 10 Jan 2023 17:36

Tgt Ion:105	Resp:	35357
Ion Ratio	Lower	Upper
105	100	
120	45.6	23.3 69.8


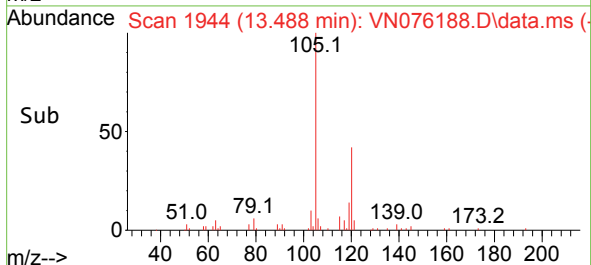

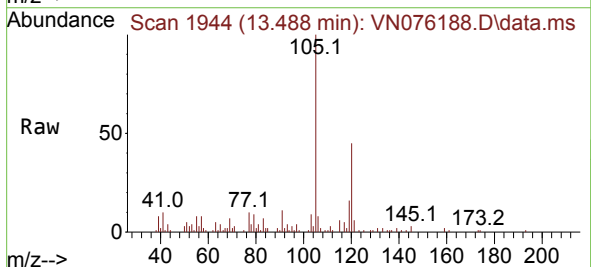




#85
 sec-Butylbenzene
 Concen: 0.476 ug/l
 RT: 13.611 min Scan# 1965
 Delta R.T. -0.006 min
 Lab File: VN076188.D
 Acq: 10 Jan 2023 17:36




Instrument :
 MSVOA_N
 ClientSampleId :


Tgt Ion:105 Resp: 8226
 Ion Ratio Lower Upper
 105 100
 134 26.0 10.1 30.1

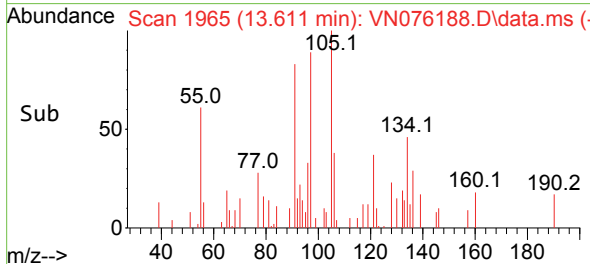

#86
 p-Isopropyltoluene
 Concen: 2.695 ug/l
 RT: 13.729 min Scan# 1985
 Delta R.T. -0.000 min
 Lab File: VN076188.D
 Acq: 10 Jan 2023 17:36

Tgt Ion:119 Resp: 38738
 Ion Ratio Lower Upper
 119 100
 134 26.0 13.0 39.0
 91 0.0 11.2 33.6#

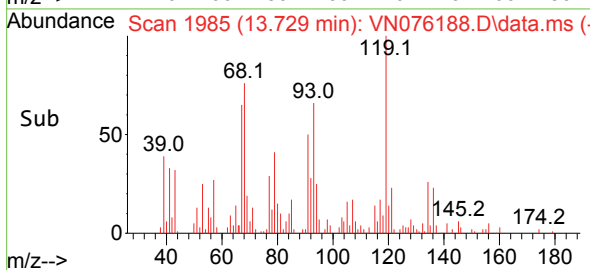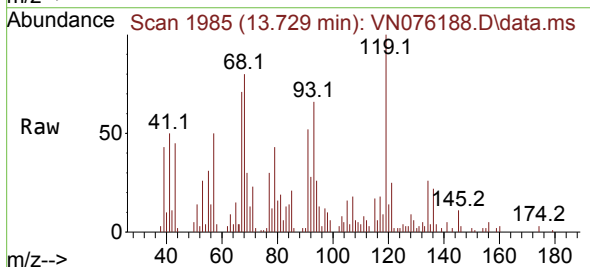



#90

Hexachloroethane

Concen: 0.361 ug/l

RT: 14.329 min Scan# 2088

Delta R.T. -0.006 min

Lab File: VN076188.D

Acq: 10 Jan 2023 17:36

Instrument :

MSVOA_N





ClientSampleId :

Tgt Ion:117 Resp: 929

Ion Ratio Lower Upper

117 100

201 0.0 38.0 114.1#

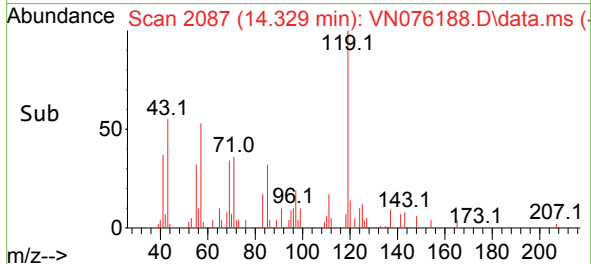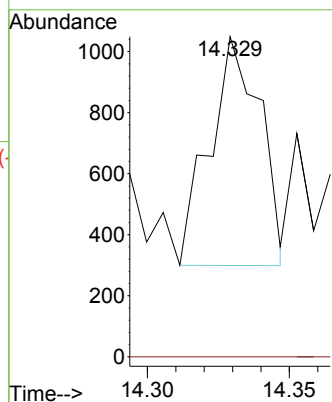

#95

Naphthalene

Concen: 2.861 ug/l

RT: 15.641 min Scan# 2310

Delta R.T. -0.000 min

Lab File: VN076188.D

Acq: 10 Jan 2023 17:36

Tgt Ion:128 Resp: 9123

Ion Ratio Lower Upper

128 100

127 23.0 10.4 15.6#

129 8.7 8.7 13.1#

