



BFB

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN011023\
Data File : VN076171.D
Acq On : 10 Jan 2023 08:33
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N121422W.M
Title : SW846 8260
Last Update : Wed Dec 14 13:03:41 2022

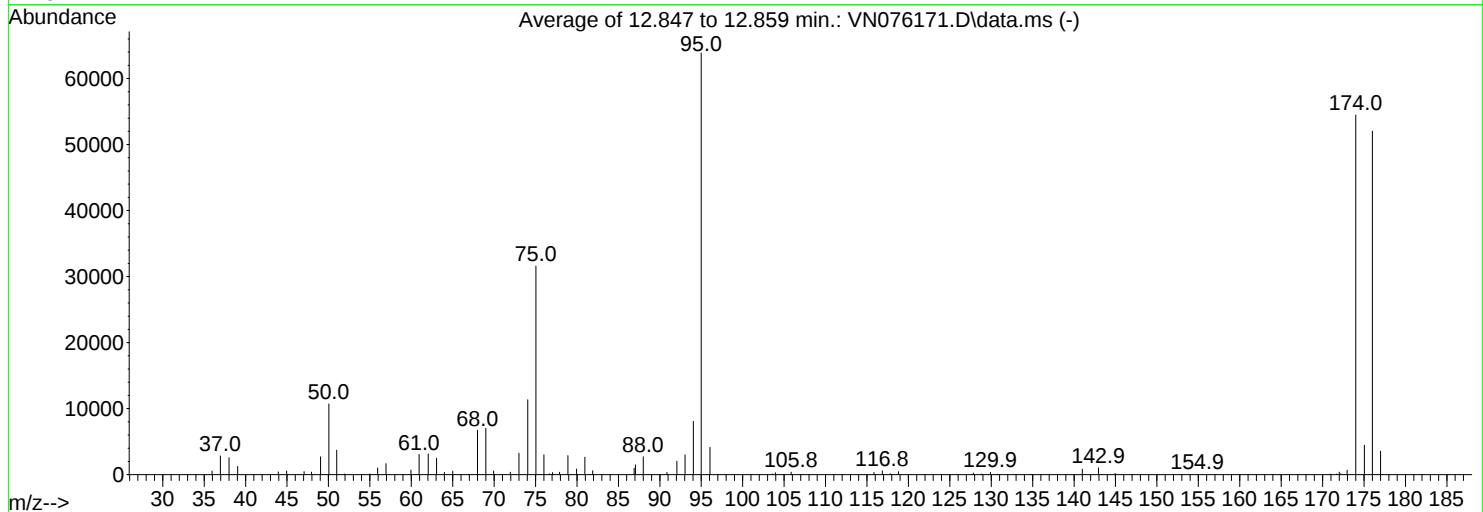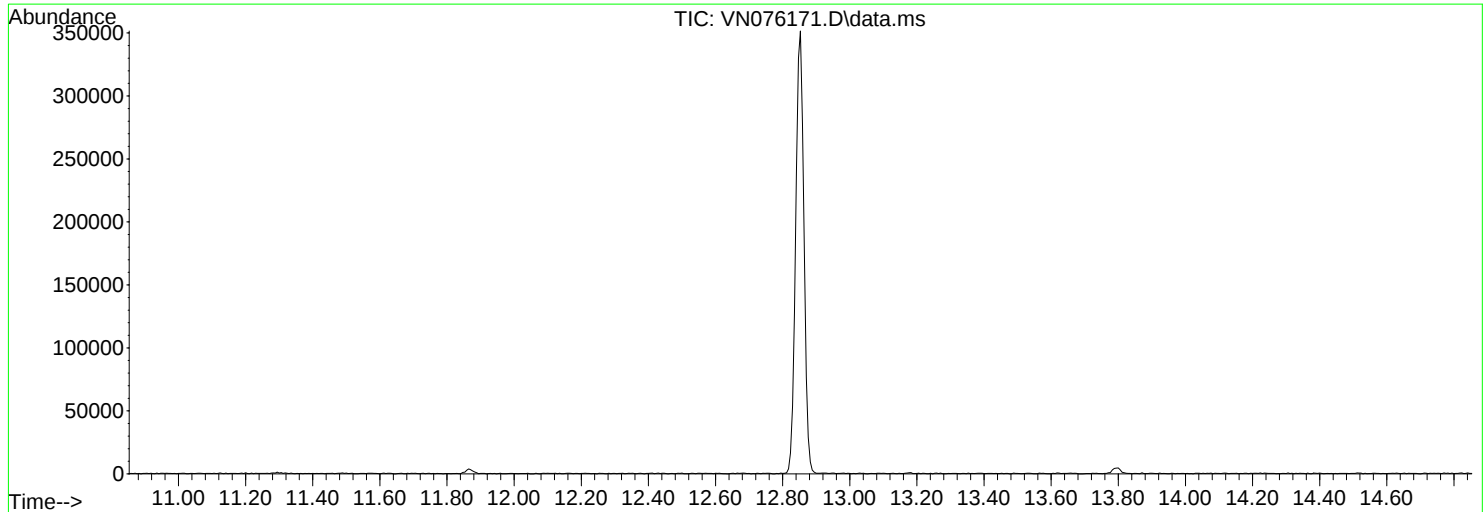

AutoFind: Scans 1835, 1836, 1837; Background Corrected with Scan 1826

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.8	10716	PASS
75	95	30	60	49.5	31605	PASS
95	95	100	100	100.0	63888	PASS
96	95	5	9	6.5	4157	PASS
173	174	0.00	2	1.2	674	PASS
174	95	50	100	85.3	54469	PASS
175	174	5	9	8.2	4456	PASS
176	174	95	101	95.5	52040	PASS
177	176	5	9	6.9	3566	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.95	571	51.95	106	66.90	55	77.90	35
36.95	2848	55.00	114	68.00	6712	78.90	288
38.00	2571	55.95	1009	69.00	7006	79.95	85
39.05	1244	56.95	1679	69.95	571	80.95	264
43.95	410	58.10	56	71.95	359	81.90	597
44.95	528	59.95	709	73.00	3247	86.90	965
47.05	459	60.95	3067	74.05	11355	87.05	1468
47.95	385	62.05	3154	75.05	31605	88.00	2714
49.05	2683	63.05	2500	76.00	3004	90.85	352
50.05	10716	64.00	351	76.70	119	92.05	2035
51.00	3721	65.00	529	77.05	315	93.05	2998

Average of 12.847 to 12.859 min.: VN076171.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
94.05	8083	117.80	145	154.90	57		
95.00	63888	118.80	471	170.90	106		
96.05	4157	127.85	244	171.70	102		
97.00	67	128.80	108	172.00	390		
103.60	99	129.90	346	172.20	113		
103.95	297	130.80	64	172.95	674		
104.90	57	134.80	56	174.00	54469		
105.85	381	137.00	64	175.05	4456		
107.10	56	141.00	837	176.00	52040		
115.85	335	142.95	1021	177.00	3566		
116.85	573	144.95	198	178.00	61		