

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN020223\
 Data File : VN076508.D
 Acq On : 02 Feb 2023 14:28
 Operator : JC\MD
 Sample : PB150614TB
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 PB150614TB


Quant Time: Feb 03 00:59:37 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N011623W.M
 Quant Title : SW846 8260
 QLast Update : Tue Jan 17 03:59:22 2023
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.229	168	488262	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.106	114	817443	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.870	117	753336	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.794	152	296231	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.582	65	288747	52.816	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	= 105.640%	
35) Dibromofluoromethane	8.171	113	245821	48.073	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	= 96.140%	
50) Toluene-d8	10.571	98	968707	51.296	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	= 102.600%	
62) 4-Bromofluorobenzene	12.853	95	327671	53.151	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	= 106.300%	
Target Compounds						
					Qvalue	
3) Chloromethane	2.377	50	1176	0.227	ug/l	93
16) Acetone	4.447	43	38098	21.671	ug/l	97
18) Methyl Acetate	5.053	43	3762	0.633	ug/l #	75
20) Methylene Chloride	5.294	84	25368	4.342	ug/l	93
25) 2-Butanone	7.500	43	5842	2.183	ug/l #	78
29) Tetrahydrofuran	7.853	42	639	0.387	ug/l #	59
31) Cyclohexane	8.229	56	9531	1.135	ug/l #	13
36) 1,1-Dichloropropene	8.229	75	37897	5.216	ug/l #	50
37) Ethyl Acetate	7.571	43	50907	8.765	ug/l	99
38) Carbon Tetrachloride	8.229	117	50775	6.266	ug/l #	16
42) 1,2-Dichloroethane	8.688	62	2190	0.295	ug/l #	73
43) Isopropyl Acetate	8.694	43	246678	26.018	ug/l #	90
45) 1,2-Dichloropropane	9.741	63	3062	0.589	ug/l #	42
48) Methyl methacrylate	9.676	41	6593	1.469	ug/l #	38
49) 1,4-Dioxane	9.706	88	73	0.771	ug/l #	31
51) 4-Methyl-2-Pentanone	10.453	43	23758	4.269	ug/l #	73
54) cis-1,3-Dichloropropene	10.359	75	113211	13.551	ug/l #	61
57) 1,3-Dichloropropane	11.206	76	14854	1.646	ug/l #	42
59) 2-Hexanone	11.170	43	236671	58.680	ug/l #	21
74) N-amyl acetate	12.494	43	4672	0.709	ug/l #	62
76) 1,2,3-Trichloropropane	12.853	75	170518	31.242	ug/l #	1
77) Bromobenzene	12.982	156	1228	Below Cal		96
81) trans-1,4-Dichloro-2-b...	12.853	75	170518	95.774	ug/l #	11
87) 1,3-Dichlorobenzene	13.735	146	3148	0.291	ug/l	88
88) 1,4-Dichlorobenzene	13.735	146	3148	0.407	ug/l	89
89) n-Butylbenzene	14.059	91	4489	0.290	ug/l	97
91) 1,2-Dichlorobenzene	14.117	146	3204	0.298	ug/l	96
92) 1,2-Dibromo-3-Chloropr...	14.729	75	268	0.234	ug/l #	19
93) 1,2,4-Trichlorobenzene	15.394	180	3561	1.972	ug/l	93
95) Naphthalene	15.641	128	19864	3.082	ug/l	98
96) 1,2,3-Trichlorobenzene	15.841	180	5085	2.156	ug/l	92

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Quant Time: Feb 03 00:59:37 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N011623W.M
Quant Title : SW846 8260
QLast Update : Tue Jan 17 03:59:22 2023
Response via : Initial Calibration





#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 8.229 min Scan# 10

Delta R.T. -0.001 min

Lab File: VN076508.D

Acq: 02 Feb 2023 14:28

Instrument :

MSVOA_N

ClientSampleId :





PB150614TB

Tgt Ion:168 Resp: 488262

Ion Ratio Lower Upper

168 100

99 60.1 41.6 62.4

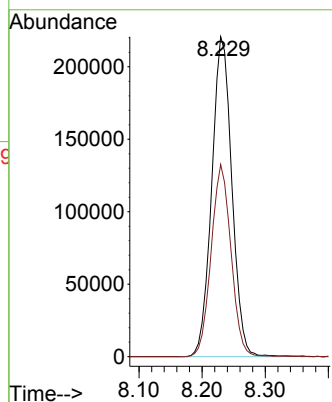

#3

Chloromethane

Concen: 0.227 ug/l

RT: 2.377 min Scan# 55

Delta R.T. 0.006 min

Lab File: VN076508.D




Acq: 02 Feb 2023 14:28


Tgt Ion: 50 Resp: 1176

Ion Ratio Lower Upper

50 100

52 27.0 24.8 37.2


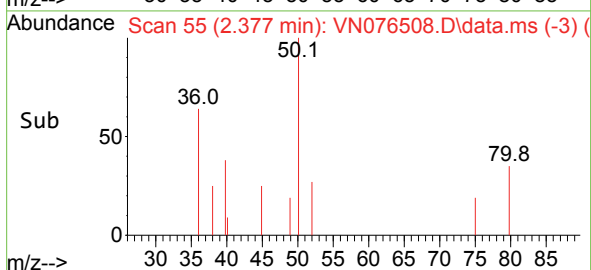






#16
Acetone
Concen: 21.671 ug/l
RT: 4.447 min Scan# 406
Delta R.T. 0.005 min
Lab File: VN076508.D
Acq: 02 Feb 2023 14:28




Instrument :
MSVOA_N
ClientSampleId :
PB150614TB


Tgt Ion: 43 Resp: 38098
Ion Ratio Lower Upper
43 100
58 31.5 26.7 40.1

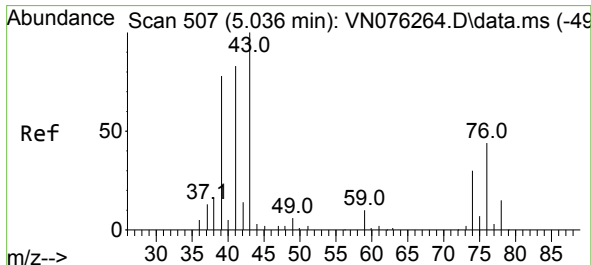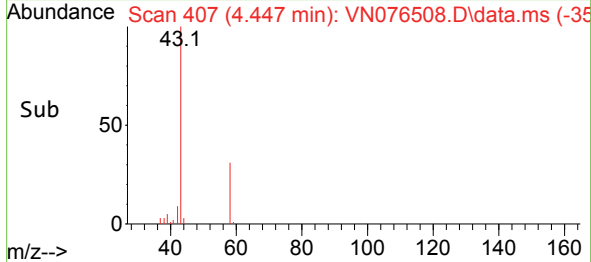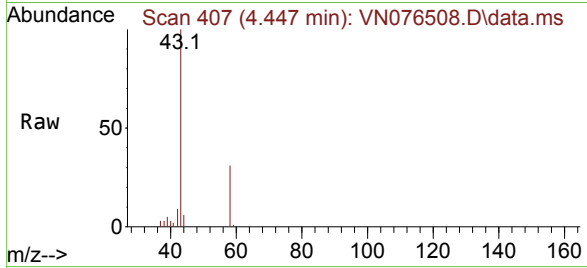

#18
Methyl Acetate
Concen: 0.633 ug/l
RT: 5.053 min Scan# 510
Delta R.T. 0.017 min
Lab File: VN076508.D
Acq: 02 Feb 2023 14:28

Tgt Ion: 43 Resp: 3762
Ion Ratio Lower Upper
43 100
74 15.8 23.3 34.9#




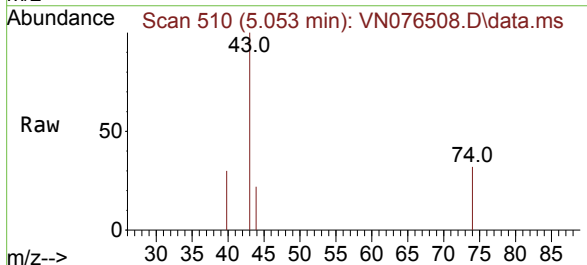




#20
Methylene Chloride
Concen: 4.342 ug/l
RT: 5.294 min Scan# 51
Delta R.T. 0.005 min
Lab File: VN076508.D
Acq: 02 Feb 2023 14:28




Instrument :
MSVOA_N
ClientSampleId :
PB150614TB


Tgt Ion: 84	Resp: 25368
Ion Ratio	Lower Upper
84 100	
49 112.9	84.5 126.7
51 35.6	26.0 39.0
86 59.4	52.0 78.0

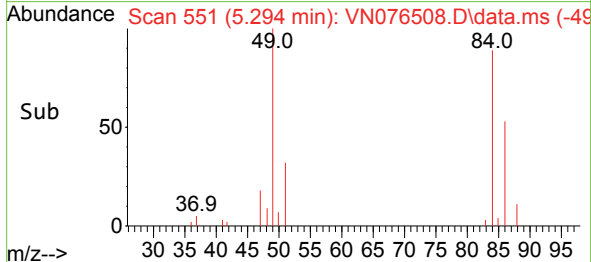

#25
2-Butanone
Concen: 2.183 ug/l
RT: 7.500 min Scan# 926
Delta R.T. 0.012 min
Lab File: VN076508.D
Acq: 02 Feb 2023 14:28

Tgt Ion: 43	Resp: 5842		
Ion Ratio	Lower	Upper	
43 100			
72 21.4	27.4	41.2#	


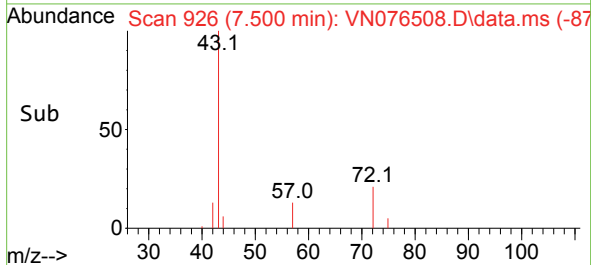






#29
Tetrahydrofuran
Concen: 0.387 ug/l
RT: 7.853 min Scan# 91
Delta R.T. 0.012 min
Lab File: VN076508.D
Acq: 02 Feb 2023 14:28




Instrument :
MSVOA_N
ClientSampleId :
PB150614TB


Tgt Ion: 42 Resp: 639
Ion Ratio Lower Upper
42 100
72 20.5 44.0 66.0#
71 27.5 41.1 61.7#



#31
Cyclohexane
Concen: 1.135 ug/l
RT: 8.229 min Scan# 1050
Delta R.T. -0.030 min
Lab File: VN076508.D
Acq: 02 Feb 2023 14:28

Tgt Ion: 56 Resp: 9531
Ion Ratio Lower Upper
56 100
69 167.3 25.8 38.8#
84 134.8 79.0 118.4#





#33

1,2-Dichloroethane-d4

Concen: 52.816 ug/l

RT: 8.582 min Scan# 1110

Delta R.T. 0.000 min

Lab File: VN076508.D

Acq: 02 Feb 2023 14:28

Instrument :

MSVOA_N

ClientSampleId :





PB150614TB

Tgt Ion: 65 Resp: 288747

Ion Ratio Lower Upper

65 100

67 51.2 0.0 104.6

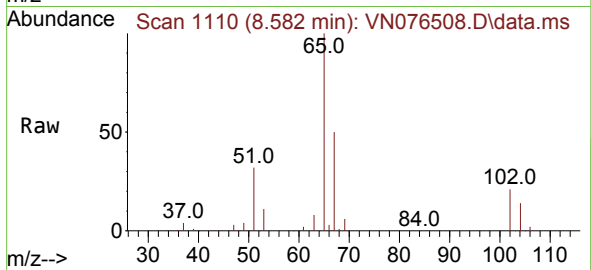

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 9.106 min Scan# 1199

Delta R.T. -0.000 min

Lab File: VN076508.D

Acq: 02 Feb 2023 14:28




Tgt Ion: 114 Resp: 817443


Ion Ratio Lower Upper

114 100

63 17.9 0.0 35.8


88 15.4 0.0 28.0

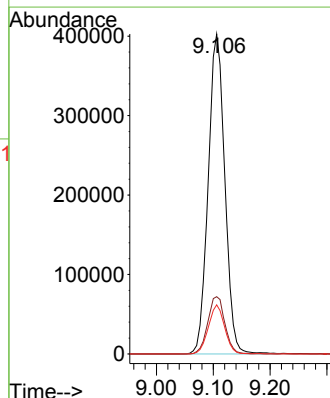






#35
Dibromofluoromethane
Concen: 48.073 ug/l
RT: 8.171 min Scan# 1040
Delta R.T. -0.000 min
Lab File: VN076508.D
Acq: 02 Feb 2023 14:28

Instrument :
MSVOA_N
ClientSampleId :
PB150614TB







Tgt Ion:113 Resp: 245821
Ion Ratio Lower Upper
113 100
111 102.6 82.7 124.1
192 18.7 15.6 23.4

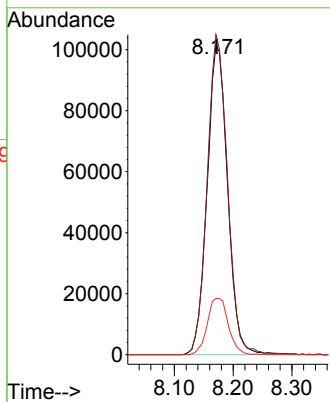

#36
1,1-Dichloropropene
Concen: 5.216 ug/l
RT: 8.229 min Scan# 1050
Delta R.T. -0.148 min
Lab File: VN076508.D
Acq: 02 Feb 2023 14:28

Tgt Ion: 75 Resp: 37897
Ion Ratio Lower Upper
75 100
110 10.7 18.8 56.3#
77 0.0 25.0 37.4#




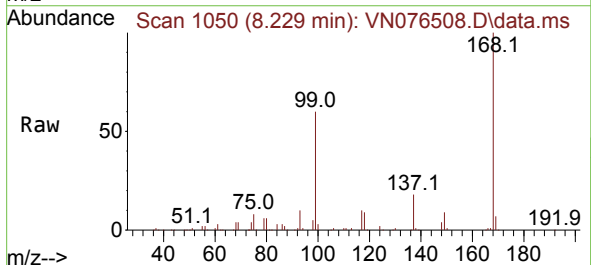




#37
Ethyl Acetate
Concen: 8.765 ug/l
RT: 7.571 min Scan# 91
Delta R.T. 0.006 min
Lab File: VN076508.D
Acq: 02 Feb 2023 14:28




Instrument :
MSVOA_N
ClientSampleId :
PB150614TB


Tgt Ion: 43 Resp: 50907
Ion Ratio Lower Upper
43 100
61 14.9 11.1 16.7
70 12.4 10.0 15.0



#38
Carbon Tetrachloride
Concen: 6.266 ug/l
RT: 8.229 min Scan# 1050
Delta R.T. -0.136 min
Lab File: VN076508.D
Acq: 02 Feb 2023 14:28

Tgt Ion: 117 Resp: 50775
Ion Ratio Lower Upper
117 100
119 4.4 75.4 113.0#
121 0.0 24.2 36.2#

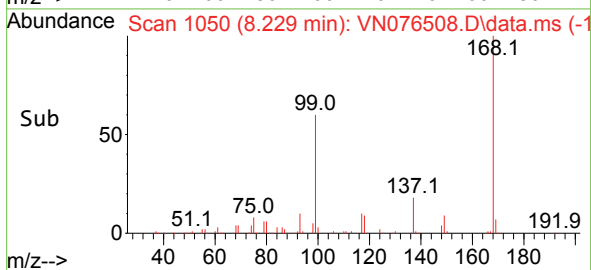

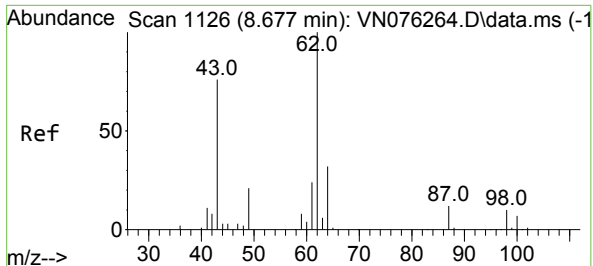

#42

1,2-Dichloroethane

Concen: 0.295 ug/l

RT: 8.688 min Scan# 1128

Delta R.T. 0.011 min

Lab File: VN076508.D

Acq: 02 Feb 2023 14:28

Instrument :

MSVOA_N

ClientSampleId :





PB150614TB

Tgt Ion: 62 Resp: 2190

Ion Ratio Lower Upper

62 100

98 0.0 0.0 20.4

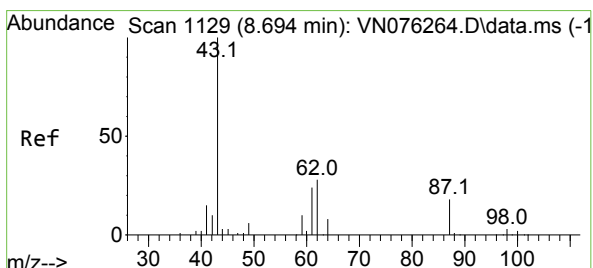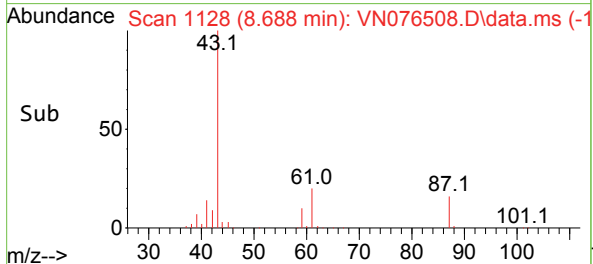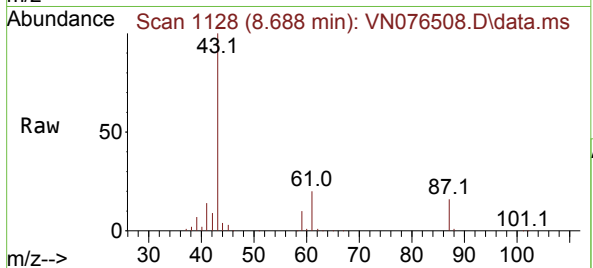

#43

Isopropyl Acetate

Concen: 26.018 ug/l

RT: 8.694 min Scan# 1129

Delta R.T. 0.000 min

Lab File: VN076508.D

Acq: 02 Feb 2023 14:28




Tgt Ion: 43 Resp: 246678


Ion Ratio Lower Upper

43 100

61 21.3 23.5 35.3#

87 16.3 13.8 20.6

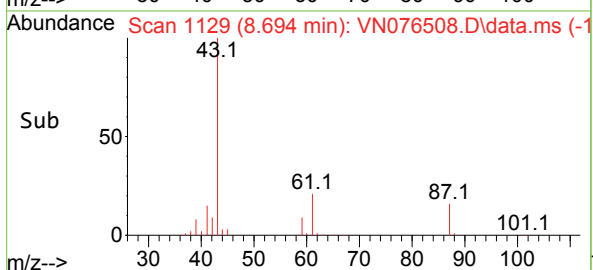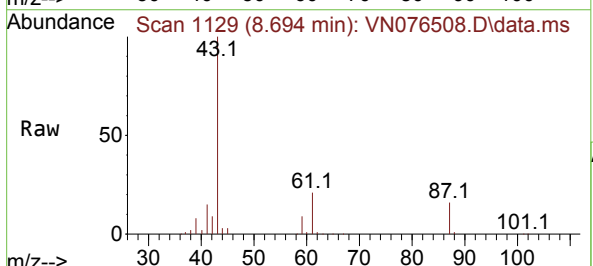



#45

1,2-Dichloropropane

Concen: 0.589 ug/l

RT: 9.741 min Scan# 11

Delta R.T. 0.117 min

Lab File: VN076508.D

Acq: 02 Feb 2023 14:28

Instrument :

MSVOA_N

ClientSampleId :





PB150614TB

Tgt Ion: 63 Resp: 3062

Ion Ratio Lower Upper

63 100

65 0.0 26.4 39.6#



#48

Methyl methacrylate

Concen: 1.469 ug/l

RT: 9.676 min Scan# 1296

Delta R.T. -0.006 min

Lab File: VN076508.D

Acq: 02 Feb 2023 14:28




Tgt Ion: 41 Resp: 6593


Ion Ratio Lower Upper

41 100

69 4.1 80.8 121.2#

39 59.7 54.4 81.6

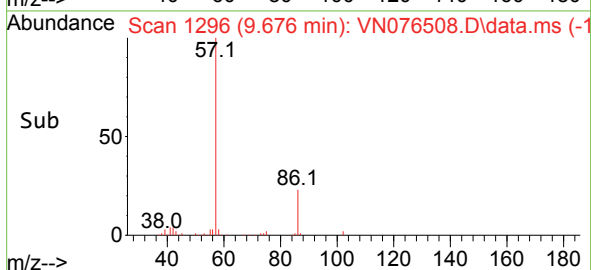



#49

1,4-Dioxane

Concen: 0.771 ug/l

RT: 9.706 min Scan# 11

Delta R.T. 0.006 min

Lab File: VN076508.D

Acq: 02 Feb 2023 14:28

Instrument :

MSVOA_N

ClientSampleId :

PB150614TB





Tgt Ion: 88 Resp: 73

Ion Ratio Lower Upper

88 100

43 0.0 18.1 27.1#

58 0.0 46.5 69.7#

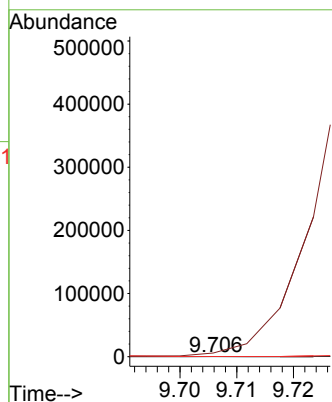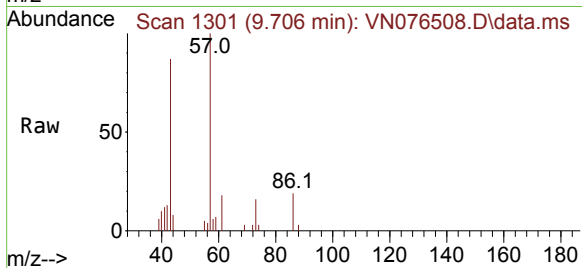

#50

Toluene-d8

Concen: 51.296 ug/l

RT: 10.571 min Scan# 1448

Delta R.T. -0.000 min

Lab File: VN076508.D




Acq: 02 Feb 2023 14:28


Tgt Ion: 98 Resp: 968707

Ion Ratio Lower Upper

98 100

100 65.4 52.2 78.4

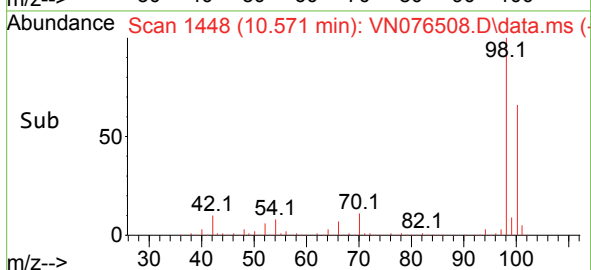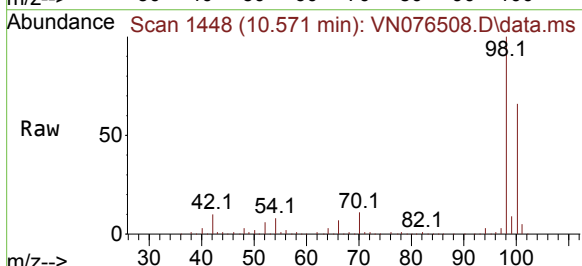



#51

4-Methyl-2-Pentanone

Concen: 4.269 ug/l

RT: 10.453 min Scan# 1428

Delta R.T. 0.006 min

Lab File: VN076508.D

Acq: 02 Feb 2023 14:28

Instrument :

MSVOA_N

ClientSampleId :





PB150614TB

Tgt Ion: 43 Resp: 23758

Ion Ratio Lower Upper

43 100

58 26.3 35.1 52.7#



#54

cis-1,3-Dichloropropene

Concen: 13.551 ug/l

RT: 10.359 min Scan# 1412

Delta R.T. 0.047 min

Lab File: VN076508.D

Acq: 02 Feb 2023 14:28




Tgt Ion: 75 Resp: 113211


Ion Ratio Lower Upper

75 100

77 0.3 26.5 39.7#

39 29.4 37.1 55.7#









#57
1,3-Dichloropropane
Concen: 1.646 ug/l
RT: 11.206 min Scan# 11
Delta R.T. 0.041 min
Lab File: VN076508.D
Acq: 02 Feb 2023 14:28




Instrument :
MSVOA_N
ClientSampleId :
PB150614TB


Tgt Ion: 76 Resp: 14854
Ion Ratio Lower Upper
76 100
78 0.0 26.4 39.6#

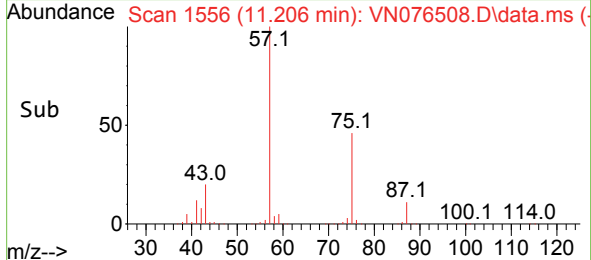

#59
2-Hexanone
Concen: 58.680 ug/l
RT: 11.170 min Scan# 1550
Delta R.T. -0.024 min
Lab File: VN076508.D
Acq: 02 Feb 2023 14:28

Tgt Ion: 43 Resp: 236671
Ion Ratio Lower Upper
43 100
58 0.0 30.1 90.3#


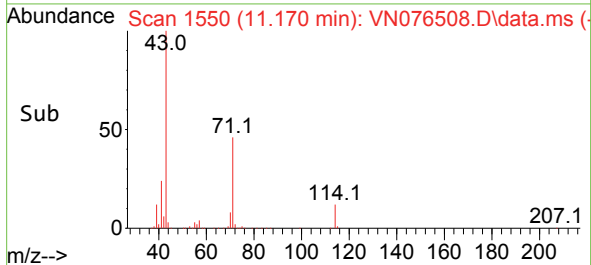






#62
4-Bromofluorobenzene
Concen: 53.151 ug/l
RT: 12.853 min Scan# 1836
Delta R.T. 0.006 min
Lab File: VN076508.D
Acq: 02 Feb 2023 14:28




Instrument :
MSVOA_N
ClientSampleId :
PB150614TB


Tgt Ion: 95 Resp: 327671
Ion Ratio Lower Upper
95 100
174 80.3 0.0 174.6
176 76.1 0.0 167.8

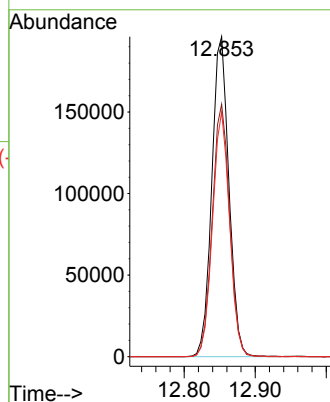

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.870 min Scan# 1669
Delta R.T. 0.005 min
Lab File: VN076508.D
Acq: 02 Feb 2023 14:28

Tgt Ion: 117 Resp: 753336
Ion Ratio Lower Upper
117 100
82 53.1 42.2 63.2
119 31.3 26.9 40.3


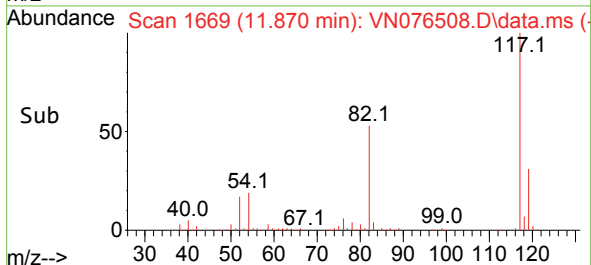






#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.794 min Scan# 1996
Delta R.T. -0.000 min
Lab File: VN076508.D
Acq: 02 Feb 2023 14:28




Instrument :
MSVOA_N
ClientSampleId :
PB150614TB


Tgt Ion:152 Resp: 296231
Ion Ratio Lower Upper
152 100
115 59.6 29.6 88.9
150 159.7 0.0 351.4

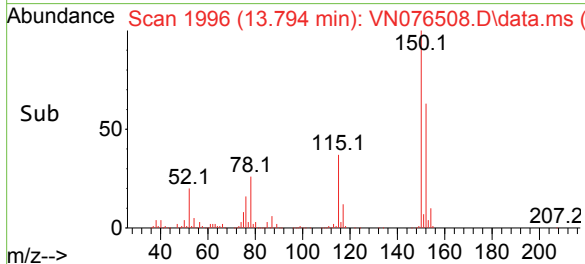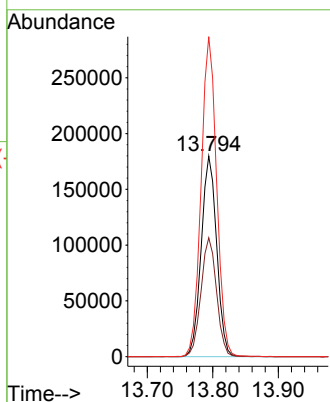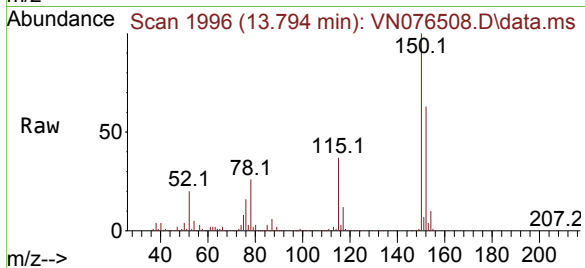

#74
N-ethyl acetate
Concen: 0.709 ug/l
RT: 12.494 min Scan# 1775
Delta R.T. -0.000 min
Lab File: VN076508.D
Acq: 02 Feb 2023 14:28

Tgt Ion: 43 Resp: 4672
Ion Ratio Lower Upper
43 100
70 19.8 41.2 61.8#
55 14.7 21.0 31.6#
61 7.4 21.6 32.4#


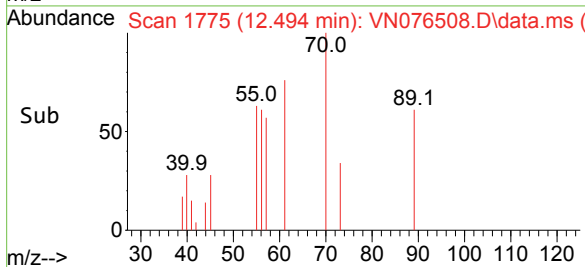

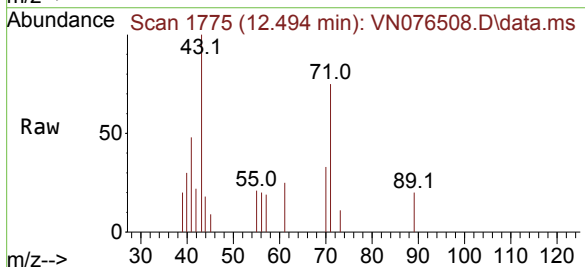




#76
1,2,3-Trichloropropane
Concen: 31.242 ug/l
RT: 12.853 min Scan# 1836
Delta R.T. -0.141 min
Lab File: VN076508.D
Acq: 02 Feb 2023 14:28




Instrument :
MSVOA_N
ClientSampleId :
PB150614TB


Tgt Ion: 75 Resp: 170518
Ion Ratio Lower Upper
75 100
77 1.0 75.2 225.6#



#77
Bromobenzene
Concen: Below Cal
RT: 12.982 min Scan# 1858
Delta R.T. 0.000 min
Lab File: VN076508.D
Acq: 02 Feb 2023 14:28

Tgt Ion:156 Resp: 1228
Ion Ratio Lower Upper
156 100
77 179.4 93.4 280.2
158 95.5 48.4 145.2


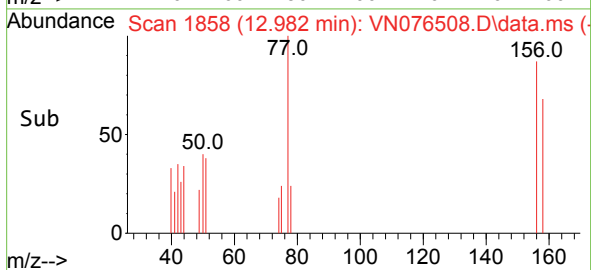






#81
trans-1,4-Dichloro-2-butene
Concen: 95.774 ug/l
RT: 12.853 min Scan# 1836
Delta R.T. 0.118 min
Lab File: VN076508.D
Acq: 02 Feb 2023 14:28




Instrument :
MSVOA_N
ClientSampleId :
PB150614TB


Tgt Ion: 75 Resp: 170518
Ion Ratio Lower Upper
75 100
53 0.0 75.8 113.8#
89 0.0 37.0 55.6#

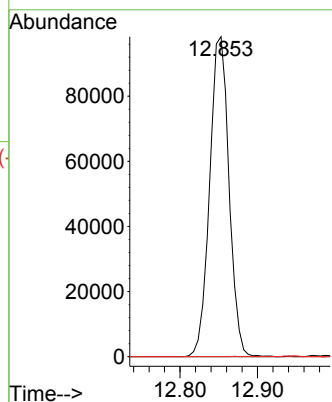

#87
1,3-Dichlorobenzene
Concen: 0.291 ug/l
RT: 13.735 min Scan# 1986
Delta R.T. 0.000 min
Lab File: VN076508.D
Acq: 02 Feb 2023 14:28


Tgt Ion:146 Resp: 3148
Ion Ratio Lower Upper
146 100
111 35.3 19.9 59.7
148 75.3 31.6 94.8

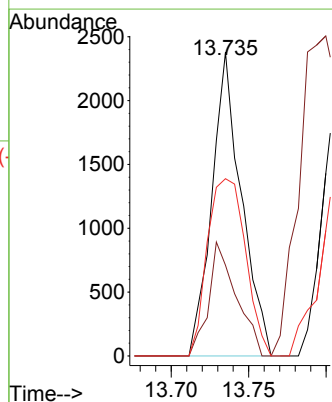






#88
1,4-Dichlorobenzene
Concen: 0.407 ug/l
RT: 13.735 min Scan# 1999
Delta R.T. -0.077 min
Lab File: VN076508.D
Acq: 02 Feb 2023 14:28


Instrument :
MSVOA_N
ClientSampleId :
PB150614TB





Tgt Ion:146 Resp: 3148
Ion Ratio Lower Upper
146 100
111 35.3 19.1 57.5
148 75.3 31.9 95.9




#89
n-Butylbenzene
Concen: 0.290 ug/l
RT: 14.059 min Scan# 2041
Delta R.T. -0.000 min
Lab File: VN076508.D
Acq: 02 Feb 2023 14:28



Tgt Ion: 91 Resp: 4489
Ion Ratio Lower Upper
91 100
92 53.3 26.3 78.9
134 29.3 13.2 39.5



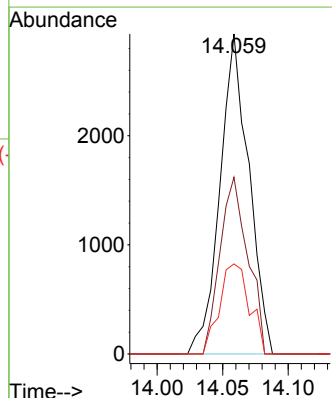
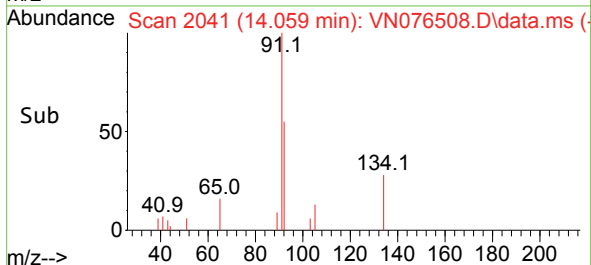




#91
1,2-Dichlorobenzene
Concen: 0.298 ug/l
RT: 14.117 min Scan# 2049
Delta R.T. 0.011 min
Lab File: VN076508.D
Acq: 02 Feb 2023 14:28




Instrument :
MSVOA_N
ClientSampleId :
PB150614TB


Tgt Ion:146 Resp: 3204
Ion Ratio Lower Upper
146 100
111 45.5 20.3 60.8
148 63.1 31.8 95.4

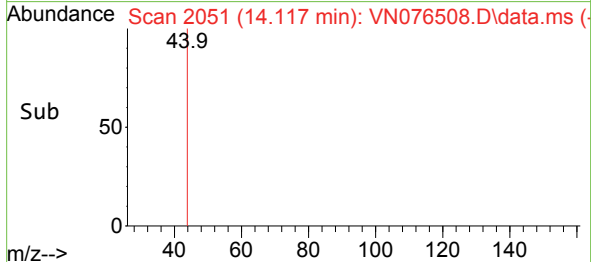

#92
1,2-Dibromo-3-Chloropropane
Concen: 0.234 ug/l
RT: 14.729 min Scan# 2155
Delta R.T. 0.006 min
Lab File: VN076508.D
Acq: 02 Feb 2023 14:28

Tgt Ion: 75 Resp: 268
Ion Ratio Lower Upper
75 100
155 0.0 45.0 135.0#
157 41.0 58.3 174.9#

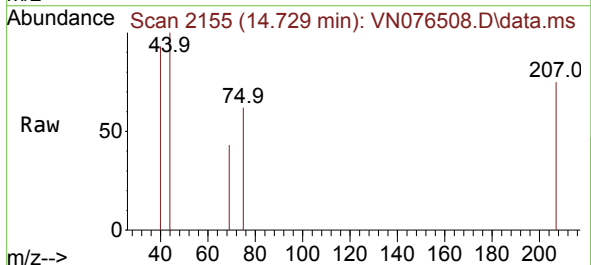

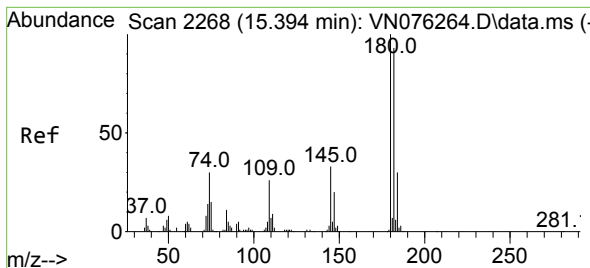

#93

1,2,4-Trichlorobenzene

Concen: 1.972 ug/l

RT: 15.394 min Scan# 21

Delta R.T. -0.000 min

Lab File: VN076508.D

Acq: 02 Feb 2023 14:28

Instrument :

MSVOA_N

ClientSampleId :

PB150614TB





Tgt Ion:180 Resp: 3561

Ion Ratio Lower Upper

180 100

182 100.5 47.0 141.2

145 35.1 15.2 45.5

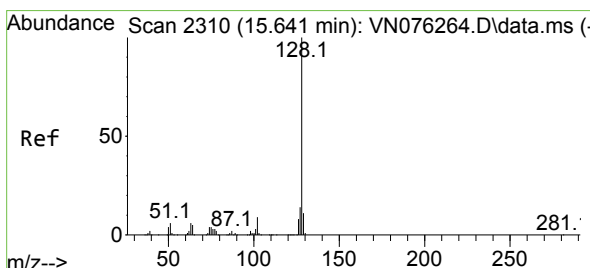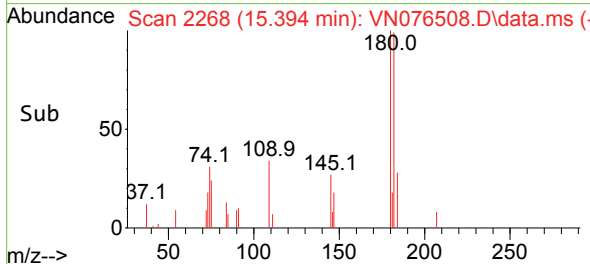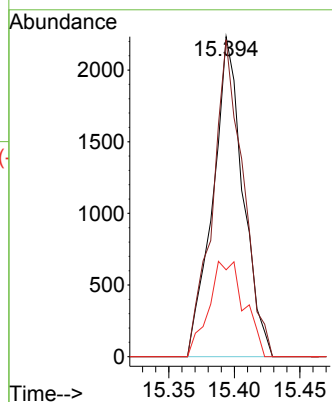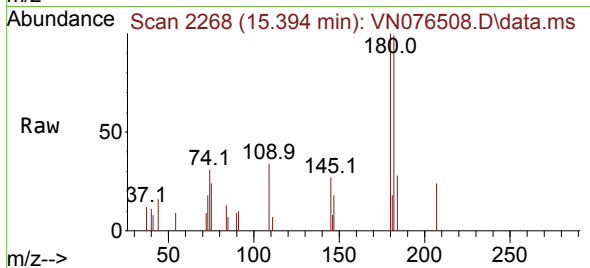

#95

Naphthalene

Concen: 3.082 ug/l

RT: 15.641 min Scan# 2310

Delta R.T. -0.000 min

Lab File: VN076508.D

Acq: 02 Feb 2023 14:28




Tgt Ion:128 Resp: 19864


Ion Ratio Lower Upper

128 100

127 13.1 10.3 15.5

129 9.2 8.6 13.0

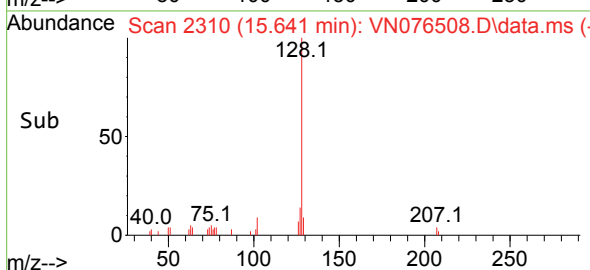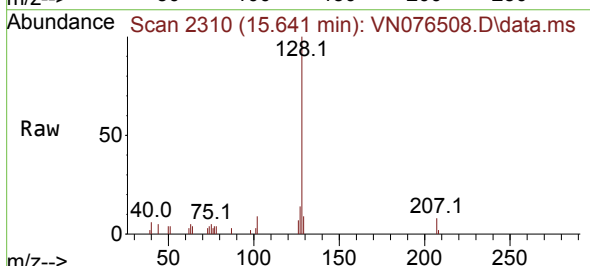



#96
 1,2,3-Trichlorobenzene
 Concen: 2.156 ug/l
 RT: 15.841 min Scan# 21
 Delta R.T. -0.000 min
 Lab File: VN076508.D
 Acq: 02 Feb 2023 14:28

Instrument :
 MSVOA_N
 ClientSampleId :
 PB150614TB

Tgt Ion:180	Resp:	5085
Ion	Ratio	Lower Upper
180	100	
182	84.8	47.5 142.5
145	30.8	15.9 47.6

