

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN020223\
 Data File : VN076512.D
 Acq On : 02 Feb 2023 16:03
 Operator : JC\MD
 Sample : 01386-14
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 JPP-15-013123

Quant Time: Feb 03 01:01:53 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N011623W.M
 Quant Title : SW846 8260
 QLast Update : Tue Jan 17 03:59:22 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	8.230	168	567627	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.106	114	938897	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.865	117	865897	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.794	152	343428	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.582	65	336981	53.021	ug/l	0.00
Spiked Amount 50.000	Range 74 - 125		Recovery = 106.040%			
35) Dibromofluoromethane	8.177	113	286600	48.798	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery = 97.600%			
50) Toluene-d8	10.571	98	1128210	52.014	ug/l	0.00
Spiked Amount 50.000	Range 86 - 113		Recovery = 104.020%			
62) 4-Bromofluorobenzene	12.853	95	382038	53.953	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery = 107.900%			
Target Compounds						Qvalue
11) Tert butyl alcohol	5.541	59	198	0.233	ug/l #	72
16) Acetone	4.447	43	35727	17.467	ug/l	95
18) Methyl Acetate	5.059	43	4136	0.599	ug/l	97
20) Methylene Chloride	5.289	84	30802	4.562	ug/l	87
25) 2-Butanone	7.494	43	5993	1.926	ug/l	90
29) Tetrahydrofuran	7.859	42	1019	0.531	ug/l #	69
31) Cyclohexane	8.224	56	11270	1.154	ug/l #	37
36) 1,1-Dichloropropene	8.230	75	44388	5.319	ug/l #	49
37) Ethyl Acetate	7.571	43	55271	8.287	ug/l	99
38) Carbon Tetrachloride	8.230	117	60154	6.463	ug/l #	17
42) 1,2-Dichloroethane	8.688	62	1903	0.223	ug/l #	73
43) Isopropyl Acetate	8.694	43	256267	23.533	ug/l #	89
45) 1,2-Dichloropropane	9.741	63	3306	0.553	ug/l #	42
48) Methyl methacrylate	9.741	41	223171	43.289	ug/l #	33
49) 1,4-Dioxane	9.741	88	496	4.560	ug/l #	1
51) 4-Methyl-2-Pentanone	10.447	43	20184	3.157	ug/l #	70
53) t-1,3-Dichloropropene	10.723	75	1990	0.239	ug/l #	48
54) cis-1,3-Dichloropropene	10.359	75	108128	11.269	ug/l #	59
56) Ethyl methacrylate	10.988	69	2073	0.252	ug/l #	1
57) 1,3-Dichloropropane	11.206	76	13993	1.350	ug/l #	42
59) 2-Hexanone	11.171	43	218034	47.066	ug/l #	21
71) Bromoform	12.853	173	1985	0.404	ug/l #	1
74) N-amyl acetate	12.488	43	2339	0.306	ug/l #	45
76) 1,2,3-Trichloropropane	12.853	75	196758	31.091	ug/l #	1
77) Bromobenzene	12.976	156	54	Below Cal	#	1
81) trans-1,4-Dichloro-2-b...	12.853	75	196758	95.325	ug/l #	11
93) 1,2,4-Trichlorobenzene	15.400	180	507	1.387	ug/l #	63
95) Naphthalene	15.635	128	2135	1.954	ug/l #	78
96) 1,2,3-Trichlorobenzene	15.853	180	549	1.247	ug/l #	81


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN020223\
Data File : VN076512.D
Acq On : 02 Feb 2023 16:03
Operator : JC\MD
Sample : 01386-14
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
JPP-15-013123

Quant Time: Feb 03 01:01:53 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N011623W.M
Quant Title : SW846 8260
QLast Update : Tue Jan 17 03:59:22 2023
Response via : Initial Calibration




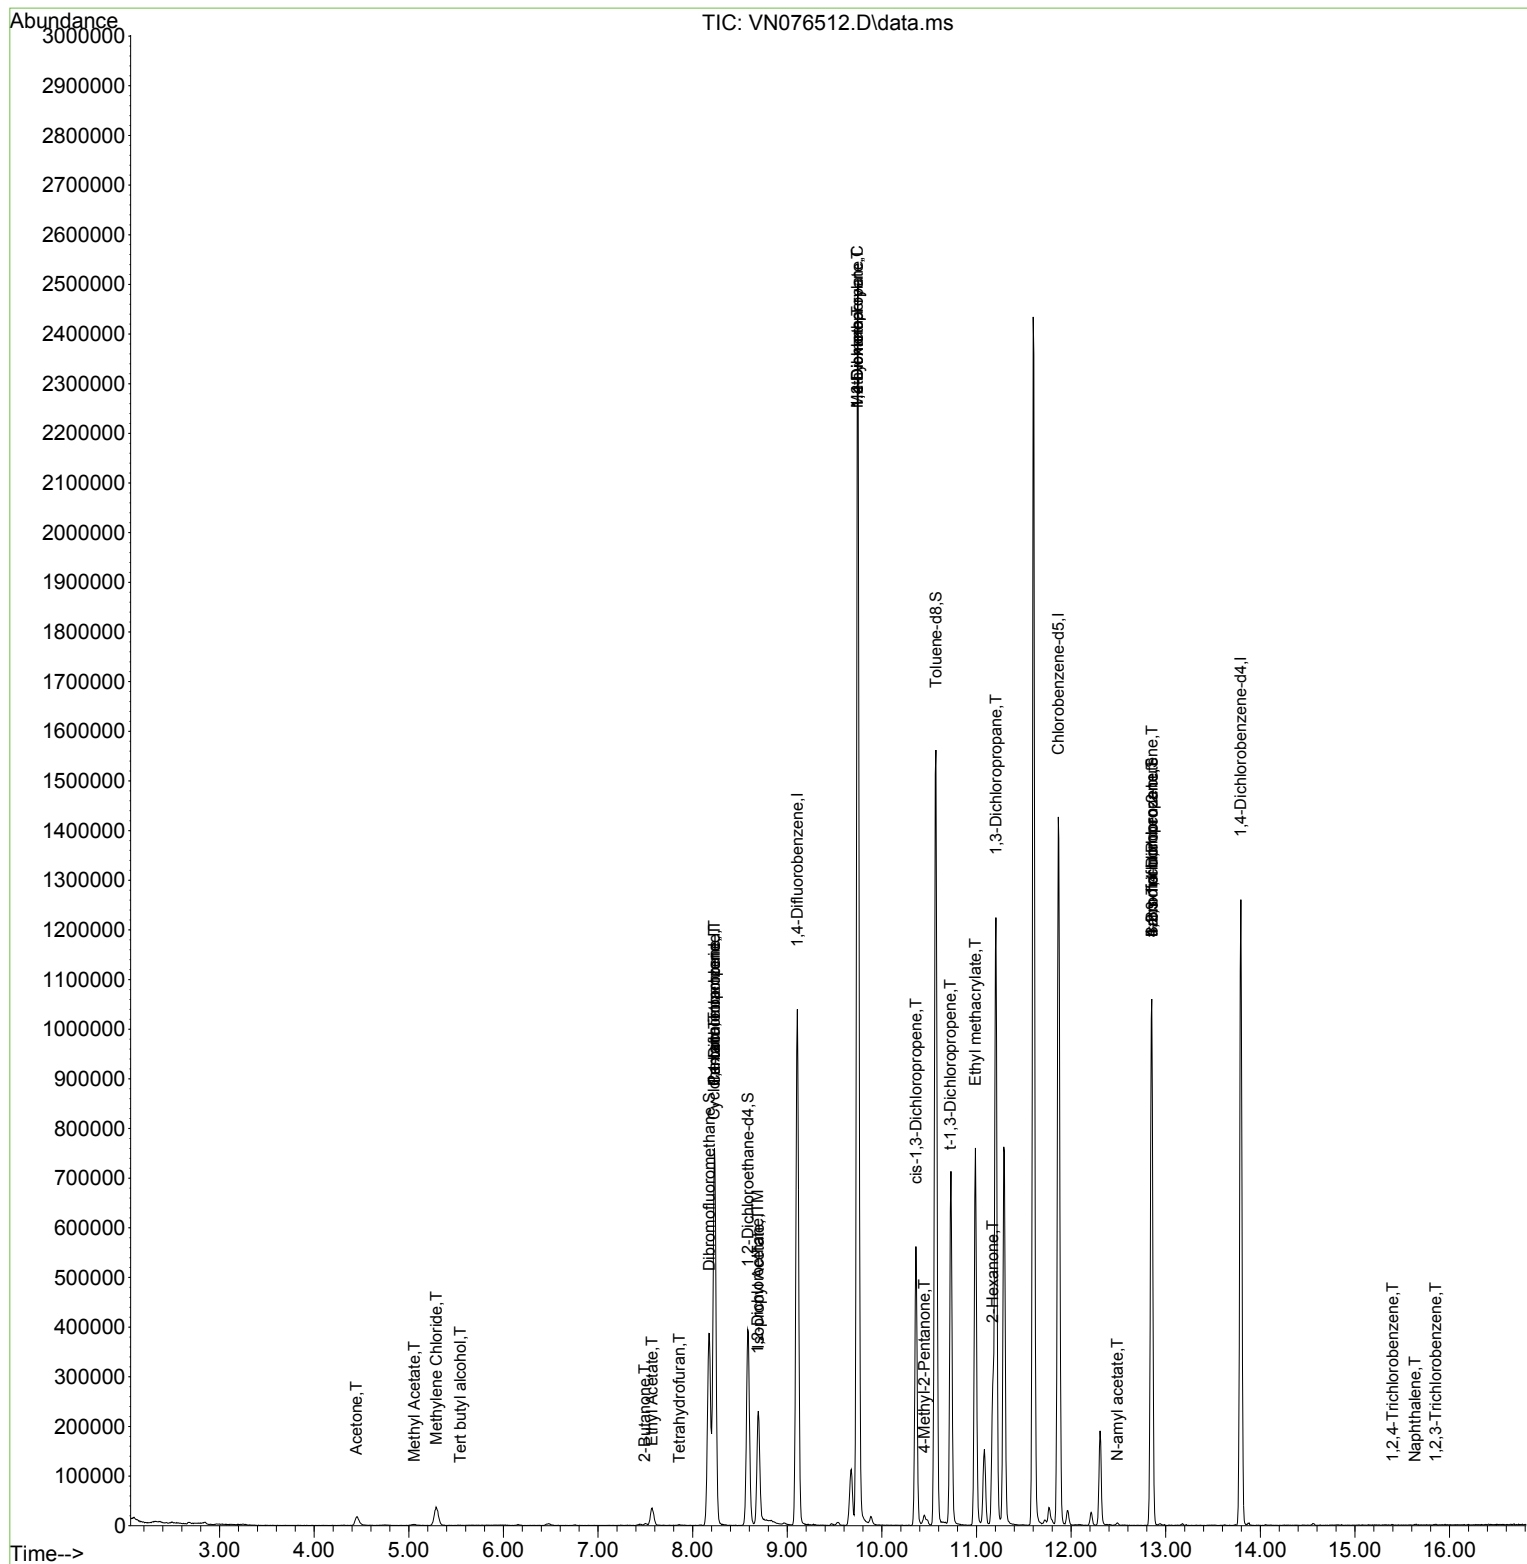




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.230 min Scan# 1050
Delta R.T. -0.000 min
Lab File: VN076512.D
Acq: 02 Feb 2023 16:03




Instrument :
MSVOA_N
ClientSampleId :
JPP-15-013123


Tgt Ion:168 Resp: 567627
Ion Ratio Lower Upper
168 100
99 60.5 41.6 62.4

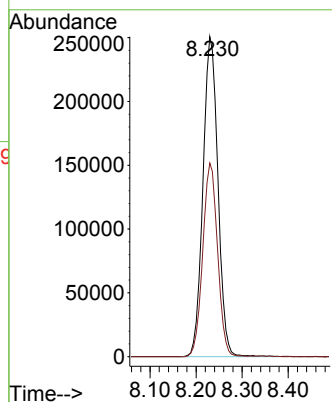

#11
Tert butyl alcohol
Concen: 0.233 ug/l
RT: 5.541 min Scan# 593
Delta R.T. 0.011 min
Lab File: VN076512.D
Acq: 02 Feb 2023 16:03

Tgt Ion: 59 Resp: 198
Ion Ratio Lower Upper
59 100
57 0.0 8.5 12.7#



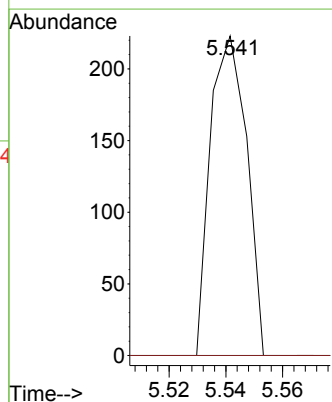
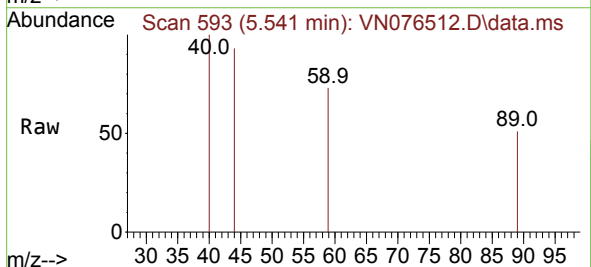




#16
Acetone
Concen: 17.467 ug/l
RT: 4.447 min Scan# 406
Delta R.T. 0.005 min
Lab File: VN076512.D
Acq: 02 Feb 2023 16:03




Instrument :
MSVOA_N
ClientSampleId :
JPP-15-013123


Tgt Ion: 43 Resp: 35727
Ion Ratio Lower Upper
43 100
58 30.6 26.7 40.1

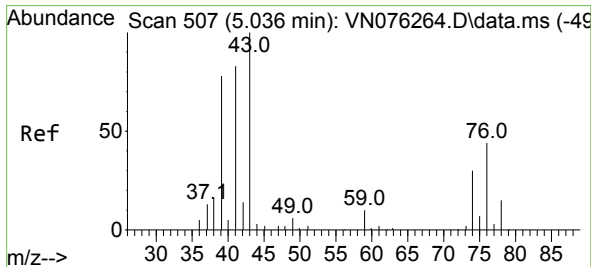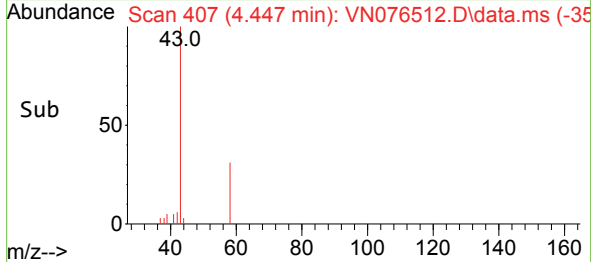

#18
Methyl Acetate
Concen: 0.599 ug/l
RT: 5.059 min Scan# 511
Delta R.T. 0.023 min
Lab File: VN076512.D
Acq: 02 Feb 2023 16:03

Tgt Ion: 43 Resp: 4136
Ion Ratio Lower Upper
43 100
74 27.8 23.3 34.9


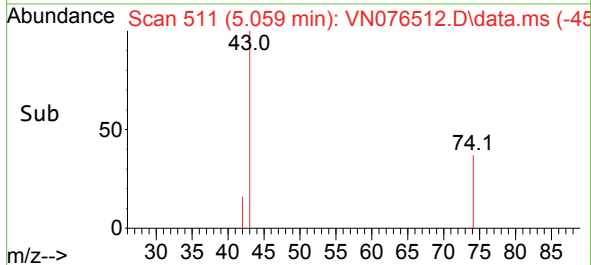

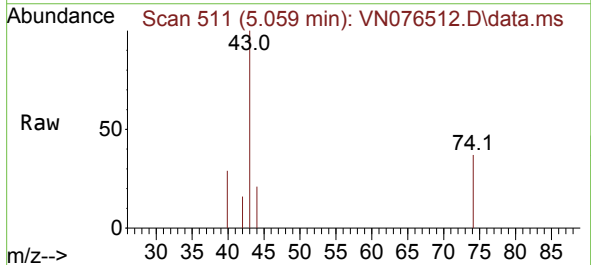




#20
Methylene Chloride
Concen: 4.562 ug/l
RT: 5.289 min Scan# 51
Delta R.T. -0.000 min
Lab File: VN076512.D
Acq: 02 Feb 2023 16:03




Instrument :
MSVOA_N
ClientSampleId :
JPP-15-013123


Tgt Ion: 84	Resp: 30802
Ion Ratio	Lower Upper
84 100	
49 124.7	84.5 126.7
51 37.5	26.0 39.0
86 70.2	52.0 78.0



#25
2-Butanone
Concen: 1.926 ug/l
RT: 7.494 min Scan# 925
Delta R.T. 0.006 min
Lab File: VN076512.D
Acq: 02 Feb 2023 16:03

Tgt Ion: 43	Resp: 5993		
Ion Ratio	Lower	Upper	
43 100			
72 28.6	27.4	41.2	

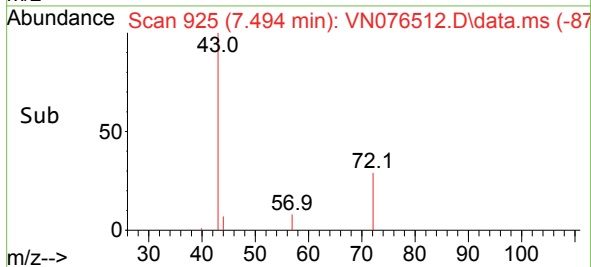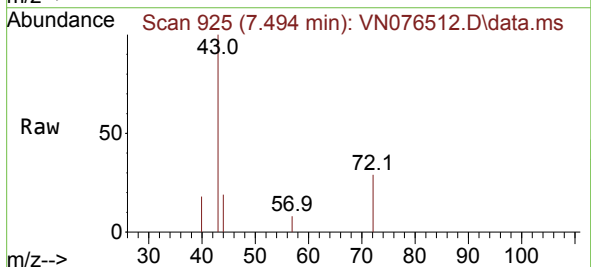



#29

Tetrahydrofuran

Concen: 0.531 ug/l

RT: 7.859 min Scan# 91

Delta R.T. 0.018 min

Lab File: VN076512.D

Acq: 02 Feb 2023 16:03

Instrument :

MSVOA_N

ClientSampleId :

JPP-15-013123





Tgt Ion: 42 Resp: 1019

Ion Ratio Lower Upper

42 100

72 29.9 44.0 66.0#

71 32.2 41.1 61.7#

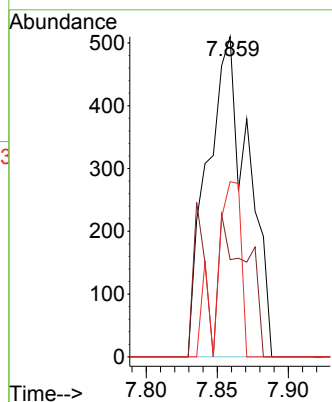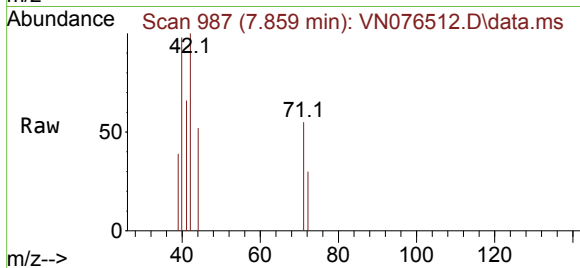

#31

Cyclohexane

Concen: 1.154 ug/l

RT: 8.224 min Scan# 1049

Delta R.T. -0.035 min

Lab File: VN076512.D

Acq: 02 Feb 2023 16:03




Tgt Ion: 56 Resp: 11270


Ion Ratio Lower Upper

56 100

69 163.9 25.8 38.8#

84 105.5 79.0 118.4




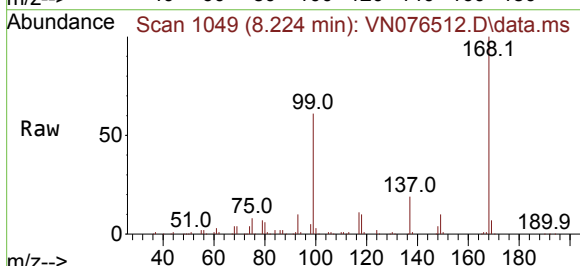




#33
 1,2-Dichloroethane-d4
 Concen: 53.021 ug/l
 RT: 8.582 min Scan# 1110
 Delta R.T. 0.000 min
 Lab File: VN076512.D
 Acq: 02 Feb 2023 16:03




Instrument :
 MSVOA_N
 ClientSampleId :
 JPP-15-013123


Tgt Ion: 65 Resp: 336981
 Ion Ratio Lower Upper
 65 100
 67 51.0 0.0 104.6



#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 9.106 min Scan# 1199
 Delta R.T. -0.000 min
 Lab File: VN076512.D
 Acq: 02 Feb 2023 16:03

Tgt Ion: 114 Resp: 938897
 Ion Ratio Lower Upper
 114 100
 63 19.0 0.0 35.8
 88 15.2 0.0 28.0

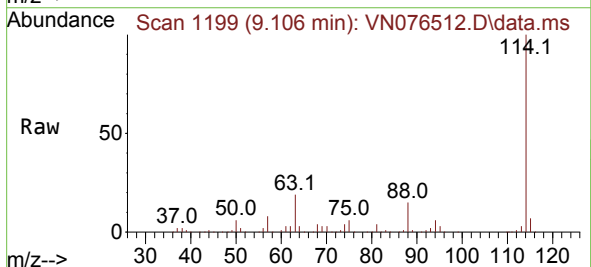



#35

Dibromofluoromethane

Concen: 48.798 ug/l

RT: 8.177 min Scan# 1

Delta R.T. 0.006 min

Lab File: VN076512.D

Acq: 02 Feb 2023 16:03

Instrument :

MSVOA_N

ClientSampleId :

JPP-15-013123





Tgt Ion:113 Resp: 286600

Ion Ratio Lower Upper

113 100

111 102.5 82.7 124.1

192 18.6 15.6 23.4



#36

1,1-Dichloropropene

Concen: 5.319 ug/l

RT: 8.230 min Scan# 1050

Delta R.T. -0.147 min

Lab File: VN076512.D

Acq: 02 Feb 2023 16:03




Tgt Ion: 75 Resp: 44388


Ion Ratio Lower Upper

75 100

110 9.8 18.8 56.3#

77 0.0 25.0 37.4#



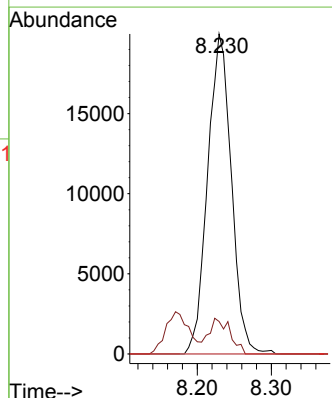





#37
Ethyl Acetate
Concen: 8.287 ug/l
RT: 7.571 min Scan# 91
Delta R.T. 0.006 min
Lab File: VN076512.D
Acq: 02 Feb 2023 16:03




Instrument :
MSVOA_N
ClientSampleId :
JPP-15-013123


Tgt Ion: 43 Resp: 55271
Ion Ratio Lower Upper
43 100
61 14.7 11.1 16.7
70 12.8 10.0 15.0

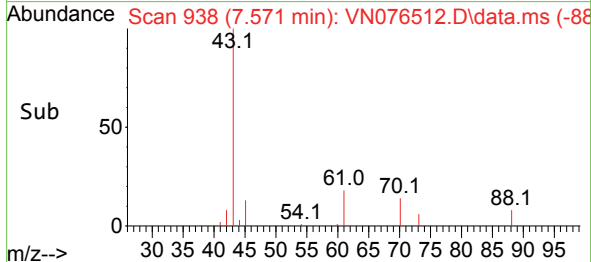

#38
Carbon Tetrachloride
Concen: 6.463 ug/l
RT: 8.230 min Scan# 1050
Delta R.T. -0.135 min
Lab File: VN076512.D
Acq: 02 Feb 2023 16:03

Tgt Ion: 117 Resp: 60154
Ion Ratio Lower Upper
117 100
119 5.5 75.4 113.0#
121 0.0 24.2 36.2#

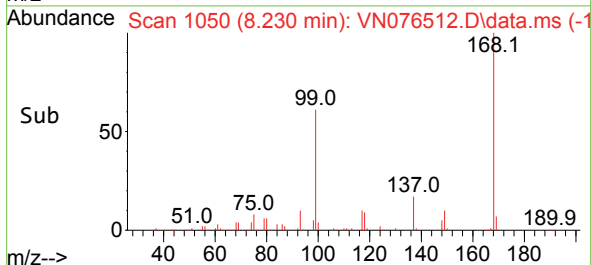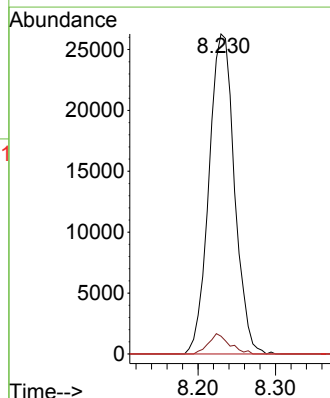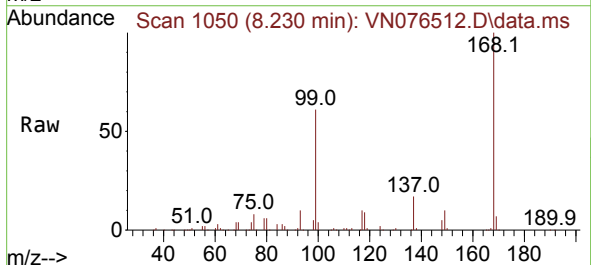



#42

1,2-Dichloroethane

Concen: 0.223 ug/l

RT: 8.688 min Scan# 1128

Delta R.T. 0.011 min

Lab File: VN076512.D

Acq: 02 Feb 2023 16:03

Instrument :

MSVOA_N

ClientSampleId :





JPP-15-013123

Tgt Ion: 62 Resp: 1903

Ion Ratio Lower Upper

62 100

98 0.0 0.0 20.4



#43

Isopropyl Acetate

Concen: 23.533 ug/l

RT: 8.694 min Scan# 1129

Delta R.T. 0.000 min

Lab File: VN076512.D

Acq: 02 Feb 2023 16:03




Tgt Ion: 43 Resp: 256267


Ion Ratio Lower Upper

43 100

61 21.3 23.5 35.3#

87 16.0 13.8 20.6









#45
1,2-Dichloropropane
Concen: 0.553 ug/l
RT: 9.741 min Scan# 11
Delta R.T. 0.117 min
Lab File: VN076512.D
Acq: 02 Feb 2023 16:03




Instrument :
MSVOA_N
ClientSampleId :
JPP-15-013123


Tgt Ion: 63 Resp: 3306
Ion Ratio Lower Upper
63 100
65 0.0 26.4 39.6#

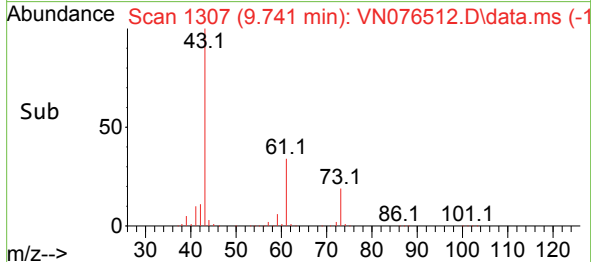

#48
Methyl methacrylate
Concen: 43.289 ug/l
RT: 9.741 min Scan# 1307
Delta R.T. 0.059 min
Lab File: VN076512.D
Acq: 02 Feb 2023 16:03

Tgt Ion: 41 Resp: 223171
Ion Ratio Lower Upper
41 100
69 0.2 80.8 121.2#
39 53.9 54.4 81.6#

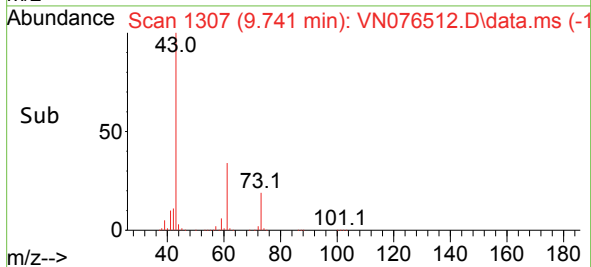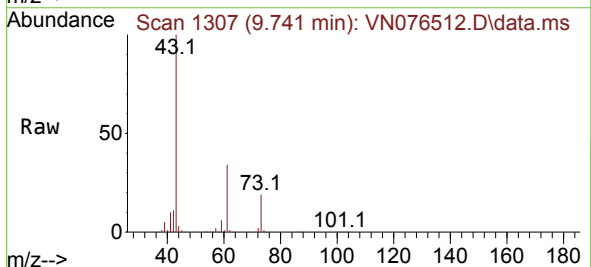



#49

1,4-Dioxane

Concen: 4.560 ug/l

RT: 9.741 min Scan# 1307

Delta R.T. 0.041 min

Lab File: VN076512.D

Acq: 02 Feb 2023 16:03

Instrument :

MSVOA_N

ClientSampleId :

JPP-15-013123





Tgt Ion: 88 Resp: 496

Ion Ratio Lower Upper

88 100

43 462839.3 18.1 27.1#

58 2131.9 46.5 69.7#

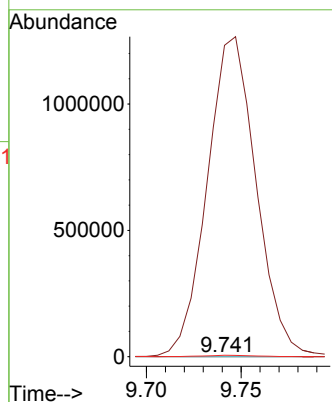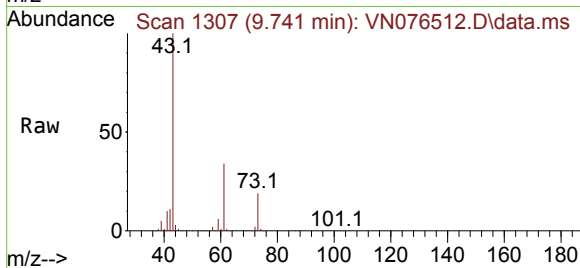

#50

Toluene-d8

Concen: 52.014 ug/l

RT: 10.571 min Scan# 1448

Delta R.T. -0.000 min

Lab File: VN076512.D




Acq: 02 Feb 2023 16:03


Tgt Ion: 98 Resp: 1128210

Ion Ratio Lower Upper

98 100

100 65.8 52.2 78.4




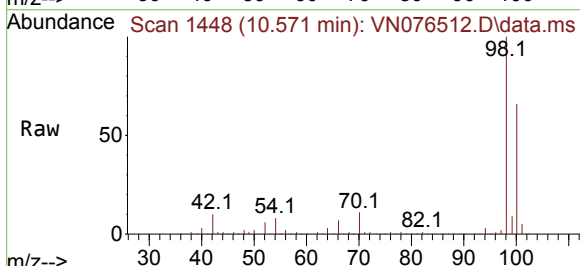




#51
4-Methyl-2-Pentanone
Concen: 3.157 ug/l
RT: 10.447 min Scan# 1427
Delta R.T. 0.000 min
Lab File: VN076512.D
Acq: 02 Feb 2023 16:03




Instrument :
MSVOA_N
ClientSampleId :
JPP-15-013123


Tgt Ion: 43 Resp: 20184
Ion Ratio Lower Upper
43 100
58 24.8 35.1 52.7#



#53
t-1,3-Dichloropropene
Concen: 0.239 ug/l
RT: 10.723 min Scan# 1474
Delta R.T. -0.112 min
Lab File: VN076512.D
Acq: 02 Feb 2023 16:03

Tgt Ion: 75 Resp: 1990
Ion Ratio Lower Upper
75 100
77 3.0 25.8 38.6#




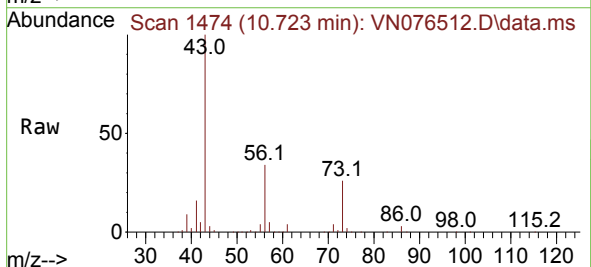


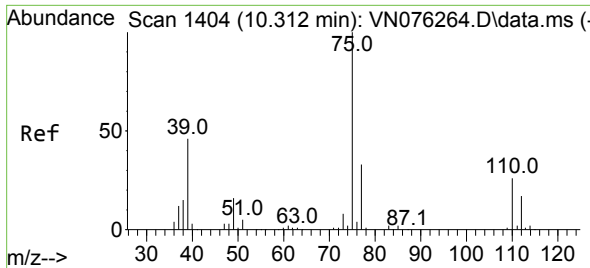

#54
 cis-1,3-Dichloropropene
 Concen: 11.269 ug/l
 RT: 10.359 min Scan# 14
 Delta R.T. 0.047 min
 Lab File: VN076512.D
 Acq: 02 Feb 2023 16:03




Instrument :
 MSVOA_N
 ClientSampleId :
 JPP-15-013123


Tgt Ion: 75 Resp: 108128
 Ion Ratio Lower Upper
 75 100
 77 0.0 26.5 39.7#
 39 27.5 37.1 55.7#

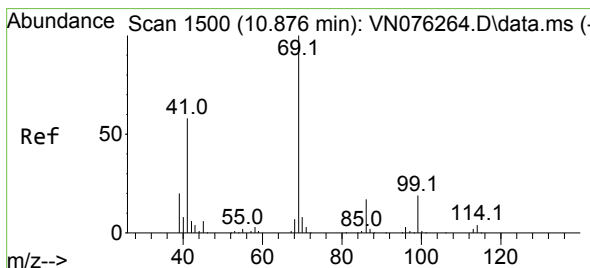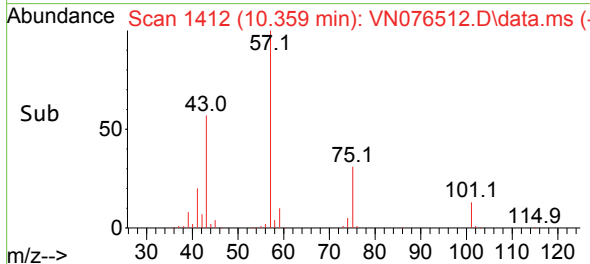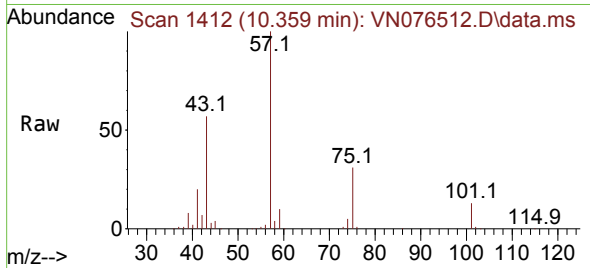

#56
 Ethyl methacrylate
 Concen: 0.252 ug/l
 RT: 10.988 min Scan# 1519
 Delta R.T. 0.112 min
 Lab File: VN076512.D
 Acq: 02 Feb 2023 16:03

Tgt Ion: 69 Resp: 2073
 Ion Ratio Lower Upper
 69 100
 41 6549.9 45.3 67.9#
 39 2734.3 29.3 43.9#


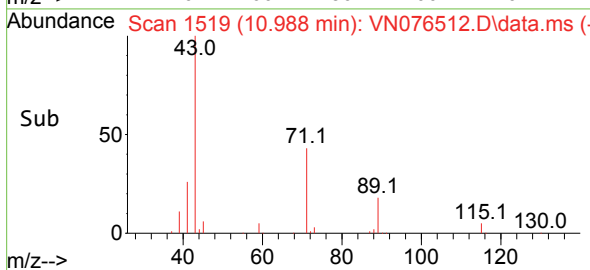

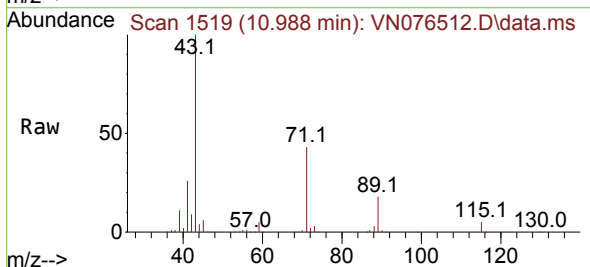


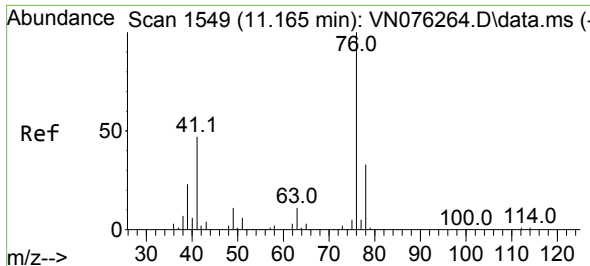

#57
1,3-Dichloropropane
Concen: 1.350 ug/l
RT: 11.206 min Scan# 1556
Delta R.T. 0.041 min
Lab File: VN076512.D
Acq: 02 Feb 2023 16:03




Instrument :
MSVOA_N
ClientSampleId :
JPP-15-013123


Tgt Ion: 76 Resp: 13993
Ion Ratio Lower Upper
76 100
78 0.0 26.4 39.6#

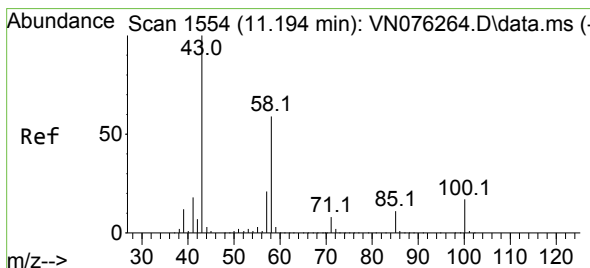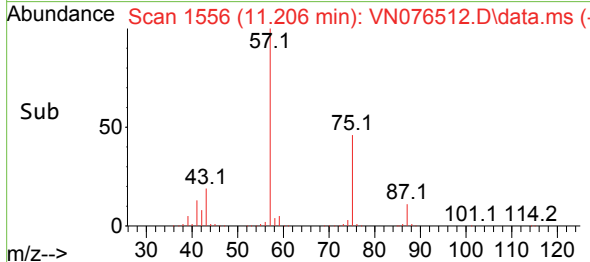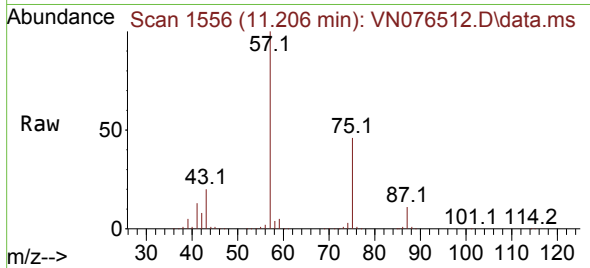

#59
2-Hexanone
Concen: 47.066 ug/l
RT: 11.171 min Scan# 1550
Delta R.T. -0.023 min
Lab File: VN076512.D
Acq: 02 Feb 2023 16:03

Tgt Ion: 43 Resp: 218034
Ion Ratio Lower Upper
43 100
58 0.0 30.1 90.3#


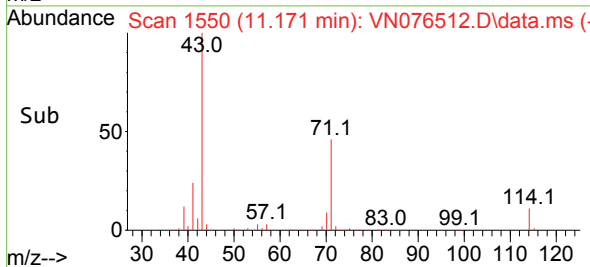

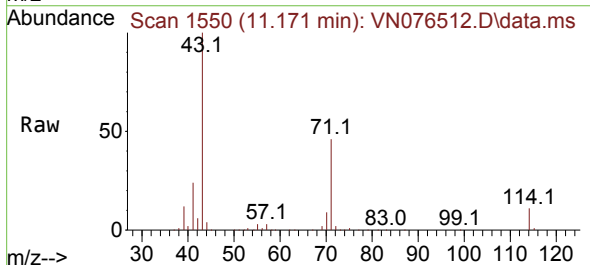




#62
4-Bromofluorobenzene
Concen: 53.953 ug/l
RT: 12.853 min Scan# 1836
Delta R.T. 0.006 min
Lab File: VN076512.D
Acq: 02 Feb 2023 16:03




Instrument :
MSVOA_N
ClientSampleId :
JPP-15-013123


Tgt Ion: 95 Resp: 382038
Ion Ratio Lower Upper
95 100
174 78.1 0.0 174.6
176 74.9 0.0 167.8

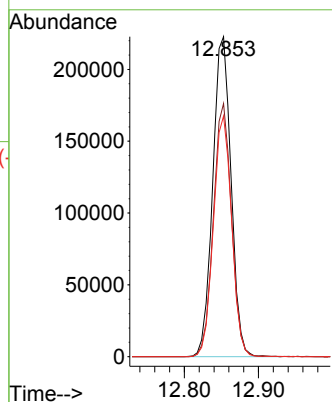

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.865 min Scan# 1668
Delta R.T. -0.000 min
Lab File: VN076512.D
Acq: 02 Feb 2023 16:03

Tgt Ion: 117 Resp: 865897
Ion Ratio Lower Upper
117 100
82 56.8 42.2 63.2
119 32.7 26.9 40.3

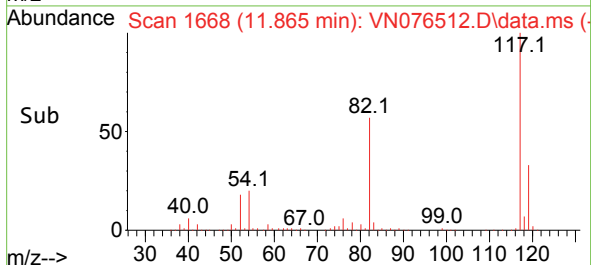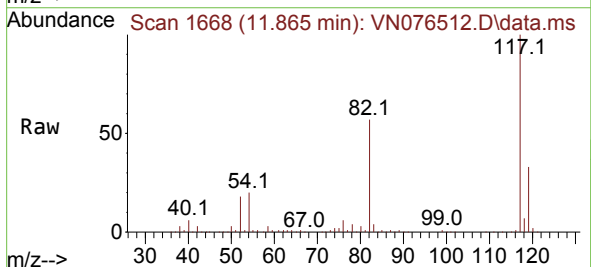



#71

Bromoform

Concen: 0.404 ug/l

RT: 12.853 min Scan# 1836

Delta R.T. 0.271 min

Lab File: VN076512.D

Acq: 02 Feb 2023 16:03

Instrument :

MSVOA_N

ClientSampleId :

JPP-15-013123





Tgt Ion:173 Resp: 1985

Ion Ratio Lower Upper

173 100

175 724.5 24.1 72.4#

254 0.0 0.0 0.0

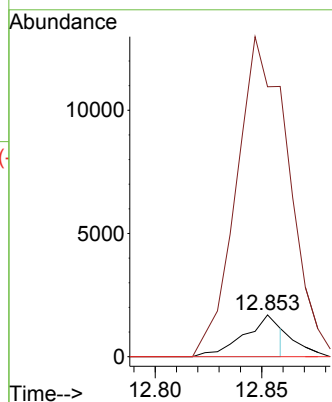

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.794 min Scan# 1996

Delta R.T. -0.000 min

Lab File: VN076512.D

Acq: 02 Feb 2023 16:03




Tgt Ion:152 Resp: 343428


Ion Ratio Lower Upper

152 100

115 61.0 29.6 88.9

150 157.3 0.0 351.4





#74

N-amyl acetate

Concen: 0.306 ug/l

RT: 12.488 min Scan# 1

Delta R.T. -0.006 min

Lab File: VN076512.D

Acq: 02 Feb 2023 16:03

Instrument :

MSVOA_N

ClientSampleId :

JPP-15-013123

Tgt Ion: 43 Resp: 2339





Ion Ratio Lower Upper

43 100

70 6.5 41.2 61.8#

55 6.1 21.0 31.6#

61 0.0 21.6 32.4#



#76

1,2,3-Trichloropropane

Concen: 31.091 ug/l

RT: 12.853 min Scan# 1836

Delta R.T. -0.141 min

Lab File: VN076512.D




Acq: 02 Feb 2023 16:03


Tgt Ion: 75 Resp: 196758

Ion Ratio Lower Upper

75 100

77 1.2 75.2 225.6#

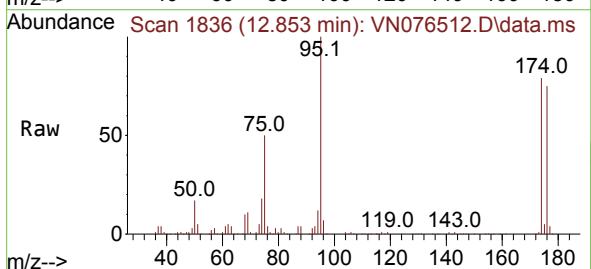



#77

Bromobenzene

Concen: Below Cal

RT: 12.976 min Scan# 1857

Delta R.T. -0.006 min

Lab File: VN076512.D

Acq: 02 Feb 2023 16:03





Instrument :

MSVOA_N

ClientSampleId :

JPP-15-013123

Tgt Ion:	156	Resp:	54
Ion	Ratio	Lower	Upper
156	100		
77	638.9	93.4	280.2#
158	98.1	48.4	145.2

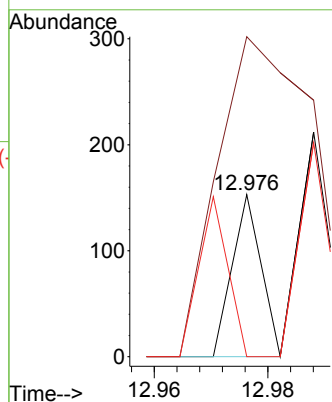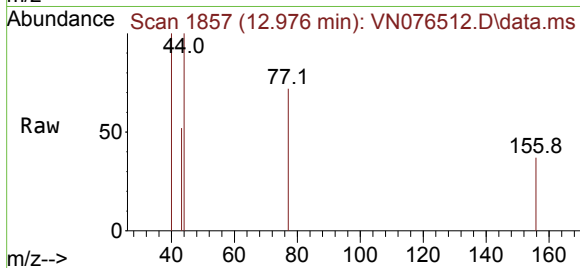

#81

trans-1,4-Dichloro-2-butene

Concen: 95.325 ug/l




RT: 12.853 min Scan# 1836


Delta R.T. 0.118 min

Lab File: VN076512.D

Acq: 02 Feb 2023 16:03

Tgt Ion:	75	Resp:	196758
Ion	Ratio	Lower	Upper
75	100		
53	0.0	75.8	113.8#
89	0.0	37.0	55.6#

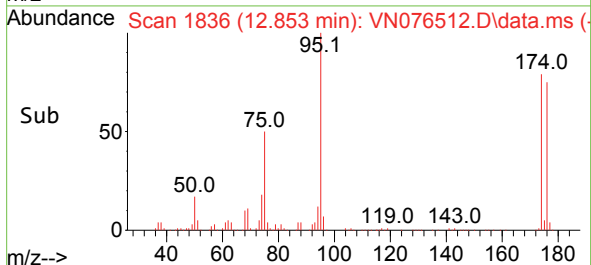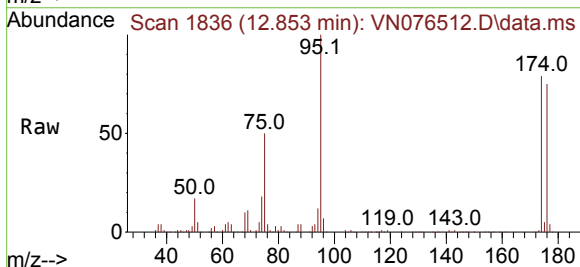

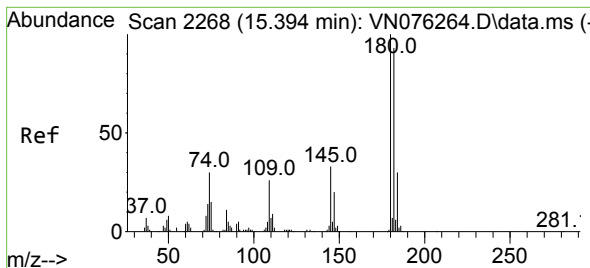

#93

1,2,4-Trichlorobenzene

Concen: 1.387 ug/l

RT: 15.400 min Scan# 21

Delta R.T. 0.006 min

Lab File: VN076512.D

Acq: 02 Feb 2023 16:03

Instrument :

MSVOA_N

ClientSampleId :

JPP-15-013123





Tgt Ion:180 Resp: 507

Ion Ratio Lower Upper

180 100

182 57.6 47.0 141.2

145 10.7 15.2 45.5#

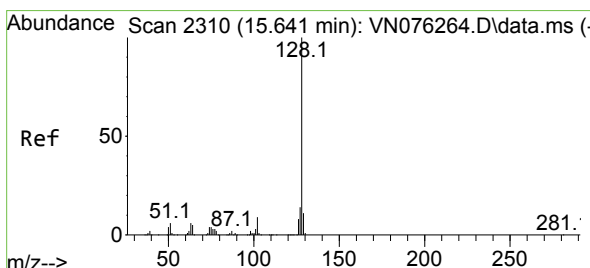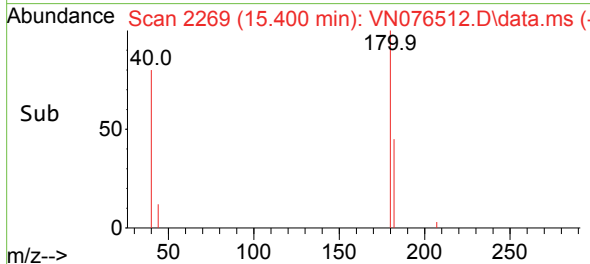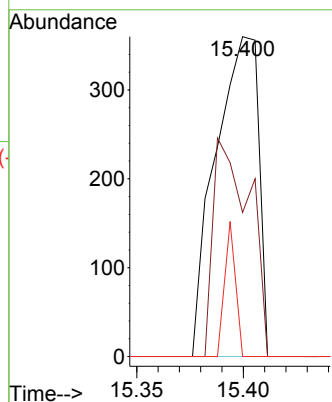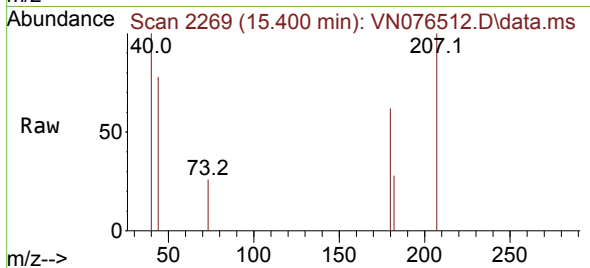

#95

Naphthalene

Concen: 1.954 ug/l

RT: 15.635 min Scan# 2309

Delta R.T. -0.006 min

Lab File: VN076512.D

Acq: 02 Feb 2023 16:03




Tgt Ion:128 Resp: 2135


Ion Ratio Lower Upper

128 100

127 6.2 10.3 15.5#

129 0.0 8.6 13.0#

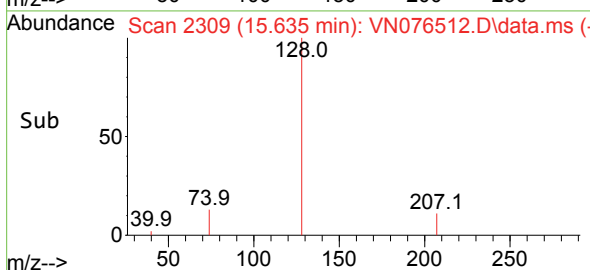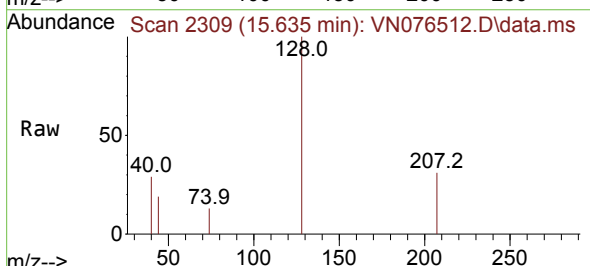



#96
 1,2,3-Trichlorobenzene
 Concen: 1.247 ug/l
 RT: 15.853 min Scan# 21
 Delta R.T. 0.012 min
 Lab File: VN076512.D
 Acq: 02 Feb 2023 16:03

Instrument :
 MSVOA_N
 ClientSampleId :
 JPP-15-013123

Tgt Ion:180 Resp: 549
 Ion Ratio Lower Upper
 180 100
 182 88.7 47.5 142.5
 145 0.0 15.9 47.6#

